

## ORIGINAL RESEARCH

Food Science &amp; Nutrition

Open Access

WILEY

# Rapid detection of *Pseudomonas aeruginosa* using a DNzyme-based sensor

Mingcan Qin<sup>1,2,3</sup>  | Xiaoyi Ma<sup>1,2,3</sup> | Shihui Fan<sup>1,2,3</sup> | Hangjie Wu<sup>1,2,3</sup> | Wanli Yan<sup>1,2,3</sup> | Xiaopeng Tian<sup>1,2,3</sup> | Jing Lu<sup>1,2,3</sup> | Mingsheng Lyu<sup>1,2,3</sup> | Shujun Wang<sup>1,2,3</sup>

<sup>1</sup>Jiangsu Key Laboratory of Marine Bioresources and Environment/Jiangsu Key Laboratory of Marine Biotechnology, Jiangsu Ocean University, Lianyungang, China

<sup>2</sup>Co-Innovation Center of Jiangsu Marine Bio-industry Technology, Jiangsu Ocean University, Lianyungang, China

<sup>3</sup>Jiangsu Marine Resources Development Research Institute, Lianyungang, China

## Correspondence

Mingsheng Lyu and Shujun Wang, Jiangsu Key Laboratory of Marine Bioresources and Environment, Jiangsu Ocean University, Lianyungang, 222005, China.  
Emails: mslu@jou.edu.cn (M.L.); sjwang@jou.edu.cn (S.W.)

## Funding information

The Research & Practice Innovation Program of Jiangsu, Grant/Award Number: SJCX19-1020 and JSIMR201926; The Priority Academic Program Development of Jiangsu Higher Education Institutions (PAPD); National Key R&D Program of China, Grant/Award Number: 2018YFC0311106

## Abstract

In the present study, a DNzyme was screened in vitro through the use of a DNA library and crude extracellular mixture (CEM) of *Pseudomonas aeruginosa*. Following eight rounds of selection, a DNzyme termed PAE-1 was obtained, which displayed high rates of cleavage with strong specificity. A fluorescent biosensor was designed for the detection of *P. aeruginosa* in combination with the DNzyme. A detection limit as low as 1.2 cfu/ml was observed. Using proteases and filtration, it was determined that the target was a protein with a molecular weight of 10 kDa–50 kDa. The DNzyme was combined with a polystyrene board to construct a simple indicator plate sensor which produced a color that identified the target within 10 min. The results were reliable when tap water and food samples were tested. The present study provides a novel experimental strategy for the development of sensors based on a DNzyme to rapidly detect *P. aeruginosa* in the field.

## KEYWORDS

DNzyme, *Pseudomonas aeruginosa*, rapid detection

## 1 | INTRODUCTION

*Pseudomonas aeruginosa* is a gram-negative bacillus widely distributed in nature, and also a common conditional pathogen on human skin and in the respiratory tract. In 1882, *P. aeruginosa* was separated from the pus of a wound by Gersard for the first time and found able to survive in wet and dry environments (Woodford & Livermore, 2009). Tap water (Garvey et al., 2016; Gautam, 2021) and medical equipment (Alvarez-Lerma et al., 2018) are often contaminated with *P. aeruginosa* which not only has innate resistance to a variety of antibiotics, it also has the propensity to develop drug resistance (Feng et al., 2019; Langendonk et al., 2021). *P. aeruginosa* accounts for 10%–15% of all nosocomial

infections (Bassetti et al., 2018), especially those in intensive care unit (ICU) (Cohen et al., 2017; Coppy et al., 2020). Its pathogenic characteristics cause secondary infections, occurring mostly when the body's immunity is reduced, such as after extensive burns (Karaky et al., 2020) and following surgery (Richards & Marshall, 2018). *P. aeruginosa* can also cause human Hospital-Acquired Pneumonia (Goncalves-De-Albuquerque et al., 2016), urinary tract infections (Pachori et al., 2019; Tumbarello et al., 2020), and bacteremia (Callejas-Díaz et al., 2019; McCarthy & Paterson, 2017). There are approximately 51,000 medical-related infections in the United States every year (Cdc, 2019).

Many robust methods exist to detect bacteria, each having its own characteristics. Traditional culture methods (Rashno Tae

This is an open access article under the terms of the Creative Commons Attribution License, which permits use, distribution and reproduction in any medium, provided the original work is properly cited.

© 2021 The Authors. Food Science & Nutrition published by Wiley Periodicals LLC.

et al., 2014) are highly accurate but are time-consuming and require specific media and differentiation tests to identify them. Immunological assays (Huang et al., 2020; Lin, Zhou, & Tang, 2017) and polymerase chain reaction (PCR) (Guo et al., 2020) technology based on nucleic acid amplification greatly shortens the duration of identification. However, immunological assays (Krithiga et al., 2016; Shahdordizadeh et al., 2017) suffer from being expensive and complicated sample preparation steps. PCR technology (Aghamollaei et al., 2015) requires DNA extraction, and dead extracted bacteria can also produce false-positive signals. Electrochemical methods (Lin, Zhou, Tang, Niessner, et al., 2017; Zhou & Tang, 2020) are highly sensitive but the external environment can easily cause interference (Sismaet et al., 2014) and additionally, requires specialized equipment. Methods allowing rapid detection are particularly useful.

Used widely as molecular tools, enzyme-based methods can also be used in biosensing (Zhang et al., 2019), environmental detection (Wang et al., 2018), and medical diagnosis (Kumar et al., 2019; Zhou et al., 2017). DNAzyme is a functional nucleic acid (Peng et al., 2020), a single-stranded DNA molecule with catalytic activity that can be isolated from random synthetic libraries by in vitro selection technology (Gu et al., 2019). It was reported that the first DNA was used for RNA cleavage (Breaker & Joyce, 1994) in 1994. Santoro and others obtained a classic  $Pb^{2+}$ -dependent 8–17 DNAzyme through in vitro screening (Santoro Sw, 1997). Subsequently, increasing numbers of metal ion-dependent DNAzymes have been discovered (Li et al., 2017; Torabi et al., 2015; Yu et al., 2018). From the unique mixture (crude extracellular mixture, CEM) resulting from microbial reproductive metabolism, Yingfu Li developed the fluorescent DNAzyme probe RDF-EC1 for the detection of *Escherichia coli* (Ali et al., 2011). M. Monsur Ali present a DNAzyme-based fluorescent paper sensor for *Klebsiella pneumoniae* (Ali, Slepenskin, et al., 2019). A colorimetric paper DNAzyme sensor for *E. coli* and *Helicobacter pylori* has undergone continuous development (Ali, Wolfe, et al., 2019; Tram et al., 2014), providing rapid bacterial detection on site. Previous reports demonstrate the unique advantages of DNAzymes in bacterial detection (McConnell et al., 2020; Zhou et al., 2020).

*Pseudomonas aeruginosa* not only contaminates medical equipment, it also is an important pathogen in sources of water and food, posing a serious threat to human health. In this study, we focused on simple and efficient detection method of *P. aeruginosa*. By integrating previously reported selecting methods (Gu et al., 2019; Li, 2011; Zhang et al., 2016) with the unmodified DNA library and the crude extracellular mixture (CEM) of *P. aeruginosa*, a highly specific DNAzyme was obtained through conventional DNAzyme selection. The DNAzyme was attached to a polystyrene board to fabricate a DNAzyme sensor "mixed read" assay (Zhang et al., 2016) that could rapidly identify *P. aeruginosa*. This study describes an effective method for screening and making other bacterial DNAzyme sensors, which provides a basis for the establishment of related detection methods for *P. aeruginosa*.

## 2 | RESULTS AND DISCUSSION

### 2.1 | DNAzyme screening and sequence analysis


DNAzyme is a DNA-based catalyst. It has the advantages of high catalytic efficiency, it is simple to synthesize and modify, and elicits no immune reaction. DNAzymes also display an interesting tertiary structure more stable than proteins. In the present study, *P. aeruginosa* extracellular product (CEM-PA) was used as a screening target. Eight rounds of screening were performed (Figure 1a) using an initial library of  $10^{13} \sim 10^{15}$  molecules containing 35 random bases and an adenine ribonucleoside (rA) cleavage site (Figure 1a). *Pseudomonas aeruginosa* CEM-PA was used directly as a target, by passing target isolation and identification in terms of time saved and cost. Through negative selection, the DNA sequences displaying nonspecific or weak binding were removed, while positive selection enriched the target-specific sequences (Figure 1b). Over the final three rounds, cleavage time was gradually reduced. This allowed DNAzyme to be screened-out which could perform cleavage quickly. In addition to the first introduction of negative selection in the third round, the yield of cleavage in other rounds increased. After round 8, cleavage yield was close to 35%. The PCR products of the 8th round were purified and sequenced.

Sangon Biotech (Shanghai, China) used the Miseq platform from Illumina for sequencing which generated 33,846 raw DNA reads. The first 10 sequences were selected by length and percentage, and compared with each other using Clustal software (Figure 1c). Except for the third sequence, only individual bases differed from each other in the other 9 sequences. Using IDT Oligo Analyzer 3.1 to predict the secondary structures of 1 and 3, termed PAE-1 and PAE-3, we found that both DNAzymes contained a special stem-loop structure (Figure 1d). To determine their activity, the sequences of PAE-1 and PAE-3 were synthesized. Using dynamic analysis, PAE-1 had greater cleavage activity (Figure 2a). The sequence of the red section of the stem ring was highly conserved on PAE-1 and PAE-3, possibly related to the active region of DNAzyme. From the predicted secondary structure, the stem rings were arranged more intensively on PAE-1, possibly the reason for its high cleavage activity.

### 2.2 | Influence of metal ions and pH on DNAzyme cleavage

The results demonstrate that the DNAzyme displayed the greatest cleavage activity at a  $Na^+$  concentration of 30 mM and  $Mg^{2+}$  concentration of 60 mM (Figure 2b). With increasing metal ion concentration, DNAzyme activity decreased sharply. This was possibly because the high concentration changed the three-dimensional structure of the DNAzyme and reduced cleavage activity.

Previous studies have shown that pH also affects DNAzyme activity (Ma et al., 2019; Ma & Liu, 2019). As displayed in Figure 2c, the lytic activity of the DNAzyme gradually increased with increasing pH. Too high a pH should not be used because  $Mg^{2+}$  can easily precipitate in alkaline conditions, affecting the accuracy of the

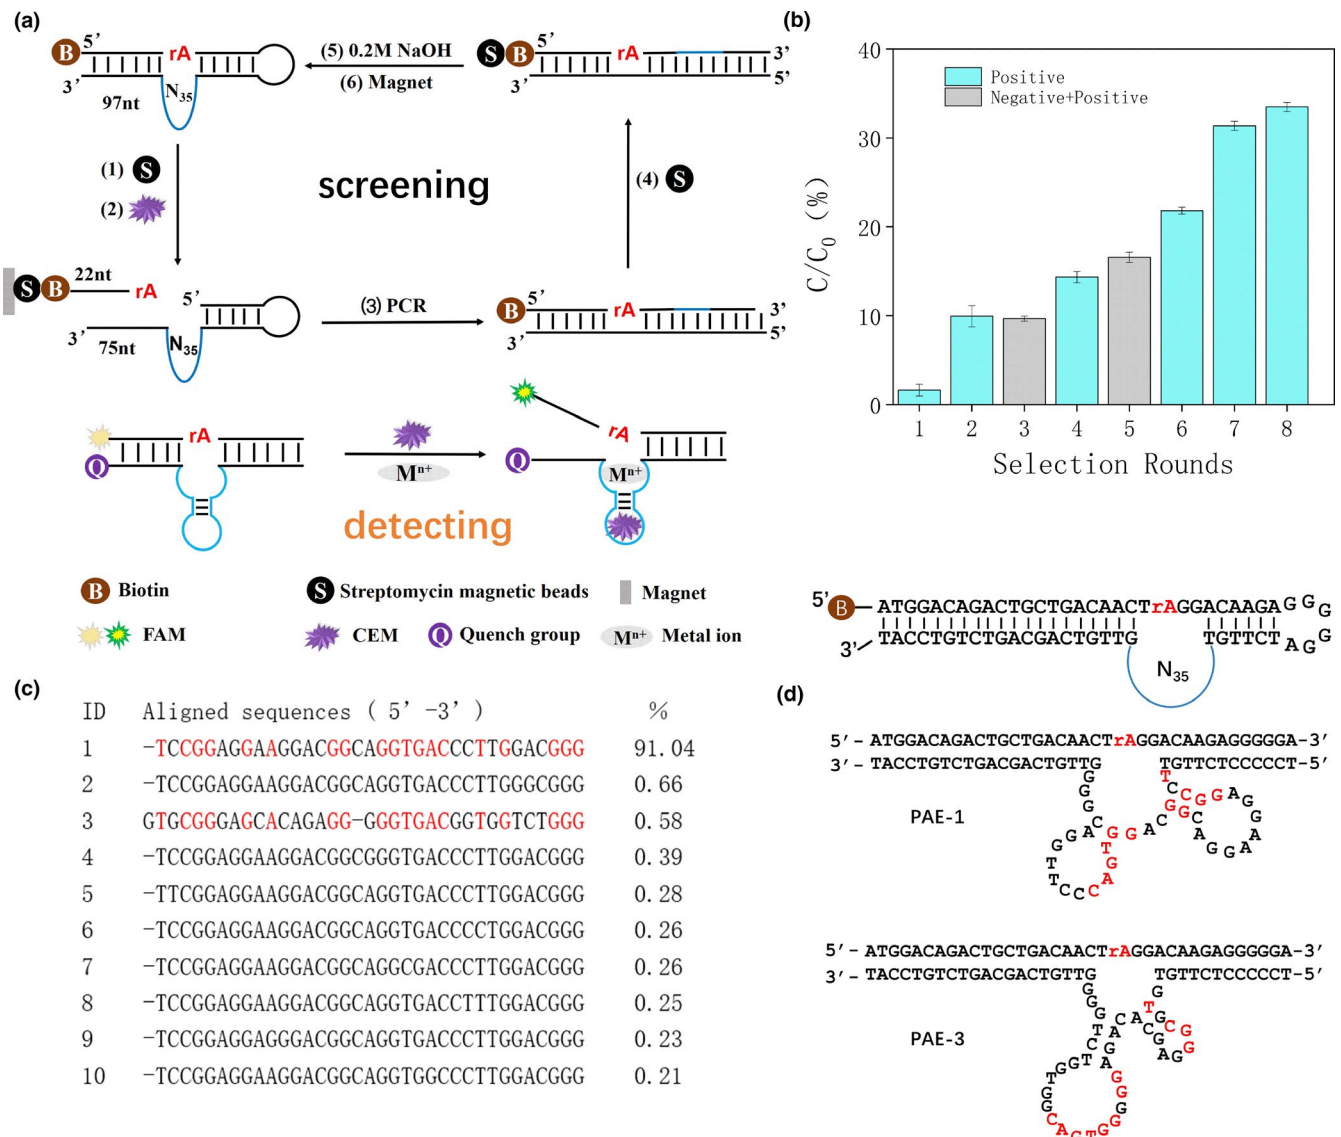

**FIGURE 1** (a) CEM-PA specific DNA enzyme selection process. The original library was fixed, the sequence was cleaved in the presence of CEM. After PCR, cleaved fragments were restored to the original full-length library to inoculate the subsequent round of selection. A molecular beacon design was used for the DNAzyme sensor. (b) Ratio of cleavage of selection progress ( $C/C_0$ ). (c) The most abundant 10 DNA sequences using deep sequencing. Red letters in bold represent highly aligned PAE-1 and PAE-3 sequences. (d) The initial library selected in vitro. The cleavage site is at the rA junction and labeled with biotin at the 5' end. Secondary structure of PAE-1 and PAE-3 DNAzymes

experiment (Figure 2c). Therefore, for subsequent experiments, a pH of 8.0 was selected.


### 2.3 | CEM composition

Crude extracellular mixture is a complex extracellular mixture, in which it is difficult to identify an effective target molecule. Li and co-workers discovered that DNAzyme cleavage was related to a transcription factor (protein) (Shen et al., 2016). It was first assumed that the target was a protein. CEM-PA was treated with trypsin to digest the proteins, or boiled in trypsin for 10 min to inactivate it, then mixed them with PAE-1 DNAzyme. Gel images and fluorescence-based


sensors indicated that Trypsin-treated CEM-PA demonstrated no signal from the PAE-1 (Figure 3a). Therefore, the target may be a protein. An estimate of the molecular weight of the protein was performed by filtering the target through multiple spin columns (3 kDa–50 kDa). The results indicate that only the 50 kDa filtrate was able to induce cleavage of PAE-1 DNAzyme (Figure 3b). Therefore, the molecular weight of the target protein was between 10 kDa and 50 kDa.

### 2.4 | Highly specific detection

Quenchanters were labeled at the 3' end of the PAE-1 DNAzyme chain, and a FAM fluorescent group was labeled at the 5' end of the substrate

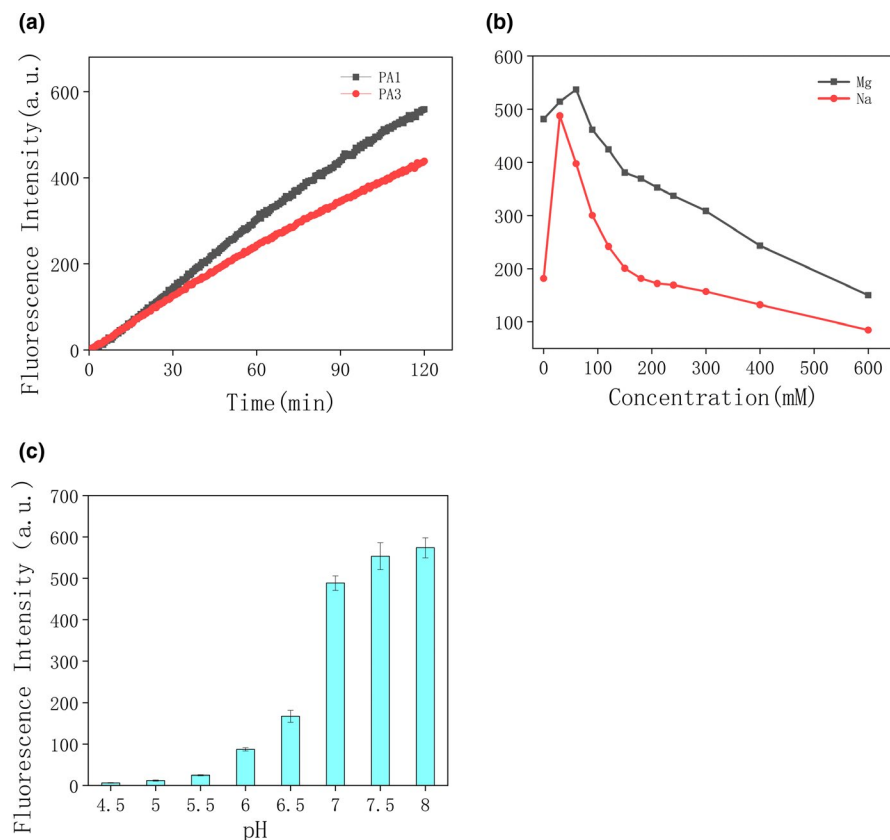

**FIGURE 2** (a) Kinetics of PAE-1 and PAE-3. (b) Effects of Na<sup>+</sup> and Mg<sup>2+</sup> concentration on cleavage activity. (c) Cleavage at different pH values

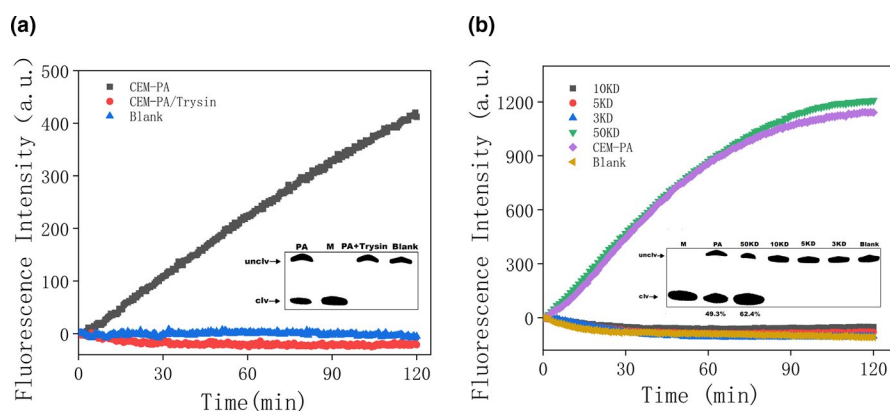


**FIGURE 3** (a) Trypsin-treated CEM-PA demonstrated no signal from the PAE-1 based biosensor. Inset: gel micrograph displaying activity. M: DNAzyme was completely cleaved by *P. aeruginosa*. (b) Assessment of the molecular weight of the target protein. Inset: gel images for each part

(Du, Li, Yang, et al., 2020; Wang et al., 2020). When annealed to form the DNAzyme, the fluorescence was quenched (Figure 1a). The DNAzyme was reacted to cleaved, and the fluorescence signal was released when the CEM-PA was added. We fixed the DNAzyme was fixed on polystyrene boards by dropping and drying naturally. Fluorescence could be observed by naked eye under blue light (490 nm).

In the present study, CEM-PA was selected as a screening target. In addition to cell metabolism, the culture medium was also a key factor affecting the results. To eliminate the possible cleavage occurring due to the medium, blank medium was incubated with the PAE-1 DNAzyme. In addition, cleavage conditions for PAE-1 DNAzyme in 7 different bacterial extracellular products were also verified. As shown in Figure 4c, the results indicate that the blank medium (labeled blank control) not only failed to allow cleavage but also resulted in quenching of fluorescence. None of the seven

bacteria displayed cleavage activity when tested. Only *V. vulnificus* fluorescence remained unchanged, while the fluorescence values of other bacteria decreased. It is possible that particular ions within the beef paste in the culture medium or CEM produced by these bacteria caused fluorescence quenching. The same results were obtained denatured polyacrylamide gel electrophoresis (Figure 4b). The DNAzyme can form loops which can bind with targets specifically through hydrophobic, electrostatic, hydrogen bonding, van der Waals force, base stacking, and shape complementarity (Gu et al., 2019; Zhang et al., 2016). The binding mechanism is similar with antibodies or aptamers which bind with targets. The combination of antibody and antigen is mainly determined by the complementarity of spatial structure. For the DNAzyme, generally, one ring of DNAzyme binds to metal ions, and another ring specifically binds to the targets. The DNAzyme only can be cleaved when both

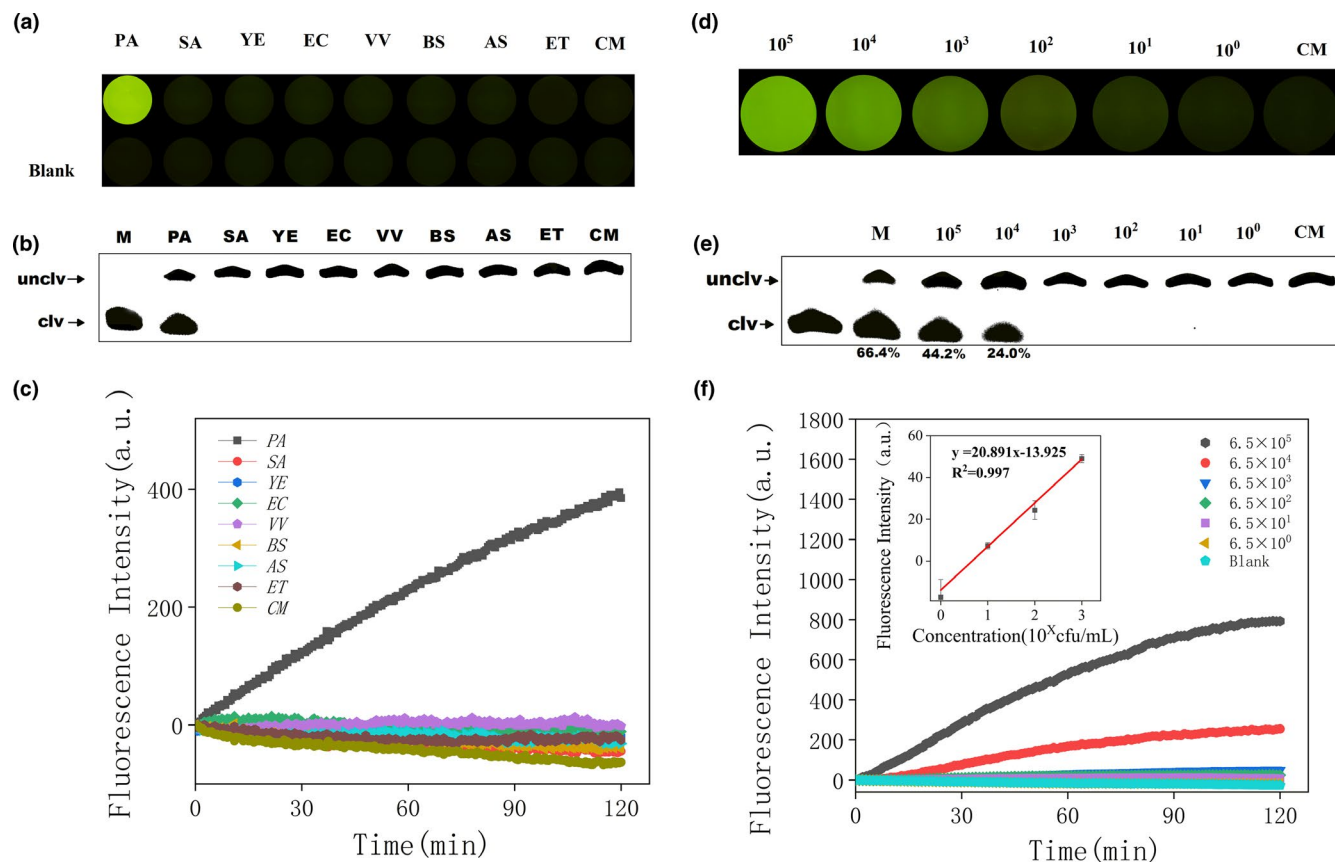

**FIGURE 4** (a) indicator plate images of PAE-1 specific detection after 10 min. PA: *Pseudomonas aeruginosa*; SA: *Staphylococcus aureus*; YE: *Yersinia enterocolitica*; EC: *Escherichia coli*; VV: *Vibrio vulnificus*; BS: *Bacillus subtilis*; AS: *Aeromonas salmonicida*; ET: *Edwardsiella tarda*; CM: Blank complete medium. (b) Image of cleavage gel for PAE-1 specificity detection within 2 hr. (c) Biosensor-based assay of PAE-1 in blank culture medium and seven different bacteria. Gel image (e), indicator plate (d), and biosensor measurement (f) of PAE-1 in different concentrations of *Pseudomonas aeruginosa* in CEM-PA. (f) Fluorescence values of *P. aeruginosa* at different concentrations (Blank: ddwater without *P. aeruginosa*). Inset: Analytical calibration curve of fluorescence values of *P. aeruginosa* (concentrations of 6.5,  $6.5 \times 10$ ,  $6.5 \times 10^2$ ,  $6.5 \times 10^3$ ) for 2 hr

the metals and targets are existed. Electrostatic, hydrogen bonding, and hydrophobic interaction promote their combination between DNAzyme and targets (Jin et al., 2021; Park et al., 2021). Aptamers are also called "artificial antibodies" (Agyei et al., 2018), aptamers and DNAzymes can form a tertiary structure and specifically binds to the target (Cui et al., 2020; Kalra et al., 2018).

## 2.5 | Highly sensitive detection

To evaluate the effective detection range of PAE-1 DNAzyme sensor, 10-fold serial dilutions of *P. aeruginosa* bacterial suspensions were produced. The number of *P. aeruginosa* in the present study was determined using a gradient dilution plate method from  $6.5 \times 10^8$  cfu/ml. When 30  $\mu$ L CEM-PA was added to 50  $\mu$ L of detection system on the indicator board sensor, the fluorescence was increased with the concentration of *P. aeruginosa* (Figure 4d). Using PAE-1 DNAzyme sensor, 10  $\mu$ L CEM-PA was added to 100  $\mu$ L of detection system, resulting in a detection limit calculated to be 1.2 cfu/ml (Figure 4f insert). Using dPAGE, 10  $\mu$ L CEM-PA added to 50  $\mu$ L of detection system resulted a clear band at  $1.3 \times 10^4$  cfu/ml (Figure 3e). We

conclude that the fluorescence sensor has the lowest detection limit when using PAE-1 DNAzyme sensor.

## 2.6 | Cleavage ratio

The first-order reaction rate equation  $Y_t = Y_0 + a(1 - e^{-bx})$  was used to conduct dynamic linear curve fitting, in which  $Y_t$  and  $Y_0$  represented the fragment intensity of DNAzyme cleavage for reaction times of  $t$  and 0, respectively, where  $B$  represented the reaction rate constant. Results of fitting indicated that PAE-1 DNAzyme displayed good cleavage performance, with a reaction rate constant of  $0.0167 \text{ min}^{-1}$  (Figure 5d). This rate indicates that the DNAzyme was effective in identifying *P. aeruginosa* using particular conditions.

## 2.7 | Indicator board sensor

We optimized the detection time of PA-1 DNAzyme on the indicator board sensor. According to the fluorescence value detected by the full-wavelength microplate reader (Figure 5a), with the extension of




time, the fluorescence value of PA-1 DNAzyme keeps increasing, and the fluorescence value remains basically unchanged after 10 min. This may indicate that the extracellular product CEM-PA of *P. aeruginosa* has completely cleaved DNAzyme. The dried DNAzyme on the polypropylene vinyl board could quickly reacted when the CEM-PA was added. After 10 min, the DNAzyme was completely cleaved by CEM-PA, and the fluorescence value reached maximum. Meanwhile, the controls could be distinguished by naked eyes under blue light. It indicated that the DNAzyme could maintain its basic structure and recover its reaction from dry state accompanied with CEM-PA solution. So, the drying did not affect the function of DNAzyme. We also tested the storage time of the PA-1 DNAzyme-based biosensor. According to the double verification of the full-wavelength microplate reader and the biosensor (Figure 5b), with the passage of time, the fluorescence value of PA-1 DNAzyme only slightly decreased, which basically remained unchanged, indicating that the DNAzyme-based biosensor can be stored for at least 12 days.

Tap water was added to the *P. aeruginosa* as the test group and tap water as the control group and tested over 3 days. As time progressed, the signal of the sensor in the experimental group increased

gradually, while that of the control group remained essentially unresponsive (Figure 5c). The experiment indicated that the indicator board sensor quickly detected real samples. The present study demonstrates a device able to rapidly determine the presence of *P. aeruginosa* in remote areas. *P. aeruginosa* not only contaminates medical equipment, but also is widely present in tap water. *P. aeruginosa* poses a serious threat to human health, and its identification has been the subject of various studies (Kaur et al., 2015; Zhong et al., 2018). In the present study, a novel strategy was developed for rapid and convenient detection of *P. aeruginosa*.

## 2.8 | Detection of *P. aeruginosa* in food

Black tea contaminated with *P. aeruginosa* contrasted greatly with uncontaminated samples and was easily detected using a blue-light transilluminator (Figure 6a). Although the brightness of the contaminated peach juice was similar to that of black tea, the background light of the control group was also very bright, so it could not be observed directly. From the brightness of the indicator board sensor,

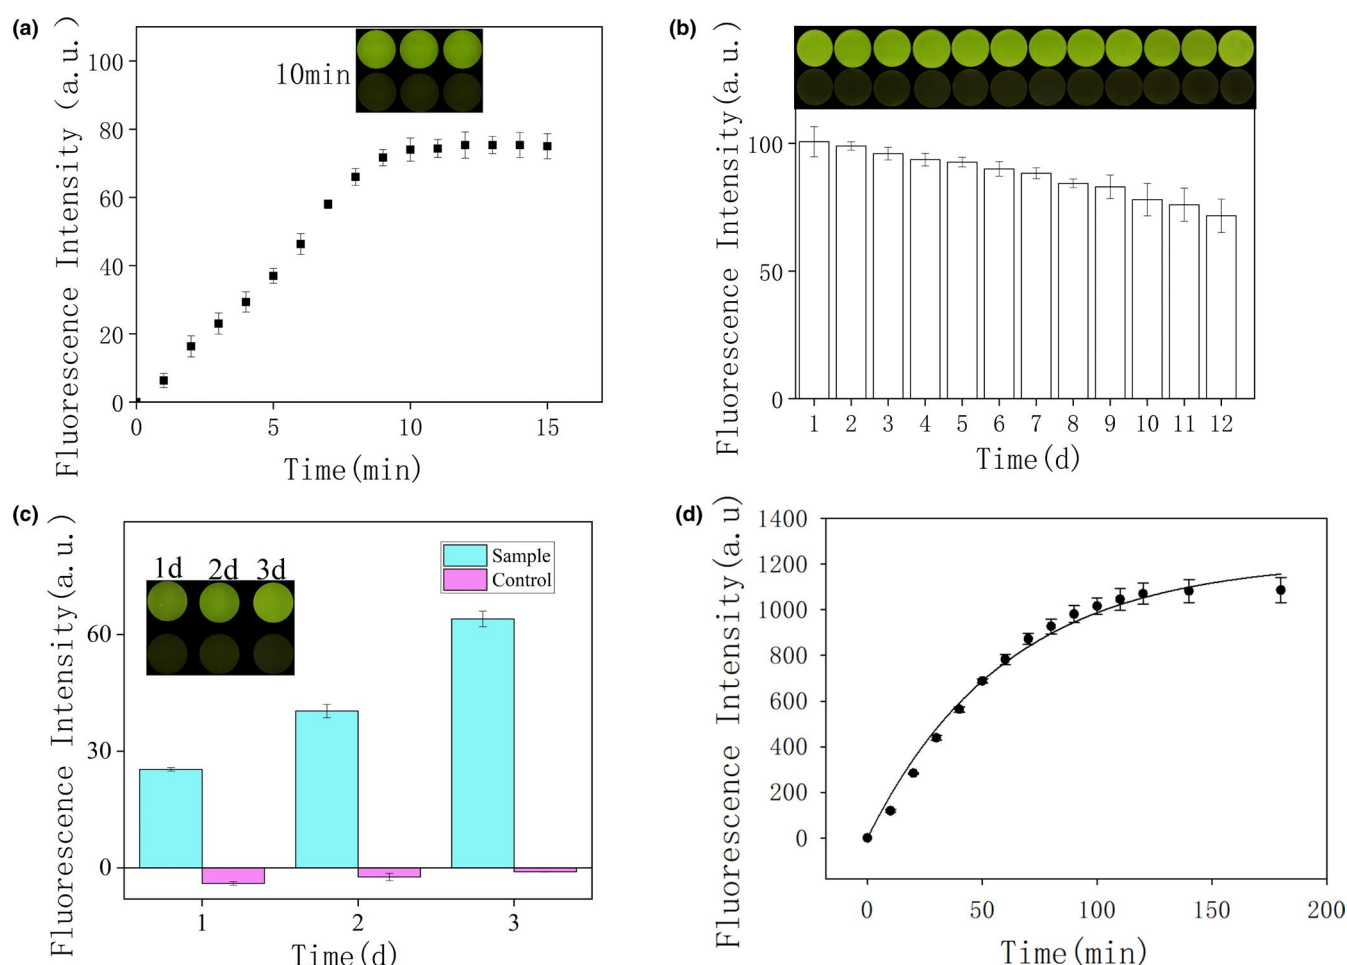

**FIGURE 5** (a) Kinetics of the indicator plate sensor over 15 min. Inset: image of the indicator board sensor after 10 min. (b) Fluorescence intensity of the indicator board sensor after 12 days. Inset: corresponding indicator board sensor image. (c) Comparison of DNAzyme cleavage activity between control and sample. Inset: Image of the indicator board sensor after 10 min after 3 days. (d) The fluorescence intensity of PAE-1 DNAzym in 3 hr. The result of the fitted curve indicates the cleavage rate of PAE-1 DNAzyme

the detection limit of *P. aeruginosa* in black tea was  $6.9 \times 10^2$  cfu/ml (Figure 6b). The results of gel electrophoresis showed the DNAzyme could be cleaved when the *P. aeruginosa* was existed in the samples of black tea, peach juice, hawthorn, and tap water (Figure 6c). The fragment of DNAzyme could be observed in the polyacrylamide gel. DNA for PCR was extracted from  $69 \text{ cfu/ml} - 6.9 \times 10^5 \text{ cfu/ml}$  *P. aeruginosa* in black tea, and 2% agarose gels showed that *P. aeruginosa* DNA remained close to 126 bp (Figure 6d). The results of both were consistent. The DNAzyme-based sensor was able to detect  $6.9 \times 10^2$  cfu/ml *P. aeruginosa* within 10 min.

### 3 | CONCLUSIONS

Here, we obtained the DNAzyme by in vitro selection that was effective for the detection of *P. aeruginosa*. Compared with the previous strategy, the DNAzyme sensor had higher sensitivity. The detection of limit could reach 1.2 cfu/ml. In the pekoe tea contaminated by *P. aeruginosa*, the detection of limit was  $6.9 \times 10^2$  cfu/ml. In particular, the methods did not require equipment and sample pretreatment. The detection of *P. aeruginosa* could be performed in site and obtained the results within 10 min. The DNAzyme sensors also could be easily applied by nontechnicians. For the limitations of DNAzyme sensors, they may interrupt by high concentration metals or extreme acidity and alkalinity in matrix. DNAzymes rely on specific auxiliary metal ions. The background of fluorescence could be affected by the matrix of samples (Cepeda-Plaza & Peracchi, 2020; Cozma et al., 2021). And now, DNAzymes sensors applied in vitro only (Lake et al., 2019). The results provide the possibility of using the DNAzyme to reduce health risks and develop fast and inexpensive biosensors.

## 4 | MATERIALS AND METHODS

### 4.1 | Materials

*Pseudomonas aeruginosa*, *Yersinia enterocolitica*, *Aeromonas salmonicida*, *Vibrio anguillarum*, *V. vulnificus*, and *Edwards tarda* were bought from the China Center of Industrial Culture Collection (CICC). *Staphylococcus aureus*, *E. coli*, and *Bacillus subtilis* were from the Marine Resources Development Institute of Jiangsu (Lianyungang). Sequences of all oligonucleotides (Table 1) were synthesized by Sangon Biotech (Shanghai, China). Beef extract, Tween-20, Ethanol absolute, Boracic acid, Tris(hydroxymethyl)aminomethane, NaOH, NaCl,  $\text{MgCl}_2$ , KCl, and the metal salts were purchased from Sinopharm (China). N-(2-Hydroxyethyl)piperazine-N'-(2-ethanesulfonic acid) (HEPES) and 2-(N-morpholino)ethanesulfonic acid (MES) were purchased from Aladdin (China). Deoxynucleotide (dNTP) mix, Taq DNA polymerase with 10×PCR buffer, 6×gel loading dye, and low molecular weight DNA ladder were obtained from New England Biolabs (Shanghai, China). Agarose was acquired from Biowest (Chai wan, Hong Kong). Tryptone and yeast extract powder were obtained from Oxoid (Hampshire, England). Buffer I was 10 mM Tris-HCL

(pH7.5), 1 mM EDTA, 1 M NaCl, 0.01% ~ 0.1% Tween-20, Buffer II was 100 mM HEPES (pH7.5), 300 mM NaCl, 30 mM  $\text{MgCl}_2$ , 0.02% Tween-20. Distilled deionized water (ddwater 18.5 MΩ cm, MilliQ system) was used. All reagents were of analytical grade.

### 4.2 | Methods

#### 4.2.1 | Preparation of screening library

The random library and its corresponding PCR primers were designed. Primer 1 was designed first, and then, primer 2 was designed according to primer 1. The 5' end of primer 2 contains biotin and a cleavage site in the middle. The library was constructed by primer 1 and primer 2. In the middle of the library are 35 random sequences randomly generated by Sangon Biotech (Shanghai, China). The 5' end of the library is phosphorylated. Primer Premier 5.0 software was used to design primer sequences to avoid hairpin formations and dimers, maximizing PCR efficiency. DNA sequences used in the experiments are listed in Table 1.


The initial library was prepared by PCR for screening for the DNAzyme. PCR reaction mixtures (50 μl) included cleaved DNA product (starting with Lib-N35-pool, 2 ~ 100 ng/μl), 1 μl each of forward primer (10 μmol/L) and reverse primer (10 μmol/L), 3 μl  $\text{MgCl}_2$  (25 mM), 1 μl dNTPs (10 mM), 1 μl Taq DNA polymerase (5 U/μl), 5 μl 10×PCR buffer (100 mM Tris-HCl, pH 8.8, 25°C, 500 mM KCl, 0.8% (v/v) NP-40), and 37 μl ddwater. PCR was conducted using the following thermocycling protocol: 94°C for 5 min, then the optimal number of cycles of 94°C for 30 s, 56°C for 30 s, and 72°C for 1 min. A final extension was performed at 72°C for 2 min. In addition, all PCR products were further concentrated by ethanol precipitation (as described in 1.2).

To determine the optimal number of cycles, PCR products were assessed every two cycles from 9 to 27 cycles. The products were checked by 2% agarose gel electrophoresis stained with Gel-red, and the optimal number determined from the results observed on a Gel Doc™ EZ (Bio-Rad, USA). This number of cycles was then used to enrich the DNA.

#### 4.2.2 | Oligonucleotide purification and recovery

##### DNA purification using 10% dPAGE Gel

The DNA library and primers were purified separately. DNA sequences were diluted with ddwater to 10 μM. Ten percent denaturing polyacrylamide gel electrophoresis (dPAGE) was used to purify the DNA using 1×TBE at 120 volts (V) for 45 min for the DNA library and 20 min for primers. The gel was observed using UV light. Target bands were cut into pieces and macerated, and 300 μl DNA elution buffer added. EP tubes were placed on a thermo-mixer and mixed at 500 r/min at 37°C for 1 hr. The samples were then centrifuged at 13,800 g for 5 min at 4°C, after which 200 μl DNA supernatant was aspirated and transferred to fresh 1.5 ml EP tubes.

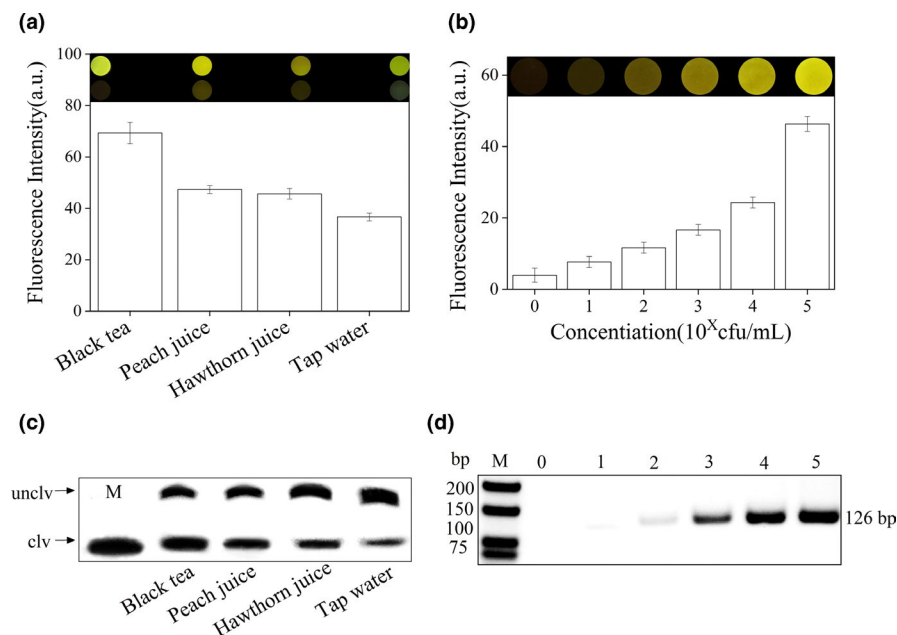

**FIGURE 6** (a) Black tea, peach juice, hawthorn juice, and tap water artificially contaminated with *P. aeruginosa*, with uncontaminated samples as controls. Using a blue-light transilluminator, fluorescence values are displayed equal to the experimental group minus the control group. (b) Fluorescence value and brightness of  $6.9 \text{ cfu/mL}$ – $6.9 \times 10^5 \text{ cfu/mL}$  *P. aeruginosa* in black tea. (c) Detection of *P. aeruginosa* in denaturing polyacrylamide gel. M: DNAzyme was completely cleaved by *P. aeruginosa*. (d) PCR amplification results of  $6.9 \text{ cfu/mL}$ – $6.9 \times 10^5 \text{ cfu/mL}$  *P. aeruginosa*

| DNA name      | DNA sequence (5'–3')                                        |
|---------------|-------------------------------------------------------------|
| Lib-N35-pool  | pGGACAAGAGGGGGATCTTGT-N <sub>35</sub> -GTTGTCAGCAGTCTGTCCAT |
| Primer 1 (P1) | ATGGACAGACTGCTGACAAC                                        |
| Primer 2 (P2) | Biotin-TGCTGACAACrAGGACAAGAGGGGGA                           |
| FAM-substrate | FAM-ATGGACAGACTGCTGACAACrAGGA CAAGAGGGGGA                   |

**TABLE 1** DNA Sequences for in vitro Selection<sup>a</sup>

Note: DNAzyme is a functional nucleic acid, a single-stranded DNA molecule with catalytic activity, that can be isolated from random DNA libraries by selection technology. We successfully screened the DNAzyme (PAE-1) with high specificity and sensitivity to directly detect *P. aeruginosa* without secondary elution. The PAE-1 could detect *P. aeruginosa* at  $1.2 \text{ cfu/mL}$  in 10 min using our designed DNAzyme-based sensor.

<sup>a</sup>p: phosphorylation; N35: 35 random nucleotides; The ribose adenine cleavage site is represented by rA; FAM: Carboxyfluorescein.

#### DNA recovery by ethanol precipitation

Sodium acetate (3 M, pH 5.2) was added 20  $\mu\text{L}$ . A 900  $\mu\text{L}$  volume of ice-cold 100% ethanol was then added and then thoroughly mixed prior to cooling to  $-20^\circ\text{C}$  for 1 h. After centrifugation at 12,000 r/min for 20 min at  $4^\circ\text{C}$ , the supernatant was discarded. The sample was rinsed in 70% ice-cold ethanol and again centrifuged. Finally, the sample was dried in a vacuum drying centrifuge at  $37^\circ\text{C}$  for 20–30 min, until the ethanol had completely evaporated.

#### 4.2.3 | Preparation of CEMs

*Pseudomonas aeruginosa* was cultured in Luria-Bertani broth (LB) at  $30^\circ\text{C}$  and agitated at 180 r/min until the optical density at 600 nm ( $\text{OD}_{600}$ ) was approximately 1.0. The broth was centrifuged at 13,800 g for 5 min at room temperature from which the supernatant was collected as a CEM. The CEM was stored at  $-20^\circ\text{C}$  until

required for additional experimentation. In addition, the number of *P. aeruginosa* cells was counted using a counting plate method. Other bacteria were cultured using optimal growth conditions, and CEMs similarly collected.

#### 4.2.4 | In vitro selection procedures

##### Linking magnetic beads with the library

Fifty microliters of streptavidin (50 mg/mL) coated magnetic beads (0.5  $\mu\text{m}$  in diameter, fully shaken, and resuspended prior to use) were mixed with 500  $\mu\text{L}$  Buffer I in a centrifuge tube. The magnetic beads were fully resuspended then separated magnetically. This procedure was repeated three times to wash the magnetic beads. The purified PCR product containing the biotin tag was dissolved in 500  $\mu\text{L}$  Buffer I and mixed with magnetic beads (5 mg/mL). The mixture was placed on a DNA mixer and incubated at  $37^\circ\text{C}$  for 30 min. It was then placed



in a magnetic separator for 1 min, after which the supernatant was removed.

#### Positive screening

The magnetic beads were suspended in 150  $\mu$ l of Buffer II. A 150  $\mu$ l aliquot of the CEM of *P. aeruginosa* (CEM-PA) was then added. Screening was performed on a DNA mixer at 37°C for 1 hr. In rounds 1–5 of screening, the duration of reaction was 1 hr. In subsequent rounds, the reaction time was 50, 40, and 30 min for rounds 6–8, respectively.

#### Negative screening

Negative screening was performed during the third and fifth rounds. Magnetic beads were suspended in 150  $\mu$ l of Buffer II. A 150  $\mu$ l aliquot of CEM was mixed with *V. anguillarum*, *E. coli*, and *S. aureus* and reacted in a DNA mixer at 37°C for 1 hr. The magnetic beads were separated and washed twice with Buffer II.

#### Creation of each new library and ratio of cleavage

After screening, the tube was placed on a magnetic separator for 1 min and the supernatant collected and alcohol extracted. The precipitate was used for PCR to restore the new library for the subsequent round of screening. A Q5000 micro-spectrophotometer (Quawell, USA) was used to measure the concentration of the cleavage fragments (concentration = C). All immobilized biotinylated DNA strands (concentration =  $C_0$ ) were released from the magnetic beads by the addition of 10 mM EDTA, pH 8.2 in 95% formamide solution, and incubation at 95°C for 2 min to break the streptavidin-biotin bonds (Ignjatovic et al., 2010). From this, the cleavage fraction was calculated ( $C/C_0$ ).

#### High-throughput sequencing

The screening process was evaluated by comparing the ratio of cleavage for each round of screening. PCR products were assessed by 2% agarose gel electrophoresis and purified by alcohol precipitation, then dissolved in ddwater. A DNA concentration of >1  $\mu$ g/ $\mu$ l was used. Sequencing was performed by Sangon Biotech (Shanghai, China).

### 4.2.5 | PAE-1 DNAzyme sensor based on fluorescence

The DNAzyme sensor molecular beacon was prepared as follows (Ali et al., 2011; Gu et al., 2019). The DNAzyme (10  $\mu$ M) and FAM-labeled substrate (15  $\mu$ M) were heated to 90°C for 5 min then gradually cooled to room temperature (20°C) to form a DNAzyme complex (5  $\mu$ M). An 86  $\mu$ l aliquot of Buffer II, 4  $\mu$ l of 5  $\mu$ M DNAzyme complex, and 10  $\mu$ l of CEM-PA were mixed in the wells of a 96-well plate for measurement of kinetics. The fluorescence intensity of each sample was measured in triplicate in a multi-function full-wavelength microplate reader (Infinite M1000 Pro, Tecan, Switzerland). Emission at a wavelength of 535 nm was measured at intervals of 30 s for 120 min at an excitation wavelength of 485 nm.

### 4.2.6 | Activity assays by dPAGE

The activity of each candidate DNAzyme was analyzed by dPAGE. Four microliters of 5  $\mu$ M DNAzyme complex were mixed with 10  $\mu$ l of CEM and 36  $\mu$ l of Buffer II then incubated for 30 min at room temperature. Termination buffer (200  $\mu$ l 6 $\times$ dPAGE gel loading dye solution and 400  $\mu$ l 8 M urea) was then added. The samples were separated by 15% dPAGE at 150 V for 1 hr, and the percentage cleavage calculated (cleaved plus uncleaved DNA = 100%) using a Bio-Rad Gel Doc™ EZ imaging system.

### 4.2.7 | Activity assays with metal ions and pH

The majority of DNA enzymes require metal ions for activity, and different concentrations of metal ions can significantly affect DNAzyme activity (Du, Li, Chai, et al., 2020; Hwang et al., 2016; Zhou et al., 2021). The addition of EDTA (300 mM) to chelate polyvalent metal ions inhibited cleavage. The effects of  $\text{Na}^+$  at different concentrations (0, 30, 60, 90, 120, 150, 180, 210, 240, 300, 400, and 600 mM) on the activity of PAE-1 DNAzyme were examined. Optimal  $\text{Na}^+$  concentration (30 mM) was used to determine the effect of different concentrations of  $\text{Mg}^{2+}$  (0, 30, 60, 90, 120, 150, 180, 210, 240, 300, 400, or 600 mM) on the activity of PAE-1 DNAzyme. Furthermore, the lytic activity of DNAzyme was measured at a gradually increasing pH.

### 4.2.8 | DNAzyme sensor

The PA-1 DNAzyme was combined with a polystyrene board to fabricate a DNAzyme sensor indicator. Twenty microliters of 5  $\mu$ M DNAzyme complex were mixed with 35.0  $\mu$ l Buffer II in a light-proof tube. A 20  $\mu$ l aliquot of the mixture was then pipetted onto the polystyrene board which was then dried at 50°C for 2 hr. To test its effectiveness, 30  $\mu$ l of CEM-PA was added to the sensor, while, similarly, 30  $\mu$ l of LB broth was added to a control sample. Fluorescence was measured when irradiated with a blue-light transilluminator (Sangon Biotech, Shanghai) or using a microplate reader (excitation 485 nm and emission 535 nm). The sensor was stored at room temperature to assess shelf life.

### 4.2.9 | Detection of *P. aeruginosa* in food

*Pseudomonas aeruginosa* was added to pekoe tea, peach juice, hawthorn juice, and tap water. A control sample without bacteria was measured. A 20  $\mu$ l aliquot of each sample was added to the sensor and incubated for 10 min. Fluorescence was measured when placed in blue-light transilluminator or using a microplate reader. Black tea, which has low background fluorescence was spiked with *P. aeruginosa* ( $6.9 \times 10^8$  cfu/ml) in a dilution gradient. Primers for the 126 bp eta gene in *P. aeruginosa* were

synthesized (primer 1: GACAACGCCCTCAGCATCA; primer 2: CAGCCAGTTCAGCGACCAA). *P. aeruginosa* DNA with the lowest dilution factor was extracted for PCR (reaction program: 94°C for 5 min; 94°C for 30 s; 54°C for 30 s; 72°C for 30 s; total of 35 cycles; 72°C for 2 min final extension) to compare the results with DNAzyme sensor.

## ACKNOWLEDGMENTS

This study was supported by the National Key R&D Program of China (2018YFC0311106). The Priority Academic Program Development of Jiangsu Higher Education Institutions (PAPD). The Research & Practice Innovation Program of Jiangsu (SJCX19-1020, ZD201918).

## CONFLICT OF INTEREST

The authors confirm that there is no conflict of interests regarding this paper.

## DATA AVAILABILITY STATEMENT

The data that support the findings of this study are available from the corresponding author upon reasonable request.

## ORCID

Mingcan Qin  <https://orcid.org/0000-0003-2967-1679>

## REFERENCES

- Aghamollaei, H., Moghaddam, M. M., Kooshki, H., Heiat, M., Mirnejad, R., & Barzi, N. S. (2015). Detection of *Pseudomonas aeruginosa* by a triplex polymerase chain reaction assay based on *lasI/R* and *gyrB* genes. *Journal of Infection and Public Health*, 8(4), 314–322. <https://doi.org/10.1016/j.jiph.2015.03.003>
- Agyei, D., Acquah, C., Tan, K. X., Hii, H. K., Rajendran, S. R. C. K., Udenigwe, C. C., & Danquah, M. K. (2018). Prospects in the use of aptamers for characterizing the structure and stability of bioactive proteins and peptides in food. *Analytical and Bioanalytical Chemistry*, 410(2), 297–306. <https://doi.org/10.1007/s00216-017-0599-9>
- Ali, M. M., Aguirre, S. D., Lazim, H., & Li, Y. (2011). Fluorogenic DNAzyme probes as bacterial indicators. *Angewandte Chemie (International Ed. in English)*, 50(16), 3751–3754. <https://doi.org/10.1002/anie.20110477>
- Ali, M. M., Slepentin, A., Peterson, E., Zhao, W. (2019). A simple DNAzyme-based fluorescent assay for *Klebsiella pneumoniae*. *ChemBioChem*, 20(7), 906–910.
- Ali, M. M., Wolfe, M., Tram, K., Gu, J., Filipe, C. D., Li, Y., & Brennan, J. D. (2019). A DNAzyme-based colorimetric paper sensor for *Helicobacter pylori*. *Angewandte Chemie (International Ed. in English)*, 58(29), 9907–9911.
- Alvarez-Lerma, F., Olaechea-Astigarraga, P., Palomar-Martinez, M., Catalan, M., Nuvials, X., Gimeno, R., Gracia-Arnillas, M. P., & Seijas-Betolaza, I. (2018). Invasive device-associated infections caused by *Pseudomonas aeruginosa* in critically ill patients: Evolution over 10 years. *Journal of Hospital Infection*, 100(3), e204–e208. <https://doi.org/10.1016/j.jhin.2018.04.027>
- Bassetti, M., Vena, A., Croxatto, A., Righi, E., & Guery, B. (2018). How to manage *Pseudomonas aeruginosa* infections. *Drugs in Context*, 7, 212527. <https://doi.org/10.7573/dic.212527>
- Breaker, R. R., & Joyce, G. F. (1994). A DNA enzyme that cleaves RNA. *Chemistry & Biology*, 1(4), 223–229. [https://doi.org/10.1016/1074-5521\(94\)90014-0](https://doi.org/10.1016/1074-5521(94)90014-0)
- Callejas-Díaz, A., Fernández-Pérez, C., Ramos-Martínez, A., Múñez-Rubio, E., Sánchez-Romero, I., & Vargas Núñez, J. A. (2019). Impact of *Pseudomonas aeruginosa* bacteraemia in a tertiary hospital: Mortality and prognostic factors. *Medicina Clínica (English Edition)*, 152(3), 83–89. <https://doi.org/10.1016/j.medcle.2018.12.003>
- Cdc. (2019). *Antibiotic Resistance Threats in the United States*. <https://doi.org/10.15620/cdc:82532>
- Cepeda-Plaza, M., & Peracchi, A. (2020). Insights into DNA catalysis from structural and functional studies of the 8–17 DNAzyme. *Organic & Biomolecular Chemistry*, 18(9), 1697–1709. <https://doi.org/10.1039/c9ob02453k>
- Cohen, R., Babushkin, F., Cohen, S., Afraimov, M., Shapiro, M., Uda, M., Khabra, E., Adler, A., Ben Ami, R., & Paikin, S. (2017). A prospective survey of *Pseudomonas aeruginosa* colonization and infection in the intensive care unit. *Antimicrobial Resistance & Infection Control*, 6, 7. <https://doi.org/10.1186/s13756-016-0167-7>
- Coppy, M., Leroyer, C., Saly, M., Venier, A. G., Slekovec, C., Bertrand, X., Parer, S., Alfandari, S., Cambau, E., Megarbane, B., Lawrence, C., Clair, B., Lepape, A., Cassier, P., Trivier, D., Boyer, A., Boulestreau, H., Asselineau, J., Dubois, V., ... Rogues, A. M. (2020). Exogenous acquisition of *Pseudomonas aeruginosa* in intensive care units: A prospective multi-centre study (DYNAPYO study). *Journal of Hospital Infection*, 104(1), 40–45. <https://doi.org/10.1016/j.jhin.2019.08.008>
- Cozma, I., McConnell, E. M., Brennan, J. D., & Li, Y. (2021). DNAzymes as key components of biosensing systems for the detection of biological targets. *Biosensors & Bioelectronics*, 177, 112972. <https://doi.org/10.1016/j.bios.2021.112972>
- Cui, X., Song, M., Liu, Y., Yuan, Y., Huang, Q., Cao, Y., & Lu, F. (2020). Identifying conformational changes of aptamer binding to theophylline: a combined biolayer interferometry, surface-enhanced Raman spectroscopy, and molecular dynamics study. *Talanta*, 217, 121073. <https://doi.org/10.1016/j.talanta.2020.121073>
- Du, J., Li, Y., Yang, B., Zhang, Y., & Zhu, S. (2020). Allosteric DNA molecular beacons: Using a novel mechanism to develop universal biosensor arrays to fully discriminate DNA/RNA analogues. *Sensors and Actuators B: Chemical*, 311, 127908.
- Du, S., Li, Y., Chai, Z., Shi, W., & He, J. (2020). Functionalization of 8–17 DNAzymes modulates catalytic efficiency and divalent metal ion preference. *Bioorganic Chemistry*, 94, 103401. <https://doi.org/10.1016/j.bioorg.2019.103401>
- Feng, W., Huang, Q., Wang, Y., Yuan, Q., Li, X., Xia, P., & Sun, F. (2019). Changes in the resistance and epidemiological characteristics of *Pseudomonas aeruginosa* during a ten-year period. *Journal of Microbiology, Immunology, and Infection*, 54(2), 261–266. <https://doi.org/10.1016/j.jmii.2019.08.017>
- Garvey, M. I., Bradley, C. W., Tracey, J., & Oppenheim, B. (2016). Continued transmission of *Pseudomonas aeruginosa* from a wash hand basin tap in a critical care unit. *Journal of Hospital Infection*, 94(1), 8–12. <https://doi.org/10.1016/j.jhin.2016.05.004>
- Gautam, B. (2021). Microbiological quality assessment (including antibiogram and threat assessment) of bottled water. *Food Sciences and Nutrition*, 9(4), 1980–1988. <https://doi.org/10.1002/fsn3.2164>
- Goncalves-De-Albuquerque, C. F., Silva, A. R., Burth, P., Rocco, P. R. M., Castro-Faria, M. V., & Castro-Faria-Neto, H. C. (2016). Possible mechanisms of *Pseudomonas aeruginosa*-associated lung disease. *International Journal of Medical Microbiology*, 306(1), 20–28. <https://doi.org/10.1016/j.ijmm.2015.11.001>
- Gu, L., Yan, W., Wu, H., Fan, S., Ren, W., Wang, S., Lyu, M., & Liu, J. (2019). Selection of DNAzymes for sensing aquatic bacteria: *Vibrio anguillarum*. *Analytical Chemistry*, 91(12), 7887–7893. <https://doi.org/10.1021/acs.analchem.9b01707>
- Guo, L., Yu, Y., Xu, W. L., Li, C. D., Liu, G. Q., Qi, L., Luo, J. X., & Guo, Y. S. (2020). Simultaneous detection of ovine and caprine DNA in meat and dairy products using triplex TaqMan real-time PCR. *Food Sciences and Nutrition*, 8(12), 6467–6476.

- Huang, L., Chen, J., Yu, Z., & Tang, D. (2020). Self-powered temperature sensor with seebeck effect transduction for photothermal-thermoelectric coupled immunoassay. *Analytical Chemistry*, 92(3), 2809–2814. <https://doi.org/10.1021/acs.analchem.9b05218>
- Hwang, K., Hosseinzadeh, P., & Lu, Y. (2016). Biochemical and biophysical understanding of metal ion selectivity of DNazymes[J]. *Inorganica Chimica Acta*, 452, 12–24. <https://doi.org/10.1016/j.ica.2016.04.017>
- Ignjatovic, V., Straka, E., Summerhayes, R., & Monagle, P. (2010). Age-specific differences in binding of heparin to plasma proteins. *Journal of Thrombosis and Haemostasis*, 8(6), 1290–1294. <https://doi.org/10.1111/j.1538-7836.2010.03847.x>
- Jin, Z., Wang, L., Cao, D., Zou, S., Chen, C., Kang, H., Song, Q., Wang, H., & Tang, Y. (2021). A new method for rapid screening of hybridoma cell clones secreting paired antibodies using sandwich cell surface fluorescence immunosorbent assay. *Analytica Chimica Acta*, 1163, 338493. <https://doi.org/10.1016/j.aca.2021.338493>
- Kalra, P., Dhiman, A., Cho, W. C., Bruno, J. G., & Sharma, T. K. (2018). Simple methods and rational design for enhancing aptamer sensitivity and specificity. *Frontiers in Molecular Biosciences*, 5, 41. <https://doi.org/10.3389/fmolb.2018.00041>
- Karaky, N., Kirby, A., McBain, A. J., Butler, J. A., El Mohtadi, M., Banks, C. E., & Whitehead, K. A. (2020). Metal ions and graphene-based compounds as alternative treatment options for burn wounds infected by antibiotic-resistant *Pseudomonas aeruginosa*. *Archives of Microbiology*, 202(5), 995–1004. <https://doi.org/10.1007/s00203-019-01803-z>
- Kaur, G., Raj, T., Kaur, N., & Singh, N. (2015). Pyrimidine-based functional fluorescent organic nanoparticle probe for detection of *Pseudomonas aeruginosa*. *Organic & Biomolecular Chemistry*, 13(16), 4673–4679. <https://doi.org/10.1039/c5ob00206k>
- Krithiga, N., Viswanath, K. B., Vasantha, V. S., & Jayachitra, A. (2016). Specific and selective electrochemical immunoassay for *Pseudomonas aeruginosa* based on pectin-gold nano composite. *Biosensors & Bioelectronics*, 79, 121–129. <https://doi.org/10.1016/j.bios.2015.12.006>
- Kumar, S., Jain, S., Dilbaghi, N., Ahluwalia, A. S., Hassan, A. A., & Kim, K.-H. (2019). Advanced selection methodologies for dnazymes in sensing and healthcare applications. *Trends in Biochemical Sciences*, 44(3), 190–213. <https://doi.org/10.1016/j.tibs.2018.11.001>
- Lake, R. J., Yang, Z., Zhang, J., & Lu, Y. (2019). DNazymes as activity-based sensors for metal ions: recent applications, demonstrated advantages, current challenges, and future directions. *Accounts of Chemical Research*, 52(12), 3275–3286. <https://doi.org/10.1021/acs.accounts.9b00419>
- Langendonk, R. F., Neill, D. R., & Fothergill, J. L. (2021). The building blocks of antimicrobial resistance in *Pseudomonas aeruginosa*: Implications for current resistance-breaking therapies. *Frontiers in Cellular and Infection Microbiology*, 11(307), 665759. <https://doi.org/10.3389/fcimb.2021.665759>
- Li, W., Zhang, Z., Zhou, W., & Liu, J. (2017). Kinetic discrimination of metal ions using DNA for highly sensitive and selective Cr(3+) detection. *ACS Sensors*, 2(5), 663–669.
- Li, Y. (2011). Advancements in using reporter DNazymes for identifying pathogenic bacteria at speed and with convenience. *Future Microbiology*, 6(9), 973–976. <https://doi.org/10.2217/fmb.11.79>
- Lin, Y., Zhou, Q., & Tang, D. (2017). Dopamine-loaded liposomes for in-situ amplified photoelectrochemical immunoassay of AFB1 to enhance photocurrent of Mn2+-Doped Zn3(OH)2V2O7 Nanobelts. *Analytical Chemistry*, 89(21), 11803–11810.
- Lin, Y., Zhou, Q., Tang, D., Niessner, R., & Knopp, D. (2017). Signal-on photoelectrochemical immunoassay for aflatoxin B1 based on enzymatic product-etching MnO2 nanosheets for dissociation of carbon dots. *Analytical Chemistry*, 89(10), 5637–5645. <https://doi.org/10.1021/acs.analchem.7b00942>
- Ma, L., Kartik, S., Liu, B., & Liu, J. (2019). From general base to general acid catalysis in a sodium-specific DNzyme by a guanine-to-adenine mutation. *Nucleic Acids Research*, 47(15), 8154–8162. <https://doi.org/10.1093/nar/gkz578>
- Ma, L., & Liu, J. (2019). An in vitro-selected DNzyme mutant highly specific for Na(+) under slightly acidic conditions. *ChemBioChem*, 20(4), 537–542. <https://doi.org/10.1002/cbic.201800322>
- Mccarthy, K. L., & Paterson, D. L. (2017). Long-term mortality following *Pseudomonas aeruginosa* bloodstream infection. *Journal of Hospital Infection*, 95(3), 292–299. <https://doi.org/10.1016/j.jhin.2016.11.014>
- Mcconnell, E. M., Morrison, D., Rey Rincon, M. A., Salena, B. J., & Li, Y. (2020). Selection and applications of synthetic functional DNAs for bacterial detection. *TrAC Trends in Analytical Chemistry*, 124, 115785. <https://doi.org/10.1016/j.trac.2019.115785>
- Pachori, P., Gothwal, R., & Gandhi, P. (2019). Emergence of antibiotic resistance *Pseudomonas aeruginosa* in intensive care unit; a critical review. *Genes & Diseases*, 6(2), 109–119. <https://doi.org/10.1016/j.gendis.2019.04.001>
- Park, J. H., Bong, J. H., Jung, J., Sung, J. S., Lee, G.-Y., Kang, M.-J., & Pyun, J.-C. (2021). Microbial biosensor for *Salmonella* using anti-bacterial antibodies isolated from human serum. *Enzyme and Microbial Technology*, 144, 109721. <https://doi.org/10.1016/j.enzmt.2020.109721>
- Peng, T., Deng, Z., He, J., Li, Y., Tan, Y., Peng, Y., Wang, X.-Q., & Tan, W. (2020). Functional nucleic acids for cancer theranostics. *Coordination Chemistry Reviews*, 403, 213080. <https://doi.org/10.1016/j.ccr.2019.213080>
- Rashno Tae, S., Khansarinejad, B., Abtahi, H., Najafimosleh, M., & Ghaznavi-Rad, E. (2014). Detection of algD, oprL and exoA genes by new specific primers as an efficient, rapid and accurate procedure for direct diagnosis of *Pseudomonas aeruginosa* strains in clinical samples. *Jundishapur Journal of Microbiology*, 7(10), e13583. <https://doi.org/10.5812/jjm.13583>
- Richards, M., & Marshall, C. (2018). A *Pseudomonas aeruginosa* infection cluster following coronary artery bypass surgery. *Infection, Disease & Health*, 23, S17. <https://doi.org/10.1016/j.idh.2018.09.067>
- Santoro Sw, J. G. (1997). A general purpose RNA-cleaving DNA enzyme. *Proceedings of the National Academy of Sciences of the United States of America*, 94(9), 4262–4266. <https://doi.org/10.1073/pnas.94.9.4262>
- Shahdordizadeh, M., Taghdisi, S. M., Ansari, N., Alebooye Langroodi, F., Abnous, K., & Ramezani, M. (2017). Aptamer based biosensors for detection of *Staphylococcus aureus*. *Sensors and Actuators B: Chemical*, 241, 619–635. <https://doi.org/10.1016/j.snb.2016.10.088>
- Shen, Z., Wu, Z., Chang, D., Chang, D., Zhang, W., Tram, K., Lee, C., Kim, P., Salena, B. J., & Li, Y. (2016). A catalytic DNA activated by a specific strain of bacterial pathogen. *Angewandte Chemie (International Ed. in English)*, 55(7), 2431–2434. <https://doi.org/10.1002/anie.201510125>
- Sismaet, H. J., Webster, T. A., & Goluch, E. D. (2014). Up-regulating pyocyanin production by amino acid addition for early electrochemical identification of *Pseudomonas aeruginosa*. *Analyst*, 139(17), 4241–4246. <https://doi.org/10.1039/c4an00756e>
- Torabi, S. F., Wu, P., Mcghee, C. E., Chen, L., Hwang, K., Zheng, N., Cheng, J., & Lu, Y. (2015). In vitro selection of a sodium-specific DNzyme and its application in intracellular sensing. *Proceedings of the National Academy of Sciences of the United States of America*, 112(19), 5903–5908. <https://doi.org/10.1073/pnas.1420361112>
- Tram, K., Kanda, P., Salena, B. J., Huan, S., & Li, Y. (2014). Translating bacterial detection by DNazymes into a litmus test. *Angewandte Chemie (International Ed. in English)*, 53(47), 12799–12802. <https://doi.org/10.1002/anie.201407021>
- Tumbarello, M., Raffaelli, F., Peghin, M., Losito, A. R., Chirico, L., Giuliano, G., Spanu, T., Sartor, A., Fiori, B., & Bassetti, M. (2020). Characterisation and risk factor profiling of *Pseudomonas aeruginosa* urinary tract infections: Pinpointing those likely to be caused by multidrug-resistant strains. *International Journal of Antimicrobial Agents*, 55(4), 105900. <https://doi.org/10.1016/j.ijantimicag.2020.105900>

- Wang, H., Liu, Y., & Liu, G. (2018). Label-free biosensor using a silver specific RNA-cleaving DNAzyme functionalized single-walled carbon nanotube for silver ion determination. *Nanomaterials (Basel)*, 8(4), 258. <https://doi.org/10.3390/nano8040258>
- Wang, L., Lyu, S., Gu, G., & Bolten, S. (2020). Selection of aptamers targeted to food-borne pathogenic bacteria *Vibrio parahaemolyticus*. *Food Sciences and Nutrition*, 8(7), 3835–3842. <https://doi.org/10.1002/fsn3.1677>
- Woodford, N., & Livermore, D. M. (2009). Infections caused by Gram-positive bacteria: A review of the global challenge. *Journal of Infection*, 59, S4–S16. [https://doi.org/10.1016/S0163-4453\(09\)60003-7](https://doi.org/10.1016/S0163-4453(09)60003-7)
- Yu, T., Zhou, W., & Liu, J. (2018). Ultrasensitive DNAzyme-based Ca(2+) detection boosted by ethanol and a solvent-compatible scaffold for Aptazyme design. *ChemBioChem*, 19(1), 31–36. <https://doi.org/10.1002/cbic.201700498>
- Zhang, W., Feng, Q., Chang, D., Tram, K., & Li, Y. (2016). In vitro selection of RNA-cleaving DNAzymes for bacterial detection. *Methods*, 106, 66–75. <https://doi.org/10.1016/j.ymeth.2016.03.018>
- Zhang, X., Xie, G., Gou, D., Luo, P., Yao, Y., & Chen, H. (2019). A novel enzyme-free electrochemical biosensor for rapid detection of *Pseudomonas aeruginosa* based on high catalytic Cu-ZrMOF and conductive Super P. *Biosensors and Bioelectronics*, 142, 111486. <https://doi.org/10.1016/j.bios.2019.111486>
- Zhong, Z., Gao, X., Gao, R., & Jia, L. (2018). Selective capture and sensitive fluorometric determination of *Pseudomonas aeruginosa* by using aptamer modified magnetic nanoparticles. *Mikrochimica Acta*, 185(8), 377. <https://doi.org/10.1007/s00604-018-2914-3>
- Zhou, Q., & Tang, D. (2020). Recent advances in photoelectrochemical biosensors for analysis of mycotoxins in food. *TrAC Trends in Analytical Chemistry*, 124, 115814. <https://doi.org/10.1016/j.trac.2020.115814>
- Zhou, W., Ding, J., & Liu, J. (2017). Theranostic DNAzymes. *Theranostics*, 7(4), 1010–1025. <https://doi.org/10.7150/thno.17736>
- Zhou, W., Xu, L., & Jiang, B. (2021). Target-initiated autonomous synthesis of metal-ion dependent DNAzymes for label-free and amplified fluorescence detection of kanamycin in milk samples. *Analytica Chimica Acta*, 1148, 238195. <https://doi.org/10.1016/j.aca.2020.12.070>
- Zhou, Z., Zhang, Y., Guo, M., Huang, K., & Xu, W. (2020). Ultrasensitive magnetic DNAzyme-copper nanoclusters fluorescent biosensor with triple amplification for the visual detection of *E. coli* O157:H7. *Biosensors and Bioelectronics*, 167, 112475. <https://doi.org/10.1016/j.bios.2020.112475>

**How to cite this article:** Qin M, Ma X, Fan S, et al. Rapid detection of *Pseudomonas aeruginosa* using a DNAzyme-based sensor. *Food Sci Nutr*. 2021;00:1–12. <https://doi.org/10.1002/fsn3.2367>