

Accepted Manuscript

A novel electrochemical biosensor based on Fe₃O₄ nanoparticles-polyvinyl alcohol composite for sensitive detection of glucose

Niuosha Sanaeifar, Mohammad Rabiee, Mojgan Abdolrahim, Mohammadreza Tahriri, Daryoosh Vashaei, Lobat Tayebi

PII: S0003-2697(16)30411-0

DOI: [10.1016/j.ab.2016.12.006](https://doi.org/10.1016/j.ab.2016.12.006)

Reference: YABIO 12573

To appear in: *Analytical Biochemistry*


Received Date: 11 September 2016

Revised Date: 8 December 2016

Accepted Date: 9 December 2016

Please cite this article as: N. Sanaeifar, M. Rabiee, M. Abdolrahim, M. Tahriri, D. Vashaei, L. Tayebi, A novel electrochemical biosensor based on Fe₃O₄ nanoparticles-polyvinyl alcohol composite for sensitive detection of glucose, *Analytical Biochemistry* (2017), doi: 10.1016/j.ab.2016.12.006.

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

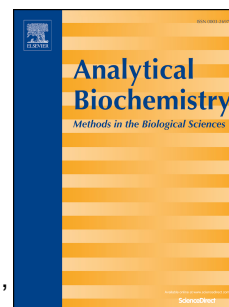

A Novel Electrochemical Biosensor Based on Fe₃O₄ Nanoparticles-Polyvinyl Alcohol Composite for Sensitive Detection of Glucose

Niuosha Sanaeifar¹, Mohammad Rabiee¹, Mojgan Abdolrahim¹, Mohammadreza Tahriri^{1,2*},
Daryoosh Vashae³, Lobat Tayebi^{2,4#}

¹ Biomaterial Group, Faculty of Biomedical Engineering, Amirkabir University of Technology,
Tehran, Iran

² Marquette University School of Dentistry, Milwaukee, WI, 53233, USA

³ Electrical and Computer Engineering Department, North Carolina State University, Raleigh, NC
27606, USA

⁴ Department of Engineering Science, University of Oxford, Oxford OX1 3PJ, UK

* Corresponding Author:

mohammadreza.tahriri@marquette.edu

Co-corresponding Author:

lobat.tayebi@marquette.edu

Abstract

In this research, a new electrochemical biosensor was constructed for the glucose detection. Iron oxide nanoparticles (Fe₃O₄) were synthesized through co-precipitation method. Polyvinyl alcohol-Fe₃O₄ nanocomposite was prepared by dispersing synthesized nanoparticles in the polyvinyl alcohol (PVA) solution. Glucose oxidase (GOx) was immobilized on the PVA-Fe₃O₄

nanocomposite via physical adsorption. The mixture of PVA, Fe_3O_4 nanoparticles and GOx was drop cast on a tin (Sn) electrode surface (GOx/PVA- Fe_3O_4 /Sn). The Fe_3O_4 nanoparticles were characterized by X-ray diffraction (XRD). Also, Fourier transform infrared (FTIR) spectroscopy and field emission scanning electron microscopy (FE-SEM) techniques were utilized to evaluate the PVA- Fe_3O_4 and GOx/PVA- Fe_3O_4 nanocomposites. The electrochemical performance of the modified biosensor was investigated using electrochemical impedance spectroscopy (EIS) and cyclic voltammetry (CV). Presence of Fe_3O_4 nanoparticles in the PVA matrix enhanced the electron transfer between enzyme and electrode surface and the immobilized GOx showed excellent catalytic characteristic toward glucose. The GOx/PVA- Fe_3O_4 /Sn bioelectrode could measure glucose in the range from 5×10^{-3} to 30 mM with a sensitivity of $9.36 \mu\text{A mM}^{-1}$ and exhibited a lower detection limit of 8 μM at a signal-to-noise ratio of 3. The value of Michaelis-Menten constant (K_M) was calculated as 1.42 mM. The modified biosensor also has good anti-interfering ability during the glucose detection, fast response (10 s), good reproducibility and satisfactory stability. Finally, the results demonstrated that the GOx/PVA- Fe_3O_4 /Sn bioelectrode is promising in biosensor construction.

Keywords: Biosensor, Electrochemical, Glucose, Fe_3O_4 nanoparticles, Poly(vinyl alcohol), Electrode

1. Introduction

The accurate detection of glucose concentration is vital in various fields such as biology, biochemistry, clinical chemistry and food analysis. For this aim, glucose biosensor is widely used for determination of glucose in blood and food [1-5]. Between several detection methods, electrochemical biosensors have attracted considerable attention due to their excellent

selectivity, simplicity and low cost [4, 6]. Electrochemical techniques, particularly amperometric biosensors based on glucose oxidase (GOx) immobilization, which can catalyze the oxidation of glucose, have been widely used in glucose sensing [7-9].

Different types of nanomaterials with various size, shapes, physical and chemical properties owing to advances in synthetic methodologies are being extensively used in biosensors [10-16]. These materials exhibit significant benefits due to their small size, large surface-to-volume ratio, optical characteristics and high catalytic properties compared to macroscale materials. Because of their adsorption ability, they are useful for the immobilization of biomolecules such as GOx [17-20]. Moreover, the capability of nanoparticles in electron transfer improvement between electrode and active site of the enzyme make them suitable for applying in enzymatic biosensors applications [17]. Wide variety of metal nanoparticles including gold (Au) [21, 22], silver (Ag) [23], palladium (Pd) [24], platinum (Pt) [25, 26] and metal oxide [27] nanoparticles have been extensively used to construct different sensors, due to their unique features [28]. In recent years, Fe_3O_4 magnetic nanoparticles have attracted a lot of attention in many fields such as biotechnology, pharmacy, cell separation and drug delivery, owing to their interesting properties including biocompatibility, low toxicity, strong supermagnetism, catalytic activity and the ease of preparation process. These magnetic nanoparticles are appropriate for immobilization of different biomolecules such as enzymes. Therefore, it would be promising to use them in biosensor applications [29-33]. It must be mentioned that, by modifying these nanoparticles, using conductive polymers and biopolymers, can be overcome the problems of aggregation and rapid degradation [17].

A number of polymers have been used to stabilize the biomolecules in the design of biosensors. Among them, polyvinyl alcohol (PVA) has been widely utilized as a matrix for entrapment of GOx due to its biocompatibility, non-toxicity, water solubility, good chemical and thermal stability. PVA has large numbers of hydroxyl groups, which provides a biocompatible microenvironment [34, 35].

Xin et al. have studied screen-printed carbon electrode modified by Fe_3O_4 -Au magnetic nanoparticles coated horseradish peroxidase and graphene sheets-nafion film based hydrogen peroxide biosensor [36]. Godarzi et al. have prepared carbon nanotubes decorated by Fe_3O_4 nanoparticles for highly stable and selective non-enzymatic glucose biosensor [37]. Yang et al. have described core-shell Fe_3O_4 -enzyme-polypyrrole nanoparticles for glucose biosensor using potentiometric technique [38]. Tan et al. have prepared PVA/ZnO nanorods composite films for hydrogen peroxide biosensor [39]. Lad et al. have fabricated PVA-silica hybrid films for encapsulation of GOx based glucose biosensor using electrochemical technique [40]. Fang et al. have designed glassy carbon electrode modified by PVA-multiwalled carbon nanotubes-Pt nanoparticles hybrids for non-enzymatic hydrogen peroxide sensor [41].

In this work, a novel glucose biosensor was presented. It was fabricated by dispersing synthesized Fe_3O_4 nanoparticles in the PVA solution and then GOx was immobilized by physical adsorption in the PVA- Fe_3O_4 nanocomposite, drop cast on a tin (Sn) electrode surface (GOx/PVA- Fe_3O_4 /Sn). Finally, the characterization and electrochemical performance of the modified biosensor were examined and discussed in this paper.

2. Experimental procedures

2.1. Reagents

Ferrous chloride anhydrous (FeCl_2) and ferric chloride anhydrous (FeCl_3) were products of Sigma–Aldrich. Hydrochloric acid 37% (HCl) was purchased from Scharlau. Sodium hydroxide (NaOH) was bought from Merck. These materials have been used for the synthesis of Fe_3O_4 nanoparticles. PVA (87–89% hydrolyzed, average $M_w = 72000$), D(+)-glucose and GOx (Type VII-S, 250000 U g^{-1}) were obtained from Sigma-Aldrich. Disodium phosphate (Na_2HPO_4) and monopotassium phosphate (KH_2PO_4) were used for preparation of phosphate buffer solution (PBS). All chemicals were used without further purification. Also, distilled water was employed for preparation of all aqueous solution.

2.2. Preparation of Fe_3O_4 nanoparticles

Fe_3O_4 nanoparticles have been synthesized by earlier protocol reported co-precipitation method [42]. 5.2 g (0.03 mol) of FeCl_3 and 2.0 g (0.015 mol) of FeCl_2 ($\text{Fe(II)}:\text{Fe(III)}=0.5$) were dissolved in the aqueous solution containing 0.85 mL of 37% HCl and 25 mL of deoxygenated water with vigorous stirring. The mixed solution of iron salts was added drop-wise into 250 mL of 1.5 M NaOH under vigorous stirring at room temperature. After the complete addition of the cationic solution into alkaline solution, the stirring continued for 30 min to complete the nucleation process and formation of Fe_3O_4 nanoparticles. During the procedure nitrogen gas was bubbling through solution and the measured pH value was between 11-12. The black precipitate was separated by centrifugation at 4000 rpm for 15 min and washed three times with deoxygenated water to remove unreacted reagents and salts (The reaction of hydrochloric

acid and sodium hydroxide produces salt (NaCl)). To neutralize anionic charge on nanoparticles, 500 mL of 0.01 M HCl then added into the mixture with stirring. The magnetic nanoparticles were separated by centrifugation at 4000 rpm for 15 min and deionized water was added to peptize the synthesized Fe_3O_4 nanoparticles (with concentration of 10 mg mL^{-1}).

2.3. Construction of GOx/PVA- Fe_3O_4 /Sn electrode

A PVA (3%) solution was prepared by dissolving 3 g of PVA in 100 mL distilled water under magnetic stirring at 85°C for 2 h. The solutions of glucose oxidase 1, 2, 4, 6 and 8 mg mL^{-1} were prepared in PBS buffer (pH=7). The optimum concentration of glucose oxidase (4 mg mL^{-1}) was chosen by comparing the current response of 5 GOx/PVA- Fe_3O_4 /Sn electrode in the presence of 5 mM glucose concentration, which is described in the results and discussions (section 3.5). All the modified electrodes reported in this study were prepared by 4 mg mL^{-1} glucose oxidase. 100 μL Fe_3O_4 nanoparticles in deionized water (10 mg mL^{-1}) was dispersed in 500 μL PVA solution by vigorous stirring at room temperature. As a result, suspension consisting of PVA and dispersed Fe_3O_4 nanoparticles was obtained. Resulting solution and 250 μL of prepared GOx solution was slowly mixed for 1 minute. Subsequently, 10 μL of this mixture was drop cast on the surface of the Sn electrode and then dried in air at room temperature to fabricate GOx/PVA- Fe_3O_4 /Sn electrode.

2.4. Apparatus and measurements

X-ray diffraction (XRD) (Co-K α , Philips) was used to investigate the crystalline structure of Fe_3O_4 nanoparticles and the average crystallite size of Fe_3O_4 nanoparticles were calculated

using PANalytical X'Pert HighScore software according to Scherrer equation. The PVA-Fe₃O₄ and its interaction with GOx were characterized by Fourier transform infrared (FTIR) spectrophotometer (Nicolet, NEXUS 670). Field emission scanning electron microscopy (FE-SEM) (TESCAN, Mira 3-XMU) was used to study the surface morphology of the prepared nanocomposite films. Electrochemical impedance spectroscopy (EIS) was performed on PVA/Sn, PVA-Fe₃O₄/Sn electrode and GOx/PVA-Fe₃O₄/Sn bioelectrode with 4 mg mL⁻¹ GOx in the absence of glucose in the frequency range, 0.01 to 10⁵ Hz. Cyclic voltammetry (CV) of PVA/Sn film, PVA-Fe₃O₄/Sn electrode and GOx/PVA-Fe₃O₄/Sn bioelectrode with 4 mg mL⁻¹ GOx were investigated between -0.9 and 0.7 V with the scan rate of 50 mVs⁻¹. All electrochemical measurements were carried out on an Autolab Potentiostat/Galvanostat at room temperature in PBS buffer (pH=7) solution, utilizing three-electrode system with a Sn electrode as working electrode, a Pt wire as auxiliary electrode and an Ag/AgCl electrode as reference.

3. Results and discussion

3.1. Characterization of Fe₃O₄ nanoparticles, PVA-Fe₃O₄ nanocomposite and GOx/PVA-Fe₃O₄/Sn electrode

Fig. 1 shows the XRD pattern of the synthesized Fe₃O₄ nanoparticles. The 2θ values of the Fe₃O₄ nanoparticle 21.3°, 34.9°, 41.5°, 50.3°, 62.6°, 67.0°, and 73.8° correspond to the crystal planes of (111), (220), (311), (400), (422), (511) and (440), respectively, which is quite similar to that reported before for magnetite nanoparticles [43]. The reflection planes are broad, indicating the nanosize of the synthesized Fe₃O₄ particles. No peaks of impurities are

observed in XRD pattern, revealing the high purity of the Fe_3O_4 nanoparticles. The average crystallite size of the Fe_3O_4 nanoparticles, calculated using Scherrer Eq (1):

$$D = \frac{0.9\lambda}{\beta \cos \theta} \quad (1)$$

Where, D is the average crystallite size, λ is the wavelength of X-ray radiation, β is the full width at half the maximum height (rad) and θ is the Bragg's angle in degree. The calculated average crystallite size from (311) diffraction peak is about 3 nm.

(Figure 1)

The FTIR spectrum (see Fig. 2a) displays the major peaks related to pure PVA. The absorption band at 3433.98 cm^{-1} is attributed to the stretching of O-H, 2921.68 cm^{-1} peak is related to the symmetric stretching of CH_2 , 1714.24 cm^{-1} peak is due to carbonyl groups and 1660.66 cm^{-1} peak is assigned to the symmetric stretching of carboxylate anion ($-\text{COO}-$). The peak at 1444.67 cm^{-1} corresponds to the O-H and C-H bending. The band at 1103.16 cm^{-1} can be attributed to the C-O stretching and O-H bending vibrations [40, 44, 45].

The FTIR spectrum of PVA- Fe_3O_4 nanocomposite is represented in Fig. 2b. The absorption band at 629.44 cm^{-1} is associated with the Fe-O stretching vibration and torsional vibration in the tetrahedral and octahedral sites [17]. These results indicate that the Fe_3O_4 nanoparticles are presented in PVA film. Fig. 2b obviously reveals the characteristic absorption bands of PVA and Fe_3O_4 nanoparticles.

The FTIR spectra of GOx and GOx/PVA-Fe₃O₄ nanocomposite are shown in Fig. 2c and 2d, respectively. Two major IR absorption bands related to amide I and II have been extensively used for characterization of GOx. The amide I absorption band appears at 1640.29 cm⁻¹ belonging to the C=O stretching vibration in the protein's backbone. The band at 564.10 cm⁻¹ exhibits the characteristics of N-H bending and C-N stretching of amid II [46]. The FTIR spectrum of the GOx/PVA-Fe₃O₄ nanocomposite shows characteristic absorption bands of GOx and PVA-Fe₃O₄ nanocomposite. Amide I and II IR bands are also observed in the spectrum of GOx/PVA-Fe₃O₄ nanocomposite. However, the peaks that correspond to functional groups of GOx and PVA-Fe₃O₄ nanocomposite overlap, thus the IR peaks shape become broader.

(Figure 2)

The morphology of PVA/Sn film, PVA-Fe₃O₄/Sn electrode and GOx/PVA-Fe₃O₄/Sn bioelectrode were characterized by FE-SEM (see Fig. 3). As shown in Fig. 3a the surface of PVA film seems very smooth, with no cracks or pores. As it was said, the average crystallite size of synthesized Fe₃O₄ nanoparticles is about 3 nm (according to Scherrer equation). Such small nanoparticles joined together and formed large aggregates, in order to minimize their surface energy. Fig. 3b shows that the Fe₃O₄ nanoparticles created small aggregates, after dispersing in PVA matrix. In fact, PVA matrix somehow reduced the aggregates of magnetite nanoparticles. It can be seen from this figure, the surface of PVA-Fe₃O₄ nanocomposite is granular, due to the presence of magnetite nanoparticles. Small size of the magnetite nanoparticles (high surface to volume ratio) is beneficial for immobilization of biomolecules. After the enzyme was immobilized on

the PVA-Fe₃O₄ nanocomposite, the surface morphology has changed (Fig. 3c). It seems that the enzyme molecules were absorbed uniformly on the surface of PVA-Fe₃O₄ nanocomposite, so we can conclude that the enzyme molecules were successfully immobilized on the surface of this nanocomposite.

(Figure 3)

3.2. Electrochemical impedance spectroscopic characterization of the electrodes

The PVA/Sn film, PVA-Fe₃O₄/Sn electrode and GOx/PVA-Fe₃O₄/Sn bioelectrode were monitored by EIS, which is a useful method to understand the features of the electrode surface. The linear part in the Nyquist plot of impedance spectra corresponds to the diffusion process. The semicircle part represents the electron-transfer limited process and its diameter is equal to the electron-transfer resistance, R_{et} , which controls the electron transfer kinetics of the electrode interface. Fig. 4 exhibits the Nyquist plots of the EIS of PVA/Sn, PVA-Fe₃O₄/Sn electrode and GOx/PVA-Fe₃O₄/Sn bioelectrode in phosphate buffer (pH=7) in the frequency range, 0.01 to 10⁵ Hz. The largest semicircle diameter is related to the PVA/Sn film, indicating that PVA film is formed on the electrode surface and act as an insulating layer. The semicircle diameter of PVA-Fe₃O₄ nanocomposite (curve b) is smaller than that of PVA/Sn film (curve a), which suggests that the presence of Fe₃O₄ nanoparticles can act as a nanoscale electrode and facilitate the electron transfer between the electrolyte and electrode. However, after immobilization of GOx on PVA-Fe₃O₄ nanocomposite, the semicircle diameter increased. This suggest that GOx molecules are successfully assembled on the surface of PVA-Fe₃O₄

nanocomposite, which increase the electrode resistance and hinder the electron transfer between the electrolyte solution and electrode surface.

(Figure 4)

3.3. Electrochemical behavior of the modified electrodes

To evaluate the electrochemical characteristics of the modified electrodes, the cyclic voltammetry technique is utilized. Fig. 5 illustrates the cyclic voltammograms of PVA/Sn film, PVA-Fe₃O₄/Sn electrode and GOx/PVA-Fe₃O₄/Sn bioelectrode in phosphate buffer (pH=7) at the scan rate of 50 mVs⁻¹. For the PVA/Sn electrode (curve a) the oxidation and reduction peaks are appeared at 0.07 and -0.19 V respectively. In this curve, the oxidation peak has the minimum current, indicating the formation of PVA layer on the electrode surface, which can act as a barrier for electron transfer between electrolyte solution and the electrode. The incorporation of Fe₃O₄ nanoparticles on to PVA modified Sn electrode surface leads to increase in peak current. This may be assigned to the properties of Fe₃O₄ nanoparticles, which can act as an electron transfer between the enzyme and electrode. However, after immobilization of GOx onto PVA-Fe₃O₄ electrode the peak current is found to increase remarkably. This improved peak current is attributed to the redox characteristics of active sites of the immobilized GOx, which promotes the electron transfer between GOx and electrode.

(Figure 5)

3.4. Effect of scan rate

The CVs of the GOx/PVA-Fe₃O₄/Sn bioelectrode in PBS (pH 7) over the potential range from -0.9 to 0.7 V with different scan rates are exhibited in Fig. 6. As can be seen, both the oxidation and reduction peaks current are increased linearly with increasing scan rates in the range from 10 to 400 mVs⁻¹ with linear correlation coefficient 0.9899, which is shown in the inset of Fig. 6. The peak-to-peak separation (ΔE) has not changed by increasing the scan rates from 10-400 mVs⁻¹ and it is almost independent of the scan rates, indicating that Fe₃O₄ nanoparticles can transfer electrons relatively fast and reversibly in this composite film. These results show that PVA-Fe₃O₄ nanocomposite can provide enough accessibility to electrons to transfer between the enzyme and the electrode. As a result, this nanocomposite can be employed for the immobilization of GOx.

(Figure 6)

3.5. Optimization of experimental variables

3.5.1. Effect of enzyme concentration on the current response of the biosensor

The current response of glucose biosensor can be affected by the amount of GOx loading. Fig. 7 represents the effect of GOx concentration on the performance of the glucose biosensor. The result shows that the current response increases with the increasing of GOx loading for 5 mM glucose concentration. As can be seen, the peak current is saturated, when GOx concentration is more than 4 mg mL⁻¹. Thus, the optimal concentration of GOx for the biosensor is chosen 4 mg mL⁻¹.

(Figure 7)

3.5.2. Effect of pH on the current response of the biosensor

The effect of pH value on the performance of the biosensor is important because the enzymatic activity is affected by pH value. Fig. 8 shows the amperometric response of GOx/PVA-Fe₃O₄/Sn bioelectrode at different pH values. It can be seen, the current response is increased with the increase of pH from 4 to 7 and the maximum current is obtained at pH=7, then decreased at higher pH. The enzyme will be denatured in strong acidic or alkaline conditions, therefore pH =7 is chosen as an optimum for the following study.

(Figure 8)

3.6. Electrochemical response of GOx/PVA-Fe₃O₄/Sn bioelectrode to glucose

Cyclic voltammetry responses of GOx/PVA-Fe₃O₄/Sn bioelectrode with GOx concentration of 4 mg mL⁻¹ in different glucose concentrations in PBS buffer (pH=7) at scan rate of 50 mVs⁻¹ are illustrated in Fig. 9. As can be seen, there are no H₂O₂ redox peaks in the CV measurements. This may be related to the composite of PVA and Fe₃O₄ nanoparticles, which can accept electrons better than oxygen from the reduced enzyme. After enzymatic reaction, the GOx re-oxidized and the PVA-Fe₃O₄ nanocomposite film accepts electrons, therefore causing increases in the redox peaks of PVA-Fe₃O₄ nanocomposite. The redox current peaks are increased with increasing the glucose concentration. The GOx/PVA-Fe₃O₄/Sn bioelectrode has

the response time of 10 s, which is related to the fast electron transfer characteristic of PVA-Fe₃O₄ nanocomposite.

Fig. 9

Fig. 10 displays the glucose calibration plot in the range of 5×10^{-3} to 30 mM. The linear part of the calibration curve in the range of 5×10^{-3} - 2 mM with correlation coefficient of 0.993 shows that the GOx/PVA-Fe₃O₄/Sn bioelectrode has well performance in glucose solution with a sensitivity of $9.36 \mu\text{A mM}^{-1}$. The sensitivity of this bioelectrode is higher than those reported in previous literatures [25, 32]. The limit of detection (LOD) was calculated using the following equation (2):

$$LOD = \frac{K \times S}{m} \quad (2)$$

Where K is the signal-to-noise ratio, S is the standard deviation of y-residuals of regression line and m is the slope of the linear plot. Signal-to-noise ratio is usually chosen to be 2 or 3, which 2 is related to a confidence level of 92.1% and 3 is related to a confidence level of 98.3% [47]. LOD was calculated to be 8 μM at a signal-to-noise ratio of 3 and the standard deviation of y-residuals of 24.96 nA with confidence limits of 13.27 ± 3.89 . The LOD is lower than those calculated in previous reports [25, 48]. The Michaelis-Menten constant (K_m) was calculated from the Lineweaver-Burk equation (3):

$$1/I_{ss} = (K_m/I_{max}) (1/C) + 1/I_{max} \quad (3)$$

Where I_{ss} is the steady-state current, K_m is the Michaelis-Menten constant, I_{max} is the maximum current of the reaction and C is the concentration of the substrate. K_m was obtained

to be 1.42 mM and $I_{\max}$ was 49.9 μA . The calculated K_m is lower than GOx/gold-platinum alloy nanoparticles/carbon nanotubes/chitosan (5.2 mM) [49], chitosan-ferrocene/graphene oxide/GOx (2.1 mM) [50] and GOx immobilized on the ZnO nanotubes (19 mM) [51]. It could be concluded that the modified biosensor has higher affinity to glucose.

(Figure 10)

3.7. Reproducibility and stability of the modified biosensor

The reproducibility of the glucose biosensor is investigated by monitoring the current response of 5 GOx/PVA- Fe_3O_4 /Sn bioelectrode samples in the presence of 5 mM glucose as shown in Table 1. The relative standard deviation (RSD) was calculated using the following equation (4):

$$\text{RSD (\%)} = \frac{\text{Standard deviation}}{\text{Average}} \times 100 \quad (4)$$

The standard deviation, average and RSD were calculated as 1.269, 29.998 and 4.2%, respectively. The RSD was 4.2%, indicating the good reproducibility of the modified enzyme electrode. The modified electrode was kept at 4 °C in PBS when not in used. The current response of biosensor is maintained about 81% of its initial response after a month. The results are suggesting that good stability of biosensor could be attributed to the Fe_3O_4 nanoparticles, which can provide biocompatible environment for immobilization of GOx and stabilize the enzyme bioactivity [1, 17].

(Table 1)

3.8. Interference studies at GOx/PVA-Fe₃O₄/Sn bioelectrode

Fig. 11 shows the effect of different interferents including 0.2 mM uric acid (UA), 0.1 mM ascorbic acid (AA) and 2.5 mM cholesterol with glucose (5 mM) on the GOx/PVA-Fe₃O₄/Sn bioelectrode in phosphate buffer (pH 7) solution. The obtained results indicate that the addition of UA and AA do not cause significant change in current response for the detection of glucose. However, decrease of the peak current for cholesterol in glucose biosensor is observed. It could be concluded that the GOx/PVA-Fe₃O₄/Sn modified electrode displays good anti-interfering ability for the glucose detection.

(Figure 11)

4. Conclusions

We have presented a novel glucose biosensor using PVA-Fe₃O₄ nanocomposite as an ideal matrix for GOx entrapment. The dispersion of Fe₃O₄ nanoparticles in PVA matrix not only promote electron transfer between enzyme and electrode, but also provide a biocompatible environment for enzyme immobilization. The GOx/PVA-Fe₃O₄/Sn bioelectrode performed good electrocatalytic activity with a wide linearity, high sensitivity and low detection limit. In addition, the modified biosensor displayed good anti-interfering capability toward glucose detection, fast response, good reproducibility and satisfactory stability. Finally, the investigations ascertained that the GOx/PVA-Fe₃O₄/Sn bioelectrode has great potential for the construction of biosensors.

References

- [1] L. Yang, X. Ren, F. Tang, and L. Zhang, "A practical glucose biosensor based on Fe₃O₄ nanoparticles and chitosan/nafion composite film," *Biosensors and Bioelectronics*, vol. 25, pp. 889-895, 2009.
- [2] J. Lin, C. He, Y. Zhao, and S. Zhang, "One-step synthesis of silver nanoparticles/carbon nanotubes/chitosan film and its application in glucose biosensor," *Sensors and Actuators B: Chemical*, vol. 137, pp. 768-773, 2009.
- [3] B. Bahmani, F. Moztarzadeh, M. Rabiee, and M. Tahriri, "Development of an electrochemical sulfite biosensor by immobilization of sulfite oxidase on conducting polyaniline film," *Synthetic Metals*, vol. 160, pp. 2653-2657, 2010.
- [4] S. Yazdanpanah, M. Rabiee, M. Tahriri, M. Abdolrahim, and L. Tayebi, "Glycated hemoglobin-detection methods based on electrochemical biosensors," *TrAC Trends in Analytical Chemistry*, vol. 72, pp. 53-67, 2015.
- [5] B. Bahmani, F. Moztarzadeh, M. Hossini, M. Rabiee, M. Tahriri, M. Rezvannia, *et al.*, "A sulfite biosensor fabricated by immobilization of sulfite oxidase on aluminum electrode modified with electropolymerized conducting film (polyaniline)," *Asian Journal of Chemistry*, vol. 21, p. 923, 2009.
- [6] M. Abdorahim, M. Rabiee, S. N. Alhosseini, M. Tahriri, S. Yazdanpanah, S. H. Alavi, *et al.*, "Nanomaterials-based electrochemical immunosensors for cardiac troponin recognition: An illustrated review," *TrAC Trends in Analytical Chemistry*, vol. 82, pp. 337-347, 2016.
- [7] X. Chen, J. Zhu, Z. Chen, C. Xu, Y. Wang, and C. Yao, "A novel bienzyme glucose biosensor based on three-layer Au-Fe₃O₄@SiO₂ magnetic nanocomposite," *Sensors and Actuators B: Chemical*, vol. 159, pp. 220-228, 2011.
- [8] K. Xue, S. Zhou, H. Shi, X. Feng, H. Xin, and W. Song, "A novel amperometric glucose biosensor based on ternary gold nanoparticles/polypyrrole/reduced graphene oxide nanocomposite," *Sensors and Actuators B: Chemical*, vol. 203, pp. 412-416, 2014.
- [9] S. Liu and H. Ju, "Reagentless glucose biosensor based on direct electron transfer of glucose oxidase immobilized on colloidal gold modified carbon paste electrode," *Biosensors and Bioelectronics*, vol. 19, pp. 177-183, 2003.
- [10] M. Abdolrahim, M. Rabiee, S. N. Alhosseini, M. Tahriri, S. Yazdanpanah, and L. Tayebi, "Development of optical biosensor technologies for cardiac troponin recognition," *Analytical biochemistry*, vol. 485, pp. 1-10, 2015.
- [11] E. Mohagheghpour, M. Rabiee, F. Moztarzadeh, M. Tahriri, M. Jafarbeglou, D. Bizari, *et al.*, "Controllable synthesis, characterization and optical properties of ZnS: Mn nanoparticles as a novel biosensor," *Materials Science and Engineering: C*, vol. 29, pp. 1842-1848, 2009.
- [12] E. Mohagheghpour, R. Salimi, H. Sameie, F. Moztarzadeh, M. Roohnikan, M. A. M. Farsi, *et al.*, "A new optical bio-sensor: Wet-chemical synthesis and surface treatment of nanocrystalline Zn_{1-x}S: Mn²⁺ x," in *Optical Sensors*, 2011, p. SWC4.
- [13] M. K. S. FUNKCIONALIZIRANI, "THE WET-CHEMICAL SYNTHESIS OF FUNCTIONALIZED Zn_{1-x}O/Mn_x QUANTUM DOTS UTILIZABLE IN OPTICAL BIOSENSORS," *Materiali in tehnologije*, vol. 47, pp. 235-237, 2013.
- [14] M. Tayebi, M. T. Yarak, A. Mogharei, M. Ahmadi, M. Tahriri, D. Vashae, *et al.*, "Thioglycolic Acid-Capped CdS Quantum Dots Conjugated to α -Amylase as a Fluorescence Probe for Determination of Starch at Low Concentration," *Journal of Fluorescence*, pp. 1-8, 2016.

- [15] M. Tayebi, M. T. Yarak, M. Ahmadi, M. Tahriri, D. Vashae, and L. Tayebi, "Determination of total aflatoxin using cysteamine-capped CdS quantum dots as a fluorescence probe," *Colloid and Polymer Science*, pp. 1-10, 2016.
- [16] M. Tayebi, M. T. Yarak, M. Ahmadi, A. Mogharei, M. Tahriri, D. Vashae, *et al.*, "Synthesis, Surface Modification and Optical Properties of Thioglycolic Acid-Capped ZnS Quantum Dots for Starch Recognition at Ultralow Concentration," *Journal of Electronic Materials*, pp. 1-8, 2016.
- [17] A. Kaushik, R. Khan, P. R. Solanki, P. Pandey, J. Alam, S. Ahmad, *et al.*, "Iron oxide nanoparticles-chitosan composite based glucose biosensor," *Biosensors and bioelectronics*, vol. 24, pp. 676-683, 2008.
- [18] K. J. Cash and H. A. Clark, "Nanosensors and nanomaterials for monitoring glucose in diabetes," *Trends Mol Med*, vol. 16, pp. 584-93, Dec 2010.
- [19] A. Chen and S. Chatterjee, "Nanomaterials based electrochemical sensors for biomedical applications," *Chem Soc Rev*, vol. 42, pp. 5425-38, Jun 21 2013.
- [20] H. Ju, X. Zhang, and J. Wang, *NanoBiosensing: Principles, Development and Application*: Springer Science & Business Media, 2011.
- [21] S. Zeng, K.-T. Yong, I. Roy, X.-Q. Dinh, X. Yu, and F. Luan, "A Review on Functionalized Gold Nanoparticles for Biosensing Applications," *Plasmonics*, vol. 6, pp. 491-506, 2011.
- [22] J. M. Pingarrón, P. Yáñez-Sedeño, and A. González-Cortés, "Gold nanoparticle-based electrochemical biosensors," *Electrochimica Acta*, vol. 53, pp. 5848-5866, 2008.
- [23] R. Rawal, S. Chawla, and C. S. Pundir, "Polyphenol biosensor based on laccase immobilized onto silver nanoparticles/multiwalled carbon nanotube/polyaniline gold electrode," *Anal Biochem*, vol. 419, pp. 196-204, Dec 15 2011.
- [24] Z. Chang, H. Fan, K. Zhao, M. Chen, P. He, and Y. Fang, "Electrochemical DNA Biosensors Based on Palladium Nanoparticles Combined with Carbon Nanotubes," *Electroanalysis*, vol. 20, pp. 131-136, 2008.
- [25] X. Jiang, Y. Wu, X. Mao, X. Cui, and L. Zhu, "Amperometric glucose biosensor based on integration of glucose oxidase with platinum nanoparticles/ordered mesoporous carbon nanocomposite," *Sensors and Actuators B: Chemical*, vol. 153, pp. 158-163, 2011.
- [26] H. Wu, J. Wang, X. Kang, C. Wang, D. Wang, J. Liu, *et al.*, "Glucose biosensor based on immobilization of glucose oxidase in platinum nanoparticles/graphene/chitosan nanocomposite film," *Talanta*, vol. 80, pp. 403-6, Nov 15 2009.
- [27] N. Chauhan and C. S. Pundir, "An amperometric biosensor based on acetylcholinesterase immobilized onto iron oxide nanoparticles/multi-walled carbon nanotubes modified gold electrode for measurement of organophosphorus insecticides," *Anal Chim Acta*, vol. 701, pp. 66-74, Sep 2 2011.
- [28] Y. Du, X. L. Luo, J. J. Xu, and H. Y. Chen, "A simple method to fabricate a chitosan-gold nanoparticles film and its application in glucose biosensor," *Bioelectrochemistry*, vol. 70, pp. 342-7, May 2007.
- [29] Y. Xing, Y.-Y. Jin, J.-C. Si, M.-L. Peng, X.-F. Wang, C. Chen, *et al.*, "Controllable synthesis and characterization of Fe₃O₄/Au composite nanoparticles," *Journal of Magnetism and Magnetic Materials*, vol. 380, pp. 150-156, 2015.
- [30] G.-S. Lai, H.-L. Zhang, and D.-Y. Han, "Amperometric hydrogen peroxide biosensor based on the immobilization of horseradish peroxidase by carbon-coated iron nanoparticles in combination with chitosan and cross-linking of glutaraldehyde," *Microchimica Acta*, vol. 165, pp. 159-165, 2008.
- [31] J. Li and H. Gao, "A Renewable Potentiometric Immunosensor Based on Fe₃O₄ Nanoparticles Immobilized Anti-IgG," *Electroanalysis*, vol. 20, pp. 881-887, 2008.

- [32] B.-W. Lu and W.-C. Chen, "A disposable glucose biosensor based on drop-coating of screen-printed carbon electrodes with magnetic nanoparticles," *Journal of magnetism and magnetic materials*, vol. 304, pp. e400-e402, 2006.
- [33] M. Rieth, *Nano-engineering in Science and Technology* vol. 20: World Scientific, 2003.
- [34] J. Kumar and S. F. D'Souza, "Preparation of PVA membrane for immobilization of GOD for glucose biosensor," *Talanta*, vol. 75, pp. 183-8, Mar 15 2008.
- [35] S. Shukla, S. R. Deshpande, S. K. Shukla, and A. Tiwari, "Fabrication of a tunable glucose biosensor based on zinc oxide/chitosan-graft-poly (vinyl alcohol) core-shell nanocomposite," *Talanta*, vol. 99, pp. 283-287, 2012.
- [36] Y. Xin, X. Fu-bing, L. Hong-wei, W. Feng, C. Di-zhao, and W. Zhao-yang, "A novel H₂O₂ biosensor based on Fe₃O₄-Au magnetic nanoparticles coated horseradish peroxidase and graphene sheets-Nafion film modified screen-printed carbon electrode," *Electrochimica Acta*, vol. 109, pp. 750-755, 2013.
- [37] S. Masoomi-Godardi, A. Khodadadi, M. Vesali-Naseh, and Y. Mortazavi, "Highly stable and selective non-enzymatic glucose biosensor using carbon nanotubes decorated by Fe₃O₄ nanoparticles," *Journal of The Electrochemical Society*, vol. 161, pp. B19-B25, 2014.
- [38] Z. Yang, C. Zhang, J. Zhang, and W. Bai, "Potentiometric glucose biosensor based on core-shell Fe₃O₄-enzyme-polypyrrole nanoparticles," *Biosensors and Bioelectronics*, vol. 51, pp. 268-273, 2014.
- [39] S. Tan, X. Tan, J. Jiang, J. Xu, J. Zhang, D. Zhao, *et al.*, "Hydrogen peroxide biosensor based on poly (vinyl alcohol)/ZnO nanorods composite films," *Journal of Electroanalytical Chemistry*, vol. 668, pp. 113-118, 2012.
- [40] U. Lad, G. M. Kale, and R. Bryaskova, "Glucose oxidase encapsulated polyvinyl alcohol-silica hybrid films for an electrochemical glucose sensing electrode," *Analytical chemistry*, vol. 85, pp. 6349-6355, 2013.
- [41] Y. Fang, D. Zhang, X. Qin, Z. Miao, S. Takahashi, J.-i. Anzai, *et al.*, "A non-enzymatic hydrogen peroxide sensor based on poly (vinyl alcohol)-multiwalled carbon nanotubes-platinum nanoparticles hybrids modified glassy carbon electrode," *Electrochimica Acta*, vol. 70, pp. 266-271, 2012.
- [42] Y. S. Kang, S. Risbud, J. F. Rabolt, and P. Stroeve, "Synthesis and characterization of nanometer-size Fe₃O₄ and γ -Fe₂O₃ particles," *Chemistry of Materials*, vol. 8, pp. 2209-2211, 1996.
- [43] R. Hachani, M. Lowdell, M. Birchall, A. Hervault, D. Mertz, S. Begin-Colin, *et al.*, "Polyol synthesis, functionalisation, and biocompatibility studies of superparamagnetic iron oxide nanoparticles as potential MRI contrast agents," *Nanoscale*, 2016.
- [44] C.-M. Tang, Y.-H. Tian, and S.-H. Hsu, "Poly (vinyl alcohol) Nanocomposites Reinforced with Bamboo Charcoal Nanoparticles: Mineralization Behavior and Characterization," *Materials*, vol. 8, pp. 4895-4911, 2015.
- [45] N. Labidi and A. Djebaili, "Studies of the mechanism of polyvinyl alcohol adsorption on the calcite/water interface in the presence of sodium oleate," *Journal of Minerals and Materials Characterization and Engineering*, vol. 7, p. 147, 2008.
- [46] E. F. d. Reis, F. S. Campos, A. P. Lage, R. C. Leite, L. G. Heneine, W. L. Vasconcelos, *et al.*, "Synthesis and characterization of poly (vinyl alcohol) hydrogels and hybrids for rMPB70 protein adsorption," *Materials Research*, vol. 9, pp. 185-191, 2006.
- [47] D. A. Skoog, D. M. West, F. J. Holler, and S. R. Crouch, *Fundamentals of analytical chemistry*: Nelson Education, 2013.
- [48] Y. Du, X.-L. Luo, J.-J. Xu, and H.-Y. Chen, "A simple method to fabricate a chitosan-gold nanoparticles film and its application in glucose biosensor," *Bioelectrochemistry*, vol. 70, pp. 342-347, 2007.

- [49] X. Kang, Z. Mai, X. Zou, P. Cai, and J. Mo, "A novel glucose biosensor based on immobilization of glucose oxidase in chitosan on a glassy carbon electrode modified with gold–platinum alloy nanoparticles/multiwall carbon nanotubes," *Analytical biochemistry*, vol. 369, pp. 71-79, 2007.
- [50] J.-D. Qiu, J. Huang, and R.-P. Liang, "Nanocomposite film based on graphene oxide for high performance flexible glucose biosensor," *Sensors and Actuators B: Chemical*, vol. 160, pp. 287-294, 2011.
- [51] T. Kong, Y. Chen, Y. Ye, K. Zhang, Z. Wang, and X. Wang, "An amperometric glucose biosensor based on the immobilization of glucose oxidase on the ZnO nanotubes," *Sensors and Actuators B: Chemical*, vol. 138, pp. 344-350, 2009.

Figure captions

Figure 1. XRD pattern of the synthesized Fe_3O_4 nanoparticles

Figure 2. FTIR spectra of (a) PVA, (b) PVA- Fe_3O_4 nanocomposite, (c) GOx and (d) GOx/PVA- Fe_3O_4 nanocomposite

Figure 3. FE-SEM micrographs of (a) PVA, (b) PVA- Fe_3O_4 nanocomposite and (c) GOx/PVA- Fe_3O_4 on Sn electrode

Figure 4. EIS of (a) PVA/Sn film, (b) PVA- Fe_3O_4 /Sn electrode and (c) GOx/PVA- Fe_3O_4 /Sn bioelectrode

Figure 5. CVs of (a) PVA, (b) PVA- Fe_3O_4 /Sn electrode and (c) GOx/PVA- Fe_3O_4 /Sn bioelectrode

Figure 6. CVs of GOx/PVA- Fe_3O_4 /Sn bioelectrode at different scan rates. Inset: plot of current vs. $V^{1/2}$

Figure 7. Effect of different amounts of enzyme concentration on the current response

Figure 8. Effect of pH value on the current response

Figure 9. CVs of GOx/PVA- Fe_3O_4 /Sn bioelectrode in different glucose concentration

Figure 10. Calibration curve of GOx/PVA- Fe_3O_4 /Sn bioelectrode in the glucose range of 5×10^{-3} to 30 mM

Figure 11. The effect of interference on the GOx/PVA- Fe_3O_4 /Sn bioelectrode

Figures

Figure 1

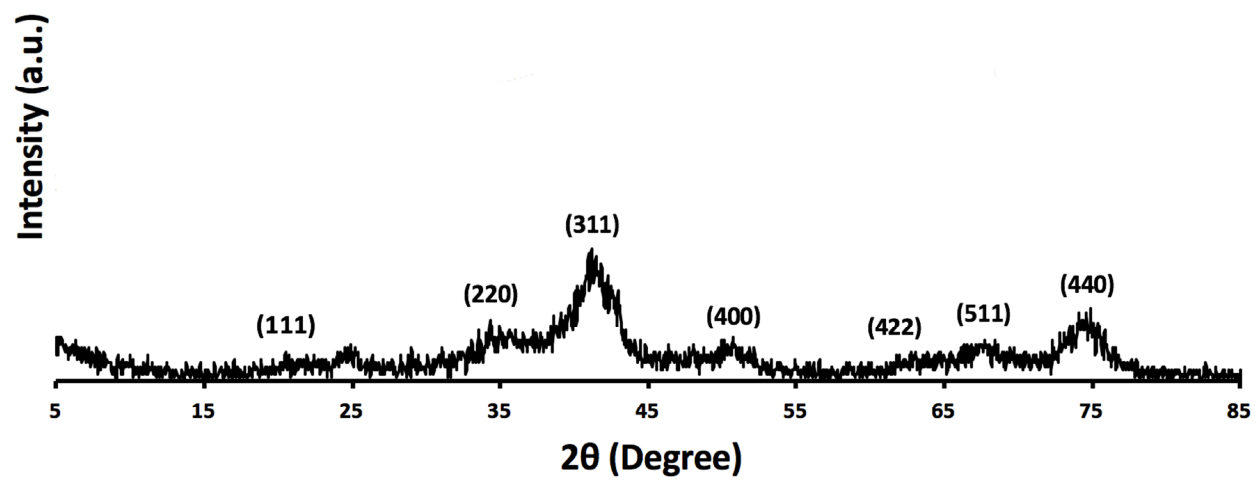


Figure 2

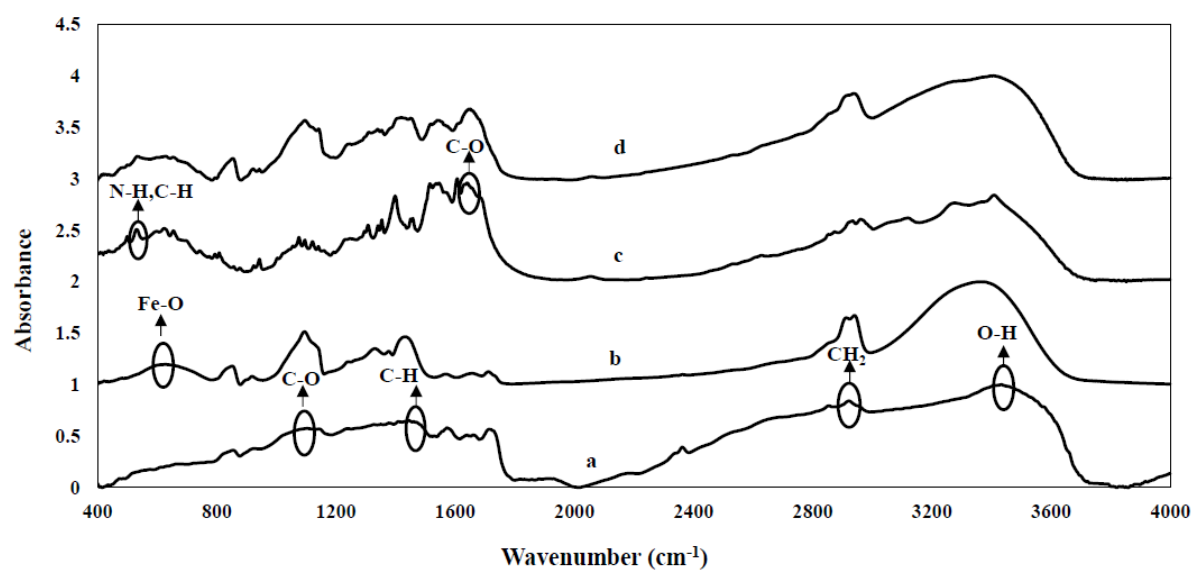
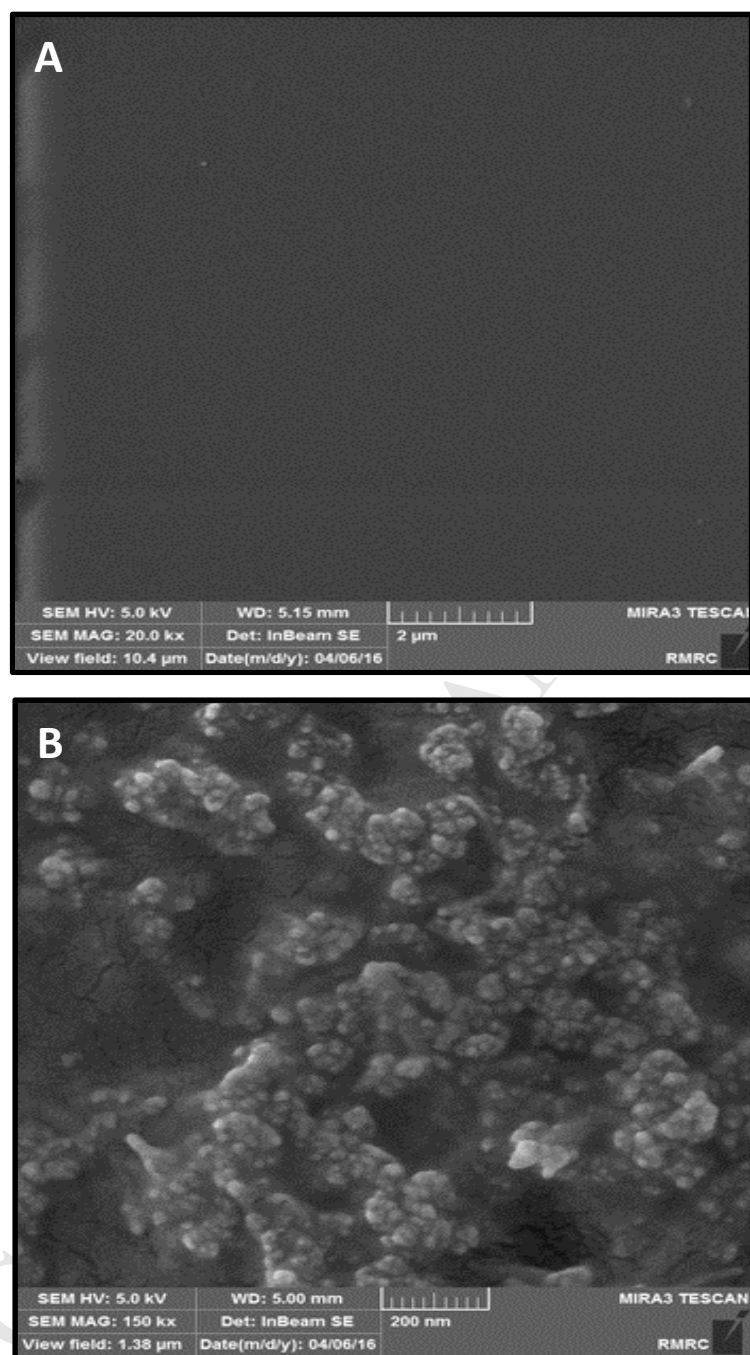


Figure 3



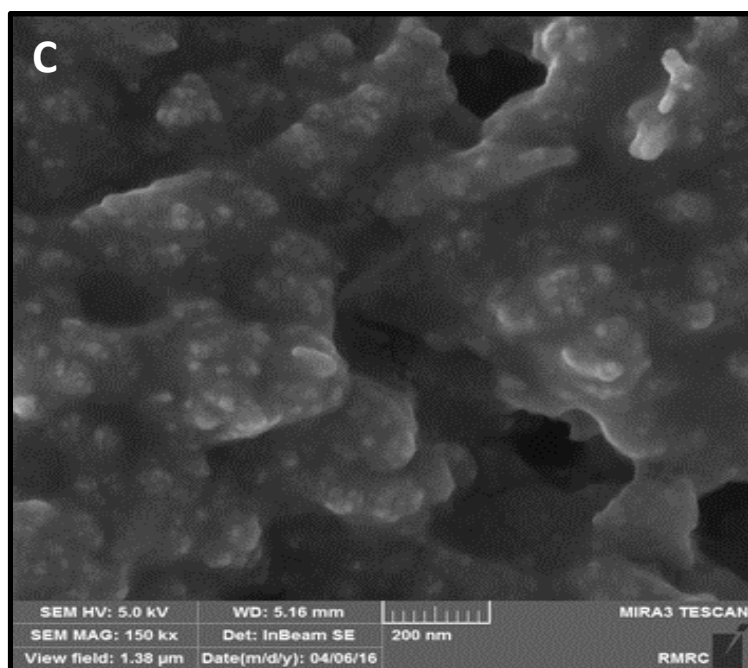


Figure 4

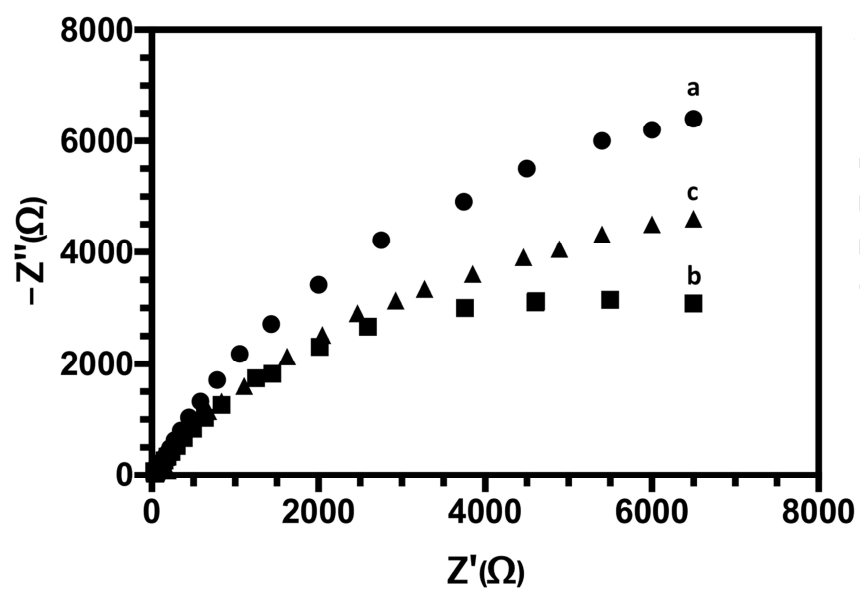


Figure 5

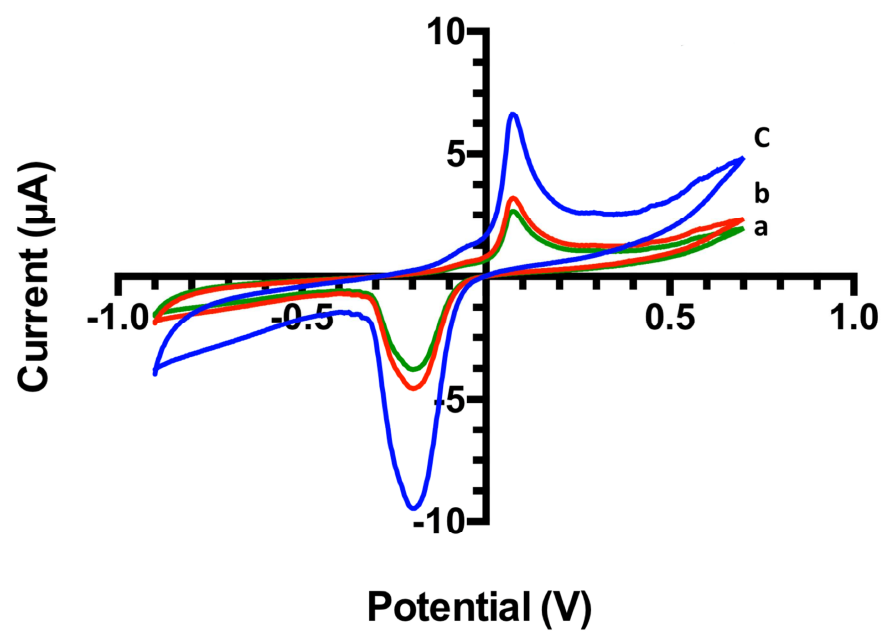


Figure 6

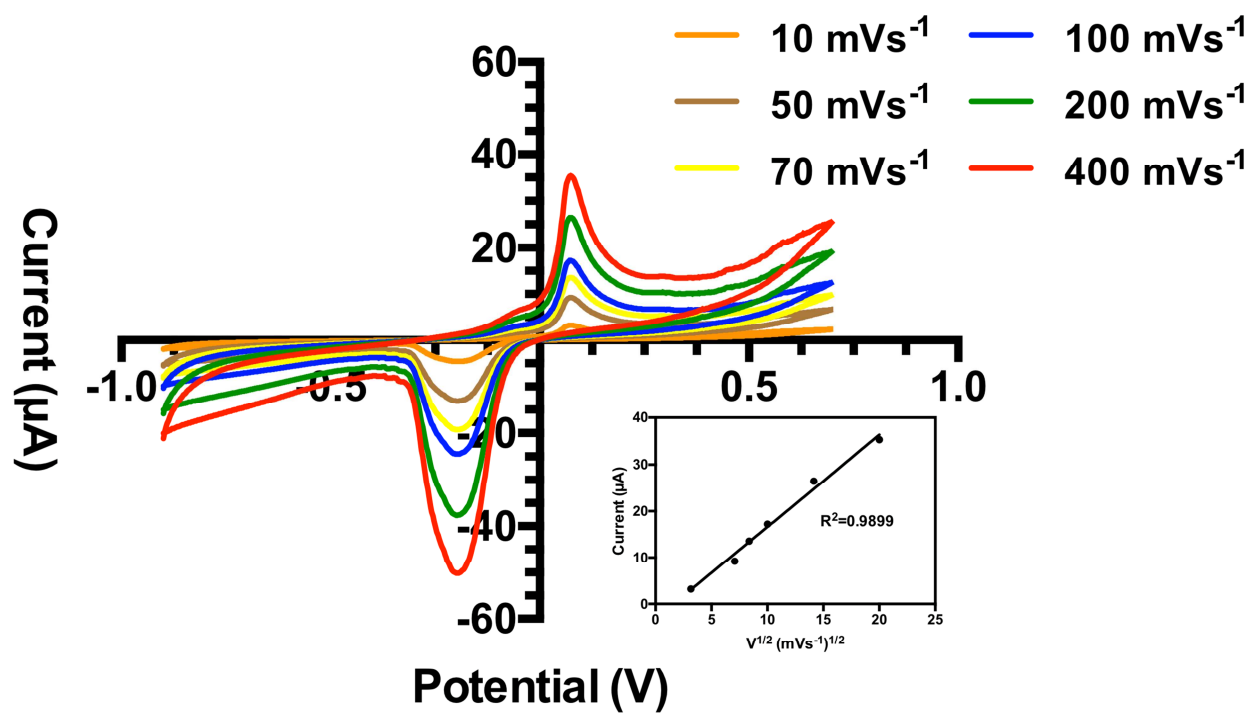


Figure 7

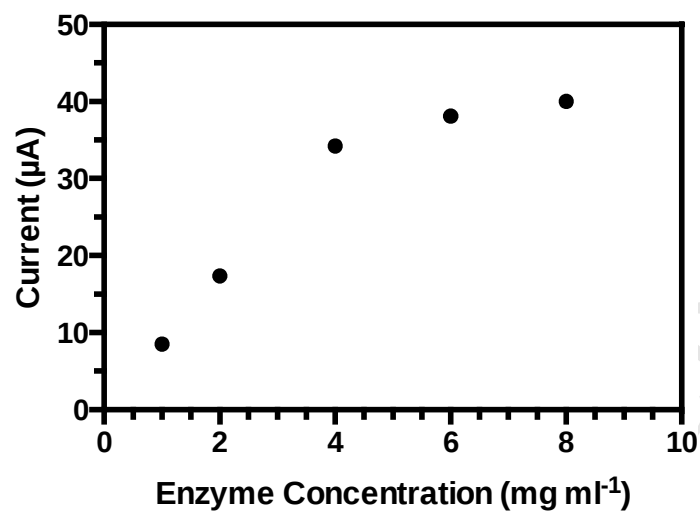


Figure 8

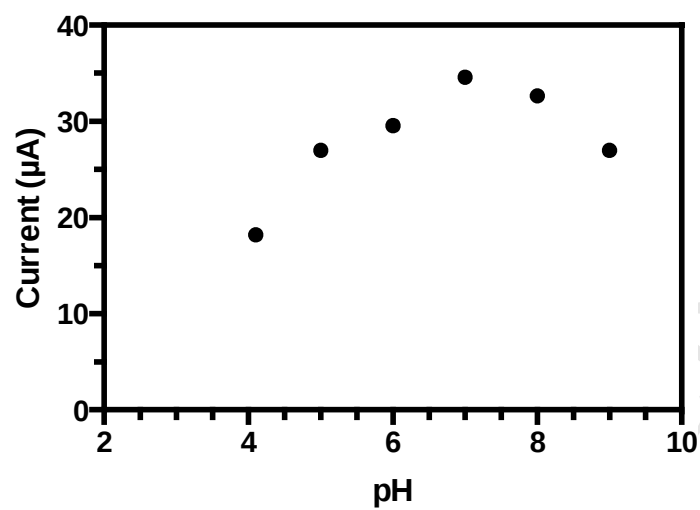


Figure 9

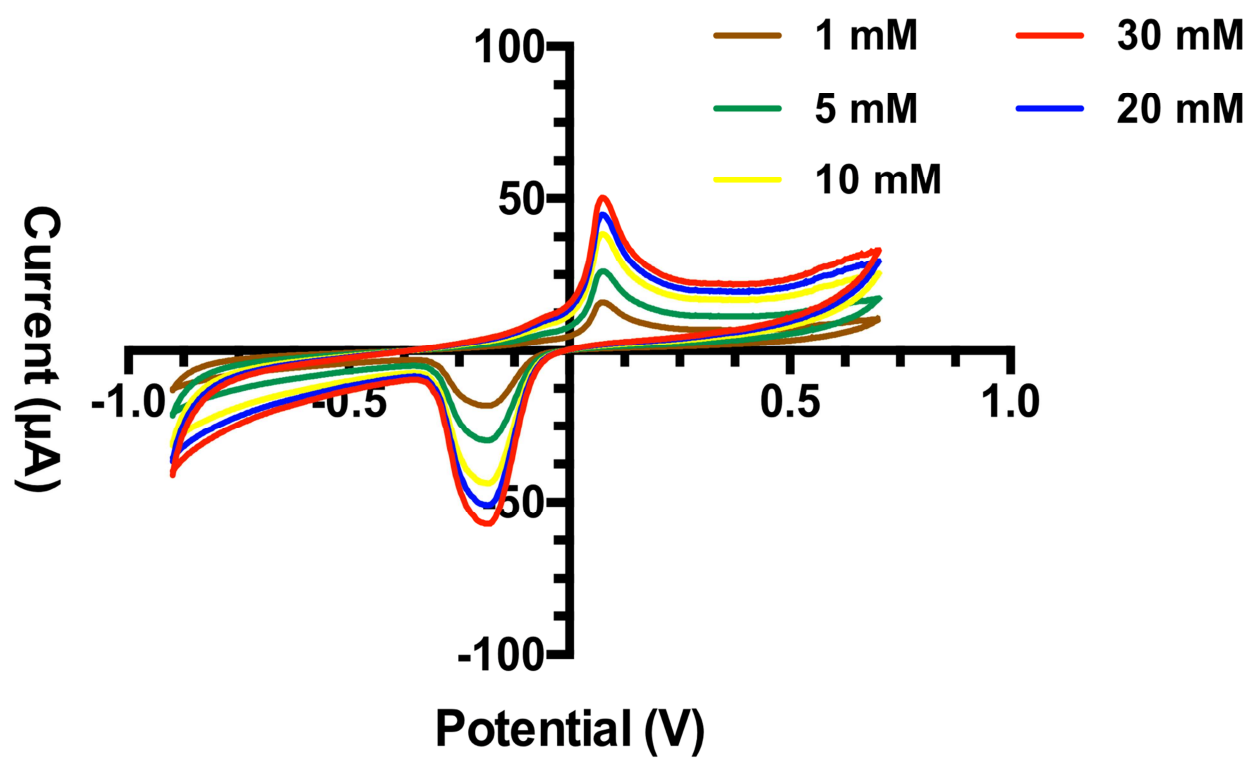


Figure 10


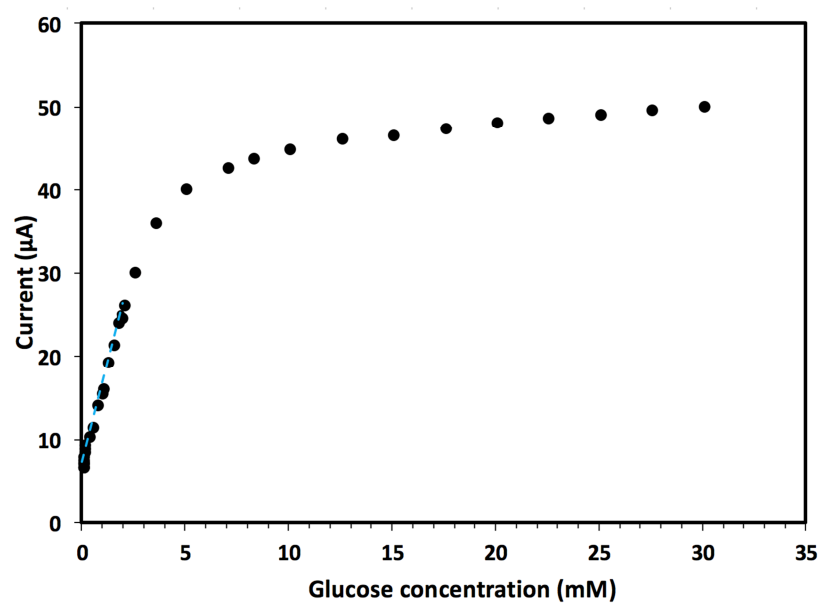


Figure 11

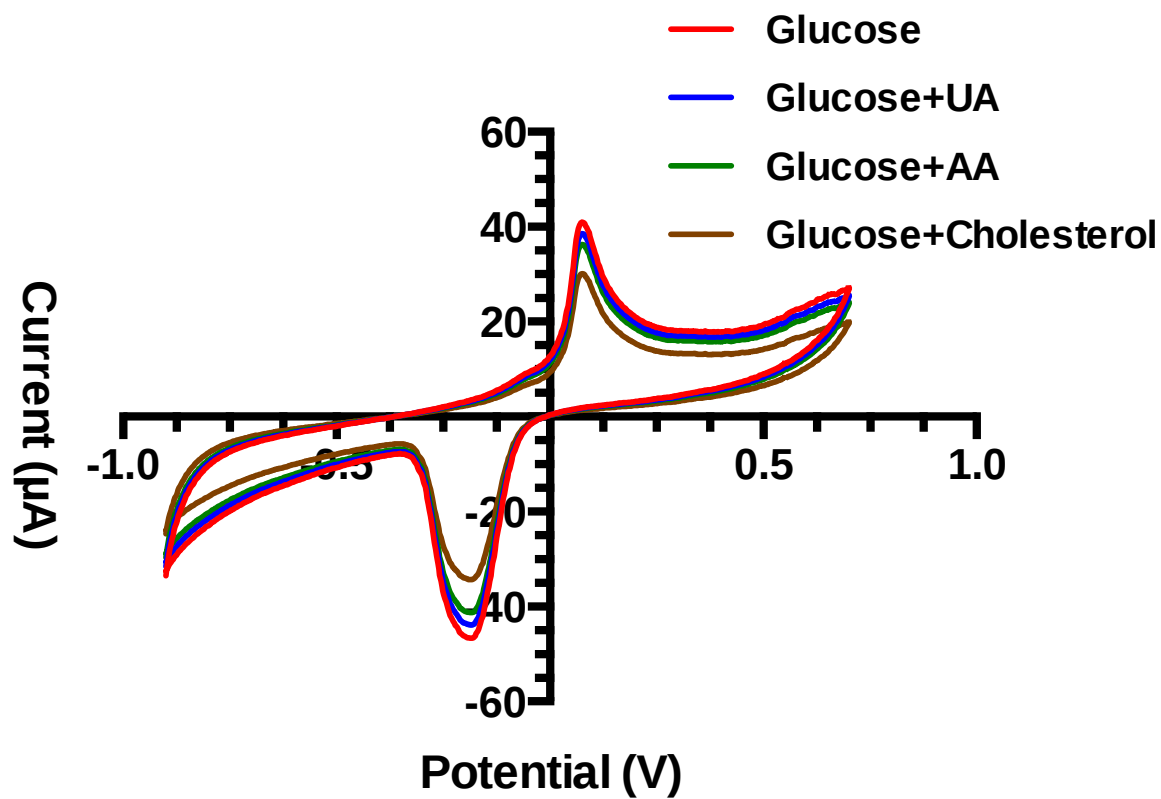

Table

Table 1. The current response of 5 GOx/PVA-Fe₃O₄/Sn bioelectrode in the presence of 5 mM glucose

Sample	Current (μA)
1	30.24
2	28.31
3	31.68
4	30.95
5	28.81