



Amperometric biosensor based on reductive H_2O_2 detection using pentacyanoferrate-bound polymer for creatinine determination

Chi-Hua Nieh^a, Seiya Tsujimura^b, Osamu Shirai^a, Kenji Kano^{a,*}

^a Division of Applied Life Sciences, Graduate School of Agriculture, Kyoto University Sakyo, Kyoto 606-8502, Japan


^b Division of Materials Science, Faculty of Pure and Applied Sciences, University of Tsukuba 1-1-1 Tennodai, Tsukuba, Ibaraki 305-8573, Japan

HIGHLIGHTS

- ▶ PVI[Fe(CN)₅] has a low reactivity against sarcosine oxidase (SOD).
- ▶ PVI[Fe(CN)₅] is suitable as a mediator for the SOD/peroxidase sensing system.
- ▶ The catalytic effects of mediator are related to the hydrophilic/phobic properties.
- ▶ The proposed biosensing method is applicable for urine creatinine determination.

GRAPHICAL ABSTRACT

The detection mechanism of creatinine biosensor. CNH: creatinine amidohydrolase, CRH: creatine amidohydrolase, SOD: sarcosine oxidase, POD: peroxidase. The hollow arrows and the cross symbol indicate the extremely low reactivity of PVI[Fe(CN)₅] against SOD.

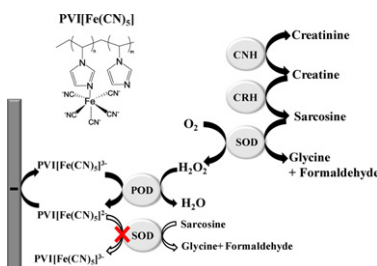

ARTICLE INFO

Article history:

Received 5 October 2012

Received in revised form

28 December 2012

Accepted 31 December 2012

Available online 9 January 2013

Keywords:

Pentacyanoferrate-bound poly(1-vinylimidazole)
Creatinine amidohydrolase
Reductive H_2O_2 detection
Peroxidase
Nafion
Urine creatinine test

ABSTRACT

Pentacyanoferrate-bound poly(1-vinylimidazole) (PVI[Fe(CN)₅]) was selected as a mediator for amperometric creatinine determination based on the reductive H_2O_2 detection. Creatinine amidohydrolase (CNH), creatine amidohydrolase (CRH), sarcosine oxidase (SOD), peroxidase (POD), and PVI[Fe(CN)₅] were crosslinked with poly(ethylene glycol) diglycidyl ether (PEGDGE) on a glassy carbon (GC) electrode for a creatinine biosensor fabrication. Reduction current was monitored at -0.1 V in the presence of creatinine and O_2 . It is revealed that PVI[Fe(CN)₅] is suitable as a mediator for a bioelectrocatalytic reaction of POD, since PVI[Fe(CN)₅] neither reacts with reactants nor works as an electron acceptor of SOD. The amounts of PVI[Fe(CN)₅], PEGDGE, and enzymes were optimized toward creatinine detection. Nafion as a protecting film successfully prevented the enzyme layer from interferences. The detection limit and linear range in creatinine determination were $12 \mu\text{M}$ and $12\text{--}500 \mu\text{M}$ ($R^2 = 0.993$), respectively, and the sensitivity was $11 \text{ mA cm}^{-2} \text{ M}^{-1}$, which is applicable for urine creatinine tests. The results of the creatinine determination for four urine samples measured with this proposed method were compared with Jaffe method, and a good correlation was obtained between the results.

© 2013 Elsevier B.V. All rights reserved.

1. Introduction

Creatinine is the final product of creatine metabolism in muscle of mammals and is mainly filtered out of blood in kidneys.

The creatinine levels are related to the state of renal function, thyroid malfunction, and muscular disorders. The physiologically normal concentration ranges of creatinine in serum and urine are $40\text{--}150 \mu\text{M}$ and $2.5\text{--}23 \text{ mM}$, respectively; high creatinine level may result from renal impairment, while the low creatinine level indicates decreased muscle mass [1,2]. The determination of urine creatinine is also important in other disease measurements since it is widely used as a calibration index for evaluating disease markers

* Corresponding author. Tel.: +81 75 753 6392; fax: +81 75 753 6456.
E-mail address: kano.kenji.5z@kyoto-u.ac.jp (K. Kano).



based on the constant excretion rate every day [3]. The current clinical determination of creatinine is based on colorimetric Jaffe reaction, which involves the formation of red products with picric acid in alkaline solution [4]. However, Jaffe method shows poor selectivity since it is affected by numerous metabolites containing carbonyl group found in biological samples, such as glucose, bilirubin, and ascorbic acid [5,6]. To increase specificity, creatinine deiminase (CD) has been utilized to generate ammonia for amperometric detection though it is interfered from endogenous ammonia [7,8].

Rather than CD, creatinine amidohydrolase (CNH), creatine amidohydrolase (CRH), and sarcosine oxidase (SOD) have more widely been utilized for creatinine determination in amperometric method based on the detection of oxygen consumption or generated H_2O_2 , which are so-called the first generation biosensor [9,10]. The reaction mechanism of creatinine is shown as follows:



In the detection of oxygen consumption, the signal response is seriously influenced by the concentration of dissolved oxygen in samples and the diffusion rate of oxygen from the bulk solution to the surface of the working electrode. On the other hand, the direct electro-oxidation of H_2O_2 requires high operation potential (+0.7 V vs. Ag/AgCl), which often accompanies serious interference problem from other electroactive metabolites in physiological fluids.


In order to overcome this problem, the second generation biosensors have been evolved by using mediators to regenerate oxidized SOD (Eqs. (4) and (5)) [11]. Mediators shuttle electrons from the redox center of SOD to electrode (Eqs. (5) and (6)), which provides higher signal response and lower operating potential.



Various kinds of redox mediators such as DCPIP, PMS, ferricyanide, and benzoquinone were utilized for the SOD reaction [12,13]. Nevertheless, the mediating capabilities of DCPIP, PMS and ferricyanide for SOD reaction are not good, and in our knowledge, most of quinones react with sarcosine to generate colored products. Furthermore, O_2 needs to be removed to avoid the competition with the mediator, which is difficult in practical analysis.

On the other hand, mediated biosensors (such as iron or osmium complexes) coupled with peroxidase (POD) allow the determination of H_2O_2 at low operating potentials around 0V vs. Ag/AgCl, with high sensitivity, high stability, and elimination of the undesirable oxidation of interferents [14–16]. However, there is one thing to be concerned that mediators may react with both of oxidase and POD to cause a decrease in the electrochemical response of mediator reduction [17,18]. Therefore, it is necessary to select an appropriate mediator with selective reactivity against POD alone.

In this study, pentacyanoferrate-bound poly(1-vinylimidazole) ($\text{PVI}[\text{Fe}(\text{CN})_5]$) is selected as a mediator between POD and an electrode for creatinine determination considering its poor mediating capability against SOD. $\text{PVI}[\text{Fe}(\text{CN})_5]$ has been synthesized in our group for fast mediated electron transfer (MET) and immobilization of bilirubin oxidase for oxygen reduction [19]. This kind of electron-conducting hydrogel can covalently bind enzymes, and it provides

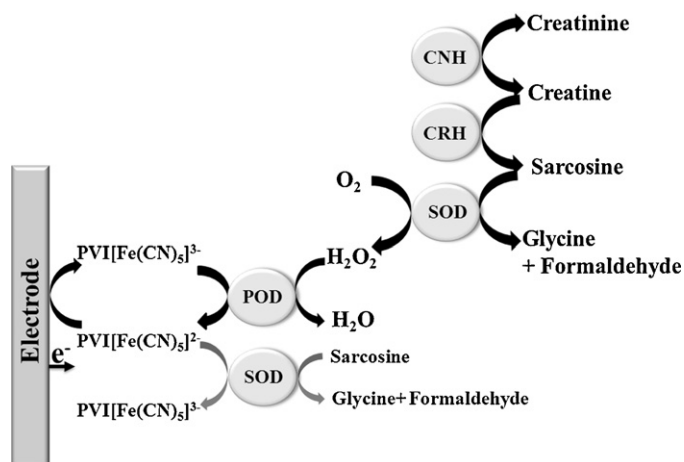

Scheme 1. Reaction scheme of creatinine biosensor based on the reductive H_2O_2 detection mediated by $\text{PVI}[\text{Fe}(\text{CN})_5]$. The gray arrows represent a plausible but unfavorable reaction pathway, which leads to negative interference.

three-dimensional electrocatalysts which are not leachable but swollen in water to form stable redox hydrogels for MET between the redox center of enzymes and electrode [20]. The principle of the creatinine detection is shown in Scheme 1. The three enzymes, POD, and $\text{PVI}[\text{Fe}(\text{CN})_5]$ were crosslinked with poly(ethylene glycol) diglycidyl ether (PEGDGE) on a glassy carbon (GC) electrode. Creatinine was hydrolyzed and oxidized to generate H_2O_2 , then the reduction current of $\text{PVI}[\text{Fe}(\text{CN})_5]$ was observed due to the H_2O_2 reduction through POD. The catalytic effect of $\text{PVI}[\text{Fe}(\text{CN})_5]$ on SOD and POD, electrode optimization, interference effect, and the comparison with Jaffe method will be described.

2. Experimental

2.1. Reagents

2,2'-Azobisisobutyronitrile (AIBN), sodium pentacyanonitrosylferrate(III) dihydrate ($\text{Na}_2[\text{Fe}(\text{CN})_5(\text{NO})] \cdot 2\text{H}_2\text{O}$), sarcosine, creatine, creatinine, ascorbic acid (AA), uric acid (UA), and saturated picric acid solution were obtained from Wako Chem. Co. (Osaka, Japan). POD from horseradish (257 U mg^{-1}), SOD from microorganism (16.6 U mg^{-1}), CRH from microorganism (13 U mg^{-1}), and CNH from microorganism (258 U mg^{-1}) were purchased from Toyobo Co. (Osaka, Japan). 1-Vinylimidazole, PEGDGE, Nafion (5 wt% in mixture of lower aliphatic alcohols and water, contains 45% water), acetaminophen, and dopamine were from Sigma-Aldrich (USA). UA solution was prepared by dissolving in 10 mM NaOH, and the enzymes, substrates, several interferences and PEGDGE solutions were prepared using 100 mM phosphate buffer (pH 7.0). Other chemicals were of analytical grade and used as received. Urine samples were donated from healthy volunteers.

2.2. Instrumentation

2.2.1. Synthesis of $\text{PVI}[\text{Fe}(\text{CN})_5]$

Poly(1-vinylimidazole) (PVI) was synthesized according to the literature [20]. In brief, 6 mL of 1-vinylimidazole was mixed with 0.5 g of AIBN and was heated under stirring at 70°C for 2 h in Ar. After cooling, the yellow precipitate was dissolved by adding methanol. The solution was added dropwise to acetone under strong stirring. White PVI powder was obtained after filtering and drying. $\text{PVI}[\text{Fe}(\text{CN})_5]$ was then synthesized as reported [19]. Briefly, 200 mg of $\text{Na}_2[\text{Fe}(\text{CN})_5(\text{NO})] \cdot 2\text{H}_2\text{O}$ and 188 mg of PVI were dissolved in 50 mL of 0.6 M NaOH and refluxed at 65°C for 24 h. The mixture was dialyzed against distilled water overnight, followed

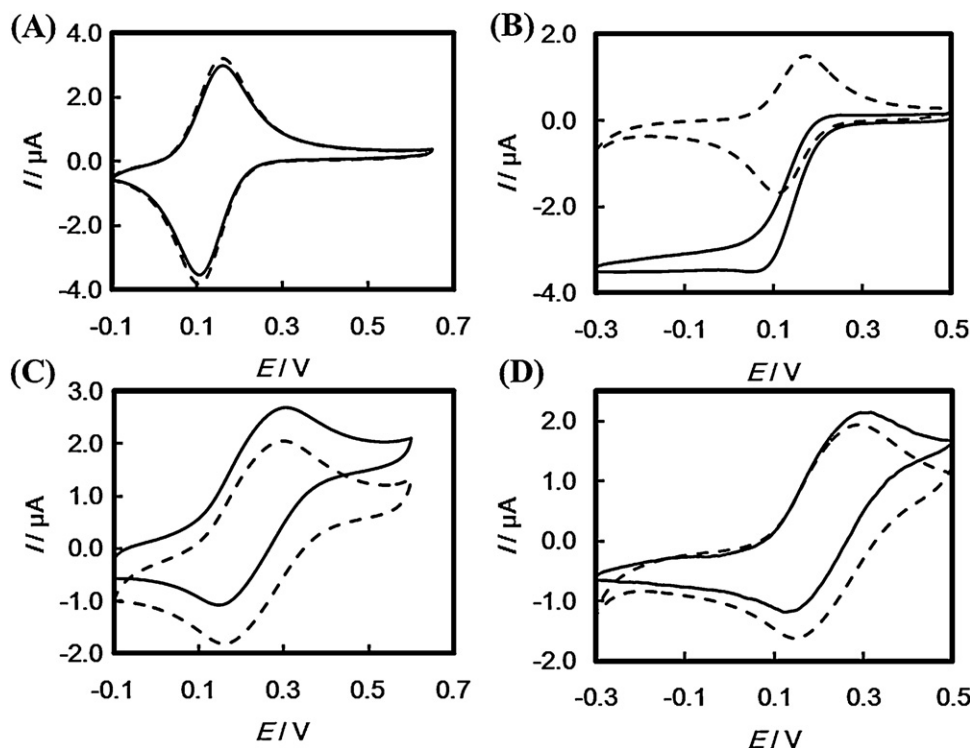


Fig. 1. Cyclic voltammograms of (A) SOD-PVI[Fe(CN)₅] electrode, (B) SOD/POD-PVI[Fe(CN)₅] electrode, (C) SOD-PVI[Os(dmebpy)₂Cl] electrode, and (D) SOD/POD-PVI[Os(dmebpy)₂Cl] electrode. (A) and (C) were measured in Ar-saturated solutions, while (B) and (D) were measured in air-saturated solutions. The dash line represents the measurement in 10 mM phosphate buffer (pH 7.0), while the solid line represents the measurement in 5 mM sarcosine. Scan rate: 20 mV s⁻¹. Electrode conditions, SOD: 0.83 U, POD: 2.57 U, PEGDGE: 11 μg, PVI[Fe(CN)₅]: 30 μg, PVI[Os(dmebpy)₂Cl]: ca. 40 μg.

by centrifugation at 5000 g for 20 min two times to remove precipitate. The suspension was vacuum freeze-dried at -40 °C for 24 h to get light yellow PVI[Fe(CN)₅] powder. The stock solution of PVI[Fe(CN)₅] was prepared in a 10 mM phosphate buffer solution at pH 7.0.

2.2.2. Fabrication of enzymes and PVI[Fe(CN)₅]-modified electrode

The surface of a GC electrode (3 mm diameter, BAS) was polished with alumina powder, washed with distilled water and dried before use. 2 μL of PVI[Fe(CN)₅], 1 μL of PEGDGE, and 2 μL of enzyme solution were successively cast onto the surface of GC electrode and well mixed with a syringe needle. The electrode was dried at 4 °C for 24 h. Before measurements, the proposed electrode was immersed into 100 mM phosphate buffer (pH 7.0) for at least 30 min. For interference tests, 5 μL of 1% Nafion in ethanol was cast onto the surface of the proposed electrode and air-dried before immersing the electrode into buffer for pre-conditioning.

2.3. Procedures

2.3.1. Electrochemical measurements

All electrochemical investigations were carried out in 100 mM phosphate buffer (pH 7.0) under moderate stirring at 25 °C with an electrochemical analyzer (BAS CV 50 W, BAS Inc., Japan). A platinum wire electrode and an Ag/AgCl/sat. KCl electrode were used as the counter and reference electrodes, respectively.

2.3.2. Creatinine determination by Jaffe method

This electro-enzymatic method was compared with spectrophotometric Jaffe method [21]. One hundred μL of urine sample or creatinine standard solution (0.5–2.5 mg mL⁻¹) prepared in a 10 mM HCl solution was added into a reagent solution containing

2 mL of saturated picric acid solution and 150 μL of 10 wt% NaOH. After 10 min incubation at room temperature, 7.75 mL of distilled water was added into the test solution. After 5.0 min, and the absorbance at λ = 520 nm was measured with a spectrophotometer (MultiSpec-1500, Shimadzu Co., Japan).

3. Results and discussion

3.1. Catalytic effect of PVI[Fe(CN)₅] on SOD and POD

In oxidase/peroxidase bienzyme system, mediators oxidized in the POD reaction may also be reduced by receiving the electron from the reduced oxidase generated in the substrate oxidation, which interferes with the detection of mediator reduction on the electrode. To evaluate the mediating effect for mediator selection, PVI[Fe(CN)₅] and PVI[Os(4,4'-dimethyl-2,2'-bipyridine)₂Cl] (PVI[Os(dmebpy)₂Cl]), which was synthesized according to the literature [22,23], were used to investigate the interactions with SOD and POD. The cyclic voltammetric responses of SOD/POD-PVI[Fe(CN)₅]-modified GC electrode and SOD-PVI[Fe(CN)₅]-modified GC electrode were shown in Fig. 1. In Fig. 1A, PVI[Fe(CN)₅] did not mediate the SOD reaction, while the catalytic reduction current from the POD reaction was clearly observed (Fig. 1B).

On the other hand, PVI[Os(dmebpy)₂Cl] synthesized according to the literature [22,23] reacted with SOD; the catalytic oxidation current of creatinine was obtained (Fig. 1C). Therefore, in the cyclic voltammogram of SOD/POD-PVI[Os(dmebpy)₂Cl] electrode, the catalytic reduction current from POD reaction was hardly observed as shown in Fig. 1D.

The reason which causes the difference in the reactivity between PVI[Fe(CN)₅] and PVI[Os(dmebpy)₂Cl] can be explained as follows. Originally, the meditating capability of hexacyanoferrate ion on the

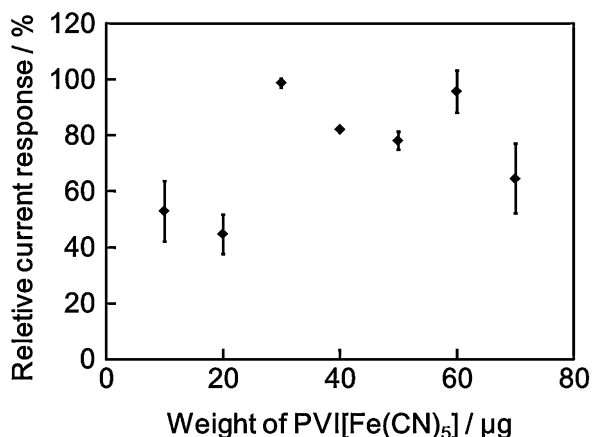


Fig. 2. Dependence of the current response on the PVI[Fe(CN)₅] amount for the detection of 100 μM creatinine at −0.1 V. Error bars with $n = 3$. Electrode conditions, CNH: 1.29 U, CRH: 0.26 U, SOD: 0.33 U, POD: 1.03 U, PEGDGE: 20 μg.

SOD reaction is very low, because the flavin adenine dinucleotide (FAD), the redox center of SOD, locates in hydrophobic surroundings; hexacyanoferrate with negatively charged ligands would be difficult to enter into the deeply buried FAD due to the electrostatic repulsion [24]. After binding pentacyanoferrate with PVI, it may become more difficult to enter the active site of SOD due to the increased charge density and fixation. For this reason, there is no mediating effect of PVI[Fe(CN)₅] on the SOD reaction. On the other hand, Os(dmbpy)₂Cl is more hydrophobic than pentacyanoferrate, which decreases the difficulty in entering the active site of the oxidase. In POD reaction, both of the polymers can transfer electrons to the protoheme, the redox center of POD. A reasonable explanation is that the location of protoheme is near the surface of POD, and the size of POD is smaller than that of SOD, which shortens the distance between the mediator and the redox center [25]. Therefore, it is easier for PVI[Fe(CN)₅] to react with POD than with SOD. Thus, the data in Fig. 1 clearly confirm the concept that PVI[Fe(CN)₅] has extremely low reactivity against SOD, while it has high reactivity against POD; the linear range of H₂O₂ measured by the POD/PVI[Fe(CN)₅]-modified sensor was from 3 to 65 μM and the sensitivity was approximately 410 mA cm^{−2} M^{−1} (data not shown). Based on the results, PVI[Fe(CN)₅] is suitable as a mediator for the SOD/POD bienzyme system, and the signal intensity was practically independent of the oxygen tension at least in the range from 0.2 to 1 atm (data not shown).

3.2. Optimization of enzymes and PVI[Fe(CN)₅]-modified electrode

Fig. 2 shows the effect of the PVI[Fe(CN)₅] amount fabricated with the four enzymes on the GC electrode. Over 30 μg of PVI[Fe(CN)₅], the amperometric response did not vary dramatically from each other. However, with a large amount of PVI[Fe(CN)₅], the longer time was needed to get the steady state (e.g., 600 s for one injection for the electrode containing 50 μg of PVI[Fe(CN)₅], while 300 s for the electrode containing 30 μg of PVI[Fe(CN)₅]). It indicates that the thick film of the polymer increases the difficulty of the substrate permeation. Considering the current response and the time to reach the steady state, 30 μg of PVI[Fe(CN)₅] was selected in the following experiments.

The weight percentage of PEGDGE was then examined in the range from 2.5% to 38.8% of the total weight of the cast on the electrode. The time to reach the steady state increased with an increase in the percentage of PEGDGE above 11.2%, while the magnitude of the current responses did not change significantly (data not shown).

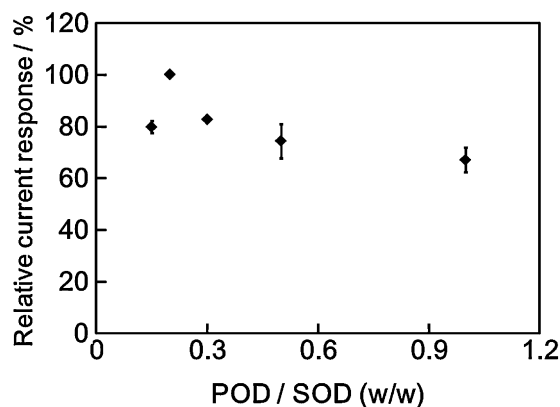


Fig. 3. Dependence of the amperometric response on the weight ratio of POD to SOD for the detection of 100 μM creatinine at −0.1 V. Error bars with $n = 3$. Electrode conditions, CNH: 1.29 U, CRH: 0.26 U, SOD: 0.33 U (20 μg), PEGDGE: 11.2%, PVI[Fe(CN)₅]: 30 μg.


The high percentage of PEGDGE increases the rigidity of the polymer film, resulting in the poor permeability of the substrate. Based on the result, the percentage of PEGDGE was optimized to be 11.2%.

Since the enzyme composition of POD and SOD may affect the biosensing performance, the effect of the POD/SOD ratio on the current response for the creatinine detection was also examined in the range from 0.15 to 1 (w/w). Fig. 3 shows that the highest current response was obtained at the ratio of 0.2 (5 μg of POD and 20 μg of SOD) for the detection of 100 μM creatinine, and the current response decreased gradually with an increase in the ratio of POD to SOD. The ratio of POD to SOD was therefore optimized to be 0.2.

The amounts of the four enzymes were then determined as follows: 1.29 U of POD, 0.42 U of SOD, 0.26 U of CRH, and 1.29 U of CNH by considering the effect of the total weight of the enzyme on the current response. The response time was approximately 150 s and the RSD in the reproducibility (in electrode-to-electrode) was 8.4% ($n = 3$).

3.3. Interference effect

The creatinine biosensor based on the reductive H₂O₂ detection at a low operating potential (−0.1 V vs. Ag|AgCl) minimizes the undesirable oxidation of electroactive interference in physiological fluids. However, some interferents such as AA may still react with POD, since they act as electron donors for the H₂O₂ reduction [26].



The reaction of the interferences with H₂O₂ catalyzed by POD (Eq. (7)) decreases the H₂O₂ concentration produced in the oxidase reaction, which causes the underestimation of the creatinine concentration. To eliminate the interference, negatively-charged Nafion was utilized as a protecting film on the top of the enzymes-PVI[Fe(CN)₅]-modified electrode to exclude anionic species such as AA and UA. The interference effect on the amperometric response measured with the proposed electrode covered with and without Nafion film is shown in Fig. 4. For the detection of 150 μM creatinine, the amperometric response with the Nafion-coated electrode was smaller than that measured the electrode without Nafion film because of the inhibition of the mass transfer. However, the interference effect was eliminated by the protection of Nafion film, while the current responses of 150 μM UA and 10 μM AA were observed at the electrode without Nafion film. In the case of urine, the normal concentrations of creatinine and UA are in the same level [27], and the concentration of creatinine is about thirty times higher than that of AA [28]. This means that Nafion used as a protecting

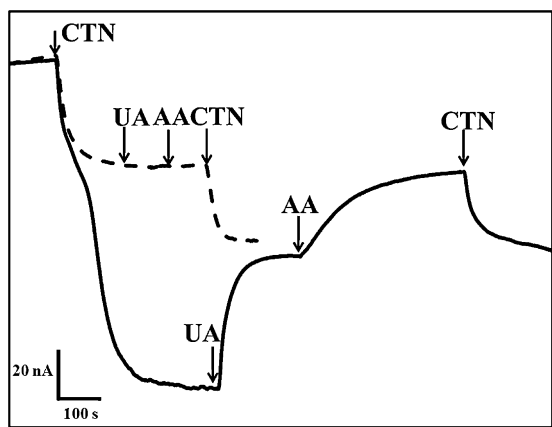


Fig. 4. Amperometric responses of the proposed electrode without Nafion (solid line) and with 5 μL of 1% Nafion (dash line). CTN: 150 μM creatinine, UA: 150 μM , AA: 10 μM . The arrows indicate the injection time of the respective solutions. Electrode conditions, CNH: 1.29 U, CRH: 0.26 U, SOD: 0.42 U, POD: 1.29 U, PEGDGE: 11.2%, $\text{PVI}[\text{Fe}(\text{CN})_5]$: 30 μg .

film satisfies the creatinine determination in real urine samples. Acetaminophen and dopamine were also tested for the interference test. Small interference effects were observed in the solutions containing 150 μM creatinine and 10 μM acetaminophen (recovery = $108 \pm 4\%$) or dopamine (recovery = $96 \pm 6\%$). Considering the fact that the concentrations of these interferences are much smaller than that of creatinine, these interferences do not seriously affect the creatinine detection in this biosensing system.

Internal creatine in urine might also interfere with creatinine determination since it reacts with CRH immobilized on the enzymes- $\text{PVI}[\text{Fe}(\text{CN})_5]$ -modified electrode to result in the overestimation of creatinine. In the case of urine, the excretion rate of creatinine is about twenty times higher than that of creatine [29]. In our experiment, as the concentration ratio of creatine to creatinine is 6.7% (10 μM creatine/150 μM creatinine), the signal ratio of creatine to creatinine is only about 2% (data not shown) though H_2O_2 generation from creatine requires fewer enzymatic steps than that from creatinine. It may be described that in neutral pH, creatinine is positively charged while creatine is a zwitterion, therefore creatinine is easier to penetrate the negatively charged Nafion film into the enzyme layer to get a larger amperometric response [30]. As a result, the internal creatine in urine does not significantly affect the creatinine determination in our method.

3.4. Comparison with Jaffe method

The amperometric response for the optimized biosensing electrode at -0.1V is presented in Fig. 5. The detection limit of creatinine is 12 μM ($\text{SN} > 3$) and the linear range is from 12 to 500 μM ($R^2 = 0.993$), and the sensitivity is $11 \text{ mA cm}^{-2} \text{ M}^{-1}$, which is sufficient for urine sample test. This method was applied to the creatinine determination of urine from four volunteers and was compared with Jaffe method which is widely used in clinical diagnosis. In the electro-enzymatic method, 10 μL of urine sample was injected into 1 mL of 100 mM phosphate buffer (pH 7.0) for measurements. Table 1 shows the creatinine concentrations evaluated from the absorbance at $\lambda = 520 \text{ nm}$ based on Jaffe method and the current response at -0.1V measured by this proposed method, respectively. Numbers 1 and 2 are the urine samples which were donated by male, while no. 3 and 4 were donated by female. The data show that the concentration of urine creatinine in male is higher than that in female, which is consistent with the typical human reference ranges, and a good correlation was obtained between the two methods. The values measured by the

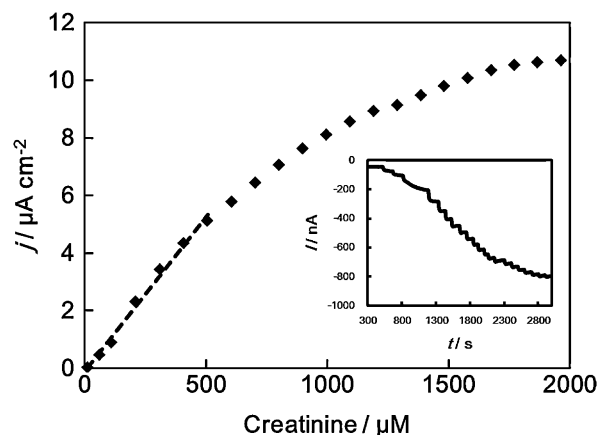


Fig. 5. Dependence of the amperometric response on the creatinine concentration at -0.1V . Electrode conditions were the same as those in Fig. 4 with Nafion film. The broken lines is a linear regression curve; current density ($\mu\text{A cm}^{-2}$) = $11 (\text{mA cm}^{-2} \text{ M}^{-1}) \times [\text{creatinine}] (\mu\text{M}) - 120 (\text{nA cm}^{-2})$, $R^2 = 0.993$. The inset shows the amperometric response.

Table 1

Determination of creatinine from urine samples.

Number	Creatinine/mM	
	Jaffe method	This method
1	17.0 ± 0.3	13.3 ± 0.5
2	17.1 ± 0.3	11.9 ± 0.1
3	5.7 ± 0.1	5.2 ± 0.2
4	11.6 ± 0.3	9.1 ± 0.4

All data are the averages of triplicate experiments.

electro-enzymatic method are lower than Jaffe method, most probably because other compounds in urine (UA or AA) caused positive interference in Jaffe method. The results also show that the creatinine concentrations of no. 1 and 2 measured by Jaffe method are similar with each other, while the value of no. 2 is smaller than that of no. 1 measured by this method. This seems to be resulted from a high concentration of interference in no. 2, which reacts with picric acid to overestimate the creatinine concentration in Jaffe method.

4. Conclusion

The creatinine biosensor based on the reductive H_2O_2 detection was successfully developed. Pentacyanoferrate-bound polymer is suitable as a mediator and appropriate for the enzyme immobilization in this biosensing system, since it only mediates the POD reaction but not against the SOD reaction. The interference effect was eliminated by the Nafion film and the proposed method is applicable for clinical diagnosis.

References

- [1] T. Arndt, *Forensic Sci. Int.* 186 (2009) 48.
- [2] U. Lad, S. Khokhar, G.M. Kale, *Anal. Chem.* 80 (2008) 7910.
- [3] S. Narayanan, H.D. Appleton, *Clin. Chem.* 26 (1980) 1119.
- [4] R.W. Bonsnes, H.H. Taussky, *J. Biol. Chem.* 158 (1945) 581.
- [5] J.A. Weber, A.P. Vanzanten, *Clin. Chem.* 37 (1991) 695.
- [6] M.H. Kroll, N.A. Roach, B. Poe, R.J. Elin, *Clin. Chem.* 33 (1987) 1129.
- [7] M. Gutierrez, S. Alegret, M. del Valle, *Biosens. Bioelectron.* 23 (2008) 795.
- [8] C.S. Rui, Y. Kato, K. Sonomoto, *Biosens. Bioelectron.* 9 (1994) 429.
- [9] T. Tsuchida, K. Yoda, *Clin. Chem.* 29 (1983) 51.
- [10] V.K. Nguyen, C.M. Wolff, J.L. Seris, J.P. Schwing, *Anal. Chem.* 63 (1991) 611.
- [11] A.E.G. Cass, G. Davis, M.J. Green, H.A.O. Hill, *J. Electroanal. Chem.* 190 (1985) 117.
- [12] A. Ramanavicius, *Anal. Bioanal. Chem.* 387 (2007) 1899.
- [13] I. Taniguchi, S. Miyamoto, S. Tomimura, F.M. Hawkrig, *J. Electroanal. Chem.* 240 (1988) 333.

- [14] H. Sakai, R. Baba, K. Hashimoto, A. Fujishima, A. Heller, *J. Phys. Chem.* 99 (1995) 11896.
- [15] H. Kinoshita, M. Torimura, K. Kano, T. Ikeda, *Electroanal.* 9 (1997) 1234.
- [16] T. Ikeda, T. Shiraishi, M. Senda, *Agric. Biol. Chem.* 52 (1988) 3187.
- [17] T.J. Ohara, M.S. Vreeke, F. Battaglini, A. Heller, *Electroanal.* 5 (1993) 825.
- [18] R. Matsumoto, M. Mochizuki, K. Kano, T. Ikeda, *Anal. Chem.* 74 (2002) 3297.
- [19] K. Ishibashi, S. Tsujimura, K. Kano, *Electrochem.* 76 (2008) 594.
- [20] T.J. Ohara, R. Rajagopalan, A. Heller, *Anal. Chem.* 65 (1993) 3512.
- [21] M. Bader, R. Wrbitzky, M. Blaszkewicz, C. van Thriel, *Arch. Toxicol.* 81 (2007) 335.
- [22] S.R. Johnson, T.D. Westmoreland, J.V. Caspar, K.R. Barqawi, T.J. Meyer, *Inorg. Chem.* 27 (1988) 3195.
- [23] T.J. Ohara, R. Rajagopalan, A. Heller, *Anal. Chem.* 66 (1994) 2451.
- [24] J.J. Kulys, N.K. Cenas, *Biochim. Biophys. Acta* 744 (1983) 57.
- [25] N.C. Veitch, *Phytochem.* 65 (2004) 249.
- [26] R. Maidan, A. Heller, *Anal. Chem.* 64 (1992) 2889.
- [27] Y.G. Zuo, Y. Yang, Z. Zhu, W.S. He, Z. Aydin, *Talanta* 83 (2011) 1707.
- [28] M.P. Westerman, Y. Zhang, J.P. McConnell, P.A. Chezick, R. Neelam, S. Freels, L.S. Feldman, S. Allen, R. Baridi, L.E. Feldman, L.W.M. Fung, *Am. J. Hematol.* 65 (2000) 174.
- [29] C. Beyer, *Clin. Chem.* 39 (1993) 1613.
- [30] J.H. Shin, Y.S. Choi, H.J. Lee, S.H. Choi, J. Ha, I.J. Yoon, H. Nam, G.S. Cha, *Anal. Chem.* 73 (2001) 5965.