



# Enzyme-based amperometric biosensors: 60 years later ... Quo Vadis?

Paolo Bollella <sup>a,b,\*</sup>


<sup>a</sup> Dipartimento di Chimica, Università degli Studi di Bari Aldo Moro, 70125, Bari, Italy

<sup>b</sup> Centre for Colloid and Surface Science, Università degli Studi di Bari Aldo Moro, 70125, Bari, Italy

## HIGHLIGHTS

- Enzyme-based Amperometric Biosensors started in the 1960s by Clark and Lyons.
- The sensitivity, calibration and validation are still issues towards PoC devices.
- “Chimeric” enzymes and sense-act-treat will be used for wearable devices.

## GRAPHICAL ABSTRACT

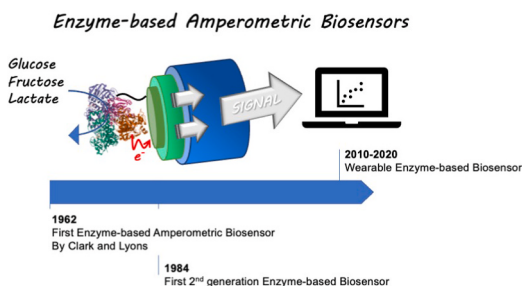

## ARTICLE INFO

### Keywords:

Enzyme-based biosensors  
Amperometry  
Modified electrodes  
Glucose  
Fructose  
Lactate

## ABSTRACT

Enzyme-based amperometric biosensors represent powerful tools for remote medicine and *in situ* analysis. Nowadays, billions of people are surrounded by enzyme-based amperometric biosensors even considering their relatively young age ... only 60 years! In this period, many researchers, dealing mostly with the same target molecules as in early times, have developed novel strategies to tackle electron transfer issues and to realise stable, sensitive, and selective biosensors. Besides marking 60 years from the first enzyme-based amperometric biosensor, this review aims at summarising the technological advancements in the field mainly considering three enzyme families: D-glucose oxidising enzymes, D-fructose oxidising enzymes and L-lactate oxidising enzymes. It is an overview of the past (previous five decades) and current advancements (2010–2020) from the electrode platform tailoring to the technological production and applications (*e.g.*, *in situ* biosensors, Point-of-Care (PoC), wearable biosensors etc.) focused on few enzymes.

## 1. Introduction

In the last 6 decades, enzyme-based biosensors have been conceived, developed, commercialised, and employed for *in situ* analysis as well as Point-of-Care (PoC) devices being able to provide a reliable output signal quantitatively correlated with a certain analyte concentration [1–4]. The first enzyme-based biosensor has been realized 60 years ago

by Clark and Lyons at the Children's Hospital of Cincinnati [5–8]. In this paper, Clark and Lyons reported the first enzyme membrane electrode by trapping a concentrated enzyme layer between two cuprophane membranes wrapped on top of a pH sensing electrode. Specifically, they immobilised glucose oxidase (GOx) within the membrane 'sandwich' enabling glucose oxidation to  $\delta$ -gluconolactone that causes an increasing of  $H^+$  concentration, corresponding to pH drop, as shown in Fig. 1A,

\* Dipartimento di Chimica, Università degli Studi di Bari Aldo Moro, 70125, Bari, Italy.

E-mail address: [paolo.bollella@uniba.it](mailto:paolo.bollella@uniba.it).

<https://doi.org/10.1016/j.aca.2022.340517>

Received 3 May 2022; Received in revised form 9 October 2022; Accepted 11 October 2022

Available online 14 October 2022


0003-2670/© 2022 Elsevier B.V. All rights reserved.

which resulted in the variation of potential (1 pH unit for a 10 mg per cent solution of glucose flowing at a rate of  $3 \text{ mL min}^{-1}$ ). Alternatively, Clark and Lyons proposed to use a hydrophobic membrane and an oxygen sensing electrode by exploiting the reaction pathway occurring at GOx, as depicted in Fig. 1B [5,9,10]. The latter will be then reviewed, cited, and mentioned as prototype of first-generation enzyme-based biosensor. In the next two decades most of the enzyme-based biosensors will be prototyped considering both configurations. In 1984, Cass et al. reported a second-generation biosensor based on ferrocene as electron accepting molecule instead of oxygen [11], that works as natural electron acceptor for oxidases (e.g., glucose oxidase (GOx), alcohol oxidase (AOx), lactate oxidase (LOx), etc.). The authors reported a layer-by-layer construction onto graphite electrode where the ferrocenium ions are acting as oxidants towards GOx. Ferrocene exhibited several features for the development of second-generation biosensors: (i) high-rate electron transfer between reduced enzyme and ferrocenium ion; (ii) good electrochemical properties of ferrocene; and (iii) low water solubility of ferrocene resulting in the effective confinement of the mediator to the electrode surface.

While discussing the advancements of enzyme-based amperometric biosensors, it is important to distinguish among different types of enzymes with respect to their electrical connection with the electrode surface [12–14]. The first group encompasses enzymes based on nicotinamide adenine dinucleotide oxidised ( $\text{NAD}^+$ ) or nicotinamide adenine dinucleotide phosphate oxidised ( $\text{NADP}^+$ ) like reductases or dehydrogenases. Both electron carriers are weakly or not bound at all to the enzymatic scaffold acting as diffusing electron relays that can be amperometrically assayed [15–17]. In this case, the electrode should be developed considering that the reaction rate of two-electron transfer reaction should be faster than the corresponding single electron transfer

avoiding the formation of radical intermediate species. Moreover, to ensure longer storage stability the enzyme should be physically entrapped or covalently bound considering a certain distance from the electrode that allows for the continuous injection/ejection of substrate/products (electron transfer reaction). Finally, the overpotential needed for the amperometric measurements should be quite small to avoid interferences by other redox molecules. Differently, the enzymes belonging to the second group contain redox moieties that are at the edge of the enzyme scaffold enabling direct electron transfer (DET) [18–20]. Notably, the enzyme orientation affects DET reaction at the electrode considering different immobilisation protocols. Although this would be the simplest electron transfer pathway as described, only few enzymes are able to exchange electrons directly with electrode surfaces due to several constraints [21,22]. The third group encloses enzymes with prosthetic groups strongly bound to the enzymatic scaffold. When adsorbed on electrodes, their redox centres cannot be oxidised/reduced at potentials not harmful for the enzyme. The electron transfer rate will be affected by the distance between their redox centres and the periphery of their protein or glycoprotein shell [23,24].

This concept has been transposed to different generations of biosensors as reviewed in many articles [25–27]. Enzyme-based amperometric biosensors can be sorted in four groups: (i) 1<sup>st</sup> generation biosensors where the substrate oxidation reaction (e.g., D-glucose, ethanol, L-lactate etc.) relates to the reduction of  $\text{O}_2$  (natural electron acceptor for many oxidases) to  $\text{H}_2\text{O}_2$ , both assayed directly at the electrode surface; (ii) 2<sup>nd</sup> generation biosensors based on immobilised electron relays (acceptors/donors) that are able to reduce/oxidise the redox active centre of enzymes during the catalytic process (e.g., pyranose dehydrogenase from *Agaricus meleagris* (PDH), GOx, AOx, etc.); (iii) 2<sup>nd</sup> generation biosensors based on diffusive electron acceptor/donor (e.

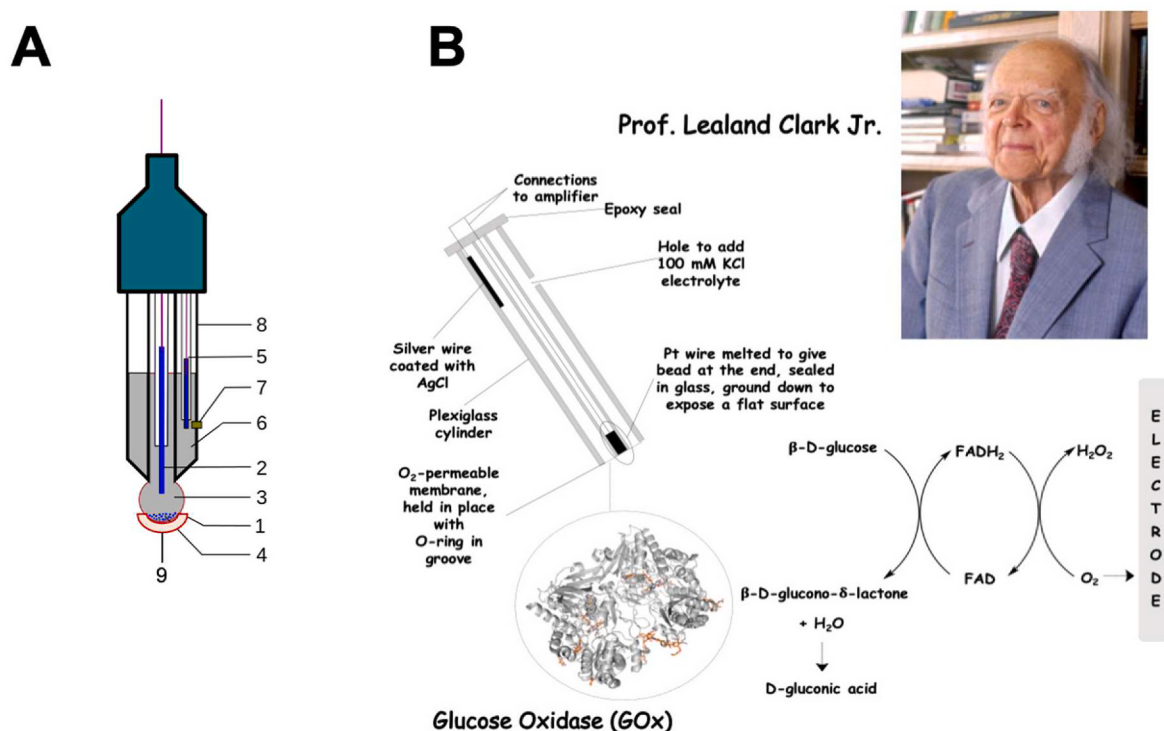

**Fig. 1.** (A) Scheme of pH sensitive glass-membrane electrode modified with GOx cuprophane membrane: 1. pH sensing part of electrode, a bulb made from a specific glass, 2. internal electrode, usually silver chloride electrode or Saturated calomel reference, 3. internal solution, usually 0.1 mol/L MeCl, 4. when using the silver chloride electrode, a small amount of AgCl can precipitate inside the glass electrode, 5. reference electrode, usually the same type as 2, 6. reference internal solution, usually 0.1 mol/L KCl, 7. junction with studied solution, usually made from ceramics or capillary with asbestos or quartz fiber. 8. body of electrode, made from non-conductive glass or plastics, 9. GOx cuprophane membrane; (B) Schematic representation of Clark's electrode to monitor  $\text{O}_2$  variation modified with a glucose oxidase (GOx) membrane known as the first reported glucose biosensor (inset) picture of Prof. Lealand Clark Jr. Panel A is reproduced from [https://commons.wikimedia.org/wiki/File:Glass\\_electrode\\_scheme\\_2.svg](https://commons.wikimedia.org/wiki/File:Glass_electrode_scheme_2.svg) under CC-BY-SA <https://creativecommons.org/licenses/by-sa/3.0/legalcode>. Panel B adopted from Ref. [210] with permission of Wiley.

g., NAD-glucose dehydrogenase where  $\text{NAD}^+$  acts as electron acceptor being converted to NADH later re-oxidised to  $\text{NAD}^+$  etc.); (iv) 3<sup>rd</sup> generation biosensors based on enzymes able to transfer electrons directly from the redox active centre to the electrode surface and *vice versa*, requiring a small overpotential to operate the amperometric detection [28,29].

Besides marking 60 years from the first enzyme-based amperometric biosensor, this review aims at summarising the technological advancements in the field mainly considering three enzyme families: D-glucose oxidising enzymes, D-fructose oxidising enzymes and L-lactate oxidising enzymes. In the next sections, the enzymatic structures of these enzymes will be presented discussing the electron transfer pathways and how they have been exploited for the development of enzyme-based amperometric biosensors. Then, three sections will follow summarising individually for each substrate (D-glucose, D-fructose, and L-lactate) several biosensing platform by comparing their analytical figures of merit. The present review will also address the future scientific and market development of enzyme-based amperometric biosensors eliciting the main challenges within the field.

## 2. D-glucose detection

Most of the research within enzyme-based amperometric biosensors is still focused considering their market within remote medicine devices and personalised medicine [30,31]. Glucose biosensors are mostly based on glucose oxidation catalysed either by oxidases or dehydrogenases.


### 2.1. D-glucose oxidising enzymes

Glucose biosensors are mostly using the following enzymes as bio-recognition elements: *Aspergillus niger* glucose oxidase (AnGOx) [32], nicotinamide amide dinucleotide (NAD)-glucose dehydrogenase [33], pyrroloquinoline quinone (PQQ)-glucose dehydrogenase [34–36], flavin adenine dinucleotide (FAD)-glucose dehydrogenase [37], cellobiose

dehydrogenases from Ascomycetes [38–40], pyranose dehydrogenase from *Agaricus meleagris* (AmPDH) and pyranose oxidase [41]. Their enzymatic structures are reported in Fig. 2.

AnGOx was defined as “an ideal enzyme” in the early 1990s [42,43]. Although it is no longer so “ideal”, AnGOx is still widely used in glucose biosensors development. GOx belongs to the CAZy auxiliary activity family 3 (AA3), which encompasses enzymes from the glucose-methanol-choline (GMC) family [44]. AA family enzymes are involved in glycoside hydrolysis and degradation of lignocellulose. AnGOx exhibits several drawbacks: (i)  $\text{O}_2$  as natural electron acceptor will always, if present, compete with any artificial mediator introduced into the system to lower the high oxidation overpotential, consequently producing  $\text{H}_2\text{O}_2$ , mainly responsible for enzyme degradation; (ii) flavin adenine dinucleotide (FAD) redox centre is strongly but not covalently bound and immobilising AnGOx on an electrode surface may trigger protein unfolding accompanied by FAD ejection (being wrongly interpreted as the enzyme bound FAD), (iii) as GOx oxidises glucose on the C1 carbon, it is only active for the  $\beta$ -form, and (iv) the glycosylated wild type enzyme does not exhibit any direct electron transfer (DET) features given the thickness of glycosylation shell ( $>18$  Å). Most of the researchers focused on DET not only as a scientific challenge but also for practical reasons to simplify biosensors and minimise the influence of other possible interfering components on the amperometric output [45]. However, the electron transfer process through AnGOx takes place as follows:


FAD accepts the electrons donated from D-glucose molecule being reduced to  $\text{FADH}_2$  (equation (1));



The cofactor is regenerated by reacting with  $\text{O}_2$ , leading to the formation of  $\text{H}_2\text{O}_2$  (equation (2));



In the last step,  $\text{H}_2\text{O}_2$  is oxidised at a modified electrode (equation

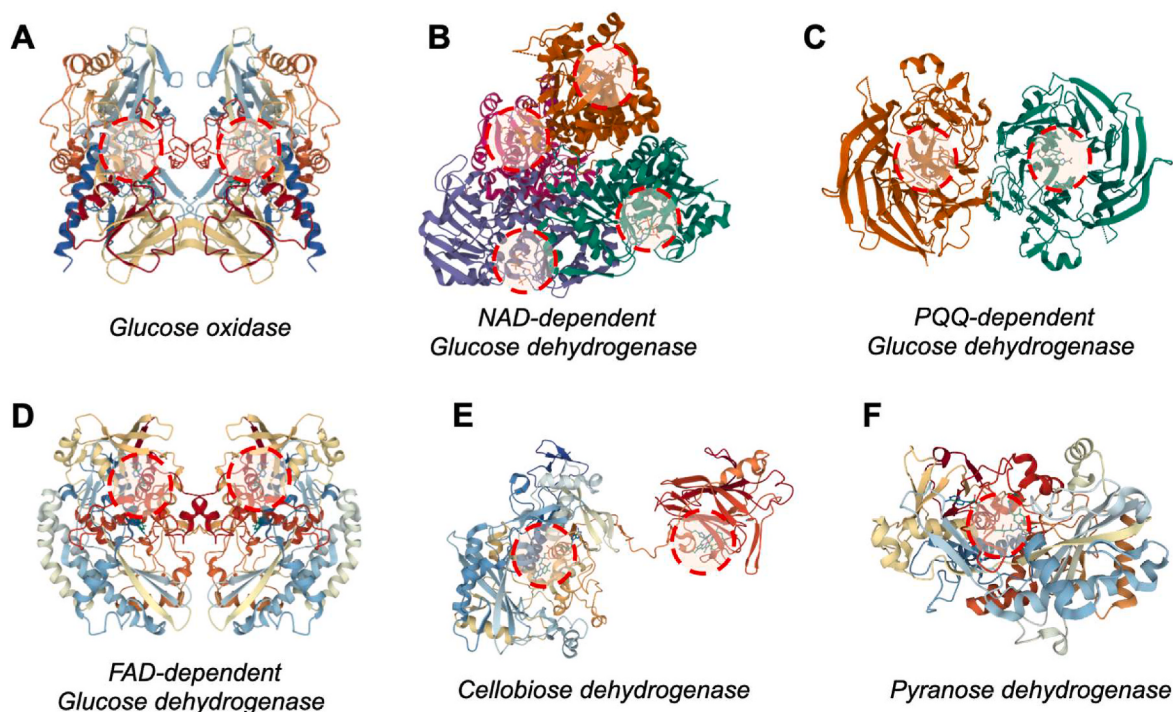

**Fig. 2.** Crystal structures of (A) glucose oxidase from *Aspergillus niger* (PDB file: 1GAL); (B) *Sulfolobus solfataricus* Glucose Dehydrogenase 1 (PDB file: 2CDB); (C) PQQ-dependent Glucose Dehydrogenase from *Acinetobacter calcoaceticus* (PDB file: 1CQ1); (D) *Aspergillus flavus* FADGDH (PDB file: 4YNU); (E) Cellobiose dehydrogenase from *Neurospora crassa* NcCDH (PDB file: 4QI7); (F) pyranose dehydrogenase from *Agaricus meleagris* (PDB file: 4H7U). The redox centres are highlighted with red circles. (For interpretation of the references to colour in this figure legend, the reader is referred to the Web version of this article.)

(3)) either Prussian Blue (PB) or noble metal (e.g., platinum, rhodium etc.), being proportional to glucose oxidised molecules (analytical targets) [46,47].




Indeed, several approaches aiming at minimising the influence of  $\text{O}_2$  on  $\text{AnGOx}$  have been explored towards the development of glucose biosensors. For instance,  $\text{AnGOx}$  can be immobilised within thick osmium redox hydrogels where  $\text{O}_2$  is consumed in the outer sensor layer. Although a considerable volume of the hydrogel is not involved in the catalytic response creating a mass-transfer barrier, the absence of  $\text{O}_2$  in the inner area does not hinder the electron transfer to osmium atoms [48,49]. Instead, mass-transfer limitations can be avoided by exploiting a layer-by-layer construction of the electrode platform, for example alternating poly-(allylamine) osmium redox mediator and  $\text{AnGOx}$  layers [50].

Alternatively, enzymatic bioengineering can be a viable tool to improve selectively the enzymatic activity towards a certain substrate [51]. In this regard, Marin-Navarro et al. increased the activity and thermal stability of  $\text{AnGOx}$  through two mutations: T554 M generating a sulfur-II interaction and Q90R/Y509E resulting in a new salt bridge near the interphase of the dimeric protein structure [52]. In another report,  $\text{AnGOx}$  stability was improved by varying the net charge of the enzyme from  $-67$  to  $+78$  via chemical modification of its  $-\text{COOH}$  groups with polyamines. All chemically modified  $\text{AnGOx}(n)$  were adsorbed onto graphene oxide (GO) modified electrode. While controlling the net charge, the authors were able to retain  $\text{AnGOx}$  activity preventing protein unfolding that may occur during the enzyme operation [53].

Another research direction explored to decrease  $\text{O}_2$  sensitivity of  $\text{AnGOx}$  was pursued by replacing the natural flavin with 7,8-dichloro-FAD [54] or through genetic engineering “site-directed mutations on Val464 of GOx from *Penicillium amagasakiense*” [55].

$\text{AnGOx}$  was alternatively replaced with other  $\text{D-glucose}$  oxidising enzymes. For instance, glucose dehydrogenases (GDHs) (soluble and membrane bound) possessing pyrroloquinoline quinone (PQQ) [56–59] and flavin adenine dinucleotide (FAD) [60–62] as the prosthetic group, respectively, have been highly focused as a possible ideal enzyme for mediator-type glucose biosensor, because of its high catalytic efficiency ( $k_{\text{cat}}/K_{\text{m}}$ ) and independence of  $\text{O}_2$ . However, GDHs also exhibit substrate specificity (oxidation of  $\beta$ -form) and thermal stability [63]. The quino-protein GDH uses PQQ cofactor as electron relays (equation (4)):



Indeed, this ET mechanism does not require any additional electron acceptor like oxygen or  $\text{NAD}^+$ . PQQ(red) is later re-oxidised at the electrode surface. PQQ-GDH owns a high electron transfer rate system especially while compared to other glucose oxidising systems. PQQ-GDH stability can be increased through protein engineering and addition of  $\text{Ca}^{2+}$  ions that enhance the electron transfer rate from PQQ groups [64,65].



Regarding PQQ-GDH, there are several claims about its DET features, which can be argued considering PQQ as mediator itself [66–68]. In addition, PQQ-GDH is less selective particularly with respect to maltose (oligomeric form containing two  $\text{D-glucose}$  units). However, EFCs are mostly based on PQQ-GDH modified electrodes, where selectivity should not be accounted [69–71].

Besides PQQ-GDH, FAD-dependent GDH can be exploited to develop glucose biosensors that are  $\text{O}_2$  insensitive. Several types of FAD-GDHs have been investigated such as FAD-GDH from *A. sp.* (e.g., *A. terreus*, *A. niger*), *Thermoascus crustaceus* and *Glomerella cingulata* coupled to electrodes through mediated electron transfer [72–75]. Moreover, DET of FAD-GDH has been recently achieved combining *T. crustaceus* FAD-GDH with SWCNT [76]. Alternatively, FAD-GDH has been recently fused with a molecular mediator, so called 2.5th generation biosensor [77], and with a minimal cytochrome *c* reported as DET [78,79].

Despite several papers based on NAD-dependent GDH, this enzyme is

not considered a good candidate for glucose biosensors development mainly because of diffusing electron acceptors, not efficiently re-oxidised at the modified electrode surface (i.e.,  $\text{NAD}^+/\text{NADH}$  redox couple that exhibits complex electrochemistry in both states) [80,81].

NAD-dependent GDH oxidises  $\text{D-glucose}$  to  $\delta$ -glucolactone transferring two electrons to  $\text{NAD}^+$  that is reduced to NADH. The latter is re-oxidised at the electrode surface from a mediator/catalyst as schematically reported below (equations (5) and (6)):



Furthermore, many studies focused on alternative FAD-dependent  $\text{D-glucose}$  oxidising enzymes like pyranose oxidase (glucose 2-oxidase, POx), pyranose dehydrogenase (PDH), cellobiose dehydrogenase (CDH) from Ascomycetes. Differently from previously reported glucose oxidising enzymes, POx and PDH oxidise sugars not at C1 but at C2/C3 because they are anomeric insensitive. In addition, they can oxidise sugars multiple times, and PDH owns a covalently bound FAD-cofactor, ensuring long-term stability, which is usually an issue for enzyme-based amperometric biosensors [41,82,83].

Cellobiose dehydrogenases (CDHs) are different from the structural point of view, encompassing two different domains: a catalytic FAD domain (dehydrogenase type) and a *heme b*-cytochrome domain as a “built in mediator” [40,84]. Only Class II CDHs from Ascomycetes are able to oxidise glucose [85,86].

## 2.2. *D-glucose* biosensors

In this section, the most representative cases of amperometric glucose biosensors based on glucose oxidase, PQQ-, FAD- and NAD-dependent GDH (mostly last decade) are discussed considering pros and cons about the electrode modification and technological advancement.

Considering Clark's research, many glucose sensing electrodes were initially developed considering enzyme-based membranes. They exhibited many advantages like high selectivity (depending on membrane permeability) [87] towards many interferents present in bodily fluids and enhanced linear range mainly due to diffusion limitations. However, they suffered  $\text{pO}_2$  variations in blood, hence, needing an additional control with a non-enzymatic  $\text{O}_2$  electrode to normalise the current output [88]. Exploiting a platinum electrode, the potential applied for the oxidation of  $\text{H}_2\text{O}_2$  is quite high (at least 0.6 V vs. Ag/AgCl). Conversely, on modified solid electrodes (without membrane), the overpotential for  $\text{H}_2\text{O}_2$  oxidation/reduction could be lowered close to 0.0 V (vs. Ag/AgCl) to enhance current output and selectivity. Many examples modifying the electrode surface with Prussian Blue (PB), also known as ferric hexacyanoferrate have been reported [89–91]. Alternatively, the electrode can be modified with several nanomaterials and polymers to facilitate electron transfer processes [92,93]. Horseradish peroxidase (HRP) has been also used as a biocatalyst for  $\text{H}_2\text{O}_2$  reduction, increasing the selectivity but also increasing the complexity of biosensors. In this case, the stability of the enzyme layer could be enhanced by using immobilisation strategies relying on physical entrapment (e.g., Nafion layers etc.) [94,95].


Alternatively, to minimise the electrochemical interferents several molecular mediators like ferrocene [96], neutral red [97], and osmium polymers [98], have been exploited to develop 2<sup>nd</sup> generation glucose biosensors. However, the competition between  $\text{O}_2$  and other electron mediators should be accounted. For example, thermally reduced graphene oxide was combined with a conducting polymer, namely polyaniline (PANI), to support the immobilisation of GOx physically entrapped within glutaraldehyde layer operating both as 1<sup>st</sup> ( $\text{H}_2\text{O}_2$  oxidation at the electrode) and 2<sup>nd</sup> generation (mediated by diffusing N-methylphenazonium methyl sulfate (PMS)). Indeed, this platform exhibited an extended linear range due to the combination of both

electron transfer pathways and the presence of a membrane-like layer limiting substrate diffusion [99]. A similar approach has been exploited by Ramanavicius with the development of reagent-less glucose biosensor based on a nanobiocomposite, namely poly(1, 10-phenanthroline-5,6-dione), poly(pyrrole-2-carboxylic acid) covalently linking GOx (via EDC/NHS reaction) and mixed with gold nanoparticles. Notably, the nanobiocomposite material was acting both as mediator and as immobilising linker. Also in this case, the extended linear range resulted from the competition of both electron transfer pathways (1<sup>st</sup> and 2<sup>nd</sup> generation). Conversely, the presence of gold nanoparticles ensured higher enzyme stability (retained 96% of initial signal after 14 days) [100]. Moreover, some efforts have been focused on the immobilisation of GOx by using chitosan (natural linear amine-rich polysaccharide) or other cross-linking agents like glutaraldehyde or thiol linkers to enhance the enzyme loading [101,102]. Recently, GOx based devices have been implemented on alternative scaffolds towards wearable or minimally invasive biomedical applications. For instance, filter paper was proposed as a bioreactor for the synthesis of PB nanoparticles, used as a catalyst for H<sub>2</sub>O<sub>2</sub> reduction (produced by GOx upon glucose oxidation). This platform was developed by using both wax- and screen-printing techniques. In particular, the former was used to design the area dedicated for the deposition of PB nanoparticles, while the latter was employed to print the three-electrode electrochemical configuration. Paper Blue biosensor exhibited a linear range up to 5 mM, with a sensitivity of 1.70  $\mu\text{A}/\text{mM}$ , and a LOD of 0.17 mM for H<sub>2</sub>O<sub>2</sub> detection, while a linear range up to 25 mM for glucose detection. The porosity of the paper was exploited to store the reagents to develop reagent-free PoC devices, as shown in Fig. 3 [103]. Alternatively, a glucose biosensing systems have been also integrated into highly stretchable and microneedles-based platforms towards next generation electronic textile for minimally invasive and continuous biomarkers monitoring [104–107]. Despite the immobilisation strategy and the integration of nanomaterials and conductive polymers [108–110] as well as in novel minimally invasive platforms, the limit of detection for GOx-based 2nd generation glucose biosensors is still in the micromolar range as well as the dynamic linear range is quite narrow mainly due to


the limited amount of enzyme molecules tightly connected to the electron mediator and the presence of O<sub>2</sub>, acting as natural electron acceptor for GOx.

To overcome the O<sub>2</sub> dependence, many researchers employed oxygen-independent pyrrole quinoline quinone glucose dehydrogenase (PQQ-GDH). Despite its ability to communicate in DET, PQQ-GDH was initially used with diffusing and immobilised redox mediators, namely ferricyanide [111], 2,4,7-trinitro-9-fluorenone (TNF) [112] and osmium redox polymers [113] obtaining quite extended dynamic linear ranges probably due to the possibility of the enzyme to communicate both directly and through the electronic mediator. To realise a DET-based biosensor, PQQ-GDH from *Acinetobacter calcoaceticus* was covalently immobilised onto a composite based on polyaniline and MWCNTs deposited on gold electrode exhibiting a wide linear range [114]. due to the properties of conducting polymers improving the electron transfer rate and increasing the enzyme loading. The same research group proposed the assembling of electroactive multilayers assisted by deoxyribonucleic acid (DNA) as a negatively charged building block [115] to achieve an artificial signal chain. Despite tailoring a novel electrode surface that can be potentially used to create biomimicking machinery, this platform has a limited catalytic efficiency as well as analytical figures of merit. Successively, Lisdat and his co-workers reported the electron transfer process of PQQ-GDH onto polythiophene copolymers modified MWCNTs, as shown in Fig. 4 [116]. In this particular case, the authors deposited thiols ended CNTs, followed by the electropolymerisation of different thiophene monomers performed in organic solvent, later thoroughly rinsed with water to avoid any protein inactivation. The bioelectrocatalytic response was linear from 1  $\mu\text{M}$  to 500  $\mu\text{M}$ . Later, the same authors attempted the same electropolymerisation in water-based monomer solution obtaining a wider dynamic linear range up to 2 mM probably due to the variation of apparent Michaelis constant of the enzyme onto the modified electrode [117].

Alternatively, another O<sub>2</sub> independent GDH (FAD-dependent) from *Aspergillus species* deposited onto MWCNTs modified with chitosan was employed [118]. Specifically, FAD-dependent GDH were extracted from *Aspergillus* sp. and *Aspergillus oryzae*, exhibiting similar performance in

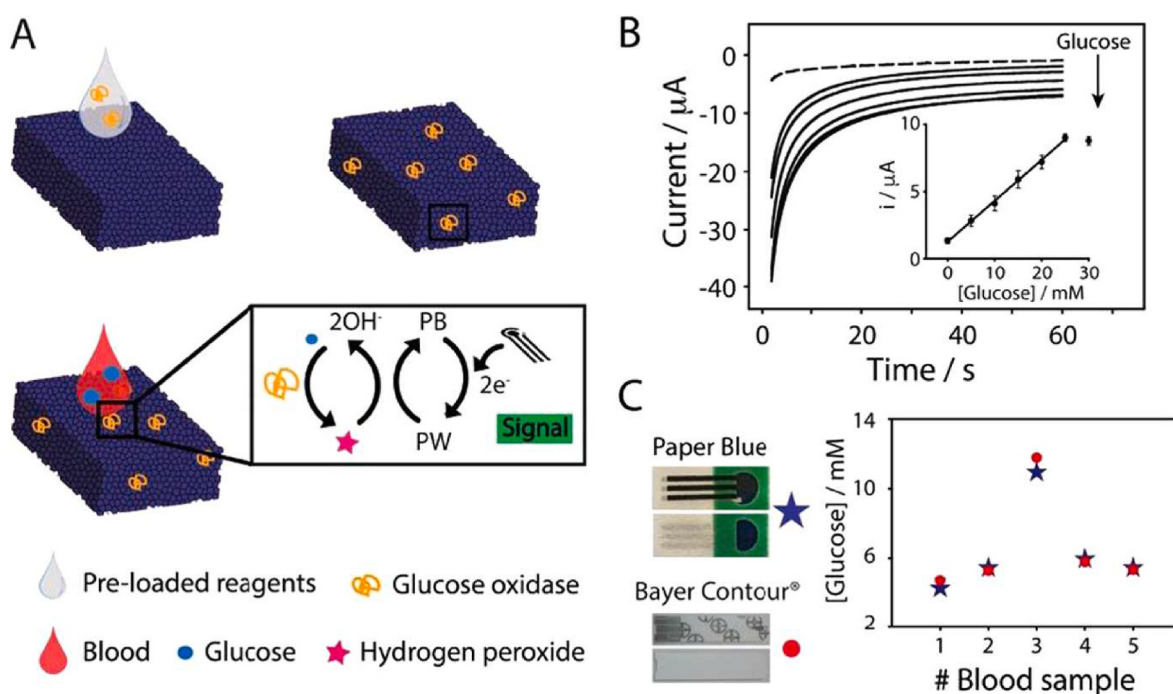

**Fig. 3.** (A) Scheme of Paper Blue biosensor. (B) Calibration curve and amperometric responses upon addition of glucose up to 30 mM. (C) Comparison Paper Blue with Bayer Contour® on 5 blood samples. Reproduced with permission of Elsevier Ltd from Ref. [103]. (For interpretation of the references to colour in this figure legend, the reader is referred to the Web version of this article.)

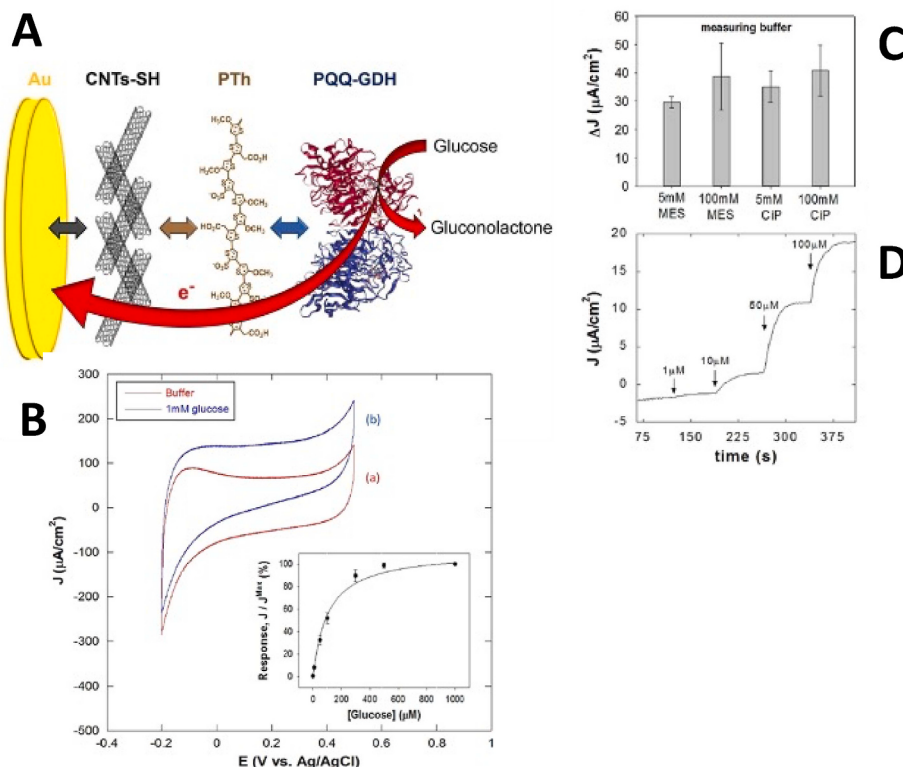

**Fig. 4.** (A) Schematic representation of PQQ-GDH modified electrode; (B) Cyclic voltammograms before (a, red curve) and after (b, blue curve) the addition of 1 mM glucose, (scan rate 10 mV/s) and insert plot of the amperometric current density versus the glucose concentration in stirred solution measured by amperometry at 0 V vs. Ag/AgCl; (C) Evaluation of the effect of the measuring buffer solution on the bioelectrocatalysis in presence of 1 mM glucose; (D) Amperometric experiment performed at a fixed potential of 0 V vs. Ag/AgCl and measuring the anodic current density with additions of glucose to the stirred solution. Experiments were performed in 100 mM CiP buffer, 1 mM CaCl<sub>2</sub>, pH 6.5. Error bars refer to the standard deviations calculated from three different electrodes (PQQ-GDH/PTh/MWCNTs/Au). Abbreviations: gold electrode (Au), thiol ended multi walled carbon nanotubes (CNTs-SH), polythiophenes (PTh), PQQ-dependent glucose dehydrogenase (PQQ-GDH), 2-ethanesulfonic acid (MES) and citrate-phosphate buffer (CiP). Panels A–D reproduced from Ref. [116] with permission of Elsevier Ltd. (For interpretation of the references to colour in this figure legend, the reader is referred to the Web version of this article.)

MET, with a long storage-stability (6 months) due to the effective connection enzyme-mediator and its insensitivity to O<sub>2</sub>.

In another report, Cohen et al. cloned, overexpressed, and purified the FAD-GDH from *T. emersonii* in *E. coli*. After biochemical characterisation, the amperometric biodevice reported a linear range 0–20 mM by operating both in MET and DET [119].

Even not being the best O<sub>2</sub> independent candidate glucose oxidising enzyme, NAD-dependent GDH has been used to develop several sensing platforms. Using several iron-sulfur cluster both to enhance the electron transfer and wire NAD-dependent GDH [120], the authors obtained a linearly dependent response in the range 0.1–100 mM with a LOD varying based on Fe–S structure. The metal-anchorable sulfur atom, the strong  $\pi$ -coordinating iron atom, the favorable redox properties, low cost, and natural abundance make Fe–S an excellent electron-mediating relay capable of wiring redox active sites to electrode surfaces. Alternatively, the combination of GDH with diaphorase onto Osmium Redox Polymers (ORP) bound through avidin-biotin complex on indium tin oxide (ITO) electrodes, successfully employed for glucose sensing in artificial human serum avidin solution (5% w/v) [121].

A novel approach has been proposed by Zebda et al., who reported the integration of NAD<sup>+</sup> dependent GDH with 3D carbon nanotube network modified with poly-methylene green. The proposed electrode reported an onset potential for glucose oxidation at  $-0.2$  V vs SCE, achieving a plateau already at  $+0.1$  V, potentially minimising the effect of several interferents on the analytical response. The pellet-based platform reported a linear range 50  $\mu$ M–20 mM with a sensitivity of  $50.8 \cdot 10^{-3}$  A mM<sup>-1</sup> cm<sup>-2</sup> and a stability over 1 year [122].

Dilgin et al. immobilised NAD-dependent GDH from *Pseudomonas* onto pyrocatechol violet (Pcv)-modified graphite pencil electrode (GPE), where Pcv is acting as a catalyst towards the oxidation of NADH (enzymatically generated) to NAD<sup>+</sup>. The proposed biosensor exhibited a linear response within the range 5–500  $\mu$ M with a LOD of 1.2  $\mu$ M and a sensitivity of 2.78 nA  $\mu$ M<sup>-1</sup> cm<sup>-2</sup>. In addition, to minimise the effect of electrochemical interferents like ascorbic acid, uric acid and dopamine, usually present in biomedical and food samples, the authors used a

water-insoluble pre-oxidant within the flow injection analysis system, namely sodium bismuthate. This approach allowed to perform a selective glucose detection in real samples without further electrode modification (e.g., selective membrane deposition etc.) [123].

The analytical figures of merit like limit of detection (LOD), dynamic linear range, sensitivity and storage stability are summarised in Table 1 for quantitative comparison. The dynamic linear range is limited by two parameters the intrinsic K<sub>M</sub>, related to the enzyme properties like substrate affinity or isoelectric point (important for protein conformation and orientation on the electrode surface), and the apparent K<sub>M</sub>, mostly affected by the electronic connection of the enzyme with the electrode (in 1<sup>st</sup>, 2<sup>nd</sup> or 3<sup>rd</sup> generation) and the morphology of the electrode surface (i.e., the presence of nanomaterials, electrode porosity, presence of membranes etc.). Indeed, the presence of membranes or porous electrode structure are hindering the diffusion of the substrate towards the enzyme increasing the apparent K<sub>M</sub>, resulting in the extension of dynamic linear range. The sensitivity (considered as the slope of the calibration curve) and LOD are mostly affected by the enzyme loading where immobilisation strategies, nanomaterials and electronic mediators are playing an important role towards increasing the sensitivity and decreasing the LOD. Most of the electrode platforms herein reviewed, exhibited a good storage stability (>50% of initial activity retained after few weeks) mainly due to the presence of nanomaterials acting as stabilising materials.

### 3. D-fructose detection

The detection of D-fructose has been relevantly under-taken in the last decades, but high fructose consumption will may cause an endemic obesity status not only because of diabetes type II mellitus (glucose intake related pathology) [124,125]. Nowadays, the consumption high-fructose corn syrup (HFCS) beverages as well as soft drinks has become very popular among young generations causing more often the onset of obesity at paediatric level [126]. This may occur because of the increased production of non-alcoholic fatty liver. Over 70% of all foods

**Table 1**

Analytical figures of merit for reviewed glucose biosensors. Abbreviations: glucose oxidase (GOx), horseradish peroxidase (HRP), poly(toluidine blue) (pTB), reduced graphene oxide (rGO), glassy carbon electrode (GCE), polyaniline:reduced graphene oxide composite (PANI:rGO), graphite (GR), poly(pyrrole-2-carboxylic acid) (PPCA), gold nanoparticles (AuNPs), poly(1,10-phenanthroline-5,6-dione) (PPD), chitosan (Chit), Prussian Blue (PB), gold deposited on styrene-ethylene/butylene-styrene fibers (Au-SEBS), screen-printed carbon electrodes (SPCE), nafion (Naf), Nickel Hexacyanoferrate (NiHx), polyacrylic acid (PAA), poly(3,4-ethylenedioxythiophene) (PEDOT), PQQ-dependent glucose dehydrogenase (PQQ-GDH), thiophene polymer (ThP), thiolated carbon nanotubes (CNTs-SH), gold electrode (Au), NAD-dependent glucose dehydrogenase (NAD-GDH), poly-methylene green (pMG), 3D-carbon network (3DC), pyrocatechol violet (Pcv), graphite pencil electrode (GPE).

| Electrode Platform                                     | Linear Range/<br>mM | Sensitivity                                           | Limit of Detection/<br>mM | Stability                                         | Ref   |
|--------------------------------------------------------|---------------------|-------------------------------------------------------|---------------------------|---------------------------------------------------|-------|
| GOx-HRP-PTB/rGO/GCE                                    | 0.08–1              | 0.34 $\mu\text{A mM}^{-1}$                            | 0.05                      | 50% of the original output retained after 2 weeks | [94]  |
| GOx/PANI:rGO/GR                                        | 0.5–50              | 2.8 $\mu\text{A mM}^{-1}$                             | 0.089                     | 50% of original output retained after 8 days      | [99]  |
| GOx-PPCA(AuNPs)/PPD/GR                                 | 0.2–150             | 0.135 $\mu\text{A mM}^{-1}$                           | 0.08                      | 96% of original signal after 14 days              | [100] |
| Chit-GOx/PB/Au-SEBS                                    | <0.5                | 11.7 $\mu\text{A mM}^{-1} \text{cm}^{-2}$             | 0.006                     | 8 days                                            | [104] |
| GOx/PB/rGO/SPCE                                        | <3 4–8              | 27.78 $\mu\text{A mM}^{-1} \text{cm}^{-2}$            | 0.00794                   | 15 days                                           | [106] |
| Naf/GOx/NiHx/PB/SPCE                                   | 2.5–15              | 109.7 nA $\text{mM}^{-1}$                             | /                         | 14 h of continuous operation                      | [107] |
| Chit/GOx/TiO <sub>2</sub> NTs/Ti                       | 0.3–1.5             | 5.46 $\mu\text{A mM}^{-1}$                            | 0.07                      | 85% of initial current after 30 days              | [108] |
| GOx/PB/Carbon                                          | 0.25–2              | 2.14 $\mu\text{A mM}^{-1}$                            | 0.01                      | 72% of initial current after 45 days              | [109] |
| GOx/PAA/PEDOT                                          | 0.96–30             | 2.74 $\times 10^{-4} \text{ A M}^{-1}$                | 0.29                      | 30 days                                           | [110] |
| PQQ-GDH/ThP/CNTs-SH/Au (aqueous electropolymerisation) | 0.05–0.5            | 246 $\mu\text{A cm}^{-2} \text{mM}^{-1}$              | 0.001                     | 70% of initial signal retained after 15 days      | [117] |
| NAD-GDH/pMG/3DC                                        | 0.5–20              | 50.8 $\cdot 10^{-3} \text{ A mM}^{-1} \text{cm}^{-2}$ | /                         | 1 year                                            | [122] |
| NAD-GDH/Pcv/GPE                                        | 0.05–0.5            | 2.78 nA $\mu\text{M}^{-1} \text{cm}^{-2}$             | 1.2                       | /                                                 | [123] |

contain some amounts of added sugar, and consumption of soft drinks increased by five times since 1950 [127]. Data analysis suggested that consumption of sugar-sweetened beverages is related to the risk of diabetes, the metabolic syndrome and cardiovascular disease in adults and in children. Drinking two sugar-sweetened beverages per day for 6 months induced features of the metabolic syndrome and fatty liver. In this regard, the development of highly selective and sensitive biosensing platform will play a key role in the early detection as well in the development of personalised treatment based on remotely operating physicians. This will enable a powerful control of this high-risk pathology as well the correct management without the needs of hospitalisation [128,129].

Most of fructose biosensors, if not all, are developed considering fructose dehydrogenase (FDH) as bioreceptor. Fructose dehydrogenase is a membrane-bound oxidoreductase extracted from bacteria belonging to the acetic acid bacteria (AAB) family. In this group, only *Acetobacter* and *Gluconobacter* can oxidise D-fructose producing 5-keto-D-fructose. In the past, it was believed as PQQ-dependent protein [130], but recently Kano and his group demonstrated the presence of a flavin DH type domain and 3 heme c in the cytochrome domain. Hence, the protein now is enclosed in the flavohemoproteins family [131,132].

FDH, being a heterotrimeric protein, encompasses three subunits: subunit I (DH<sub>FDH</sub>), which is the catalytic domain, with a flavin group able to oxidise D-fructose to 5-keto-D-fructose in a  $2\text{H}^+/2\text{e}^-$  electron transfer process; subunit II (CYT<sub>FDH</sub>), acting as a built-in electron acceptor with three heme c moieties covalently bound to the enzyme scaffold (only two heme c are involved in the electron transfer process); and subunit III, ensuring the enzyme stability [4,133–135]. Unfortunately, its crystal structure is still under investigation. This would enable the development of highly efficient enzyme-based amperometric biosensors considering the possibility to engineer specific sites within the enzymatic structure.

The electron process occurs in three steps: (i) oxidation of D-fructose with the concomitant reduction of FAD to FADH<sub>2</sub>; followed by (ii) FADH<sub>2</sub> reoxidation in two sub-sequent monoelectronic processes, eliciting an internal electron transfer (iii) that propagates through CYT<sub>FDH</sub> domain involving heme c<sub>1</sub> and heme c<sub>2</sub>.

In the presence of a redox mediator, this can mediate both the electron transfer from the flavin DH domain and from the cytochrome domain. It would be hard to understand the preferred pathway, hence they are classified as 2nd generation biosensors [136].

Few examples of FDH based biosensors will be reviewed considering the analytical figures of merit, which are resumed in Table 2. As reported in Table 2, all platforms exhibited a relatively extended linear range (considering the intrinsic  $K_M \sim 8$ ) [137]. The sensitivity is mostly affected by the enzyme loading (electroactive area). Most of the FDH-based electrodes have been tested with flow injection analysis (FIA) because of their potential integration in an on-line sensing unit in a manufacturing process. Using biosensors in industrial bioprocess monitoring and control has been hindered by the absence of adequate sampling techniques.

Considering FDH as a membrane-bound protein, other scientists

**Table 2**

Analytical figures of merit for reviewed fructose biosensors. Abbreviations: fructose dehydrogenase (FDH), carbon nanotubes (CNTs), liquid cubic phase (LCP), thermally reduced graphene oxide (TRGO), 3-mercaptopropionic acid (3-MPA), nanoporous gold (NPG), 2-carboxy-6-naphthoyl (CNPh), 4-mercaptophenol (4-MPh), highly porous gold (h-PG), 2-aminoanthracene (2-ANT), single walled carbon nanotubes (SWCNTs), glassy carbon electrode (GCE).

| Electrode Platform   | Linear Range/<br>mM | Sensitivity                                        | Limit of Detection/<br>mM | Stability                                     | Ref   |
|----------------------|---------------------|----------------------------------------------------|---------------------------|-----------------------------------------------|-------|
| FDH/LCP/CNTs/Carbon  | <10                 | 4 $\mu\text{A mM}^{-1}$                            | /                         | /                                             | [138] |
| FDH/TRGO/Carbon      | 0.7–8.8             | 14.5 $\mu\text{A mM}^{-1} \text{cm}^{-2}$          | 0.7                       | 10% decrease after 5 days                     | [139] |
| FDH/3-MPA/NPG        | 0.05–0.3            | 3.7 $\mu\text{A } \mu\text{M}^{-1} \text{cm}^{-2}$ | 0.0012                    | 25% retained after 6 days                     | [142] |
| FDH/CNPh/NPG         | 0.05–0.3            | 3.7 $\mu\text{A } \mu\text{M}^{-1} \text{cm}^{-2}$ | 0.0012                    | 40% retained after 6 days                     | [142] |
| FDH/4-MPh/h-PG       | 0.05–5              | 175 $\mu\text{A mM}^{-1} \text{cm}^{-2}$           | 0.0003                    | 90% of original output retained after 90 days | [143] |
| FDH/2-ANT/SWCNTs/GCE | 0.05–5              | 47 $\mu\text{A mM}^{-1} \text{cm}^{-2}$            | 0.0009                    | 90% of original output retained after 60 days | [146] |

tried to recreate a comfortable environment for the enzyme using crystalline cubic phase (LCP) and CNTs (combination of hydrophobic materials) [138] or thermally reduced graphene oxide [139].

The influence of gold nanopores on the bioelectrocatalytic behaviour of FDH investigated. Indeed, the authors reported a wet chemistry based method, notably de-alloying, for the preparation of nanopores with controlled size ranging from 9 up to 62 nm [140,141]. The electrode was further modified either with a self-assembled monolayer of 3-mercaptopropionic acid (3-MPA) or via diazonium salt electrografting of 2-carboxy-6-naphthoyl moieties. FDH was finally cross-linked onto the modified electrode through carbodiimide (CMC), as displayed in Fig. 5. The proposed biosensors reported a linearity in the amperometric response within the range of 0.05–0.3 mM, with a LOD of 1.2  $\mu\text{M}$  and a sensitivity of 3.7  $\mu\text{A cm}^{-2} \mu\text{M}^{-1}$  [142].

By increasing the pore sizes ranging from 10 up to 50  $\mu\text{m}$  (internal nanoporous structure) it was possible to enhance real surface area from 0.073  $\text{cm}^2$  to 24  $\text{cm}^2$  (300 times higher) [143]. The proposed biosensor exhibited a dynamic linear range 10 times larger compared to the previous platform probably because of the increased porosity of the electrode surface that hinders the diffusion of the substrate (also controlled through FIA).

Similarly, FDH was immobilised on a porous gold microelectrode to achieve a substrate-transfer-controlled current. Indeed, the anodization of the microdisk electrode allowed to increase the surface area by 170-fold, with pores sizes within the range 20–200 nm. The authors hypothesised that the concave shape of the pores would be able to orient FDH more effectively, resulting in a mass-transfer limited current roughly 300 times higher than the planar electrode. The proposed platform exhibited a linear range up to 10 mM with enhanced selectivity towards both enzymatic and electrochemical interferents. The catalytic current density for the oxidation of 1.0 mM D-fructose is independent of the storage time for up to 6 days [144]. Moreover, FDH could be stabilised by using self-assembled monolayers (SAMs) growth onto NPG electrodes, where the authors realized a site-oriented immobilisation based on the study of charge distribution of FDH surface. Electrostatic surface mapping evidenced the distribution of polar/hydrophilic amino acid residues, which shows an overall quite hydrophilic surface with both positive and negative charges nearby the heme 2c [145].

Alternatively, the possibility to perform a site-oriented immobilisation of FDH was performed through a hydrophobic pocket within the second subunit of the enzyme, being very close to the heme  $c_1$  and  $c_2$  responsible as built-in mediators for the DET mechanism of FDH. The

electrode was modified through the electrografting of diazonium salt of 2-aminoanthracene on the surface of single walled carbon nanotubes (SWCNTs). As shown in Fig. 6, it was possible to isolate the contribution of each heme to the electrocatalytic wave (overall  $485 \pm 21 \mu\text{A cm}^{-2}$  at 0.4 V). FDH/2-ANT/SWCNT/GCE platform exhibited a great stability retaining 90% of the activity after 60 days, with a LOD of 0.9  $\mu\text{M}$  and a very high sensitivity ( $47 \pm 1 \mu\text{A mM}^{-1} \text{cm}^{-2}$ ) [146]. In 2021, it was attempted as a proof-of-concept the development of 'real' self-powered biosensor trying to exploit the concept of self-charging bio-supercapacitors [147]. Notably, the device encompassed two different parts: biocatalytic electrodes and charge storing elements. In this regard, the biocatalytic electrode where working as a normal enzymatic fuel cell depending on D-fructose concentration, while the charge storing part was needed to supply energy to the analytical device. This represents an extremely new concept that enabled not only to obtain a self-standing biosensor (charging time 70 min) but also an enhanced sensitivity, notably  $3.82 \pm 0.01 \text{mW cm}^{-2} \text{mM}^{-1}$ , which is 100 times higher with

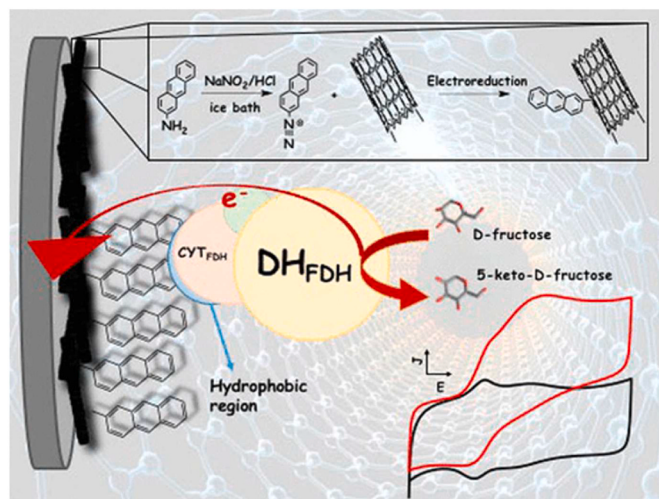


Fig. 6. Schematic representation of FDH modified electrode with the electrografting of *in situ* prepared diazonium salt of 2-aminoanthracene cation acting as a plug-in for the hydrophobic pocket in the second subunit of FDH. This figure was reproduced from Ref. [146] with permission of the American Chemical Society (ACS).

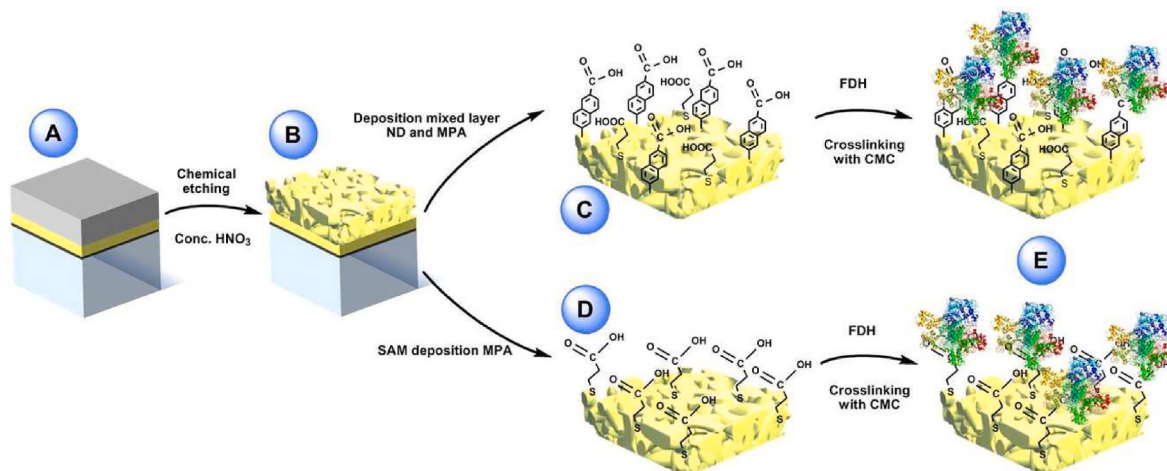


Fig. 5. (A) Sputtered glass sheet with layers of titanium, pure gold and gold/silver alloy (bottom to top). (B) Nanoporous gold (NPG) electrode surface post-dealloying by concentrated nitric acid. (C) Electrochemical reduction of ND on the NPG surface utilizing a single scan and subsequent filling of the void spaces with MPA. (D) Preparation of a MPA SAM on NPG substrate by immersion over night at 4 °C. (E) After adsorption of FDH on the two modified electrodes the enzyme was crosslinked using CMC (sizes not to scale). Panels A–E were adopted from Ref. [142] with permission of Wiley. (For interpretation of the references to colour in this figure legend, the reader is referred to the Web version of this article.)

respect to the same EFC operated as self-powered biosensor.

#### 4. L-lactate detection

Recently, clinical diagnostics focused also on lactate as biomarker to assess patients' health conditions and actuate a continuous and remote surveillance for sport medicine and food industry [148–150]. The latter had a critical role in the last few years in the development of emerging wearable or minimally invasive technologies ranging from tattoo or smart watches to wrist bands or smart gloves, till microneedles and smart packaging [151–153]. However, the lactate physiological level in blood is within 0.5–15 mM rising to 25 mM under intense workout conditions [154]. This has a key role in the anaerobic metabolism. When there is not enough energy supply from the aerobic pathway, there is an increase of lactate concentration due to anaerobic metabolism activation [155]. The accumulation of lactate could result in pathologic state like lactic acidosis, without adequate clearance by liver and kidney. In healthy humans, lactate levels are strictly controlled by lactate homeostasis. The production of lactate is directly related with the increasing of  $H^+$  within the cell with the contemporary regeneration of bicarbonate to neutralize the protons and prevent the loss of bicarbonate [156]. This allows to keep an internal pH of approximately 7.2–7.4. There are two classes of diseases causing lactic acidosis: the first related with decreased tissue oxygenation like shock, left ventricular failure, sepsis and poisoning with carbon monoxide and cyanide; and the second ones related to the administration of specific drugs responsible for renal and hepatic system failure, diabetes and malignancy or inborn error metabolism [157].

Lactate biosensors are usually enclosing two families of enzymes, notably lactate oxidases and dehydrogenases. L-lactate oxidase is a globular flavoprotein that can be extracted from several bacterial sources like *Pediococcus*, *Aerococcus viridans*, and *Mycobacterium segmantis* [158–160]. The enzyme contains flavin mononucleotide catalysing the oxidation of L-lactate to pyruvate with the contemporary reduction of  $O_2$  to  $H_2O_2$ . Since  $O_2$  is naturally working as electron acceptor, both  $O_2$  and the related product  $H_2O_2$  can be electrochemically monitored to obtain an amperometric output that is proportional to L-lactate concentration [161].

Although this represents the most viable approach, there are several concerns about the selectivity and reproducibility of the results mainly due to the required high overpotential needed to oxidise/reduce  $H_2O_2$  and the fluctuation of  $O_2$  in the solution, not considering its limited availability while working in bodily fluids (0.22 mM), which would

hinder the sensing reaction. Dehydrogenases could be potentially a solution considering their  $O_2$  insensitivity [162]. LDH is a tetrameric protein ubiquitously present in animals, plants, and prokaryotes. It has important medical significance as it is present throughout the tissues, such as blood cells and heart muscle. It is released during tissue damage, so it basically acts as a marker of common injuries and disease. L-LDH and D-LDH (EC 1.1.1.27 and EC 1.1.1.28, respectively) catalyse the oxidation of lactate to pyruvate and *vice versa* in the presence of  $NAD(P)^+/NAD(P)H$  and represent a good candidate for the development of lactate biosensors without any  $O_2$  sensitivity.  $NAD(P)^+$  works as diffusing electron acceptor, hence the electrode surface should be modified with a catalyst specifically oxidising  $NAD(P)H$  in order to realise a 2nd generation biosensor based on mediated electron transfer [163,164].

In Table 3, the analytical parameters of few lactate biosensors have been reviewed. Most of the electrode platforms are using LOx in combination with HRP or a catalyst like Prussian Blue (PB) able to reduce  $H_2O_2$ . There are also few examples where  $H_2O_2$  is oxidised like platinum electrodes or modified carbon electrodes. In both cases, it was possible to observe narrow linear ranges that are unsuitable to monitor lactate sweat levels that achieve 20 mM during sport activity. However, lactate production is monitored also at level of cell cultures or industrial fermentation processes where concentrations fall within the dynamic ranges reported in Table 3 [165–175]. Depending on application, several lactate biosensors have been developed as laboratory stand, portable, or hand-held device, and commercialised by several companies. Nova biomedical and Axon Lab developed a biosensor able to monitor lactate in a small sample of blood, hence not providing continuous monitoring. In 2022, Abbott Laboratories developed a 'bio-wearable' platform able to monitor glucose, lactate, ketones and alcohol based on CGM technology. Alternatively, Innovative Sensor Technology (IST) released a multi-parametric sensor based on a small flow cell (1  $\mu$ L) able to monitor glucose, lactate, glutamine and glutamate simultaneously. For instance, Pinnacle Technologies Inc. commercialises a lactate biosensor able to monitor real-time changes in rodents' brain. This type of biosensor is based on most of the previously reviewed platforms encompassing a platinum-iridium electrode, where platinum act as catalyst for  $H_2O_2$  oxidation, further modified with LOx as specific bio-receptor immobilised onto a selective membrane (preventing uneven electrochemical interferences) and bovine serum albumin to prevent aspecific protein adsorption phenomena. The proposed platform exhibits a linear range up to 2 mM and can provide continuous monitoring of brain lactate concentration changes for more than 96 h. Recently,

**Table 3**

Analytical figures of merit for reviewed lactate biosensors. Abbreviations: lactate oxidase (LOx), copper based molecular organic framework (Cu-MOF), platinum electrodeposition (PtE), chitosan (Chit), screen-printed carbon electrode (SPCE), gold nanoparticles (AuNPs), carbon nanotubes (CNTs), reduced graphene oxide (rGO), graphite (G), Poly(3,4-ethylenedioxythiophene) (PEDOT), Prussian Blue (PB), platinum electrode (Pt), multi-walled carbon nanotubes (MWCNTs), methylene blue (MB), gold microparticles (AuMPs), laser-irradiated graphene (LIG), graphene nanoribbons (GNR), 4-aminobenzoic acid (BzA), glassy carbon electrode (GCE), platinum nanoparticles (PtNP), electrochemically reduced graphene oxide (ERGO), poly(allylamine hydrochloride) (PAH), screen-printed electrode (SPE), polyurethane (PU), nanoporous gold (NPG), carbon fibre microelectrodes (CFM), polyaniline (PANI).

| Electrode Platform                  | Linear Range/mM | Sensitivity                     | Limit of Detection/ $\mu$ M | Stability                                      | Ref   |
|-------------------------------------|-----------------|---------------------------------|-----------------------------|------------------------------------------------|-------|
| LOx-Cu-MOF/Chit/PtE/SPCE            | 0.00075–1       | 14.65 $\mu$ A $M^{-1}$          | 0.75                        | 50 days                                        | [165] |
|                                     | 4–50            | 0.207 $\mu$ A $M^{-1}$          | /                           |                                                |       |
| LOx/AuNPs/CNTs/rGO/Pt               | 0.05–100        | 35.3 $\mu$ A $mM^{-1} cm^{-2}$  | 2.3                         | 1 month                                        | [166] |
| L-LDH/AuNP/ERGO/PAH/SPE             | 0.5–3           | 1.08 $\mu$ A $mM^{-1} cm^{-2}$  | 1                           | 75% of initial output after 7 weeks            | [167] |
|                                     | 4–16            | 0.28 $\mu$ A $mM^{-1} cm^{-2}$  | /                           |                                                |       |
| LOx/PB/PEDOT/LIG                    | <18             | 2.23 $\mu$ A $mM^{-1}$          | /                           | /                                              | [168] |
| LOx/BzA/GNR/GCE                     | 0.035–28        | 5.5 $\mu$ A $mM^{-1}$           | 11                          | 30 days                                        | [169] |
| LOx/PB-RGO-PU/G                     | <10             | 3.58 $\mu$ A $mM^{-1}$          | 400                         | /                                              | [170] |
| LOx/PtNP-NPG/CFM                    | <1              | 0.75 nA $mM^{-1}$               | 13                          | 95% of initial output after 5 days             | [171] |
| LOx/Chit/Pt/LSG                     | 0.2–3           | 35.8 $\mu$ A $mM^{-1} cm^{-2}$  | 110                         | /                                              | [172] |
| LOx/Pedot/SPCE                      | 0.25–1          | 43.42 $\mu$ A $mM^{-1} cm^{-2}$ | 83                          | 30 days                                        | [173] |
|                                     | 1–40            | 0.32 $\mu$ A $mM^{-1} cm^{-2}$  | /                           |                                                |       |
| LOx/SPCE                            | <1.5            | 21.8 $\mu$ A $mM^{-1} cm^{-2}$  | /                           | /                                              | [174] |
| LOx/Pt/PANI/MXene                   | 0.005–5         | 0.62 $\mu$ A $mM^{-1}$          | 5                           | 30 days                                        | [175] |
| LOx/MB/MWCNTs-AuMPs/Au microneedles | 0.01–0.2        | 1473 $\mu$ A $mM^{-1} cm^{-2}$  | 2.4                         | Retained 90% of initial response up to 30 days | [180] |

Gaston Crespo and Maria Cuartero funded *IDRO BV* with the contribution of European Institute of Innovation and Technology (EIT), commercializing their recent platform for lactate monitoring. This platform was developed after a perspective on the impact of lactate monitoring on sports physiology [176]. *IDRO*'s patch is developed as a flexible and wearable biosensor enabling real-time data and boosting athletes' performance.

Besides the detection of lactate in food and some bodily fluids, more recently, lactate has been widely investigated for the development of many minimally to non-invasive biosensors based on microneedles or tattoos technology [177–179]. In this regard, Wang and his co-workers developed a flexible printed temporary-transfer tattoo reporting a linear range up to 20 mM. This kind of technology allowed to achieve a real monitoring of lactate during prolonged exercise reflecting the variation of sweat production correlated with lactate profile, as shown in Fig. 7. This electrochemical platform led to the development of several platforms for different analytes useful for the remote medical control not only during sport activities but also for other military and biomedical applications [151].

More recently, the first 2nd generation microneedle-based biosensor to detect lactate in the interstitial fluid was developed. The latter being in communication with the peripheral blood system contains analytes in a concentration that could be easily correlated with the ones in blood. The authors electrodeposited gold microparticles with carbon nanotubes, followed by methylene blue electropolymerisation. The proposed platform exhibited a LOD of 3  $\mu\text{M}$ , definitely below the ones previously reported and a sensitivity of  $178.4 \mu\text{A cm}^{-2} \text{mM}^{-1}$  [180]. This platform has been coupled with a glucose biosensor based on FAD-dependent GDH and used in a simulated model to reproduce the upper layer of skin based on a hydrogel system crossed by a microfluidic system, hence reproducing the exchange between the peripheral blood system and interstitial fluid [181,182].

### 5. Enzyme-based amperometric biosensors: technological and marketing challenges

As reported in the previous sections, the technological development of enzyme-based amperometric biosensors is evolving towards the on-line and *in situ* monitoring. Nowadays, biosensors are not only conceived depending on the analytes and analytical figures of merit, but they are

encapsulated in polymers integrated in materials and objects commonly used during day life [183–185]. A particular example is the development of glucose biosensors towards the management and treatment of diabetes considering some intravascular and subcutaneous applications. In this case (implanted sensors), there several technical issues related with the biofouling of the electrode surface, as well as potential tissue damage and biocompatibility of all materials employed to modify the electrode surface [186]. This is re-routing the interest of biosensing community towards minimally invasive (microneedles and tattoos) and hand-held biosensors.

There is great engagement on this side also for clinical, environmental, and pharmaceutical applications. What is limiting the technological advancement of biosensors? The key issue is the scalability to produce biosensors that contains several biological elements that are particularly expensive. On the other hand, the limiting aspect is the bioproduction process that does not exhibit the same kinetics of biosensor production. This is important to ensure continuous supply for the production. In this regard, the scientific community is trying to develop biosensing platforms that could be reused multiple times exhibiting a great operational and storage stability over months [187, 188]. Another issue is related to the immobilisation of the bioprobe. Recently, most of the preparation protocols endowed the electropolymerisation or electrodeposition process enabling a precise and reproducible immobilisation, which plays a pivotal role in the analytical figures of merit for the biosensors developed [189].

This is also interesting for the development of micro- and ultra-microelectrodes (UMEs) that are currently used for the development of biosensors [190].

An important issue/challenge, towards the employment of enzyme-based amperometric biosensors as Point-of-Care (PoC) devices, is the robustness of the electrode platform either in terms of calibration or analysis of real samples [191]. The reliability of enzyme-based biosensors depends mostly on the calibration procedure that should account for the operating conditions. For instance, considering glucose biosensors, for many years the basis for calibration was the assumption that blood glucose concentration was like the one in subcutaneous interstitial fluid. This is not true. In addition, the ratio of blood/tissue glucose is not constant but depends on several factors related to the physiology of glucose and insulin. In this specific case, the reliability of the calibration is low. For other types of substrates, the relationship between blood levels and peripheral bodily fluids might be considerably more complicated. For real sample analysis, enzyme-based electrodes are usually undergoing a progressive denaturation of the enzyme layer and surface fouling. To prevent enzyme denaturation, it is possible to control the rate-limiting step through porous electrode structures or diffusion-limiting membranes that are reducing signal variations even in the case of substantial loss of enzymatic activity. The membrane also serves to protect the active electrode surface from direct contact with the sample and hence minimizes fouling. Antifouling coatings onto electrodes (without enzyme) may also result in robust electrochemical biosensors. Moreover, hydrogel coatings were reported to reduce ionic and bulky interferences.

The development of PoC devices for electrochemical biosensing is one of the main challenges in this field. Currently, much effort has been exerted in the miniaturization of electrochemical transducers and readout instruments to achieve real-time, PoC and easy-to-use analysis in the field [192]. With respect to biosensor marketing, only PoC devices gained reasonable attention mostly because of their portability, low-cost (depending on the bioreceptor and analytical target), fast response and nowadays also their eco-impact [193]. This means that most of the disposable part of the biosensors like polymers to modify the electrodes as well nanomaterials or supports need to be recyclable. The focus on the ecological impact of PoC devices has been particularly raised during the COVID-19 pandemic and it clearly needs to be addressed carrying on research on the average lifetime of materials and considering if such recycling process is sustainable both from the economic and

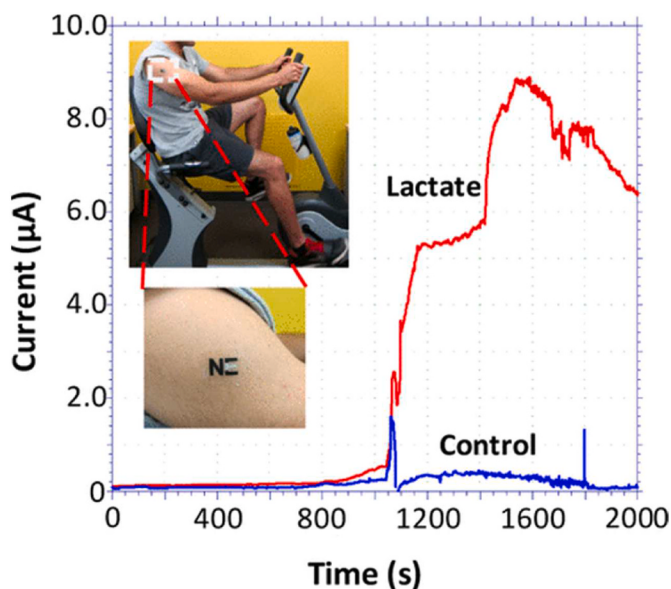


Fig. 7. Lactate profile obtained using tattoo-based biosensor during aerobic exercise. Figure reproduced from Ref. [151] with permission of American Chemical Society (ACS).

environmental point of view.

Besides the eco-impact, especially glucose and lactate monitoring are experiencing a shifting from traditional blood self-testing platforms towards wearable technologies, moving from PoC or lab-on-chip devices to lab-on-skin devices. Although electronic textile or e-textile are still at the early stage, such revolutionary epidermal sensing technology will offer the possibility of a continuous monitoring of health and disease status. Many researchers are currently working on the integration through microfluidic apparatus or even directly screen-printing or stencil-printing the electrodes on clothes. Except CGM (as previously reported for lactate), there are no commercial sensing platforms as worn technologies perhaps due to limited sensor stability (related biofouling and receptor degradation) and the limited understanding of the correlation between sweat and blood analyte concentrations. The correlation between epidermal electrochemical sensors and blood biomarkers levels will require large-scale clinical trials and broad validation efforts [194]. Only few examples of microneedles-based platforms are commercialised by start-up companies like *San Diego-based Biolinq*, who reported its first successful human trial with results showing promising correlation and no lag time compared to the venous blood (June 2020). For instance, *Caura (UK)* is focused on monitoring simultaneously glucose and heart rate, while *Melbourne-based Nutromics (Australia)* is working on microneedles for personalised nutrition. Besides continuous biomarkers monitoring, the big challenge for microneedles is about a reproducible skin penetration especially regarding the elasticity of the skin, which results in a counteracting force to the penetration and thus, to a partial or incomplete piercing. Moreover, one should also consider the skin thickness variation depending on the age, gender, body mass index, and ethnicity of the wearer. In addition, researchers need to account for biofouling effects (decreasing sensor reproducibility and lifetime) and the evaluation of the analytical performance to fine tune eventually connected drug-releasing units, operating as a sense-act-treat device [195,196].

The market of enzyme-based amperometric biosensors is moving towards achieving zero eco-impact of biosensing platform, cost-effective platform and reliable biosensors that could be used in several fields going from precision and remote medicine till smart food packaging. For instance, global biosensor market size was valued at USD 27.5 billion in 2021 and it is expected to expand annually by 8% between 2022 and 2030. However, the biosensors market will reach USD 49.6 billion by

2030 on a worldwide base, as shown in Fig. 8 [197]. The increasing preference for non-invasive biosensors, research collaboration and agreements between diverse manufacturers raised the popularity of self-testing/medicating devices, consolidating biosensors market. Furthermore, in November 2019, scientists from Brazil and the U.S. developed a biosensor that is a glasses-based device that can give diabetics a less invasive test by measuring blood glucose levels through tears. From a technical point of view, the market is dominated by electrochemical based platforms that captured the largest revenue share approximately of 71.1% in 2021 (Fig. 8), probably to the ease of biochemical measurement protocols, low detection limits, wide linear response range, excellent stability, and repeatability are all advantages of electrochemical biosensors. They also exhibit robustness, compatibility with new microfabrication technologies, ease of operation, low cost, disposability, independence from sample turbidity, and low power.

## 6. Conclusions and future perspectives

After marking 60 years since the development of the first biosensing platform, the enzyme-based biosensing technology has moved a big step forward considering the technological issues encountered during these six decades. Nowadays, most of the enzyme-based biosensors are employed for the diabetes management and treatment (when connected with insulin pumps) and online target analysis. In addition, many enzymatic biosensors have been also used for pesticides and toxins detection. In this review, we have considered most of the enzymes widely used for biosensors development focusing on glucose, fructose, and lactate detection. In this regard, the electron transfer process has been deeply discussed as well as their importance from the analytical point of view. Afterwards, the analytical figures of merit of several enzyme-based amperometric biosensors were schematically summarised to provide a complete view of the state-of-the-art.

As future perspective, the enzymatic biosensing community will move along two main routes: (i) the development of wearable devices that could potentially work as actuators and (ii) the possibility to overcome the limit of detection limit, usually within the micromolar range. The first route is currently under investigation. Knowledge about the composition of bodily fluids is crucial for the development of wearable devices. Thanks to real-time biomarkers monitoring, information on wellness and health, and enhancement of the management of

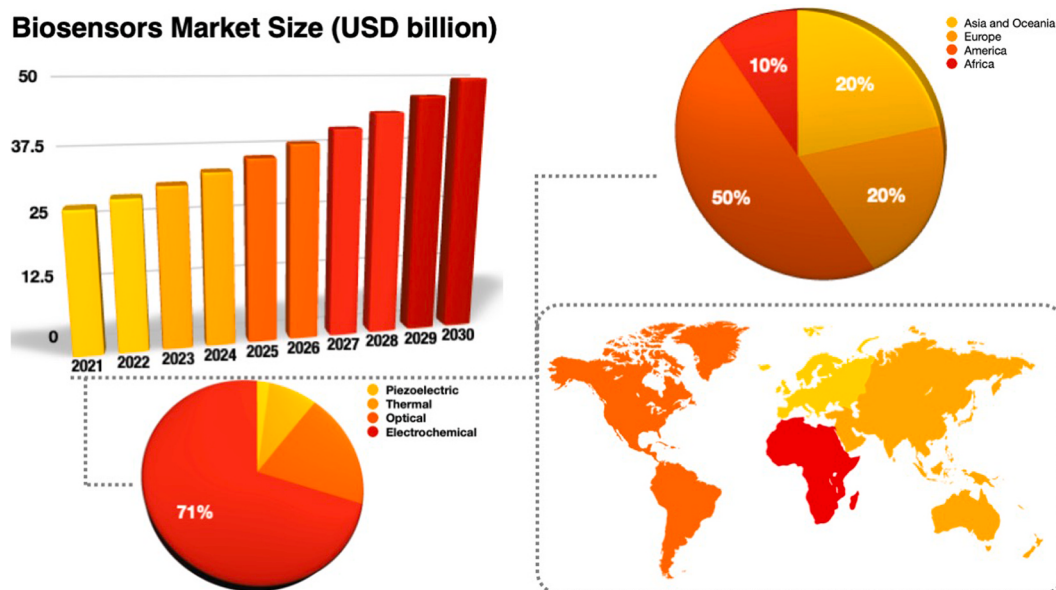


Fig. 8. Projection of Biosensors Market Size 2021–2030 with a focus on the distribution by transduction techniques and region for 2021. Data obtained from Ref. [197].

chronic diseases are provided, alerting the user or medical professionals of abnormal or unforeseen situations. To achieve wearable sensing, the (bio)sensing elements must be in direct contact with biofluids, hence they need to comply with body shape (comfortable wearing) by using advanced smart materials that are flexible and stretchable [198]. Although a first report on this technology was published [199], there are plenty of potential developments based on the bio(triggered) drug release, stretchable and flexible platform. The bio(triggered) release could be achieved integrating two-electrode systems encompassing a sensing/actuating electrode and the actuated electrode being often used for drug release or to activate a second sensing process [200]. The former can be activated by O<sub>2</sub> reduction to H<sub>2</sub>O biocatalyzed by multicopper oxidases (MCOs) that are 'locally' increasing the pH (stimuli) [201]. Alternatively, reaction products like H<sub>2</sub>O<sub>2</sub> can activate the release from hydrogel layers. In this regard, nanozymes can be easily integrated to replace enzymes and increase the robustness of such platforms. Nanozymes are nanomaterials owning enzyme-like properties, which catalyse the conversion of substrate to product (catalytic activity). In the last decade, 'naked' gold nanoparticles (NPs), functionalized AuNPs, Fe<sub>3</sub>O<sub>4</sub> NPs have reported oxidase- or peroxidase-like activity that can be easily employed for the development of (bio) sensing and sense-act-treat devices [202]. They certainly exhibit increased robustness compared to enzymes; however, they lack selectivity as major drawback, additionally, they are unable to reproduce all the reactions catalysed by enzymes. This could be easily implemented exploiting Boolean Logic Gates and "Chimeric" enzymes [203–207]. Recent technological advancements in soft actuators, flexible bioelectronics, and wireless data acquisition systems have enabled the development of ergonomic, lightweight, and low-cost wearable devices. For instance, wearable (bio)sensing gloves merged with sensory feedback devices could enhance hand sensations for healthcare, robotics and virtual reality applications [208]. About the second route, recently Bollella and his co-workers proposed the combination of self-powered biosensor (or enzymatic-fuel cell) with a bipolar junction transistor in extended base configuration [209,210]. In this approach, being the base current controlled, there is the possibility to minimise the signal noise, increase the signal-to-noise ratio and amplify the current output to achieve sub-nanomolar if not lower LOD, which has so far never been achieved with wide-field single molecule electrochemistry approach. The latter can pave the way for unforeseen development for PoC and Point-of-Use devices. Achieving single-molecule diagnostics with electrochemical transduction (considering enzymatic reaction) will have a great impact on PoC and Point-of-Use devices broadening the range of applications where early detection plays a key role.

#### Authors' contributions

All authors have thoroughly contributed to conceive and write this article. The final version was approved by all authors.

#### Declaration of competing interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

#### Data availability

No data was used for the research described in the article.

#### Acknowledgements

PB acknowledges the following funding: Biosensori analitici usa-getta a base di transistori organici auto-alimentati per la rivelazione di biomarcatori proteomici alla singola molecola per la diagnostica decentrata dell'HIV (6CDD3786); Research for Innovation

REFIN—Regione Puglia POR PUGLIA FESR-FSE 2014/2020.

#### References

- [1] G. Davis, Electrochemical techniques for the development of amperometric biosensors, *Biosensors* 1 (1985) 161–178.
- [2] I. Willner, E. Katz, B. Willner, Electrical contact of redox enzyme layers associated with electrodes: routes to amperometric biosensors, *Electroanalysis* 9 (1997) 965–977.
- [3] K. Habermüller, M. Mosbach, W. Schuhmann, Electron-transfer mechanisms in amperometric biosensors, *Fresenius' J. Anal. Chem.* 366 (2000) 560–568.
- [4] P. Bollella, L. Gorton, Enzyme based amperometric biosensors, *Curr. Opin. Electrochem.* 10 (2018) 157–173.
- [5] L.C. Clark Jr., C. Lyons, Electrode systems for continuous monitoring in cardiovascular surgery, *Ann. N. Y. Acad. Sci.* 102 (1962) 29–45.
- [6] J. Wang, Electrochemical glucose biosensors, *Chem. Rev.* 108 (2008) 814–825.
- [7] J. Wang, Glucose biosensors: 40 years of advances and challenges, *Electroanal. Int. J. Devoted Fundam. Pract. Asp. Electroanal.* 13 (2001) 983–988.
- [8] A.A. Karyakin, Glucose biosensors for clinical and personal use, *Electrochem. Commun.* 125 (2021), 106973.
- [9] A.P. Turner, Biosensors—sense and sensitivity, *Science* 290 (2000) 1315–1317.
- [10] J.D. Newman, A.P. Turner, Home blood glucose biosensors: a commercial perspective, *Biosens. Bioelectron.* 20 (2005) 2435–2453.
- [11] A.E. Cass, G. Davis, G.D. Francis, H.A.O. Hill, W.J. Aston, I.J. Higgins, E. V. Plotkin, L.D. Scott, A.P. Turner, Ferrocene-mediated enzyme electrode for amperometric determination of glucose, *Anal. Chem.* 56 (1984) 667–671.
- [12] A. Heller, Electrical connection of enzyme redox centers to electrodes, *J. Phys. Chem.* 96 (1992) 3579–3587.
- [13] A. Heller, Electrical wiring of redox enzymes, *Acc. Chem. Res.* 23 (1990) 128–134.
- [14] A. Heller, B. Feldman, Electrochemical glucose sensors and their applications in diabetes management, *Chem. Rev.* 108 (2008) 2482–2505.
- [15] B. Persson, L. Gorton, A comparative study of some 3, 7-diaminophenoxazine derivatives and related compounds for electrocatalytic oxidation of NADH, *J. Electroanal. Chem. Interfacial Electrochem.* 292 (1990) 115–138.
- [16] M. Persson, M.-O. Månsson, L. Bülow, K. Mosbach, Continuous regeneration of NAD (H) covalently bound to a cysteine genetically engineered into glucose dehydrogenase, *Bio/Technology* 9 (1991) 280–284.
- [17] G. Bremle, B. Persson, L. Gorton, An amperometric glucose electrode based on carbon paste, chemically modified with glucose dehydrogenase, nicotinamide adenine dinucleotide, and a phenoxazine mediator, coated with a poly (ester sulfonic acid) cation exchanger, *Electroanalysis* 3 (1991) 77–86.
- [18] F.A. Armstrong, H.A.O. Hill, N.J. Walton, Reactions of electron-transfer proteins at electrodes, *Q. Rev. Biophys.* 18 (1985) 261–322.
- [19] M.J. Eddowes, H.A.O. Hill, Investigation of electron-transfer reactions of proteins by electrochemical methods, *Biosci. Rep.* 1 (1981) 521–532.
- [20] L.-H. Guo, H.A.O. Hill, Direct electrochemistry of proteins and enzymes, *Adv. Inorg. Chem.* 36 (1991) 341–375.
- [21] G.S. Wilson, Native Glucose Oxidase Does Not Undergo Direct Electron Transfer, 2016.
- [22] P.N. Bartlett, F.A. Al-Lolage, There is no evidence to support literature claims of direct electron transfer (DET) for native glucose oxidase (GOx) at carbon nanotubes or graphene, *J. Electroanal. Chem.* 819 (2018) 26–37.
- [23] M.J. Therien, J. Chang, A.L. Raphael, B.E. Bowler, H.B. Gray, Long-range electron transfer in metalloproteins, in: *Long-Range Electron Transf. Biol.*, Springer, 1991, pp. 109–129.
- [24] J.R. Winkler, H.B. Gray, Long-range electron tunneling, *J. Am. Chem. Soc.* 136 (2014) 2930–2939.
- [25] M. Grattieri, S.D. Minter, Self-powered biosensors, *ACS Sens.* 3 (2018) 44–53.
- [26] R.D. Milton, S.D. Minter, Direct enzymatic bioelectrocatalysis: differentiating between myth and reality, *J. R. Soc. Interface* 14 (2017), 20170253.
- [27] P. Bollella, E. Katz, Enzyme-based biosensors: tackling electron transfer issues, *Sensors* 20 (2020) 3517.
- [28] C. Spahn, S.D. Minter, Enzyme immobilization in biotechnology, *Recent Pat. Eng.* 2 (2008) 195–200.
- [29] A.K. Sarma, P. Vatsyayan, P. Goswami, S.D. Minter, Recent advances in material science for developing enzyme electrodes, *Biosens. Bioelectron.* 24 (2009) 2313–2322.
- [30] E.-H. Yoo, S.-Y. Lee, Glucose biosensors: an overview of use in clinical practice, *Sensors* 10 (2010) 4558–4576.
- [31] H. Teymourian, A. Barfidokht, J. Wang, Electrochemical glucose sensors in diabetes management: an updated review (2010–2020), *Chem. Soc. Rev.* 49 (2020) 7671–7709.
- [32] S.B. Bankar, M.V. Bule, R.S. Singhal, L. Ananthanarayan, Glucose oxidase—an overview, *Biotechnol. Adv.* 27 (2009) 489–501.
- [33] S. Abdellaoui, R.D. Milton, T. Quah, S.D. Minter, NAD-dependent dehydrogenase bioelectrocatalysis: the ability of a naphthoquinone redox polymer to regenerate NAD, *Chem. Commun.* 52 (2016) 1147–1150, <https://doi.org/10.1039/C5CC09161F>.
- [34] F. Lisdat, PQQ-GDH—Structure, function and application in bioelectrochemistry, *Bioelectrochemistry* 134 (2020), 107496.
- [35] E.J. D'costa, I.J. Higgins, A.P.F. Turner, Quinoprotein glucose dehydrogenase and its application in an amperometric glucose sensor, *Biosensors* 2 (1986) 71–87.

- [36] J.A. Duine, Quinoproteins: enzymes containing the quinonoid cofactor pyrroloquinoline quinone, topaquinone or tryptophan-tryptophan quinone, *Eur. J. Biochem.* 200 (1991) 271–284.
- [37] R.D. Milton, K. Lim, D.P. Hickey, S.D. Minter, Employing FAD-dependent glucose dehydrogenase within a glucose/oxygen enzymatic fuel cell operating in human serum, *Bioelectrochemistry* 106 (2015) 56–63.
- [38] P. Bollella, R. Ludwig, L. Gorton, Cellobiose dehydrogenase: insights on the nanostructuring of electrodes for improved development of biosensors and biofuel cells, *Appl. Mater. Today* 9 (2017) 319–332.
- [39] R. Ludwig, R. Ortiz, C. Schulz, W. Harreither, C. Sygmund, L. Gorton, Cellobiose dehydrogenase modified electrodes: advances by materials science and biochemical engineering, *Anal. Bioanal. Chem.* 405 (2013) 3637–3658.
- [40] R. Ludwig, W. Harreither, F. Tasca, L. Gorton, Cellobiose dehydrogenase: a versatile catalyst for electrochemical applications, *ChemPhysChem* 11 (2010) 2674–2697.
- [41] C.K. Peterbauer, Pyranose dehydrogenases: rare enzymes for electrochemistry and biocatalysis, *Bioelectrochemistry* 132 (2020), 107399.
- [42] R. Wilson, A.P.F. Turner, Glucose oxidase: an ideal enzyme, *Biosens. Bioelectron.* 7 (1992) 165–185.
- [43] J. Raba, H.A. Mottola, Glucose oxidase as an analytical reagent, *Crit. Rev. Anal. Chem.* 25 (1995) 1–42.
- [44] L. Sützl, C.V. Laurent, A.T. Abrera, G. Schütz, R. Ludwig, D. Haltrich, Multiplicity of enzymatic functions in the CAZy AA3 family, *Appl. Microbiol. Biotechnol.* 102 (2018) 2477–2492.
- [45] Y. Wu, S. Hu, Biosensors based on direct electron transfer in redox proteins, *Microchim. Acta* 159 (2007) 1–17.
- [46] M.K. Weibel, H.J. Bright, The glucose oxidase mechanism: interpretation of the pH dependence, *J. Biol. Chem.* 246 (1971) 2734–2744.
- [47] G.G. Guilbault, G.J. Lubrano, An enzyme electrode for the amperometric determination of glucose, *Anal. Chim. Acta* 64 (1973) 439–455.
- [48] A. Prévotau, N. Mano, Oxygen reduction on redox mediators may affect glucose biosensors based on “wired” enzymes, *Electrochim. Acta* 68 (2012) 128–133.
- [49] A. Prévotau, N. Mano, How the reduction of O<sub>2</sub> on enzymes and/or redox mediators affects the calibration curve of “wired” glucose oxidase and glucose dehydrogenase biosensors, *Electrochim. Acta* 112 (2013) 318–326.
- [50] M. Grattieri, M. Tucci, M. Bestetti, S. Trasatti, P. Cristiani, Facilitated electron hopping in nanolayer oxygen-insensitive glucose biosensor for application in a complex matrix, *Chemelectrochem* 3 (2016) 1884–1889.
- [51] O. Smutok, T. Kavetskiy, E. Katz, Recent trends in enzyme engineering aiming to improve bioelectrocatalysis proceeding with direct electron transfer, *Curr. Opin. Electrochem.* (2021), 100856.
- [52] J. Marín-Navarro, N. Roupain, D. Talens-Perales, J. Polaina, Identification and structural analysis of amino acid substitutions that increase the stability and activity of *Aspergillus Niger* glucose oxidase, *PLoS One* 10 (2015), e0144289.
- [53] M.J. Novak, A. Pattammattel, B. Koshmerl, M. Puglia, C. Williams, C.V. Kumar, Stable-on-the-table” enzymes: engineering the enzyme–graphene oxide interface for unprecedented kinetic stability of the biocatalyst, *ACS Catal.* 6 (2016) 339–347.
- [54] E. Tremey, E. Suraniti, O. Courjean, S. Gounel, C. Stines-Chaumeil, F. Louerat, N. Mano, Switching an O<sub>2</sub> sensitive glucose oxidase bioelectrode into an almost insensitive one by cofactor redesign, *Chem. Commun.* 50 (2014) 5912–5914.
- [55] E. Tremey, C. Stines-Chaumeil, S. Gounel, N. Mano, Designing an O<sub>2</sub>-insensitive glucose oxidase for improved electrochemical applications, *Chemelectrochem* 4 (2017) 2520–2526.
- [56] W. Jin, U. Wollenberger, F.W. Scheller, PQQ as redox shuttle for quinoprotein glucose dehydrogenase, *Biol. Chem.* 379 (1998) 1207–1211.
- [57] S. Igarashi, T. Ohtera, H. Yoshida, A.B. Witarto, K. Sode, Construction and characterization of mutant water-soluble PQQ glucose dehydrogenases with altered Km values—site-directed mutagenesis studies on the putative active site, *Biochem. Biophys. Res. Commun.* 264 (1999) 820–824.
- [58] S. Igarashi, K. Sode, Construction and characterization of heterodimeric soluble quinoprotein glucose dehydrogenase, *J. Biochem. Biophys. Methods* 61 (2004) 331–338.
- [59] S. Igarashi, T. Hirokawa, K. Sode, Engineering PQQ glucose dehydrogenase with improved substrate specificity: site-directed mutagenesis studies on the active center of PQQ glucose dehydrogenase, *Biomol. Eng.* 21 (2004) 81–89.
- [60] R. Bennett, E. Blochouse, D. Leech, Effect of individual plasma components on the performance of a glucose enzyme electrode based on redox polymer mediation of a flavin adenine dinucleotide-dependent glucose dehydrogenase, *Electrochim. Acta* 302 (2019) 270–276.
- [61] M.N. Zafar, N. Beden, D. Leech, C. Sygmund, R. Ludwig, L. Gorton, Characterization of different FAD-dependent glucose dehydrogenases for possible use in glucose-based biosensors and biofuel cells, *Anal. Bioanal. Chem.* 402 (2012) 2069–2077.
- [62] M.N. Zafar, X. Wang, C. Sygmund, R. Ludwig, D. Leech, L. Gorton, Electron-transfer studies with a new flavin adenine dinucleotide dependent glucose dehydrogenase and osmium polymers of different redox potentials, *Anal. Chem.* 84 (2012) 334–341.
- [63] C. Anthony, The quinoprotein dehydrogenases for methanol and glucose, *Arch. Biochem. Biophys.* 428 (2004) 2–9.
- [64] C. Tripura, A.R. Podile, Properties of a chimeric glucose dehydrogenase improved by site directed mutagenesis, *J. Biotechnol.* 131 (2007) 197–204.
- [65] A. Koushanpour, M. Gamella, Z. Guo, E. Honarvarfar, A. Poghossian, M. J. Schöning, K. Alexandrov, E. Katz, Ca<sup>2+</sup>-Switchable glucose dehydrogenase associated with electrochemical/electronic interfaces: applications to signal-controlled power production and biomolecular release, *J. Phys. Chem. B* 121 (2017) 11465–11471.
- [66] V. Flexer, F. Durand, S. Tsujimura, N. Mano, Efficient direct electron transfer of PQQ-glucose dehydrogenase on carbon cryogel electrodes at neutral pH, *Anal. Chem.* 83 (2011) 5721–5727.
- [67] D. Ivnitski, P. Atanassov, C. Applett, Direct bioelectrocatalysis of PQQ-dependent glucose dehydrogenase, *Electroanal. Int. J. Devoted Fundam. Pract. Asp. Electroanal.* 19 (2007) 1562–1568.
- [68] T. Bobrowski, E.G. Arribas, R. Ludwig, M.D. Toscano, S. Shleev, W. Schuhmann, Rechargeable, flexible and mediator-free biosupercapacitor based on transparent ITO nanoparticle modified electrodes acting in  $\mu$ M glucose containing buffers, *Biosens. Bioelectron.* 101 (2018) 84–89.
- [69] P. Bollella, I. Lee, D. Blaauw, E. Katz, A microelectronic sensor device powered by a small implantable biofuel cell, *ChemPhysChem* 21 (2020) 120–128.
- [70] S.D. Minter, B.Y. Liaw, M.J. Cooney, Enzyme-based biofuel cells, *Curr. Opin. Biotechnol.* 18 (2007) 228–234.
- [71] S. Calabrese Barton, J. Gallaway, P. Atanassov, Enzymatic biofuel cells for implantable and microscale devices, *Chem. Rev.* 104 (2004) 4867–4886.
- [72] S. Ferri, K. Kojima, K. Sode, Review of Glucose Oxidases and Glucose Dehydrogenases: a Bird’s Eye View of Glucose Sensing Enzymes, SAGE Publications, 2011.
- [73] C. Hou, Q. Lang, A. Liu, Tailoring 1, 4-naphthoquinone with electron-withdrawing group: toward developing redox polymer and FAD-GDH based hydrogel bioanode for efficient electrocatalytic glucose oxidation, *Electrochim. Acta* 211 (2016) 663–670.
- [74] H. Iwasa, A. Hiratsuka, K. Yokoyama, H. Uzawa, K. Orihara, H. Muguruma, Thermophilic *Talaromyces emersonii* Flavin adenine dinucleotide-dependent glucose dehydrogenase bioanode for biosensor and biofuel cell applications, *ACS Omega* 2 (2017) 1660–1665.
- [75] S. Tsujimura, S. Kojima, K. Kano, T. Ikeda, M. Sato, H. Sanada, H. Omura, Novel FAD-dependent glucose dehydrogenase for a dioxygen-insensitive glucose biosensor, *Biosci. Biotechnol. Biochem.* 70 (2006) 654–659.
- [76] H. Muguruma, H. Iwasa, H. Hidaka, A. Hiratsuka, H. Uzawa, Mediatorless direct electron transfer between flavin adenine dinucleotide-dependent glucose dehydrogenase and single-walled carbon nanotubes, *ACS Catal.* 7 (2017) 725–734.
- [77] M. Hatada, N. Loew, Y. Inose-Takahashi, J. Okuda-Shimazaki, W. Tsugawa, A. Mulchandani, K. Sode, Development of a glucose sensor employing quick and easy modification method with mediator for altering electron acceptor preference, *Bioelectrochemistry* 121 (2018) 185–190.
- [78] I. Algov, J. Grushka, R. Zarivach, L. Alfonta, Highly efficient flavin–adenine dinucleotide glucose dehydrogenase fused to a minimal cytochrome c domain, *J. Am. Chem. Soc.* 139 (2017) 17217–17220.
- [79] I. Algov, A. Feiertag, L. Alfonta, Site-specifically wired and oriented glucose dehydrogenase fused to a minimal cytochrome with high glucose sensing sensitivity, *Biosens. Bioelectron.* 180 (2021), 113117.
- [80] L. Gorton, Chemically modified electrodes for the electrocatalytic oxidation of nicotinamide coenzymes, *J. Chem. Soc. Faraday Trans. 1 Phys. Chem. Condens. Phases.* 82 (1986) 1245–1258.
- [81] L. Gorton, E. Domínguez, Electrocatalytic oxidation of NAD(P)H at mediator-modified electrodes, *Rev. Mol. Biotechnol.* 82 (2002) 371–392.
- [82] A.T. Abrera, H. Chang, D. Kracher, R. Ludwig, D. Haltrich, Characterization of pyranose oxidase variants for bioelectrocatalytic applications, *Biochim. Biophys. Acta BBA-Proteins Proteomics* 1868 (2020), 140335.
- [83] P. Rafighi, P. Bollella, G. Pankratova, C.K. Peterbauer, P.Ó. Conghaile, D. Leech, B. Haghighi, L. Gorton, Substrate preference pattern of *Agaricus meleagris* pyranose dehydrogenase evaluated through bioelectrochemical flow injection amperometry, *Chemelectrochem* 6 (2018) 801–809.
- [84] P. Bollella, C. Schulz, G. Favero, F. Mazzei, R. Ludwig, L. Gorton, R. Antiochia, Green synthesis and characterization of gold and silver nanoparticles and their application for development of a third generation lactose biosensor, *Electroanalysis* 29 (2017) 77–86.
- [85] P. Bollella, F. Mazzei, G. Favero, G. Fusco, R. Ludwig, L. Gorton, R. Antiochia, Improved DET communication between cellobiose dehydrogenase and a gold electrode modified with a rigid self-assembled monolayer and green metal nanoparticles: the role of an ordered nanostructuring, *Biosens. Bioelectron.* 88 (2017) 196–203.
- [86] R. Ortiz, R. Ludwig, L. Gorton, Highly efficient membraneless glucose bioanode based on *Corynebacterium thermophilus* cellobiose dehydrogenase on aryl diazonium-activated single-walled carbon nanotubes, *Chemelectrochem* 1 (2014) 1948–1956.
- [87] B. Alp, S. Mutlu, M. Mutlu, Glow-discharge-treated cellulose acetate (CA) membrane for a high linearity single-layer glucose electrode in the food industry, *Food Res. Int.* 33 (2000) 107–112.
- [88] P. Vadgama, Diffusion limited enzyme electrodes, in: *Anal. Uses Immobil. Biol. Compd. Detect. Med. Ind. Uses*, Springer, 1988, pp. 359–377.
- [89] A. Ramanavicius, A.I. Rekertaitė, R. Valiūnas, A. Valiūnienė, Single-step procedure for the modification of graphite electrode by composite layer based on polypyrrole, Prussian blue and glucose oxidase, *Sensor. Actuator. B Chem.* 240 (2017) 220–223.
- [90] A.I. Rekertaitė, A. Valiūnienė, P. Virbickas, A. Ramanavicius, Physicochemical characteristics of polypyrrole/(glucose oxidase)/(prussian blue)-based biosensor modified with Ni- and Co-hexacyanoferrates, *Electroanalysis* 31 (2019) 50–57.
- [91] I.L. de Mattos, L.V. Lukachova, L. Gorton, T. Laurell, A.A. Karyakin, Evaluation of glucose biosensors based on Prussian Blue and lyophilised, crystalline and cross-linked glucose oxidases (CLEC®), *Talanta* 54 (2001) 963–974.

- [92] J. Yoon, S.N. Lee, M.K. Shin, H.-W. Kim, H.K. Choi, T. Lee, J.-W. Choi, Flexible electrochemical glucose biosensor based on GOx/gold/MoS<sub>2</sub>/gold nanofilm on the polymer electrode, *Biosens. Bioelectron.* 140 (2019), 111343.
- [93] N. German, A. Ramanavicius, A. Ramanaviciene, Amperometric glucose biosensor based on electrochemically deposited gold nanoparticles covered by polypyrrole, *Electroanalysis* 29 (2017) 1267–1277.
- [94] F. Wang, W. Gong, L. Wang, Z. Chen, Enhanced amperometric response of a glucose oxidase and horseradish peroxidase based bienzyme glucose biosensor modified with a film of polymerized toluidine blue containing reduced graphene oxide, *Microchim. Acta* 182 (2015) 1949–1956.
- [95] A. Márquez, C. Jiménez-Jorquera, C. Domínguez, X. Muñoz-Berbel, Electrodepositable alginate membranes for enzymatic sensors: an amperometric glucose biosensor for whole blood analysis, *Biosens. Bioelectron.* 97 (2017) 136–142.
- [96] D.V. Estrada-Osorio, R.A. Escalona-Villalpando, A. Gutiérrez, L.G. Arriaga, J. Ledesma-García, Poly-L-lysine-modified with ferrocene to obtain a redox polymer for mediated glucose biosensor application, *Bioelectrochemistry* 146 (2022), 108147.
- [97] F.M. Mazar, M. Alijanianzadeh, A. Molaeirad, P. Heydari, Development of novel glucose oxidase immobilization on graphene/gold nanoparticles/poly neutral red modified electrode, *Process Biochem.* 56 (2017) 71–80.
- [98] K. Jayakumar, R. Bennett, D. Leech, Electrochemical glucose biosensor based on an osmium redox polymer and glucose oxidase grafted to carbon nanotubes: a design-of-experiments optimisation of current density and stability, *Electrochim. Acta* 371 (2021), 137845.
- [99] A. Popov, R. Aukstakojyte, J. Gaidukevic, V. Lisyte, A. Kausaite-Minkstiniene, J. Barkauskas, A. Ramanaviciene, Reduced graphene oxide and polyaniline nanofibers nanocomposite for the development of an amperometric glucose biosensor, *Sensors* 21 (2021) 948.
- [100] A. Kausaite-Minkstiniene, L. Glumbokaite, A. Ramanaviciene, A. Ramanavicius, Reagent-less amperometric glucose biosensor based on nanobiocomposite consisting of poly (1, 10-phenanthroline-5, 6-dione), poly (pyrrole-2-carboxylic acid), gold nanoparticles and glucose oxidase, *Microchem. J.* 154 (2020), 104665.
- [101] L.F. Ang, L.Y. Por, M.F. Yam, Development of an amperometric-based glucose biosensor to measure the glucose content of fruit, *PLoS One* 10 (2015), e0111859.
- [102] F. Poletti, L. Favaretto, A. Kovtun, E. Treossi, F. Corticelli, M. Gazzano, V. Palermo, C. Zanardi, M. Melucci, Electrochemical sensing of glucose by chitosan modified graphene oxide, *J. Phys. Mater.* 3 (2020), 014011.
- [103] S. Cinti, R. Cusenza, D. Moscone, F. Arduini, Paper-based synthesis of Prussian Blue Nanoparticles for the development of whole blood glucose electrochemical biosensor, *Talanta* 187 (2018) 59–64.
- [104] Y. Zhao, Q. Zhai, D. Dong, T. An, S. Gong, Q. Shi, W. Cheng, Highly stretchable and strain-insensitive fiber-based wearable electrochemical biosensor to monitor glucose in the sweat, *Anal. Chem.* 91 (2019) 6569–6576.
- [105] L. Zhao, Z. Wen, F. Jiang, Z. Zheng, S. Lu, Silk/polyols/GOD microneedle based electrochemical biosensor for continuous glucose monitoring, *RSC Adv.* 10 (2020) 6163–6171.
- [106] J. Ma, Y. Du, Y. Jiang, L. Shen, H. Ma, F. Lv, Z. Cui, Y. Pan, L. Shi, N. Zhu, Wearable healthcare smart electrochemical biosensors based on co-assembled prussian blue—graphene film for glucose sensing, *Microchim. Acta* 189 (2022) 1–9.
- [107] M. Parrilla, U. Detamornrat, J. Domínguez-Robles, R.F. Donnelly, K. De Wael, Wearable hollow microneedle sensing patches for the transdermal electrochemical monitoring of glucose, *Talanta* 249 (2022), 123695.
- [108] M. Artigues, J. Abellà, S. Colominas, Analytical parameters of an amperometric glucose biosensor for fast analysis in food samples, *Sensors* 17 (2017) 2620.
- [109] N.C. Sekar, S.A.M. Shaegh, S.H. Ng, L. Ge, S.N. Tan, A paper-based amperometric glucose biosensor developed with Prussian Blue-modified screen-printed electrodes, *Sensor. Actuator. B Chem.* 204 (2014) 414–420.
- [110] P. Krzyczmonik, E. Socha, S. Skrzypek, Electrochemical detection of glucose in beverage samples using poly (3, 4-ethylenedioxythiophene)-modified electrodes with immobilized glucose oxidase, *Electrocatalysis* 9 (2018) 380–387.
- [111] G. Li, H. Xu, W. Huang, Y. Wang, Y. Wu, R. Parajuli, A pyrrole quinoline quinone glucose dehydrogenase biosensor based on screen-printed carbon paste electrodes modified by carbon nanotubes, *Meas. Sci. Technol.* 19 (2008), 065203.
- [112] J. Razumien, V. Gurevicien, V. Laurinavicius, J.V. Gražulevičius, Amperometric detection of glucose and ethanol in beverages using flow cell and immobilised on screen-printed carbon electrode PQQ-dependent glucose or alcohol dehydrogenases, *Sensor. Actuator. B Chem.* 78 (2001) 243–248.
- [113] C. Lau, S. Borgmann, M. Maciejewska, B. Ngounou, P. Gründler, W. Schuhmann, Improved specificity of reagentless amperometric PQQ-sGDH glucose biosensors by using indirectly heated electrodes, *Biosens. Bioelectron.* 22 (2007) 3014–3020.
- [114] I.W. Schubart, G. Göbel, F. Lisdat, A pyrroloquinolinequinone-dependent glucose dehydrogenase (PQQ-GDH)-electrode with direct electron transfer based on polyaniline modified carbon nanotubes for biofuel cell application, *Electrochim. Acta* 82 (2012) 224–232.
- [115] C. Wettstein, H. Möhwald, F. Lisdat, Coupling of pyrroloquinoline quinone dependent glucose dehydrogenase to (cytochrome c/DNA)-multilayer systems on electrodes, *Bioelectrochemistry* 88 (2012) 97–102.
- [116] G. Fusco, G. Göbel, R. Zannoni, E. Kornejew, G. Favero, F. Mazzei, F. Lisdat, Polymer-supported electron transfer of PQQ-dependent glucose dehydrogenase at carbon nanotubes modified by electropolymerized polythiophene copolymers, *Electrochim. Acta* 248 (2017) 64–74.
- [117] G. Fusco, G. Göbel, R. Zannoni, M.P. Bracciale, G. Favero, F. Mazzei, F. Lisdat, Aqueous polythiophene electrosynthesis: a new route to an efficient electrode coupling of PQQ-dependent glucose dehydrogenase for sensing and bioenergetic applications, *Biosens. Bioelectron.* 112 (2018) 8–17.
- [118] R. Monošík, M. Středánský, K. Lušpai, P. Magdolen, E. Šturdík, Amperometric glucose biosensor utilizing FAD-dependent glucose dehydrogenase immobilized on nanocomposite electrode, *Enzym. Microb. Technol.* 50 (2012) 227–232.
- [119] R. Cohen, R.E. Bitton, N.S. Herzallh, Y. Cohen, O. Yehezkeili, Utilization of FAD-glucose dehydrogenase from *T. emersonii* for amperometric biosensing and biofuel cell devices, *Anal. Chem.* 93 (2021) 11585–11591.
- [120] A. Mahadevan, S. Fernando, Inorganic iron-sulfur clusters enhance electron transport when used for wiring the NAD-glucose dehydrogenase based redox system, *Microchim. Acta* 185 (2018) 1–8.
- [121] A.-M.J. Haque, P. Nandhakumar, H. Yang, Specific and rapid glucose detection using NAD-dependent glucose dehydrogenase, diaphorase, and osmium complex, *Electroanalysis* 31 (2019) 876–882.
- [122] A.B. Tahar, A. Szymczyk, S. Tingry, P. Vadgama, M. Zelmanne, S. Tsujumura, P. Cinquin, D. Martin, A. Zebda, One-year stability of glucose dehydrogenase confined in a 3D carbon nanotube electrode with coated poly-methylene green: application as bioanode for a glucose biofuel cell, *J. Electroanal. Chem.* 847 (2019), 113069.
- [123] M. Güneş, S. Karakaya, Y. Dilgin, Development of an interference-minimized amperometric-FIA glucose biosensor at a pyrocatechol violet/glucose dehydrogenase-modified graphite pencil electrode, *Chem. Pap.* 74 (2020) 1923–1936.
- [124] J.J. DiNicolantonio, J.H. O'Keefe, S.C. Lucan, Added fructose: a principal driver of type 2 diabetes mellitus and its consequences, in: *Mayo Clin. Proc.*, Elsevier, 2015, pp. 372–381.
- [125] L.H. Smith, R.H. Ettinger, D. Seligson, S. Lightcap, A comparison of the metabolism of fructose and glucose in hepatic disease and diabetes mellitus, *J. Clin. Invest.* 32 (1953) 273–282.
- [126] E. Russo, G. Leoncini, P. Esposito, G. Garibotto, R. Pontremoli, F. Viazzi, Fructose and uric acid: major mediators of cardiovascular disease risk starting at pediatric age, *Int. J. Mol. Sci.* 21 (2020) 4479.
- [127] G.A. Bray, B.M. Popkin, Calorie-sweetened beverages and fructose: what have we learned 10 years later, *Pediatr. Obes.* 8 (2013) 242–248.
- [128] J. Castillo, S. Gáspár, S. Leth, M. Niculescu, A. Mortari, I. Bontidean, V. Soukharev, S.A. Dorneanu, A.D. Ryabov, E. Csöregi, Biosensors for life quality: design, development and applications, *Sensor. Actuator. B Chem.* 102 (2004) 179–194.
- [129] N.C. Antoniadis, P.D. Rochford, J.J. Pretto, R.J. Pierce, J. Gogler, J. Steinkrug, K. Sharpe, C.F. McDonald, Pilot study of remote telemonitoring in COPD, *Telemed. E-Health.* 18 (2012) 634–640.
- [130] Y. Yamada, K. Aida, T. Uemura, A new enzyme, D-fructose dehydrogenase, *Agric. Biol. Chem.* 30 (1966) 95–96.
- [131] T. Adachi, Y. Kaida, Y. Kitazumi, O. Shirai, K. Kano, Bioelectrocatalytic performance of d-fructose dehydrogenase, *Bioelectrochemistry* 129 (2019) 1–9.
- [132] T. Adachi, Y. Kitazumi, O. Shirai, K. Kano, Recent progress in applications of enzymatic bioelectrocatalysis, *Catalysts* 10 (2020) 1413.
- [133] P. Bollella, Y. Hibino, K. Kano, L. Gorton, R. Antiochia, The influence of pH and divalent/monovalent cations on the internal electron transfer (IET), enzymatic activity, and structure of fructose dehydrogenase, *Anal. Bioanal. Chem.* 410 (2018) 3253–3264.
- [134] P. Bollella, L. Gorton, R. Antiochia, Direct electron transfer of dehydrogenases for development of 3rd generation biosensors and enzymatic fuel cells, *Sensors* 18 (2018) 1319.
- [135] P. Bollella, Y. Hibino, P. Conejo-Valverde, J. Soto-Cruz, J. Bergueiro, M. Calderón, O. Rojas-Carrillo, K. Kano, L. Gorton, The influence of the shape of Au nanoparticles on the catalytic current of fructose dehydrogenase, *Anal. Bioanal. Chem.* 411 (2019) 7645–7657.
- [136] T. Adachi, Y. Kitazumi, O. Shirai, K. Kano, Direct electron transfer-type bioelectrocatalysis of redox enzymes at nanostructured electrodes, *Catalysts* 10 (2020) 236.
- [137] M. Kizling, R. Bilewicz, Fructose dehydrogenase electron transfer pathway in bioelectrocatalytic reactions, *Chemelectrochem* 5 (2018) 166–174.
- [138] E. Nazaruk, E.M. Landau, R. Bilewicz, Membrane bound enzyme hosted in liquid crystalline cubic phase for sensing and fuel cells, *Electrochim. Acta* 140 (2014) 96–100.
- [139] I. Šakinytė, J. Barkauskas, J. Gaidukevič, J. Razumienė, Thermally reduced graphene oxide: the study and use for reagentless amperometric D-fructose biosensors, *Talanta* 144 (2015) 1096–1103.
- [140] T. Siepenkoetter, U. Salaj-Kosla, X. Xiao, S. Belochapkin, E. Magner, Nanoporous gold electrodes with tuneable pore sizes for bioelectrochemical applications, *Electroanalysis* 28 (2016) 2415–2423.
- [141] P. Bollella, Porous gold: a new frontier for enzyme-based electrodes, *Nanomaterials* 10 (2020) 722.
- [142] T. Siepenkoetter, U. Salaj-Kosla, E. Magner, The immobilization of fructose dehydrogenase on nanoporous gold electrodes for the detection of fructose, *Chemelectrochem* 4 (2017) 905–912.
- [143] P. Bollella, Y. Hibino, K. Kano, L. Gorton, R. Antiochia, Highly sensitive membraneless fructose biosensor based on fructose dehydrogenase immobilized onto aryl thiol modified highly porous gold electrode: characterization and application in food samples, *Anal. Chem.* 90 (2018) 12131–12136.
- [144] Y. Suzuki, K. Kano, O. Shirai, Y. Kitazumi, Diffusion-limited electrochemical d-fructose sensor based on direct electron transfer-type bioelectrocatalysis by a variant of d-fructose dehydrogenase at a porous gold microelectrode, *J. Electroanal. Chem.* 877 (2020), 114651.

- [145] X. Yan, S. Ma, J. Tang, D. Tanner, J. Ulstrup, X. Xiao, J. Zhang, Direct electron transfer of fructose dehydrogenase immobilized on thiol-gold electrodes, *Electrochim. Acta* 392 (2021), 138946.
- [146] P. Bollella, Y. Hibino, K. Kano, L. Gorton, R. Antiochia, Enhanced direct electron transfer of fructose dehydrogenase rationally immobilized on a 2-aminoanthracene diazonium cation grafted single-walled carbon nanotube based electrode, *ACS Catal.* 8 (2018) 10279–10289.
- [147] P. Bollella, Z. Boeva, R.-M. Latonen, K. Kano, L. Gorton, J. Bobacka, Highly sensitive and stable fructose self-powered biosensor based on a self-charging biosupercapacitor, *Biosens. Bioelectron.* 176 (2021), 112909.
- [148] J.-W. Mo, W. Smart, Lactate biosensors for continuous monitoring, *Front. Biosci.* 9 (2004) 3384–3391.
- [149] Q. Yang, P. Atanasov, E. Wilkins, Needle-type lactate biosensor, *Biosens. Bioelectron.* 14 (1999) 203–210.
- [150] L. Rassaai, W. Olthuis, S. Tsujimura, E.J. Sudhölter, A. van den Berg, Lactate biosensors: current status and outlook, *Anal. Bioanal. Chem.* 406 (2014) 123–137.
- [151] W. Jia, A.J. Bandonkar, G. Valdés-Ramírez, J.R. Windmiller, Z. Yang, J. Ramírez, G. Chan, J. Wang, Electrochemical tattoo biosensors for real-time noninvasive lactate monitoring in human perspiration, *Anal. Chem.* 85 (2013) 6553–6560.
- [152] X. Luo, W. Shi, H. Yu, Z. Xie, K. Li, Y. Cui, Wearable carbon nanotube-based biosensors on gloves for lactate, *Sensors* 18 (2018) 3398.
- [153] F. Tasca, C. Tortolini, P. Bollella, R. Antiochia, Microneedles-based electrochemical devices for transdermal biosensing: a review, *Curr. Opin. Electrochem.* 16 (2019) 42–49.
- [154] M.M. Hall, S. Rajasekaran, T.W. Thomsen, A.R. Peterson, Lactate: friend or foe, *PM&R* 8 (2016) S8–S15.
- [155] M. Adeva-Andany, M. López-Ojén, R. Funcasta-Calderón, E. Ameneiros-Rodríguez, C. Donapetry-García, M. Vila-Altesor, J. Rodríguez-Seijas, Comprehensive review on lactate metabolism in human health, *Mitochondrion* 17 (2014) 76–100.
- [156] J.D. Rabinowitz, S. Enerbäck, Lactate: the ugly duckling of energy metabolism, *Nat. Metab.* 2 (2020) 566–571.
- [157] J.B. Jeppesen, C. Mortensen, F. Bendtsen, S. Møller, Lactate metabolism in chronic liver disease, *Scand. J. Clin. Lab. Invest.* 73 (2013) 293–299.
- [158] I. Taurino, R. Reiss, M. Richter, M. Fairhead, L. Thöny-Meyer, G. De Micheli, S. Carrara, Comparative study of three lactate oxidases from *Aerococcus viridans* for biosensing applications, *Electrochim. Acta* 93 (2013) 72–79.
- [159] S. Suman, R. Singhal, A.L. Sharma, B.D. Malthotra, C.S. Pundir, Development of a lactate biosensor based on conducting copolymer bound lactate oxidase, *Sensor. Actuator. B Chem.* 107 (2005) 768–772.
- [160] E.N. Biryukova, A.Y. Arinbasarova, A.G. Medentsev, L-lactate oxidase systems of microorganisms, *Microbiology* 91 (2022) 124–132.
- [161] I. Leiros, E. Wang, T. Rasmussen, E. Oksanen, H. Repo, S.B. Petersen, P. Heikinheimo, E. Hough, The 2.1 Å structure of *Aerococcus viridans* L-lactate oxidase (LOX), *Acta Crystallogr., Sect. F: Struct. Biol. Cryst. Commun.* 62 (2006) 1185–1190.
- [162] K. Hiraka, K. Kojima, C.-E. Lin, W. Tsugawa, R. Asano, J.T. La Belle, K. Sode, Minimizing the effects of oxygen interference on L-lactate sensors by a single amino acid mutation in *Aerococcus viridans* L-lactate oxidase, *Biosens. Bioelectron.* 103 (2018) 163–170.
- [163] N. Nikolaus, B. Strehlitz, Amperometric lactate biosensors and their application in (sports) medicine, for life quality and wellbeing, *Microchim. Acta* 160 (2008) 15–55.
- [164] I.S. Kucherenko, Y.V. Topolnikova, O.O. Soldatkin, Advances in the biosensors for lactate and pyruvate detection for medical applications: a review, *TrAC, Trends Anal. Chem.* 110 (2019) 160–172.
- [165] H. Cunha-Silva, M.J. Arcos-Martínez, Dual range lactate oxidase-based screen printed amperometric biosensor for analysis of lactate in diversified samples, *Talanta* 188 (2018) 779–787.
- [166] S. Hashemzadeh, Y. Omid, H. Rafii-Tabar, Amperometric lactate nanobiosensor based on reduced graphene oxide, carbon nanotube and gold nanoparticle nanocomposite, *Microchim. Acta* 186 (2019) 1–8.
- [167] O.-M. Istrate, L. Rotariu, C. Bala, Amperometric L-Lactate biosensor based upon a gold nanoparticles/reduced graphene oxide/polyallylamine hydrochloride modified screen-printed graphite electrode, *Chemosensors* 9 (2021) 74.
- [168] L. Meng, A.P. Turner, W.C. Mak, Conducting polymer-reinforced laser-irradiated graphene as a heterostructured 3D transducer for flexible skin patch biosensors, *ACS Appl. Mater. Interfaces* 13 (2021) 54456–54465.
- [169] R. Sainz, M. Del Pozo, L. Vázquez, M. Vilas-Varela, J. Castro-Esteban, E. Blanco, M.D. Petit-Domínguez, C. Quintana, E. Casero, Lactate biosensing based on covalent immobilization of lactate oxidase onto chevron-like graphene nanoribbons via diazotization-coupling reaction, *Anal. Chim. Acta* 1208 (2022), 339851.
- [170] A. Khan, M. Winder, G. Hossain, Modified graphene-based nanocomposite material for smart textile biosensor to detect lactate from human sweat, *Biosens. Bioelectron.* X. 10 (2022), 100103.
- [171] M. Regiart, A. Ledo, E. Fernandes, G.A. Messina, C.M. Brett, M. Bertotti, R. M. Barbosa, Highly sensitive and selective nanostructured microbiosensors for glucose and lactate simultaneous measurements in blood serum and in vivo in brain tissue, *Biosens. Bioelectron.* 199 (2022), 113874.
- [172] J. Madden, E. Vaughan, M. Thompson, A. O'Riordan, P. Galvin, D. Iacopino, S. R. Teixeira, Electrochemical sensor for enzymatic lactate detection based on laser-scribed graphitic carbon modified with platinum, chitosan and lactate oxidase, *Talanta* 246 (2022), 123492.
- [173] C. Zhu, Y. Xu, Q. Chen, H. Zhao, B. Gao, T. Zhang, A flexible electrochemical biosensor based on functionalized poly (3, 4-ethylenedioxythiophene) film to detect lactate in sweat of the human body, *J. Colloid Interface Sci.* 617 (2022) 454–462.
- [174] M. Liu, M. Yang, M. Wang, H. Wang, J. Cheng, A flexible dual-analyte electrochemical biosensor for salivary glucose and lactate detection, *Biosensors* 12 (2022) 210.
- [175] S. Neampet, N. Ruecha, J. Qin, W. Wonsawat, O. Chailapakul, N. Rodthongkum, A nanocomposite prepared from platinum particles, polyaniline and a Ti3C2 MXene for amperometric sensing of hydrogen peroxide and lactate, *Microchim. Acta* 186 (2019) 1–8.
- [176] K. Van Hoovels, X. Xuan, M. Cuartero, M. Gijssels, M. Swarén, G.A. Crespo, Can wearable sweat lactate sensors contribute to sports physiology? *ACS Sens.* 6 (2021) 3496–3508.
- [177] A.V. Mohan, J.R. Windmiller, R.K. Mishra, J. Wang, Continuous minimally-invasive alcohol monitoring using microneedle sensor arrays, *Biosens. Bioelectron.* 91 (2017) 574–579.
- [178] H. Teymourian, C. Moonla, F. Tehrani, E. Vargas, R. Aghavali, A. Barfidokht, T. Tangkuaram, P.P. Mercier, E. Dassau, J. Wang, Microneedle-based detection of ketone bodies along with glucose and lactate: toward real-time continuous interstitial fluid monitoring of diabetic ketosis and ketoacidosis, *Anal. Chem.* 92 (2019) 2291–2300.
- [179] J. Min, J.R. Sempionatto, H. Teymourian, J. Wang, W. Gao, Wearable electrochemical biosensors in North America, *Biosens. Bioelectron.* 172 (2021), 112750.
- [180] P. Bollella, S. Sharma, A.E.G. Cass, R. Antiochia, Microneedle-based biosensor for minimally-invasive lactate detection, *Biosens. Bioelectron.* 123 (2019) 152–159.
- [181] P. Bollella, S. Sharma, A.E.G. Cass, R. Antiochia, Minimally-invasive microneedle-based biosensor array for simultaneous lactate and glucose monitoring in artificial interstitial fluid, *Electroanalysis* 31 (2019) 374–382.
- [182] P. Bollella, S. Sharma, A.E. Cass, F. Tasca, R. Antiochia, Minimally invasive glucose monitoring using a highly porous gold microneedles-based biosensor: characterization and application in artificial interstitial fluid, *Catalysts* 9 (2019) 580.
- [183] H.H. Weetall, Biosensor Technology what? where? when? and Why? Elsevier, 1996.
- [184] J.H. Luong, K.B. Male, J.D. Glennon, Biosensor technology: technology push versus market pull, *Biotechnol. Adv.* 26 (2008) 492–500.
- [185] M.M.P. da Silva Neves, M.B. González-García, D. Hernandez-Santos, P. Fanjul-Bolado, Future trends in the market for electrochemical biosensing, *Curr. Opin. Electrochem.* 10 (2018) 107–111.
- [186] C. Ming Li, H. Dong, X. Cao, J.H. T. Luong, X. Zhang, Implantable electrochemical sensors for biomedical and clinical applications: progress, problems, and future possibilities, *Curr. Med. Chem.* 14 (2007) 937–951.
- [187] E. Cesewski, B.N. Johnson, Electrochemical biosensors for pathogen detection, *Biosens. Bioelectron.* 159 (2020), 112214.
- [188] G. Moro, F. Bottari, J. Van Loon, E. Du Bois, K. De Wael, L.M. Moretto, Disposable electrodes from waste materials and renewable sources for (bio) electroanalytical applications, *Biosens. Bioelectron.* 146 (2019), 111758.
- [189] H. Dong, C.M. Li, W. Chen, Q. Zhou, Z.X. Zeng, J.H. Luong, Sensitive amperometric immunosensing using polypyrrolepropionic acid films for biomolecule immobilization, *Anal. Chem.* 78 (2006) 7424–7431.
- [190] P.A. Kottke, C. Kranz, Y.K. Kwon, J.-F. Masson, B. Mizaikoff, A.G. Fedorov, Theory of polymer entrapped enzyme ultra-microelectrodes: Fundamentals, *J. Electroanal. Chem.* 612 (2008) 208–218.
- [191] E. Bakker, Can calibration-free sensors be realized? *ACS Sens.* 1 (2016) 838–841.
- [192] E.T. da Silva, D.E. Souto, J.T. Barragan, J. de F. Giarola, A.C. de Moraes, L. T. Kubota, Electrochemical biosensors in point-of-care devices: recent advances and future trends, *ChemElectroChem* 4 (2017) 778–794.
- [193] V. Zucolotto, Specialty grand challenges in biosensors, *Front. Sens.* (2020) 3.
- [194] K. Mahato, J. Wang, Electrochemical sensors: from the bench to the skin, *Sensor. Actuator. B Chem.* 344 (2021), 130178.
- [195] H. Teymourian, F. Tehrani, K. Mahato, J. Wang, Lab under the skin: microneedle based wearable devices, *Adv. Healthc. Mater.* 10 (2021), 2002255.
- [196] D.R. Seshadri, R.T. Li, J.E. Voos, J.R. Rowbottom, C.M. Alfes, C.A. Zorman, C. K. Drummond, Wearable sensors for monitoring the physiological and biochemical profile of the athlete, *NPJ Digit. Med.* 2 (2019) 1–16.
- [197] Biosensors market size, growth, trends, Report 2022 to 2030, (n.d.), <https://www.precedenceresearch.com/biosensors-market>. (Accessed 9 October 2022).
- [198] J. Kim, A.S. Campbell, B.E.-F. de Ávila, J. Wang, Wearable biosensors for healthcare monitoring, *Nat. Biotechnol.* 37 (2019) 389–406.
- [199] G. Valdés-Ramírez, J.R. Windmiller, J.C. Claussen, A.G. Martínez, F. Kuralay, M. Zhou, N. Zhou, R. Polsky, P.R. Miller, R. Narayan, Multiplexed and switchable release of distinct fluids from microneedle platforms via conducting polymer nanoactuators for potential drug delivery, *Sensor. Actuator. B Chem.* 161 (2012) 1018–1024.
- [200] M. Zhou, N. Zhou, F. Kuralay, J.R. Windmiller, S. Parkhomovsky, G. Valdés-Ramírez, E. Katz, J. Wang, A self-powered “sense-act-treat” system that is based on a biofuel cell and controlled by boolean logic, *Angew. Chem.* 124 (2012) 2740–2743.
- [201] X. Xiao, K.D. McGourty, E. Magner, Enzymatic biofuel cells for self-powered, controlled drug release, *J. Am. Chem. Soc.* 142 (2020) 11602–11609.
- [202] M. Liang, X. Yan, Nanozymes: from new concepts, mechanisms, and standards to applications, *Acc. Chem. Res.* 52 (2019) 2190–2200.
- [203] P. Bollella, M. Bellare, V.K. Kadambar, Z. Guo, K. Alexandrov, A. Melman, E. Katz, Boolean logic networks mimicked with chimeric enzymes activated/inhibited by several input signals, *ChemPhysChem* 21 (2019) 589–593.

- [204] P. Bollella, Z. Guo, S. Edwardraja, V.K. Kadambar, K. Alexandrov, A. Melman, E. Katz, Self-powered molecule release systems activated with chemical signals processed through reconfigurable Implication or Inhibition Boolean logic gates, *Bioelectrochemistry* 138 (2021), 107735.
- [205] G. Strack, M. Pita, M. Ornatska, E. Katz, Boolean logic gates that use enzymes as input signals, *Chembiochem* 9 (2008) 1260–1266.
- [206] Z. Guo, W.A. Johnston, V. Stein, P. Kalimuthu, S. Perez-Alcala, P.V. Bernhardt, K. Alexandrov, Engineering PQQ-glucose dehydrogenase into an allosteric electrochemical Ca<sup>2+</sup> sensor, *Chem. Commun.* 52 (2015) 485–488.
- [207] P. Bollella, S. Edwardraja, Z. Guo, C.E. Vickers, J. Whitfield, P. Walden, A. Melman, K. Alexandrov, E. Katz, Connecting artificial proteolytic and electrochemical signaling systems with caged messenger peptides, *ACS Sens.* 6 (2021) 3596–3603.
- [208] C. Demolder, A. Molina, F.L. Hammond III, W.-H. Yeo, Recent advances in wearable biosensing gloves and sensory feedback biosystems for enhancing rehabilitation, prostheses, healthcare, and virtual reality, *Biosens. Bioelectron.* 190 (2021), 113443.
- [209] A. Tricase, A. Imbriano, E. Macchia, L. Sarcina, C. Scandurra, F. Torricelli, N. Cioffi, L. Torsi, P. Bollella, Enzyme based amperometric wide field biosensors: is single molecule detection possible? *Electrochem. Sci. Adv.* (2022), e2100215.
- [210] L. Sarcina, E. Macchia, A. Tricase, C. Scandurra, A. Imbriano, F. Torricelli, N. Cioffi, L. Torsi, P. Bollella, Enzyme based field effect transistor: state-of-the-art and future perspectives, *Electrochem. Sci. Adv.* (2022), e2100216.



**Paolo Bollella** is an assistant professor at University of Bari in the Department of Chemistry. Till December 2020, he was a Research Assistant Professor at Clarkson University in the Department of Chemistry and Biomolecular Science (USA). After his PhD, he joined the Department of Analytical Chemistry at Åbo Akademi in Turku (Finland) with a Johan Gadolin PostDoc fellowship awarded from the board of Johan Gadolin Process Chemistry Center. In October 2018, he joined the group of “Bioelectronics & Bionanotechnology” led by Prof. Evgeny Katz. In March 2019, he was awarded with the Minerva Prize for the Scientific Research – Merit Mention for the achievements obtained during his doctoral thesis based on the study of Mediated/Direct Electron Transfer of Redox Protein for Biosensors and Biofuel Cells Applications. In 2020, he was recognized among the top 100000 most influencing scientists and engineers (statistical analysis elaborated by Stanford University). He is author of 72 papers on peer-reviewed international journals (Hirsch-index 20), 3 book chapters, 1 student book, 2 proceedings and almost 60 oral or poster contributions to national and international conferences.