

A colorimetric aptamer biosensor based on cationic polymer and gold nanoparticles for the ultrasensitive detection of thrombin

Zhengbo Chen*, Yuan Tan, Chenmeng Zhang, Lu Yin, He Ma, Nengsheng Ye, Hong Qiang, Yuqing Lin

Department of Chemistry, Capital Normal University, Beijing 100048, China

ARTICLE INFO

Article history:

Received 4 November 2013

Received in revised form

21 December 2013

Accepted 5 January 2014

Available online 11 January 2014

Keywords:

Gold nanoparticles

Cationic polymer

Colorimetry

Thrombin

Aptamer

ABSTRACT

A colorimetric assay for the ultrasensitive determination of thrombin based on cationic polymer and gold nanoparticles was presented, in which unmodified gold nanoparticles (AuNPs) was used as probes and 21-mer thrombin-binding aptamer (TBA) as sensing elements. Upon the addition of thrombin, TBA interacted specifically with thrombin to form a G-quadruplex structure. As a result, the conformation change facilitated the cationic polymer, poly(diallyldimethylammonium chloride) (PDDA)-induced AuNP aggregation. Thus, the visible change in color from wine-red to blue–purple was readily seen by the naked eye. The colorimetric sensor could detect thrombin down to 1 pM with high selectivity in the presence of other interfering proteins. Furthermore, the assay was successfully employed to determine thrombin in human serum sample, which suggested its great potential for diagnostic purposes.

© 2014 Elsevier B.V. All rights reserved.

1. Introduction

Thrombin is an important multifunctional enzyme involved in many physiological and pathological processes, such as blood coagulation, thrombosis, inflammation, angiogenesis, tumor growth and metastasis (Zhao and Gao, 2013). Thrombin can be used as a therapeutic and a biomarker for diagnosis of some diseases, such as pulmonary metastases and diseases associated with coagulation abnormalities (Licari and Kovacic, 2009; Kitamoto et al., 2008). Under normal conditions, the concentration of thrombin in blood varies from nanomolar to low micromolar levels during the coagulation progress (Arai et al., 2006). The current clinical methods for protein detection rely heavily on antibodies (Shuman and Majerus, 1976; Bichler et al., 1991; Zhu et al., 2000). Although these conventional strategies provide accurate and sensitive detection of proteins, there are still some inconveniences that exist, such as the utilization of radioactive substances, enzyme labeling, time-consuming processes, and technical expertise as well as sophisticated equipment. Thus, development of protein sensing methods that are rapid, simple, sensitive, selective, on-site and cost-effective is still highly desirable.

Aptamers are single stranded DNA molecules or RNA that selectively bind to various target molecules with high affinity, such as small molecules, proteins and drugs (Zuo et al., 2007; Lai et al., 2007; Bang et al., 2013). Compared to traditional molecular

recognition system, aptamers have a lot of advantages in terms of the simplicity of synthesis. Aptamers can be stored stable for a long term, ease of labeling, excellent stability, wide applicability, and high sensitivity. As a consequence, their properties make them very attractive for applications in medical diagnosis, environmental monitoring and biological analysis (Li et al., 2010; Song et al., 2008; Zhang et al., 2008; Wang et al., 2009). Different detection techniques such as optical (Chang et al., 2010; Huang et al., 2010; Yan et al., 2011), electrochemical (Bang et al., 2005; He et al., 2007; Xiao et al., 2005; Zhao et al., 2011), surface enhanced resonance Raman scattering (SERRS) (Cho et al., 2008), electrochemiluminescence (Wang et al., 2011), surface plasmon resonance (Ostatna et al., 2008; Polonschii et al., 2010) and so on have been developed to detect thrombin. However, they are limited by the sensitivity, in which only nanomolar or micromolar concentrations of thrombin are detectable. Compared with those sophisticated equipment, colorimetric sensors gained increasing attention for its very short assay time (merely several minutes), relatively low cost and no requirement for skillful technicians (Han and Kim, 2002). Until now, colorimetric aptasensor for thrombin detection has rarely been reported.

Herein, we developed a simple and ultrasensitive colorimetric aptasensor for thrombin detection based on AuNPs and water-soluble cationic polymer (PDDA) instead of salt with a high concentration, because the sensors based on salt-induced AuNP aggregation suffer from relatively higher detection limits (Yang et al., 2011; Zheng et al., 2011; Song et al., 2011). Otherwise, PDDA exhibits not only a significant advantage in relation to the aggregation of AuNPs but also electrostatic interactions with DNA

* Corresponding author. Tel.: +86 10 68903047.
E-mail address: czb979216@sina.com (Z. Chen).

(Ofir et al., 2008; Peng et al., 2006; Xia et al., 2010). Using these properties, we developed a colorimetric aptamer biosensor for thrombin detection based on PDDA and TBA-mediated aggregation of AuNPs. The results indicated that the method was simple, cheap, and highly sensitive and selective for thrombin detection and could be successfully used in the quantitative detection of thrombin in human serum samples.

2. Experimental

2.1. Reagents and apparatus

TBA oligonucleotides (5'-TTTGGTGGTGTGGTGGTTT-3') were synthesized by Sangon Biotechnology Co. Ltd. (Shanghai, China). Sodium tetrachloroaurate(III) (HAuCl₄), sodium citrate and tris-base were purchased from Sigma-Aldrich (USA). PDDA was obtained from Aladdin reagent (Shanghai) Co. Ltd. All other reagents are of analytical reagent grade. All solutions were prepared with Tris-HCl buffer solution (pH 7.41).

Ultraviolet-visible (UV-vis) absorption spectra were recorded on an UV-2550 Spectrophotometer (Shimadzu Corporation). Transmission electron microscope (TEM) observations were carried out with a JEOL JEM2010 microscope at 200 kV.

2.2. Preparation of AuNPs

The 15-nm diameter AuNPs were prepared by the citrate-mediated reduction of HAuCl₄ according to the published protocol (Storhoff et al., 1998). The obtained AuNP solution (4.9 nM) was cooled to room temperature and stored at 4 °C. The concentration of these AuNP solution was determined by UV-vis spectroscopy using an extinction coefficient of $2.7 \times 10^8 \text{ M}^{-1} \text{ cm}^{-1}$ at $\lambda = 520 \text{ nm}$ for 15 nm AuNPs (Jin et al., 2003).

2.3. General procedure of colorimetric sensing of thrombin

First, 498 μL of thrombin with various concentrations were respectively added into a 1.5 mL plastic vial containing 1 μL TBA solution (10 μM) in 20 mM Tris-HCl buffer solution (pH 7.41). After incubation for 20 min at 37 °C, 1 μL of PDDA solution (10 μM) was added. Reacting for 10 min, then 500 μL of AuNP solution (4.9 nM) was added quickly into this vial and mixed thoroughly. After another 5 min of incubation, 1000 μL of the resulting solution was transferred to a 1 cm micro quartz cuvette for spectral recording. In addition to incubation of thrombin at 37 °C, all other assays were performed at room temperature.

3. Results and discussion

3.1. Principle of colorimetric method for thrombin detection

A schematic representation of the mechanism of the colorimetric sensing thrombin is illustrated in Fig. 1. In the absence of target thrombin, free single-stranded DNA (ssDNA) with a random coil structure interacted with cationic polymer, PDDA through electrostatic interaction. Aptamer and PDDA formed a duplex structure (Wu et al., 2012). Thus PDDA was not sufficient to induce the aggregation of AuNPs. However, upon the addition of thrombin, the aptamer with a random coil structure could be changed into a G-quadruplex structure. Therefore, the remaining PDDA could link the AuNPs together to make the aggregation. The aggregation of AuNPs led to a change in color from wine-red to blue-purple.

3.2. Optimization of experimental conditions

To optimize the sensing conditions, various concentrations of PDDA (1, 3, 5, 8, 10, 30 and 50 nM) were added into a micro cuvette containing 500 μL Tris-HCl buffer solution (20 mM, pH 7.41), then

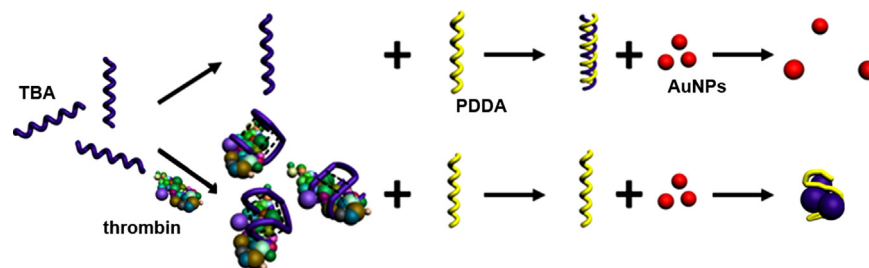


Fig. 1. Schematic representation of the sensing procedure for colorimetric detection of thrombin based on cationic polymer and gold nanoparticles.

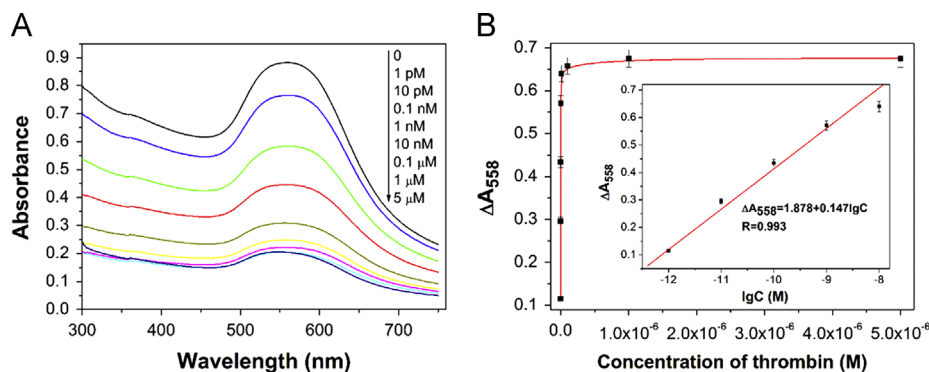


Fig. 2. (A) The UV-vis absorbance spectra of AuNPs in the presence of 10 nM PDDA and 10 nM TBA in 20 mM Tris-HCl buffer solution (pH 7.41) containing different concentrations of Thrombin (1 pM–5 μM). (B) The peak absorbance change at 558 nm as a function of thrombin concentration. Inset: the peak absorbance change of 558 nm is linear with logarithm of thrombin concentration over the range from 1 pM to 10 nM.

500 μL of AuNP solution was transferred into the vial. The UV–vis absorbance values showed that 10 nM PDDA was suitable to aggregate all the AuNPs (Fig. S1, Table S1). Thus, 10 nM PDDA was chosen for the following experiment. Subsequently, the concentration of the TBA was studied at a fixed concentration of 10 nM PDDA. First, varying concentrations of TBA (1, 3, 5, 8, 10, 30 and 50 nM) were incubated in 500 μL Tris–HCl buffer solution containing 10 nM PDDA for 20 min, and then 500 μL of constant AuNP solution was added. The result showed that 10 nM of TBA was chosen as an optimum reaction concentration to detect thrombin (Fig. S2, Table S2).

3.3. In vitro detection of thrombin

The optimized sensor was applied to the detection of thrombin, which was monitored visually with a UV–vis spectrophotometer, the naked eye, and TEM imaging. A series of different concentrations of thrombin were respectively added and their UV–vis spectra were recorded, as shown in Fig. 2A. As higher concentrations of thrombin ranging from 1 pM to 5 μM were added, the absorption intensity of the AuNPs at 520 nm gradually decreased. Increase of concentrations of thrombin led to decrease in absorbance peak at 558 nm up to 1 μM . Fig. 2B shows the derived calibration curves corresponding to Fig. 2A. As can be seen in Fig. 2B, the ΔA_{558} was proportional to the log value of thrombin concentration over the range of 1 pM–10 nM (inset of Fig. 2B). The linear equation could be fitted as $\Delta A_{558} = 1.878 + 0.147 \lg C$, ($R = 0.993$) with a limit detection of 1 pM. The relative standard

deviation for results from the TBA/PDDA/AuNPs for each thrombin concentration, are listed in Table S3. These indicate that the proposed biosensor offers excellent reproducibility (RSDs < 3.11%, $n = 3$). The experimental results revealed that the color of the AuNP solution underwent an obvious change from wine-red to blue–purple with the increase of thrombin concentration, as shown in Fig. 3. In the absence of thrombin, the color of the AuNP solution was red, implying that the AuNPs were still dispersed. This was because aptamer interacts with PDDA to form a duplex

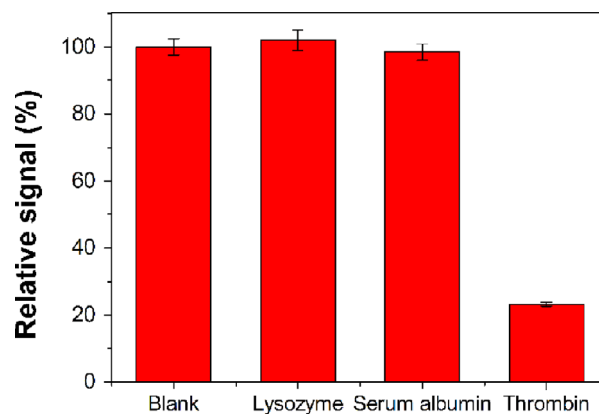


Fig. 5. Specificity of aptasensor for thrombin. The values of A_{558} for other competing proteins (lysozyme and serum albumin) were measured at the same concentration of 1 μM .

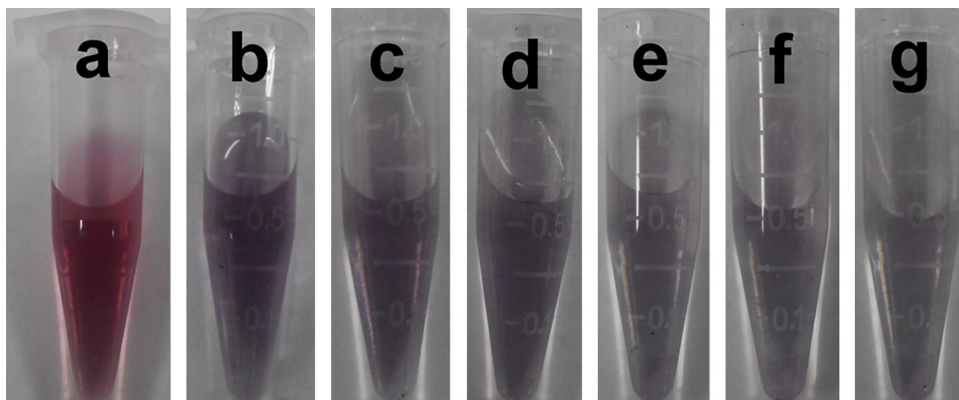


Fig. 3. Visual color changes upon treatment of the TBA/AuNP system with or without various thrombin in the presence of PDDA. (a) 4.9 nM AuNPs; (b) 10 nM TBA–10 nM PDDA–4.9 nM AuNPs; (c) 1 pM thrombin–10 nM TBA–10 nM PDDA–4.9 nM AuNPs; (d) 10 pM thrombin–10 nM TBA–10 nM PDDA–4.9 nM AuNPs; (e) 10 nM thrombin–10 nM TBA–10 nM PDDA–4.9 nM AuNPs; (f) 1 μM thrombin–10 nM TBA–10 nM PDDA–4.9 nM AuNPs; (g) 0.1 μM thrombin–10 nM TBA–10 nM PDDA–4.9 nM AuNPs. (For interpretation of the references to color in this figure legend, the reader is referred to the web version of this article.)

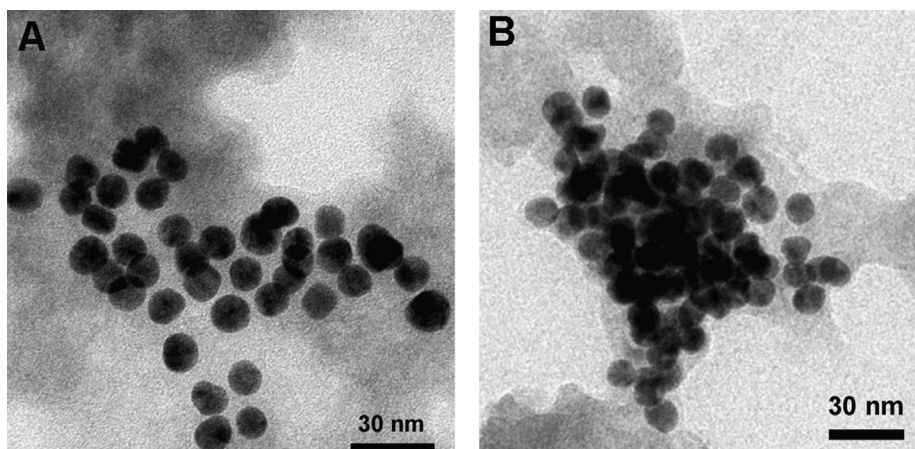


Fig. 4. TEM images of (A) 4.9 nM AuNPs–10 nM TBA–10 nM PDDA, and (B) 4.9 nM AuNPs–10 nM TBA–1 μM thrombin–10 nM PDDA.

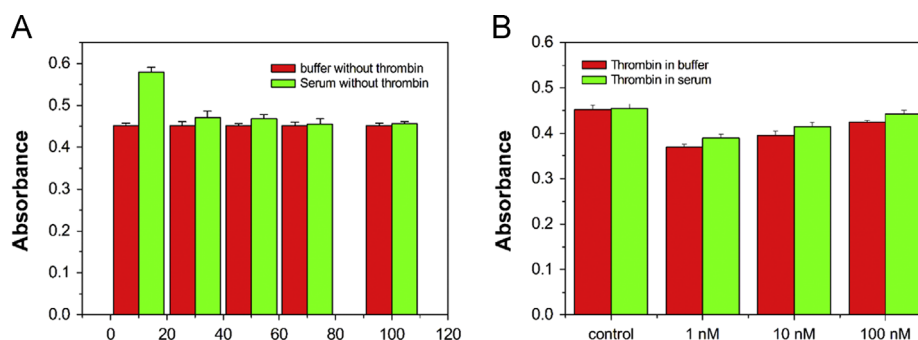


Fig. 6. Results obtained from the testing of (A) Tris-HCl buffer solution and serum samples with different dilution ratios without thrombin, and (B) 70-fold diluted serum samples spiked with different concentrations of thrombin.

structure through electrostatic interactions and the concentration of PDDA was not sufficient for aggregation of the AuNPs. When the concentration of thrombin was increased to 0.1 μM , the color of the AuNP solution was blue–purple. These were consistent with the fact that the TBA interacts with thrombin to form a stabilized G-quadruplex and the degree of aggregation of the AuNPs was induced by the interaction of the AuNPs with PDDA. The state of the AuNP solution was further confirmed by TEM imaging. Fig. 4A shows that the AuNPs was still dispersed after the addition of PDDA in the presence of TBA. Fig. 4B clearly displays that the AuNPs aggregated after the addition of PDDA in the presence of both thrombin and TBA.

3.4. Detection specificity

The developed colorimetric aptasensor was also specific. To evaluate this property, we challenged the system with the target thrombin (1 μM) and several nontargeted proteins such as lysozyme and serum albumin (all at such as 1 μM). Fig. 5 shows that significant change in absorbance value is only observed for the target thrombin and not for other nontargeted proteins, speaking to the excellent selectivity of the sensor for thrombin over other selected proteins.

3.5. Detection of thrombin in human serum sample

The performance of the thrombin sensor in a real human serum sample is further investigated. First, the tolerance of the present method under the different dilution rates of human serum was investigated by analyzing different dilution ratios (1:10, 1:30, 1:50, 1:70, 1:100) of human serum without thrombin, as shown in Fig. 6A. It was obvious that the absorbance values from the diluted serum were comparable to those from Tris-HCl buffer solution when the dilution ratio was up to 1:70. Then, the 70-fold dilution of human serum samples were spiked with thrombin three concentrations (1, 10, and 100 nM) and measured. As shown in Fig. 6B, comparable responses were found for thrombin in both buffer and serum. The results showed that the designed thrombin sensor still worked well in real serum samples.

4. Conclusion

To sum up, we take advantage of the color change of AuNPs induced by the cationic polymer, PDDA to develop a colorimetric sensor for visual detection of thrombin. The new method offered several advantages over current thrombin detection techniques. First, the colorimetric method did not require complicated and expensive instruments, which can be readily seen by the naked eye or with the aid of simple UV–vis spectrometer. Second, using this aptasensor, the limit of thrombin detection for the naked eye

within 10 min was as low as 1 pM, which was useful for rapid and ultrasensitive detection of thrombin. Third, the sensor showed excellent specificity to target thrombin compared with protein competitors. Finally, this method was well applied for thrombin determination in human serum samples. These advantages substantially made this method promising for rapid detection of thrombin in aqueous solution.

Acknowledgments

All authors gratefully acknowledge the financial support of the Natural Science Foundation of China (No. 21005050, 21375088).

Appendix A. Supporting information

Supplementary data associated with this article can be found in the online version at <http://dx.doi.org/10.1016/j.bios.2014.01.012>.

References

- Arai, T., Miklosy, J., Klegeris, A., Guo, J.P., McGeer, P.L., 2006. *J. Neuropathol. Exp. Neurol.* 65, 19–25.
- Bang, G.S., Cho, S.Y., Kim, B.G., 2005. *Biosens. Bioelectron.* 21, 863–870.
- Bang, G.S., Cho, S.Y., Lee, N., Lee, B.R., Kim, J.H., Kim, B.G., 2013. *Biosens. Bioelectron.* 39, 44–50.
- Bichler, J., Siebeck, M., Maschler, R., Pelzer, H., Fritz, H., 1991. *Blood Coagul. Fibrinolysis* 2, 129–133.
- Chang, H., Tang, L., Wang, Y., Jiang, J., Li, J., 2010. *Anal. Chem.* 82, 2341–2346.
- Cho, H., Baker, B.R., Wachsmann-Hogiu, S., Pagba, C.V., Laurence, T.A., Lane, S.M., Lee, L.P., Tok, J.B.H., 2008. *Nano Lett.* 8, 4386–4390.
- Han, M.S., Kim, D.H., 2002. *Angew. Chem. Int. Ed.* 114, 3963–3965.
- He, P., Shen, L., Cao, Y., Li, D., 2007. *Anal. Chem.* 79, 8024–8029.
- Huang, D.W., Niu, C.G., Qin, P.Z., Ruan, M., Zeng, G.M., 2010. *Talanta* 83, 185–189.
- Jin, R.C., Wu, G.S., Li, Z., Mirkin, C.A., Schatz, G.C., 2003. *J. Am. Chem. Soc.* 125, 1643–1654.
- Kitamoto, Y., Nakamura, E., Kudo, S., Tokunaga, H., Murakami, E., Noguchi, K., Imamura, T., 2008. *Clin. Chim. Acta* 398, 159–160.
- Lai, R.Y., Plaxco, K.W., Heeger, A.J., 2007. *Anal. Chem.* 79, 229–233.
- Li, D., Song, S., Fan, C., 2010. *Acc. Chem. Res.* 43, 631–641.
- Licari, L.G., Kovacic, J.P., 2009. *J. Vet. Emerg. Crit. Care* 19, 11–22.
- Ofir, Y., Samanta, B., Rotello, V.M., 2008. *Chem. Soc. Rev.* 37, 1814–1825.
- Ostatna, V., Vaisocherova, H., Homola, J., Hianik, T., 2008. *Anal. Bioanal. Chem.* 391, 1861–1869.
- Peng, H., Soeller, C., Trivas-Sejdic, J., 2006. *Chem. Commun.*, 3735–3737.
- Polonschii, C., David, S., Tombelli, S., Mascini, M., Gheorghiu, M., 2010. *Talanta* 80, 2157–2164.
- Shuman, M.A., Majerus, P.W., 1976. *J. Clin. Invest.* 58, 1249–1258.
- Song, K.M., Cho, M., Jo, H., Min, K., Jeon, S.H., Kim, T., Han, M.S., Ku, J.K., Ban, C., 2011. *Anal. Chem.* 415, 175–181.
- Song, S.P., Wang, L.H., Li, J., Fan, C.H., Zhao, J.L., 2008. *TrAC, Trends Anal. Chem.* 27, 108–117.
- Storhoff, J.J., Elghanian, R., Mucic, R.C., Mirkin, C.A., Letsinger, R.L., 1998. *J. Am. Chem. Soc.* 120, 1959–1964.
- Wang, J., Cao, Y., Chen, G.F., Li, G.X., 2009. *Biosens. Bioelectron.* 10, 2171–2176.
- Wang, J., Shan, Y., Zhao, W.W., Xu, J.J., Chen, H.Y., 2011. *Anal. Chem.* 83, 4004–4011.
- Wu, Y., Zhan, S., Wang, F., He, L., Zhi, W., Zhou, P., 2012. *Chem. Commun.* 48, 4459–4461.

- Xia, F., Zuo, X., Yang, R., Xiao, Y., Kang, D., Vallee-Belisle, A., Gong, X., Heeger, A.J., Plaxco, K.W., 2010. *J. Am. Chem. Soc.* 132, 1252–1254.
- Xiao, Y., Lubin, A.A., Heeger, A.J., Plaxco, K.W., 2005. *Angew. Chem. Int. Ed.* 117, 5592–5595.
- Yan, S., Huang, R., Zhou, Y., Zhang, M., Deng, M., Wang, X., Weng, X., Zhou, X., 2011. *Chem. Commun.* 47, 1273–1275.
- Yang, C., Wang, Y., Marty, J.L., Yang, X.R., 2011. *Biosens. Bioelectron.* 26, 2724–2727.
- Zhang, J., Wang, L.H., Pan, D., Song, S.P., Boey, F.Y.C., Zhang, H., Fan, C.H., 2008. *Small* 4, 1196–1200.
- Zhao, J., Chen, G.F., Zhu, L., Li, G.X., 2011. *Electrochem. Commun.* 13, 31–33.
- Zhao, Q., Gao, J., 2013. *Chem. Commun.* 49, 7720–7722.
- Zheng, Y., Wang, Y., Yang, X.R., 2011. *Sens. Actuators, B* 156, 95–99.
- Zhu, H., Klemic, J.F., Chang, S., Bertone, P., Casamayor, A., Klemic, K.G., Smith, D., Gerstein, M., Reed, M.A., Snyder, M., 2000. *Nat. Genet.* 26, 283–289.
- Zuo, X., Song, S., Zhang, J., Pan, D., Wang, L., Fan, C., 2007. *J. Am. Chem. Soc.* 129, 1042–1043.