

Erratum

Corrigendum to “Electrochemical biosensor for Mycobacterium tuberculosis DNA detection based on gold nanotubes array electrode platform” [Biosensors and Bioelectronics 78 (2016) 483-488]




Sri Ramulu Torati^a, Venu Reddy^{a,b}, Seok Soo Yoon^c, CheolGi Kim^a

^a Department of Emerging Materials Science, DGIST, Daegu, 711-873, Republic of Korea

^b School of Engineering Science and Technology, University of Hyderabad, Gachibowli, Hyderabad-500046, India

^c Department of Physics, Andong National University, Andong 760-749, Korea

We are sorry to inform that there is a technical error need to be revised: the ng/mL should be revised to ng/μL in inset of Fig. 5b. The corresponding Figure (Fig. 5b) should be replaced. The corrected Fig.5b is given below. The authors would like to apologize for any inconvenience caused.

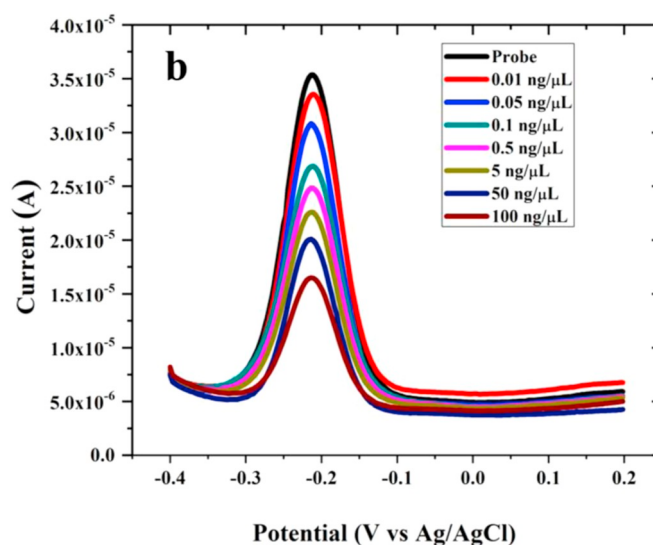

DOI of original article: <https://doi.org/10.1016/j.bios.2015.11.098>

<https://doi.org/10.1016/j.bios.2018.11.024>