

Accepted Manuscript

Scanning electrochemical microscopy imaging of poly (3,4-ethylenedioxythiophene)/thionine electrodes for lactate detection via NADH electrocatalysis

Susan Warren, Grigore Munteanu, Dhanraj Rathod, Timothy McCormac, Eithne Dempsey



PII: S0956-5663(19)30333-1

DOI: <https://doi.org/10.1016/j.bios.2019.04.042>

Reference: BIOS 11274

To appear in: *Biosensors and Bioelectronics*

Received Date: 23 January 2019

Revised Date: 8 April 2019

Accepted Date: 21 April 2019

Please cite this article as: Warren, S., Munteanu, G., Rathod, D., McCormac, T., Dempsey, E., Scanning electrochemical microscopy imaging of poly (3,4-ethylenedioxythiophene)/thionine electrodes for lactate detection via NADH electrocatalysis, *Biosensors and Bioelectronics* (2019), doi: <https://doi.org/10.1016/j.bios.2019.04.042>.

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

Scanning electrochemical microscopy imaging of poly (3,4-ethylendioxythiophene)/thionine electrodes for lactate detection via NADH electrocatalysis

Susan Warren^{ia}, Grigore Munteanu^a, Dhanraj Rathod^{ia}, Timothy McCormac^b, Eithne Dempsey^{c*}.

^a *Centre of Applied Science for Health (CASH), TU Dublin - Tallaght Campus, Dublin 24, Ireland.*

^b *Dundalk Institute of Technology, Dundalk, Co. Louth, Ireland.*

^c *Department of Chemistry, Maynooth University, Maynooth Co. Kildare, Ireland*

* Corresponding author. Tel.: +353 4747172; eithne.dempsey@mu.ie

Abstract

Herein we report the use of scanning electrochemical microscopy (SECM) together with electrochemical and spectroscopic techniques to develop and characterise a stable and uniformly reactive chemically modified platinum electrode for NADH electrocatalysis. In order to achieve this, a range of different approaches for thionine entrapment within an electropolymerised poly(3,4-ethylendioxythiophene) (PEDOT) film were evaluated using SECM imaging in the presence of NADH, demonstrating the uniformity of the reactive layer towards NADH oxidation. The effect of electrolyte type and time scale employed during PEDOT electropolymerisation was examined with respect to thionine loading and the resulting charge transport diffusion coefficient (D_{CT}) estimated via chronoamperometry. These studies indicated a decrease in D_{CT} as thionine loading increased within the PEDOT film, suggesting that charge transport was diffusion limited within the film. Additionally, thionine functionalised nanotubes were formed, providing a stable support for lactate

dehydrogenase entrapment while lowering the rate of thionine leaching, determined via SECM imaging and enabling lactate determination at $E_{app} = 0.0$ V vs Ag/AgCl over the range 0.25-5 mM in the presence of 1 mM NAD^+ .

Keywords: Thionine, poly-3,4-ethylenedioxythiophene (PEDOT), multiwalled carbon nanotubes (MWNT), lactate biosensor, lactate dehydrogenase (LDH), scanning electrochemical microscopy (SECM), charge transport studies.

Present addresses

Dhanraj Rathod, Cefa-Cilinas Biotics Pvt Ltd, Aurangabad, Maharashtra, India.

Susan Warren, TU Dublin - City Centre Campus, Kevin Street
Centre for Research in Engineering Surface Technology (CREST)
FOCAS Research Institute, Dublin Institute of Technology, Kevin Street, Dublin 8, Ireland

Keywords

Scanning electrochemical microscopy, PEDOT, thionine, charge transport, lactate detection, NADH catalysis.

1. Introduction

More than 400 dehydrogenase enzymes catalyse reactions in the presence of their cofactor, nicotinamide adenine dinucleotide (NAD^+) or nicotinamide adenine dinucleotide phosphate (NADP^+), which act as the electron and hydrogen acceptor in the reaction catalysed by the enzyme to generate the reduced NAD(P)H coenzyme [1]. Direct electrochemical oxidation of NAD(P)H is achievable on bare electrodes, however its high overpotential can lead to undesirable side reactions and is subject to interferences from electroactive materials within a sample matrix (ascorbic and uric acids). Many organic mediators have been investigated to help overcome this, the majority of which possess a quinone or phenyldiimine structure. Examples of such materials include organic dyes e.g. Meldola's Blue [2-5], methylene green/ blue [6,7] Nile Blue A [8], Prussian Blue [9,10] and thionine [11-14]. One of the main issues with these redox active dyes is their high water solubility, which causes them to readily diffuse from their immobilised state at the electrode surface into the bulk solution. In addition to ease of surface attachment and stability, ensuring facile charge transport between immobilised redox sites is important such that the whole redox film contributes to NADH oxidation [15].

There have been some reports of non-covalent modification of carbon nanotubes with functional molecules such as NAD^+ [16] and thionine [17]. The positive charge of these molecules in solution enables adsorption onto nanotube walls via π - π stacking interactions and so anchors the mediator to a stable support material. Prevention of aggregation and improved solubilisation of nanotubes has been an area of significant interest and has obtained some success via attachment of polymers [18], and ionic

modification with dispersion with surfactants [19]. Bandyopadhyaya *et al.* [20] presented an alternative to these approaches through non-specific physical adsorption of the biopolymer Gum Arabic, and proposed the use of a 0.5-15% wt solution which allows for a stable aqueous suspension of full length tubes, which can be dried and resuspended with ease. The application of conducting polymers as an immobilisation matrix for redox materials and biological components has achieved much attention [21-25] and recent reports regarding the use of PEDOT describe the immobilisation of catechin [26] and 4-phenyl azo aniline [27] for the electrooxidation of NADH. Balamurugan *et al.*, [28] describe a PEDOT coated electrode modified with silver nanoparticles and Meldola's Blue for NADH detection with minimal interference of electroactive compounds.

Scanning electrochemical microscopy (SECM) has been proven experimentally to be a very versatile technique for the visualisation of localised chemical and electrochemical activity within surface confined films and is the subject of recent reviews [29-31]. It is based on a scanning microelectrode in close contact with a surface of interest with current dependant on local concentration of electroactive species, realising electron transfer kinetics, high resolution imaging and topography examinations [32]. SECM can pattern the substrate surface, visualise its topography and prove chemical reactivity on the μm or nm scale [33].

Unlike STM and AFM tips which are sharp cones, a typical SECM tip is a conductive disk surrounded by a flat ring of insulating glass. This ultramicroelectrode (UME), capable of moving in x, y and z directions, is positioned very close to an interface, and can be used to investigate the topography, reactivity or permeability of that

surface with high spatial resolution [34]. The tip can induce chemical changes and collect electrochemical information while approaching or scanning the surface of interest, which can be biased, serving as the second electrode [33].

Studies of redox enzymes commonly utilise either feedback or generation/collection modes, both tip and substrate currents being measured in the latter case. In Substrate Generation – Tip Collection (SG-TC) mode, the tip probes reactions that occur at a substrate, which is held at a constant potential while the tip travels within a thick diffusion layer generated by the substrate electrode. When scanning in the x/y direction over the substrate, the tip can identify hot spots where reactions occur at higher rates [35]. In this mode, an enzyme causes regeneration of a mediator species, which is consumed at the ultramicroelectrode and the rate of the enzyme reaction is transduced into current measured by the SECM. The magnitude of the feedback response depends on the rate at which the enzyme catalytically regenerates the bulk form of the species [36].

The theory and experimental applications of SECM – induced transfer (SECMIT) has been described by Barker *et al.* [37], as an approach for probing partitioning of electroactive solutes between two immiscible phases. The equilibrium is perturbed by electrolysis of the target species at the UME tip which is placed close to the interface with the second phase. Gonsalves *et al.* [38] have employed the induced transfer (SECMIT) mode of SECM to image the permeability of methyl viologen in articular cartilage. By scanning the UME over the sample surface, detection of methyl viologen was performed amperometrically via the UME.

Prior work in our group has reported a Thionine/PEDOT catalytic layer for NADH oxidation [39]. Here we advance the work with exploitation of thionine functionalised carbon nanotubes (MWNTs) using Gum Arabic as suspension reagent, in order to limit leaching of thionine from the electrode surface and to further exploit amine functionalities as a linker group for enzyme attachment. The characterisation and performance of thionine modified carbon nanotubes as a support for the stabilisation of thionine on the electrode surface and for the fixation of lactate dehydrogenase is examined here for the first time, realising successful lactate detection. Complementary electrochemical characterisation and SECM imaging evaluate the films via different modes, SECMIT and Substrate Generation-Tip collection (SG-TC), allowing for optimisation of the immobilisation method in terms of thionine uniformity, reactivity and stability.

2. Experimental

2.1. *Instrumentation and Reagents*

All electrochemical experiments were carried out on a CHI 1030 or CHI 660a electrochemical workstation (CH Instruments). A single-compartment electrochemical cell was used with platinum counter electrode and a saturated Ag/AgCl reference for aqueous solutions. Working electrodes were 3 mm diameter platinum discs. SECM analysis was carried out using a CHI920 bipotentiostat / SECM equipped with an adjustable stage for tilt correction. The tip electrodes used were 10 and 25 μm platinum microelectrodes obtained from CH Instruments. RG values of 5-10 were calculated based on $RG = r_g/a$ where r_g is the outer radius of the insulating sheath and a is the microelectrode radius. UV Spectroscopy was carried out on a T80 UV-Visible spectrometer - PG Instruments. SEM analysis was performed

using a Joel LV-6390. 3,4-ethylene dioxythiophene/EDOT, LiClO₄, sodium *p*-toluene sulphonate, thionine acetate, ethanol, nitric acid, multiwall carbon nanotubes, Gum Arabic, NADH, NAD⁺, lactate dehydrogenase 579 units/mg (USB), 25% glutaraldehyde, sodium lactate, ferrocene methanol, phosphate buffered saline (pH 7.4) were received from Sigma Aldrich and used as received unless otherwise specified.

2.2. Procedures

2.2.1. Preparation of Thionine Modified Functionalised Multiwalled Carbon Nanotubes (Th-fMWNT's)

100 mg of multiwalled carbon nanotubes (MWNTs) were sonicated in deionised water for 30 minutes, followed by filtration through a polycarbonate membrane. The solid was washed several times with deionised water, ensuring the filtrate was clear. The washed solid was then refluxed in 10% HNO₃ at 80°C for 24 hrs with vigorous stirring. The acid solution was filtered through a hydrophobic PTFE (polytetrafluoroethylene) membrane, followed by washing with deionised water and acetone several times. The acid functionalised MWNT's (fMWNTs) were then dried at 110 °C for 12 hrs under vacuum. 2 mg of fMWNT were suspended in 2 cm³ deionised water with the aid of mild sonication (400 W). 100-150 µM thionine was added to the suspension and shaken for *ca.* 2 minutes until the solution turned clear and the nanotubes fell out of suspension, indicating absorption of thionine onto the nanotubes. Gum Arabic was added to the solution to a final concentration of 1% and sonication was carried out to re-suspend the modified nanotubes, denoted Th-fMWNT.

2.2.2. Lactate Dehydrogenase attachment to Th-fMWNT (LDH-Th-fMWNT)

7.6 μl of 2.5% glutaraldehyde was added to a stable suspension of Th-fMWNT's (2 cm^3) and stirred for 1 hour to activate the amine groups on the thionine. Meanwhile lactate dehydrogenase was dissolved in 2 cm^3 PBS and mixed with the Th-fMWNT / glutaraldehyde solution. Stirring was maintained for a number of hours at room temperature and the solution was maintained at $4\text{ }^\circ\text{C}$ overnight. Modification of Pt electrodes with this material was achieved by depositing $5\text{ }\mu\text{L}$ of the solution onto the surface of the electrode and allowing it to air dry for ~ 30 minutes.

2.2.3. Electrochemical Procedures

Pt electrodes were cleaned by polishing with alumina slurries (1, 0.5 and $0.05\text{ }\mu\text{m}$) with washing and gentle sonication in between each grade. Prior to polymer deposition the electrode was electrochemically activated in $0.5\text{ M H}_2\text{SO}_4$ via potential cycling between $-1.5 - +1.5\text{ V}$ vs. Ag/AgCl with stirring, followed by holding the electrode at -1.5 V vs. Ag/AgCl for 900 s, with stirring.

2.2.3.1 Formation of Thionine-PEDOT and PEDOT/Thionine films

Thionine-PEDOT films were prepared as described previously [39]. Briefly, films were formed from 10 mM thionine acetate, 15 mM EDOT in 10 mM LiClO_4 via chronocoulometry (5 mC charge passed at $E_{\text{APP}} 1.2\text{ V}$ vs. Ag/AgCl).

In the case of PEDOT/Thionine and PEDOT/Th-fMWNT films an activated Pt electrode was modified with PEDOT using chronocoulometry to form a 79.6 mC.cm^{-2} film - $E_{\text{APP}} +1.2\text{ V}$ vs Ag/AgCl from a solution of 10 mM EDOT aqueous solution with 0.1 M electrolyte. Thionine was then incorporated into this film by placing the PEDOT modified electrode in a 0.5 mM aqueous thionine solution and holding the

applied potential at -0.5 V vs. Ag/AgCl for various time periods (15 to 90 min). The electrode was then rinsed with deionised water prior to use. For inclusion of Th-fMWNT, the same procedure was followed, where a stable suspension of the Th-fMWNT's replaced the thionine solution.

2.2.3.2. Charge Transport Diffusion Coefficient (D_{CT}) Determination by Chronoamperometry

The PEDOT/Thionine modified (Pt) electrodes were analysed in PBS pH 7.4. The electrodes were first subjected to potential cycling at 0.1 V.s^{-1} ($-0.7 \rightarrow +0.4$ V vs. Ag/AgCl, for 25 cycles) and then 5 mV.s^{-1} for 3 cycles (over the same range) to ensure any loosely bound thionine was removed from the electrode surface, and that stable currents were obtained. Two sets of potentials were determined from the stable CV. For background measurements, the potentials were chosen where no redox reaction occurs, i.e. potentials prior to oxidation and following the reduction wave; normally -0.7 to -0.6 V vs. Ag/AgCl. This single step measurement was carried out 5 times and an average current obtained. For the actual measurements, the potential was stepped from a region prior to thionine oxidation i.e. -0.7 V vs. Ag/AgCl, to a region where the current was diffusion controlled, typically $+0.35$ V vs. Ag/AgCl. This current measurement was taken 5 times and averaged. Background subtraction was then applied to the averaged results.

2.2.4. Film Preparation on ITO Slides - UV Analysis

ITO slides were cleaned with IPA, followed by soaking in 10% NaOH at 55°C for 3 minutes, after which the slides were rinsed with deionised water and dried to ensure no water marks were present prior to use. Cleaned slides were stored in ethanol until

use, with adequate rinsing with deionised water and drying prior to use. A specific area ($\sim 1 \text{ cm}^2$) was marked off using masking tape to allow for accurate film measurements. Once the films were formed on the surface as described above, the modified slides were soaked in deionised water until the leaching of loosely bound thionine had ceased. The films were then allowed to dry under ambient conditions and then stored in the dessicator overnight, or until their use.

2.2.5. SECM Procedures

2.2.5.1. Modification of SECM Tip Electrode for Imaging of Enzyme Substrate

A 25 μm Pt tip electrode was scanned in a solution of ferrocenemethanol to ensure that the expected electrochemical response was achieved. If deemed necessary the tip electrode was activated in 0.5 M H_2SO_4 as described in section 2.2.3. The tip was then modified with a PEDOT film as described above (2.2.3.1), following which Th-fMWNT was incorporated over a 2 hour time frame by cathodic constant potential deposition at $E_{\text{app}} = -0.5 \text{ V vs. Ag/AgCl}$ (PEDOT/Th-fMWNT).

2.2.5.2. SECM Substrate Generation – Tip Collection (SG-TC) Imaging for NADH Reactivity

The PEDOT/Thionine layer under investigation was deposited onto the Pt substrate electrode ($d=2 \text{ mm}$), rinsed to remove any unbound thionine and inserted into the SECM cell. The unmodified tip electrode was a 25 μm Pt microelectrode (cleaned and activated as above) and was placed into the tip holder so as to barely touch the substrate electrode and then withdrawn a safe distance ($z / \mu\text{m}$) in order not to touch the film during imaging. Imaging was carried out at a rate of $500 \mu\text{m.s}^{-1}$ for all images.

The substrate electrode was maintained at the reduction potential of the thionine in the PEDOT film (-0.2 V vs Ag/AgCl) while the tip (+0.1 V vs Ag/AgCl) played the role of generating oxidised thionine sites thus triggering NADH electrocatalysis (Scheme 1 (a)) using substrate generation-tip collection mode.

2.2.5.3. Induced transfer (SECMIT) mode imaging for Thionine Film Stability

The PEDOT/Thionine layer under investigation was deposited onto the Pt substrate electrode (d=2 mm), rinsed well to remove any unbound thionine and inserted into the SECM cell. The unmodified tip was placed into the tip holder so as to barely touch the substrate electrode and then withdrawn a safe distance ($z / \mu\text{m}$) in order not to touch the film during imaging. Imaging was performed at a rate of $500 \mu\text{m.s}^{-1}$ in all cases. The substrate electrode was maintained at the reduction potential of the thionine/PEDOT film (-0.5 V vs Ag/AgCl) while the tip was held at the oxidation potential (+0.4 V vs Ag/AgCl). (Scheme 1 (b)) so as to enable detection of leached thionine from the substrate modified film (PEDOT/Thionine).

2.2.5.4. SECM Substrate Generation – Tip Collection (SG-TC) Imaging of NADH

Generation at Lactate Dehydrogenase Modified Electrode

The modified (PEDOT/Th-fMWNT) tip electrode was prepared as described above, while the substrate electrode was modified with 10 μL of the enzyme-Th-fMWNT mixture (prepared according to section 2.2.2) and air dried for 1 hour. Imaging was carried out initially in 1 mM NAD^+ /PBS pH 7.4, $E_{\text{SUBSTRATE}}$: OFF E_{TIP} : +0.3V vs. Ag/AgCl. 5 mM Lactate was added to solution and the image repeated to detect the NADH generated at the tip electrode (Scheme 1 (c)). This mode generated catalytic signals associated with substrate generated NADH at a thionine modified tip, thus

enabling the lactate dehydrogenase enzyme layer reactivity to be imaged in the presence of enzyme substrate (lactate).

2.2.6. UV Analysis – Determination of Thionine Concentration in PEDOT films

UV-visible spectroscopy was performed using aqueous solutions of thionine (10 – 70 μM in PBS pH 7.4) and the molar extinction coefficient (ϵ 22814 $\text{M}^{-1}\cdot\text{cm}^{-1}$) calculated and used to determine thionine concentration within the PEDOT films. UV analysis of the PEDOT/Thionine films was achieved using a PEDOT film as background in order to eliminate any interference from the UV absorption of the PEDOT film itself.

2.2.7. Scanning Electron Microscopy Analysis

PEDOT/Th-fMWNT films were prepared on Pt electrodes as described in section 2.2.3.1. rinsed well with deionised water and dried overnight. The electrodes were analysed dry without sputter coating using an accelerating voltage of 5 kV.

3. Results and Discussion

3.1. Formation of Thionine-PEDOT and PEDOT/Thionine Films

These electrodes were prepared as described above (2.2.3.1) where thionine was incorporated into a PEDOT film both (a) during [Thionine/PEDOT] and (b) following [PEDOT/Thionine] electropolymerisation at Pt electrodes. In the case of the former (a), the thionine concentration must be sufficiently high such that PEDOT polymerisation is hindered, enabling sufficiently high thionine loading to be realised. Thionine has a tendency to form aggregates in solution if the concentration is too high [40], which can influence film reproducibility and performance. This approach (a) is

based on prior work in our group [39] which generated an NADH electrocatalytic layer with subsequent glutamate detection (at glutamate dehydrogenase modified electrodes). Further optimisation of this immobilisation approach was deemed necessary in order to improve thionine loading and uniformity (hence approach (b) as outlined below). The assistance of scanning probe electrochemical methods and charge transport investigations also enabled successful lactate biosensing at a lactate dehydrogenase modified electrode (LDH-Th-fMWNT).

Incorporation of thionine into a PEDOT film following electropolymerisation [PEDOT/Thionone (b)], via the subsequent application of a reduction potential (-0.5 V vs. Ag/AgCl) in the presence of 0.5 mM thionine allowed for better control of thionine loading. The thickness of the PEDOT layer was critical in that it must be sufficient to give uniform coverage of the electrode area and be capable of retaining a suitable volume of thionine, but not so thick so as to hinder charge transport to the electrode surface. Thionine loading using this approach can be controlled using the timescale of the experiment at thionine concentrations where aggregation is eliminated. A comparison of the electrochemistry of two such films indicated enhanced thionine redox activity in the case of the film formed by incorporation of thionine following PEDOT formation via chronocoulometry [PEDOT/Thionine]. Voltammetric responses (data not shown) resulted in $E_{p(a)} = -0.02$ V and $E_{p(c)} = -0.5$ V with $\Delta E_p = 0.43$ V and $E_{1/2} = -0.215$ vs. Ag/AgCl for the 2 electron 1 proton process at pH 7.4 (scan rate 0.1 Vs^{-1}).

3.2. Reactivity of PEDOT/Thionine films by SECM Imaging with NADH in Solution

Films were analysed using SECM (at a 25 μM Pt tip electrode) in the presence of 1 mM NADH in order to determine the uniformity of the reactive layer on the electrode surface (Format (a) in Scheme 1). The considered mechanism for this process is that the tip is close enough to the modified surface in order to influence the regeneration of the oxidised form of thionine and detect enhanced currents associated with the catalytic interaction of thionine (ox) and NADH at the substrate modified PEDOT/Thionine layer).

Figure 1 (a, b) shows SECM images of the redox films formed by the two different immobilisation methods, (a) where thionine was incorporated during PEDOT polymerisation [39] and (b) where the thionine was incorporated following PEDOT formation (as described above). It was apparent that method (b) produces a more uniformly reactive film with almost an order of magnitude higher (3.95×10^{-10} A) anodic response relative to that of (a) (5.55×10^{-11} A). All films discussed from this point onwards were prepared using method (b) as described above in section 2.2.3.1.

3.3. Influence of electrolyte type and polymerisation potential on PEDOT Formation and Thionine Inclusion

Dopant anions employed during the electropolymerisation procedure can have a profound effect on the resulting polymer. Smaller dopant anions can result in a denser polymer framework while the incorporation of larger anions can generate a more porous polymer structure [41]. In this work the effect of using both *p*-toluenesulphonate and perchlorate as the dopant anions during PEDOT electropolymerisation was investigated. These films were analysed in terms of their ability to effectively 'load' thionine. As expected, when *p*-toluene sulphonate was

used for PEDOT polymerisation, the time required to achieve maximum loading time (at $E_{APP} = -0.5$ V) from a 0.5 mM thionine solution increased from 45 minutes (in the case of ClO_4^-) up to 75 minutes for the larger anion (sodium *p* – toluene sulphonate). These results support the idea that the larger the dopant anion the more porous the film and therefore a longer time is required to obtain a stable saturation thionine film concentration. Figure 1(c) shows a comparison of cyclic voltammograms of PEDOT/Thionine films prepared in the presence of (a) perchlorate, and (b) *p*-toluene sulphonate, following 45 minutes thionine inclusion time (at -0.5 V vs. Ag/AgCl in 0.5 mM thionine). Results indicated that the thionine oxidation and reduction peaks were more evident in the case of the sodium *p* –toluene sulphonate film and resulted in a smaller ΔE_p (104 mV vs. 228 mV) relative to films formed from LiClO_4 . Therefore 0.1 M sodium *p* –toluene sulphonate was chosen as the preferred electrolyte for further PEDOT electropolymerisation studies. The effect of PEDOT electropolymerisation potential was also investigated during chronocoulometric film formation. As expected, when E_{APP} was reduced from +1.2 to + 0.8 V vs. Ag/AgCl, the time taken to obtain 79.6 mC.cm^{-2} increased significantly. No dramatic difference in thionine loading between the films formed at different potentials was observed, and therefore the optimum, +1.2 V vs. Ag/AgCl was employed for all film formation.

3.4. UV-Visible Spectroscopic Analysis of PEDOT/Thionine Films

UV spectra were obtained for an aqueous solution of thionine (0.5 mM), and each PEDOT/Thionine film prepared on ITOs as per section 2.2.4 using either LiClO_4 or *p*-toluene sulphonate electrolyte. Free thionine showed a sharp band at λ_{max} 600 nm (α band) attributed to the monomeric form, and a shoulder at 560 nm (β band) which may be attributed to higher aggregates of thionine [42-43]. For the PEDOT/Thionine

films formed on ITOs the λ_{max} was observed at 570 nm, attributable to the large thionine aggregation within the film with higher wavelength signal at 620 nm. The absorbance ratios of the two signals for the ITO loaded films were close to 1:1 or 0.51:0.49 (and did not change upon varying thionine concentration), whereas for the solution of free thionine the absorbance ratios were 0.4:0.6 (560:600 nm), which based on prior reports, implies that the red shift of the band at 600 nm may be attributed to oligomer formation via electron releasing groups (NH_2 pendant groups) and the proposed N-C coupling forming nitrogen bridges between monomer units [40,44]. A similar red shift of 10 and 20 nm (respectively) was evident in our system in the case of both peaks.

3.5. Effect of thionine loading on D_{CT} values obtained via chronoamperometry.

PEDOT films were loaded with thionine as per section 2.2.3.1 over time periods 15-90 min in order to determine the optimum/maximum thionine incorporation time. Chronoamperometric measurements were carried out to determine the D_{ct} values for each film in PBS electrolyte. ITO slides were prepared in parallel and analysed using UV-visible spectroscopy to measure the thionine concentration with respect to loading time. Table 1 (A) shows that thionine concentration within the PEDOT/ $LiClO_4$ film increases up to 45 minutes and then starts to decrease. Therefore 45 minutes was taken as the maximum loading time for these films. Table 1(B) shows the corresponding data for PEDOT/sodium p-toluene sulphonate films indicating that an increase in thionine concentration with time occurred up to 75 minutes, after which time it started to decrease. The main contrast between Tables 1a) and b) is that thionine concentration shows a greater variation with loading time in the case of the PEDOT/ $LiClO_4$ films. The PEDOT/ sodium p-toluene sulphonate films show almost

70% loading after only 15 minutes, in comparison to only 38% with the PEDOT/LiClO₄. Both films exhibit similar thionine concentrations and comparable D_{CT} values.

Both films demonstrate a dramatic decrease in D_{CT} as the thionine loading increases. This trend suggests a principal role of physical diffusion of the redox species in charge transport through the film, which would be evidence of a reduced mobility at high surface concentration [45-47]. From this observation, the mechanism of charge transport can be considered as diffusion. These results are in agreement with a previous report by Guadalupe *et al* [42], where the charge transport properties of thionine and other cationic dyes within a Nafion film were investigated. In comparison to this reported work, the D_{ct} values for our system are higher ($18.9 - 364 \times 10^{-9} \text{ cm}^2 \cdot \text{s}^{-1}$ in comparison to $1.4 - 28 \times 10^{-9} \text{ cm}^2 \cdot \text{s}^{-1}$). This improvement could be attributed to the use of the conducting polymer, PEDOT. It is worth noting that the PEDOT/NapTS film presents a higher D_{CT} at maximum loading than its counterpart, 3.4×10^{-8} vs. $1.8 \times 10^{-8} \text{ cm}^2 \cdot \text{s}^{-1}$, suggesting that the PEDOT/sodium *p*-toluene sulphonate counterion framework allows for better diffusion of thionine within the film. Film studies from this point onwards refer to PEDOT films prepared with sodium *p*-toluene sulphonate and subsequently loaded with thionine.

3.6. Characterisation of Thionine-Modified fMWNTs

Previous work in our group [39] demonstrated that incorporation of nanotubes into the sensor design enhanced performance of the resulting glutamate dehydrogenase biosensor. By modifying MWNT with thionine using an approach similar to that of Wang *et al* [17], and then by incorporating them into a preformed PEDOT film (0.1

M sodium p-toluene sulphonate), successful immobilisation of Th-fMWNT onto the electrode surface was achieved. SEM images of PEDOT/Thionine films are non-descript polymer films that have no distinct characteristic features. Figure 2(a) and (b) shows the SEM images of the PEDOT/Th-fMWNT films for 1 and 2 hour loading times. As is evident from these images, the polymer films exhibit a ‘grainy’ surface structure, which increases from 1 to 2 hours loading time. This ‘grainy’ topography is attributed to the Th-fMWNT’S being incorporated into the PEDOT film.

3.7. Stability study for PEDOT/Th and PEDOT/Th-fMWNT films using SECMIT Imaging

SECMIT imaging of PEDOT/Th and PEDOT/Th-fMWNT films was carried out by effectively monitoring the leaching of thionine from the film under investigation. Desorption was examined by rastering the tip electrode over the modified substrate electrode while subjecting it to a cathodic potential. Desorbed thionine can diffuse to the UME tip where it is oxidised, contributing to the tip current [48] from the substrate. This procedure was repeated, monitoring the decrease in thionine from the film over time (working solutions were changed in between each image to minimise interference). Figure 3 shows images of this process for (a) PEDOT/Thionine film and (b) PEDOT/Thionine-fMWNT film over a continuous imaging period of 1.5 – 6.5 hours. As the imaging time increases, depletion of thionine was observed to be more significant in the case of the PEDOT/Thionine film as the brown electroactive layer becomes the green depleted area of the electrode. Imaging after 6.5 hours showed no thionine response for the PEDOT/Thionine film, while the PEDOT/Th-fMWNT still exhibited a thionine signal up to and longer than 9 hours imaging time. As expected, PEDOT/Th-fMWNT films leach thionine at a slower rate relative to PEDOT/Thionine

films, due to the thionine being adsorbed in a more stable fashion onto the MWNT scaffold.

3.8. *SECM Analysis of Lactate dehydrogenase mounted on a solid support of Th-fMWNT.*

Thus far we have demonstrated a novel immobilisation method of thionine into a preformed PEDOT polymer and have extended this methodology to incorporate thionine-modified MWNTs. Next, the biocatalyst lactate dehydrogenase (LDH) was partially crosslinked to Th-fMWNT using glutaraldehyde according to the procedure in 2.2.2. In the presence of 1 mM cofactor NAD^+ , the substrate (lactate) was oxidised by the biocatalyst to pyruvate with formation of NADH, being then re-oxidised by the immobilised thionine layer. Increased anodic thionine signals at 0.0 V were monitored in response to increasing lactate additions (0-50 μM) (the mechanism is based on that proposed previously by our group [39]). By monitoring the thionine film response to lactate additions an increased catalytic current was evident which corresponds to re-oxidation of the reduced NADH enzyme cofactor.

Figure 4(a) shows a cyclic voltammogram of the LDH-Th-fMWNT deposited directly onto the surface of a glassy carbon electrode, with inset calibration plot for lactate additions in the presence of 1 mM NAD^+ , E_{APP} 0.0 V vs Ag/AgCl. The calibration curve of lactate, is linear with respect to $(\text{conc.})^{1/2}$ with sensitivity 20.86 $\text{nA mM}^{-1/2}$, standard deviation 13.8 ($n=3$) over the range 0.5 -5 mM. Hence, this demonstrates some heterogeneity of the developed electrode which can be attributed to the effect of cross linking of the enzyme by glutaraldehyde and thionine, as previously reported by Juang *et al.* [49]. Analytical response to NADH alone

resulted in sensitivity $3.71 \pm 0.3145 \text{ nA mM}^{-1}$ ($n=3$) with LOD of $0.186 \mu\text{M}$ and r^2 of 0.9995. The low operating voltage ($E_{\text{app}} = 0.0 \text{ V}$ hydrodynamic amperometry) ensures minimal interference from electroactive species and from direct NADH surface oxidation signals.

SECM was then used to examine the enzyme activity of the enzyme deposit layer. Due to the high overpotential platinum towards NADH produced from the active LDHase enzyme in the presence of lactate, we opted to modify the tip electrode with a NADH sensitive layer - the stabilised PEDOT/Th-fMWNT film. The data presented in Figure 4(b), in addition to that shown in Figure 4(a), proves the analytical applicability of the developed electrode. The average current density of the substrate electrode in the presence of 5 mM lactate increases 2 fold, from $3.7 \mu\text{A.cm}^{-2}$ in the absence of lactate, to $7.0 \mu\text{A.cm}^{-2}$ when lactate is added to the system. It should be noted that the data presented in Figure 4(b) was obtained in conditions far from that optimal for SECM imaging (distance, z , between the tip and the substrate electrodes was chosen as $800 \mu\text{m}$ to avoid direct contact between these electrodes). Under these conditions, activity of the substrate electrode with respect to lactate concentration is comparable with the activity of the electrode used for registration of the lactate calibration curve (inset Figure 4(a)). The calculated value of current density for 5 mM lactate is approximately equal to $8 \mu\text{A.cm}^{-2}$. Consequently, the efficiency of the “generation-collection” mode of SECM using a tip electrode modified by the same film as the substrate electrode is close to 50%, which also confirms the analytical applicability of the developed electrode. Figure 4(b), shows the increase in current generated after lactate is added to the system, confirming the activity of the enzyme on the thionine-fMWNT support. This experiment demonstrates the ability of the

thionine-fMWNT material to act as an electrocatalyst for NADH oxidation as well as a 'scaffold' for the attachment of dehydrogenase enzymes.

4. Conclusions

We have demonstrated a novel immobilisation method for thionine and thionine functionalised nanotubes, entrapped in a preformed PEDOT polymer film, examined with respect to surface electrochemical interrogation tools (SEM and SECM) and deployed in relation to lactate biosensing at a lactate dehydrogenase/thionine loaded modified electrode.

- (a) Charge transport studies of thionine doped PEDOT films deduce that the mechanism of charge transport within the film was predominantly diffusion, as interpreted from the dramatic decrease in D_{CT} as the thionine loading within the film increased. D_{CT} values were of the magnitude $36.4 \times 10^{-8} - 1.9 \times 10^{-8} \text{ cm}^2 \cdot \text{s}^{-1}$ and $12.8 \times 10^{-8} - 3.43 \times 10^{-8} \text{ cm}^2 \cdot \text{s}^{-1}$ for PEDOT-Thionine films grown in the presence of lithium perchlorate and sodium *p*-toluene sulphonate respectively.
- (b) SECM – induced transfer mode was employed as a tool to monitor the leaching of thionine from the PEDT/Thionine films over time, resulting in the conclusion that thionine stability was enhanced using Th-fMWNT (prepared via electrostatic loading of thionine onto activated MWCNTs).
- (c) It was also demonstrated that the Th-fMWNT can be used as a solid support for dehydrogenase enzymes through partial crosslinking of the respective thionine functional (amine) groups with lactate dehydrogenase. The resulting electrode was shown to be analytically applicable through the use of standard electrochemical techniques, CV and hydrodynamic amperometry.

(d) SECM experiments at the enzyme modified substrate electrode showed a two-fold increase in current density ($8 \mu\text{A}\cdot\text{cm}^{-2}$) when 5 mM lactate was added to the system in the presence of 1 mM NAD^+ . Analytical applicability of the developed sensor was also confirmed by the efficiency of the ‘generation-collection’ mode of SECM being close to 50%.

Further work has the potential to expand the range of dehydrogenase systems under examination together with a kinetic evaluation of enzyme loaded films with the aid of suitable SECM quantitative and imaging modes.

Acknowledgements

The authors acknowledge the Programme for Research in Third Level Institutions Cycle 4, Higher Education Authority for the financial support to carry out this work.

References

- [1] Z. Jing-Li, N. Ping-Ping, Z. Hai-Tao, Z. Ji-Mei, Progress of Electrochemical Biosensors based on Nicotinamide Dinucleotide(phosphate)-Dependent Dehydrogenases, Chinese Journal of Analytical Chemistry 37 (2009) 617-623.
- [2] C.M. Maroneze, L.T. Arenas, R.C.S. Luz, E.V. Benvenutti, R. Landers, Y. Goshikem, Meldola Blue immobilized on a new $\text{SiO}_2/\text{TiO}_2$ /graphite composite for electrocatalytic oxidation of NADH, Electrochimica Acta 53 (2008) 4167-4175.
- [3] A. Vasilescu, T. Noguer, S. Andreescu, C. Calas-Blanchard, C. Bala, J.-L. Marty, Strategies for developing NADH detectors based on Meldola Blue and screen-printed electrodes: a comparative study, Talanta 59 (2003) 751-765.

- [4] A. Vasilescu, S. Andrescu, C. Bala, S.C. Litescu, T. Noguer, J.-L. Marty, Screen-printed electrodes with electropolymerized Meldola Blue as versatile detectors in biosensors, *Biosensors and Bioelectronics* 18 (2003) 781-790.
- [5] B. Prieto-Simón, J. Macanás, M. Muñoz, E. Fàbregas, Evaluation of different mediator-modified screen-printed electrodes used in a flow system as amperometric sensors for NADH, *Talanta*, 71 (2007), 2102–2107.
- [6] R. A. Rincon, K. Artyushkova, M. Mojica, M. N. Germain, S. D. Minter, Structure and Electrochemical Properties of Electrocatalysts for NADH Oxidation, *Electroanalysis* 2010 , 22, No. 7-8, 799 – 806.
- [7] E. Al-Jawadi, S. Poller, R. Haddad, W. Schuhmann, NADH oxidation using modified electrodes based on lactate and glucose dehydrogenase between an electrocatalyst film and redox catalyst modified polymers” *Microchim. Acta* (2012) 177: 405-410.
- [8] P. Du, S. Liu, P. Wu, C. Cai, Single-walled carbon nanotubes functionalized with poly(nile blue A) and their application to dehydrogenase-based biosensors *Electrochimica Acta*, 53 (2007) 1811–1823.
- [9] A. Gurban, T. Noguer, C. Bala, L. Rotariu, Improvement of NADH detection using Prussian blue modified screen-printed electrodes and different strategies of immobilisation *Sensors and Actuators B* 128 (2008) 536–544.
- [10] I.B. Rejeb, F. Arduini, A. Amine, M. Gargouri, G. Palleschi, Amperometric biosensor based on Prussian Blue-modified screen-printed electrode for lipase activity and triacylglycerol determination *Anal. Chim. Acta* 594 (2007) 1–8.
- [11] Q. Gao, X. Cui, F. Yang, Y. Ma, X. Yang, Preparation of poly(thionine) modified screen-printed carbon electrode and its application to determine NADH

in flow injection analysis system, *Biosensors and Bioelectronics*, 19 (2003) 277-282.

[12] B. Persson, L. Gorton, A comparative study of some 3,7-diaminophenoxazine derivatives and related compounds for electrocatalytic oxidation of NADH, *J. Electroanal. Chem.* 292 (1990) 115-138.

[13] M.L.C. Passos, M.L.M.F.S. Saraiva, J.L.F.C. Lima, A thionine-based reversible redox sensor on a sequential injection system, *Anal. Chim. Acta*, 668 (2010) 41-46.

[14] Meng, P. Wu, G. Chen, C. Cai Low Overpotential Detection of NADH and Ethanol Based on Thionine Single-Walled Carbon Nanotube Composite, *J. Electroanal. Soc.* 155 (2008) F231-F236.

[15] S. Ashok Kumar and S.M Chen, "Electroanalysis of NADH using conducting and redox active polymer/carbon nanotubes modified electrodes – a review" *Sensors* 8 (2008) 739-766.

[16] H. Zhou, Z. Zhang, P. Yu, L. Su, T. Ohsaka, L. Mao, Noncovalent Attachment of NAD⁺ Cofactor onto Carbon Nanotubes for Preparation of Integrated Dehydrogenase Based Electrochemical Biosensors, *Langmuir* 26 (2010) 6028-6032.

[17] Z. Wang, M. Li, Y. Zhang, J. Yuan, Y. Shen, L. Niu, A. Ivaska, Thionine-interlinked multi-walled carbon nanotube/gold nanoparticle composites, *Carbon* 45 (2007) 2111-2115.

[18] J.E. Riggs, Z. Guo, D.L. Carroll, Y.-P. Sun, Strong luminescence of solubilized carbon nanotubes, *J. Amer. Chem. Soc.* 122 (2000) 5879-5880.

- [19] B. Vigolo, A. Pénicaudl, C. Coulon, C. Sauder, R. Pailler, C. Journet, P. Bernier, P. Poulin, Macroscopic fibers and ribbons of orientated carbon nanotubes, 290 (2000) 1331-1334.
- [20] R. Bandyopadhyaya, E. Nativ-Roth, O. Regev, R. Yerushalmi-Rozen, Stabilization of individual nanotubes in aqueous solutions, *Nanoletters* 2 (2002) 25-28.
- [21] M. Ates, A review study of biosensor systems based on conducting polymers, *Materials Science and Engineering C* 33, 2013, 1853-1859.
- [22] R. Jain, N. Jadon, A. Pawaiya, Polypyrrole based next generation electrochemical sensors and biosensors: a review *TrAC Trends in Analytical Chemistry* vol 97, 2017 363-373.
- [23] L. Xia, Z. Wei, M. Wan, Conducting polymer nanostructures and their application in biosensors, *Journal of Colloid and Interface Science* 241 (2010) 1-11.
- [24] B.D. Malhotra, A. Chaubey, S.P. Singh, Prospects of conducting polymers in biosensors, *Analytica Chimica Acta* 578 (2006) 59-74.
- [25] M. Gerard, A. Chaubey, B.D. Malhotra, Application of conducting polymers to biosensors, *Biosensors and Bioelectronics* 17 (2002) 345-359.
- [26] V.S. Vasantha, S.-M. Chen, Synergistic effect of a catechin-immobilized poly(3,4-ethylenedioxythiophene)-modified electrode on electrocatalysis of NADH in the presence of ascorbic acid and uric acid *Electrochimica Acta* 52 (2006) 665-674.
- [27] A. Balamurugan, S.-M. Chen, Voltammetric oxidation of NADH at phenyl azo aniline/PEDOT modified electrode *Sensors and Actuators B* 129 (2008) 850-858.


- [28] A. Balamurugan, K.-K. Ho, S.-M. Chen, T.-Y. Huang, Electrochemical sensing of NADH based on Meldola Blue immobilized silver nanoparticle-conducting polymer electrode, *Colloids and Surfaces A:Physiochemical and Engineering Aspects* 362 (2010) 1-7.
- [29] D. Polcari, P. Dauphin-Ducharme and J. Mauzeroll, Scanning Electrochemical Microscopy: A comprehensive review of experimental parameters from 1989 to 2015 *Chem. Rev.* 116 (2016) 13234-13278.
- [30] C. G. Zoski, Review – Advances in Scanning Electrochemical Microscopy, *J. of the Electrochemical Society* 163 (4) (2016) H3088-H3100.
- [31] S. Amemiya, A. J. Bard, F-R F. Fan, M.V. Mirkin and P.R. Unwin, Scanning Electrochemical Microscopy, *Annual Rev. Anal. Chem.* 1 (2008) 95-131.
- [32] I. Morkvenaite-Vilkonciene, A. Ramanaviciene, P. Genyes and A. Ramanavicius, Evaluation of enzymatic kinetics of GOx-based electrodes by scanning electrochemical microscopy at redox competition mode, *Electroanalysis* 29 (2017) 1532-1542.
- [33] P. Sun., F.O. Laforge and M.V. Mirkin, Scanning electrochemical microscopy in the 21st century, *Phys. Chem. Chem. Phys.*, 9 (2007) 802-823.
- [35] T. Kai, C.G. Zoski and A.J. Bard, Scanning electrochemical microscopy at the nanometer level, *Chem. Commun.* 54 (2018) 1934-1947.
- [34] D.O. Wipf, in : A.J. Bard, M.V. Mirkin (Ed.), *Scanning Electrochemical Microscopy*, Marcel Dekker Inc., New York, 2001, Ch. 2.
- [36] D.T. Pierce, P. R. Unwin and A.J. Bard scanning Electrochemical Microscopy Studies of enzyme mediator kinetics for membrane and surface immobilised glucose oxidase *Anal. Chem.* 64 (1992) 1795-1804.

- [37] A.L. Barker, J.V. Macpherson, C. J. Slevin and P. R. Unwin, "Scanning Electrochemical Microscopy (SECM) as a probe of transfer processes in two phase systems: theory and experimental applications of SECM-induced transfer with arbitrary partition coefficients, diffusion coefficients and interfacial kinetics" *J. Phys. Chem. B* 102 (1998) 1586-1598.
- [38] M. Gonsalves, J.V. Macpherson, D. O'Hare, C.P. Winlove, P.R. Unwin, High resolution imaging of the distribution and permeability of methyl viologen dication in bovine articular cartilage using scanning electrochemical microscopy, *Biochimica et Biophysica Acta*, 1524 (2000) 66-74.
- [39] S.Warren, D.Rathod, T.McCormac, E. Dempsey, Investigations into the use of a thionine/PEDOT layer as an NADH electrocatalyst with applications in glutamate sensing, *ECS Transactions* 25 (2010) 21-32.
- [40] V.E. Nicotra, M.F. Mora, R.A. Iglesias, A.M. Baruzzi, Spectroscopic characterization of thionine species in different media, *Dyes and Pigments* 76 (2008) 315-318.
- [41] A. Abd-Elwahed, R. Holze, Ion size and size memory effects with electropolymerized polyaniline, *Synthetic Metals* 131 (2002) 61-70.
- [42] A.R. Guadalupe, K.E. Liu, H.D. Abruna, Transport properties of cationic dyes in Nafion films: unusually high diffusion coefficients and aggregation effects, *Electrochimica Acta* 36 (1991) 881-887.
- [43] R. Tamilarasan, P. Natarajan, Photovoltaic conversion by macromolecular thionine films, *Nature* 292 (1981) 224-225.
- [44] K. Viswanathan, P. Natarajan, Photophysical properties of thionine and phenosafranine dyes covalently bound to macromolecules, *J. Photochem. Photobiol. A: Chem.* 95 (1996) 245-253.

- [45] S. Warren, T. McCormac, E.M. Mihaylova, E. Dempsey, Investigation into charge transport dynamics of [Os(bpy)₂(picolinate)]Cl Nafion films, *Electroanalysis* 18 (2006) 1778 – 1785.
- [46] T. Komura, T. Yamaguchi, H. Sato, H. Shimatani, K. Takahashi, Incorporation of 1,1'-dibenzyl-4,4'-bipyridium cation into Nafion films and charge transport in loaded film electrodes, *Electrochimica Acta* 46 (2001) 3579-3588.
- [47] M. Somasundrum, J.V. Bannister, Redox reactions in the presence of an ion-exchange/hydrogel composite film, *Electroanalysis* 9 (1997) 56-62.
- [48] M. V. Mirkin in A.J. Bard, M.V. Mirkin (Ed.), *Scanning Electrochemical Microscopy*, Marcel Dekker Inc., New York, 2001, Ch. 5.
- [49] R.-S. Juang, F.-C. Wu, R.-L. Tseng, Use of chemically modified chitosan beads for sorption and enzyme immobilisation, *Advances in Environmental Research* 6 (2002) 171-177.

^I Present address: CREST Technology Gateway, FOCUS Research Institute, Technological University Dublin, Kevin St, Dublin Ireland.

^{II} Present address: Cefa-Cilinas Biotics Pvt Ltd, Aurangabad, Maharashtra, India.

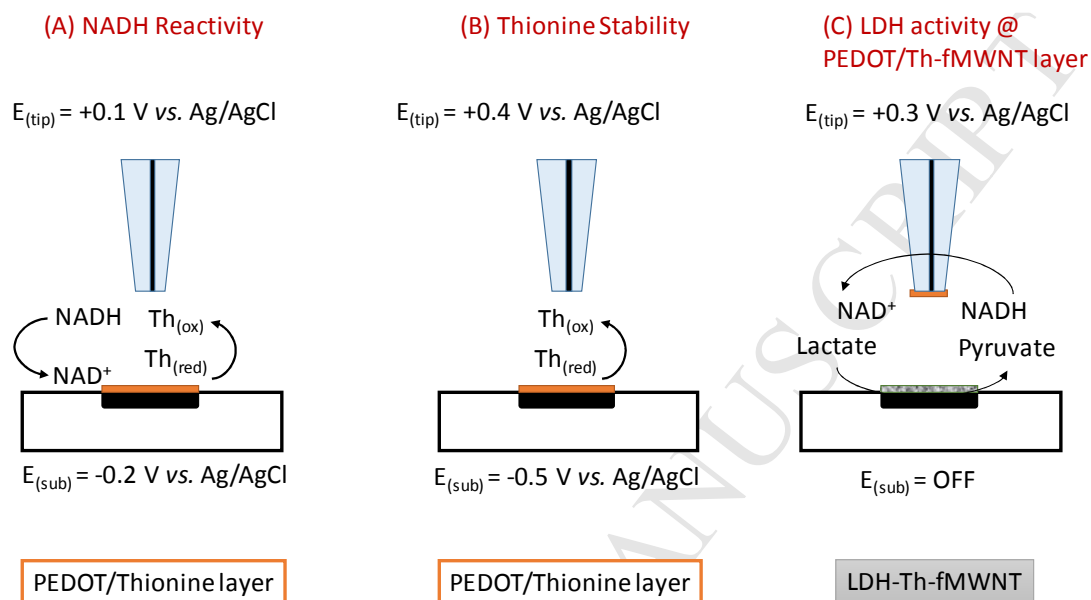

Scheme 1

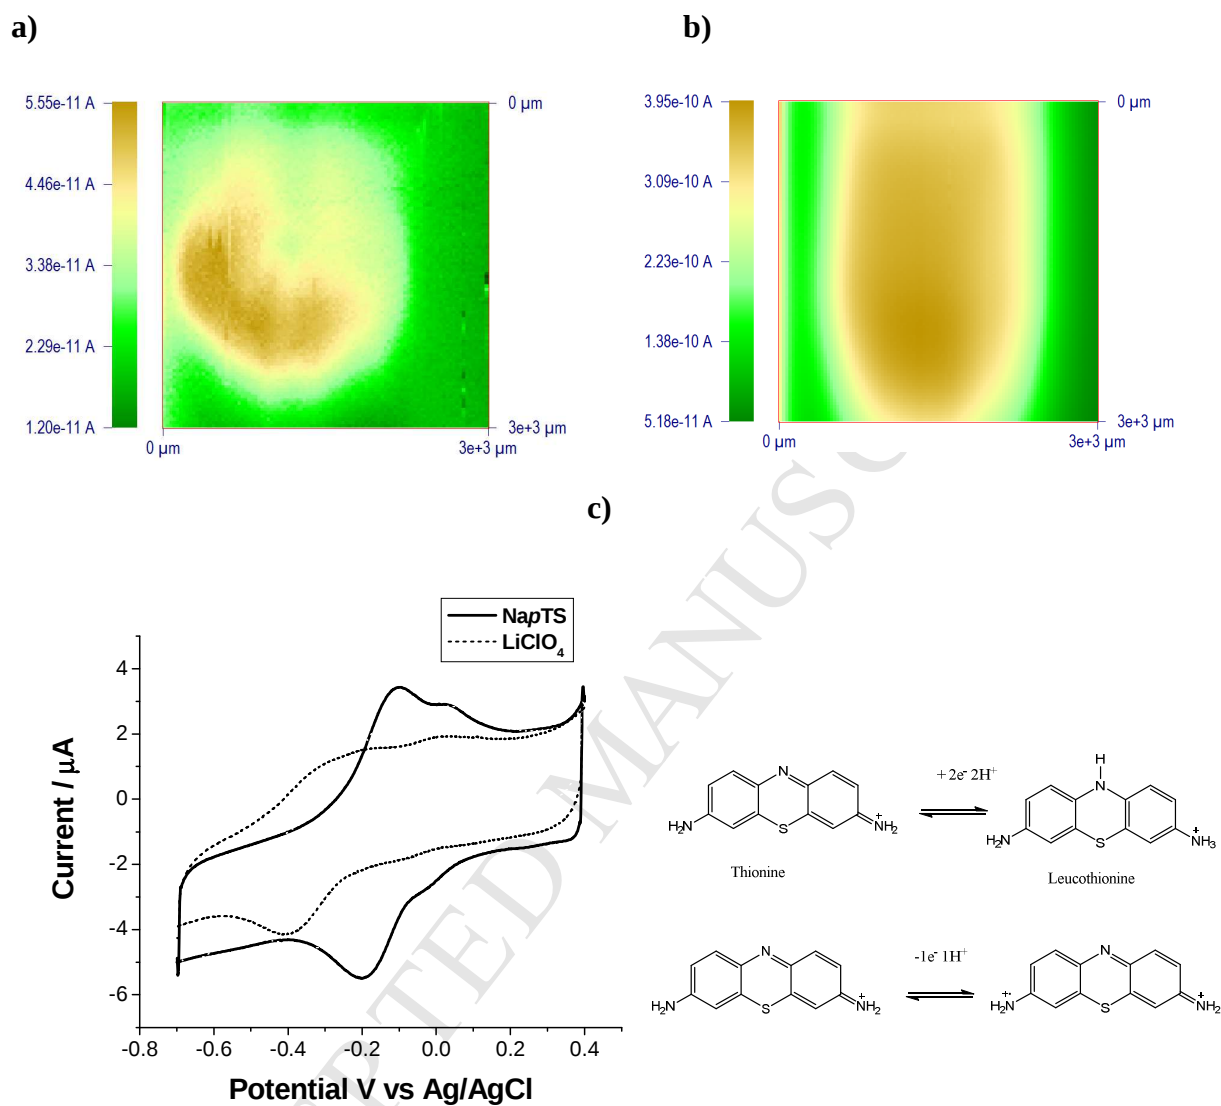


Figure 1



Table 1.**(A)**

Thionine time / min	λ / nm	Absorbance	Concentration / mol.cm^{-3A}	% Loading	D_{CT} / $\text{cm}^2.\text{s}^{-1}$
15	566	0.215	4.06×10^{-6}	37.8	36.44×10^{-8}
30	571	0.327	6.18×10^{-6}	57.8	9.56×10^{-8}
45	572	0.57	10.78×10^{-6}	100	1.89×10^{-8}
60	571	0.495	9.36×10^{-6}	87.1	3.47×10^{-8}
75	571	0.428	8.09×10^{-6}	75.5	8.82×10^{-8}

^A Concentration calculated from Beer Lambert Law applying ϵ $2.2814 \times 10^4 \text{ M}^{-1}.\text{cm}^{-1}$, where $l = 0.001\text{cm}$.

(B)

Thionine time / min	λ / nm	Absorbance	Concentration / mol.cm^{-3A}	% Loading	D_{CT} / $\text{cm}^2.\text{s}^{-1}$
15	572	0.150	6.58×10^{-6}	69.8	12.75×10^{-8}
30	573	0.205	8.99×10^{-6}	95.4	6.36×10^{-8}
45	572	0.201	8.81×10^{-6}	93.5	5.84×10^{-8}
60	572	0.206	9.03×10^{-6}	95.8	7.12×10^{-8}
75	574	0.215	9.424×10^{-6}	100	3.432×10^{-8}
90	572	0.209	9.161×10^{-6}	97.2	10.660×10^{-8}

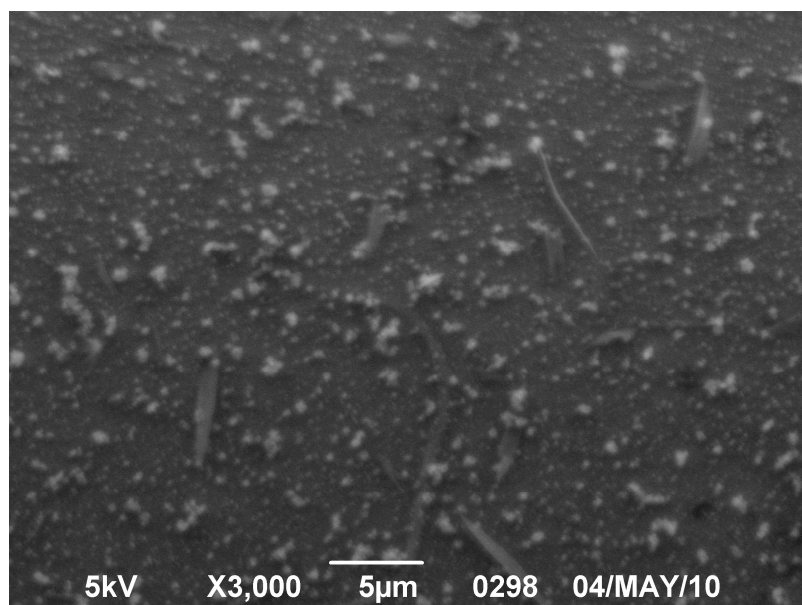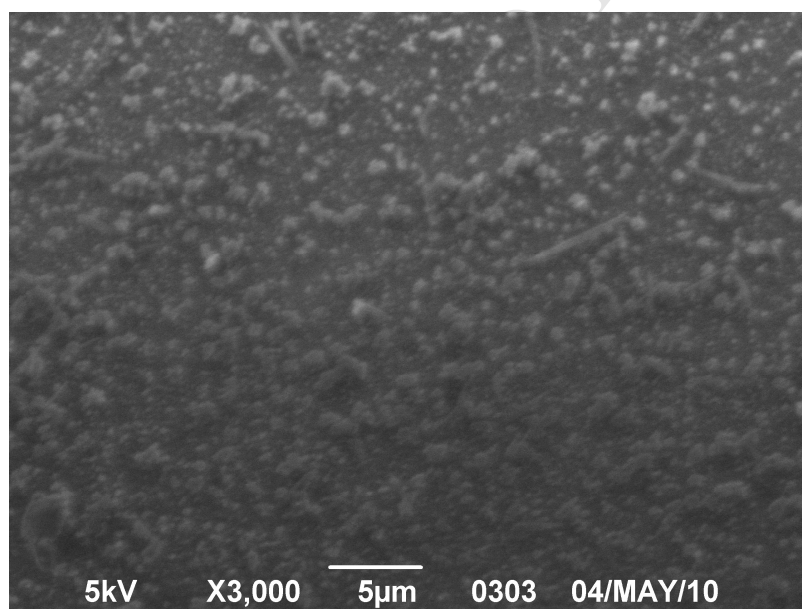(a)**(b)****Figure 2**



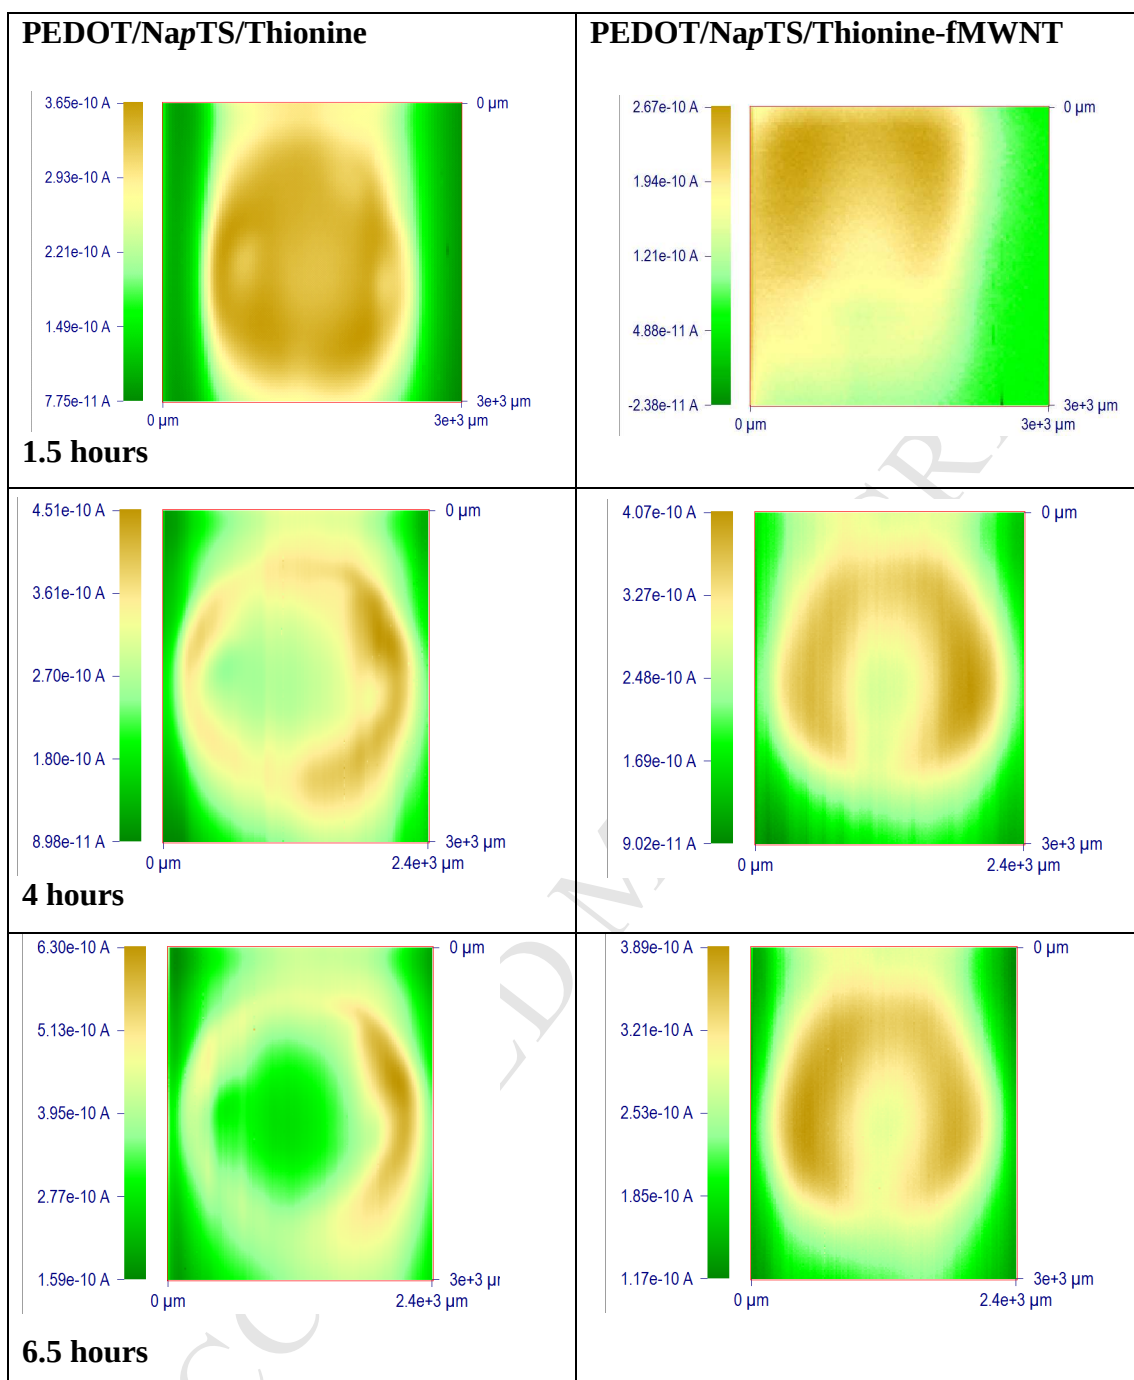


Figure 3

(a)

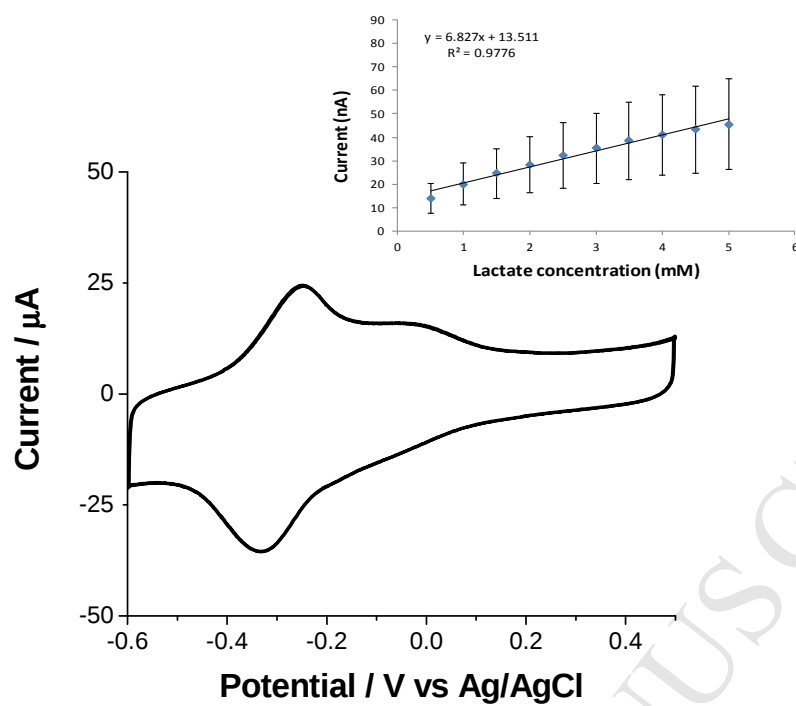

(b)

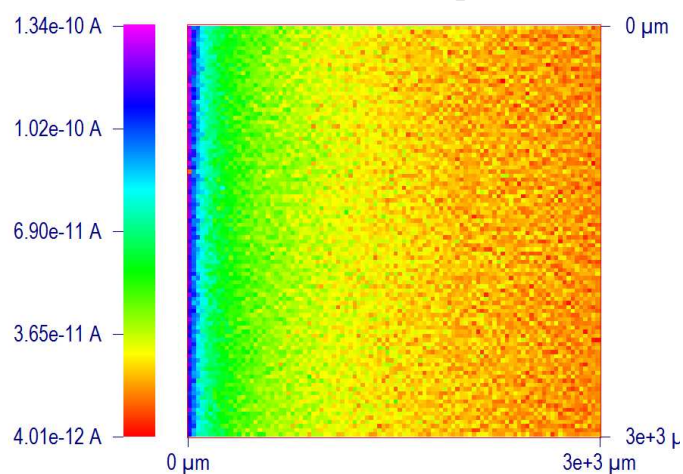

(c)

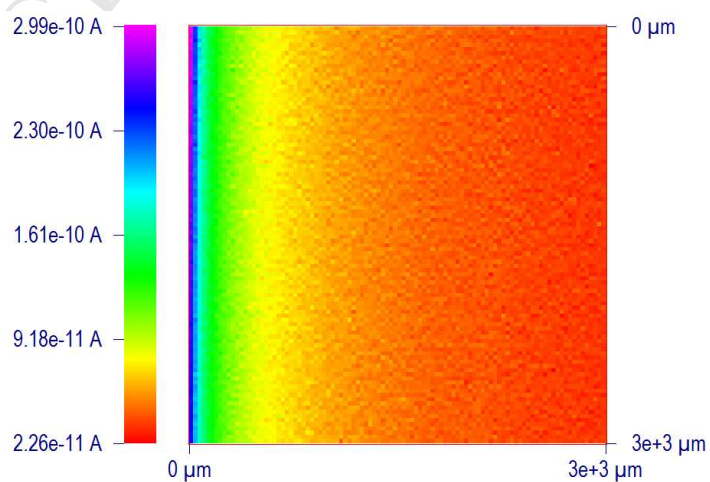


Figure 4

Legends

Scheme 1. Schematics representing the modes substrate generation tip collection (a) and (c) and SECM induced transfer (b) applied for SECM imaging experiments.

Table 1: (A) Thionine concentration levels for varying loading times into PEDOT/LiClO₄ with corresponding D_{CT} values. (B) Thionine concentration levels for varying loading times in PEDOT/sodium *p*-toluene sulphonate and corresponding D_{CT} values.

Figure 1. SECM imaging at 500 $\mu\text{m.s}^{-1}$ in 1 mM NADH, PBS pH 7.4, E_{SUBSTRATE} - 0.2 V vs Ag/AgCl, E_{TIP} +0.1 V vs Ag/AgCl, z -80 μm ; for films formed by thionine incorporation (a) during PEDOT electropolymerisation (Thionine-PEDOT) and (b) after PEDOT electropolymerisation (PEDOT/Thionine), (c) cyclic voltammograms of PEDOT/Thionine films formed using LiClO₄ or sodium *p*-toluene sulphonate (NapTS) as electropolymerisation electrolyte, 45 minutes thionine inclusion period. Associated redox processes for thionine proton dependant reduction to Leucothionine and oxidation to the radical cation form.

Figure 2. SEM BEC images of PEDOT/Th-fMWNT films after a) 1 hour and b) 2 hours loading indicating increased surface density of thionine entrapped MWCNTs.

Figure 3. SECMIT images of the leaching of thionine from prepared films over time (1.5-6.5 hrs) for both PEDOT/Thionine and PEDOT/Th-fMWNT surfaces. E_{SUBSTRATE}: -0.5 V vs. Ag/AgCl and E_{TIP}: +0.4 V vs. Ag/AgCl, z = -300 μm .

Figure 4 (a) Cyclic voltammogram of lactate dehydrogenase modified thionine-fMWNT and inset amperometric calibration plot for additions of 0.5 mM lactate in the presence of 1 mM NAD⁺ at 0.0 V vs. Ag/AgCl. Standard deviation across the analytical test range for lactate was 13.8 for n=3 measurements at each concentration. (b) SECM images at a modified 25 μm Pt tip electrode of LDH/Th-fMWNT (substrate) in 1 mM NAD⁺ in PBS and (c) LDH/Th-fMWNT in 1 mM NAD⁺ PBS + 5 mM lactate. E_{SUBSTRATE}: off, E_{TIP} : +0.3 V vs. Ag/AgCl, z =800 μm .

Highlights

Scanning electrochemical microscopy imaging of poly (3,4-ethylenedioxythiophene)/thionine electrodes for lactate detection via NADH electrocatalysis

Scanning electrochemical microscopy (SECM) has been employed coupled with an electrochemical/spectroscopic and surface investigations into thionine entrapment within an electropolymerised poly(3,4-ethylenedioxythiophene) (PEDOT) film for NADH electrocatalysis and lactate biosensing.

Declaration of interests

☒ The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

☐ The authors declare the following financial interests/personal relationships which may be considered as potential competing interests:

--

Credit Author Statement***Susan Warren***

Conceptualisation, data curation, analysis and investigation; Generation of experimental data in relation to the electrochemical and surface analysis data together with SECM analysis. Writing, review and editing.

Dhanraj Rathod

Data curation and methodology; Provision of the multiwalled carbon nanotubes and assistance with thionine modification methodology.

Grigore Munteanu

Data curation and methodology, formal analysis; Worked jointly as a postdoctoral research fellow at the time with Susan Warren to generate SECM data.

Eithne Dempsey

Conceptualisation and funding acquisition, Writing, review and editing; Lead supervisor of the postdocs and postgraduate student, input into experimental design. Corresponding author.

Timothy McCormac

Funding acquisition, Co-supervisor of the postdocs and postgraduate student