

Accepted Manuscript

A microfluidic biosensor for online and sensitive detection of *Salmonella* typhimurium using fluorescence labeling and smartphone video processing

Siyuan Wang, Lingyan Zheng, Gaozhe Cai, Ning Liu, Ming Liao, Yanbin Li, Xibin Zhang, Jianhan Lin



PII: S0956-5663(19)30398-7

DOI: <https://doi.org/10.1016/j.bios.2019.111333>

Article Number: 111333

Reference: BIOS 111333

To appear in: *Biosensors and Bioelectronics*

Received Date: 12 March 2019

Revised Date: 10 May 2019

Accepted Date: 15 May 2019

Please cite this article as: Wang, S., Zheng, L., Cai, G., Liu, N., Liao, M., Li, Y., Zhang, X., Lin, J., A microfluidic biosensor for online and sensitive detection of *Salmonella* typhimurium using fluorescence labeling and smartphone video processing, *Biosensors and Bioelectronics* (2019), doi: <https://doi.org/10.1016/j.bios.2019.111333>.

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

A microfluidic biosensor for online and sensitive detection of *Salmonella typhimurium* using fluorescence labeling and smartphone video processing

Siyuan Wang¹, Lingyan Zheng¹, Gaozhe Cai¹, Ning Liu¹, Ming Liao², Yanbin Li³, Xibin Zhang⁴,
Jianhan Lin^{1*}

¹ Key Laboratory of Agricultural Information Acquisition Technology, Ministry of Agriculture and Rural Affairs, China Agricultural University, Beijing 100083, China

² College of Veterinary Medicine, South China Agricultural University, Guangzhou 510642, China

³ Department of Biological and Agricultural Engineering, University of Arkansas, Fayetteville, Arkansas 72701, US

⁴ College of Food Science and Engineering, Shandong Agricultural University, Taian 271018, China

*Corresponding author: Dr. Jianhan Lin, Phone/Fax: +86-10-62737599; Email: jianhan@cau.edu.cn

Abstract: Early screening of foodborne pathogens is a key to ensure food safety. In this study, we developed a microfluidic biosensor for online and sensitive detection of *Salmonella* based on immunomagnetic separation, fluorescence labeling and smartphone video processing. First, the immune magnetic nanoparticles were used to specifically separate and efficiently concentrate the target bacteria and the magnetic bacteria were formed. Then, the magnetic bacteria were labeled with the immune fluorescent microspheres and the fluorescent bacteria were formed. Finally, the fluorescent bacteria were continuously injected into the microfluidic chip on the smartphone-based fluorescent microscopic system, and the fluorescent spots were online counted using the smartphone App based on inter-frame difference algorithm to obtain the amount of the target bacteria. Under the optimal conditions, this proposed biosensor was able to quantitatively detect *Salmonella typhimurium* ranging from 1.4×10^2 to 1.4×10^6 CFU/mL, and its lower detection limit was 58 CFU/mL. This biosensor could be extended for detection of multiple foodborne pathogens using different fluorescent materials.

Keywords: Microfluidic biosensor; fluorescence labeling; smartphone video processing; magnetic separation; *Salmonella typhimurium*

1. Introduction

Foodborne pathogens are a main factor for the outbreaks of foodborne diseases. According to the World Health Organization (WHO), there are over 150 million diarrheal cases in the world every year, 70% of which are related to foodborne pathogens (World Health Organization 2018). Among these foodborne pathogens, *Salmonella* with 2,523 serotypes receives the most concerns (Malorny et al. 2009) since it is widely found in various foods and can result in severe diseases sometimes. At present, there are some existing methods for detection of *Salmonella*. The traditional culture plating is the gold standard method based on bacteria growing in agar-based growth medium. It has high accuracy and sensitivity, however it takes a few days (2-4 d) to obtain final results and is not suitable for in-field detection (Lee et al. 2015; Rohde et al. 2017). Enzyme-linked immunosorbent assay (ELISA) is a recommended method based on the immunological reaction between antigen and antibody. It is rapid (2-4 h), high-throughput and specific, however it has a low sensitivity and is often subject to cross contamination (Miller et al. 2011; Zhang et al. 2017). Polymerase chain reaction (PCR) is recommended for rapid detection of *Salmonella* and featured with short time (2-4 h), high throughput and high sensitivity, but it requires complex DNA extraction procedure and professional facilities (Jyoti et al. 2010; Lungu et al. 2012). Thus, there is an urgent demand on rapid and sensitive detection methods of foodborne pathogens.

As an alternative for bacteria detection, fluorescent biosensors have been often reported to detect *Salmonella* in recent years. In most studies, fluorescent biosensors were developed first using immune magnetic nanoparticles to capture the target bacteria to form the magnetic bacteria, then using fluorescent materials such as fluorescein (Lee et al. 2017) and quantum dots (Yang and Li 2006) to conjugate the magnetic bacteria to form the fluorescent bacteria, and finally measuring the fluorescent signals to determine the amount of the target bacteria. The reported fluorescent biosensors were often able to detect foodborne bacteria as low as 10^1 - 10^3 CFU/mL (Bayramoglu et al. 2018; Li et al. 2018). Recently, an interesting fluorescent biosensor was reported by Wang et al. (Wang and Kang 2016) for bacteria detection using single-stranded DNA aptamers conjugated silica fluorescent nanoparticles to label the target *Salmonella* cells, which then could be counted on a fluorescent microscope to obtain quantitative results. Although immunofluorescent assays have been widely used for bacteria detection due to their high sensitivity, good specificity and fast speed (Duedu and French 2017), they are still faced with some challenges, such as non-specific adsorption to proteins, cells, nucleic acids and other substances in real samples, resulting in inevitable background noises and false positives (Lee et al. 2014; Wang and Duncan 2017). Thus, combination of immunomagnetic separation and immunofluorescent assays might be promising to develop new rapid, sensitive and non-contact methods for bacteria detection.


In recent years, microfluidics has received extensive attentions and been frequently used for biological detection due to its outstanding advantages, such as small size, less reagent consumption, high reaction efficiency, low cost, easy integration, automatic operation and point-of-care diagnosis (Fang et al. 2010; Kulinsky et al. 2013; Whitesides 2013). At present,

optical detection and electrochemical detection are often used with microfluidics to develop microfluidic biosensors (Hassan et al. 2016; Martinez et al. 2008; Nie et al. 2010; Stott et al. 2010). An example is a microfluidic chip for ultrasensitive detection of *Salmonella* Typhimurium reported by He et al. (He et al. 2013) using positive dielectrophoresis enrichment and fluorescent nanoparticles label. It could detect *Salmonella* as low as 56 CFU/mL in 2 h. Another interesting sample is a microfluidic chip with magnetically fluidized bed reported by Srbova et al. (Srbova et al. 2017) for immune separation of *Salmonella* in milk. This microfluidic chip had a separation efficiency of up to 99% for *Salmonella*. Besides, Altintas et al. (Altintas et al. 2018) reported a microfluidic biosensor for real-time and automatic detection of *Escherichia coli* using electrochemical amperometry to achieve a lower detection limit of 50 CFU/mL. With more and more popularity of smartphones, they have been often applied to develop rapid and in-field detection assays of foodborne pathogens due to their portability, low cost and easy operation (Jing et al. 2014; Zangheri et al. 2015). Shrivastava et al. (Shrivastava et al. 2018) developed a smartphone-based fluorescent biosensor for detection of *Staphylococcus aureus* in a culture-free, rapid and quantitative manner from minimally processed liquid samples using aptamer functionalized fluorescent magnetic nanoparticles, and the lower detection limit of 10 CFU/mL could be obtained by counting the bacteria on the static fluorescence images. Cui et al. (Cui et al. 2018) proposed a digital standard plate count method based on micro-droplet turbidity imaging and it could detect living bacteria in infant milk powder as low as 100 CFU/mL within 6 h. To the best of our knowledge, all the existing smartphone based biosensing methods are based on static image analysis, which are very difficult to realize on-line detection of foodborne bacteria (Wang et al. 2016; Zheng et al. 2019).


Zhu et al. (Zhu et al. 2011) reported a similar method using fluorescent labeling and smartphone video processing for cell counting. The authors used white blood cells in human whole blood as research model and integrated optofluidic fluorescent microscopy and flow cytometry on a smartphone. However, this proposed system could not be directly used for counting bacteria since the size of human white blood cell (10-12 μm) is much larger than foodborne bacteria (1-2 μm), which need higher resolution and larger magnification. More importantly, the video was post processed, indicating that this proposed system was not suitable for online identification. Therefore, further study based on this method might provide a promising way to detect single bacterium.

In this work, we developed a novel microfluidic biosensor for on-line, rapid and sensitive detection of *Salmonella* typhimurium combining immunomagnetic separation, fluorescence labeling and smartphone video processing. As shown in Scheme 1, the magnetic nanoparticles (MNPs) modified with the monoclonal antibodies (MAbs) against *Salmonella* typhimurium were first used to separate the target bacteria from the sample background to form the MNP-bacteria complexes (magnetic bacteria), which then reacted with the fluorescent microspheres (FMSs) modified with the polyclonal antibodies (PAbs) against *Salmonella* typhimurium to form the MNP-bacteria-FMS complexes (fluorescent bacteria). After the fluorescent bacteria were

magnetically separated to remove the unbound FMSs, efficiently concentrated in small volume of PBS and continuously injected into the microfluidic chip, the smartphone based fluorescent microscopic system was used with the LED light source for fluorescent excitation to monitor the flowing fluorescent spots and the amount of the fluorescent bacteria was calculated through real-time video processing.

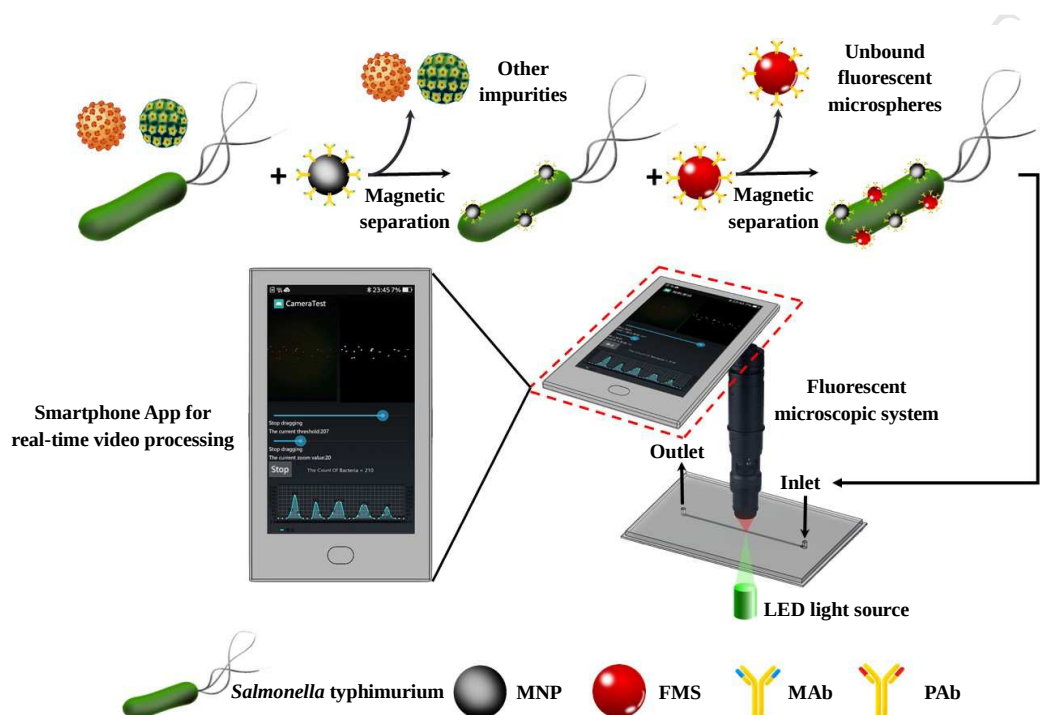

(a)

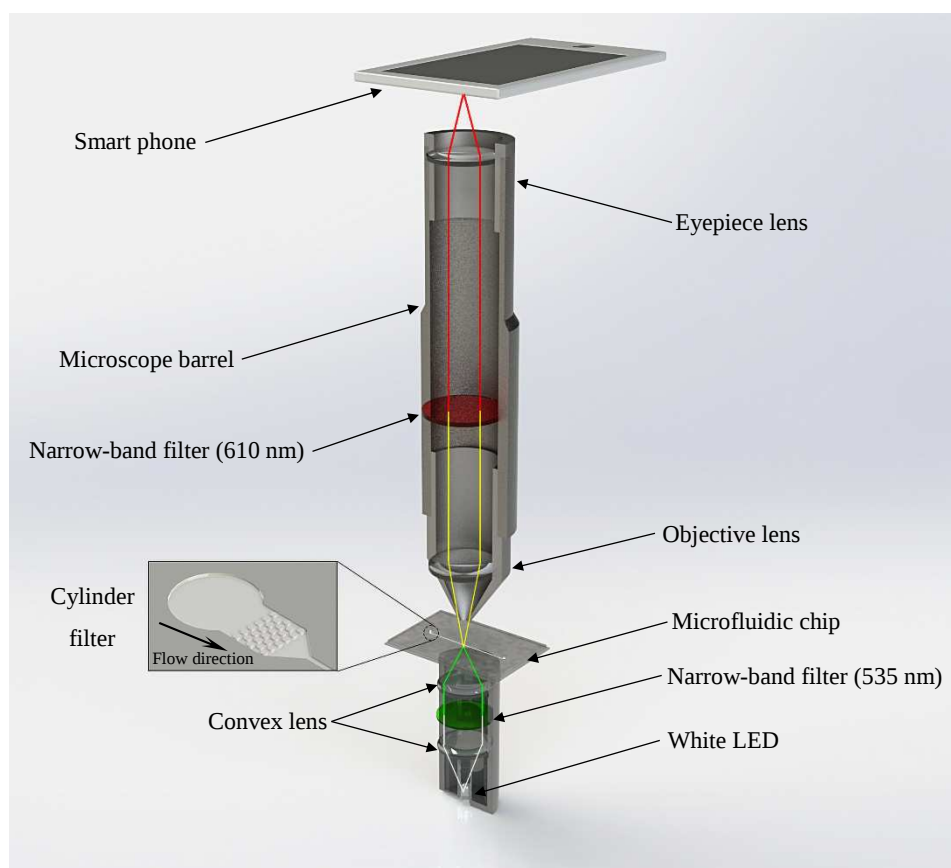

(b)

Scheme 1. (a) The principle of the proposed microfluidic biosensor for on-line, rapid and sensitive detection of *Salmonella typhimurium*; (b) The structure of the smartphone based fluorescent microscopic system.

2. Materials and Methods

2.1. Materials

Salmonella typhimurium (ATCC 14028) was used as target bacteria, and *Listeria monocytogenes* (ATCC 13932), *E. coli* O157:H7 (ATCC 43888) and *Vibrio parahaemolyticus* (ATCC 17802) were used as non-target bacteria. The MAbs (1 mg/mL) against *Salmonella typhimurium* from Meridian (Memphis, TN, US) and the PABs (2.5 mg/mL) against *Salmonella typhimurium* from Fitzgerald (Acton, Massachusetts, US) were used for immunological reaction with *Salmonella typhimurium*. The biotin labeling kit from Elabscience (Wuhan, China) was used for the modification of biotin onto the MAbs. The streptavidin modified MNPs (1 mg/mL) with the diameter of 150 nm from Ocean Nano (MHS-150-10, Dunedin, FL, US) were used for immunomagnetic separation of *Salmonella typhimurium*. The carboxylate FMSs (10 mg/mL) with the diameter of 150 nm from VDO Biotech (FR150C, excitation wavelength: 535 nm, emission wavelength: 610 nm, Suzhou, China) were used for labelling *Salmonella typhimurium* as detection signal. N-(3-dimethylaminopropyl)-N'-ethylcarbodiimide hydrochloride (EDC·HCl) was used for modifying the FMSs with the PABs. Phosphate buffered saline (PBS, 10 times concentrated, pH 7.4) from Sigma-Aldrich (St. Louis, MO, US) was 10-fold diluted with deionized water to prepare

the buffer solution. Tween-20 from Amresco (Solon, OH, US) was used for washing. Bovine serum albumin (BSA) from Sigma Aldrich was used for blocking. Brain heart infusion (BHI) medium from Remel (Lenexa, KS, US) and Luria-Bertani (Lee et al.) medium (Aoboxing Biotech, Beijing, China) fluorescen were used for bacterial culture. Deionized water produced by Advantage 10 (18.2 MΩ·cm, Billerica, MA, US) was used for preparing all the solutions.

2.2. Fabrication of the microfluidic detecting chip

The microfluidic detecting chip is the key component of this proposed biosensor. It composed of two parts: (1) a fan-shaped cylinder filter for avoiding the blocking of the chip by the large-sized particles in the sample and enhancing the dispersion of the fluorescent bacteria, and (2) a line-shaped microchannel for observing and counting the fluorescent spots. As shown in Scheme 1(b), the cylinder filter had five rows of staggered micro-cylinders with a diameter of 50 μm, a height of 25 μm and an interval of 50 μm, and the straight microchannel had a width of 25 μm, a height of 25 μm and a length of 50 mm. The mold of the microfluidic channel was fabricated using SU8 photolithography. After the prepolymer and the curing agent from Dow Corning (Sylgard 184, Midland, US) were mixed at the ratio of 10:1 and used to make the poly (dimethoxy) silane (PDMS) microchannel, the microchannel and the glass plate from Sail Brand (7101, Jinan, China) were processed by surface oxygen plasma (Harrick Plasma, Ithaca, NY, US) and bonded to fabricate the microfluidic chip. The photo of the microfluidic chip is shown in Figure S1.

2.3. Development of the smartphone based fluorescent microscopic system

The fluorescent microscopic system is another key component of this proposed biosensor. It composed of three parts: (1) the light source for fluorescent excitation, (2) the fluorescent microscope for optical amplifier, and (3) the smartphone App for real-time video processing. The structure of the fluorescent microscopic system is shown in Scheme 1(b). The light source with the wavelength of 535 nm was obtained using a 5W white LED from Rongcheng Microelectronics (KB0603, Shenzhen, China) to provide the light beam, two convex lenses with the focus length of 50 mm from Yajamei optics (YJM-50, Shenzhen, China) to focus the diverging beam, a narrow-band optical filter with the central wavelength of 535 nm from Hoda lens optics (D20-BPOD3-535, Shenzhen, China) to allow the penetration of the light with the wavelength of around 535 nm, and a 3D-printed holder to precisely fix these optical components.

The fluorescent microscope was constructed using flat-field achromatic objective lens with the magnification of 40 times, the numerical aperture of 0.65 and the working distance of 0.53 cm, a large flat-field coated eyepiece lens with the magnification of 25 times, the focus length of 12.5 mm, the view field of Φ6.5 mm, a narrow-band optical filter with the central wavelength of 610 nm and a 3D-printed holder to precisely fix these optical components. Both the objective lens and the eyepiece lens were purchased from Jiangnan Yongxin Optics (Nanjing, China) with the total magnification of 1000 times. The optical filter was purchased from Hoda Lens Optics (D20-BPOD3-610) and installed between the eyepiece lens and the objective lens to only allow

the penetration of the light with the wavelength of around 610 nm, which was the same with the emission wavelength of the FMSs. The fluorescent image or video were converged on the smartphone's CMOS sensor. The light source, the microfluidic chip, the fluorescent microscope and the smartphone were precisely aligned from bottom to top with appropriate spaces.

The smartphone App was developed under the Android operating system installed on a low-cost smartphone (Honor 9, Huawei, Shenzhen, China) with 4 GB RAM, 2.4 GHz CPU and 20 million pixels camera. The light source was first used to continuously excite the fluorescent bacteria to emit the fluorescent signals when they flowed through the microchannel. The video stream of the microchannel was then obtained from the camera and extracted into a sequence of grayscale frames. Finally, two adjacent frames were compared using the inter-frame difference algorithm to obtain the binarized difference images, and the flowing fluorescent spots could be accurately identified in the difference images by setting an appropriate threshold and counted to determine the total amount of the bacteria. The App is shown in supplemental Video S1. The detailed dimension of the fluorescent microscopic system and the interface function description of the App are shown in Figure S2 and Figure S3, respectively.

2.4. Modification of the FMSs with the PABs

First, 20 µg of the FMSs and 68 µg of the PABs against *Salmonella typhimurium* were added into 3 mL of PB buffer (pH 6.0, 10 mM) and stirred 30 min for better electrostatic adsorption. Then, 40 µg of EDC was added and stirred at room temperature for 30 min. This step was repeated 3 times to allow complete reaction between the PABs and the carboxyl groups on the surface of the FMSs. Finally, 80 mg of BSA and 120 µg of EDC were added and stirred at room temperature for 60 min to minimize non-specific adsorption, followed by centrifuging at 10,000 rpm for 15 min to remove the surplus BSA and resuspending in 1 mL of PB buffer (pH 7.4, 10 mM) containing 5% sucrose and 0.02% sodium azide. The immune FMSs with the concentration of 0.2 mg/mL were stored in 4°C for future use. To verify the successful synthesis of the immune FMSs, the dynamic light scattering analysis was conducted and the results are shown in Figure S2.

2.5. Separation and detection of *Salmonella typhimurium* in pure culture

The target bacteria were first separated with the immune MNPs and then labelled with the fluorescent FMSs. Prior to test, the streptavidin modified MNPs and the biotinylated MABs were mixed for 45 min to form the immune MNPs with the concentration of 1 mg/mL. Then, 20 µg of the immune MNPs were incubated with the bacterial samples with different concentrations ranging from 1.4×10^1 to 1.4×10^6 CFU/mL for 45 min to form the magnetic bacteria, respectively. After magnetic separation for 2 min to remove the background and washing with 500 µL of PBST (PBS with 0.05% Tween 20), 4 µg of the immune FMSs were incubated with the magnetic bacteria for 45 min to form the fluorescent bacteria. Finally, after magnetic separation for 2 min to remove surplus FMSs and washing with 500 µL of PBST, the fluorescent bacteria were concentrated in 50 µL of PBS.

The fluorescent bacteria were detected using the microfluidic chip and the fluorescent microscopic system. The fluorescent bacteria were continuously injected into the microfluidic chip using a precise syringe pump (Pump 11 elite, Harvard Apparatus, Holliston, MA, US). The light source with the wavelength of 535 nm was used to excite the FMSs on the fluorescent bacteria. The smartphone App was used with the developed fluorescent microscopic system to monitor and count the fluorescent spots when they were flowing through the microchannel, and the mathematical model of this biosensor was established by plotting the number of fluorescent spots with the concentration of the bacteria.

2.6. Detection of *Salmonella typhimurium* in apple juice

Apple juice was purchased from a local supermarket to simulate the real food sample. According to China's national standards on detection of *Salmonella* in foods (GB 4789), 25 mL of apple juice sample were first mixed with 225 mL of sterile PBS and homogenized for 2 min. Then, different concentrations of the target bacteria were added into 1 mL of the mixture, respectively, to obtain the spiked sample containing the target bacteria with the concentration from 1.4×10^1 to 1.4×10^6 CFU/mL. After that, each spiked sample was magnetically separated using the immune MNPs to form the magnetic bacteria, followed by being labeled with the immune FMSs to form the fluorescent bacteria. Finally, the fluorescent bacteria were detected using the microfluidic chip and the fluorescent microscopic system under the optimal conditions to obtain the concentration of the bacteria.

Results and Discussions

3.1. Continuous counting of the fluorescent spots

Accurate counting of the fluorescent spots is crucial to the development of this proposed biosensor. The feasibility of this proposed fluorescent microscopic system for counting the fluorescent spots was first confirmed. The resolution (d) of the microscopic system can be calculated using the following equation:

$$d = 0.61 \times \lambda / N_a \quad (1)$$

where, λ is the wavelength of the emitting light, and N_a is the numerical aperture of the objective lens, i.e., the resolution of this microscopic system was calculated to be around 572 nm, which was much smaller than the size of the fluorescent bacteria (1-3 μ m). Thus, this fluorescent microscopic system was able to identify a single fluorescent bacterium.

To further evaluate the performance of this proposed fluorescent microscopic system, its field depth was also confirmed. The field depth (t) of this microscopic system can be calculated using the following equation:

$$t = (n \times \lambda) / (2 \times N_a^2) + (1000 \times n) / (M \times N_a \times 7) \quad (2)$$

where, n is the refractive index between the objective lens and the sample, and M is the total magnification of the microscope, i.e., the field depth of this microscopic system was calculated to be around 1 μ m, indicating that this microscopic system was able to observe and precise count

1/25 of the total fluorescent spots when they were flowing through the microchannel since the total depth of the channel was 25 μm .

For online identification and counting of the fluorescent spots, the inter-frame difference method was used to identify the flowing fluorescent spots in the difference images and the threshold for image binarization plays an important role. Thus, different grayscale thresholds ranging from 10 to 60 were applied to identify the fluorescent spots in a 2-min-long video of *Salmonella typhimurium* at the concentration of 1.4×10^5 CFU/mL in the microfluidic channel. The exact number of the fluorescent spots was counted by naked eyes to be 62. As shown in Fig. 1, when the thresholds were between 10 and 30, the results for counting the fluorescent spots were around 60 and very close to the actual number. However, when the thresholds were between 40 and 60, the results ranged from 17 to 1 and were obviously different from the actual number. Besides, when the thresholds were less than 10, the fluorescent spots were not identified probably due to the background noises and light field changes. Thus, the optimal threshold of 20 was used in this study.

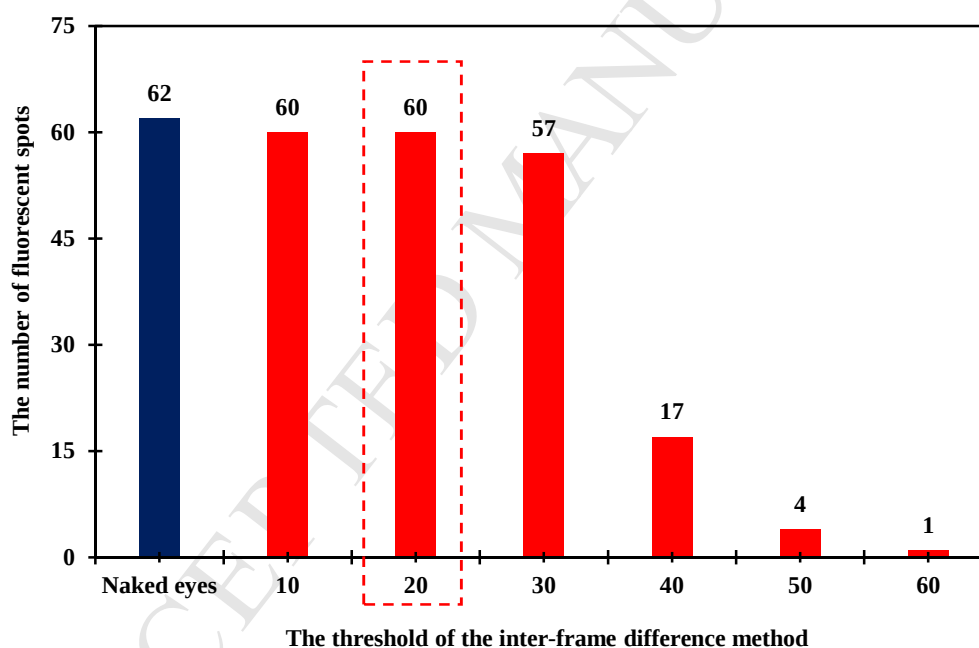


Fig. 1. Optimization of the threshold for the inter-frame difference method.

3.2 Optimization of the immune FMSs

In this study, the immune FMSs were used to label the bacteria for quantitative detection of the target bacteria. The amount of the FMSs on each bacteria has great impact on accurate identification of the bacteria. Therefore, different amounts of the immune FMSs were used to label *Salmonella typhimurium* at the concentration of 1.4×10^5 CFU/mL. After the fluorescent bacteria were injected into the microfluidic chip at the flow rate of 20 $\mu\text{L/h}$, they were continuously monitored and counted for 15 min using the smartphone App and the fluorescent microscopic system. As shown in Fig. 2, when the amount of the FMSs increased from 0.5 μg to 4.0 μg , the

number of the fluorescent spots was counted from 170 to 450 and had only a little increase to 464 when the amount of FMSs was 8.0 μg . However, the theoretical number of the bacteria was ~ 560 , which was around 100 more than the highest counted number. This probably was due to the following reasons: (1) the fluorescent microscopic system could only focus on one focal plane, (2) some target bacteria were lost during magnetic separation; (3) some target bacteria were not labeled with sufficient FMSs resulting in unsuccessful identification of the fluorescent bacteria; (4) some fluorescent bacteria were aggregated into larger ones; and (5) some fluorescent bacteria were not identified due to the relatively high flow rate. Thus, the optimal amount of 4.0 μg for the FMSs was used in this study.

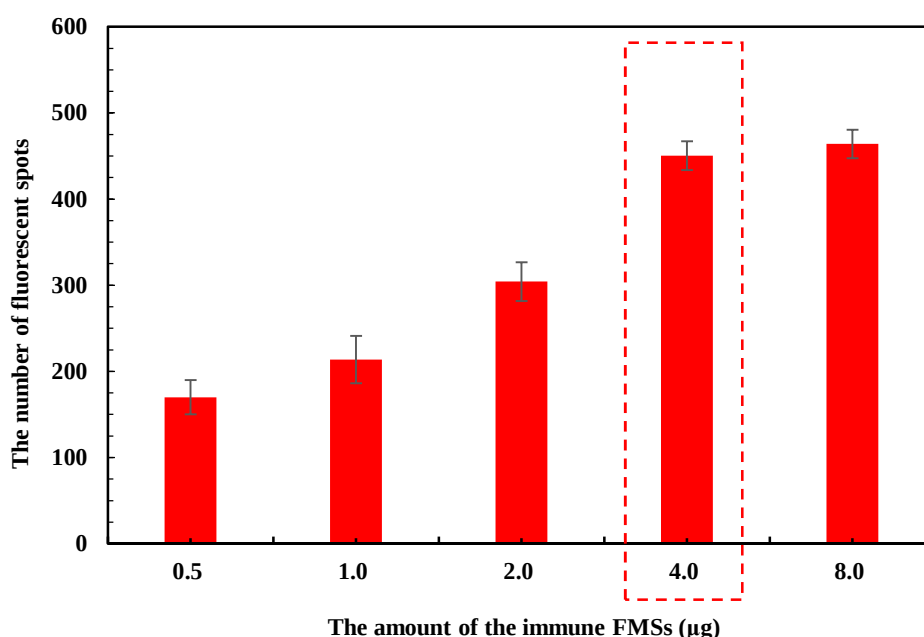



Fig. 2. Optimization of the amount of the immune FMSs.

3.3 Optimization of the flow rate and the detection time


In this study, the flow rate of the fluorescent bacteria and the detection time for counting the fluorescent bacteria have great impact on the accuracy and sensitivity of this proposed biosensor. Different flow rates ranging from 5 $\mu\text{L}/\text{h}$ to 100 $\mu\text{L}/\text{h}$ were applied to inject the fluorescent bacteria into the microfluidic chip for 15 min to count the amount of the target bacteria using the smartphone App. As shown in Fig. 3(a), when the flow rate changed from 5 $\mu\text{L}/\text{h}$ to 20 $\mu\text{L}/\text{h}$, the number of the fluorescent spots was counted to increase from 272 to 870. However, when the flow rate kept increasing to 100 $\mu\text{L}/\text{h}$, the number of the fluorescent spots did not obviously increase, which might be mainly due to the processing limitation of the video stream using the smartphone. Thus, the optimal flow rate of 20 $\mu\text{L}/\text{h}$ was used in this study.

Besides, different detection times were applied to count the fluorescent bacteria using the smartphone App when they were flowing through the microfluidic chip at the flow rate of 20

μL/h for 15 min. The relative standard deviation of three parallel tests on the same concentration of the fluorescent bacteria was used to optimize the detection time. As shown in Fig. 3(b), when the detection time changed from 1 min to 15 min, the relative standard deviation decreased from 4.8% to 1.1%, and when the detection time was increased to 25 min, the relative standard deviation remained the same level. Thus, the optimal detection time of 15 min was used in this study.

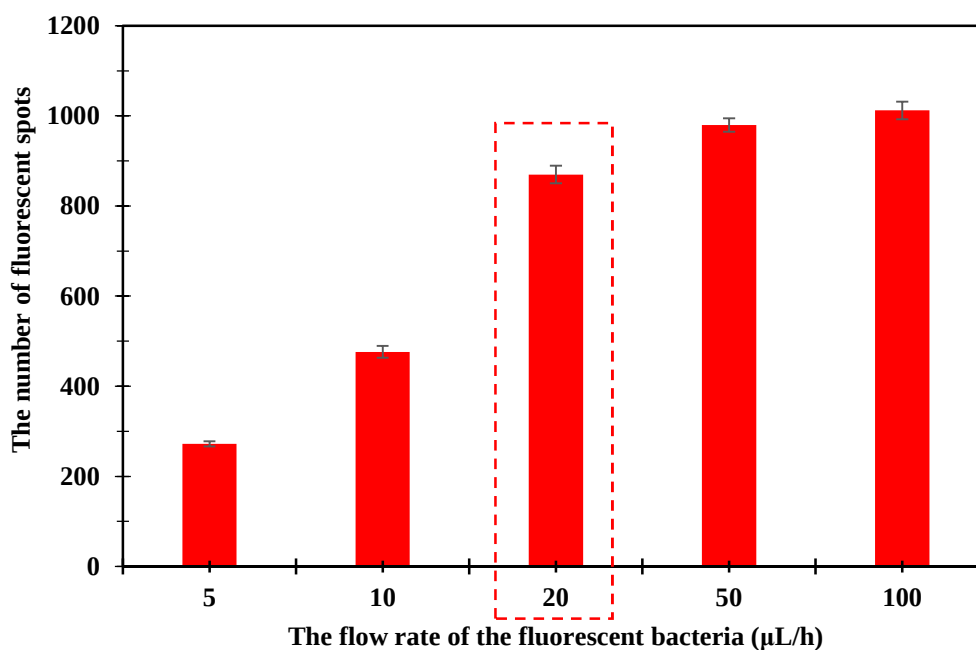

(a)

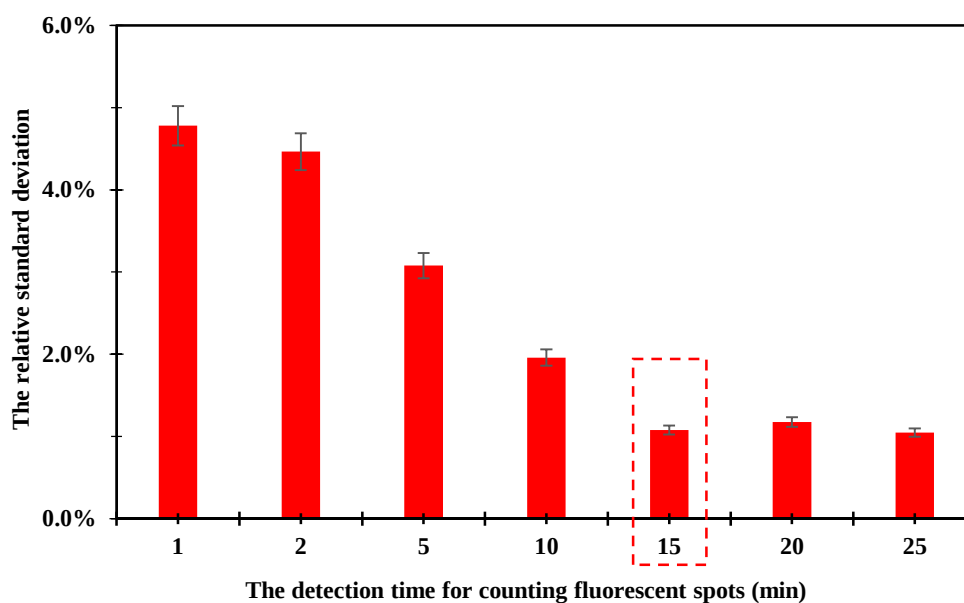

(b)

Fig. 3. (a) Optimization of the flow rate; (b) Optimization of the detection time.

3.4 Detection of *Salmonella typhimurium* using the proposed biosensor


To detect an unknown concentration of *Salmonella typhimurium* in a sample, the calibration curve of this biosensor was established. The target bacteria were first cultured in 5 mL of LB liquid medium at 37°C for 12-16 h. Then, each culture was serially diluted using the sterile PBS to obtain the bacteria with the final concentrations from 1.4×10^1 to 1.4×10^6 CFU/mL. Finally, different concentrations of *Salmonella typhimurium* ranging from 1.4×10^1 to 1.4×10^6 CFU/mL were detected at the optimal conditions using the proposed biosensor. As shown in Fig. 4(a), when the concentration (C) of *Salmonella* changed from 1.4×10^1 to 1.4×10^6 CFU/mL, the number (N) of the fluorescent spots increased from 83 to 844. A good exponential relationship between the number and the concentration was found and could be expressed as:

$$N = 40.97 \times C^{0.21} \quad (3)$$


Based on three times of signal-to-noise ratio, the lower detection limit of this proposed biosensor was calculated to be 58 CFU/mL. The high sensitivity of this biosensor was attributed to the following aspect: (1) the smartphone App based on the inter-frame difference algorithm for accurate and online counting of the fluorescent spots; (2) the fluorescent microscopic system with optical filters for significant amplification of the fluorescent bacteria at a low background noise level; and (3) the cylinder filter at the entry of the microfluidic chip for better dispersion of the fluorescent bacteria and less interferences from the sample background.

To evaluate the specificity of this proposed biosensor, *Listeria monocytogenes*, *E. coli* O157:H7 and *Vibrio parahaemolyticus* were used as non-target bacteria. Both the target bacteria and the non-target bacteria at the same concentration of 10^5 CFU/mL and three negative controls were detected using the proposed biosensor. As shown in Fig. 4(b), the number of the target bacteria was 450, which was much larger than those of the non-target bacteria (70-90), indicating that the proposed biosensor has a good specificity. This is due to the good specificity of the MAbs for separation of *Salmonella typhimurium* and the PABs for labeling of *Salmonella typhimurium*. Besides, as shown in Fig. 4(c)-(e), transmission electron microscopy (TEM) was used to characterize the MNPs and the FMSs and verify the successful forming of the fluorescent bacteria.

Finally, the proposed biosensor was compared with some previously reported smartphone-based biosensors, and the result was shown in Table S1.

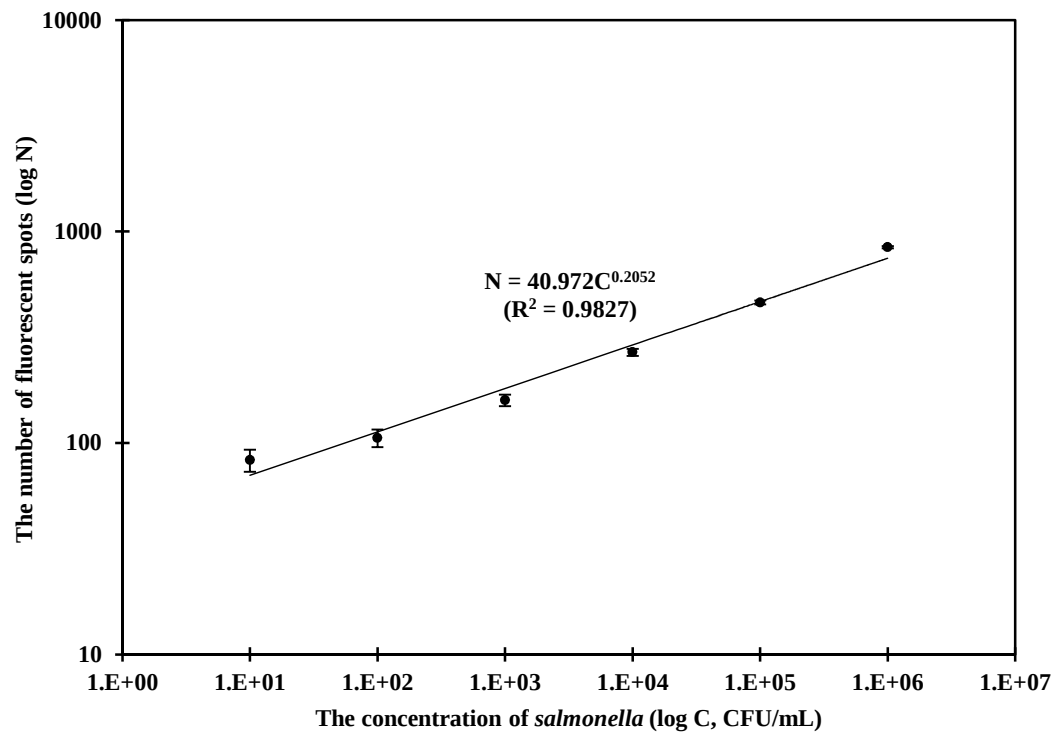

(a)

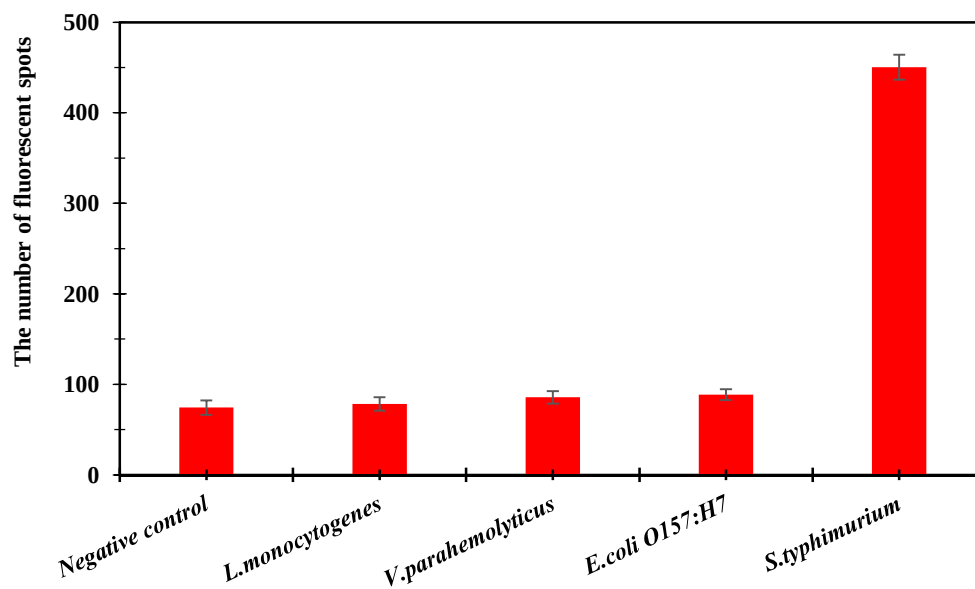

(b)

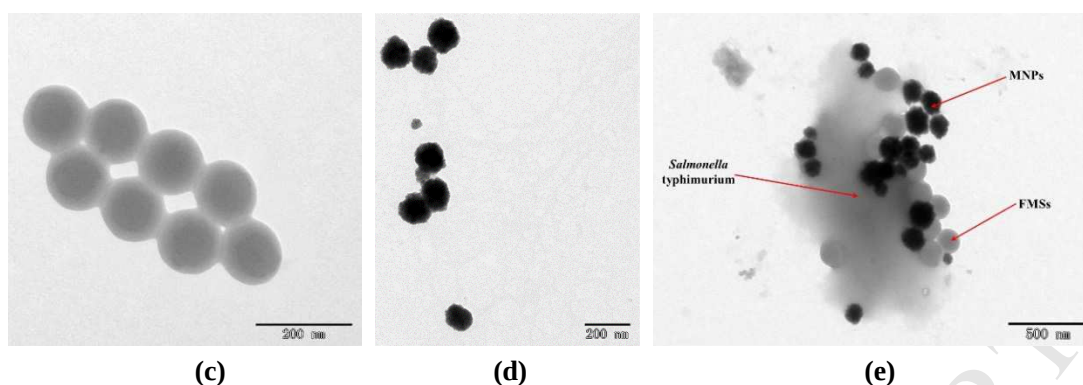


Fig. 4. (a) Calibration curve of this proposed biosensor; (b) The specificity of the proposed biosensor to the non-target bacteria; (c) The TEM image of the FMSs; (d) The TEM image of the MNPs; (e) The TEM image of the fluorescent bacteria.

3.5 Detection of *Salmonella typhimurium* in the spiked apple juice

To further evaluate the applicability of this proposed biosensor for *Salmonella* in real samples, apple juice purchased from local supermarket was used and pretreated based on China's food safety national standards. The spiked samples were prepared using the method described in section 2.6 and finally detected using this proposed biosensor under the optimal conditions. All the samples were parallel tested three times, and all the data were the average of the three experiments. The recovery of the spiked bacteria was calculated as the ratio of the detected concentration of bacteria to the concentration of the spiked bacteria. As shown in Table 1, the recoveries for different concentrations of *Salmonella* in apple juice ranged from 84.82% to 98.39% with an average recovery of 92.64%, indicating that the proposed biosensor was applicable for detection of *Salmonella* in real samples.

Table 1. Detection of *Salmonella typhimurium* in apple juice using the proposed biosensor.

No.	The concentration of the spiked bacteria (CFU/mL)	The number of the fluorescent spots in spiked samples	The detected concentration of bacteria (CFU/mL)	Recovery (%)	CV (%)
1	1.4×10^2	98	126	90.00	6.38
2	1.4×10^3	167	1257	89.79	2.97
3	1.4×10^4	269	13546	96.76	2.93
4	1.4×10^5	477	137746	98.39	2.86
5	1.4×10^6	875	1187480	84.82	2.17

4 Conclusions

In this study, we successfully developed a microfluidic biosensor for online, rapid and sensitive detection of *Salmonella typhimurium* using immunomagnetic separation, fluorescent

labeling, microfluidic chip and smartphone video processing. Under the optimal conditions, the proposed biosensor was able to detect *Salmonella typhimurium* as low as 58 CFU/mL within 2 h, and has shown great potential for on-line monitoring of foodborne pathogens. At present, this biosensor is mainly limited by the video processing speed and image capturing quality. The sensitivity of this biosensor can be further improved using brighter fluorescent materials to label the bacteria for amplification of the fluorescent signals and higher-performance smartphones or devices with faster CPU speed and higher camera resolution to process the video for more accurate and faster counting of the fluorescent bacteria. Besides, online and accurate detection of single bacterium can be expected to realize by combining this biosensing method with microfluidics.

Acknowledgments

This study was supported by the National Natural Science Foundation of China (31802219), Walmart Foundation (SA1703161) and Walmart Food Safety Collaboration Center.

References

- World Health Organization, 2018, <https://www.who.int/en/news-room/fact-sheets/detail/food-safety>
- Altintas, Z., Akgun, M., Kokturk, G., Uludag, Y., 2018. A fully automated microfluidic-based electrochemical sensor for real-time bacteria detection. *Biosensors & Bioelectronics* 100, 541-548.
- Bayramoglu, G., Ozalp, V.C., Dincbal, U., Arica, M.Y., 2018. Fast and Sensitive Detection of *Salmonella* in Milk Samples Using Aptamer-Functionalized Magnetic Silica Solid Phase and MCM-41-Aptamer Gate System. *Acs Biomaterials Science & Engineering* 4(4), 1437-1444.
- Cui, X., Ren, L., Shan, Y., Wang, X., Yang, Z., Li, C., Xu, J., Ma, B., 2018. Smartphone-based rapid quantification of viable bacteria by single-cell microdroplet turbidity imaging. *Analyst* 143(14), 10.1039.C1038AN00456K.
- Duedu, K.O., French, C.E., 2017. Two-colour fluorescence fluorimetric analysis for direct quantification of bacteria and its application in monitoring bacteria growth in cellulose degradation systems. *Journal of Microbiological Methods* 135(Complete), 85-92.
- Fang, X., Liu, Y., Kong, J., Jiang, X., 2010. Loop-Mediated Isothermal Amplification Integrated on Microfluidic Chips for Point-of-Care Quantitative Detection of Pathogens. *Analytical Chemistry* 82(7), 3002-3006.
- Hassan, U., Watkins, N.N., Jr, R.B., Damhorst, G., Bashir, R., 2016. Microfluidic differential immunocapture biochip for specific leukocyte counting. *Nature Protocols* 11(4), 714-726.
- He, X., Hu, C., Guo, Q., Wang, K., Li, Y., Shangguan, J., 2013. Rapid and ultrasensitive *Salmonella Typhimurium* quantification using positive dielectrophoresis driven on-line enrichment and fluorescent nanoparticles label. *Biosensors & Bioelectronics* 42(1), 460-466.
- Jing, J., Wang, X., Ran, C., Ren, Y., Hu, C., Xu, Z., Gang, L.L., 2014. Smartphone based portable bacteria pre-concentrating microfluidic sensor and impedance sensing system. *Sensors & Actuators B Chemical* 193(3), 653-659.
- Jyoti, A., Ram, S., Vajpayee, P., Singh, G., Dwivedi, P.D., Jain, S.K., Shanker, R., 2010. Contamination of surface and potable water in South Asia by *Salmonellae*: Culture-independent quantification with molecular beacon real-time PCR. *Science of the Total Environment* 408(6), 1256-1263.

- 424 Kulinsky, L., Noroozi, Z., Madou, M., 2013. Present technology and future trends in point-of-care
425 microfluidic diagnostics. *Methods in Molecular Biology* 949, 3.
- 426 Lee, J.J., Jeong, K.J., Hashimoto, M., Kwon, A.H., Rwei, A., Shankarappa, S.A., Tsui, J.H., Kohane,
427 D.S., 2014. Synthetic Ligand-Coated Magnetic Nanoparticles for Microfluidic Bacterial Separation
428 from Blood. *Nano Letters* 14(1), 1.
- 429 Lee, K.M., Runyon, M., Herrman, T.J., Phillips, R., Hsieh, J., 2015. Review of Salmonella detection
430 and identification methods: Aspects of rapid emergency response and food safety. *Food Control* 47,
431 264-276.
- 432 Lee, S.C., Kim, M.S., Yoo, K.C., Ha, N.R., Moon, J.Y., Lee, S.J., Yoon, M.Y., 2017. Sensitive
433 fluorescent imaging of Salmonella enteritidis and Salmonella typhimurium using a polyvalent directed
434 peptide polymer. *Microchimica Acta*, 1-10.
- 435 Li, X., Zheng, L., Zhang, H., Xiu, J., Lin, J., 2018. An ultrasensitive fluorescent biosensor using high
436 gradient magnetic separation and quantum dots for fast detection of foodborne pathogenic bacteria.
437 *Sensors & Actuators B Chemical* 265, S0925400518304921.
- 438 Lungu, B., Waltman, W.D., Berghaus, R.D., Hofacre, C.L., 2012. Comparison of a real-time PCR
439 method with a culture method for the detection of Salmonella enterica serotype enteritidis in naturally
440 contaminated environmental samples from integrated poultry houses. *J Food Prot* 75(4), 743-747.
- 441 Malorny, B., Huehn, S., Dieckmann, R., Krämer, N., Helmuth, R., 2009. Polymerase Chain Reaction
442 for the Rapid Detection and Serovar Identification of Salmonella in Food and Feeding Stuff. *Food*
443 *Analytical Methods* 2(2), 81-95.
- 444 Martinez, A.W., Phillips, S.T., Whitesides, G.M., 2008. Three-dimensional microfluidic devices
445 fabricated in layered paper and tape. *Proc Natl Acad Sci U S A* 105(50), 19606-19611.
- 446 Miller, N.D., Davidson, P.M., D'Souza, D.H., 2011. Real-time reverse-transcriptase PCR for
447 Salmonella Typhimurium detection from lettuce and tomatoes. *LWT - Food Science and Technology*
448 44(4), 1088-1097.
- 449 Nie, Z., Deiss, F., Liu, X., Akbulut, O., GM, W., 2010. Integration of paper-based microfluidic devices
450 with commercial electrochemical readers. *Lab on A Chip* 10(22), 3163-3169.
- 451 Rohde, A., Hammerl, J.A., Boone, I., Jansen, W., Fohler, S., Klein, G., Dieckmann, R., Dahouk, S.A.,
452 2017. Overview of validated alternative methods for the detection of foodborne bacterial pathogens.
453 *Trends in Food Science & Technology* 62(Complete), 113-118.
- 454 Shrivastava, S., Lee, W.I., Lee, N.E., 2018. Culture-free, highly sensitive, quantitative detection of
455 bacteria from minimally processed samples using fluorescence imaging by smartphone. *Biosensors &*
456 *Bioelectronics* 109, 90-97.
- 457 Srbova, J., Krulisova, P., Holubova, L., Pereiro, I., Bendali, A., Hamiot, A., Podzemna, V., Macak, J.,
458 Dupuy, B., Descroix, S., 2017. Advanced Immunocapture of Milk-borne Salmonella by Microfluidic
459 Magnetically Stabilized Fluidized Bed. *Electrophoresis* 39(3).
- 460 Stott, S.L., Hsu, C.H., Tsukrov, D.I., Yu, M., Miyamoto, D.T., Waltman, B.A., Rothenberg, S.M., Shah,
461 A.M., Smas, M.E., Korir, G.K., 2010. Isolation of circulating tumor cells using a
462 microvortex-generating herringbone-chip. *Proceedings of the National Academy of Sciences of the*
463 *United States of America* 107(43), 18392-18397.
- 464 Wang, L.J., Sun, R., Vasile, T., Chang, Y.C., Li, L., 2016. High-Throughput Optical Sensing
465 Immunoassays on Smartphone. *Analytical Chemistry* 88(16), 8302-8308.
- 466 Wang, Q.Y., Kang, Y.J., 2016. Bioprobes Based on Aptamer and Silica Fluorescent Nanoparticles for
467 Bacteria Salmonella typhimurium Detection. *Nanoscale Research Letters* 11(1), 150.

- 468 Wang, Y., Duncan, T.V., 2017. Nanoscale sensors for assuring the safety of food products. *Curr Opin*
469 *Biotechnol* 44(Complete), 74-86.
- 470 Whitesides, G.M., 2013. Cool, or simple and cheap? Why not both? *Lab on A Chip* 13(1), 11-13.
- 471 Yang, L., Li, Y., 2006. Simultaneous detection of *Escherichia coli* O157:H7 and *Salmonella*
472 *Typhimurium* using quantum dots as fluorescence labels. *Analyst* 131(3), 394-401.
- 473 Zangheri, M., Cevenini, L., Anfossi, L., Baggiani, C., Simoni, P., Di, N.F., Roda, A., 2015. A simple
474 and compact smartphone accessory for quantitative chemiluminescence-based lateral flow
475 immunoassay for salivary cortisol detection. *Biosensors & Bioelectronics* 64, 63-68.
- 476 Zhang, G., Ali, L., Gill, V., Tatavarthy, A., Deng, X., Hu, L., Brown, E.W., Hammack, T.S., 2017.
477 Development and Validation of a Cultural Method for the Detection and Isolation of *Salmonella* in
478 Cloves. *Journal of Food Protection* 80(3), 376.
- 479 Zheng, L., Cai, G., Wang, S., Liao, M., Li, Y., Lin, J., 2019. A microfluidic colorimetric biosensor for
480 rapid detection of *Escherichia coli* O157:H7 using gold nanoparticle aggregation and smart phone
481 imaging. *Biosensors & Bioelectronics* 124-125, 143-149.
- 482 Zhu, H., Mavandadi, S., Coskun, A.F., Yaglidere, O., Ozcan, A., 2011. Optofluidic fluorescent imaging
483 cytometry on a cell phone. *Analytical Chemistry* 83(17), 6641-6647.

Highlights

1. Smartphone video processing was first time used to count fluorescent bacteria.
2. A facile microscopic system was developed to amplify fluorescent signals.
3. This biosensor was able to detect *Salmonella* as low as 58 CFU/mL in 2 h.
4. The mean recovery of *Salmonella* in spiked apple juice was ~93%.

Authors Contribution

In this paper, Wang, S. contributed to the software development, experiment execution and data collection, original draft. Zheng, L contributed to the methodology and formal analysis. Cai, G contributed to the hardware and visualization. Liu, N, Liao, M, Li, Y and Zhang, X contributed to the project administration and funding acquisition. Lin, J contributed to the conceptualization, supervision and writing - review & editing.

Declaration of interests

☒ The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

☐ The authors declare the following financial interests/personal relationships which may be considered as potential competing interests:

--