



Tunable 3D nanofibrous and bio-functionalised PEDOT network explored as a conducting polymer-based biosensor

Lingyin Meng, Anthony P.F. Turner¹, Wing Cheung Mak^{*}

Biosensors and Bioelectronics Centre, Division of Sensor and Actuator Systems, Department of Physics, Chemistry and Biology, Linköping University, SE-581 83, Linköping, Sweden

ARTICLE INFO

Keywords:

Conducting polymer
Bio-nano-PEDOT
Nanofibre
Carboxylic acid functionalisation
Biosensor interface

ABSTRACT

Conducting polymers that possess good electrochemical properties, nanostructured morphology and functionality for bioconjugation are essential to realise the concept of all-polymer-based biosensors that do not depend on traditional nanocatalysts such as carbon materials, metal, metal oxides or dyes. In this research, we demonstrated a facile approach for the simultaneous preparation of a bi-functional PEDOT interface with a tunable 3D nanofibrous network and carboxylic acid groups (i.e. Nano-PEDOT-COOH) via controlled co-polymerisation of EDOT and EDOT-COOH monomers, using tetrabutylammonium perchlorate as a soft-template. By tuning the ratio between EDOT and EDOT-COOH monomer, the nanofibrous structure and carboxylic acid functionalisation of Nano-PEDOT-COOH were varied over a fibre diameter range of 15.6 ± 3.7 to 70.0 ± 9.5 nm and a carboxylic acid group density from 0.03 to $0.18 \mu\text{mol cm}^{-2}$. The nanofibres assembled into a three-dimensional network with a high specific surface area, which contributed to low charge transfer resistance and high transduction activity towards the co-enzyme NADH, delivering a wide linear range of 20–960 μM and a high sensitivity of $0.224 \mu\text{A } \mu\text{M}^{-1} \text{ cm}^{-2}$ at the Nano-PEDOT-COOH50% interface. Furthermore, the carboxylic acid groups provide an anchoring site for the stable immobilisation of an NADH-dependent dehydrogenase (i.e. lactate dehydrogenase), via EDC/S-NHS chemistry, for the fabrication of a Bio-Nano-PEDOT-based biosensor for lactate detection which had a response time of less than 10 s over the range of 0.05–1.8 mM. Our developed bio-Nano-PEDOT interface shows future potential for coupling with multi-biorecognition molecules via carboxylic acid groups for the development of a range of advanced all-polymer biosensors.

1. Introduction

Poly(3,4-ethylenedioxythiophene) (PEDOT), an emerging conducting polymer (CP) with extraordinary redox reversibility, biocompatibility and electrochemical properties, shows considerable potential as an interfacing material in biosensing to bridge between the organic electronics world and bioelectronics, since PEDOT possess sufficient similarities in its organic chemical nature with biological molecules to facilitate the concept of all-polymer biosensors (Inal et al., 2018). One key to merge organic electronics and bioelectronics is to establish an effective signal transduction interface between biomolecules and PEDOT. However, the lack of reactive functional groups for bioconjugation and the relatively low electrochemical catalytic activity of pristine PEDOT, has hindered the development of a direct PEDOT-based electrochemical biosensors with bioelectrochemical signal transduction

between the catalytic enzyme and PEDOT. In most of the reported PEDOT sensors and biosensors, nanomaterials were used as dopants to prepare PEDOT-composites, including carbon materials (carbon nanotubes, graphene), metal or metal oxides (Au, TiO_2) and dyes (Prussian blue) (Lin et al., 2010; Meng et al., 2019; Wang et al., 2018). The PEDOT mainly served as a conducting matrix while the bioelectrochemical signal transduction still relied on the doped carbon, metal or dye nanocatalyst. Thus, pure PEDOT interfaces possessing functionality for both bioconjugation and good electrochemical activity are still largely absent while remaining critical for future advances in biosensing.

Functionalisation endows conducting polymers (CPs) with functional groups that facilitate effective immobilisation of biorecognition molecules for biosensing applications. In recent years, much effort has been devoted to design functionalised CPs with active chemical groups, such as carboxylic acid (Luo et al., 2009), amine (Godeau et al., 2016),

^{*} Corresponding author..

E-mail address: wing.cheung.mak@liu.se (W.C. Mak).

¹ Current address: , SATM, Cranfield University, Bedfordshire, MK430AL, UK.


phosphorylcholine (Goda et al., 2015), sialic acid (Hai et al., 2017) etc. Of these, the functionalisation of CPs with carboxylic acid groups delivers more profound value compared to the others because of the variety of biological molecules, such as nucleotides and proteins (antibodies and enzymes), that can be covalently immobilised on the CP transducer interface, via ethyl(dimethylaminopropyl) carbodiimide (EDC)/N-hydroxysulfosuccinimide (NHS) chemistry. The introduction of carboxylic acid groups can be achieved either by using carboxylic acid containing molecules as a dopant during polymerisation or by using their derivatives (e.g. EDOT-COOH) as monomers. Carboxylic acid containing molecules, such as citrate (Meng et al., 2019a) and hyaluronic acid (Mantione et al., 2016) can be incorporated into the CP matrix as a dopant to compensate for the backbone charge, thus endowing the resulting CP interface with a high $-\text{COOH}$ density. However, this strategy suffers from several drawbacks including potential leakage of dopant, difficulty in controlling the amount of dopant and destruction of the CP's bulk properties and conductivity. Alternatively, CP derivatives bearing carboxylic acid groups have been used for the preparation of a close-structured planar functionalised PEPOT film coupled with DNA and/or antibodies for indirect affinity biosensing (Luo et al., 2009; Sekine et al., 2011).

Advances in nanomaterials based on conventional carbon (CNTs, graphene) and metal nanomaterials (Au, Pt nanoparticles) used in bioelectronics (Jin et al. 2018a, 2018b) encourages the exploration of nanostructured CPs. Nanostructured CPs inherit prominent physical-chemical properties from their bulk polymer equivalents, while acquiring beneficial nanomaterial characteristics such as large active


surface area to promote catalytic reactions. While bulk CP interfaces may suffer from hysteresis and sluggish electron/mass transfer, nanostructured CPs are capable of realising effective electrode interface kinetics and facilitate signal transfer due to their high surface area and porous structure, leading to faster response times and high sensitivity for the resulting sensors (Lu et al., 2019). Various CP structures, including nano and microspheres (Nguyen et al., 2015; Vagin et al., 2016), hollow-capsules (Wannapob et al., 2015), nanowires (Travas-Sejdic et al., 2014) and nanotubes (Lin et al., 2016), have been implemented via sacrificial hard-template (e.g. calcium carbonate and polystyrene), soft-template (e.g. surfactants) or template-free (dimer as seeds) fabrication. Although these techniques yield a controlled nanostructured CP interface, the demand for a high density of functional groups for bio-recognition elements still remains unfulfilled.

In this study, we developed an innovative bioorganic/organic polymer bio-interface possessing functionality for bioconjugation and good electrochemical properties for signal transduction towards an all-polymer-based biosensor. By combining functionalisation and nanostructure formation strategies, we demonstrate herein a facile approach for the simultaneous preparation of a bi-functional PEDOT interface with a tunable 3D nanofibrous network and carboxylic acid groups (i.e. Nano-PEDOT-COOH) via controlled co-polymerisation of EDOT and EDOT-COOH monomers using tetrabutylammonium perchlorate (TBAP) as a soft-template (Scheme 1a). The ratio between EDOT and EDOT-COOH was evaluated to modulate the resulting nanostructure morphologies and density of the carboxylic acid groups. The 3D nanofibrous network endowed the Nano-PEDOT-COOH interface with enhanced

a Nano-PEDOT-COOH

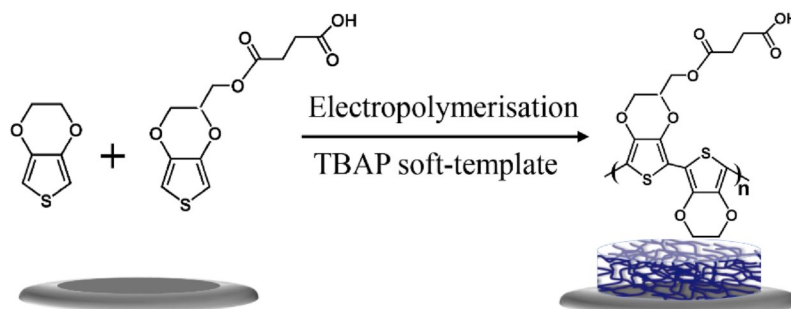

b Bio-Nano-PEDOT

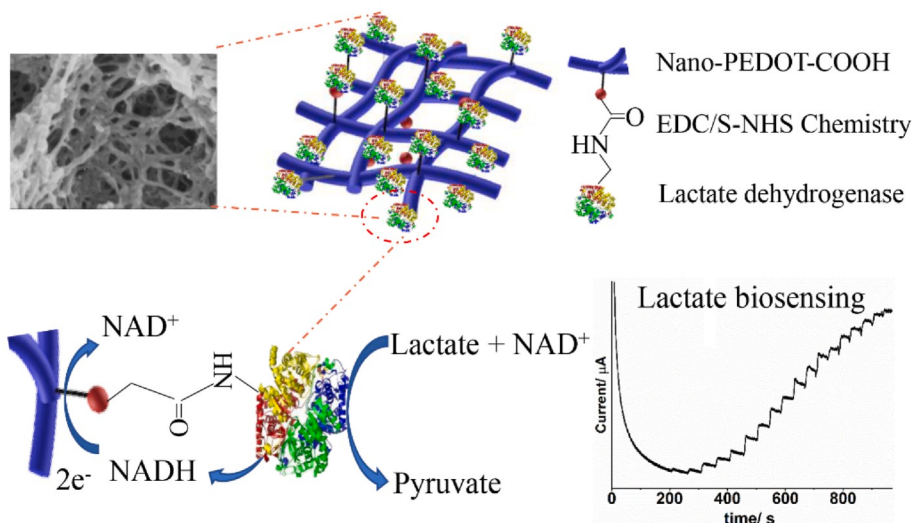

Scheme 1. Schematic of (a) 3D Nano-PEDOT-COOH network preparation via co-polymerisation of EDOT and EDOT-COOH monomers using TBAP as a soft-template; (b) Bio-Nano-PEDOT: Nano-PEDOT-COOH bio-conjugation with lactate dehydrogenase via EDC/S-NHS chemistry for lactate biosensing.

charged transfer and catalytic activity towards the electrochemical oxidation of NADH, which may be ascribed to the relatively large 3D active surface area and porous structure. Furthermore, the carboxylic acid functionality provided anchoring sites for the stable immobilisation of a NADH-dependent dehydrogenase (i.e. lactate dehydrogenase) via EDC/S-NHS chemistry for the fabrication of a Bio-Nano-PEDOT-based biosensor for lactate detection that delivers a fast response time and high sensitivity (Scheme 1b). This strategy also provides a generic design for electrocatalytic devices based on the many available NADH-dependent dehydrogenase enzymes.

2. Experimental section

2.1. Materials

3, 4-ethylenedioxythiophene (EDOT), potassium ferricyanide ($K_3[Fe(CN)_6]$), potassium ferrocyanide ($K_4[Fe(CN)_6]$), hexaammineruthenium(III) chloride ($[Ru(NH_3)_6]Cl_3$), hexaammineruthenium(II) chloride ($[Ru(NH_3)_6]Cl_2$), toluidine blue O (TBO), potassium chloride (KCl), tetrabutylammonium perchlorate (TBAP), anhydrous acetonitrile (CH_3CN), ethanolamine (EA, $NH_2CH_2CH_2OH$), sodium L-lactate, N-(3-dimethylaminopropyl)-N'-ethylcarbodiimide hydrochloride (EDC), N-hydroxysulfosuccinimide (S-NHS), fluorescein isothiocyanate conjugated bovine serum albumin (FITC-BSA), L-lactate dehydrogenase (LDH, from porcine heart, 250 U mg^{-1}), ascorbic acid (AA) and uric acid (UA) were purchased from Sigma-Aldrich (USA). 3,4-ethylenedioxythiophene derivative bearing 4-methoxy-4-oxobutanoic acid (EDOT-COOH, 1H NMR spectrum in Fig. S1) was provided by Shanghai Zhixing Chemical Technology (China). β -nicotinamide adenine dinucleotide reduced disodium salt hydrate (NADH) was bought from VWR (Sweden). Human serum (Type AB) was purchased from PAA Laboratories GmbH (Austria). β -Nicotinamide adenine dinucleotide solution (oxidised form, NAD^+), disodium hydrogen phosphate monohydrate ($Na_2HPO_4 \cdot H_2O$) and potassium dihydrogen phosphate (KH_2PO_4) were purchased from Merck (Darmstadt, Germany). 0.1 M phosphate buffer solutions (PBS 7.4) were prepared by mixing Na_2HPO_4 and KH_2PO_4 stock solution. All chemicals were of analytical grade and used without any further treatment. Deionised water from Milli-Q System was used throughout.

2.2. Electropolymerisation of nano-PEDOT-COOH

Glassy-carbon electrodes (GCE, diameter 3 mm; surface area 0.0707 cm^2) were carefully polished with 0.3 and 0.05 μm aluminum slurries and rinsed with deionised water under sonication. A mixture of monomer solution with a final concentration of 10 mM was prepared by dissolving EDOT and EDOT-COOH monomers at different concentration in acetonitrile containing 0.1 M TBAP. Different nanostructured PEDOT-COOH electrodes were electropolymerised in the 10 mM monomer solution (containing 2.5, 5, 7.5, 10 mM of EDOT-COOH) using a constant potential of 1.2 V (Ag/Ag $^+$ as reference) with fixed charge of 20 mC. After rinsing with anhydrous acetonitrile, the resulting nanostructured PEDOT-COOH electrodes were dried in the air and denoted as Nano-PEDOT-COOH25%, Nano-PEDOT-COOH50%, Nano-PEDOT-COOH75% and Nano-PEDOT-COOH100%, respectively. Indium tin oxide coated glass (ITO) with a confined surface area of $1 \times 0.6 cm^2$ was used as an alternative working electrode during electropolymerisation for the characterisation experiments.

2.3. Bio-conjugation of nano-PEDOT-COOH

The Nano-PEDOT-COOH interface was activated by applying 20 μL of EDC (50 mM) and S-NHS (50 mM) for 30 min followed by rinsing with water. 10 μL of enzyme LDH (2 mg mL^{-1}) was applied on the activated Nano-PEDOT-COOH surface and incubated for 2 h. The unreacted carboxylic acid groups were then deactivated by applying 10 μL of ethanolamine (1 mM) for 30 min. Finally, the LDH bio-conjugated

Nano-PEDOT-COOH (Bio-Nano-PEDOT) electrodes were rinsed with PBS solution to remove excess enzymes. In order to examine the charge effect on the NADH response, ethanolamine was used to neutralise the carboxylic acid groups of the Nano-PEDOT-COOH to suppress the repulsion effect between the carboxylic acid groups and NADH.

In parallel, fluorescence microscopy was used to characterise the bio-conjugation of Nano-PEDOT-COOH using FITC-BSA. PEDOT-COOH50%/ITO was treated with 100 μL of EDC (50 mM) and sulfo-NHS (50 mM) for 30 min. After rinsing with water, 40 μL of FITC-BSA (1 mg mL^{-1}) was placed on the activated PEDOT-COOH surface for 2 h. Excess FITC-BSA were then washed with water and dried under a gentle stream of nitrogen gas. As control, PEDOT-COOH50%/ITO was treated with the same procedure with the exception of the activation of the carboxylic acid groups by EDC/S-NHS.

2.4. Characterisations and electrochemical measurements

Scanning electron microscopy (SEM) images were recorded using a LEO 155 Gemini (Zeiss, Germany) electron microscope. Fourier transform infrared (FTIR) spectroscopy was performed using a VERTEX spectrometer (Bruker, USA) equipped with an attenuated total reflection (ATR) measuring cell. The density of carboxylic acid groups on different Nano-PEDOT-COOH biointerfaces were examined via toluidine blue O (TBO) staining assay (Meng et al., 2019a). In brief, PEDOT-COOH electrodes (0.6 cm^2) were incubated in 2 mM TBO solution (0.1 mM KOH) for 2 h. Under alkaline conditions, the carboxylic acid groups deprotonated to bind with the positively charged TBO molecules with a ratio of 1:1. Nonspecifically bound TBO molecules were removed from the PEDOT-COOH surface by rinsing with 0.1 mM KOH solution several times. Finally, the samples were soaked in 5 mL 50% acetic acid for 30 min to desorb the TBO molecules. Absorbance spectroscopy was performed using a UV-vis spectrophotometer (UV-2450, Shimadzu, Japan) at 631 nm with an established standard calibration curve for TBO concentration vs. Absorbance (Regression equation: $A = 0.0533 + 0.0589R$, $R^2 = 0.997$).

All electrochemical measurements were performed using a CompactStat potentiostat (Ivium, Netherlands) at room temperature with a conventional three-electrode system comprising a platinum wire as the counter electrode, a glassy carbon working electrode, and a silver/silver chloride (Ag/AgCl) electrode as the reference. Electrochemical impedance spectroscopy (EIS) measurements were performed at PEDOT-COOH electrodes in 2 mM $Fe(CN)_6^{3-/4-}$ in 0.1 M KCl over the frequency range 0.01 Hz–100 kHz and at 5 mV amplitude. The impedance spectra were then fitted to an equivalent electrical circuit via ZSimpWin Software (AMETEK Scientific instruments).

3. Results and discussion

3.1. Nanofibrous structure and carboxylic acid functionality of nano-PEDOT-COOH

The surface morphology of various Nano-PEDOT-COOH films with different ratio of EDOT-COOH were examined using SEM (Fig. 1a and b). Fig. 1a shows that all Nano-PEDOT-COOH films possess a network of interconnected nanofibres with varying fibre diameters supported by a spherical hub-like structure. With an increased amount of EDOT-COOH (from 25% to 100%), the aspect ratio of the resulting nanofibres decreased resulting in a relatively closed-structured film, which is ascribed to the hindrance due to the carboxylic acid side chains causing a steric effect. The high-magnification SEM images in Fig. 1b show the nanofibrous morphology of the Nano-PEDOT-COOH25%–100%. The Nano-PEDOT-COOH25% and Nano-PEDOT-COOH50% were composed of a three-dimensional network assembly of a relatively open-structured and thinner nanofibres with a fibre diameter of 15.6 ± 3.7 nm and 25.5 ± 6.5 nm, respectively. In contrast, the Nano-PEDOT-COOH75% and Nano-PEDOT-COOH100% were composed of relatively close-structured

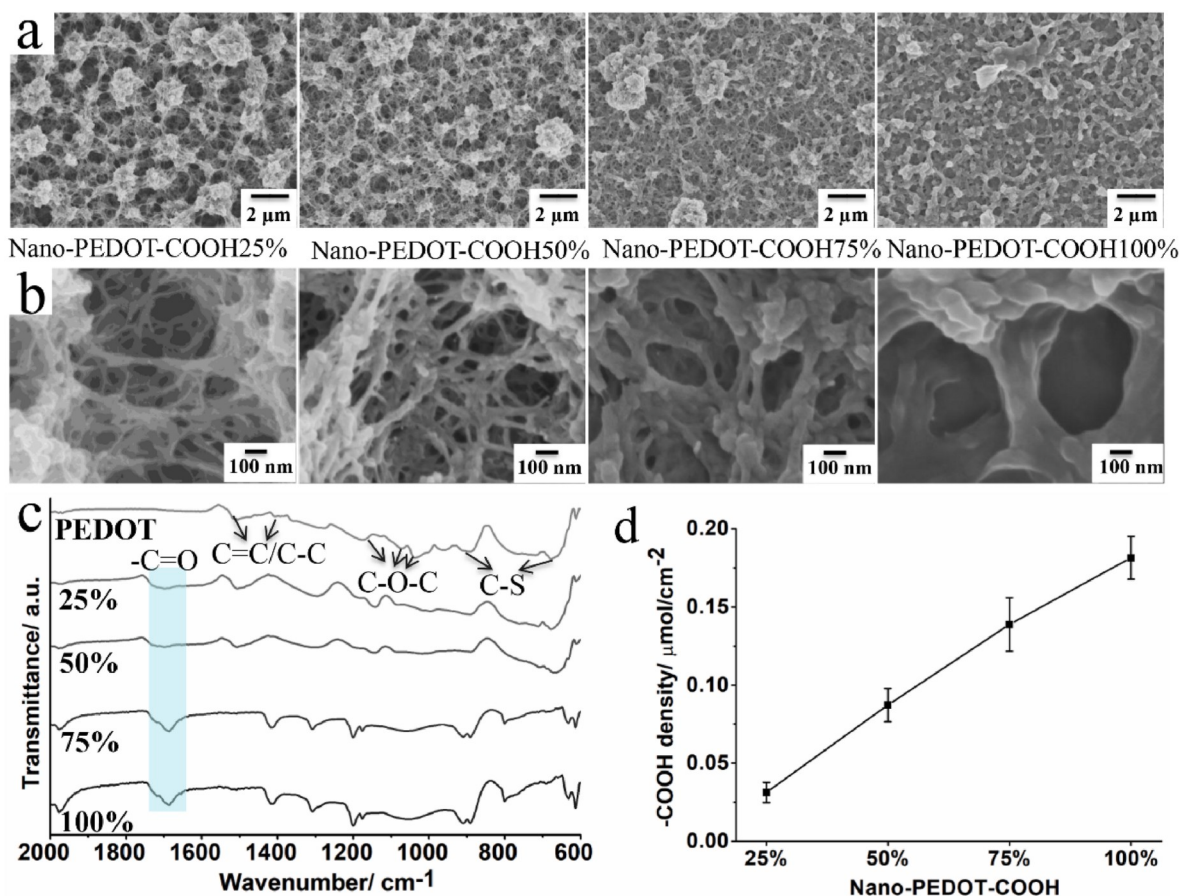


Fig. 1. (a) SEM images of Nano-PEDOT-COOH with different amounts of EDOT-COOH ranging from 25 to 100%; (b) High magnification SEM images; (c) FTIR spectra of PEDOT and nano-PEDOT-COOH25–100%; (d) Carboxylic acid density on Nano-PEDOT-COOH25–100% surface estimated by the TBO staining technique.

and thicker nanofibres with an increased fibre diameter of 35.0 ± 7.6 nm and 70.0 ± 9.5 nm, respectively. In addition to the nanofibrous structure, the presence of carboxylic acid groups was examined using ATR-FTIR (Fig. 1c). The existence of bands at 1750 and 1680 cm^{-1} related to -C=O for PEDOT-COOH25%–100%, implies the successful co-

polymerisation of EDOT-COOH into the Nano-PEDOT-COOH matrix. The total surface density of carboxylic acid groups on the Nano-PEDOT-COOH surfaces was quantified by the TBO staining technique as previously reported (Meng et al., 2019a; Rödiger et al., 2011). Fig. 1d displays the linear increase of carboxylic acid group density from 0.03 $\mu\text{mol cm}^{-2}$

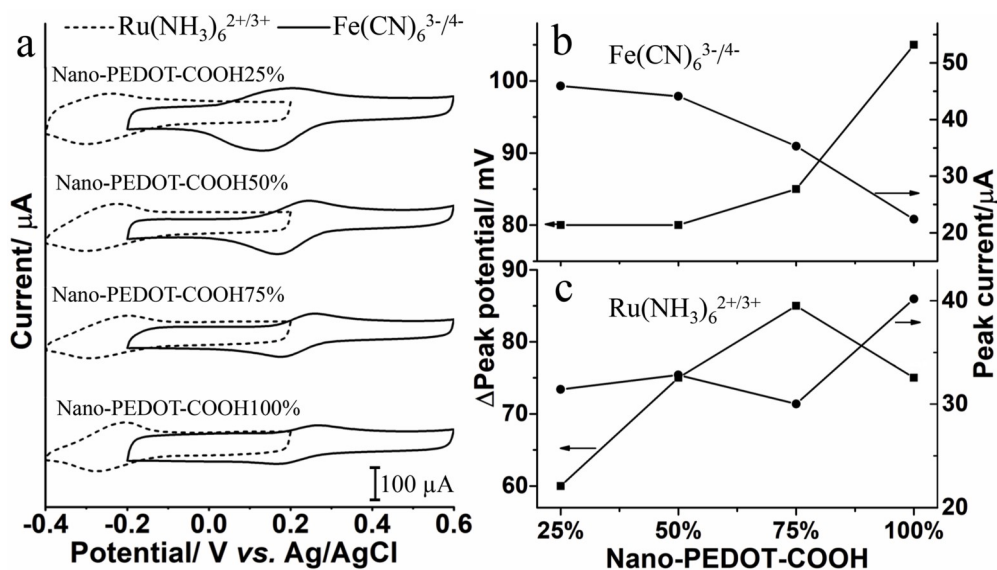


Fig. 2. (a) Cyclic voltammograms of different Nano-PEDOT-COOH modified electrodes in 2 mM $\text{Fe(CN)}_6^{3-/4-}$ (solid curve), $\text{Ru(NH}_3)_6^{2+/3+}$ (dashed curve) in 0.1 M KCl; Corresponding redox peak potential and peak current of different Nano-PEDOT-COOH modified electrodes to 2 mM $\text{Fe(CN)}_6^{3-/4-}$ (b) and $\text{Ru(NH}_3)_6^{2+/3+}$ (c) in 0.1 M KCl. Scan rate of 50 mV s^{-1} .

for PEDOT-COOH25% to $0.18 \mu\text{mol cm}^{-2}$ for PEDOT-COOH100%. These results reveal that the higher ratio of EDOT-COOH monomer contributes to higher carboxylic acid density on the resulting Nano-PEDOT-COOH surface and an increased diameter of the resulting nanofibrous structure.

3.2. Effects of nanofibrous structure and carboxylic acid groups on nano-PEDOT-COOH electrochemical properties

The electrochemical properties of the series of Nano-PEDOT-COOH polymers with different nanostructure and carboxylic acid density were investigated by using two differently charged redox probes (i.e., negatively-charged $\text{Fe}(\text{CN})_6^{3-/4-}$ and positively-charged $\text{Ru}(\text{NH}_3)_6^{2+/3+}$). As shown in Fig. 2a, all Nano-PEDOT-COOH modified electrodes exhibit quasi-reversible peaks with slightly different peak separations (ΔE_p) and peak current (I_p) for both the redox probes. For the negatively-charged $\text{Fe}(\text{CN})_6^{3-/4-}$ probe (Fig. 2b), the Nano-PEDOT-COOH25% showed the smallest ΔE_p of 80 mV and the highest anodic peak current of 45.9 μA , while a further increased portion of EDOT-COOH in the Nano-PEDOT-COOH matrix resulted in increases of ΔE_p and decreases of peak current, reaching a ΔE_p of 105 mV and an anodic peak current of 22.4 μA . These electrochemical characteristics can be ascribed to the successful incorporation of negatively-charged carboxylic acid groups on the Nano-PEDOT-COOH interfaces repulsing the $\text{Fe}(\text{CN})_6^{3-/4-}$ probe, as well as the aspect ratio of the nanofibre structure (i.e. thicker and shorter length fibres) and relatively dense spatial arrangement limiting the accessible active surface of the nanofibres.

In contrast, the electrochemical characteristics of Nano-PEDOT-COOH towards positively-charged $\text{Ru}(\text{NH}_3)_6^{2+/3+}$ can be seen in Fig. 2c. In the range of Nano-PEDOT-COOH25–75%, the nanostructure dominated the electrochemical properties; the Nano-PEDOT-COOH interface composed of a nanofibrous structure with a higher aspect ratio (thinner and longer) showed a gradual reduction of ΔE_p from 85 mV to 60 mV with improved electrode kinetics. Meanwhile, despite the fact that the Nano-PEDOT-COOH100% was composed of nanofibres with a relatively lower aspect ratio, it showed a ΔE_p of 75 mV; the electrostatic attraction of the positively-charged $\text{Ru}(\text{NH}_3)_6^{2+/3+}$ by the relatively high carboxylic acid density compensated the effect of the nano-structure. At the same time, the anodic peak current of Nano-PEDOT-COOH25–75% showed a relatively steady value of $\sim 30 \mu\text{A}$, while the peak current of Nano-PEDOT-COOH100% increased to $\sim 40 \mu\text{A}$.

Electrochemical impedance spectroscopy (EIS) was performed to evaluate the electrochemical properties for various Nano-PEDOT-COOH interfaces, as shown in Fig. 3. An equivalent electrical circuit with adequate fit to the original data (inset of Fig. 3a) was developed to model the behavior of Nano-PEDOT-COOH electrodes in $\text{Fe}(\text{CN})_6^{3-/4-}$ in 0.1 M KCl, comprising the solution resistance (R_{sol}), the electron transfer resistance between the redox couple and the electrode interface (R_{ct}), the electronic bulk capacitance (C_d), the finite-length Warburg diffusion impedance (Z_D) and the diffusion impedance of the redox probes in the solution (Z_W) (Sundfors and Bobacka, 2004; Sundfors et al., 2002). Fig. 3b summarises the fitted parameters for various Nano-PEDOT-COOH interfaces. The R_{sol} for different Nano-PEDOT-COOH interfaces remained similar. The R_{ct} increased gradually as the carboxylic acid groups of the Nano-PEDOT-COOH increased, which is in good agreement with the trends in ΔE_p and peak current obtained from the CVs shown in Fig. 2b. The trend in R_{ct} as a function of EDOT-COOH provides evidence of the successful incorporation of carboxylic acid groups into the Nano-PEDOT-COOH interfaces because of the increased electrostatic repulsion effect and relatively dense spatial interface with a higher EDOT-COOH component. Moreover, the C_d decreased as the carboxylic acid groups of the Nano-PEDOT-COOH increased, which is ascribed to the relatively dense spatial arrangement resulting in limited accessible active surface area at high amounts of EDOT-COOH.

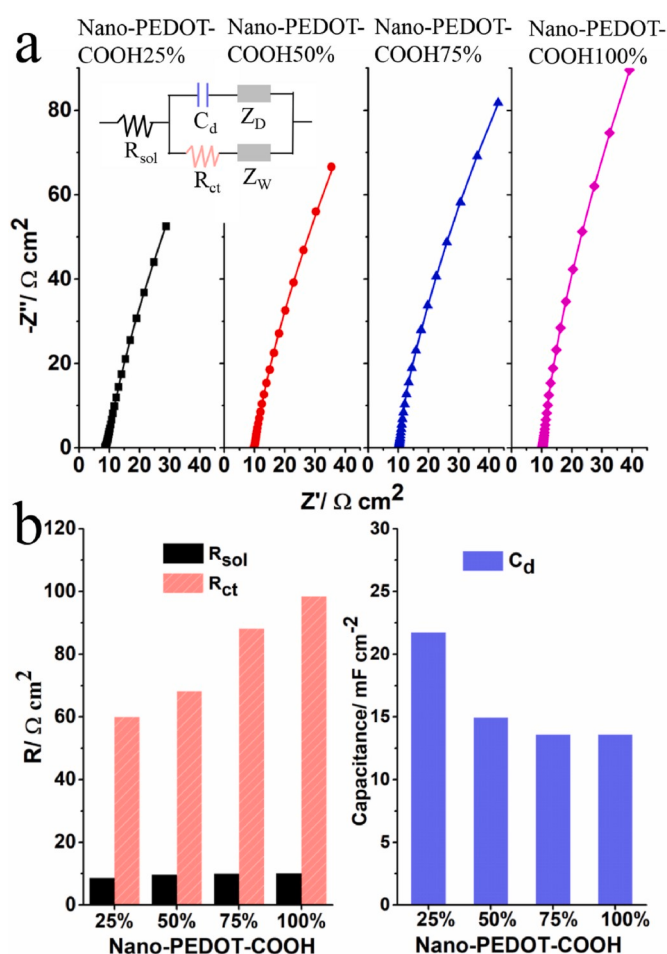


Fig. 3. (a) EIS analysis of different Nano-PEDOT-COOH modified electrodes in Nyquist plots obtained in 2 mM $\text{Fe}(\text{CN})_6^{3-/4-}$ in 0.1 M KCl, inset is the equivalent circuits; (b) Corresponding curve fitting parameters.

3.3. Effect of the nanofibrous structured PEDOT on NADH sensing

The carboxylic acid moieties in the Nano-PEDOT-COOH primarily served as an intermediate functional group for bioconjugation that was reacted during covalent coupling of biomolecules or neutralised by the capping reagent. Therefore, the electrochemical performance of the resulting Bio-Nano-PEDOT-based biosensor was mainly dominated by the net effect of the nano-structure morphology. NADH was chosen as the model to evaluate the biomolecules transducing property at the Nano-PEDOT-COOH interface, since NADH is one of the most important co-enzymes in the human body, and can be potentially coupled to a wide range of NADH-dependent dehydrogenases for applications in biosensing and bioelectrocatalysis (Meng et al., 2018). Fig. 4a shows cyclic voltammograms of various Nano-PEDOT-COOH/GCE and bare GCE in the presence of 2 mM NADH in 0.1 M PBS (pH = 7.4). Compared to bare GCE, all Nano-PEDOT-COOH modified electrodes showed negatively shifted oxidation peak potentials and increased peak currents. In order to investigate the net effect of the nano-structured morphology towards NADH electrochemical oxidation, it was necessary to eliminate the electrostatic repulsion effect caused by the carboxylic acid groups. This was achieved by using ethanolamine (EA) to neutralise the carboxylic acid groups by conversion into hydroxy groups with EDC/S-NHS chemistry. Fig. 4a shows the net effect of the nano-structured morphologies of various EA-neutralised Nano-PEDOT-COOH25–100% electrodes with further negatively shifted oxidation peak potentials and increased peak currents. Fig. 4b summarises the key parameters from the CVs. We observed gradual decreases in peak potential from 0.53 V to

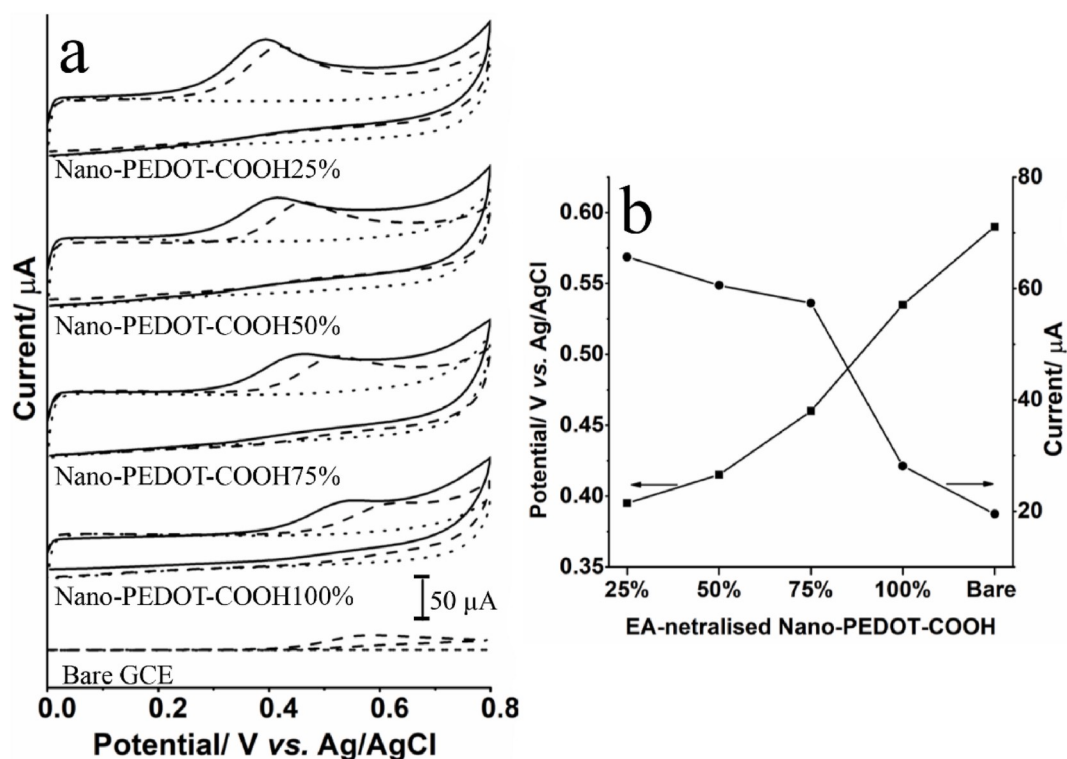


Fig. 4. (a) CV responses of different Nano-PEDOT-COOH modified electrodes with (dash: un-neutralised, solid: EA-neutralised) and without (dotted line) 2 mM NADH in 0.1 M PBS (pH = 7.4); (b) Corresponding NADH oxidation peak potentials and peak currents of EA-neutralised Nano-PEDOT-COOH modified electrodes to 2 mM NADH in 0.1 M PBS (pH = 7.4). Scan rate of 50 mV s⁻¹.

0.40 V and increases in peak current from 28.1 μA to 68.5 μA, when the EA-neutralised Nano-PEDOT-COOH was composed of a nanofibrous structure with a higher aspect ratio (i.e. Nano-PEDOT-COOH25% has the highest aspect ratio nanofibrous structure, and Nano-PEDOT-COOH100% has the lowest aspect ratio nanofibrous structure in Fig. 1b). This result demonstrated that the nanofibrous structure with a high aspect ratio endowed the EA-neutralised Nano-PEDOT-COOH interface with improved NADH sensing. In general, both the EA-neutralised Nano-PEDOT-COOH25% and Nano-PEDOT-COOH50% showed good electrochemical performance for detection of NADH (where Nano-PEDOT-COOH25% was slightly better). However, for further biosensor development work, the key is to establish an effective signal transduction interface between the biomolecules and PEDOT. Therefore, it is necessary to compromise on the electrochemical performance with respect to the number of carboxylic acid functional groups for immobilisation of biomolecules. With this consideration, Nano-PEDOT-COOH50% was chosen as a balance between a carboxylic acid group density of 0.08 μmol cm⁻² (Fig. 1d) and good NADH oxidation properties with a relatively low peak potential of 0.42 V and a high peak current of 60.6 μA.

3.4. NADH transduction and biomolecule conjugation for lactate biosensing

The amperometric response of NADH on EA-neutralised Nano-PEDOT-COOH50% was measured at 0.42 V by successive addition of NADH in 0.1 M PBS (pH 7.4). As can be seen from Fig. 5a, EA-neutralised Nano-PEDOT-COOH50% modified electrodes exhibited a fast response to the successive additions of NADH and reached a 95% steady-state current within 5 s. The corresponding calibration curves are shown in Fig. 4b. The response current of EA-neutralised Nano-PEDOT-COOH50% modified electrode was linearly proportional to NADH concentration over a wide linear range of 20–960 μM ($R^2 = 0.997$). The sensitivity for NADH sensing was calculated to be 0.224 μA μM⁻¹ cm⁻²,

with a detection limit of 2.04 μM (3σ/slope). The analytical performance was compared with other conventional carbon-based (graphene, CNTs), polymer-based electrodes and their composites with metal nanoparticles described in the literature (Table S1). It is important to note that those reports are mainly based on nano-catalyst modified electrodes such as graphene, CNT, metal nanoparticles and advanced polymer composite doped with nano-catalysts, while our 3D nanofibrous PEDOT network without nanocatalyst could detect NADH at a relatively low oxidation peak potential with comparable sensitivity and wide linear range, due to its high surface area and porous structure to facilitate signal transduction. Moreover, PEDOT possesses several inherent advantages such as light weight, flexibility, ease of fabrication, low cost and good biocompatibility as a sensing interface.

A Bio-Nano-PEDOT-based biosensor was constructed using NADH-dependent lactate dehydrogenase (LDH) coupled with the Nano-PEDOT-COOH50%. The control experiment (Fig. 5c) displayed no observable response to successive injections of 0.2 and 1 mM lactate with the naked Nano-PEDOT-COOH50% electrode. In order to visualise the successful conjugation of biomolecules onto the Nano-PEDOT-COOH50% interface, a fluorescently-labelled FITC-BSA protein was used as a model that covalently bound onto the Nano-PEDOT-COOH50% via EDC/S-NHS chemistry and then the interface was examined using fluorescence microscopy. Fig. 5d shows the fluorescence micrograph of the resulting FITC-BSA conjugated Nano-PEDOT-COOH50% with a strong, well-covered and homogenous distribution of the fluorescence signal, which indicates a good immobilisation efficiency, while the control experiment without EDC/S-NHS activation of carboxylic acid groups showed a weak and insignificant fluorescence signal, indicating that the immobilisation was not due to non-specific physical adsorption onto the Nano-PEDOT-COOH interface.

After bioconjugation of LDH, the analytical performance of the LDH-Nano-PEDOT biosensor for lactate detection was evaluated. Fig. 5e shows typical current-time curve of the LDH-Nano-PEDOT biosensor responses to successive addition of lactate at 0.45 V in 0.1 M PBS (pH

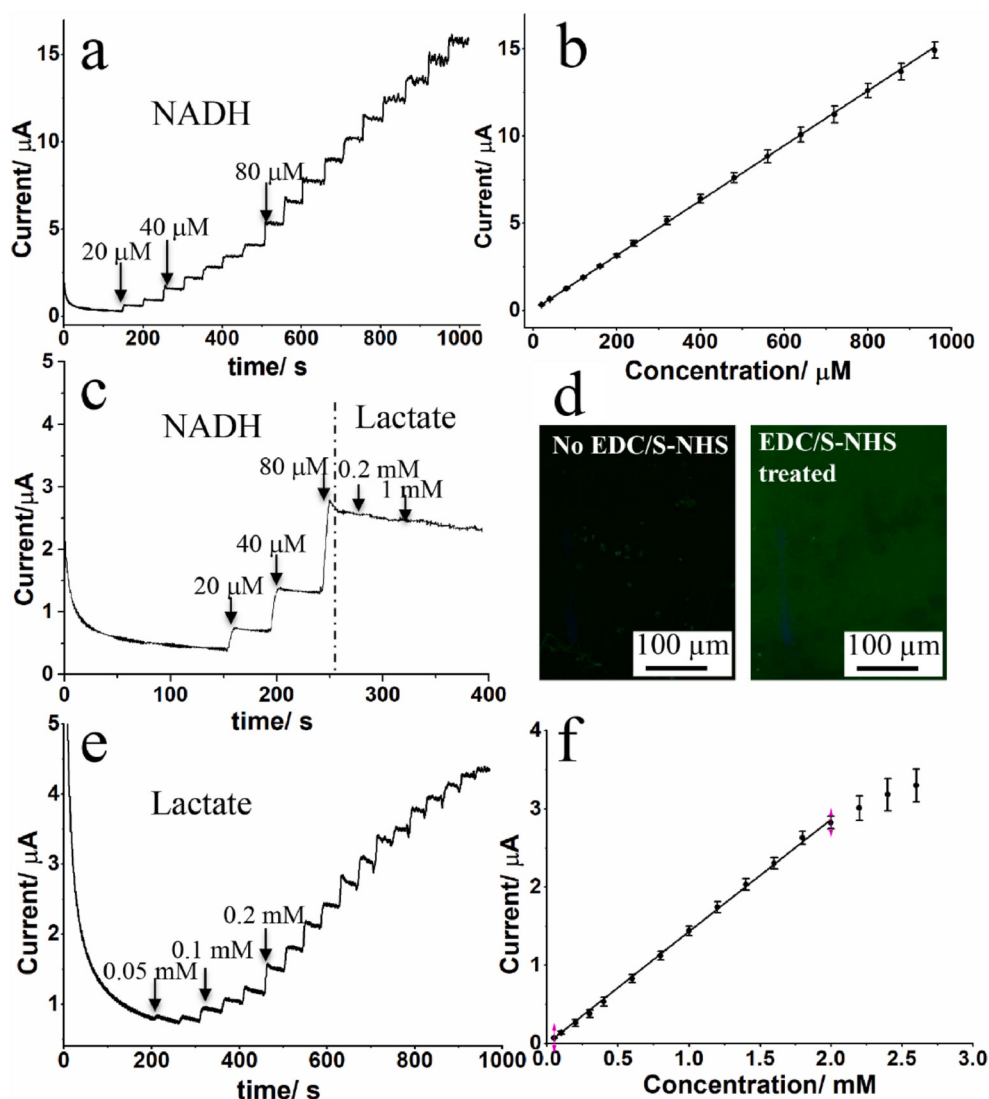


Fig. 5. (a) Current-time response curve of EA-neutralised Nano-PEDOT-COOH50% at 0.420 V for successive injections of NADH in 0.1 M PBS (pH 7.4); (b) Corresponding calibration curve for NADH sensing, $n = 3$; (c) Current-time response curve of EA-neutralised Nano-PEDOT-COOH50% at 0.420 V for varying concentration of NADH and lactate; (d) Fluorescence microscopy image of a FITC-BSA Bio-Nano-PEDOT interface without (left) and with (right) treatment; (e) Current-time response curve of LDH-Nano-PEDOT at 0.450 V for successive injection of lactate in 0.1 M PBS (pH 7.4); (f) Corresponding calibration curve for lactate biosensing, $n = 3$.

7.4) containing 3 mM NAD^+ . A stepwise increase in current response was observed for each successive addition of lactate, reaching 95% of the steady-state current within 10 s. The steady state current response (Fig. 5f) was linear with respect to lactate concentration over the range of 0.05–1.8 mM ($R^2 = 0.995$) with a sensitivity of $20.26 \mu\text{A mM}^{-1} \text{cm}^{-2}$. The biosensing mechanism is based on a relay bioelectrochemical signal transduction between the LDH (bioorganic molecule) and the Nano-PEDOT (organic molecule), during which LDH catalyses the conversion of lactate to pyruvate and NADH in the presence of NAD^+ , followed by the Nano-PEDOT electrode catalytically oxidising NADH to generate a signal current. The linear range of the all-polymer lactate biosensor was comparable, or in some cases better, than reported values of other advanced nanomaterial-based biosensors in the literature, such as $\text{Fe}_3\text{O}_4/\text{MWCNTs}$ ($\sim 300 \mu\text{M}$) (Teymourian et al., 2012), pTTCA/MWNT ($5\text{--}90 \mu\text{M}$) (Rahman et al., 2009), metal nitride/graphene nanohybrids ($10\text{--}220 \mu\text{M}$) (Wen et al., 2011) and Au NPs silicate network ($100\text{--}600 \mu\text{M}$) (Jena and Raj, 2006). The selectivity, storage-stability and practical applicability of the fabricated lactate biosensor in serum samples were examined and the results are shown in Fig. S2. The selectivity of the biosensor was evaluated against the common interfering electroactive species uric acid and ascorbic acid, which showed insignificant responses. The stability of the biosensor was tested for 7 days storage in PBS at 4°C , and it retained 95% of its signal responses after storage for 5 days, while the signal responses decreased to 78% at 7 days, likely due to

enzyme degradation. We demonstrated the practical use of the biosensor for detection of various concentration of lactate in spiked serum samples and obtained a high recovery value of (95.8–101%). Thus, we successfully demonstrated a Bio-Nano-PEDOT (all-bioorganic/organic polymer) biosensor that did not require metal/carbon nanocatalysts by combining functionalisation and nanostructure formation strategies, thus providing a sound basis for future development of a range of advanced NADH-dehydrogenase coupled all-polymer-based wearable and flexible biosensors.

4. Conclusions

We have demonstrated a facile approach for simultaneous preparation of a Nano-PEDOT-COOH interface with a tunable 3D nanofibrous network and carboxylic acid groups via controlled co-polymerisation of EDOT and EDOT-COOH monomers at different ratios using TBAP as a soft-template. The nanofibres assembled into a three-dimensional porous network with high specific surface area, which resulted in a low charge transfer resistance for probes used with CV and EIS, and excellent oxidation of the co-enzyme NADH over a wide linear range and with high sensitivity. The carboxylic acid groups on the Nano-PEDOT-COOH (organic molecule) provided anchoring sites for the stable immobilisation of NADH-dependent LDH (bioorganic molecule) via EDC/S-NHS chemistry for the fabrication of Bio-Nano-PEDOT lactate

biosensor, thus realising an all-polymer biosensor without the use of traditional nanocatalysts such as carbon materials, metal, metal oxides or dyes. This Bio-Nano-PEDOT interface provides a sound basis for future development of a wide range of advanced NADH-dehydrogenase coupled biosensors fabricated entirely from polymers. This paves the way for the creation of new bioorganic electronic devices for sensing, biotransformation and energy generation.

Declaration of competing interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper

CRediT authorship contribution statement

Lingyin Meng: Conceptualization, Formal analysis, Writing - original draft. **Anthony P.F. Turner:** Formal analysis. **Wing Cheung Mak:** Conceptualization, Formal analysis, Writing - review & editing, Supervision.

Acknowledgments

The authors would like to acknowledge the Swedish Research Council (VR-2015-04434) and the China Scholarship Council (File no. 201606910036) for generous financial support to carry out this research.

Appendix A. Supplementary data

Supplementary data to this article can be found online at <https://doi.org/10.1016/j.bios.2020.112181>.

References

Goda, T., Toya, M., Matsumoto, A., Miyahara, Y., 2015. *ACS Appl. Mater. Interfaces* 7 (49), 27440–27448.

- Godeau, G., Darmanin, T., Guittard, F., 2016. *J. Appl. Polym. Sci.* 133 (11).
- Hai, W., Goda, T., Takeuchi, H., Yamaoka, S., Horiguchi, Y., Matsumoto, A., Miyahara, Y., 2017. *ACS Appl. Mater. Interfaces* 9 (16), 14162–14170.
- Inal, S., Rivnay, J., Sui, A.-O., Malliaras, G.G., McCulloch, I., 2018. *Acc. Chem. Res.* 51 (6), 1368–1376.
- Jena, B.K., Raj, C.R., 2006. *Anal. Chem.* 78 (18), 6332–6339.
- Jin, H., Guo, H., Gao, X., Gui, R., 2018a. *Sensor. Actuator. B Chem.* 277, 14–21.
- Jin, H., Zhao, C., Gui, R., Gao, X., Wang, Z., 2018b. *Anal. Chim. Acta* 1025, 154–162.
- Lin, K.-C., Tsai, T.-H., Chen, S.-M., 2010. *Biosens. Bioelectron.* 26 (2), 608–614.
- Lin, Y.-F., Li, C.-T., Ho, K.-C., 2016. *J. Mater. Chem. A* 4 (2), 384–394.
- Lu, C.-F., Liao, S.-F., Wang, K.-H., Chen, C.-T., Chao, C.-Y., Su, W.-F., 2019. *Nanoscale* 11 (43), 20977–20986.
- Luo, S.-C., Xie, H., Chen, N., Yu, H.-h., 2009. *ACS Appl. Mater. Interfaces* 1 (7), 1414–1419.
- Mantione, D., del Agua, I., Schaafsma, W., Diez-Garcia, J., Castro, B., Sardon, H., Mecerreyes, D., 2016. *Macromol. Biosci.* 16 (8), 1227–1238.
- Meng, L., Turner, A.P.F., Mak, W.C., 2018. *Biosens. Bioelectron.* 120, 115–121.
- Meng, L., Turner, A.P.F., Mak, W.C., 2019a. *ACS Appl. Mater. Interfaces* 11 (37), 34497–34506.
- Meng, L., Turner, A.P.F., Mak, W.C., 2019. *Biotechnol. Adv.* 39, 107398.
- Nguyen, V.-Q., Schaming, D., Martin, P., Lacroix, J.-C., 2015. *ACS Appl. Mater. Interfaces* 7 (39), 21673–21681.
- Rahman, M., Shiddiky, M.J., Rahman, M.A., Shim, Y.-B., 2009. *Anal. Biochem.* 384 (1), 159–165.
- Rödiger, S., Ruhland, M., Schmidt, C., Schröder, C., Grossmann, K., Böhm, A., Nitschke, J.R., Berger, I., Schimke, I., Schierack, P., 2011. *Anal. Chem.* 83 (9), 3379–3385.
- Sekine, J., Luo, S.C., Wang, S., Zhu, B., Tseng, H.R., Yu, H., 2011. *Adv. Mater.* 23 (41), 4788–4792.
- Sundfors, F., Bobacka, J., 2004. *J. Electroanal. Chem.* 572 (2), 309–316.
- Sundfors, F., Bobacka, J., Ivaska, A., Lewenstam, A., 2002. *Electrochim. Acta* 47 (13–14), 2245–2251.
- Teymourian, H., Salimi, A., Hallaj, R., 2012. *Biosens. Bioelectron.* 33 (1), 60–68.
- Travas-Sejdic, J., Aydemir, N., Kannan, B., Williams, D., Malmström, J., 2014. *J. Mater. Chem. B* 2 (29), 4593–4609.
- Vagin, M.Y., Jeerapan, I., Wannapob, R., Thavarungkul, P., Kanatharana, P., Anwar, N., McCormac, T., Eriksson, M., Turner, A.P.F., Jager, E.W.H., Mak, W.C., 2016. *Electrochim. Acta* 190, 495–503.
- Wang, G., Morrin, A., Li, M., Liu, N., Luo, X., 2018. *J. Mater. Chem. B* 6 (25), 4173–4190.
- Wannapob, R., Vagin, M.Y., Jeerapan, I., Mak, W.C., 2015. *Langmuir* 31 (43), 11904–11913.
- Wen, Z., Cui, S., Pu, H., Mao, S., Yu, K., Feng, X., Chen, J., 2011. *Adv. Mater.* 23 (45), 5445–5450.