

Accepted Manuscript

Microwave-assisted preparation of N-doped carbon dots as a biosensor for electrochemical dopamine detection

Yuliang Jiang, Bingxiang Wang, Fandian Meng, Yixiang Cheng, Chengjian Zhu


PII: S0021-9797(15)00377-X
DOI: <http://dx.doi.org/10.1016/j.jcis.2015.04.016>
Reference: YJCIS 20390

To appear in: *Journal of Colloid and Interface Science*

Received Date: 21 March 2015
Accepted Date: 9 April 2015

Please cite this article as: Y. Jiang, B. Wang, F. Meng, Y. Cheng, C. Zhu, Microwave-assisted preparation of N-doped carbon dots as a biosensor for electrochemical dopamine detection, *Journal of Colloid and Interface Science* (2015), doi: <http://dx.doi.org/10.1016/j.jcis.2015.04.016>

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting proof before it is published in its final form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

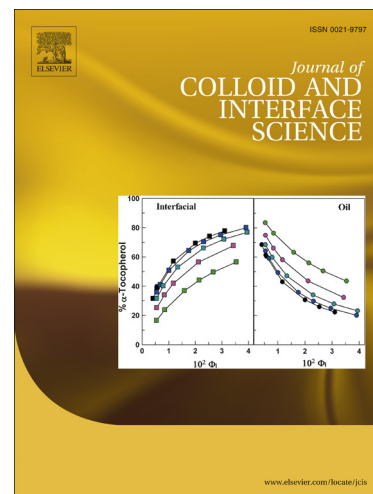

Microwave-assisted preparation of N-doped carbon dots as a biosensor for electrochemical dopamine detection

Yuliang Jiang^{a,b}, Bingxiang Wang^b, Fandian Meng^a, Yixiang Cheng^{a,*}, Chengjian Zhu^{a,*}

^a Key Lab of Mesoscopic Chemistry of MOE, School of Chemistry and Chemical Engineering, Nanjing University, Nanjing 210093, China.

^b School of Chemistry and Materials Science, Nanjing Normal University, Nanjing 210097, China.

Abstract: A new N-doped carbon dots (NCDs) could be prepared by using the microwave-assisted technique within 10 minutes without the need for any solvent or catalyst. The NCDs exhibited a highly sensitive electrochemical response toward dopamine (DA) in Phosphate Buffered Saline (PBS) (pH=6.5). The detection limit of DA was calculated by differential pulse voltammetry (DPV) as low as 1.2×10^{-9} mol/L with a linear dynamic range of 5.0×10^{-8} to 8.0×10^{-6} mol/L. These results suggested that this new NCDs could be effectively used for the direct and rapid detection of trace levels of DA in human serum and urine samples.

Keywords: Microwave-assisted technique, N-doped carbon dots, Electrochemical detection, Differential pulse voltammetry

1.Introduction

The neurotransmitter dopamine (DA) plays an important role in the central nervous system of biological organisms [1], but abnormal levels of DA in the brain can often lead to Parkinson's disease, Alzheimer's disease, or schizophrenia [2-6]. Therefore, the development of highly selective and sensitive analytical methods on the direct and rapid determination of trace dopamine is of great significance. So far, various analytical methods, such as liquid chromatography, chemiluminescence, capillary electrophoresis, fluorescence techniques[7-11] have been used for

*Corresponding authors. E-mail: yxcheng@nju.edu.cn, cjzhu@nju.edu.cn; Fax: +86-25-88317761;

Tel: +86-25-83686508

dopamine determination. However, most of these techniques are limited by time consuming, high

cost, complicated equipment requirements, lack of sensitivity and selectivity. Recently, electrochemical techniques have received considerable interest for the real-time detection of DA at low concentration condition due to their simple, high sensitivity and rapid response. It is well known that bare electrodes for detection of DA is ineffective[12], therefore there is an urgent need for developing novel sensors, which can offer high sensitivity and selectivity for the direct detection of DA at low concentration in the presence of interfering compounds.

As a new member of the carbon family, carbon quantum dots (CQDs) can exhibit excellent optical and electro-optical properties due to their quantum confinement and edge effect [13], which could be considered as a promising material in replacement of traditional semiconductor quantum dots and organic dyes in various applications, including sensors, bioimaging, photovoltaics, and energy-conversion devices [14-19] due to low toxicity, good photo-stability, excellent biocompatibility, high chemical stability [20-23]. So far, many efforts have been devoted to developing methods for the preparation of CQDs including laser ablation [24], electrochemical synthesis [25], chemical oxidation [26], microwave synthesis [27], and solvothermal methods [28]. Among these methods, microwave-assisted irradiation technique can effectively offer both rapid and uniform heating of the reaction medium, which can shorten the reaction time and greatly improve the product yield and purity [29-33]. Therefore, microwave-assisted irradiation technique can be regarded as a simple, direct and efficient approach for the preparation of CQDs[34-36].

In this study, we described a novel and large-scale strategy for the high-yield synthesis of NCDs based on the microwave irradiation technique without any solvent or catalyst by using the starting product diethanolamine (DEA). Herein, DEA can serve as both a carbon source and a nitrogen source. Furthermore, the resulting NCDs possess a large number of hydroxyl and amino

groups on the surface of NCDs which can attract the electroactive compound dopamine (DA) and act as a novel electrochemical sensor for the direct detection of trace levels of DA in human serum and urine samples with a high sensitivity and excellent selectivity.

2. Materials and methods

2.1. Reagents and chemicals

Both dopamine and ascorbic acid in 99% purity were purchased from Sigma-Aldrich Chemical Company. Ethanol, ethyl acetate (EA), tetrahydrofuran (THF), dimethylformamide (DMF), dimethyl sulfoxide (DMSO) and diethanolamine (DEA) were commercially available and directly used without further purification. Phosphate Oxygen-free nitrogen was bubbled through the cell prior to each experiment. All experiments were carried out at room temperature.

2.2. Apparatus

The particle size distributions of the NCDs were observed using transmission electron microscopy (TEM). The IR spectrum of NCDs was measured by a Nicolet Nexus 670 Fourier transform infrared (FT-IR) spectrophotometer with a resolution of 4 cm^{-1} and scan times of 64. IR sample was prepared by applying the NCDs ethanol solution on the surface of a KBr wafer and then dried under an infrared lamp. Ultraviolet-Visible (UV-vis) absorption spectrum was measured with a Varian Cary 50 spectrophotometer at 1 cm of the light path length. X-ray photoelectron spectroscopy (XPS) was carried out on a PHI 5000 Versa probe electron spectrometer from ULVAC-PHI. All electrochemical measurements were carried out with a CHI660E (Shanghai CH Instrument Company, China). Cyclic voltammetry (CV) and differential pulse voltammetry (DPV) were performed with a conventional three-electrode system with glassy carbon electrode (GCE) as the working electrode (WE), a platinum counter electrode (CE) and an Ag/AgCl (sat. KCl) reference electrode (RE). Microwave reactor (Yu Hua Instrument, China,

1kW, 2.45 GHz).

2.3. Microwave-assisted preparation of NCDs

Typical preparation of NCDs were described as follows: 5 mL DEA was put into a 25 mL quartz ampoule, and then the ampoule was placed inside the microwave reactor and irradiated for 10 min (1 kW, 2.45 GHz). After cooling to room temperature, the resulting dark-yellow transparent solution is mixed with ultra pure water and centrifuged at a 10,000 rpm for 10 min, and then further filtered by a 0.22 μm syringe filter to remove the large particles. The obtained NCDs were concentrated by freezing (-80°C) and drying under vacuum.

3. Results and discussion

3.1. Characterization of NCDs

The solubility of the resulting NCDs were tested in several common solvents which was carried out by dissolving 10 mg of NCDs in 5 mL of water, ethanol, EA, THF, DMF and DMSO (Fig. S1), respectively. In each case, NCDs could form a clear solution in these solvents. As evident from the TEM image of NCDs (Fig. 1a), it could be clearly observed that the NCDs could be highly dispersed in aqueous solution, and their nanoparticle diameters are distributed in the range of 8-25 nm with an average diameter of 16.4 nm (Fig. 1b).

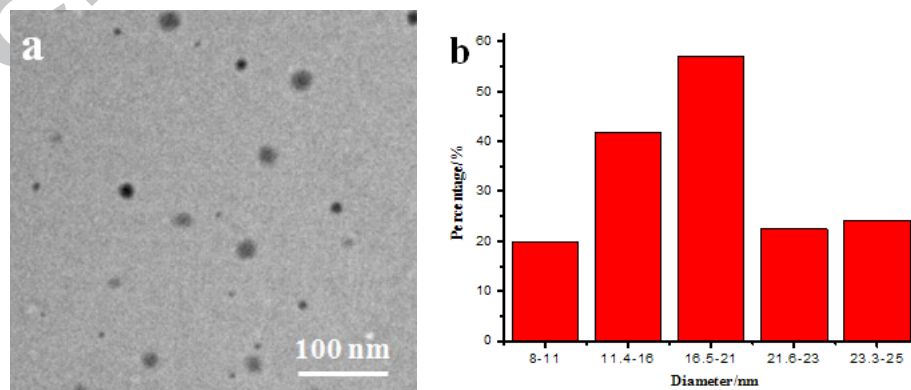


Fig. 1. (a) TEM image of NCDs; (b) Particle size distribution of NCDs

Fig. 2 provides the FT-IR spectrum of the NCDs with some main absorption peaks such as

the O–H stretching vibration at 3363 cm^{-1} , C–H stretching vibrations at 2980 and 2870 cm^{-1} , strong C=O stretching vibration at 1643 cm^{-1} , C=C stretching vibrations at 1571 cm^{-1} , the characteristic stretch band of the amine C=N bond at 1470 cm^{-1} , indicating that the surface of NCDs is rich in negatively charged carboxylic acid groups and dopamine molecule can bind to NCDs particles through electrostatic interaction or hydrogen bond. Element analysis data (C 72.65%, N 5.670%, O 20.78%) of NCDs were performed by XPS technique (Fig. S3) which can further confirm this NCDs containing carbon, nitrogen and oxygen elements as FT-IR spectrum described above. The UV-Vis absorption spectra of NCDs and DEA (Fig. S4) revealed that only the NCDs can exhibit an absorption peak at 285 nm arising from a $\pi\text{--}\pi^*$ transition of the C=C bond which may be formed by the microwave irradiation process.

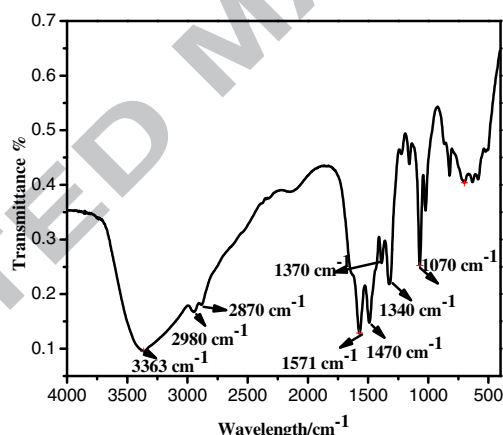


Fig. 2. The FT-IR spectrum of NCDs

3.2. Effect of buffer pH

The effect of pH on the electrochemical response of DA attached to NCDs-modified electrode were examined by DPV within a pH range of 6.0 to 9.0 (Fig. S5). It is clearly found that the peak current and the reduction peak potential are changed with the variation of solution pH, which indicated that protons can participate in the electrochemical reaction of DA [35]. The maximum value appeared at pH 6.0 which was selected as optimal pH for the electrochemical detection in the

following experiments.

3.3. Electrochemical properties

The DPV responses of the NCDs-modified electrode after incubation in a DA solution of concentration ranging from 0 μM to 8 μM in a pH=6.5 buffer shows that the peak current increases as the increase of DA concentration, and the oxidation peak current (I_{pa}) has a good linear relationship in the DA concentration range from 0.05 to 8.00 μM (Fig. 3a). As shown in Fig. 3b, this linear regression equation was described as $I_{pa} (\mu\text{A}) = 0.563C (\mu\text{M}) + 0.839$ ($R^2 = 0.998$), giving a detection limit of 1.2 nmol/L based on signal-to-noise ratio of 3 ($S/N = 3$). These results are comparable with previously published reports based on other electrochemical methods (Table 1), which further demonstrates that this new NCDs sensor can show a satisfactory electro-analytical performance on its DA measurement. The excellent electro-catalytic ability of the modified electrode is attributed to the large number of carboxylic groups and amino groups on the surface of NCDs that can effectively interact with DA.

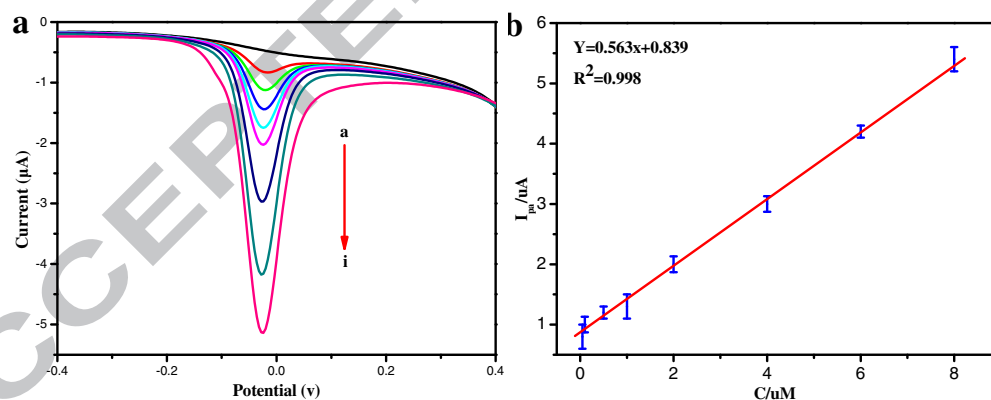


Fig. 3. (a) DPV response to 0, 0.05, 0.1, 0.5, 1, 2, 4, 6, 8 μM of DA (from a to i), (b) Calibration plot of DPV peak current vs logarithm of target DA concentration.

Table.1 Comparison of electro analytical parameters for the determination of dopamine at NCDs modified electrode with other reported modified electrodes

Electro	Detection limit (μM)	Linear range (μM)	Method	Ref.
Graphene	2.6	4–100	DPV ^a	36
PEDOT/Pd composite	0.5	0.5–1.0	DPV	37
Chitosan–grapheme	1.0	1.0–24	DPV	38
GNS/PEI/AuNP	0.2	2–48	DPV	39
PPy–RGOc	1	0.01–10	DPV	40
NGa	0.25	0.5–170	DPV	41
HAu-Gg	0.05	0.08–600	Amperometry	42
NCDs	0.0012	0.05–8.00	DPV	This work

^a DPV – Differential pulse voltammetry.

3.4. Interference

It is well known that ascorbic acid (AA) is the main substance in coexistence with DA in biological samples. Herein, we further investigated the DPV response of a 5 μM DA and 0.25 mM AA at the NCDs modified electrode. As shown in Fig. S6, two well-resolved oxidation peaks (>0.58 V) were obtained, which indicates that the DPV response signal of DA could be clearly observed in the presence of interfering compound AA. Therefore, this kind of new N-doped carbon dots (NCDs) prepared by using the microwave-assisted technique can act as a highly selective and sensitive material for the direct and rapid detection of DA at low concentration.

3.5. Analysis of DA in real life samples.

To further evaluate the applicability of the proposed sensor, the concentration limit of DA in human serum and urine samples were determined by applying the standard addition method. Herein, the known quantities of dopamine were added into two above samples which were diluted with PBS (pH= 6.5) to a ratio of 1:50 (v/v). The analytical results were summarized in Table 2, and DPV responses were shown in Fig.S7. The recovery was in the range of 95.00–104.00%, and the RSD value is less than 3%, demonstrating that the obtained N-doped carbon dots as the modified electrode can exhibit good accuracy for direct determination of DA in real life samples.

Table.2 Determination of DA in human serum and urine samples at NCDs modified electrode.

Sample	Added (M)	Found(M)	Recovery(%)	^a RSD (%)
Serum	1×10^{-7}	0.95×10^{-7}	95.00	1.84
	5×10^{-7}	4.88×10^{-7}	97.60	1.92
	1×10^{-6}	1.02×10^{-6}	102.00	2.22
	5×10^{-6}	4.95×10^{-6}	99.00	2.42
Urine	1×10^{-7}	1.04×10^{-7}	104.00	1.85
	5×10^{-7}	4.92×10^{-7}	98.40	1.97
	1×10^{-6}	1.05×10^{-6}	105.00	2.36
	5×10^{-6}	5.02×10^{-6}	100.40	2.76

RSD value reported is for n=3. The serum and urine samples were diluted 50 times with PBS (pH=6.5) before measurement.

3.6. Stability, reproducibility studies

In this study, NCDs were used intermittently and stored for two weeks in order to examine the stability of the modified electrode. The current signals could show a less than 4.2% decrease relative to the initial response indicating that the obtained NCDs can show an excellent stability of the proposed modified electrode. Meanwhile, five parallel measurements of DA (1.0×10^{-6} mol/L) were carried out, and the relative standard deviation (RSD) is 3.25% indicating that the NCDs modified electrode also has good reproducibility.

4. Conclusions

A new type of NCDs could be prepared through a one-step microwave irradiation method within just 10 minutes by using DEA as both a carbon and nitrogen source without any solvent or catalyst. The obtained NCDs can act as the modified electrode and exhibit high selectivity, good stability and reproducibility for the direct and rapid detection of real-life DA samples at low concentrations.

Acknowledgements

This work was supported by the National Natural Science Foundation of China (51173078, 21172106, and 21474048), open project of Beijing National Laboratory for

Molecular Sciences and a Project Funded by the Priority Academic Program Development of Jiangsu Higher Education Institutions (PAPD).

Appendix A. Supplementary material

Supplementary data associated with this article can be found, in the online version, at <http://dx.doi.org/10.1016/xxx>

References

- [1] (a) A. Sauerbier, R. Chaudhuri, K.B. Ganglia 3 (2013) 159; (b) J. Zhang, L. Zhu, J. Du, B. Liu, Neural Regen. Res. 2 (2007) 18.
- [2] L.L. Liu, Q. Li, N.J. Li, J.H. Ling, R. Liu, Y.X. Wang, L.X. Sun, X.H. Chen, K. Bi, J. Sep. Sci. 34 (2011) 1198.
- [3] S.R. Ali, Y.F. Ma, R.R. Parajuli, Y. Balogun, W.Y.C. Lai, H.X. He, Anal. Chem. 79 (2007) 2583.
- [4] Y.Z. Zhou, H.Y. Zhang, H.D. Xie, B. Chen, L. Zhang, X.H. Zheng, P. Jia, Electrochim. Acta 75 (2012) 360.
- [5] A.A. Ensafi, A. Arabzadeh, H. Karimi-Maleh, Anal. Lett. 43 (2010) 1976.
- [6] H.X. Li, Y. Wang, D.X. Ye, J. Luo, B.Q. Su, S. Zhang, J.L. Kong, Talanta 127 (2014) 255.
- [7] J. Kehr, X. J. Hu, T. Yoshitake, D. Scheller, J. Chromatogr., B: Anal. Technol. Biomed. Life Sci. 845 (2007) 109.
- [8] L. Li, H. Liu, Y. Shen, J. Zhang, J. J. Zhu, Anal. Chem. 83 (2011) 661.
- [9] Y. Wang, H. Chen, J. Chromatogr., A 1080 (2005) 192.
- [10] M. Shou, C. R. Ferrario, K. N. Schultz, T. E. Robinson, R. T. Kennedy, Anal. Chem. 78 (2006) 6717.
- [11] D. P. Nikolelis, D. A. Drivelos, M. G. Simantiraki, S. Koinis, Anal. Chem. 76 (2004) 2174.
- [12] C.Wang, R.Yuan, Y.Q. Chai, S.H. Chen, F.X. Hu, M.H. Zhang, Microchim. Acta 741 (2012) 15–20.
- [13] Y.Q.Dong, J.P. Lin, Y.M.Chen, F.F.Fu, Y.W.Chi, G.N.Chen, Nanoscale 2014, 6,7410
- [14] C.F. Zhou, W. Jiang, B. K. Vias, Colloids Surf., B 118 (2014) 72.
- [15] Y. Xue, J. Liu, H. Chen, R. Wang, D. Li, J. Qu, L. Dai, Angew. Chem., Int. Ed. 51 (2012) 1.
- [16] Y. Li, Y. Zhao, H. Cheng, Y. Hu, G. Shi, L. Dai, L. Qu, J. Am. Chem. Soc. 134 (2012) 15.
- [17] L.Q. Zhang, S. Dai, L. Li, J. Am. Chem. Soc. 134 (2012) 18932.
- [18] S.J. Zhu, Q.G. Meng, L. Wang, J.H. Zhang, Y.B. Song, H. Jin, K. Zhang, H.C. Sun, H.Y. Wang, B. Yang, Angew. Chem., Int. Ed. 52 (2013) 3953.
- [19] A.W. Zhu, Q. Qu, X.L. Shao, B. Kong, Y. Tian, Angew. Chem., Int. Ed. 51 (2012) 7185.
- [20] S.P. Pei, J. Zhang, M.P. Gao, D.Q.Wua, Y.X. Yang, R.L. Liu, J. Colloid Interface Sci. 439 (2015) 129.
- [21] B. Kong, A.W. Zhu, C.Q. Ding, X.M. Zhao, B. Li, Y. Tian, Adv. Mater. 24 (2012) 5844.
- [22] B.F.Hana, W.X.Wang, H.Y. Wua, F.Fang, N.Z. Wang, X.J. Zhang, S.K. Xua, Colloids Surf., B 100 (2012) 209.
- [23] S.B.Ruan, B.Y. Zhu, H.J. Zhang, J.T. Chen, S. Shen, J. Qian, Q. He, H.L. Gao, J. Colloid Interface Sci. 422 (2014) 25.
- [24] X. Li, H. Wang, Y. Shimizu, A. Pyatenko, K. Kawaguchi, N. Koshizaki, Chem. Commun. 47(2011), 932.
- [25] Y.M. Long, C.H. Zhou, Z.L. Zhang, Z.Q. Tian, L. Bao, Y. Lin, D.W. Pang, J. Mater. Chem. 22(2012)

5917.

- [26] L. Cao, X. Wang, M. J. Meziani, F. Lu, H. Wang, P. G. Luo, Y. Lin, B. A. Harruff, L. M. Veca, D. Murray, S. Y. Xie, Y. P. Sun, *J. Am. Chem. Soc.* 129(2007) 11318.
- [27] a) S. Qu, X. Wang, Q. Lu, X. Liu, L. Wang, *Angew. Chem. Int. Ed.* 51(2012) 12215; b) L. Tang, R. Ji, X. Cao, J. Lin, H. Jiang, X. Li, K. S. Teng, C. M. Luk, S. Zeng, J. Hao, S. P. Lau, *ACS Nano* 6(2012) 5102.
- [28] W. S. Kwon, G. J. Lee, S. G. Do, T. Joo, S. W. Rhee, *Small* 10(2014) 506.
- [29] Y. Liu, N. Xiao, N. Q. Gong, H. Wang, X. Shi, W. Gu, L. Ye, *Carbon* 68 (2014) 258.
- [30] Z. M. Luo, D. L. Yang, G. Q. Qi, J. Z. Shang, H. P. Yang, Y. L. Wang, L. H. Yuwen, T. Yu, W. Huang, L. H. Wang, *J. Mater. Chem. A* 48 (2014) 20605.
- [31] L. L. Li, J. Ji, R. Fei, C. Z. Wang, Q. Lu, J. R. Zhang, L. P. Jiang, J. J. Zhu, *Adv. Funct. Mater.* 22 (2012) 2971.
- [32] Q. L. Wang, H. Z. Zheng, Y. J. Long, L. Y. Zhang, M. Gao, W. J. Bai, *Carbon* 49 (2011) 3134.
- [33] V. K. Ponnusamy, V. Mani, S. M. Chen, W. T. Huang, J. F. Jen, *Talanta* 120 (2014) 148.
- [34] Q. L. Wang, H. Z. Zheng, Y. J. Long, L. Y. Zhang, M. Gao, W. J. Bai, *Carbon* 49 (2011) 3134–3140.
- [35] X. H. Wang, K. G. Qu, B. L. Xu, J. S. Ren, X. G. Qu, *J. Mater. Chem.* 21 (2011) 2445–2450.
- [36] G. Zheng, M. Chen, X. Y. Liu, J. Zhou, J. Xie, G. W. Diao, *Electrochim. Acta* 136 (2014) 301.
- [37] S. Harish, J. Mathiyarasu, K. L. N. Phani, V. Yegnaraman, *J. Appl. Electrochem.* 38 (2008) 1583.
- [38] D. Han, T. Han, C. Shan, A. Ivaska, L. Niu, *Electroanalysis* 22 (2010) 2001.
- [39] V. K. Ponnusamy, V. Mani, S. M. Chen, W. T. Huang, J. F. Jen, *Talanta* 120 (2014) 148.
- [40] Z. H. Sheng, X. Q. Zheng, J. Y. Xu, W. J. Bao, F. B. Wang, X. H. Xia, *Biosens. Bioelectron.* 34 (2012) 125.
- [41] T. Qian, S. S. Wu, J. Shen, *Chem. Commun.* 49 (2013) 4610.
- [42] W. C. Zhu, T. Chen, X. M. Ma, H. Y. Ma, S. H. Chen, *Colloids Surf., B* 111 (2013) 321.
- [43] Y. R. Kim, S. Bong, Y. J. Kang, Y. Yang, R. K. Mahajan, J. S. Kim, H. Kim, *Biosens. Bioelectron.* 25 (2010) 2366.

Graphical

A new N-doped carbon dots (NCDs) could be prepared by one step rapid microwave irradiation method in high yield and exhibit highly sensitive electrochemical response toward dopamine (DA) in PBS (pH=6.5) buffer solution. This new NCDs could be used for the detection of trace levels of DA in human serum and urine samples.

