

Author's Accepted Manuscript

A novel amperometric enzyme inhibition biosensor based on xanthine oxidase immobilised onto glassy carbon electrodes for bisphenol A determination

Najib Ben Messaoud, Mariana Emilia Ghica, Cherif Dridi, Mounir Ben Ali, Christopher M.A. Brett



PII: S0039-9140(18)30267-4
DOI: <https://doi.org/10.1016/j.talanta.2018.03.031>
Reference: TAL18465

To appear in: *Talanta*

Received date: 29 December 2017
Revised date: 6 March 2018
Accepted date: 11 March 2018

Cite this article as: Najib Ben Messaoud, Mariana Emilia Ghica, Cherif Dridi, Mounir Ben Ali and Christopher M.A. Brett, A novel amperometric enzyme inhibition biosensor based on xanthine oxidase immobilised onto glassy carbon electrodes for bisphenol A determination, *Talanta*, <https://doi.org/10.1016/j.talanta.2018.03.031>

This is a PDF file of an unedited manuscript that has been accepted for publication. As a service to our customers we are providing this early version of the manuscript. The manuscript will undergo copyediting, typesetting, and review of the resulting galley proof before it is published in its final citable form. Please note that during the production process errors may be discovered which could affect the content, and all legal disclaimers that apply to the journal pertain.

A novel amperometric enzyme inhibition biosensor based on xanthine oxidase immobilised onto glassy carbon electrodes for bisphenol A determination

Najib Ben Messaoud^{a,b}, Mariana Emilia Ghica^d, Cherif Dridi^a,
Mounir Ben Ali^{a,c}, Christopher M.A. Brett^{d,*}

^a *NANOMISENE Lab, LR16CRMN01, Centre for Research on Microelectronics and Nanotechnology CRMN of Sousse, Technopark of Sousse B.P. 334, Sahloul, 4034 Sousse, Tunisia*

^b *University of Sousse, High School of Sciences and Technology of Hammam Sousse, 4011, Hammam Sousse, Tunisia*
^c *University of Sousse, ISSAT of Sousse, Cité Ettafala, 4003 Ibn Khaldoun Sousse, Tunisia*

^d *Department of Chemistry, Faculty of Sciences and Technology, University of Coimbra, 3004-535 Coimbra, Portugal*

*Corresponding author:

Tel: +351-239854470

Fax: +351-239827703

E-mail: cbrett@ci.uc.pt

Abstract

A novel and simple biosensor for the determination of bisphenol A (BPA) based on xanthine oxidase (XOD) enzymatic inhibition has been developed. The biosensor was prepared from xanthine oxidase immobilised by crosslinking with glutaraldehyde, with hypoxanthine as enzyme substrate, and was successfully applied to the determination of BPA using fixed potential amperometry. Biosensor performance was optimised with respect to the applied potential, influence of pH of the electrolyte solution, XOD loading and the substrate concentration. The enzyme inhibition mechanism was evaluated from Cornish-Bowden plus Dixon plots and was found to be reversible and competitive with an apparent inhibition constant of 8.15 nM. Under optimised conditions, the determination of BPA can be achieved in the linear range up to 41 nM with a detection limit of 1.0 nM, which is equal to the lowest reported in the literature, with very good repeatability and reproducibility. The selectivity of the biosensor was evaluated by performing an interference study and found to be excellent; and stability was investigated. It was successfully applied to the detection of BPA in mineral water and in river water.

Keywords: Bisphenol A; enzyme inhibition biosensor; xanthine oxidase, fixed potential amperometry

1. Introduction

Concerns are growing among the public and the scientific community with respect to chemicals, known collectively as endocrine disrupting compounds (EDCs), and which have been extensively studied in relation to malformation, cancers, sexual precocity, neural and behavioral changes in infants and children [1, 2].

Bisphenol A (BPA), one of the typical endocrine-disrupting chemicals, is suspected of interfering with the normal function of the endocrine system causing adverse effects for humans and wildlife [3]; it can mimic the body's own hormones and lead to an increased risk of cancer [4, 5]. However, BPA is important as a major component in the production of polycarbonate (PC) and epoxy resin (EP), which are extensively used to make plastic food and beverage containers, water bottles, baby bottles, and some dental sealants. Moreover, what is more serious is that the migration of BPA from these materials into food has been reported [6–9], and which can lead to acute toxicity to aquatic organisms and has also been shown to occur in human cultured cells [10–12]. Additionally, BPA may even induce obesity, diabetes, infertility, birth defects, prostate cancer and breast cancer [13, 14]. During the past few years, the frequent environmental accidents resulting from BPA have been considered as one of the most fundamental concerns at a global level. Bisphenol A is present in raw sewage, in river water and sediments, and can also migrate into drinking water. It is released into the environment due to domestic and industrial activities. Thus, it is very important to remove BPA from the environment and to determine its presence in trace quantities. In this context, a rapid, simple, sensitive and high-selective electroanalytical method for the determination of bisphenol A would be highly desirable.

Until now, the analytical techniques for determination of BPA are mainly high performance liquid chromatography (HPLC) [15], gas chromatography (GC) [16], mass spectrometry [17], immunochemical methods [6], immunochromatographic lateral flow assay [18], and enzyme-

linked immunosorbent assay [19]. However, all these technologies are time-consuming, use expensive instrumentation and require large sample volumes [20]. Electrochemical biosensors, on the contrary, have shown advantages like simplicity, rapidity and low cost and have the benefit of high sensitivity, potential for miniaturization, specificity, the possibility of in situ analysis and allowing the determination of environmental pollutants. Nowadays, the various biosensors that have been fabricated for bisphenol A analysis involve incorporation of different biomolecules such as peptides [21–23], antibodies [24–26], aptamers [27–29] and enzymes [30–34]. Most of the enzyme biosensors for BPA are based on tyrosinase [30, 33, 34], or laccase [35]. The major drawbacks of most of these is that some chemical species can be interferents and behave like the enzyme substrate, interact specifically with the immobilized enzyme or can bind to the immobilized enzyme, causing changes in its active site. Enzyme inhibition is the result of a reduction in observed enzymatic activity caused by the presence of an inhibitor in the system [36]. Thus, biosensors based on enzyme inhibition are reliable tools for the detection of many toxic compounds and are extremely useful for application in clinical, food and environmental samples [37].

In the present work, xanthine oxidase (XOD) enzyme-based electrodes are proposed for the first time for inhibitive determination of bisphenol A. The experimental conditions influencing the analytical performance of the XOD biosensor were optimised. The response of the sensor to bisphenol A was evaluated by measuring the activity of xanthine oxidase after adding different concentrations of BPA. The biosensor exhibited an attractive performance for determination of BPA, with good selectivity and stability. Practical application of the developed modified electrode to the determination of BPA was successfully carried out.

2. Experimental

2.1. Reagents and solutions

Xanthine oxidase (E.C. 1.1.3.22, from buttermilk 0.068 U/mg) and glutaraldehyde (GA) (25 % v/v) aqueous solution were acquired from Fluka, bovine serum albumin (BSA) and hypoxanthine were from Aldrich. BPA was obtained from Sigma–Aldrich.

All solutions were prepared using Millipore Milli-Q nanopure water (resistivity > 18 MΩ cm). The phosphate buffer solution (PB), 0.1 M was prepared over the pH range of 6.0–8.0 and was used as supporting electrolyte for biosensor evaluation and for all the electrochemical measurements. A stock solution of 0.2 M BPA was prepared in methanol and stored in a refrigerator at 4 °C. For BPA detection, the stock solution was diluted with buffer to 1.0 μM and from this solution small aliquots (2–10 μL) were added to the cell. Experiments were performed at room temperature, 25±1 °C.

2.2. Electrochemical instrumentation and measurements

All electrochemical measurements were performed with a conventional three-electrode system in an electrochemical cell of 2 mL volume, containing the glassy carbon electrode (GCE) as working electrode with 0.00785 cm² surface area, a platinum electrode as counter electrode and an Ag/AgCl electrode as reference electrode.

The amperometric measurements were carried out at room temperature using a computer controlled IviumStat electrochemical analyser with IviumSoft software (version 2.024, Ivium Technologies, The Netherlands).

The pH measurements were carried out with a Crison 2001 micro pH-meter (Spain) at room temperature.

2.3. Enzyme immobilization

The immobilization of xanthine oxidase (XOD) onto the surface of the GCE was done by cross-linking with glutaraldehyde and bovine serum albumin (BSA) as previously described for several enzyme biosensors [38–40] in order to increase the attachment of the enzyme to the transducer and facilitate electron exchange between substrate and enzyme active centre. A mixture of 3 mg of XOD and 3 mg of BSA in 30 μL phosphate buffer (pH=7) was prepared. From this solution, 1 μL (which is equivalent to 0.0068 U XOD) was placed over the GCE, and immediately 1 μL of the cross-linking agent glutaraldehyde (2.5 % v/v in Milli-Q water) was added and then dried at room temperature for 1 to 2 h. The electrodes were kept at 4 $^{\circ}\text{C}$ in phosphate buffer, pH 7.0 until needed.

2.4. Enzyme inhibition measurements

In order to evaluate the inhibition of the activity of xanthine oxidase, the XOD/GCE modified electrode was dipped into a stirred phosphate buffer solution at pH 7.5, and a fixed potential of -0.5 V vs. SCE was applied. After stabilisation of the baseline current, a fixed amount of hypoxanthine (substrate) was added to record a steady-state current (I_0) before adding the inhibitor. The concentration of added bisphenol A was increased to inhibit the xanthine oxidase activity, and the current decrease (I_1), which is proportional to the final concentration of the inhibitor in solution, was recorded. In order to evaluate the percentage of inhibition (I (%)) due to the bisphenol A inhibitor, the following expression was used:

$$I(\%) = \frac{I_0 - I_1}{I_0} \times 100$$

3. Results and discussion

3.1. Biosensor for bisphenol A development and optimization

Experimental variables that can affect the performance of the amperometric inhibition biosensors, namely the pH of the supporting electrolyte, the applied potential, the substrate concentration, and the enzyme loading, were studied in order to optimise response to bisphenol A by inhibition.

3.1.1. Effect of pH

Taking into account previous work based on XOD [40] initial measurements were performed at an applied potential of -0.3 V. The effect of the pH value of the 0.1 M phosphate buffer solution was examined in the range from 6.0 to 8.0. The response of the biosensor to 10 nM bisphenol A, in the presence of 0.3 mM hypoxanthine varied significantly with pH. The dependence of the current response on pH is illustrated in Figure 1. As can be seen, the amperometric signal rises with increase in pH from 6.0 to 7.5, where a maximum is exhibited, and then decreases. Thus, phosphate buffer solution pH=7.5 was chosen as the most suitable for amperometric measurements.

3.1.2. Effect of the applied potential

In order to optimise the response of the XOD/GCE biosensor towards bisphenol A, the amperometric response to 10 nM bisphenol A was tested in the presence of 0.3 mM hypoxanthine at fixed potentials from -0.5 V to -0.1 V vs Ag/AgCl (Figure 2). As can be seen, the response to BPA decreases with a less negative potential value. The higher current response is exhibited at -0.5 V vs. Ag/AgCl, which was chosen for further studies.

3.1.3. Effect of substrate concentration

The substrate concentration can influence the monitoring of enzymatic activity under inhibition conditions. The effect of substrate concentration on inhibition can be tested by measuring the activity of XOD with varying concentrations of hypoxanthine substrate and injecting the same concentration of BPA inhibitor. Thus, the sensitivity of the biosensor to bisphenol A as a function of three hypoxanthine concentrations 0.3, 0.5 and 1.0 mM was examined (not shown). The sensitivity to bisphenol A increases with decrease in hypoxanthine concentration. The highest sensitivity for BPA determination was achieved in the presence of the lowest concentration of hypoxanthine tested, namely 0.3 mM, the response decrease being 89 % of this for 0.5 mM and 53 % for 1.0 mM. In order to achieve high sensitivity of the response to BPA, a concentration of 0.3 mM of hypoxanthine was selected for further experiments.

3.1.4. Effect of enzyme concentration

The amount of enzyme was varied in order to optimise the response, by keeping the concentration of BSA (10 %) constant and varying the concentration of XOD. Figure 3 shows the response of bisphenol A for various enzyme concentrations: 0.0034, 0.0068 or 0.0136 U immobilised on the GCE. An increase of the response toward bisphenol A by 48 % is clearly observed when increasing the enzyme concentration from 0.0034 to 0.0068 U, but a decrease of 40 % for 0.0136 U compared with 0.0034 U. Thus a XOD concentration of 0.0068 U immobilised on the GCE was chosen for future experiments.

3.2 Analytical performance of the biosensor for bisphenol A

The amperometric measurement of bisphenol A at the XOD/GCE biosensor was carried out in 0.1 M phosphate buffer solution, pH 7.5, at an applied potential of -0.5 V vs. Ag/AgCl and in

the presence of 0.3 mM hypoxanthine. Aliquots of stock solution of bisphenol A were added, leading to a decrease in the hypoxanthine response, that can be deduced to be due to inhibition of XOD activity, as illustrated in Figure 4(a). Although in other work [41], performed under different experimental conditions, it was found that BPA can activate XOD, here there is inhibition. Their matrix (animal models and cell cultures) is significantly more complex than that used by us and XOD is in solution rather than immobilised. Immobilisation often leads to restrictions in the enzyme conformations, which can greatly influence the apparent enzyme activity. In [41] it was found that BPA induces secondary structure alterations of XOD and this probably forms the basis of the explanation for the different observed behaviour.

In Figure 4(b), the calibration curve for bisphenol A gives a linear response between 1.0 and 41 nM of bisphenol A following the equation $-\Delta j (\mu\text{A cm}^{-2}) = 0.0245c (\text{nM}) + 0.00065$ ($R^2 = 0.9998$), and a detection limit calculated as $(3 \times \text{SD}_{\text{blank}})/\text{slope}$ was 1.0 nM. A comparison of the performance achieved by the new biosensor and other BPA biosensors in the literature is shown in Table 1. The detection limit for bisphenol A achieved here is significantly lower than most of the biosensors and is only equalled by two tyrosinase-based biosensors [2, 3].

The inhibition constant, K_i , can be determined from the Dixon plot [47], Figure 5(a), in which the inverse of the enzyme activity is plotted vs. inhibitor concentration for at least two different enzyme-substrate concentrations. For the evaluation of this constant, the Dixon plot was made for three different substrate (hypoxanthine) concentrations: 0.3, 0.5 and 1.0 mM. Following this method, the extrapolated abscissa intercept of each linear plot corresponds to the inhibition constant, which was determined to be $K_i = 8.15 \text{ nM}$.

3.3. Determination of the type of inhibition

For the evaluation of the type of enzyme inhibition, the data were analysed using Dixon and Cornish-Bowden plots. The Dixon plot by itself cannot clearly distinguish between competitive and mixed reversible inhibition. In the Cornish-Bowden plot [48], the ratio of substrate concentration over enzyme activity is plotted vs. inhibitor concentration, but cannot always distinguish between mixed and uncompetitive inhibition. By using both Dixon and Cornish-Bowden plots, it is possible to elucidate the type of inhibition. Figure 5 (a) and (b) show Dixon and Cornish-Bowden plots using three different concentrations of hypoxanthine, 0.3, 0.5 and 1.0 mM. From the Dixon plot, the crossing lines enable it to be deduced that the inhibition is mixed or competitive. The same inhibition data in the Cornish-Bowden plot show that the inhibition is competitive because the straight lines drawn through the experimental points are parallel. Further evidence that the mechanism of inhibition by bisphenol A is competitive is the fact that inhibition is decreased by increasing the amount of substrate, from 48.4% in the presence of 0.3 mM hypoxanthine to 22.1% in the presence of 1.0 mM hypoxanthine.

3.4. Interference studies

Several phenolic compounds and inorganic ions were measured to examine whether they interfere with the determination of bisphenol A. Under the optimal conditions, the influence of some potential interferent species on the current response of 30 nM BPA was studied. The results indicated that the presence of 100-fold concentration of interfering substances had no significant influence on the signals of BPA with the deviation below $\pm 7\%$. The results are shown in Table 2. The proposed sensor is thus demonstrated to show good selectivity for the determination of BPA in real samples.

3.5. Reproducibility, repeatability and lifetime

Reproducibility, tested by measuring the same concentration, 30 nM, of BPA at five different electrodes prepared in the same way, gave a relative standard deviation (RSD) of 3.2 % (Figure 6a). The repeatability of the modified electrode was investigated by recording the response at a fixed concentration, 30 nM BPA five successive times (Figure 6b). The RSD of these five measurements was 2.4%.

The lifetime of the biosensor was monitored daily by measuring the response to BPA in the presence of hypoxanthine during 15 days. After this period, the response to BPA dropped to 75 % of the initial value (Figure 6c). This is a bit less than for other biosensors for BPA [2, 22], but is similar to that obtained in [30] with tyrosinase, and can be ascribed to a decrease in xanthine oxidase activity, as previously observed [40]. However, such a loss of activity does not compromise use as an effective inhibition biosensor.

3.6. Application

To evaluate the fabricated enzyme inhibition biosensor for bisphenol A determination in environmental samples, application of the biosensor was examined by recovery measurements in mineral water and in river water in which no BPA was detected previously. The results are presented in Table 3. The average recovery was in the range of 97.9–103 %, which indicates the efficacy of the biosensor for practical analysis.

4. Conclusions

A novel, easy to prepare electrochemical enzyme biosensor for inhibition assays, based on xanthine oxidase immobilised on glassy carbon electrode has been developed for bisphenol A. The optimised biosensor exhibited high sensitivity and low detection limit, with good selectivity and stability, and enabled successful detection in water samples. The inhibition

constant was determined by using a Dixon plot together with the Cornish-Bowden plot, and the enzyme inhibition mechanism of BPA on the XOD activity the inhibition was shown to be competitive. The biosensor described here has a simpler architecture and showed much better performance than other biosensors reported in the literature for BPA and is a new and promising approach for its detection.

Acknowledgments

NBM thanks the Tunisian Ministry of Higher Education and scientific research for a “Bourse d’alternance” fellowship. The authors gratefully acknowledge the financial support from the European Commission 7th Framework Programme Marie Curie Actions People IRSES N°294993 SMARTCANCERSENS and Fundação para a Ciência e a Tecnologia (FCT), Portugal projects PTDC/QEQ-QAN/2201/2014, in the framework of Project 3599-PPCDT, and UID/EMS/00285/2013 (both co-financed by the European Community Fund FEDER). MEG thanks FCT for a postdoctoral fellowship SFRH/BPD/103103/2014.

References

- [1] M. Portaccio, D. Di Tuoro, F. Arduini, M. Lepore, D.G. Mita, N. Diano, L. Mita, D. Moscone, A thionine-modified carbon paste amperometric biosensor for catechol and bisphenol A determination, *Biosens. Bioelectron.* 25 (2010) 2003–2008.
- [2] M. Han, Y. Qu, S. Chen, Y. Wang, Z. Zhang, M. Ma, Z. Wang, G. Zhan, C. Li, Amperometric biosensor for bisphenol A based on a glassy carbon electrode modified with a nanocomposite made from polylysine, single walled carbon nanotubes and tyrosinase, *Microchim. Acta* 180 (2013) 989–996.
- [3] D. Pan, Y. Gu, H. Lan, Y. Sun, H. Gao, Functional graphene-gold nano-composite fabricated electrochemical biosensor for direct and rapid detection of bisphenol A, *Anal. Chim. Acta* 853 (2015) 297–302.
- [4] A.M. Soto, C. Sonnenschein, Environmental causes of cancer: endocrine disruptors as carcinogens, *Nat. Rev. Endocrinol.* 6 (2010) 363–370.
- [5] L. Wu, D. Deng, J. Jin, X. Lu, J. Chen, Nanographene-based tyrosinase biosensor for rapid detection of bisphenol A, *Biosens. Bioelectron.* 35 (2012) 193–199.
- [6] A. Ballesteros-Gómez, S. Rubio, D. Pérez-Bendito, Analytical methods for the determination of bisphenol A in food, *J. Chromatogr. A* 1216 (2009) 449–469.
- [7] N.C. Maragou, E.N. Lampi, N.S. Thomaidis, M.A. Koupparis, Determination of bisphenol A in milk by solid phase extraction and liquid chromatography–mass spectrometry, *J. Chromatogr. A* 1129 (2006) 165–173.
- [8] Z. Brenn-Struckhova, M. Cichna-Markl, Determination of bisphenol A in wine by sol-gel immunoaffinity chromatography, HPLC and fluorescence detection, *Food Addit. Contam.* 23 (2006) 1227–1235.
- [9] C. Brede, P. Fjeldal, I. Skjevra, H. Herikstad, Increased migration levels of bisphenol A from polycarbonate baby bottles after dishwashing, boiling and brushing, *Food Addit. Contam.* 20 (2003) 684–689.
- [10] C.A. Staples, J.W. Davis, An examination of the physical properties, fate, ecotoxicity and potential environmental risks for a series of propylene glycol ethers, *Chemosphere* 49 (2002) 61–73.
- [11] N. Suzuki, A. Hattori, Bisphenol A suppresses osteoclastic and osteoblastic activities in the cultured scales of goldfish, *Life Sci.* 73 (2003) 2237–2247.
- [12] Y. Nakagawa, T. Suzuki, S. Tayama, Metabolism and toxicity of benzophenone in isolated rat hepatocytes and estrogenic activity of its metabolites in MCF-7 cells, *Toxicology* 156 (2000) 27–36.

- [13] L.N. Vandenberg, R. Hauser, M. Marcus, N. Olea, W.V. Welshons, Human exposure to bisphenol A (BPA), *Reprod. Toxicol.* 24 (2007) 139–177.
- [14] H. Mielke, U. Gundert-Remy, Bisphenol A levels in blood depend on age and exposure, *Toxicol. Lett.* 190 (2009) 32–40.
- [15] S.H. Yang, A.A. Morgan, H.P. Nguyen, H. Moore, B.J. Figard, K.A. Schug, Quantitative determination of Bisphenol A from human saliva using bulk derivatization and trap-and-elute liquid chromatography coupled to electrospray ionization mass spectrometry, *Environ. Toxicol. Chem.* 30 (2011) 1243–1251.
- [16] A.R. Fontana, M. Muñoz de Toro, J.C. Altamirano, One-step derivatization and preconcentration microextraction technique for determination of bisphenol A in beverage samples by gas chromatography- mass spectrometry, *J. Agric. Food Chem.* 59 (2011) 3559–3565.
- [17] J. Zhang, G.M. Cooke, I.H. Curran, C.G. Goodyer, X.-L. Cao, GC–MS analysis of bisphenol A in human placental and fetal liver samples, *J. Chromatogr. B* 879 (2011) 209–214.
- [18] Z. Mei, Y. Deng, H. Chu, F. Xue, Y. Zhong, J. Wu, H. Yang, Z. Wang, L. Zheng, W. Chen, Immunochromatographic lateral flow strip for on-site detection of bisphenol A, *Microchim. Acta* 180 (2013) 279–285.
- [19] M.-P. Zhao, Y.-Z. Li, Z.-Q. Guo, X.-X. Zhang, W.-B. Chang, A new competitive enzyme-linked immunosorbent assay (ELISA) for determination of estrogenic bisphenols, *Talanta* 57 (2002) 1205–1210.
- [20] J. Huang, X. Zhang, S. Liu, Q. Lin, X. He, X. Xing, W. Lian, Electrochemical sensor for bisphenol A detection based on molecularly imprinted polymers and gold nanoparticles, *J. Appl. Electrochem.* 41 (2011) 1323–1328.
- [21] L. Yang, H. Zhao, S. Fan, B. Li, C.-P. Li, A highly sensitive electrochemical sensor for simultaneous determination of hydroquinone and bisphenol A based on the ultrafine Pd nanoparticle@ TiO₂ functionalized SiC, *Anal. Chim. Acta* 852 (2014) 28–36.
- [22] Y. Qu, M. Ma, Z. Wang, G. Zhan, B. Li, X. Wang, H. Fang, H. Zhang, C. Li, Sensitive amperometric biosensor for phenolic compounds based on graphene–silk peptide/tyrosinase composite nanointerface, *Biosens. Bioelectron.* 44 (2013) 85–88.
- [23] K.S. Kim, J. Jang, W.-S. Choe, P.J. Yoo, Electrochemical detection of Bisphenol A with high sensitivity and selectivity using recombinant protein-immobilized graphene electrodes, *Biosens. Bioelectron.* 71 (2015) 214–221.

- [24] M.-H. Piao, H.-B. Noh, M.A. Rahman, M.-S. Won, Y.-B. Shim, Label-Free Detection of Bisphenol A Using a Potentiometric Immunosensor, *Electroanalysis* 20 (2008) 30–37.
- [25] M.A. Rahman, M.J. Shiddiky, J.-S. Park, Y.-B. Shim, An impedimetric immunosensor for the label-free detection of bisphenol A, *Biosens. Bioelectron.* 22 (2007) 2464–2470.
- [26] X. Wang, S. Reisberg, N. Serradji, G. Anquetin, M.-C. Pham, W. Wu, C.-Z. Dong, B. Piro, E-assay concept: Detection of bisphenol A with a label-free electrochemical competitive immunoassay, *Biosens. Bioelectron.* 53 (2014) 214–219.
- [27] Y. Zhu, C. Zhou, X. Yan, Y. Yan, Q. Wang, Aptamer-functionalized nanoporous gold film for high-performance direct electrochemical detection of bisphenol A in human serum, *Anal. Chim. Acta* 883 (2015) 81–89.
- [28] K.V. Ragavan, L.S. Selvakumar, M.S. Thakur, Functionalized aptamers as nano-bioprobes for ultrasensitive detection of bisphenol-A, *Chem. Commun.* 49 (2013) 5960–5962.
- [29] L. Zhu, Y. Cao, G. Cao, Electrochemical sensor based on magnetic molecularly imprinted nanoparticles at surfactant modified magnetic electrode for determination of bisphenol A, *Biosens. Bioelectron.* 54 (2014) 258–261.
- [30] J. Kochana, K. Wapiennik, J. Kozak, P. Knihnicki, A. Pollap, M. Woźniakiewicz, J. Nowak, P. Kościelniak, Tyrosinase-based biosensor for determination of bisphenol A in a flow-batch system, *Talanta* 144 (2015) 163–170.
- [31] P. Sun, Y. Wu, An amperometric biosensor based on human cytochrome P450 2C9 in polyacrylamide hydrogel films for bisphenol A determination, *Sens. Actuators B Chem.* 178 (2013) 113–118.
- [32] X. Jiang, W. Ding, C. Luan, Q. Ma, Z. Guo, Biosensor for bisphenol A leaching from baby bottles using a glassy carbon electrode modified with DNA and single walled carbon nanotubes, *Microchim. Acta* 180 (2013) 1021–1028.
- [33] K.K. Reza, M.A. Ali, S. Srivastava, V.V. Agrawal, A.M. Biradar, Tyrosinase conjugated reduced graphene oxide based biointerface for bisphenol A sensor, *Biosens. Bioelectron.* 74 (2015) 644–651.
- [34] N. Wang, H.-Y. Zhao, X.-P. Ji, X.-R. Li, B.-B. Wang, Gold nanoparticles-enhanced bisphenol A electrochemical biosensor based on tyrosinase immobilized onto self-assembled monolayers-modified gold electrode, *Chin. Chem. Lett.* 25 (2014) 720–722.
- [35] M. Portaccio, D. Di Tuoro, F. Arduini, D. Moscone, M. Cammarota, D.G. Mita, M. Lepore, Laccase biosensor based on screen-printed electrode modified with thionine–

- carbon black nanocomposite, for bisphenol A detection, *Electrochim. Acta* 109 (2013) 340–347.
- [36] S. Kurbanoglu, S.A. Ozkan, A. Merkoçi, Nanomaterials-based enzyme electrochemical biosensors operating through inhibition for biosensing applications, *Biosens. Bioelectron.* 89 (2017) 886–898.
- [37] A. Amine, F. Arduini, D. Moscone, G. Palleschi, Recent advances in biosensors based on enzyme inhibition, *Biosens. Bioelectron.* 76 (2016) 180–194.
- [38] M.E. Ghica, R.C. Carvalho, A. Amine, C.M.A. Brett, Glucose oxidase enzyme inhibition sensors for heavy metals at carbon film electrodes modified with cobalt or copper hexacyanoferrate, *Sens. Actuators B Chem.* 178 (2013) 270–278.
- [39] M.E. Ghica, C.M. Brett, Glucose oxidase inhibition in poly (neutral red) mediated enzyme biosensors for heavy metal determination, *Microchim. Acta* 163 (2008) 185–193.
- [40] A.C. Torres, M.E. Ghica, C.M.A. Brett, Design of a new hypoxanthine biosensor: xanthine oxidase modified carbon film and multi-walled carbon nanotube/carbon film electrodes, *Anal. Bioanal. Chem.* 405 (2013) 3813–3822.
- [41] L. Ma, J. Hu, J. Li, Y. Yang, L. Zhang, L. Zou, R. Gao, C. Peng, Y. Wang, T. Luo, X. Xiang, H. Qing, X. Xiao, C. Wu, Z. Wang, J.C. He, Q. Li, S. Yang, Bisphenol A promotes hyperuricemia via activating xanthine oxidase, *FASEB J.* 32 (2017) 1007–1016.
- [42] X. Lu, X. Wang, L. Wu, L. Wu, L. Fu, Y. Gao, J. Chen, Response characteristics of bisphenols on a metal–organic framework-based tyrosinase nanosensor, *ACS Appl. Mater. Interfaces* 8 (2016) 16533–16539.
- [43] N. Singh, K.K. Reza, M.A. Ali, V.V. Agrawal, A.M. Biradar, Self assembled DC sputtered nanostructured rutile TiO₂ platform for bisphenol A detection, *Biosens. Bioelectron.* 68 (2015) 633–641.
- [44] R. Li, Y. Wang, Y. Deng, G. Liu, X. Hou, Y. Huang, C. Li, Enhanced biosensing of bisphenol A using a nanointerface based on tyrosinase/reduced graphene oxides functionalized with ionic liquid, *Electroanalysis*. 28 (2016) 96–102.
- [45] L. Liu, X. Kang, C. Chen, H. Zhang, C. Chen, Q. Xie, L-tyrosine polymerization-based ultrasensitive multi-analyte enzymatic biosensor, *Talanta*. 179 (2018) 803–809.
- [46] X. Xu, Q. Zheng, G. Bai, L. Song, Y. Yao, X. Cao, S. Liu, C. Yao, Polydopamine induced in-situ growth of Au nanoparticles on reduced graphene oxide as an efficient

biosensing platform for ultrasensitive detection of bisphenol A, *Electrochimica Acta*. 242 (2017) 56–65.

- [47] M. Dixon, The determination of enzyme inhibitor constants, *Biochem. J.* 55 (1953) 170–171.
- [48] A. Cornish-Bowden, A simple graphical method for determining the inhibition constants of mixed, uncompetitive and non-competitive inhibitors, *Biochem. J.* 137 (1974) 143–144.

Tables

Table 1. Performance comparison of the developed biosensor for BPA detection with other biosensors in the literature

Electrode configuration	Linear range / μM	Detection limit / nM	Reference
Tyr/SWCNT-PolyLys/GCE	0.004-11.5	0.97	[2]
Tyr-GR-Au-CS/GCE	0.0025-3.0	1.0	[3]
Tyr/TiO ₂ -MWCNT-PDDA-Nafion/GCE	0.28-45.05	66	[30]
CYP2C9-PAM/GCE	1.25-10	580	[31]
ctDNA-SWNT/GCE	0.01-20	5.0	[32]
Tyr-rGO-CS/ITO	0.01-50	0.74	[33]
Tyr/nano-Au/T-NH ₂ /AuE	0.399-234	133	[34]
Lacc-TH-CB/SPE	0.5-50	200	[35]
CuMOF-Tyr-CS/GCE	0.05-3.0	13	[42]
Tyr-APTES-nTiO ₂ /Ti	0.01-1.0	10	[43]
Tyr-DAPPT-rGO/GCE	0.001-38	0.35	[44]
PLT-Tyr-GOx/AuE	0.05-1.0	16	[45]
Tyr/Au@PDA-rGO-CS/GCE	0.012-3.68	0.1	[46]
XOD/GCE	0.001-0.041	1.0	This work

Tyr: tyrosinase; Lacc: laccase; XOD: xanthine oxidase; CYP2C9: human cytochrome P450 2C9; ctDNA: calf thymus DNA; SWCNT: single-walled carbon nanotubes; MWCNTs: multi-walled carbon nanotubes; GR: graphene; rGO: reduced graphene oxide; PolyLys: poly(lysine); PDDA: poly(diallyldimethylammonium chloride); PAM: polyacrylamide; T-NH₂: thioctic acid amide; TH: thionine; CuMOF: copper centered metal-organic framework; APTES: 3-aminopropyltriethoxysilane; nTiO₂: nanostructured titanium dioxide; DAPPT: 1,3-di(4-amino-1-pyridinium) propane tetrafluoroborate ionic liquid; PDA: polydopamine; PLT: L-tyrosine polymer; CS: chitosan; GCE: glassy carbon electrode; SPE: screen printed electrode; ITO: indium tin oxide

Table 2. Interferences from other species on the inhibition response to 30 nM BPA, concentration ratio 100:1 (3000 nM)

Interferent	<i>I</i> change (%)
K ⁺	-6.8
Na ⁺	3.4
Mg ²⁺	-2.8
Zn ²⁺	-1.3
Ethanol	2.4
Methanol	2.9
Hydroquinone	-5.0
Phenol	-3.6

Table 3. Determination of bisphenol A in water samples

Sample	Added (nM)	Found (nM)	Recovery (%)
Mineral Water	4.80	4.73	98.5
	8.00	8.15	101.8
River Water	4.80	4.70	97.9
	8.00	8.24	103.0

Figure captions

Figure 1. Effect of pH on the amperometric response to 10 nM BPA in 0.1 M PB at XOD/GCE biosensor in the presence of 0.3 mM hypoxanthine. Applied potential -0.3 V vs. Ag/AgCl.

Figure 2. Effect of the applied potential on the amperometric response to 10 nM BPA at XOD/GCE biosensor in 0.1 M PB pH 7.5 in the presence of 0.3 mM hypoxanthine.

Figure 3. Calibration curves for the determination of BPA in 0.1 M PB pH 7.5 for three different enzyme concentrations in the presence of 0.3 mM hypoxanthine. Applied potential -0.5 V vs Ag/AgCl.

Figure 4. (a) Amperometric response at XOD/GCE in the presence of 0.3 mM hypoxanthine and (b) corresponding calibration curve and degree of inhibition for different concentrations of BPA in 0.1 M PBS pH 7.5. Applied potential - 0.5 V vs Ag/AgCl.

Figure 5. (a) Dixon plots and (b) Cornish-Bowden plots for BPA for three different hypoxanthine concentrations.

Figure 6. Graphical representation of (a) repeatability; (b) reproducibility and (c) stability of the XOD/GCE biosensor.

Figures

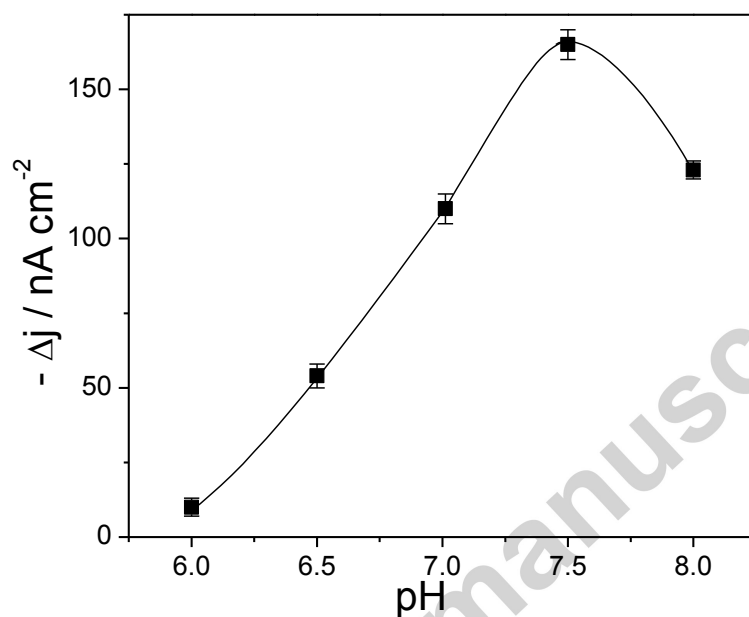


Figure 1. Effect of pH on the amperometric response to 10 nM BPA in 0.1 M PB at XOD/GCE biosensor in the presence of 0.3 mM hypoxanthine.

Applied potential -0.3 V vs. Ag/AgCl.

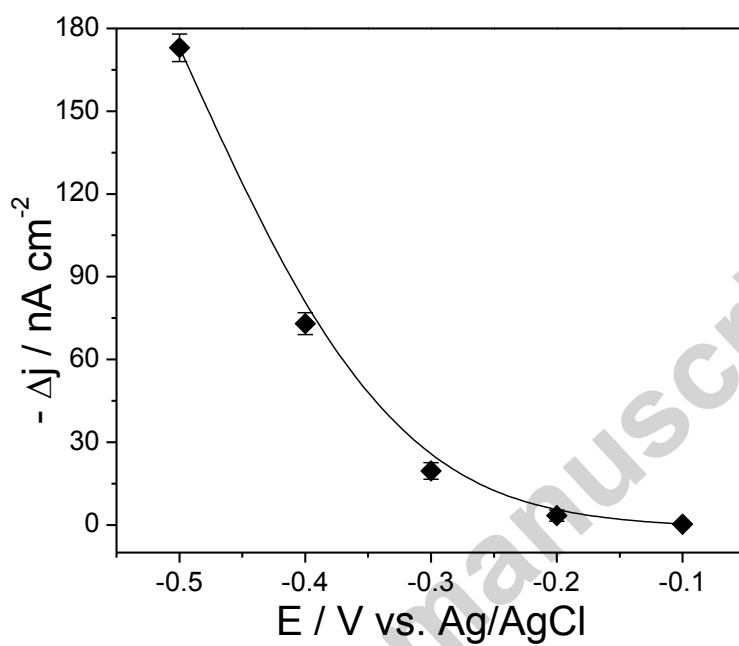


Figure 2. Effect of the applied potential on the amperometric response of 10 nM BPA at XOD/GCE biosensor in 0.1 M PB, pH 7.5 in the presence of 0.3 mM hypoxanthine.

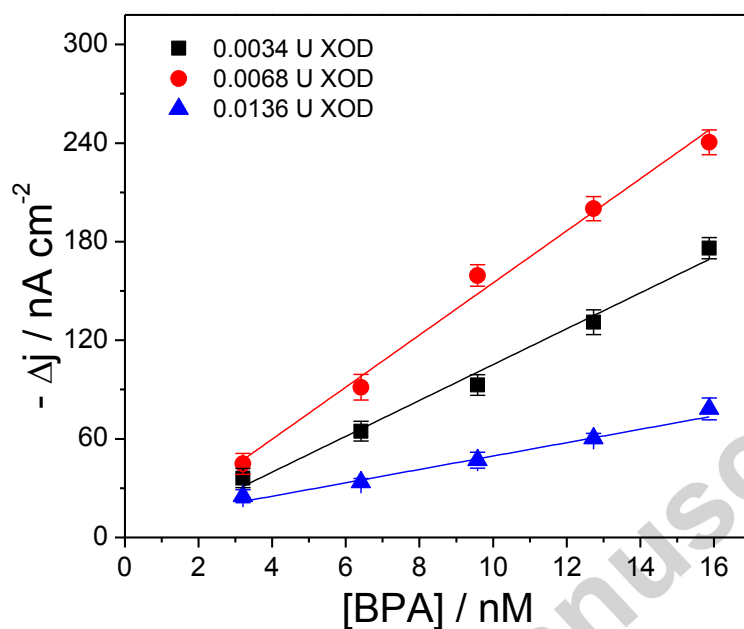


Figure 3. Calibration curves for the determination of BPA in 0.1 M PB pH 7.5 for three different enzyme concentrations in the presence of 0.3 mM hypoxanthine. Applied potential -0.5 V vs. Ag/AgCl.

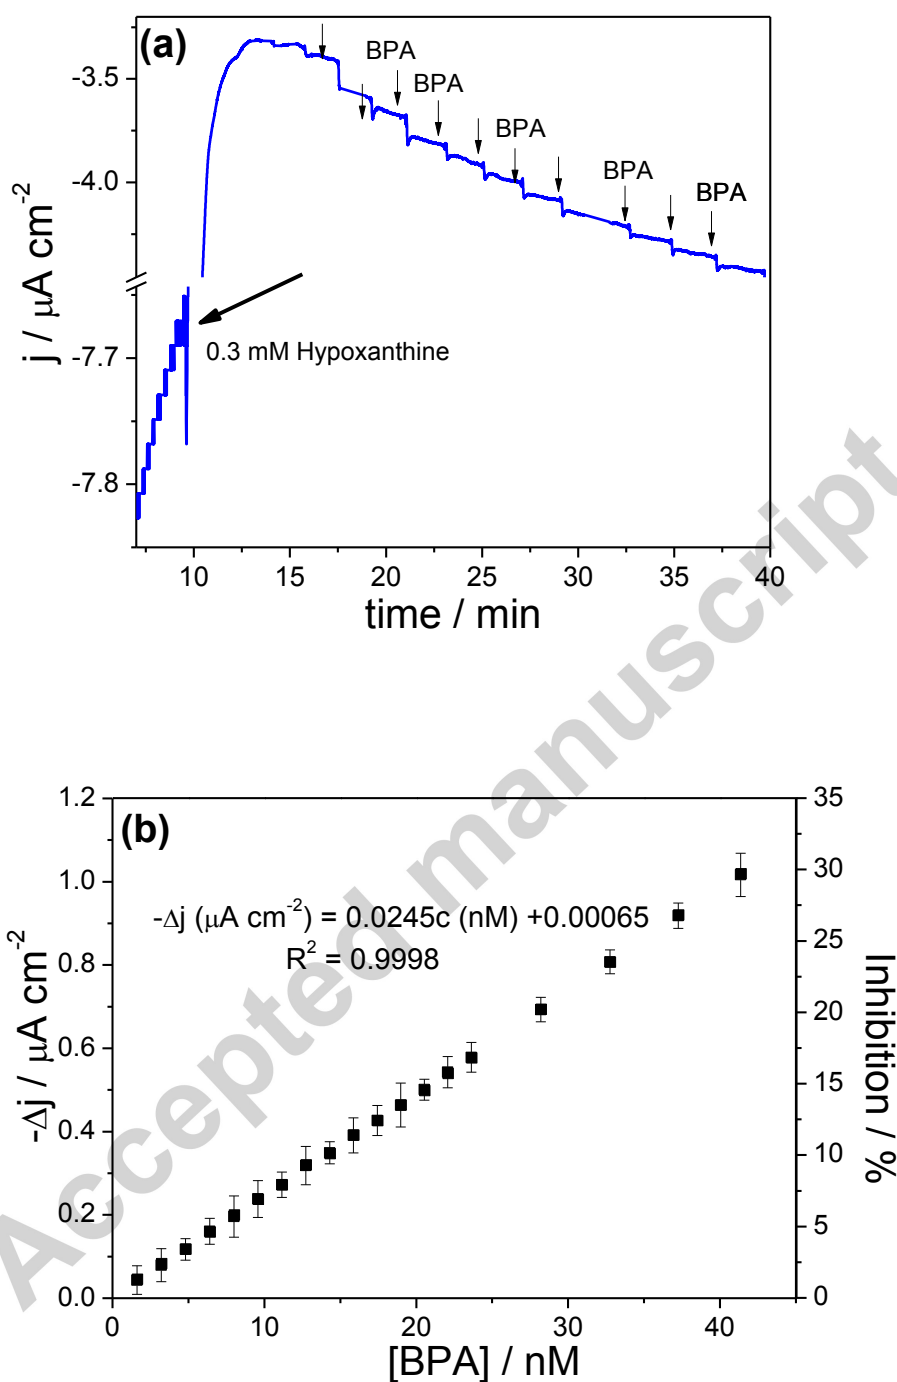


Figure 4. (a) Amperometric response at XOD/GCE in the presence of 0.3 mM hypoxanthine and (b) corresponding calibration curve and degree of inhibition for different concentrations of BPA in 0.1 M PB pH 7.5. Applied potential – 0.5 V vs Ag/AgCl.

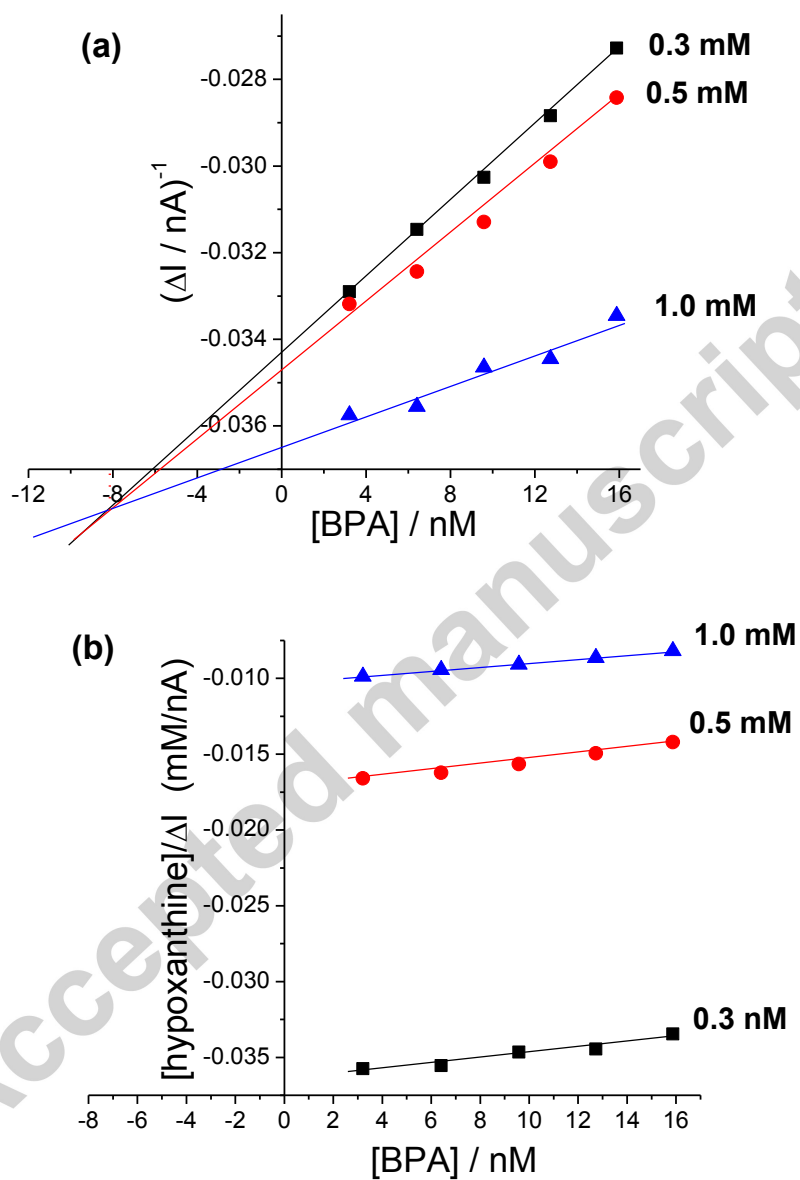


Figure 5. (a) Dixon plots and (b) Cornish-Bowden plots for BPA for three different hypoxanthine concentrations.

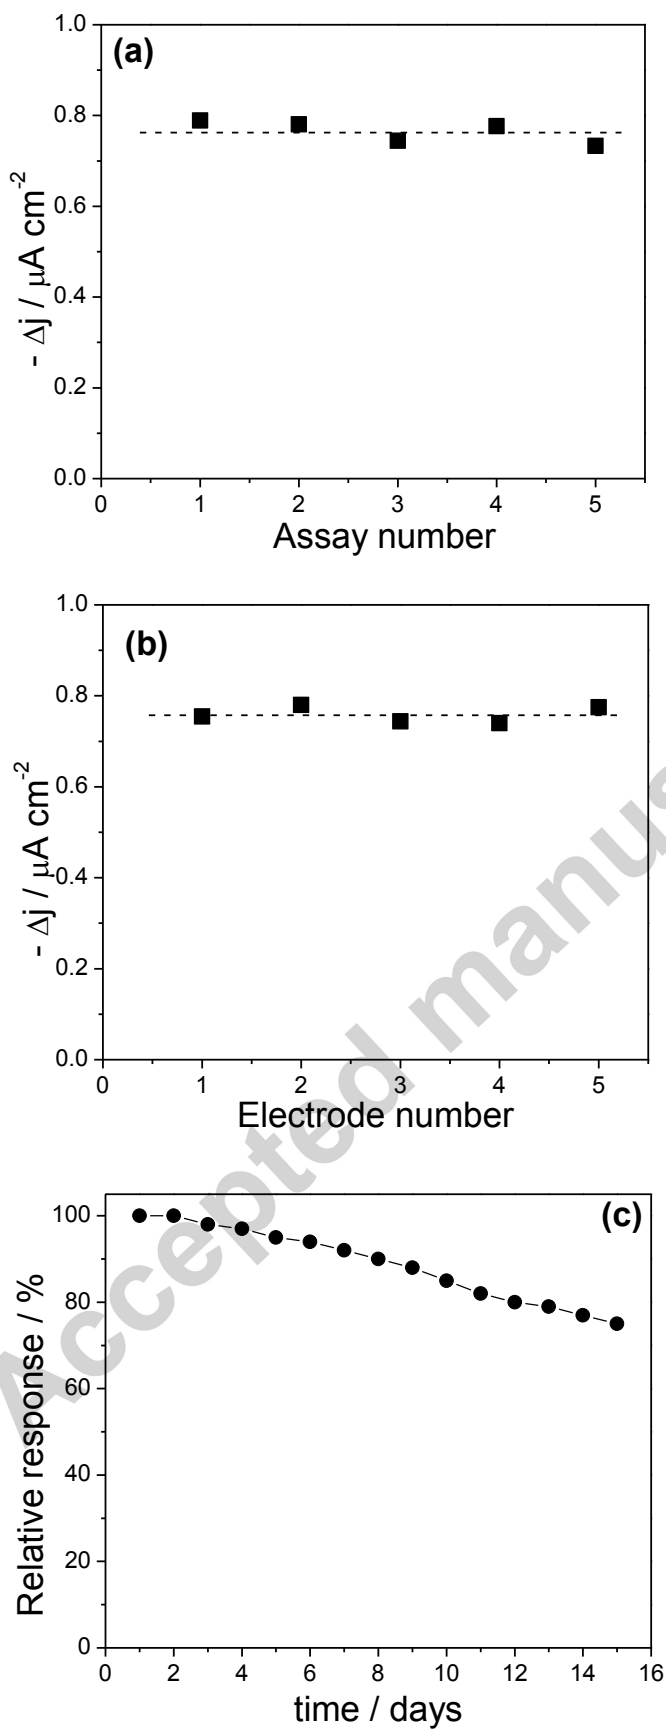


Figure 6. Graphical representation of (a) repeatability; (b) reproducibility and (c) stability of the XOD/GCE biosensor.

Highlights

- A novel electrochemical enzyme inhibition biosensor for bisphenol A was developed
- The biosensor uses xanthine oxidase enzyme and hypoxanthine enzyme substrate
- A very low detection limit of 1 nM was achieved
- The enzyme inhibition mechanism is reversible and competitive
- Application to analysis of mineral and river waters is demonstrated

Graphical abstract

A novel amperometric enzyme inhibition biosensor based on xanthine oxidase immobilised onto glassy carbon electrodes for bisphenol A determination

N. Ben Messaoud, M.E. Ghica, C. Dridi, M. Ben Ali, C.M.A. Brett

