

Article

A Tetrahedral DNA Nanostructure-Based MicroRNA Biosensor Coupled with Catalytic Recycling of the Analyte

Peng Miao, Bidou Wang, Xifeng Chen, Xiaoxi Li, and Yuguo Tang

ACS Appl. Mater. Interfaces, **Just Accepted Manuscript** • Publication Date (Web): 04 Mar 2015Downloaded from <http://pubs.acs.org> on March 5, 2015**Just Accepted**

"Just Accepted" manuscripts have been peer-reviewed and accepted for publication. They are posted online prior to technical editing, formatting for publication and author proofing. The American Chemical Society provides "Just Accepted" as a free service to the research community to expedite the dissemination of scientific material as soon as possible after acceptance. "Just Accepted" manuscripts appear in full in PDF format accompanied by an HTML abstract. "Just Accepted" manuscripts have been fully peer reviewed, but should not be considered the official version of record. They are accessible to all readers and citable by the Digital Object Identifier (DOI®). "Just Accepted" is an optional service offered to authors. Therefore, the "Just Accepted" Web site may not include all articles that will be published in the journal. After a manuscript is technically edited and formatted, it will be removed from the "Just Accepted" Web site and published as an ASAP article. Note that technical editing may introduce minor changes to the manuscript text and/or graphics which could affect content, and all legal disclaimers and ethical guidelines that apply to the journal pertain. ACS cannot be held responsible for errors or consequences arising from the use of information contained in these "Just Accepted" manuscripts.

**ACS Publications**
High quality. High impact.

ACS Applied Materials & Interfaces is published by the American Chemical Society.
1155 Sixteenth Street N.W., Washington, DC 20036
Published by American Chemical Society. Copyright © American Chemical Society.
However, no copyright claim is made to original U.S. Government works, or works
produced by employees of any Commonwealth realm Crown government in the course
of their duties.

**A Tetrahedral DNA Nanostructure-Based MicroRNA Biosensor
Coupled with Catalytic Recycling of the Analyte**

Peng Miao,^{*,†,‡} Bidou Wang,[†] Xifeng Chen,[†] Xiaoxi Li,[§] and Yuguo Tang^{*,†,‡}

[†] CAS Key Lab of Bio-Medical Diagnostics, Suzhou Institute of Biomedical Engineering and Technology, Chinese Academy of Sciences, Suzhou 215163, China

[‡] University of Chinese Academy of Sciences, Beijing 100049, China

[§] Department of Biochemistry and National Key Laboratory of Pharmaceutical Biotechnology, Nanjing University, Nanjing 210093, China

^{*} Corresponding authors. Tel.: +86 512 69588279; Fax: +86 512 69588283.

E-mail addresses: miaopeng@sibet.ac.cn (P. Miao); tangyg@sibet.ac.cn (Y. G. Tang).

Abstract

MicroRNAs are not only important regulators of a wide range of cellular processes, but also identified as promising disease biomarkers. Due to the low contents in serum, microRNAs are always difficult to be accurately detected. In this paper, an electrochemical biosensor for ultrasensitive detection of microRNA based on tetrahedral DNA nanostructure is developed. Four DNA single strands are engineered to form a tetrahedral nanostructure with a pendant stem-loop, and modified on a gold electrode surface, which largely enhances the molecular recognition efficiency. Moreover, taking advantage of strand displacement polymerization, catalytic recycling of microRNA, as well as silver nanoparticles (AgNPs)-based solid-state Ag/AgCl reaction, the proposed biosensor exhibits high sensitivity with the limit of detection (LOD) down to 0.4 fM. This biosensor shows great clinical value and may have practical utility in early diagnosis and prognosis of certain diseases.

Keywords: microRNA; tetrahedral DNA nanostructure; strand displacement reaction; silver nanoparticles; linear sweep voltammetry.

INTRODUCTION

MicroRNAs belong to small endogenous noncoding RNAs and regulate almost every cellular processes like cell growth, differentiation, apoptosis and autophagy at the post-transcriptional level.¹⁻³ In recent years, the investigation of biological roles of microRNA and potential clinical applications have been paid more and more attention.⁴⁻⁷ It is reported that the variation of numerous abnormal cellular processes accompanies the up- or down-regulation of microRNA expression.⁸ Therefore, microRNAs may provide a rich platform of biomarkers associating different diseases, and may greatly improve disease diagnosis in decreasing the percentage of false positives or replacing uncomfortable traditional diagnostic procedures.⁹⁻¹⁰ For example, although colonoscopy is the gold standard for the detection of colorectal cancer, the resulted discomfort makes it not suitable for cancer screening in general population. Plasma miR-409-3p, miR-7, and miR-93 levels can be detected and then used to distinguish colorectal cancer from healthy groups with high diagnostic accuracy.¹¹ Lung cancer is a major cause of death not only in China, but also in many western countries. Most of screening methods involve invasive operations and are always inaccurate. The level of miRNA-21 is found to be much higher in the serum or exhaled breath condensate of non-small-cell lung cancer patients and may have significant diagnostic value.¹²

At present, tremendous progresses have been made for the detection of microRNA.¹³⁻¹⁵ Northern blotting is widely accepted as the gold standard. Quantitative polymerase chain reaction (qPCR) is also a popular technique for

microRNA detection.¹⁶ However, these methods require labor intensive operations or expensive instruments and reagents, which cannot meet the high standards for point-of care testing (POCT) of microRNAs. Electrochemical biosensors have been utilized in many bioanalytical applications, owing to the advantages of simplicity, low cost, high sensitivity and fast response compared with other techniques like fluorescent assays.¹⁷⁻²³ Therefore, electrochemical techniques are promising analytical tools. However, due to the features of low contents, short sequences and high sequence homology among family members of microRNAs, signal amplification strategies should be included in electrochemical detection of microRNA.²⁴⁻²⁵ Moreover, optimization of electrode surface modification can also help improve the sensitivity and specificity.²⁶⁻²⁷

Herein, we fabricate an electrochemical biosensor for ultrasensitive detection of microRNA based on tetrahedral DNA nanostructure coupled with catalytic recycling of microRNA. The application of tetrahedral DNA nanostructure makes DNA monolayers well aligned on the surface of electrode with controlled density and orientation,²⁸⁻²⁹ which cuts the “backfilling” process like mercaptohexanol incubation and simplifies the immobilization steps.³⁰ The reactivity and accessibility can also be improved due to the DNA scaffold.³¹ In addition, strand displacement polymerization is employed which leads to the recycling of microRNA and the enzymatic amplification contributes to the high sensitivity of this method.³²⁻³³ The limit of detection (LOD) is as low as 0.4 fM. Single-base mismatch can be distinguished. This method also performs well for the detection of microRNA levels of breast cancer

patients. Therefore, it offers a great promise for early diagnosis and prognosis of certain diseases.

EXPERIMENTAL

Materials and Chemicals. Tris(2-carboxyethyl)phosphine hydrochloride (TCEP), diethypyrocarbonate (DEPC), silver nitrate (AgNO_3), sodium borohydride (NaBH_4) and trisodium citrate were purchased from Sigma-Aldrich (USA). Klenow fragment was obtained from New England Biolabs Ltd. (Beijing, China). Human serum samples were supplied by local hospital (Suzhou, China). Other reagents were of analytical grade and were used as received. All solutions were prepared with Milli-Q water ($18 \text{ M}\Omega\cdot\text{cm}$ resistivity) from a Millipore system. Oligonucleotides used were synthesized and purified by Takara Biotechnology Co., Ltd. (Dalian, China). The corresponding sequences were listed in Table 1.

Preparation of AgNPs-Labeled Signal Probe. Bare AgNPs were prepared by the borohydride reduction of AgNO_3 following the previously reported protocol.³⁴ Briefly, 100 mL of AgNO_3 and trisodium citrate solution was prepared with the concentration of 0.25 mM. Then, it was mixed with 3 mL of NaBH_4 solution (10 mM) under stirring for 30 min. The mixed solution exhibited the color of bright yellow and were left overnight in dark. The prepared AgNPs were then purified by three cycles of centrifugation at 12000g for 30 min. Afterward, AgNPs were incubated in signal probe (10 μM) for 24 h and were then further purified by centrifugation.

Self-Assembly of Tetrahedral DNA Nanostructure at Gold Electrode. The gold electrode with the diameter of 2 mm was cleaned prior to any modification.³⁵ It

was firstly soaked in piranha solution (98% H₂SO₄ : 30% H₂O₂ = 3 : 1) for 5 min (*Caution: Piranha solution reacts violently with organic solvents and should be handled with great care!*). Then, it was polished on P5000 sand paper and alumina slurry (1, 0.3 and 0.05 μm). Afterward, the electrode was cleaned by ultra-sonicating in ethanol and double-distilled water. The electrode was then treated with 50% HNO₃ for 30 min and electrochemically cleaned with 0.5 M H₂SO₄.

The tetrahedral DNA nanostructure consisted of four DNA strands were formed based on a modified protocol.³⁶ Tetrahedron A, B, C, and D were separately dissolved in the buffer solution (10 mM Tris-HCl, 10 mM TCEP, 50 mM MgCl₂, pH 8.0) with the concentration of 4 μM. To form the tetrahedral DNA nanostructure, 25 μL of each strands were mixed, heated to 95 °C for 2 min and then cooled to 4 °C. Afterward, 10 μL of the tetrahedral DNA nanostructure was dipped on the cleaned gold electrode and the reaction lasted for 8 h.

Strand Displacement and MicroRNA Recycling. 50 μL polymerase reaction solution (10 mM Tris-HCl, 50 mM NaCl, 10 mM MgCl₂, 1 mM dithiothreitol) containing 5 units of Klenow fragment, 2.5 nmol of dNTPs, 1 nmol of signal probe and different amount of microRNA were prepared. The tetrahedral DNA nanostructure modified electrode was incubated in the above polymerase reaction solution at 37 °C for 4 h.

Electrochemical Measurements. All electrochemical experiments were carried out on a CHI 660D electrochemical workstation (CH instruments, Shanghai, China). A three electrode system was used, which contained the platinum auxiliary electrode,

the Ag/AgCl reference electrode and the tetrahedral DNA nanostructure modified working electrode. Electrochemical impedance spectra (EIS) were performed in 5 mM $\text{Fe(CN)}_6^{3-/4-}$ with 1 M KNO_3 . The bias potential was 0.204 V, the amplitude was 5 mV and the frequency range was from 1 to 100 000 Hz. Linear sweep voltammetry (LSV) experiments were performed at room temperature. The scan rate was 100 mV/s and the electrolyte was 0.1 M KCl.

RESULTS AND DISCUSSION

Sensing Principle. Generally, a tetrahedral DNA nanostructure is designed with a pendant stem-loop to recognize target microRNA. As shown in Figure 1, four DNA single strands, tetrahedron A, B, C, and D, are engineered to form the six edges of the tetrahedral nanostructure through hybridization. Three vertexes of tetrahedron are modified with thiols, which facilitates the immobilization on the gold electrode surface.³⁷ Tetrahedron A also includes the stem-loop sequence, in which the underlined parts hybridize with each other and the italic part is the complementary sequence of target microRNA. Since tetrahedral DNA nanostructure-bottomed scaffold supports the stem-loop in the upright orientation, molecular recognition efficiency can be largely enhanced. In the presence of microRNA, the loop of tetrahedron A is opened by hybridization, which also releases single-stranded stem part that is complementary to the sequence within the signal probe. Signal probe is labeled with AgNPs, the diameter of which is around 4 nm (Figure S1). Since the $-(\text{CH}_2)_6-$ spacer between AgNPs and DNA sequence in the signal probe is flexible, the hybridization between signal probe and tetrahedron A is feasible. Moreover, Klenow

fragment can then initiate the polymerization of signal probe and the lengthening of new strand releases microRNA, which opens more loops, helps more signal probe hybridizations and triggers new strand displacement polymerization reactions. Finally, multiplication of AgNPs-labeled signal probes are localized on the electrode surface, which provide intensive electrochemical signals from highly characteristic solid-state Ag/AgCl reaction.³⁸

EIS Characterization. Electrochemical impedance spectra are employed to characterize the electrode modification steps. As shown in Figure 2a, nyquist plot of bare gold electrode contains no semicircle domain, indicating limited interfacial charge transfer resistance. After the immobilization of tetrahedral DNA nanostructure, a large semicircle is observed due to electrostatic repulsion towards $\text{Fe}(\text{CN})_6^{3-/4-}$ (Figure 2b). In the presence of microRNA and Klenow fragment, a large number of signal probes can be localized on the electrode surface. Figure 2c shows an even larger semicircle, which is ascribed to the repulsion from the hybridized signal probes without AgNPs labels. In the case of AgNPs-labeled signal probe, the semicircle gets much smaller (Figure 2d). The reason is that AgNPs is oxidized to Ag^+ , which facilitates the electron transfer between electrochemical species and electrode, and the interfacial charge transfer resistance is declined sharply. EIS results have confirmed well the electrode modification steps.

Linear Sweep Voltammetry Measurement of MicroRNA. We have then carried out LSV³⁹ to quantitatively determine microRNA concentration. As depicted in Figure 3, no current peak is present on bare gold electrode and tetrahedral DNA

1
2
3
4 nanostructure modified electrode in the absence of microRNA. A sharp current peak is
5
6 observed with 100 fM microRNA-mediated loop opening, signal probe
7
8 immobilization and catalytic recycling (curve c). However, if the signal probe is not
9
10 labeled with AgNPs, no peak appears (curve d), which demonstrates that the
11
12 electrochemical signal comes from stripping of AgNPs. Figure 4 shows the LSV
13
14 curves for the detection of microRNA with a series of concentrations. The inset
15
16 reveals a linear relationship between peak current and the logarithmic microRNA
17
18 concentration. The fitting equation is $y = -4.646 x - 71.316$ ($n = 3$, $R^2 = 0.995$), where
19
20 y is peak current and x is the logarithm of microRNA concentration. LOD is
21
22 calculated to be 0.4 fM (signal to noise ratio of 3), which is quite low.
23
24
25
26
27
28

29 The selectivity of this microRNA biosensor is then checked by comparing the
30
31 LSV results of single-base mismatch microRNAs, which are displayed in Figure 5.
32
33 The obtained low peak currents in the cases of mismatch microRNAs demonstrate
34
35 that they cannot initiate signal probe immobilization effectively, which verify the high
36
37 selectivity of this method.
38
39
40

41 **Detection of MicroRNA in Human Serum Samples.** Serum is a kind of
42
43 samples that can be conveniently obtained and tested for the detection of different
44
45 disease biomarkers. To further check the practical utility of this microRNA biosensor,
46
47 serum samples from breast cancer patients are directly detected. Then, we add
48
49 different amount of target microRNA to the samples and again measure target
50
51 microRNA levels by the proposed method. Table 2 shows the detected results and the
52
53 recoveries, which verify that this method is accurate and can be effectively applied in
54
55
56
57
58
59
60

biological fluids.

CONCLUSIONS

In summary, we have fabricated an electrochemical biosensor for ultrasensitive detection of microRNA based on tetrahedral DNA nanostructure, coupled with strand displacement polymerization-mediated catalytic recycling of microRNA. The electrochemical signal originates from AgNPs-based solid-state Ag/AgCl reaction on signal DNA probe. This method is simply operated and highly sensitive due to the tetrahedral DNA nanostructure and strand displacement amplification. The LOD is 0.4 fM and a wide linear range is obtained from 1 fM to 1 nM. It is also examined by human serum samples and the satisfactory results demonstrate its potential practical utility towards microRNA assay for early diagnosis and prognosis of certain diseases.

ACKNOWLEDGMENTS

This work was supported by the National Natural Science Foundation of China (Grant no. 31400847) and the Natural Science Foundation of Jiangsu Province of China (Grant No. BK20141204).

Supporting Information Available

Additional information as noted in text. This material is available free of charge via the Internet at <http://pubs.acs.org>.

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

REFERENCES

(1) Jing, Z.; Han, W. D.; Sui, X. B.; Xie, J. S.; Pan, H. M. Interaction of Autophagy with MicroRNAs and Their Potential Therapeutic Implications in Human Cancers. *Cancer Lett.* **2015**, *356*, 332-338.

(2) Yang, L.; Liu, C. H.; Ren, W.; Li, Z. P. Graphene Surface-Anchored Fluorescence Sensor for Sensitive Detection of MicroRNA Coupled with Enzyme-Free Signal Amplification of Hybridization Chain Reaction. *ACS Appl. Mater. Interfaces* **2012**, *4*, 6450-6453.

(3) Raitoharju, E.; Oksala, N.; Lehtimaki, T. MicroRNAs in the Atherosclerotic Plaque. *Clin. Chem.* **2013**, *59*, 1708-1721.

(4) Leite-Moreira, A. M.; Lourenco, A. P.; Falcao-Pires, I.; Leite-Moreira, A. F. Pivotal Role of MicroRNAs in Cardiac Physiology and Heart Failure. *Drug Discovery Today* **2013**, *18*, 1243-1249.

(5) Yin, P. T.; Shah, B. P.; Lee, K. B. Combined Magnetic Nanoparticle-based MicroRNA and Hyperthermia Therapy to Enhance Apoptosis in Brain Cancer Cells. *Small* **2014**, *10*, 4106-4112.

(6) Su, T. H.; Liu, C. H.; Liu, C. J.; Chen, C. L.; Ting, T. T.; Tseng, T. C.; Chen, P. J.; Kao, J. H.; Chen, D. S. Serum MicroRNA-122 Level Correlates with Virologic Responses to Pegylated Interferon Therapy in Chronic Hepatitis C. *Proc. Natl. Acad. Sci. U. S. A.* **2013**, *110*, 7844-7849.

(7) Kasuga, H.; Fukuyama, M.; Kitazawa, A.; Kontani, K.; Katada, T. The MicroRNA miR-235 Couples Blast-Cell Quiescence to the Nutritional State. *Nature*

2013, 497, 503-506.

(8) Catto, J. W. F.; Miah, S.; Owen, H. C.; Bryant, H.; Myers, K.; Dudziec, E.; Larre, S.; Milo, M.; Rehman, I.; Rosario, D. J.; Di Martino, E.; Knowles, M. A.; Meuth, M.; Harris, A. L.; Hamdy, F. C. Distinct MicroRNA Alterations Characterize High- and Low-Grade Bladder Cancer. *Cancer Res.* **2009**, 69, 8472-8481.

(9) Jou, A. F. J.; Lu, C. H.; Ou, Y. C.; Wang, S. S.; Hsu, S. L.; Willner, I.; Ho, J. A. A. Diagnosing the miR-141 Prostate Cancer Biomarker Using Nucleic Acid-Functionalized CdSe/ZnS QDs and Telomerase. *Chem. Sci.* **2015**, 6, 659-665.

(10) Tran, H. V.; Piro, B.; Reisberg, S.; Nguyen, L. H.; Nguyen, T. D.; Duc, H. T.; Pham, M. C. An Electrochemical ELISA-Like Immunosensor for MiRNAs Detection Based on Screen-Printed Gold Electrodes Modified with Reduced Graphene Oxide and Carbon Nanotubes. *Biosens. Bioelectron.* **2014**, 62, 25-30.

(11) Wang, S. Y.; Xiang, J. B.; Li, Z. Y.; Lu, S. H.; Hu, J.; Gao, X.; Yu, L.; Wang, L.; Wang, J. P.; Wu, Y.; Chen, Z. Y.; Zhu, H. G. A Plasma MicroRNA Panel for Early Detection of Colorectal Cancer. *Int. J. Cancer* **2015**, 136, 152-161.

(12) Mozzoni, P.; Banda, I.; Goldoni, M.; Corradi, M.; Tiseo, M.; Acampa, O.; Balestra, V.; Ampollini, L.; Casalini, A.; Carbognani, P.; Mutti, A. Plasma and EBC MicroRNAs as Early Biomarkers of Non-Small-Cell Lung Cancer. *Biomarkers* **2013**, 18, 679-686.

(13) Dong, H. F.; Lei, J. P.; Ding, L.; Wen, Y. Q.; Ju, H. X.; Zhang, X. J. MicroRNA: Function, Detection, and Bioanalysis. *Chem. Rev.* **2013**, 113, 6207-6233.

(14) Miao, P.; Meng, F. Y.; Wang, B. D.; Zhu, X. L.; Tang, Y. G. Highly Sensitive

MicroRNA Quantification with Zero Background Signal from Silver Nanoparticles.

Electrochem. Commun. **2015**, *51*, 89-92.

(15) Yan, L.; Yan, Y. Y.; Pei, L.; Wei, W.; Zhao, J. A G-Quadruplex DNA-Based, Label-Free and Ultrasensitive Strategy for MicroRNA Detection. *Sci. Rep.* **2014**, *4*, 7400.

(16) Chen, C. F.; Ridzon, D. A.; Broomer, A. J.; Zhou, Z. H.; Lee, D. H.; Nguyen, J. T.; Barbisin, M.; Xu, N. L.; Mahuvakar, V. R.; Andersen, M. R.; Lao, K. Q.; Livak, K. J.; Guegler, K. J. Real-Time Quantification of MicroRNAs by Stem-Loop RT-PCR. *Nucleic Acids Res.* **2005**, *33*, e179.

(17) Yang, F.; Zuo, X. L.; Li, Z. H.; Deng, W. P.; Shi, J. Y.; Zhang, G. J.; Huang, Q.; Song, S. P.; Fan, C. H. A Bubble-Mediated Intelligent Microscale Electrochemical Device for Single-Step Quantitative Bioassays. *Adv. Mater.* **2014**, *26*, 4671-4676.

(18) Miao, P.; Liu, L.; Li, Y.; Li, G. X. A Novel Electrochemical Method to Detect Mercury (II) Ions. *Electrochem. Commun.* **2009**, *11*, 1904-1907.

(19) Li, D.; Liu, J. Q.; Barrow, C. J.; Yang, W. R. Protein Electrochemistry Using Graphene-Based Nano-Assembly: An Ultrasensitive Electrochemical Detection of Protein Molecules via Nanoparticle-Electrode Collisions. *Chem. Commun.* **2014**, *50*, 8197-8200.

(20) Shin, I. S.; Chand, R.; Lee, S. W.; Rhee, H. W.; Kim, Y. S.; Hong, J. I. Homogeneous Electrochemical Assay for Protein Kinase Activity. *Anal. Chem.* **2014**, *86*, 10992-10995.

(21) Kabashima, T.; Yu, Z. Q.; Tang, C. H.; Nakagawa, Y.; Okumura, K.; Shibata, T.;

Lu, J. Z.; Kai, M. A Selective Fluorescence Reaction for Peptides and Chromatographic Analysis. *Peptides* **2008**, *29*, 356-363.

(22) Tonooka, K.; Kabashima, T.; Shibata, T.; Tang, C. H.; Yu, Z. Q.; Kai, M. S. Facile Assay of Telomerase Activity Utilizing a DNA-Detectable Chemiluminogenic Reagent. *Anal. Sci.* **2008**, *24*, 471-475.

(23) Yu, Z. Q.; Kabashima, T.; Tang, C. H.; Shibata, T.; Kitazato, K.; Kobayashi, N.; Lee, M. K.; Kai, M. Selective and Facile Assay of Human Immunodeficiency Virus Protease Activity by a Novel Fluorogenic Reaction. *Anal. Biochem.* **2010**, *397*, 197-201.

(24) Miao, P.; Wang, B. D.; Yu, Z. Q.; Zhao, J.; Tang, Y. G. Ultrasensitive Electrochemical Detection of MicroRNA with Star Trigon Structure and Endonuclease Mediated Signal Amplification. *Biosens. Bioelectron.* **2015**, *63*, 365-370.

(25) Zhu, G. C.; Liang, L.; Zhang, C. Y. Quencher-Free Fluorescent Method for Homogeneously Sensitive Detection of MicroRNAs in Human Lung Tissues. *Anal. Chem.* **2014**, *86*, 11410-11416.

(26) Pawlak, M.; Grygoliwicz-Pawlak, E.; Crespo, G. A.; Mistlberger, G.; Bakker, E. PVC-Based Ion-Selective Electrodes with Enhanced Biocompatibility by Surface Modification with "Click" Chemistry. *Electroanalysis* **2013**, *25*, 1840-1846.

(27) Ning, L. M.; Li, X. X.; Yang, D. W.; Miao, P.; Ye, Z. H.; Li, G. X. Measurement of Intracellular pH Changes Based on DNA-Templated Capsid Protein Nanotubes. *Anal. Chem.* **2014**, *86*, 8042-8047.

- (28) Pei, H.; Wan, Y.; Li, J.; Hu, H. Y.; Su, Y.; Huang, Q.; Fan, C. H. Regenerable Electrochemical Immunological Sensing at DNA Nanostructure-Decorated Gold Surfaces. *Chem. Commun.* **2011**, 47, 6254-6256.
- (29) Lu, N.; Pei, H.; Ge, Z. L.; Simmons, C. R.; Yan, H.; Fan, C. H. Charge Transport within a Three-Dimensional DNA Nanostructure Framework. *J. Am. Chem. Soc.* **2012**, 134, 13148-13151.
- (30) Miao, P.; Tang, Y. G.; Wang, B. D.; Han, K.; Chen, X. F.; Sun, H. X. An Aptasensor for Detection of Potassium Ions Based on RecJ(f) Exonuclease Mediated Signal Amplification. *Analyst* **2014**, 139, 5695-5699.
- (31) Li, Z. H.; Zhao, B.; Wang, D. F.; Wen, Y. L.; Liu, G.; Dong, H. Q.; Song, S. P.; Fan, C. H. DNA Nanostructure-Based Universal Microarray Platform for High-Efficiency Multiplex Bioanalysis in Biofluids. *ACS Appl. Mater. Interfaces* **2014**, 6, 17944-17953.
- (32) Zou, B. J.; Song, Q. X.; Wang, J. P.; Liu, Y. L.; Zhou, G. H. Invasive Reaction Assisted Strand-Displacement Signal Amplification for Sensitive DNA Detection. *Chem. Commun.* **2014**, 50, 13722-13724.
- (33) Hu, Y. H.; Xu, X. Q.; Liu, Q. H.; Wang, L.; Lin, Z. Y.; Chen, G. N. Ultrasensitive Electrochemical Biosensor for Detection of DNA from *Bacillus subtilis* by Coupling Target-Induced Strand Displacement and Nicking Endonuclease Signal Amplification. *Anal. Chem.* **2014**, 86, 8785-8790.
- (34) Miao, P.; Han, K.; Sun, H. X.; Yin, J.; Zhao, J.; Wang, B. D.; Tang, Y. G. Melamine Functionalized Silver Nanoparticles as the Probe for Electrochemical

Sensing of Clenbuterol. *ACS Appl. Mater. Interfaces* **2014**, *6*, 8667-8672.

(35)Miao, P.; Wang, B. D.; Han, K.; Tang, Y. G. Electrochemical Impedance Spectroscopy Study of Proteolysis Using Unmodified Gold Nanoparticles. *Electrochem. Commun.* **2014**, *47*, 21-24.

(36)Ge, Z. L.; Lin, M. H.; Wang, P.; Pei, H.; Yan, J.; Sho, J. Y.; Huang, Q.; He, D. N.; Fan, C. H.; Zuo, X. L. Hybridization Chain Reaction Amplification of MicroRNA Detection with a Tetrahedral DNA Nanostructure-Based Electrochemical Biosensor. *Anal. Chem.* **2014**, *86*, 2124-2130.

(37)Hsu, M. H.; Chuang, H.; Cheng, F. Y.; Huang, Y. P.; Han, C. C.; Chen, J. Y.; Huang, S. C.; Chen, J. K.; Wu, D. S.; Chu, H. L.; Chang, C. C. Directly Thiolated Modification onto the Surface of Detonation Nanodiamonds. *ACS Appl. Mater. Interfaces* **2014**, *6*, 7198-7203.

(38)Zhang, J.; Ting, B. P.; Jana, N. R.; Gao, Z. Q.; Ying, J. Y. Ultrasensitive Electrochemical DNA Biosensors Based on the Detection of a Highly Characteristic Solid-State Process. *Small* **2009**, *5*, 1414-1417.

(39)Meng, F. B.; Yang, J. H.; Liu, T.; Zhu, X. L.; Li, G. X. Electric Communication between the Inner Part of a Cell and an Electrode: The Way To Look inside a Cell. *Anal. Chem.* **2009**, *81*, 9168-9171.

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Figures and Tables

Figure 1. Schematic illustration of the tetrahedral DNA nanostructure-based microRNA biosensor.

Figure 2. Nyquist diagrams of impedance spectra for (a) bare gold electrode, (b) tetrahedral DNA nanostructure modified electrode, (c) after strand displacement and catalytic recycling of microRNA with signal probe which is not labeled with AgNPs, (d) is the case using AgNPs-labeled signal probe.

Figure 3. Linear sweep voltammograms of (a) bare gold electrode, tetrahedral DNA nanostructure modified electrode after strand displacement reaction in the (b) absence and (c) presence of 100 fM microRNA, (d) is the case in the presence of 100 fM microRNA using signal probe without AgNPs labels.

Figure 4. Linear sweep voltammograms of tetrahedral DNA nanostructure modified electrode for the detection of microRNA with the concentration of 1 fM, 5 fM, 10 fM, 100 fM, 1 pM, 10 pM, 100 pM and 1 nM (from top to bottom). Inset is the calibration plot of the peak current versus the logarithmic microRNA concentration. Error bars represent standard deviations of three independent measurements.

Figure 5. Comparison of LSV signal intensity in the cases of target and three single-base mismatch microRNAs with the concentration of 100 fM.

Table 1. DNA and RNA sequences used in this work.

Table 2. Measurements of miRNA-21 in serum samples from breast cancer patients.

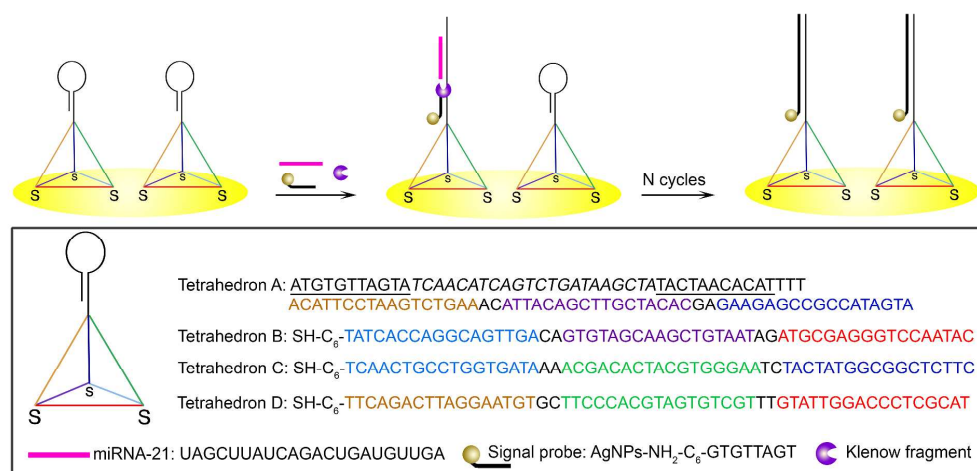


Figure 1. Schematic illustration of the tetrahedral DNA nanostructure-based microRNA biosensor.

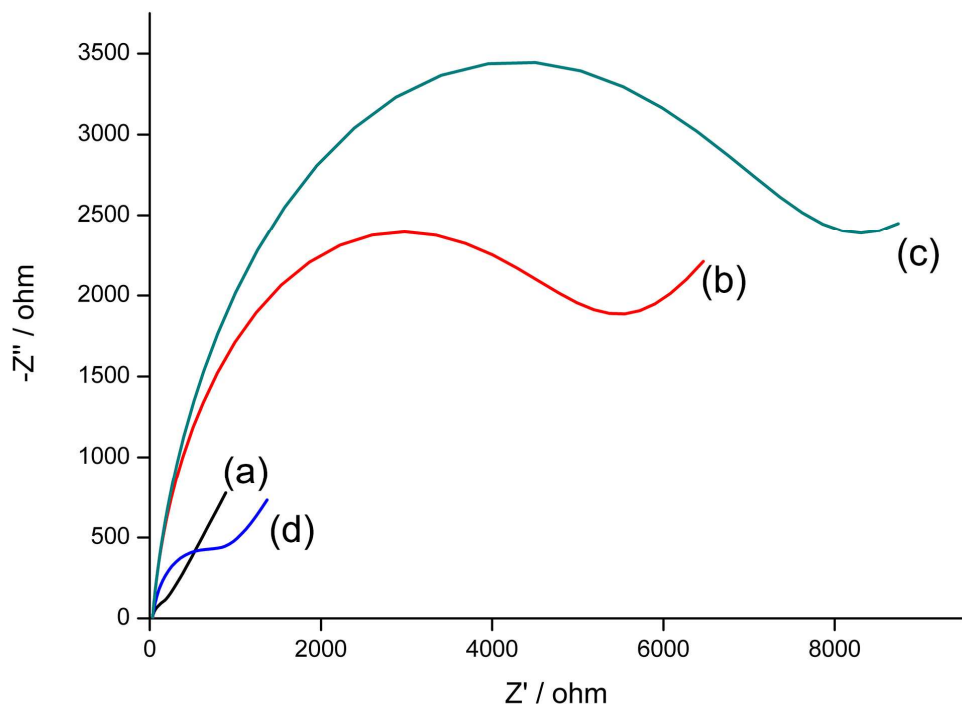


Figure 2. Nyquist diagrams of impedance spectra for (a) bare gold electrode, (b) tetrahedral DNA nanostructure modified electrode, (c) after strand displacement and catalytic recycling of microRNA with signal probe which is not labeled with AgNPs, (d) is the case using AgNPs-labeled signal probe.

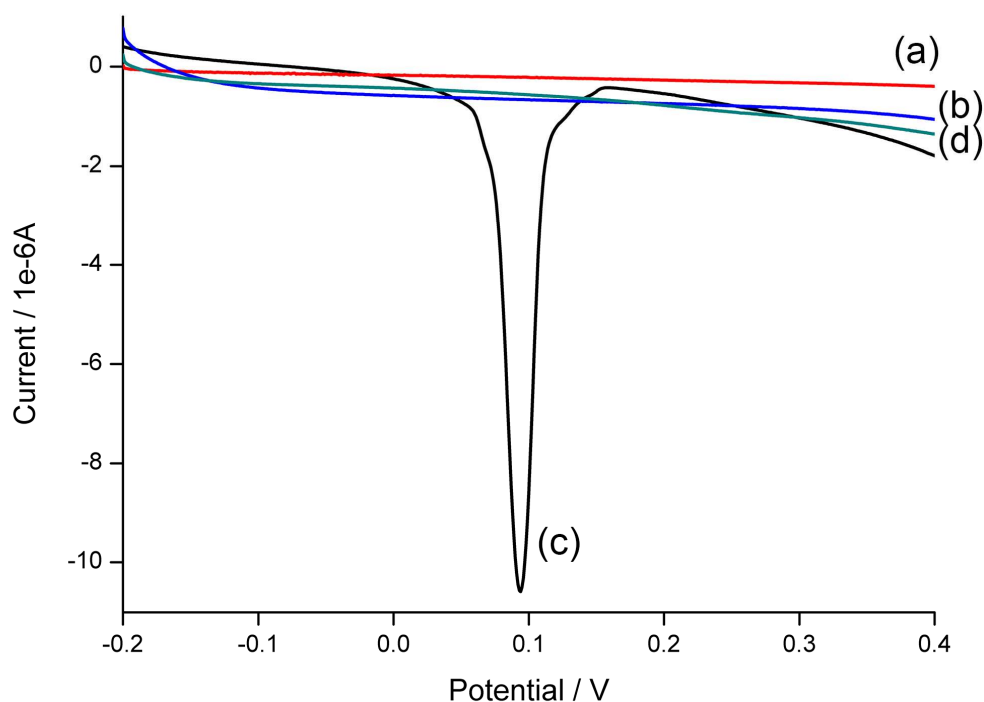


Figure 3. Linear sweep voltammograms of (a) bare gold electrode, tetrahedral DNA nanostructure modified electrode after strand displacement reaction in the (b) absence and (c) presence of 100 fM microRNA, (d) is the case in the presence of 100 fM microRNA using signal probe without AgNPs labels.

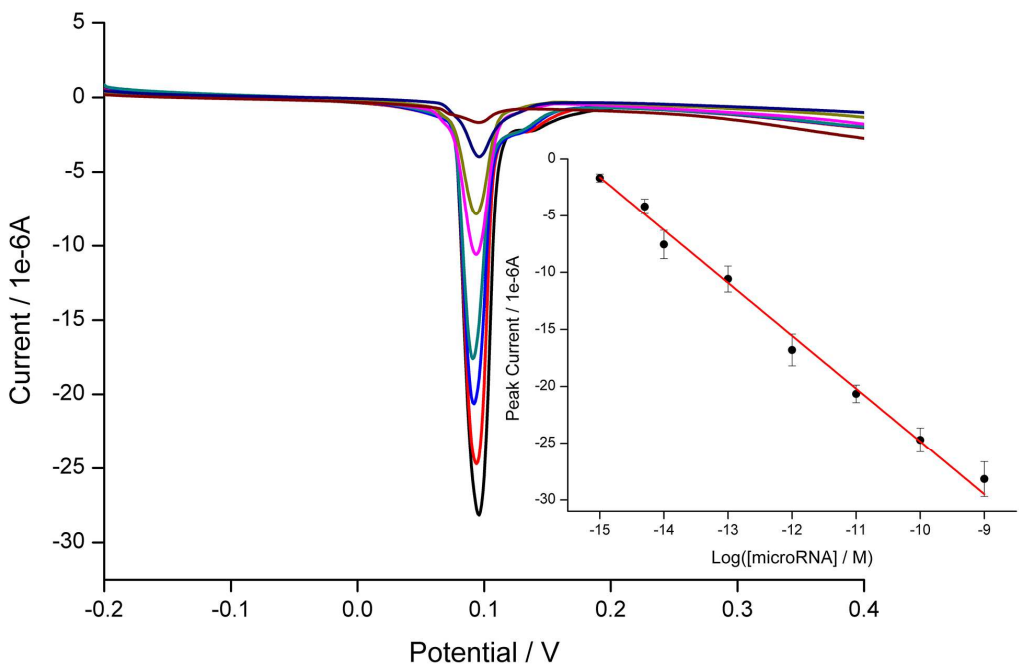


Figure 4. Linear sweep voltammograms of tetrahedral DNA nanostructure modified electrode for the detection of microRNA with the concentration of 1 fM, 5 fM, 10 fM, 100 fM, 1 pM, 10 pM, 100 pM and 1 nM (from top to bottom). Inset is the calibration plot of the peak current versus the logarithmic microRNA concentration. Error bars represent standard deviations of three independent measurements.

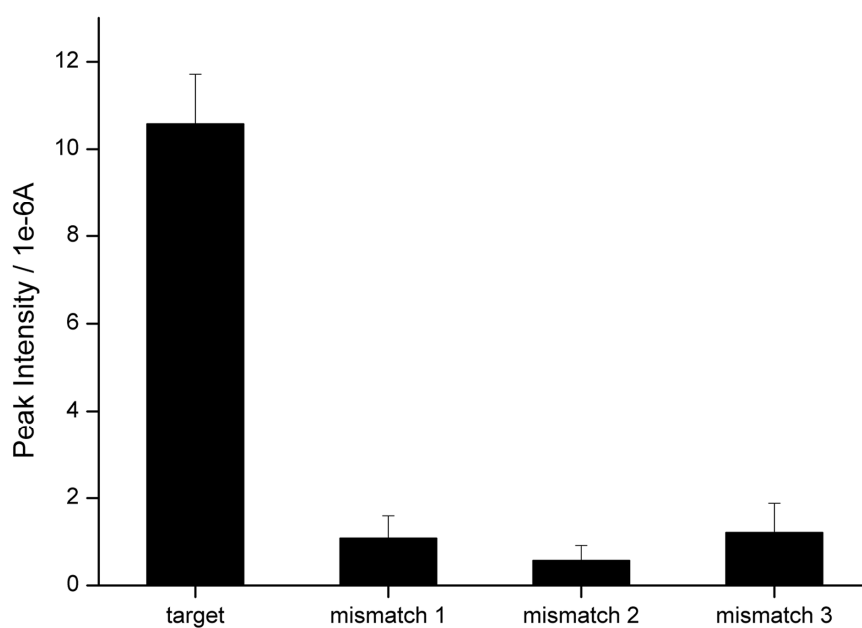


Figure 5. Comparison of LSV signal intensity in the cases of target and three single-base mismatch microRNAs with the concentration of 100 fM.

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Table 1. DNA and RNA sequences used in this work.

Name	Sequence (5'-3')
Tetrahedron A	ATGTGTTAGTATCAACATCAGTCTGATAAGCTATACTAACAC ATTTTACATTCCCTAAGTCTGAAACATTACAGCTTGCTACACG AGAAGAGCCGCCATAGTA
Tetrahedron B	SH-C ₆ -TATCACCAGGCAGTTGACAGTGTAGCAAGCTGTAAT AGATGCGAGGGTCCAATAC
Tetrahedron C	SH-C ₆ -TCAACTGCCTGGTGATAAAACGACACTACGTGGGAA TCTACTATGGCGGCTCTTC
Tetrahedron D	SH-C ₆ -TTCAGACTTAGGAATGTGCTTCCCACGTAGTGTGCGTT TGTATTGGACCCTCGCAT
miRNA-21	UAGCUUAUCAGACUGAUGUUGA
Mismatch 1	U <u>C</u> GCUUAUCAGACUGAUGUUGA
Mismatch 2	UAGCUUAUCAG <u>T</u> CUGAUGUUGA
Mismatch 3	UAGCUUAUCAGACUGAUGU <u>A</u> GA
Signal probe	AgNPs-NH ₂ -C ₆ -GTGTTAGT

Table 2. Measurements of miRNA-21 in serum samples from breast cancer patients.

Sample	Detected (pM)	Added (pM)	Found (pM)	Recovery (%)
Serum 1	0.86	1.0	1.92	103.2
		5.0	5.99	102.2
Serum 2	1.43	1.0	2.37	97.5
		5.0	6.53	101.6

TOC

