

Article

3D Cu foam-supported single crystalline mesoporous Cu₂O nanothorn arrays for ultra-highly sensitive and efficient nonenzymatic detection of glucose

Chaoqun Dong, Hua Zhong, Tianyi Kou, Jan Frenzel, Gunther Eggeler, and Zhonghua Zhang

ACS Appl. Mater. Interfaces, **Just Accepted Manuscript** • DOI: 10.1021/acsami.5b05738 • Publication Date (Web): 25 Aug 2015Downloaded from <http://pubs.acs.org> on August 27, 2015**Just Accepted**

"Just Accepted" manuscripts have been peer-reviewed and accepted for publication. They are posted online prior to technical editing, formatting for publication and author proofing. The American Chemical Society provides "Just Accepted" as a free service to the research community to expedite the dissemination of scientific material as soon as possible after acceptance. "Just Accepted" manuscripts appear in full in PDF format accompanied by an HTML abstract. "Just Accepted" manuscripts have been fully peer reviewed, but should not be considered the official version of record. They are accessible to all readers and citable by the Digital Object Identifier (DOI®). "Just Accepted" is an optional service offered to authors. Therefore, the "Just Accepted" Web site may not include all articles that will be published in the journal. After a manuscript is technically edited and formatted, it will be removed from the "Just Accepted" Web site and published as an ASAP article. Note that technical editing may introduce minor changes to the manuscript text and/or graphics which could affect content, and all legal disclaimers and ethical guidelines that apply to the journal pertain. ACS cannot be held responsible for errors or consequences arising from the use of information contained in these "Just Accepted" manuscripts.



ACS Publications

3D Cu foam-supported single crystalline mesoporous Cu₂O
nanothorn arrays for ultra-highly sensitive and efficient
nonenzymatic detection of glucose

Chaoqun Dong,^a Hua Zhong,^b Tianyi Kou,^{a,†} Jan Frenzel,^c Gunther Eggeler,^c
Zhonghua Zhang^{a,*}

^aKey Laboratory for Liquid-Solid Structural Evolution and Processing of Materials (Ministry of Education), School of Materials Science and Engineering, Shandong University, Jingshi Road 17923, Jinan 250061, P.R. China

^bDermatological department of Qilu Hospital of Shandong University, Jinan Culture Road 107, Jinan 250012, P. R. China

^cInstitut für Werkstoffe, Ruhr Universität Bochum, Bochum 44780, Germany

[†] Present address: Department of Chemistry and biochemistry, University of California Santa Cruz, 1156 High Street, Santa Cruz 95064, United States

*Corresponding author. Email: zh_zhang@sdu.edu.cn (Z. Zhang), Tel/Fax: +86-531-88396978.

Keywords: biosensors, catalysis, nanostructures, nanothorn arrays, hybrid materials

Abstract

Highly sensitive and efficient biosensors play a crucial role in clinical, environmental, industrial and agricultural applications, and tremendous efforts have been dedicated to advanced electrode materials with superior electrochemical activities and low cost. Here, we report a 3D binder-free Cu foam-supported Cu₂O nanothorn arrays electrode developed *via* facile electrochemistry. The nanothorns *in-situ* growing along the specific direction of $\langle 01\bar{1} \rangle$ have single crystalline features and mesoporous surface. When using as a potential biosensor for the non-enzyme glucose detection, the hybrid electrode exhibits multi-stage linear detection ranges with ultrahigh sensitivities (maximum of 97.9 mA mM⁻¹ cm⁻²) and an ultralow detection limit of 5 nM. Furthermore, the electrode presents outstanding selectivity and stability towards glucose detection. The distinguished performances endow this novel electrode with powerful reliability for analyzing human serum samples. These unprecedented sensing characteristics could be ascribed to the synergistic action of superior electrochemical catalytic activity of nanothorn arrays with dramatically enhanced surface area and intimate contact between the active material (Cu₂O) and current collector (Cu foam), concurrently supplying good conductivity for electrons/ions transport during glucose biosensing. Significantly, our finding could guide the fabrication of new metal oxide nanostructures with well-organized morphologies and unique properties as well as low materials cost.

Introduction

Highly sensitive and efficient detection of glucose concentration plays a critical role in clinical, environmental, industrial and agricultural applications, and various approaches to glucose sensing have been explored based on electrochemical, fluorescent, optical, transdermal and acoustic signals.^{1, 2} Among these techniques, the electrochemical biosensors have aroused more interests in the past decades, owing to their unbeaten virtues such as high sensitivity, lower detection limit, high selectivity, and easy operation.³⁻⁵ Most previous research on the electrochemical detection of glucose was involved in the use of glucose oxidase (GOD), which can identify glucose molecules quickly and accurately by catalyzing the oxidation process of glucose to gluconolactone.^{6, 7} Whereas, due to the intrinsic properties of enzymes, GOD-based biosensors suffer from poor reproducibility, complex enzyme immobilization and high sensitivity to the external conditions (for example, temperature, pH, humidity and so on), leading to a decrease in GOD activity in certain cases.^{8, 9} Besides, the high price of enzymes impedes the broader applications of enzymatic glucose. Because of these, the emergence of non-enzyme biosensors has provided another choice for stable and cost-effective glucose biosensing devices.¹⁰

The intimate relationship between the microstructures and corresponding biological sensing properties of the active materials such as dimension, shape, porosity and surface area has stimulated tremendous efforts to develop novel enzyme-free electrode materials to realize the optimization of mass- and charge transport and then minimize resistances during biosensing.¹¹⁻¹³ Nanostructured metal

1
2
3
4 oxides have been found to possess interesting nano-morphology, multiple oxidation
5
6 states, and good biological compatibility.^{6, 14, 15} These unique properties of nanosized
7
8 metal oxides could alleviate the problems of expensive enzymatic glucose sensors.
9
10 Nevertheless, metal oxides possess the inferior electronic conductivity, which greatly
11
12 restricts their wide applications for biosensors with superior performance.¹¹ To
13
14 improve the electronic conductivity of oxides, it is normal to construct composite
15
16 materials by hybridizing with carbon-based materials¹⁶⁻¹⁸ and noble metal
17
18 nanoparticles.^{19, 20} Moreover, the intimate interface contact between the current
19
20 collector and the highly electrocatalytic materials is crucial to enhance the electronic
21
22 conductivity of electrodes and taking full advantage of electroactive substances.
23
24
25
26
27

28
29 Among various nonenzymatic metal oxides-based glucose sensors,
30
31 nanostructured copper oxides (Cu₂O and CuO) arouse considerable attention owing to
32
33 their outstanding electrochemical activity, low-cost, ease of synthesis, and other
34
35 advantages.²¹⁻²³ For example, Kong et al.²⁴ developed a copper oxide electrode with
36
37 hollow structure and good glucose sensing properties. However, it is so far a
38
39 formidable task to fabricate glucose biosensors with superior performance, which can
40
41 continuously detect low glucose concentrations in unconventional body fluids (like
42
43 tears, saliva, etc.).^{11, 21}
44
45
46
47
48

49 Here, we report a 3D Cu foam-supported mesoporous Cu₂O nanothorn arrays
50
51 electrode, fabricated through a facile and economic electrochemical route, for
52
53 enzyme-free electrochemical glucose detector. The nanothorns growing along the
54
55 specific direction of $\langle 01\bar{1} \rangle$ have single crystalline features and mesoporous surface.
56
57
58
59
60

Most importantly, such hybrid electrode can detect ultralow-concentration glucose (ultrahigh sensitivity: $97.9 \text{ mA mM}^{-1} \text{ cm}^{-2}$ and ultralow detection limit: 5 nM). These remarkable biosensing performance can be attributed to the synergistic effect of the dramatically enhanced surface area of the electrocatalytic material (Cu_2O) and the perfect architecture in which mesoporous Cu_2O nanothorn arrays *in-situ* grow on the Cu substrate surface.

Experimental Section

Fabrication of the Cu foam-supported Cu_2O electrode. The Cu foam-supported Cu_2O was prepared by first anodization using a two-electrode system (Cu foam as the anode and a graphite plate as the cathode) at room temperature, followed by cyclic voltammetry (CV) electro-oxidation in a three-electrode configuration (Pt foil as the counter electrode and Ag/AgCl electrode as the reference electrode) controlled by a potentiostat (CHI 660E, Shanghai, Chenhua). The electrolyte for anodization was a $0.4 \text{ M H}_2\text{C}_2\text{O}_4$ aqueous solution with a little amount of HF, and the electro-oxidation was performed in a 1 M KOH aqueous solution. Thus, the hybrid electrode (Cu_2O nanothorn arrays on Cu foam) was obtained. The detailed experimental procedure and the calculating method of the mass of the active material (here, Cu_2O nanothorns) growing on the substrate was demonstrated in our previous work.²⁵ And the mass loading of Cu_2O nanothorn arrays per area was 1.72 mg cm^{-2} .

Characterization. X-ray diffraction (XRD, Rigaku D/max-rB) with Cu $K\alpha$ radiation was used to analyze the phase constitution of the as-synthesized samples.

X-ray photoelectron spectroscopy (XPS, ESCALAB 250) was performed to obtain surface elemental information of the hybrid electrode. All reported binding energy values were calibrated to the C 1s peak at 284.8 eV. Scanning electron microscope (SEM, LEO 1530 VP) and transmission electron microscope (TEM, FEI Tecnai G2) with selected-area electron diffraction (SAED) were used to characterize the surface morphology and structure of the Cu foam-supported Cu₂O electrode. A V-Sorb 2800P surface area and pore size analyzer was used to obtain nitrogen adsorption/desorption isotherms at 77 K.

Electrochemical measurement. All of the CV and amperometric tests were conducted using a potentiostat (CHI 660E, Shanghai, Chenhua) in a three-electrode cell (Pt foil as the counter electrode and Ag/AgCl electrode as the reference electrode) at room temperature. The Cu foam-supported Cu₂O electrode was directly served as the working electrode for detection of glucose. The CVs were collected in a 0.1 M NaOH aqueous electrolyte without and with various concentrations of glucose. The amperometric responses of the Cu foam-supported Cu₂O electrode to glucose were measured at the applied potential of 0.55 V (vs. Ag/AgCl), and the glucose concentrations ranged from 0.1 μM to 1 mM. In addition, for the sake of showing its potential for practical applications, the Cu foam-supported Cu₂O electrode was utilized to detect blood glucose concentrations of human serum samples.

Results and discussion

As illustrated in **Figure 1**, we proposed such a kind of hybrid structure that

nanothorn-like Cu_2O *in situ* grows on the skeleton surface of the Cu foam with 3D continuous skeletons (**Figure 2a**). Firstly, the unique mesoporous nanothorn-like structure of Cu_2O provides a high specific surface area and high usage of active materials, and produces interconnected nanoporous channels that can effectively facilitate charge/ion transfer and mass transport for the electrocatalysis. Secondly, highly conductive Cu foam serves both as the current collector and the substrate to supporting the active materials, which can well promote the transfer of electrons. Simultaneously, the 3D continuous large pores could accelerate the glucose transport to the skeleton-supported catalysts. Furthermore, the *in situ* growth of Cu_2O nanothorns on the Cu foam facilitates the integration of electroactive materials and current collector without any additional contact resistance and additive/binders. Such a unique structure was predicted to promote the biosensing performance towards the glucose oxidation to a great extent.

Based upon the above concept, the Cu foam-supported Cu_2O nanothorn arrays electrode was successfully synthesized by the aforementioned method. The XRD pattern of the Cu foam-supported Cu_2O electrode is given in **Figure S1**, showing Bragg reflections of Cu and Cu_2O phases. The diffraction peaks at 2θ of 36.4° , 42.3° , 61.3° , 73.5° well agree with the (111), (200), (220) and (311) reflections of Cu_2O (JCPDS no. 05-0667) respectively. Moreover, three diffraction peaks located at 2θ of 43.3° , 50.4° , 74.1° were indexed to the face centered cubic (fcc) Cu (JCPDS no. 04-0836). The elemental information that the nanostructured Cu_2O grows on the Cu foam was also supported by the XPS results after surface etching by Ar^+ sputtering

(**Figure 3** and **Figure S2**). The Cu 2p_{3/2} spectrum (**Figure 3a**) reveals the presence of a peak located at 932.3 eV. However, this peak at 932.3 eV cannot demonstrate that the peak is ascribed to Cu⁺ because the Cu 2p_{3/2} binding energy peaks of metallic copper and Cu₂O are so similar that the two substances cannot be definitely discerned only by the peak position of Cu 2p_{3/2}. Nevertheless, weak satellite peaks between 941.0 and 948.0 eV can be clearly observed, which is the typical characteristic of Cu₂O.²⁶⁻²⁷ Besides, the Auger electron spectrum (Cu L₃M_{4,5}M_{4,5}) of the as-prepared electrode was also obtained under X-ray radiation (**Figure 3b**). The binding energy peak position of Cu L₃M_{4,5}M_{4,5} is 569.8 eV, which matches well with the electron state of Cu₂O. And the binding energy peak of CuO is invisible.²⁶ Therefore, the aforementioned XPS results can confirm the information of Cu₂O growing on the skeleton surface of Cu foam again.

Figure 2 presents low and high magnification SEM images of the as-obtained hybrid electrode. Obviously, Cu₂O with a particular nanothorn-like morphology *in situ* grows on the surface of skeletons of the Cu substrate, and its surface roughness is remarkably enhanced. With careful observation (**Figure 2c**) we can find that nanothorns with several micrometers in length interconnect with each other, giving rise to micron-sized channels among the nanothorns, which are expected to facilitate the fast diffusion of electrolyte onto the surface of nanothorns.


TEM was used to determine further details of the nanothorn-like structure (**Figure 4** and **Figure S3**). The nanothorns are confirmed to have widths of *ca.* 20-40 nm and lengths of several micrometers. They are self-assembled at an angle to the

skeleton surface of the Cu foam, forming nanothorn arrays interconnected with multiple junctions (**Figure 4a** and **Figure S3a**). Some nanothorns tend to form clusters with similar growth directions. The SAED pattern (inset in **Figure 4b**) shows that the nanothorns have single crystalline features. This spot-type pattern can be attributed to the [011]-zone-axis diffraction of the fcc Cu₂O. Moreover, the diffraction spots are indexed according to the (*h k l*) reflections of Cu₂O (JCPDS no. 05-0667), which are well consistent with the XRD results (**Figure S1**). Unexpectedly, the zoom-in TEM image (**Figure 4c**) obviously indicates porous characteristic of the nanothorns surface. The pores are *ca.* 2-6 nm in diameter, being expected to dramatically enhance the surface area of the nanothorns. Eventually, the N₂ adsorption/desorption results (**Figure S4**) verify the mesoporous structure of the as-obtained electrode, and the specific surface area determined by Brunauer-Emmett-Teller (BET) is 173.34 m² g⁻¹ (calculated according to the Cu₂O mass). Moreover, even if the whole mass of the Cu foam-supported Cu₂O nanothorn arrays electrode is taken into account, the BET value is still as large as 5.36 m² g⁻¹. The HRTEM images of the Cu₂O nanothorns (**Figure 4d** and **Figure S3b**) provide further insight into its crystalline structure. The spacings of some lattice fringes are about 2.28 Å and 2.51 Å, which are close to the *d* spacing of the (200) and (11 $\bar{1}$) planes of crystalline Cu₂O. The fast Fourier transformation (FFT) was also performed to further investigate the crystalline nature of the nanothorns (inset in **Figure 4d** and inset in **Figure S3b**). The corresponding spot verifies the single crystalline characteristic of the Cu₂O nanothorns. Combining the FFT pattern with the HRTEM

image (**Figure 4d**), we can conclude that the nanothorns grow along the specific direction of $\langle 01\bar{1} \rangle$, as indicated by the blue arrow. Based upon the aforementioned results, the Cu foam-supported Cu_2O nanothorn arrays were successfully achieved as we have assumed.

In this work, the Cu foam-supported Cu_2O nanothorn arrays electrode was explored as a nonenzymatic biosensor for glucose detection, and its electrocatalytic activity was assessed by CV measurement. **Figure 5a** presents the CV results of the Cu foam-supported Cu_2O electrode in a 0.1 M NaOH aqueous solution with diverse glucose concentrations (from 0 to 0.8 mM). Upon the stepwise glucose addition, significant enhancement of anodic currents can be seen, while the cathodic peak currents obviously decrease, suggesting the excellent catalytic properties of the Cu foam-supported Cu_2O electrode toward the glucose oxidation. Although the underlying mechanism is so far unknown, it has been recognized that it is Cu(III) species rather than Cu(I) or Cu(II) that serve as the mediator for electron transfer.^{28,29} The possible mechanism is proposed as follows for glucose detection. Firstly, Cu(I) is electrochemically oxidized to $\text{Cu}(\text{OH})_2$ and then transformed to CuO. Further, the produced CuO is oxidized to CuOOH. According to the following reactions, the CuO/CuOOH redox couple could catalyze the oxidation of glucose to form gluconolactone, giving rise to the enhancement of anodic currents and the decline of the cathodic currents.^{30,31}





Furthermore, the CVs of the Cu foam-supported Cu₂O electrode in the 0.1 M NaOH solution containing 0.5 mM glucose at various scan rates were recorded, as depicted in **Figure 5b**. It is noted that both the anodic and cathodic peak current densities are enhanced with increasing scan rate, while the cathodic peaks potentials shift negatively, suggesting a quasi-reversible electron transfer reaction for the above electrochemical reaction.³² Moreover, the peak current densities for both the oxidation and reduction are directly proportional to the square root of the scan rate, as depicted in **Figure 5c**. This demonstrates that the redox reaction on the Cu foam-supported Cu₂O electrode is a typical diffusion-controlled electrochemical process.³¹ And the diffusion coefficient (*D*) for the transfer of glucose during the electrocatalysis was calculated on the basis of the Randles-Sevcik equation:^{33, 34}

$$I_p = 2.69 \times 10^5 n^{3/2} A D^{1/2} C v^{1/2} \quad (5)$$

where *I_p* is the peak current density, *n* is the electron transfer number, *A* is the electrode surface geometrical area, *C* is the bulk concentration and *v* is the scan rate. From the slop of *I_p* vs. *v*^{1/2}, the diffusion coefficient of glucose was calculated to be 0.29 cm² s⁻¹.

To acquire the optimal amperometric parameter for detection of glucose, the potential dependence of the current response was studied with continuous addition of 0.1 mM glucose under stirred conditions (**Figure 5d** and **Figure S5**). A notably enhanced current response can be seen due to each addition of glucose when a

potential between 0.25 V and 0.6 V vs. Ag/AgCl was applied. Furthermore, the sensitivity of the Cu foam-supported Cu₂O electrode increases with the incremental applied potential. Yet, the background current and noise also increases accordingly with the increasing potential. After comparison, the optimal potential was discovered to be 0.55 V vs. Ag/AgCl, which was used in the following amperometric measurements. In addition, the current densities show good linear correlations with the glucose concentration at various applied potentials (0.25-0.6 V vs. Ag/AgCl), suggesting wide applications of the present hybrid electrode for glucose biosensing (**Figure S5**).

Figure S6a displays the chronoamperometry response of the Cu foam-supported Cu₂O nanothorn arrays electrode in the 0.1 M NaOH solution without and with various concentrations of glucose. It can be seen that the increasing concentration of glucose leads to the remarkable increasing of current. The relationship between current density and the minus square roots of time at the stable stage of electrocatalysis was shown in **Figure S6b**, and it shows a good linear relation for a certain time range. The *D* value of glucose can also be calculated according to the Cottrell equation:³⁴

$$j = nFD^{1/2}C\pi^{-1/2}t^{-1/2} \quad (6)$$

where *j* is the current density, *F* is the Faraday constant and *t* is the time. The *D* value was estimated to be 0.066 cm² s⁻¹ using the slope of the line in **Figure S6b**, which is much larger than the previously published results.¹⁶ Furthermore, the value of catalytic rate constant (*K*_{cat}) could also be determined from the following

equation.³⁴

$$\frac{j_{cat}}{j_d} = \pi^{1/2} (K_{cat} C t)^{1/2} \quad (7)$$

where j_{cat} is the catalytic current of glucose oxidation, j_d is the limiting current without glucose, C and t are the concentration of glucose and time elapsed respectively. For a certain time range (16 s - 64 s), the value of j_{cat}/j_d exhibits a linear dependence on $t^{1/2}$ (**Figure S6c**). Based upon the slope of j_{cat}/j_d vs. $t^{1/2}$ plot, K_{cat} was obtained as $2.1 \times 10^7 \text{ cm}^3 \text{ mol}^{-1} \text{ s}^{-1}$, indicating fast catalytic rate of the present hybrid electrode.

The Cu foam-supported Cu₂O nanothorn arrays electrode well responds to the continuous addition of glucose with concentrations of 0.1 μM to 200 μM at 0.55 V vs. Ag/AgCl, and the corresponding amperometric curve is presented in **Figure 6a**. Towards lower glucose concentrations, the sensitive current response curve is shown in the inset of **Figure 6a**. Owing to the integration of the highly enhanced surface area of the nanoporous Cu₂O nanothorn arrays and the excellent conductivity of the binder-free electroactive material/substrate (current collector) nanostructure, the hybrid electrode gives the steep and stable amperometric response with significantly improved current density after each addition of glucose, even when the glucose concentration was diluted to 0.1 μM. The Cu foam-supported Cu₂O electrode can sensitively and rapidly respond to the glucose detection, and the involved current can be well enhanced owing to the concentration increase of glucose, which is further verified by the corresponding calibration curve (**Figure 6b**). As displayed in **Figure 6c** and **Figure S7**, the Cu foam-supported Cu₂O electrode displays multi-linear

detection ranges, strongly depending on the concentration of glucose added. As the glucose is diluted to 0.1 μM , it is astonishing that the Cu foam-supported Cu_2O nanothorn arrays electrode provides a superb sensitivity of $97.9 \text{ mA mM}^{-1} \text{ cm}^{-2}$ towards the glucose detection. **Figure 6d** shows the amperometric response in the 0.1 M NaOH solution without and with 5 nM glucose. Despite the relatively large noise, the linear fitting results clearly reveal that the two curves show different variation tendency, which can further demonstrate that the as-prepared electrodes are able to detect the remarkably low concentration of 5 nM glucose. Such ultrahigh sensitivity and ultralow detection limit are superior to all of the other electrochemical glucose biosensors, which are summarized in **Table 1**.^{1,3,11,14,24,35-37} **Figure S8** presents the current-time curve of the Cu foam-supported Cu_2O electrode towards 10 nM glucose, displaying an obvious step-like increase of current due to the glucose addition. **Figure 6e** displays the typical amperometric detection of the Cu foam-supported Cu_2O electrode at 0.55 V vs. Ag/AgCl owing to the stepwise addition of glucose from 0.1 μM to 1 mM. It is believed that the electrochemical oxidation of glucose is a surface catalytic reaction, and normally obeys Langmuir isothermal kinetics.^{9, 31, 38} Thus the calibration curve of the Cu foam-supported Cu_2O electrode could be fitted by the Langmuir fitting equation. As illustrated in **Figure 6f**, the calibration curve can be well fitted by the Langmuir equation ($R^2=0.998$). The Langmuir fitting equation for the Cu foam-supported Cu_2O electrode is presented as $I \text{ (mA cm}^{-2}\text{)}=81.02 \times C_{\text{glucose}} \text{ (mM)}/(1.46 + C_{\text{glucose}} \text{ (mM)})$, which can meet the glucose detection for human serum in a wide concentration range (1 μM -11.4 mM).

Selectivity is also a vital parameter to evaluate the biosensing performance of the electrode for glucose apart from sensitivity.³⁹ Herein, we also investigate the effects of some species which can interfere with the glucose detection of human beings, such as urea, ascorbic acid (AA), fructose, NaCl, lactose, uric acid (UA), acetamidophenol and dopamine on the glucose current response. Given that the glucose concentration in the human blood is much higher than that of some co-existing interfering species, the anti-interference performance of the Cu foam-supported Cu₂O electrode was tested by the continuous addition of 1 mM glucose, followed by 0.02 mM of the other interferents in the 0.1 M NaOH solution. As presented in **Figure 7a** and **Figure S9**, remarkable current enhancement can be seen due to the glucose addition, while negligible current responses for the interferents. The results indicate the excellent selectivity of the Cu foam-supported Cu₂O electrode for nonenzymatic detection of glucose. All above results suggest that the Cu foam-supported Cu₂O hybrid electrode possesses excellent electrocatalytic performance for glucose oxidation and therefore is promising for constructing a highly sensitive/selective glucose biosensor.

The stability is another important issue for biosensing. The stability of the Cu foam-supported Cu₂O nanothorn arrays electrode was also investigated using the current-time measurement towards 0.1 mM glucose at 0.55 V vs. Ag/AgCl for a long period of time. We can see that the current density remains 98% of its original value over a running time of 2500 s (**Figure 7b**). Moreover, the long-term stability of the Cu foam-supported Cu₂O electrode was explored by recording the current-time response towards 1 mM glucose over 15 days. Our hybrid electrode was subjected to

the exposure of air and tested every day. As displayed in **Figure 7c**, the amperometric response is approximately 98.7% of the original value after 15 days, suggesting the excellent stability of our hybrid electrode.

These predominant properties endow this *in situ* grown hybrid electrode to exhibit high reliability for analyzing human blood serums. To confirm this conclusion, our hybrid electrode was further used to detect the glucose level in human serum samples (inset of **Figure 7d**) that were obtained from Shandong University Qilu Hospital. 100 μ L of human serum was injected into 20 mL of 0.1 M NaOH solution and the measurement was conducted at 0.55 V vs. Ag/AgCl with stirring. The obtained data are comparable to those measured using a biochemical analyzer in hospital, which have been summarized in **Figure 7d** and **Table S1**. It is clear that the values tested by the hybrid electrode are satisfactory and well consistent with the data from the biochemical analyzer, indicating its reliability for glucose determination. Therefore, the Cu foam-supported Cu₂O nanothorn arrays electrode is an outstanding candidate for the new generation electrochemical glucose sensing, especially for the extremely low concentration of glucose samples, which is promising for the glucose analysis of unconventional body fluids or diluted blood samples. Moreover, Cu foam is cheap and commercially available, and the two-step electrochemical strategy reported here is very facile. The hybrid electrode can even be produced in large scale (**Figure S10**), which signifies its potential for commercialization.

Conclusion

In summary, a unique binder-free electrode with the nanoarchitecture of 3D Cu foam/mesoporous Cu₂O nanothorn arrays was synthesized through a facile two-step anodization/electro-oxidation procedure. Serving as an enzyme-free electrochemical electrode, it exhibits ultrahigh sensitivity, ultralow detection limit, excellent selectivity and stability. The overall results illustrate that the Cu foam-supported Cu₂O nanothorn arrays electrode presents brilliant prospect for glucose detection, especially for the analysis of extremely low concentration of glucose. The impressive glucose sensing behavior of the Cu foam-supported Cu₂O nanothorns can be attributed to the mesoporous array nanostructure as well as the excellent contact between the electro-catalytic active materials (Cu₂O) and the current collector/substrate (Cu foam), which simultaneously enhances the electrocatalytic activity of the electrode and minimizes the resistances in biosensing.

Supporting Information

XRD pattern, XPS survey scan spectrum, TEM image, HRTEM image, N₂ adsorption-desorption isotherm and BJH adsorption pore size distribution, amperometric response, photographs of the Cu foam-supported Cu₂O nanothorn arrays electrode. The Supporting Information is available free of charge on the ACS Publications website.

Acknowledgements

We acknowledge the financial support from National Natural Science Foundation of China (51371106), National Basic Program of China (973, 2012CB932800), Specialized Research Fund for the Doctoral Program of Higher Education of China (20120131110017) and Young Tip-top Talent Support Project (the Organization Department of the Central Committee of the CPC). Z.H. Zhang also acknowledges the financial support from the Alexander von Humboldt Foundation (Germany).

Figures

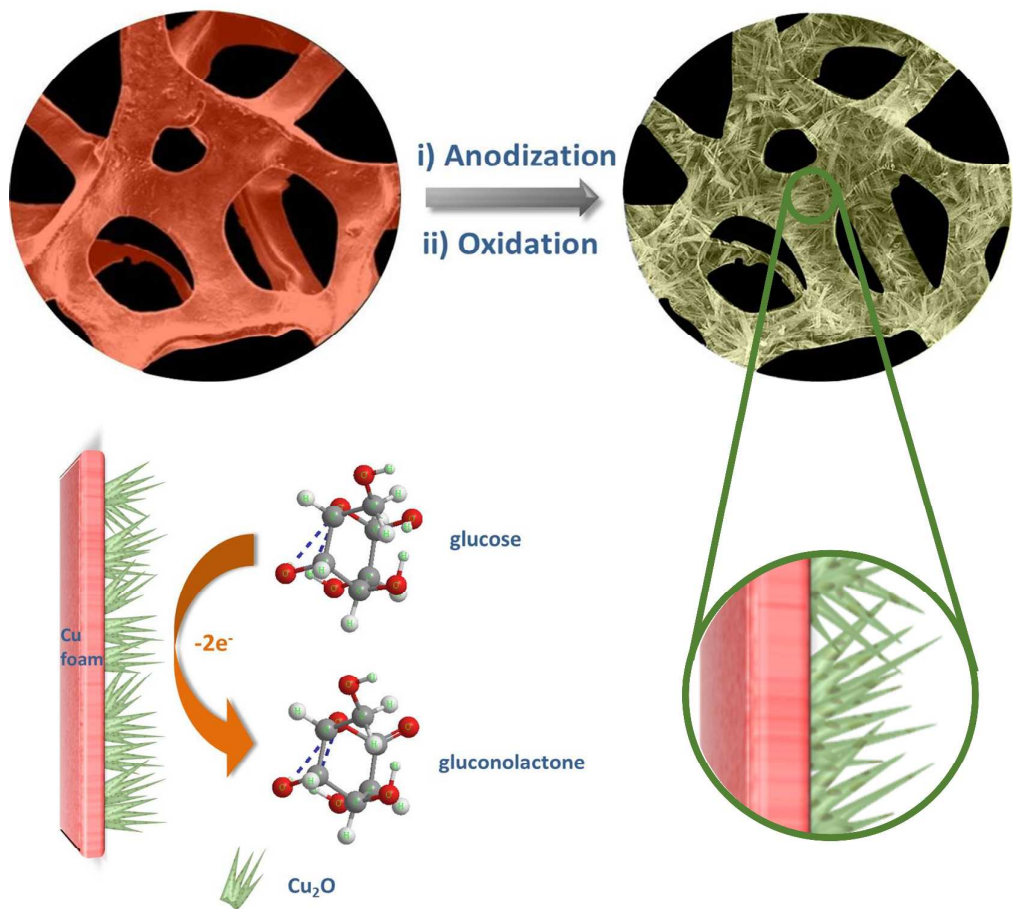


Figure 1. Schematic illustration showing the fabrication of the 3D Cu foam-supported mesoporous Cu₂O nanothorn arrays electrode and its function for the electrocatalytic oxidation of glucose.

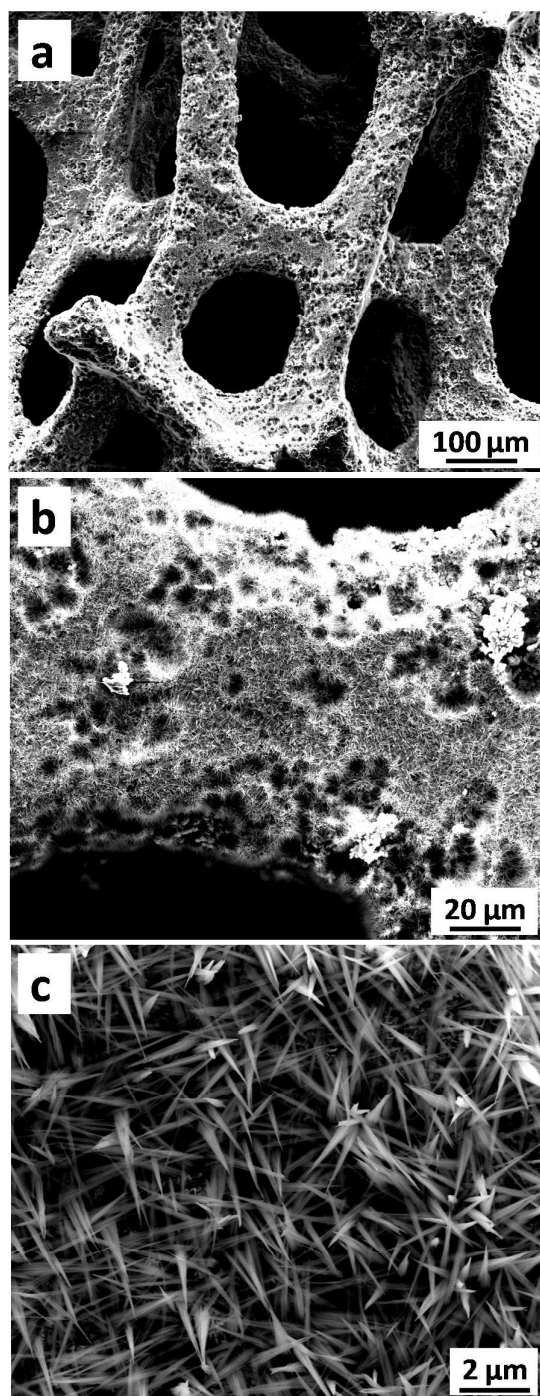


Figure 2. Typical low- (a,b) and high-magnification (c) SEM images of the Cu foam-supported Cu_2O nanothorn arrays electrode.

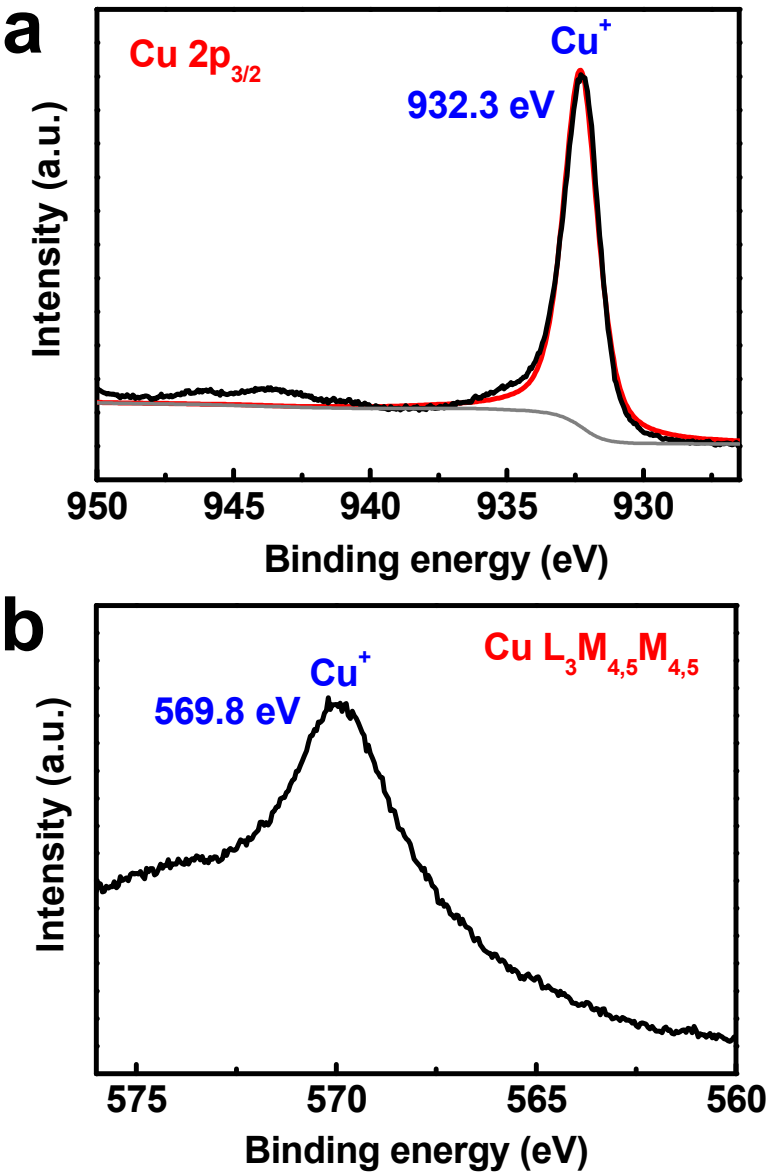


Figure 3. (a) XPS spectrum (Cu 2p_{3/2} core peak) and (b) Auger spectrum (Cu L₃M_{4,5}M_{4,5} peak) of the Cu foam-supported Cu₂O nanothorn arrays electrode.

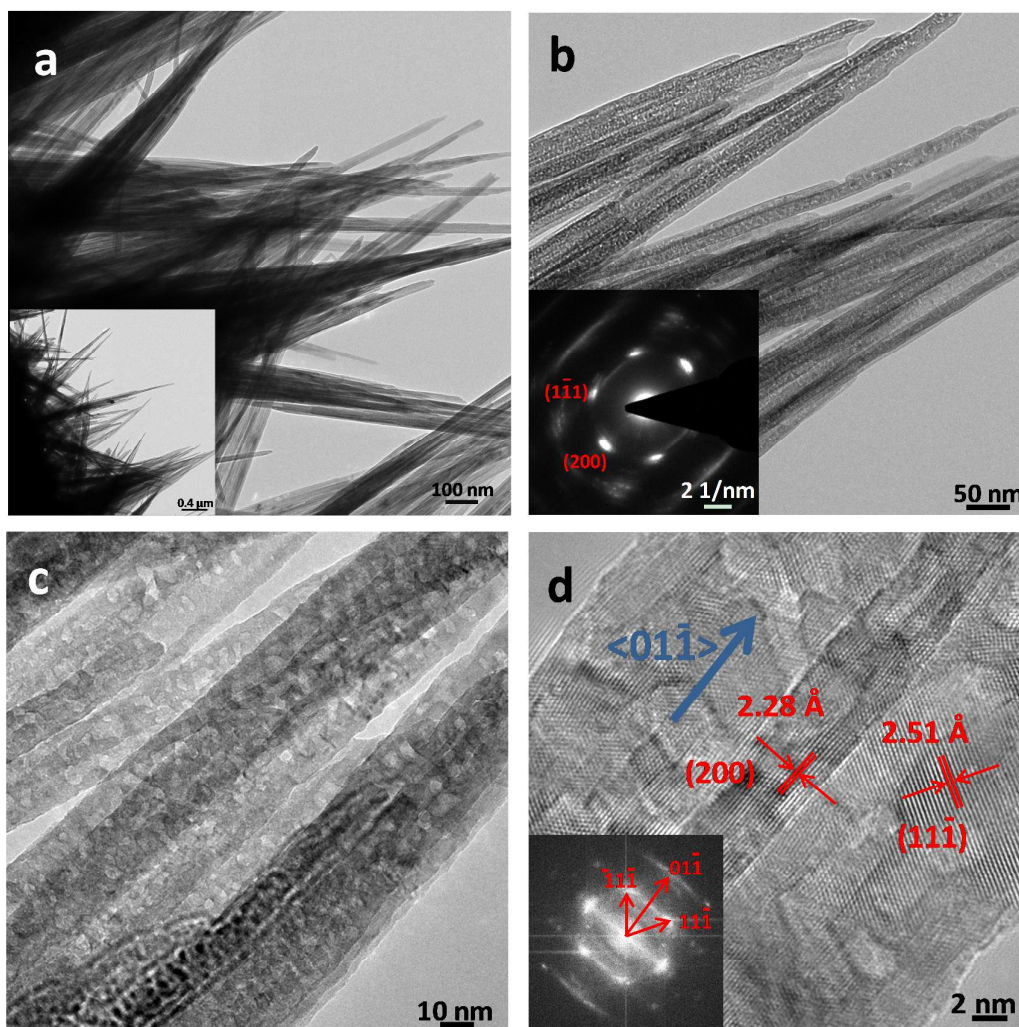


Figure 4. (a-c) TEM images of the Cu_2O nanothorn arrays grown on the skeleton of Cu foam. The inset in (a): corresponding low-magnification TEM image. The inset in (b): a $[011]$ zone axis SAED pattern obtained from Cu_2O nanothorns. (d) HRTEM image of a Cu_2O nanothorn. The inset in (d): FFT pattern corresponding to the HRTEM image.

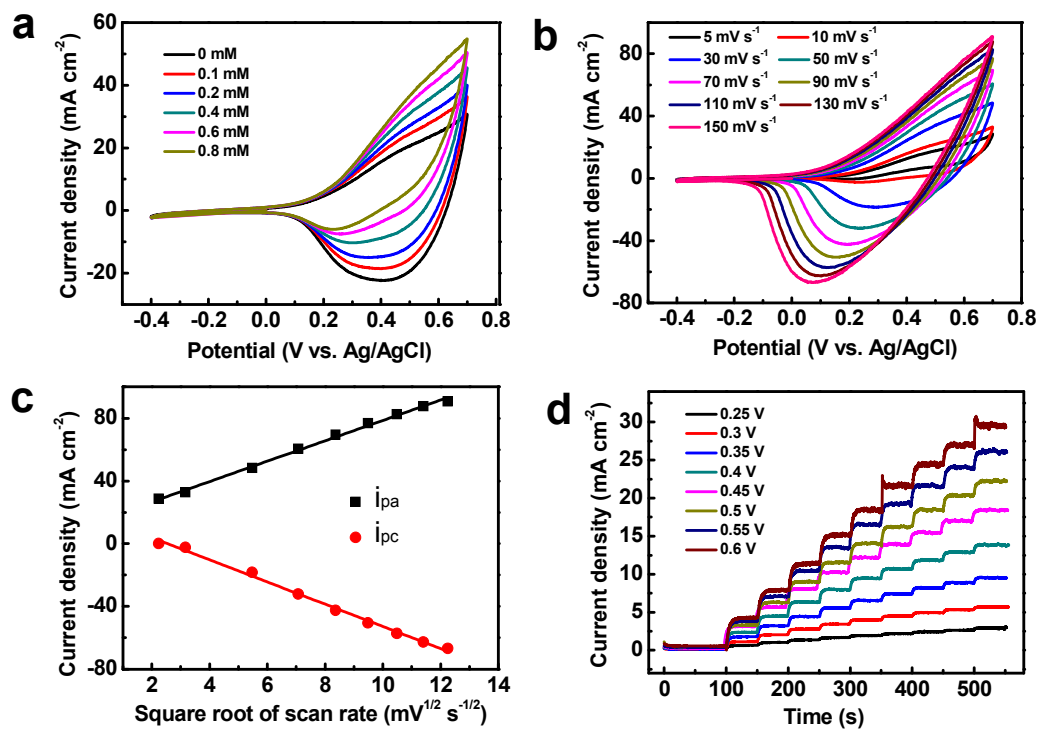


Figure 5. (a) CV curves of the Cu foam-supported Cu₂O nanothorn arrays electrode in the 0.1 M NaOH solution containing different concentrations of glucose (from 0 to 0.8 mM) at the scan rate of 20 mV s⁻¹. (b) CVs of the Cu foam-supported Cu₂O electrode in the 0.1 M NaOH solution containing 0.5 mM glucose at various scan rates. (c) Plots of peak currents as a function of the square root of the scan rate. (d) Amperometric response of the Cu foam-supported Cu₂O electrode at various potentials (vs. Ag/AgCl) in the 0.1 M NaOH solution with successive addition of 0.1 mM glucose.

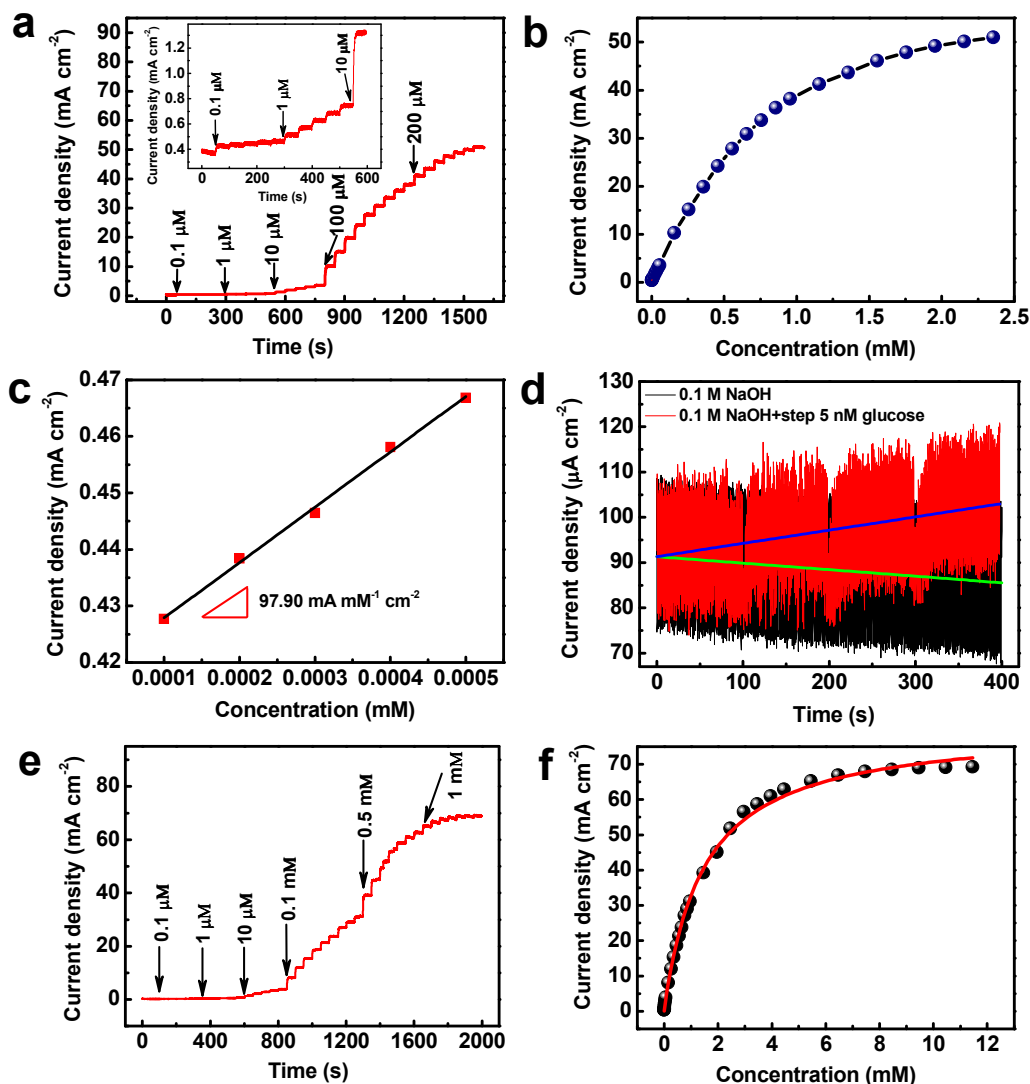


Figure 6. (a) Typical amperometric response and (b) the corresponding calibration curve of the Cu foam-supported Cu_2O nanothorn arrays electrode at 0.55 V vs. Ag/AgCl with the successive addition of glucose from 0.1 μM to 200 μM in the 0.1 M NaOH solution. Inset in (a): amperometric response towards 0.1 μM ~ 10 μM glucose. (c) Glucose sensitivity of the Cu foam-supported Cu_2O electrode for successive addition of 0.1 μM glucose. (d) Amperometric response to the 0.1 M NaOH solution without and with the extremely low limit concentration of 5 nM glucose. (e) Amperometric response and (f) the corresponding calibration curve of the Cu

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

foam-supported Cu₂O electrode at 0.55 V vs. Ag/AgCl with the successive addition of
glucose from 0.1 μM to 1 mM in the 0.1 M NaOH solution.

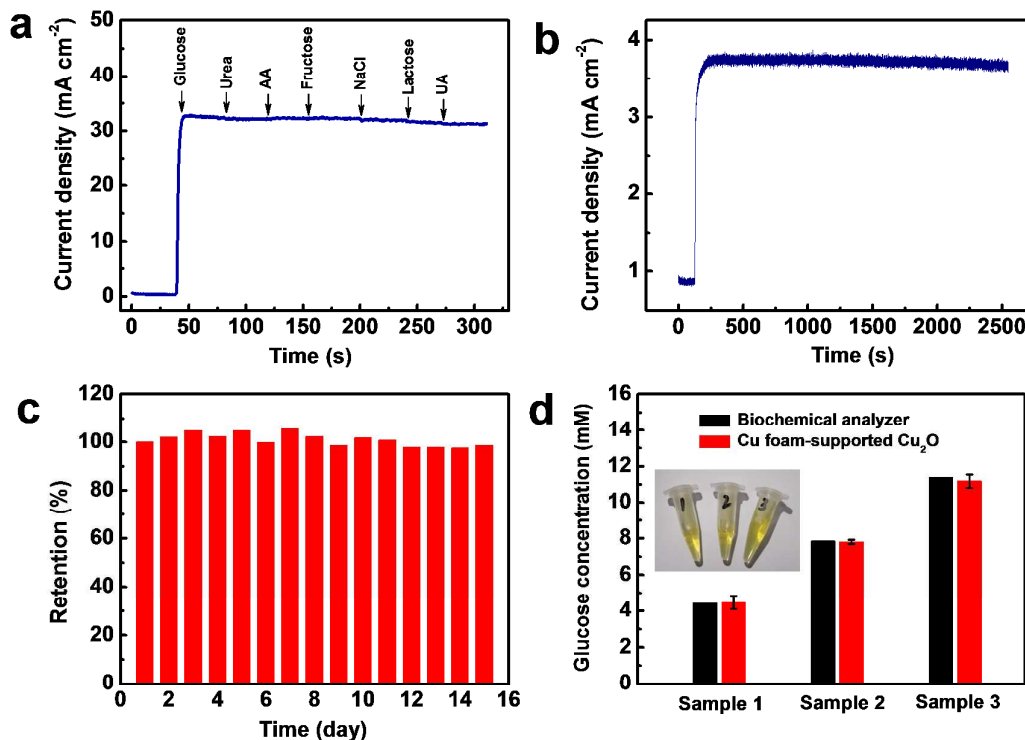


Figure 7. (a) Amperometric response of the Cu foam-supported Cu₂O nanothorn arrays electrode towards the addition of 1 mM glucose and various 0.02 mM interfering species in the 0.1 M NaOH solution at 0.55 V vs. Ag/AgCl. (b) Amperometric response of the Cu foam-supported Cu₂O electrode to 0.1 mM glucose in the 0.1 M NaOH solution at 0.55 V vs. Ag/AgCl for a long period of running time (2500 s). (c) Long-term stability of the Cu foam-supported Cu₂O electrode over 15 days. (d) The detection of glucose concentration in human serum samples by a biochemical analyzer and the Cu foam-supported Cu₂O electrode. Inset: photograph of the serum samples. Here, the blood glucose data of the serum samples by the biochemical analyzer were provided by the biochemical lab of Shandong University Qilu Hospital, Jinan, P. R. China.

Electrode material	Potential (V vs. Ag/AgCl)	Sensitivity (mA mM ⁻¹ cm ⁻²)	Detection limit (μM)	Reference
Hollow CuO polyhedron	0.55	1.112	0.33	24
CuO/SG	0.5	1.298	0.08	3
Cu foam	0.5	3.397	12.96	35
CuO nanoellipsoids	0.55	2.555	0.072	14
S/NPG/Co ₃ O ₄	0.26	12.5	0.005	11
CuO NT arrays	0.32	1.89	0.1	36
3D porous nickel	0.5	2.9	0.07	37
Ni(OH) ₂ /3D graphene	0.55	2.65	0.34	1
Cu foam-supported Cu₂O nanothorn arrays	0.55	97.9	0.005	Present work

Table 1 Comparison of the performance of the Cu foam-supported Cu₂O electrode with previously reported non-enzymatic glucose sensors with excellent property.

Notes and references

- (1) Zhan, B.; Liu, C.; Chen, H.; Shi, H.; Wang, L.; Chen, P.; Huang, W.; Dong, X. Free-Standing Electrochemical Electrode Based on Ni(OH)₂/3D Graphene Foam for Nonenzymatic Glucose Detection. *Nanoscale* **2014**, *6*, 7424-7429.
- (2) Jiang, D.; Liu, Q.; Wang, K.; Qian, J.; Dong, X.; Yang, Z.; Du, X.; Qiu, B. Enhanced Non-Enzymatic Glucose Sensing Based on Copper Nanoparticles Decorated Nitrogen-Doped Graphene. *Biosens. Bioelectron.* **2014**, *54*, 273-278.
- (3) Tian, Y.; Liu, Y.; Wang, W.-p.; Zhang, X.; Peng, W. CuO Nanoparticles on Sulfur-Doped Graphene for Nonenzymatic Glucose Sensing. *Electrochim. Acta* **2015**, *156*, 244-251.
- (4) Wang, J. Electrochemical Glucose Biosensors. *Chem. Rev.* **2008**, *108*, 814-825.
- (5) Yuan, J.; Wang, K.; Xia, X. Highly Ordered Platinum-Nanotubule Arrays for Amperometric Glucose Sensing. *Adv. Funct. Mater.* **2005**, *15*, 803-809.
- (6) Solanki, P. R.; Kaushik, A.; Agrawal, V. V.; Malhotra, B. D. Nanostructured Metal Oxide-Based Biosensors. *NPG Asia Mater.* **2011**, *3*, 17-24.
- (7) Ronkainen, N. J.; Halsall, H. B.; Heineman, W. R. Electrochemical Biosensors. *Chem. Soc. Rev.* **2010**, *39*, 1747-1763.
- (8) Wang, G.; Lu, X.; Zhai, T.; Ling, Y.; Wang, H.; Tong, Y.; Li, Y. Free-Standing Nickel Oxide Nanoflake Arrays: Synthesis and Application for Highly Sensitive Non-Enzymatic Glucose Sensors. *Nanoscale* **2012**, *4*, 3123-3127.
- (9) Zhang, Y.; Liu, Y.; Su, L.; Zhang, Z.; Huo, D.; Hou, C.; Lei, Y. CuO Nanowires Based Sensitive and Selective Non-Enzymatic Glucose Detection. *Sens. Actuators B: Chem.* **2014**, *191*, 86-93.
- (10) Guo, C.; Huo, H.; Han, X.; Xu, C.; Li, H. Ni/CdS Bifunctional Ti@TiO₂ Core-Shell Nanowire

- Electrode for High-Performance Nonenzymatic Glucose Sensing. *Anal. Chem.* **2014**, *86*, 876-883.
- (11) Lang, X.-Y.; Fu, H.-Y.; Hou, C.; Han, G.-F.; Yang, P.; Liu, Y.-B.; Jiang, Q. Nanoporous Gold Supported Cobalt Oxide Microelectrodes as High-Performance Electrochemical Biosensors. *Nat. Commun.* **2013**, *4*, 2169-2176.
- (12) Yang, W.; Ratinac, K. R.; Ringer, S. P.; Thordarson, P.; Gooding, J. J.; Braet, F. Carbon Nanomaterials in Biosensors: Should You Use Nanotubes or Graphene? *Angew. Chem. Int. Ed.* **2010**, *49*, 2114-2138.
- (13) Si, P.; Ding, S.; Yuan, J.; Lou, X. W.; Kim, D.-H. Hierarchically Structured One-Dimensional TiO₂ for Protein Immobilization, Direct Electrochemistry, and Mediator-Free Glucose Sensing. *ACS Nano* **2011**, *5*, 7617-7626.
- (14) Zhang, X.; Sun, S.; Lv, J.; Tang, L.; Kong, C.; Song, X.; Yang, Z. Nanoparticle-Aggregated CuO Nanoellipsoids for High-Performance Non-Enzymatic Glucose Detection. *J. Mater. Chem. A* **2014**, *2*, 10073-10080.
- (15) Hsu, C.-W.; Wang, G.-J. Highly Sensitive Glucose Biosensor Based on Au-Ni Coaxial Nanorod Array Having High Aspect Ratio. *Biosens. Bioelectron.* **2014**, *56*, 204-209.
- (16) Wang, L.; Zheng, Y.; Lu, X.; Li, Z.; Sun, L.; Song, Y. Sens. Dendritic Copper-Cobalt Nanostructures/Reduced Graphene Oxide-Chitosan Modified Glassy Carbon Electrode for Glucose Sensing. *Sens. Actuators B: Chem.* **2014**, *195*, 1-7.
- (17) Lu, X.; Ye, Y.; Xie, Y.; Song, Y.; Chen, S.; Li, P.; Chen, L.; Wang, L. Copper Coralloid Granule/Polyaniline/Reduced Graphene Oxide Nanocomposites for Nonenzymatic Glucose Detection. *Anal. Methods* **2014**, *6*, 4643-4651.
- (18) Dong, X.-C.; Xu, H.; Wang, X.-W.; Huang, Y.-X.; Chan-Park, M. B.; Zhang, H.; Wang, L.-H.;

- Huang, W.; Chen, P. 3D Graphene-Cobalt Oxide Electrode for High-Performance Supercapacitor and Enzymeless Glucose Detection. *ACS Nano* **2012**, *6*, 3206-3213.
- (19) Xiao, X.; Wang, M.; Li, H.; Pan, Y.; Si, P. Non-Enzymatic Glucose Sensors Based on Controllable Nanoporous Gold/Copper Oxide Nanohybrids. *Talanta* **2014**, *125*, 366-371.
- (20) Ding, Y.; Liu, Y.; Parisi, J.; Zhang, L.; Lei, Y. A Novel NiO-Au Hybrid Nanobelts Based Sensors for Sensitive and Selective Glucose Detection. *Biosens. Bioelectron.* **2011**, *28*, 393-398.
- (21) Li, Y.; Wei, Y.; Shi, G.; Xian, Y.; Jin, L. Facile Synthesis of Leaf-Like CuO Nanoparticles and Their Application on Glucose Biosensor. *Electroanalysis* **2011**, *23*, 497-502.
- (22) Dong, J.; Ren, L.; Zhang, Y.; Cui, X.; Hu, P.; Xu, J. Direct Electrodeposition of Cable-Like CuO@Cu Nanowires Array for Non-Enzymatic Sensing. *Talanta* **2015**, *132*, 719-726.
- (23) Long, M.; Tan, L.; Liu, H.; He, Z.; Tang, A. Novel Helical TiO₂ Nanotube Arrays Modified by Cu₂O for Enzyme-Free Glucose Oxidation. *Biosens. Bioelectron.* **2014**, *59*, 243-250.
- (24) Kong, C.; Tang, L.; Zhang, X.; Sun, S.; Yang, S.; Song, X.; Yang, Z. Templating Synthesis of Hollow CuO Polyhedron and Its Application for Nonenzymatic Glucose Detection. *J. Mater. Chem. A* **2014**, *2*, 7306-7312.
- (25) Dong, C.; Bai, Q.; Cheng, G.; Zhao, B.; Wang, H.; Gao, Y.; Zhang, Z. Flexible and ultralong-life cuprous oxide microsphere-nanosheets with superior pseudocapacitive properties. *RSC Adv.* **2015**, *5*, 6207-6214.
- (26) Martin, L.; Martinez, H.; Poinot, D.; Pecquenard, B.; Cras, F. L. Comprehensive X-ray photoelectron spectroscopy study of the conversion reaction mechanism of CuO in lithiated thin film electrodes. *J. Phys. Chem. C* **2013**, *117*, 4421-4430.
- (27) Svintsitskiy, D. A.; Stadnichenko, A. I.; Demidov, D. V.; Koscheev, S. V.; Boronin, A. I.

- Investigation of oxygen states and reactivities on a nanostructured cupric oxide surface. *Appl. Surf. Sci.* **2011**, 257, 8542-8549.
- (28) Wu, H.-X.; Cao, W.-M.; Li, Y.; Liu, G.; Wen, Y.; Yang, H.-F.; Yang, S.-P. In situ growth of copper nanoparticles on multiwalled carbon nanotubes and their application as non-enzymatic glucose sensor materials. *Electrochim. Acta* **2010**, 55, 3734-3740.
- (29) Kang, X.; Mai, Z.; Zou, X.; Cai, P.; Mo, J. A sensitive nonenzymatic glucose sensor in alkaline media with a copper nanocluster/multiwall carbon nanotube-modified glassy carbon electrode. *Anal. Biochem.* **2007**, 363, 143-150.
- (30) Khan, R.; Ahmad, R.; Rai, P.; Jang, L.-W.; Yun, J.-H.; Yu, Y.-T.; Hahn, Y.-B.; Lee, I.-H. Glucose-Assisted Synthesis of Cu₂O Shuriken-Like Nanostructures and Their Application as Nonenzymatic Glucose Biosensors. *Sens. Actuators B: Chem.* **2014**, 203, 471-476.
- (31) Felix, S.; Kollu, P.; Raghupathy, B.; Jeong, S. K.; Grace, A. N. Electrocatalytic Activity of Cu₂O Nanocubes Based Electrode for Glucose Oxidation. *J. Chem. Sci.* **2014**, 126, 25-32.
- (32) Ci, S.; Huang, T.; Wen, Z.; Cui, S.; Mao, S.; Steeber, D. A.; Chen, J. Nickel Oxide Hollow Microsphere for Non-Enzyme Glucose Detection. *Biosens. Bioelectron.* **2014**, 54, 251-257.
- (33) Xiao, X.; Ulstrup, J.; Li, H.; Zhang, J.; Si, P. Nanoporous Gold Assembly of Glucose Oxidase for Electrochemical Biosensing. *Electrochim. Acta* **2014**, 130, 559-567.
- (34) Bard, A. J.; Faulkner, L. R. Electrochemical Methodes: Fundamental and Applications. *John Wilney and Sons: New York* **2001**; Chapter 6.
- (35) Jin, J.; Zheng, G.; Ge, Y.; Deng, S.; Liu W.; Hui, G. A Non-Enzyme Electrochemical Qualitative and Quantitative Analyzing Method for Glucose, D-Fructose, and Sucrose Utilizing Cu Foam Material. *Electrochim. Acta* 2015, **153**, 594-601.

- (36) Xu, L.; Yang, Q.; Liu, X.; Liu, J., X. Sun, One-Dimensional Copper Oxide Nanotube Arrays: Biosensors for Glucose Detection. *RSC Adv.* 2014, **4**, 1449-1455.
- (37) Niu, X.; Lan, M.; Zhao, H.; Chen, C. Highly Sensitive and Selective Nonenzymatic Detection of Glucose Using Three-Dimensional Porous Nickel Nanostructures. *Anal. Chem.* 2013, **85**, 3561-3569.
- (38) Ding, Y.; Wang, Y.; Su, L.; Bellagamba, M.; Zhang, H.; Lei, Y. Electrospun Co_3O_4 Nanofibers for Sensitive and Selective Glucose Detection. *Biosens. Bioelectron.* **2010**, *26*, 542-548.
- (39) Chen, L. Y.; Fujita, T.; Ding, Y.; Chen, M. W. A Three-Dimensional Gold-Decorated Nanoporous Copper Core-Shell Composite for Electrocatalysis and Nonenzymatic Biosensing. *Adv. Funct. Mater.* **2010**, *20*, 2279-2285.

Table of Contents Graphic

