

Functional Nanostructured Materials (including low-D carbon)

Printed Graphene Electrochemical Biosensors Fabricated by Inkjet Maskless Lithography for Rapid and Sensitive Detection of OrganophosphatesJohn A. Hondred, Joyce Breger, Nathan Alves, Scott A. Trammell,
Scott A. Walper, Igor L. Medintz, and Jonathan C. ClaussenACS Appl. Mater. Interfaces, **Just Accepted Manuscript** • DOI: 10.1021/acsami.7b19763 • Publication Date (Web): 05 Mar 2018Downloaded from <http://pubs.acs.org> on March 6, 2018**Just Accepted**

"Just Accepted" manuscripts have been peer-reviewed and accepted for publication. They are posted online prior to technical editing, formatting for publication and author proofing. The American Chemical Society provides "Just Accepted" as a service to the research community to expedite the dissemination of scientific material as soon as possible after acceptance. "Just Accepted" manuscripts appear in full in PDF format accompanied by an HTML abstract. "Just Accepted" manuscripts have been fully peer reviewed, but should not be considered the official version of record. They are citable by the Digital Object Identifier (DOI®). "Just Accepted" is an optional service offered to authors. Therefore, the "Just Accepted" Web site may not include all articles that will be published in the journal. After a manuscript is technically edited and formatted, it will be removed from the "Just Accepted" Web site and published as an ASAP article. Note that technical editing may introduce minor changes to the manuscript text and/or graphics which could affect content, and all legal disclaimers and ethical guidelines that apply to the journal pertain. ACS cannot be held responsible for errors or consequences arising from the use of information contained in these "Just Accepted" manuscripts.



ACS Publications

is published by the American Chemical Society, 1155 Sixteenth Street N.W.,
Washington, DC 20036Published by American Chemical Society. Copyright © American Chemical Society.
However, no copyright claim is made to original U.S. Government works, or works
produced by employees of any Commonwealth realm Crown government in the course
of their duties.

Printed Graphene Electrochemical Biosensors Fabricated by Inkjet Maskless Lithography for Rapid and Sensitive Detection of Organophosphates

John A. Hondred^a, Joyce C. Breger^b, Nathan J. Alves^b, Scott A. Trammell^b, Scott A. Walper^b, Igor L. Medintz^b, Jonathan C. Claussen^{*a}

* To whom correspondence should be addressed. Tel: 515-294-4690; E-mail: jcclauss@iastate.edu

^a Department of Mechanical Engineering, Iowa State University, Ames, IA, 50011

^b Center for Bio/Molecular Science and Engineering, Code 6900, U. S. Naval Research Laboratory, Washington, DC 20375, USA

ABSTRACT:

Solution phase printing of graphene-based electrodes has recently become an attractive low-cost, scalable manufacturing technique to create in-field electrochemical biosensors. Here we report a graphene-based electrode developed *via* Inkjet Maskless Lithography (IML) for the direct and rapid monitoring of triple-O linked phosphonate organophosphates (OPs); these constitute the active compounds found in chemical warfare agents and pesticides that exhibit acute toxicity as well as long-term pollution to soils and waterways. The IML printed graphene electrode is nano/microstructured with a 1000 mW benchtop laser engraver and electrochemically deposited platinum nanoparticles (dia. ~25 nm) to improve its electrical conductivity (sheet resistance decreased from ~10 000 Ω /sq. to 100 Ω /sq.), surface area, and electroactive nature for subsequent enzyme functionalization and biosensing. The enzyme phosphotriesterase (PTE), also known as organophosphate hydrolase (OPH), was conjugated to the electrode surface *via* glutaraldehyde cross-linking. The resulting biosensor was able to rapidly measure (5 sec response time) the insecticide paraoxon (a model organophosphate) with a low detection limit (3 nM), and high sensitivity (370 nA/ μ M) with negligible interference from similar nerve agents. Moreover, the biosensor exhibited high reusability (average of 0.3%

decrease in sensitivity per sensing event), stability (90% anodic current signal retention over 1000 seconds), longevity (70% retained sensitivity after 8 weeks), and the ability to selectively sense OP in actual soil and water samples. Hence, this work presents a scalable printed graphene manufacturing technique that can be used to create OP biosensors that are suitable for in-field applications as well as, more generally, for low-cost biosensor test strips that could be incorporated into wearable or disposable sensing paradigms.

Keywords: Electrochemical Biosensor, Graphene, Inkjet Printing, Pesticide, Phosphotriesterase, Paraoxon

1. INTRODUCTION

Organophosphates (OPs) are widely used as insecticides to increase quality and yield of crops.¹⁻² While OPs are effective neurotoxins against several types of pests, they are also toxic to humans and the environment. High-level, acute exposure to OPs can lead to immediate detrimental health effects including miosis, rhinorrhea, apnea, convulsions and death.³ Subsequently, OP neurotoxins have even been weaponized into G-type chemical warfare agents such as Sarin and Soman,⁴⁻⁵ which were used in the 1994 Japan attack poisoning 600 residents⁶ and the 1999 Tokyo subway attack injuring 640 victims.⁷ In addition to such high-level acute exposure to OPs, chronic low-level exposure to OP-based pesticides is also a concern especially for farmworkers.⁸ For example, farmworkers in both developed and developing countries who work on fields sprayed with OPs expressed lower neurobehavioral performance than control farmworker groups.⁹⁻¹⁰ Despite their short half-lives (days to months), OP residues have been found in soils, sediments, and watersheds—raising health concerns for chronic and early-life exposure to non-occupational populations especially those living in agricultural communities.¹¹⁻

¹² Hence rapid and accurate detection of even low-level concentrations of OPs in the

environment are critical for effective remediation measures.¹³ While there are numerous techniques capable of detecting trace levels of OPs (*e.g.*, gas/liquid chromatography, immunoassays, and mass spectroscopy) these tests are time-consuming and must be performed in a laboratory by trained technicians.¹⁴⁻¹⁵ Currently, a rapid, inexpensive method of monitoring pesticide levels in water or soil slurries in the field does not exist.¹⁶

Electrochemical, enzymatic biosensors presents a promising solution to in-field OP monitoring.¹⁷ Enzymatic biosensors exhibit favorable characteristics for point-of-service sensing (*e.g.*, high selectivity, sensitivity, and reusability) for a wide variety of applications including medical screening,¹⁸ defense threat monitoring,¹⁹ and environmental testing.²⁰ OP enzymatic biosensors have primarily focused on using cholinesterase enzymes (*i.e.*, acetylcholinesterase or butyrylcholinesterase) that are inhibited in the presence of OP.²¹⁻²² While such inhibition-based enzyme biosensors have displayed high sensitivity and ultra-low OP detection limits, they also are prone to false-positive signals as cholinesterase enzymes can be inhibited by heavy metals or detergents that are found in soil and water samples.²³ Comparatively, the enzyme phosphotriesterase (PTE (EC 3.1.8.1)) selectively binds to OPs *via* a three O-linked binding pocket that is selective to specific ester bonds found in many OPs such as paraoxon.²⁴ PTE catalyzes paraoxon into equimoles of *p*-nitrophenol, an electroactive molecule, that can be readily monitored through direct oxidation at an applied potential of +0.95 V *vs.* a Ag/AgCl reference electrode.¹⁷ Electrochemical detection of paraoxon with carbon-based materials (*e.g.*, glassy carbon, graphite and carbon nanotubes) have been used for the direct amperometric detection of *p*-nitrophenol, due in part to their high biocompatibility with immobilized enzymes and high electrical conductivity.²⁵⁻³⁰ However, due to low sensitivity (limit of detection ~10 nM, Table 1) and the high cost associated with graphene and carbon nanotubes synthesized *via*

chemical vapor deposition, the potential of PTE biosensors for direct, in-field sensing has been limited especially as the maximum allowable OP concentration levels in drinking water begins to approach the subnanomolar range (European Union Drinking Water Directive 98/83/EC).³¹

This manuscript addresses three key issues that often hinder enzymatic OP biosensors, *i.e.*, scalable/economical manufacturing processes, surface-fouling, and low sensitivity/high detection limits. Herein, we report the first printed graphene biosensor for amperometric detection of the insecticide paraoxon, a model OP. Graphene electrodes were printed and patterned through a recently developed thin film manufacturing technique called Inkjet Maskless Lithography (IML).³² Next, the printed graphene electrodes (PGEs) were laser annealed and electrochemically deposited with platinum nanoparticles (PtNPs) to create a nano/microstructured surface that is highly conductive/electroactive with high surface area for increased enzyme loading and heterogeneous charge transport during electrochemical sensing. The graphene-based electrode was consequently biofunctionalized with the enzyme PTE through covalent crosslinking with glutaraldehyde. This biofunctionalized PtNP-IML-PGE demonstrated the lowest recorded detection limit (3 nM) and highest sensitivity (370 nA/ μ M) for any reported amperometric PTE biosensor to date. Moreover, the biosensor exhibited high reusability (average of 0.3% decrease in sensitivity per time sensed), stability (90% anodic current over 1000 seconds), longevity (70% retained sensitivity after 8 weeks), and selectivity (negligible interference to 6 similar nerve agents, ability to detect OP in water and soil samples). The performance and potential scalable manufacturing protocols of the PtNP-IML-PGE suggests they are well-suited for in-field pesticide detection or potential bioterror agent monitoring in actual biological matrices.

2. METHODS AND MATERIALS

2.1. Chemicals and Reagents

Completely chemically reduced single layer graphene was purchased from ACS materials (GN1P005). All pesticides (including paraoxon) were obtained from Chem Service (N-12816). All other chemicals and solvents were purchased from Sigma-Aldrich and were used without any other purification unless otherwise stated. Water was filtered through a B-Pure Water Purification system (resistivity, 18.2 M Ω /cm²). Screen-printed carbon electrodes (SPCE) were purchased from CH Instruments (SE 101). River water was obtained from the Des Moines River in in the state of Iowa.

2.2. Preparation and Purification of PTE

The gene encoding phosphotriesterase (EC 3.1.8.1), also known as organophosphate hydrolase (OPH), from *Brevundimonas diminuta* was synthesized by Genscript with flanking restriction enzyme sites that facilitated transfer to the bacterial expression vector pET28. Protein expression was performed in *Escherichia coli* strain BL21(DE3) (New England Biolabs, Ipswich, MA) as previously described.³³ Briefly, cultures were grown in 500 mL shake flasks containing kanamycin (25 μ g/mL) until mid-log stage. Expression of recombinant PTE was induced with 1 mM β -D-Isothiogalactopyranoside (IPTG) and continued overnight at 30 °C. Cell pellets were collected by centrifugation then lysed through a combination of EDTA treatment, lysozyme, and sonication. Insoluble material was pelleted *via* centrifugation and soluble proteins batched to immobilized metal affinity chromatography (IMAC) resin. Following an incubation to allow protein binding and batch washing to remove non-specifically bound proteins, PTE was eluted with 200 mM imidazole. The recombinant PTE was further purified by FPLC which also removed the imidazole. Protein concentration was determined using a Nanosight 1000 to

measure the absorbance at 280 nm. Calculations were based on the theoretical extinction coefficient and the molecular weight of the protein.

2.3. Biosensor Fabrication

2.3.1 Printing Graphene *via* Inkjet Maskless Lithography (IML)

Similar to our work published earlier, graphene electrodes were manufactured through Inkjet Maskless Lithography (IML).³² In summary, 150 mg of ethyl cellulose (viscosity 46 cP, 5% in toluene/ethanol 80:20), was completely dissolved in 50 mL of acetone and 10 mL of terpineol. Ethyl cellulose was used as a surfactant to increase the surface tension of the ink and subsequently promote graphene flake suspension in the ink and improve adhesion of graphene to the substrate upon printing. Pristine graphene flakes (150 mg) were added to the solution and were probe sonicated for 4 hours. Probe sonication was conducted at 70% amplitude with a 9 second pulse and 1 second rest cycle to reduce graphene size and increase graphene flake exfoliation. The ink was then filtered through a 0.8 μm syringe filter. Acetone was evaporated from the solution to yield a concentrated graphene ink (15 mg/mL) which was spin coated over an inkjet printed polymer sacrificial layer (10% formaldehyde resin, 80% cyclohexanone, 10% terpineol) on heat treated Polyethylene Terephthalate (PET (kemafoil, Coveme TSL W)). The substrate was then post-baked under a heat gun (Steinel #HB1750K) for 15 minutes at 1200 °F with a distance of 18 inches from the surface. The post-bake process significantly improved adhesion of graphene to the substrate without destroying the sacrificial polymer layer. The entire substrate was then impinged with an acetone wash-bottle to remove the sacrificial layer leaving highly defined electrodes (Supporting Information Movie S1).

2.3.2 Laser annealing

The IML graphene electrodes were laser annealed by a 1000 mW diode laser engraver (HTPOW). The wavelength of the laser was blue-violet (405 nm) which did not damage the heat-treated PET substrate. The carving time (i.e., burn time, is the amount of time the laser is positioned at one particular point on the substrate before moving onto a different substrate point) of the engraver was set at 20 ms. This carving time that was found to not degrade/destroy the integrity of the graphene electrode while maximizing its electrical conductivity and electroactive nature (Supporting Information Figure S1 & S5).

2.3.3 Electrodeposited Platinum Nanoparticles

Platinum nanoparticles (PtNPs) were electrodeposited onto the surface of the electrode using a standard three electrical setup. A platinum wire (CH Instruments CHI115) was used as the counter electrode and a Ag/AgCl single membrane electrode was used as the reference electrode (CH Instruments CHI11). A platinum electroplating solution of chloroplatinic acid and sodium sulfate was made by mixing 4 mM of H_2PtCl_6 and 0.5 M Na_2SO_4 . The electrode was then placed into the solution and PtNP were electrochemically deposited onto the surface by pulsed chronopotentiometry (istep) using pulses or cycles of 0.1 sec steps of 0 to 250 μA . This procedure provided high current density across the graphene surface which enhanced the nucleation of PtNP (25 ± 2.5 nm, $n = 25$) evenly across the graphene surface (Supporting Information Figure S2). Diameter of nanoparticles was determined using SEM micrographs (Supporting Information Figure S2) and ImageJ pixel measurement tool with a sample size of $n = 25$ PtNPs.

3.3.4 Phosphotriesterase Ink Preparation and Deposition

A PTE ink was developed by mixing 50 μL of PTE (15 μM with a molecular weight of ~ 35 kDa), 400 μL of DI water and 50 μL of 50 mg/mL Bovine Serum Albumin (BSA). The PTE

ink was thoroughly mixed using a desktop vortex (Fisher Vortex Mixer #02215365) on high for 15 seconds. BSA was added as it has shown to increase the stability of other enzymes and to a lesser extent to increase biosensor sensitivity.³⁴ Glutaraldehyde (50 μ L of 0.25%) was added to the solution to crosslink the enzyme to the surface of the electrode. The PTE ink was then drop coated onto the working electrode by hand-pipetting 10 μ L directly onto the working electrode. The biosensors were then refrigerated (~ 4 $^{\circ}$ C) for at least 12 hours during enzyme incubation and were subsequently stored in this environment until biosensor testing.

2.3.5 Electro-analytical Measurements

All electrochemical measurements were conducted using a CH Instruments potentiostat (600E series) with a typical three electrode setup which included an Ag/AgCl reference and platinum wire counter. All tests were conducted in 15 mL of PBS Buffer (1x, Sigma Aldrich), modified to pH 8.0 with NaOH—a pH more favorable to PTE performance (Supporting Information Figure S3).³⁵ Cyclic voltammetry was performed with a 50 mV/s scan rate; slow scan rates were chosen in order to minimize surface charging effects due to the double layer capacitance emanating from the high surface area of the laser annealed graphene. To increase diffusion of substrate to the enzyme, a magnetic stir bar was added and rotated at 300 rpm for amperometric measurements. Paraoxon stock solution (1 mM) was made daily as it readily photo-hydrolyzes³⁶ and was pipetted at various volumes for desired molarity for all amperometric measurements unless otherwise noted. For selectivity tests, diluted pesticide stock solutions of 0.1 mM were used as many of the tested interference pesticides have low solubility in water. Paraoxon calibration plots for the biofunctionalized PtNP-IML-PGE were conducted with a working potential of +0.95 V (vs. Ag/AgCl) as the biosensor detection limit was minimized at this working potential (Supporting Information Figure S4). To remove the

electromagnetic noise that was applied by the magnetic stirrer, data was filtered by taking the running average of 100 points with a scan rate of 0.01 sec^{-1} (running average over 1 sec). Amperometric biosensor response time was calculated by monitoring the time from the release of target analyte from the pipette tip in the test vial to the time a new steady state current response (90% max anodic current) was recorded. The biosensor detection limits was calculated using 3σ protocols; the detection limit was calculated by evaluating paroxon concentration three standard deviations from the mean of the baseline signal acquired in PBS without added nerve agent (3s).

2.3.6 SEM Images

Scanning electron microscopy (SEM) images were acquired using a FEI Quanta 250 FE-SEM. All images were magnified to 15 000x using backscattering electrons, spot size of 4.0, and with a 10 kV potential. Iridium was evenly coated using turbo-pump sputter coater to deposit a 2 nm conductive coating over all samples to improve surface imaging by preventing electrons from tunneling through the graphene surface.

3. RESULTS AND DISCUSSION

3.1. Overview of the Biosensor Fabrication

Paraoxon biosensors were fabricated by a simple four step process that utilizes printed graphene electrodes in lieu of graphene synthesized by chemical vapor deposition—a process requiring a high temperature (up to 1000°C) vacuum synthesis environment that is costly and not well-suited for scalable manufacturing (Figure 1 & Methods & Materials).³⁷ The printed graphene electrodes used herein were first fabricated through our previously reported IML technique³² that includes inkjet printing a polymer mask, spin coating a graphene flake solution, thermal post-baking the printed graphene, and finally performing an acetone rinse lift-off to form

well defined electrode patterns with a 5 mm diameter disk shaped working electrode (Figure 1a). After the graphene patterning process a laser diode engraver was used to anneal the graphene and remove non-conductive ink surfactants (Figure 1b). This laser annealing process significantly improves the electrical conductivity of the printed graphene electrodes (sheet resistance decreases from $\sim 10\,000\ \Omega/\text{sq.}$ to $100\ \Omega/\text{s}$) and adhesion of the graphene to the underlying PET surface while simultaneously nano/microstructuring the graphene surface which increases the electrode surface area and electroactivity (Figure 1b). Next, PtNP (diam. $\sim 25\ \text{nm}$) were decorated onto the laser annealed graphene through pulsed electrodeposition to further improve the electro reactivity of the biosensor (Figure 1c). Finally, PTE ink was drop coated onto the graphene platinum hybrid surface and consequently covalently bound to the surface *via* glutaraldehyde crosslinking (Figure 1d).

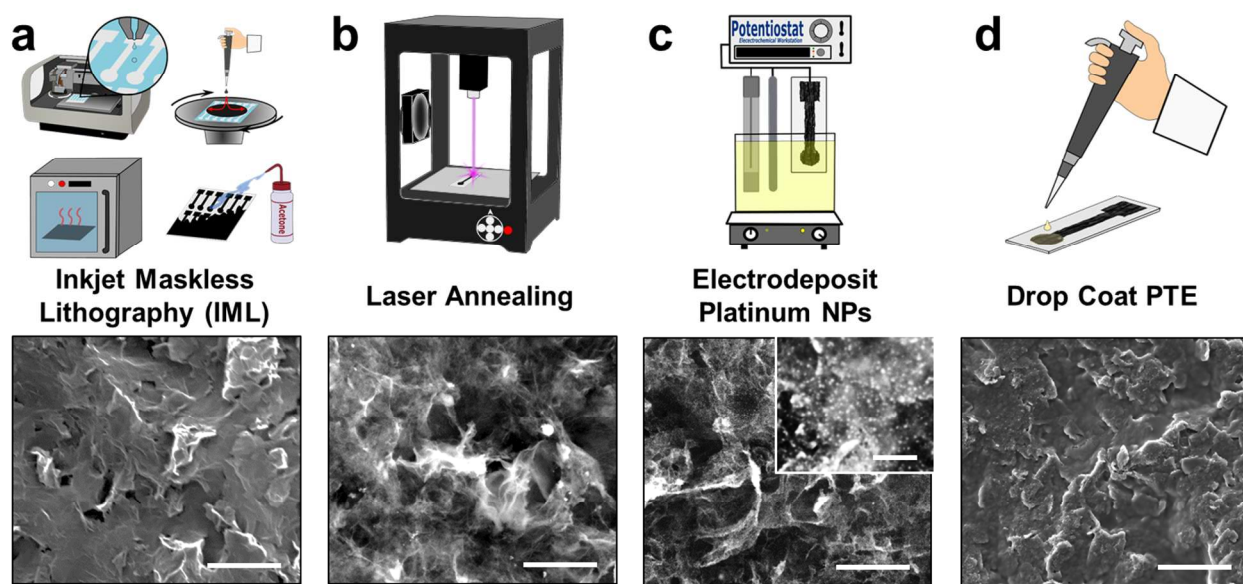


Figure 1. Schematic diagram and corresponding SEM images depicting the fabrication process steps of PtNP-IML-PGE biosensor. **(a)** Graphene patterning *via* the IML technique, **(b)** laser annealing of IML graphene electrodes, **(c)** electrodeposition of PtNPs, and **(d)** drop coating enzyme (PTE) ink. **Bottom:** Surface SEM (15 000x) corresponding to each manufacturing step, scale bar signifies 2 μm , inset (250 nm).

3.1.1 Laser Annealing Process

The electrical conductivity of the Inkjet Maskless Lithography printed graphene electrode (IML-PGE) was significantly increased by a laser annealing technique (see Methods & Materials).²⁴ The laser carving time (inversely proportional to raster rate) was incrementally increased from 5 ms to 20 ms which subsequently decreased the graphene sheet resistance two orders of magnitude from $\sim 10\,000\ \Omega/\text{sq.}$ to $100\ \Omega/\text{s}$ (Supporting Information Figure S5) while increasing the porosity and micro/nanostructuring of the graphene surface (Figure 2a & Supporting Information Figure S1) resulting in a high electroactive surface (from no electroactive surface area to $53\ \text{mm}^2$ for non-annealed IML-PGE to 20 ms laser annealed IML-PGE, respectively, See Supporting Information Figure S6). The electroactive surface area of the laser annealed IML-PGE was calculated using the Randles-Sevcik equation (Eq. 1).³⁸⁻³⁹

$$i_p = 2.69 * 10^5 AD^{\frac{1}{2}} n^{\frac{3}{2}} \nu^{\frac{1}{2}} C \quad (1)$$

where n is the number of electrons in the faradaic reaction ($n = 1$), A is the effective electroactive surface area (cm^2), D is the diffusion coefficient ($7.6 \times 10^{-6}\ \text{cm}^2/\text{s}$), C is the concentration of the bulk redox species (5 mM), ν is the scan rate (V/s), and i_p is the current (A) at the oxidation peak acquired from the CVs in Figure S6. Such increases in electrical conductivity and electroactive surface area significantly improve the oxidation rate of *p*-nitrophenol at the electrode surface as the sensitivity increases from 25 to 230 nA/ μM (Figure 2b). However, further increases in laser carving time (i.e., 50 and 100 ms) begins to smooth the IML-PGE surface (electroactive surface area decreases from $53\ \text{mm}^2$ at 20 ms to $10\ \text{mm}^2$ at 100 ms, see Supporting Information Figure S1 & Figure S6) by enhancing inter flake bonding *via* reforming of van der Waal bonds.⁴⁰⁻⁴¹ Subsequently this graphene smoothing process significantly decreases the sensitivity of the electrode, three orders of magnitude from 230 nA/ μM to 3 nA/ μM , respectively. Hence the IML-

1
2
3 PGEs used for all future experiments in this work are laser annealed with a carving time of 20
4
5 ms.
6
7

8 The laser annealing process most likely increased the electrical conductivity of the IML
9
10 printed graphene due its ability to thermally degrade/destroy non-conductive surfactants and
11
12 binders still present in the patterned graphene as well as to weld or sinter together individual
13
14 printed graphene flakes^{32, 40} Note this laser does not degrade the PET underlayer and can be
15
16 tuned to not harm even paper-based substrates.⁴⁰ Additionally, this laser annealing process,
17
18 performed in ambient air, increases the number of superficial defects while adding oxygenated
19
20 species (COOH, -C=O, and -OH) to said defect as previously reported.⁴² The increase of
21
22 graphene superficial defects has been shown to significantly increase the nucleation density of
23
24 PtNP during electrodeposition.⁴³ Such superficial oxygen species are well-suited for subsequent
25
26 enzymatic biofunctionalization *via* glutaraldehyde crosslinking as hydroxyl groups on the
27
28 graphene surface bind to the aldehyde groups in glutaraldehyde.⁴⁴ Moreover, this
29
30 micro/nanostructuring also changed the surface wettability of the graphene from one that is
31
32 hydrophilic (water contact angle (CA) < 10°) to one that is hydrophobic (CA ~90°) (insets Figure
33
34 2a).⁴¹ Such a hydrophobic electrode surface has been shown to repel the electrolyte sensing
35
36 solution that consequently reduces the double layer capacitance and decreases the sensor
37
38 background current; hydrophobic electrodes generally increase the signal-to-noise ratio of the
39
40 output signal.⁴⁵ Moreover, hydrophobic electrodes are generally less susceptible to surface-
41
42 fouling as they tend to reduce the adsorption of non-specific species that may be endogenously
43
44 found in biological matrices.⁴⁶⁻⁴⁸
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

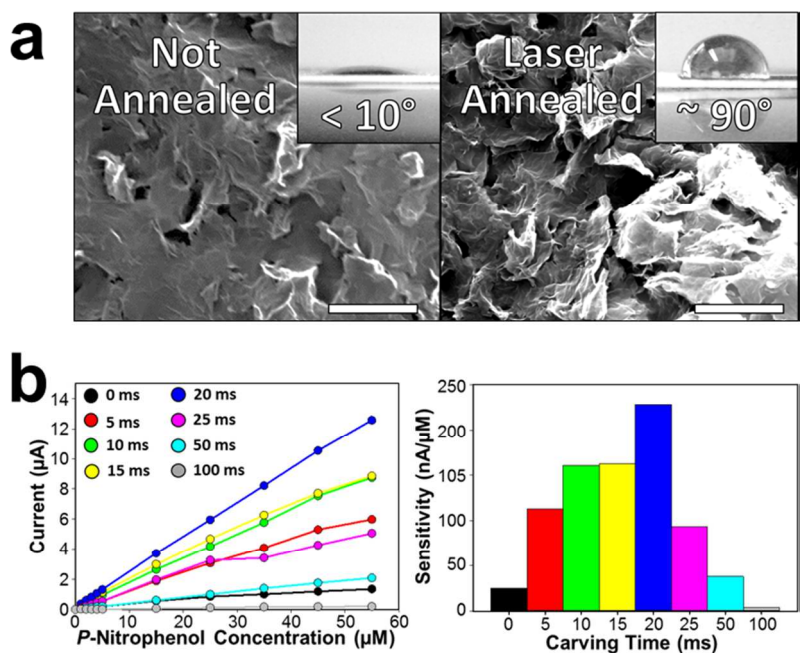


Figure 2. SEM images portraying IML printed graphene (a) without and with laser annealing (20 ms carving time). Insets display corresponding water contact angle measurements. (b) Amperometric calibration plot of *p*-nitrophenol for the IML-PGE that has been laser annealed with distinct carving time (0-100 ms) (Left). Histogram of *p*-nitrophenol sensitivity vs. laser carving time (Right).

3.1.2 Platinum Nanoparticle Decoration

PtNP (~ 25 nm in diameter) were electrodeposited onto the IML-PGE to further increase their electrocatalytic nature to *p*-nitrophenol oxidation (see Methods & Materials, Figure 3a).⁴⁹ Initially the incorporation of PtNPs on the surface of the graphene improved the biosensor sensitivity as the number of deposition pulses or cycles (0 to 75 cycles corresponding to 195 and 275 $\text{nA}/\mu\text{M}$, respectively, Figure 3b). However, after 75 electrodeposition cycles, larger ridge-like macrostructures formed (Supporting Information Figure S2) which significantly decreases the sensitivity (1000 cycles corresponding to 32 $\text{nA}/\mu\text{M}$, Figure 3b). This decrease in sensitivity is most likely due to the lower surface area and less catalytic capability of larger PtNP macrostructures as opposed to smaller PtNPs as previously illustrated with glucose biosensors

fabricated with platinum nano/microparticles electrodeposited on CVD synthesized multi-layer graphene.⁴³

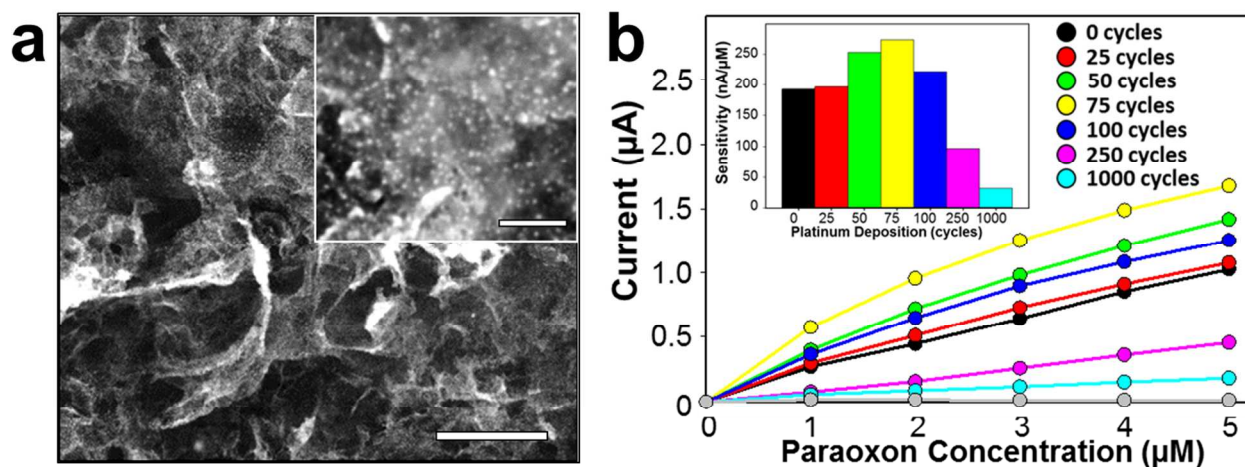


Figure 3. Platinum deposition. (a) SEM micrographs displaying the decorating of PtNPs (diam. ~25 nm) on IML-PGE surface. Scalebar is 5 μm and the inset scalebar is 200 nm. (b) Paraoxon calibration plot for IML-PGEs with increasing electrodeposition cycles. Inset: Histogram depicting the sensitivity of the PtNP-IML-PGE to paraoxon.

Cyclic voltammetry (CV) was conducted in order to measure and compare the electrochemical sensitivity to *p*-nitrophenol with a screen-printed carbon electrode (SPCE) to that of an IML printed graphene electrode (IML-PGE) that has been laser annealed as well as decorated with platinum nanoparticles (PtNP-IML-PGE) (Figure 4a & Supporting Information S6). All electrodes displayed distinct anodic peaks at an applied potential of +0.95 V vs. Ag/AgCl which corresponds to the oxidation of *p*-nitrophenol (1 mM). The IML-PGE and PtNP-IML-PGE both display a substantial increase in sensitivity to *p*-nitrophenol over the SPCE as faradaic oxidation peaks (at +0.95 V) were exhibited as follows: SPCE ~3 μA, IML-PGE ~10 μA, and PtNP-IML-PGE ~13 μA (Figure 4a). After the first scan cycle, the anodic current of the SPCE significantly decreased (>90%) due to surface-fouling (Figure 4a & Supporting Information Figure S7). As *p*-nitrophenol oxidizes the phenol leaving group polymerizes on the surface of the electrode creating an insulating/diffusion barrier. Comparatively, both the IML-

PGE and the PtNP-IML-PGE greatly resisted surface-fouling and decrease faradic current by less than 5%. We speculate that this resistance to surface-fouling is most likely due to the hydrophobic nature of the IML-PGEs as previously mentioned; similarly, other carbon nanomaterials have reported varying degrees of anti-fouling properties.⁵⁰⁻⁵²

The surface area of a SPCE and laser annealed IML-PGE and PtNP-IML-PGE were evaluated by performing CVs in ferri/ferrocyanide (Figure 4b & Supporting Information Figure S6). The anodic and cathodic currents both increase in magnitude with faster scan rates and were plotted versus the square root of the scan rate. The linearity demonstrates the process is diffusion controlled; however, the faradaic peaks shift further apart—a characteristic that is commonly attributed to porous materials that experience slower target analyte diffusion rates.⁵³ The Randles-Sevcik equation (Eq. 1 & Supporting Information Figure S6) the electrochemically active surface area was estimated as 5, 53, and 56 mm² for SPCE, laser annealed IML-PGE, and laser annealed PtNP-IML-PGE, respectively.

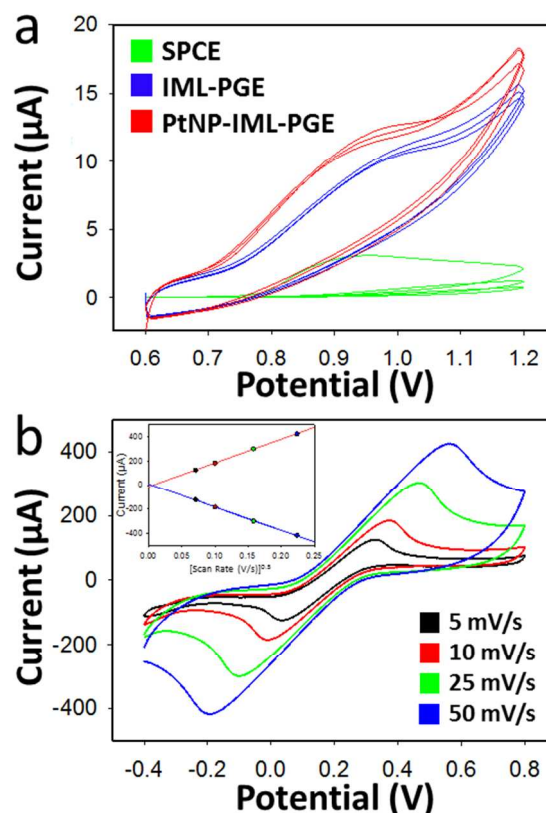


Figure 4. Transduction layer characterization (a) Cyclic voltammetry showing 3 repetitive scans in 1 mM *p*-nitrophenol with SPCE (Green), laser annealed IML-PGE (Blue), and laser annealed PtNP-IML-PGE (Red). (b) Cyclic voltammetry of laser annealed PtNP-IML-PGE in 5 mM ferro/ferricyanide with various scan rates (5-50 mV/s). Inset: Randles-Sevcik plot: anodic and cathodic currents vs. square root of scan rate.

3.1.3 Enzyme Characterization and Functionalization

The enzyme PTE was converted into an ink and assayed to monitor and improve its performance. First, it should be noted that as paraoxon diffuse to the electrode surface, PTE catalyzes paraoxon into *p*-nitrophenol which is consequently oxidized at the PtNP-IML-PGE surface during electrochemical biosensing (Figure 5a). However, before electrochemical biosensing, absorption spectroscopy was used to verify the activity of the PTE that was expressed in *Escherichia coli* strain BL21(DE3) (See Methods & Materials). The enzymatic activity of the resultant PTE ink was fluorescently monitored in a plate reader assay. PTE

degrades paraoxon by hydrolyzing the P-O bond yielding diethyl phosphate and *p*-nitrophenol which has a strong absorption at 405 nm with an extinction coefficient of $\sim 18\,000\text{ M}^{-1}\text{cm}^{-1}$, opposed to paraoxon which has minimal absorption (Figure 5a).⁵⁴ Similar to methods described,⁵⁵ three varying ratios of PTE ink (0.5, 1, and 5% which accounts for 2, 4, and 20 nM PTE) were assayed versus varying concentrations of paraoxon (1, 2, 4, 8 μM). A standard enzymatic rate reaction model was constructed using Sigma Plot's enzyme module (Figure 5b). As expected the higher concentration of PTE yielded higher V_{max} as more substrate can hydrolyze more paraoxon, ~ 350 , ~ 650 , $\sim 2300\text{ nM/sec}$ (0.5, 1, and 5%, respectively). All three ink concentrations yielded similar data for k_{cat} (Turnover number), K_M (Michaelis constant), and k_{cat}/K_M (enzymatic efficiency) of $\sim 160\text{ sec}^{-1}$, $\sim 0.270\text{ }\mu\text{M}$, $\sim 590\text{ }\mu\text{M}^{-1}\text{sec}^{-1}$, respectively. These enzyme performance characteristics were a slight improvement compared to our previous reports for PTE synthesized in a similar fashion, and hence validated that the recombinant protein was properly expressed and incubated.^{33, 56}

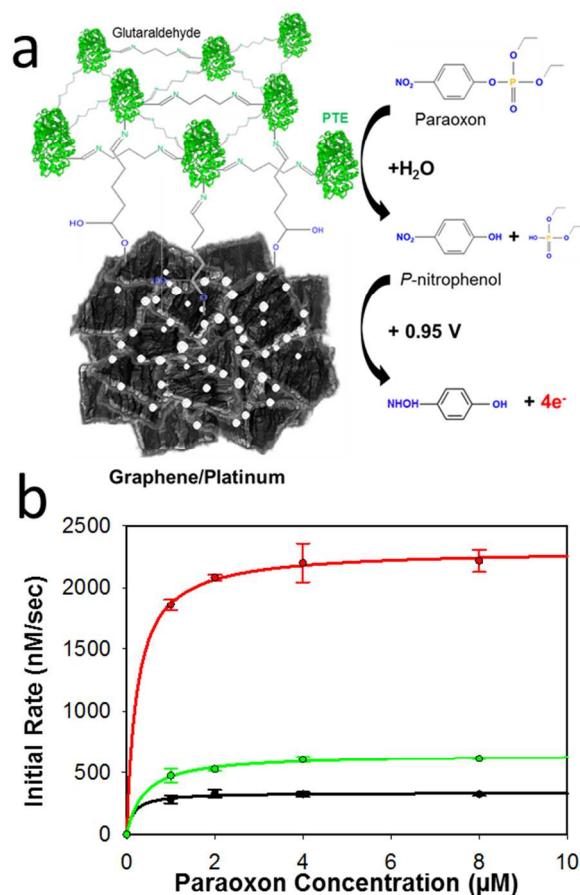


Figure 5. (a) Schematic diagram of PTE functionalized *via* glutaraldehyde to the PtNP-IML-PGE surface. Hydrolyses of paraoxon into *p*-nitrophenol due to immobilized PTE enzyme and subsequent oxidation of *p*-nitrophenol at the graphene electrode surface operating with a working potential of +0.95 V *vs.* Ag/AgCl. **(b)** Enzyme progress curve displaying the rate of *p*-nitrophenol production for various concentrations of paraoxon with enzyme inks created with distinct concentrations of PTE: 2 nM (Black), 4 nM (Green), 20 nM (Red).

The PtNP-IML-PGE was biofunctionalized with PTE enzymes by covalent crosslinking with glutaraldehyde and albumin. Glutaraldehyde crosslinking offers a straightforward and inexpensive approach to immobilizing enzymes onto electrode surfaces and in particular has shown to enhance the biosensor thermostability, reusability, and shelf-life when used to covalently link enzymes to graphene/graphene oxide electrodes.⁵⁷⁻⁵⁹ Distinct concentrations of glutaraldehyde (0.125, 0.175, 0.25, 0.325, 0.5%) within a BSA/PTE mixture were tested to determine which improved the biosensor sensitivity the most (Supporting Information Figure

S8). Increasing concentration of glutaraldehyde from 0.125% to 0.25% significantly improved the biosensor sensitivity to paraoxon (most likely through increased loading of active enzyme on the electrode surface). However, the sensitivity begins to decrease after glutaraldehyde concentrations of 0.25% due to an increased diffusion barrier which hinders paraoxon from binding to the enzyme and impedes *p*-nitrophenol from reaching the graphene transduction material after catalysis.

3.2. Biosensor Performance Characterization

3.2.1 Initial Calibration

The PTE biofunctionalized PtNP-IML-PGE was first calibrated in buffer solution *via* amperometry at an applied +0.95 V *vs.* Ag/AgCl (Figure 6a). The biosensor was capable of rapidly monitoring (response time < 10 seconds) successive paraoxon concentration increases with distinct amperometric response signals for consecutive 0.1 μ M paraoxon additions (blue arrows) and 1 μ M concentration additions (red arrows). The biosensor displayed a semi-linear characteristic calibration plot that can be fitted with a second order polynomial ($i_{pa} = -0.011[\text{paraoxon}]^2 + 0.350[\text{paraoxon}]$ where i_{pa} is the peak anodic current response with a coefficient of determination (R^2) of 0.995. However, a linear fit of this calibration plot ($i_{pa} = 0.263[\text{paraoxon}]$) yielded a lower R^2 value (0.978). This deviation from linearity is most likely due to the increased diffusion layer caused by the glutaraldehyde cross linking that limits the diffusion of paraoxon to the enzyme as well as the product (*p*-nitrophenol) to the electrode surface. Note that both the PtNP-IML-PGE and IML-PGE were biofunctionalized and linearly calibrated (Figure 6b); PtNP-IML-PGE displayed a higher sensitivity (370 nA/ μ M) and lower detection limit (3 nM, S/N=3) than the PTE biofunctionalized IML-PGE (270 nA/ μ M and 12 nM).

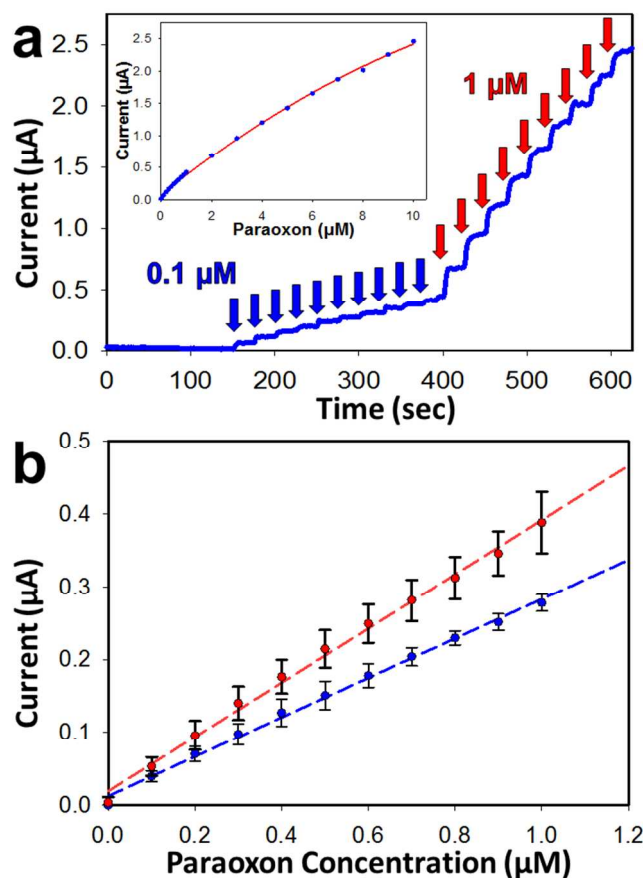


Figure 6. Biosensor calibration plots. **(a)** Amperometric response of paraoxon additions: 0.1 μM additions (blue) and 1 μM additions (red) for the PTE functionalized PtNP-IML-PGE. Inset: corresponding concentration vs. current graph (second order polynomial fit). **(b)** Paraoxon concentration vs. amperometric current response for the IML-PGE (blue) and the PtNP-IML-PGE (red) (linear fit). Error bars are standard deviation of 3 runs ($n = 3$).

These biosensor results compare quite favorably with other paraoxon electrochemical biosensors. For example, the PtNP-IML-PGE biosensor displayed the highest sensitivity and lowest detection limit of any reported electrochemical biosensor that utilizes the PTE enzyme to detect paraoxon (Table 1). Note that the PtNP-IML-PGE biosensor paraoxon sensitivity, detection limit, and linear range reported in Table 1 were all calculated using the linear fit to the calibration plot to be congruent with standard reporting practices (Figure 6b). The developed biosensor could also be implemented into high-volume manufacturing protocols (*e.g.*, roll-to-roll polymer printing and graphene coating) as there is no need for photolithography steps and

electrode patterning can be conducted on flexible, disposable substrates. Additionally, the biosensor design eliminated the need for multiple processing and sensing steps (*e.g.*, electrode polishing, multiple electrodeposition steps, a faraday cage, flow injection, or ion exchange membranes) that have been reported with previous paraoxon biosensors (Table 1).

Table 1: Performance of various direct PTE amperometric biosensors

Material/Immobilize	Sensitivity (nA/μM)	Detection Limit (nM)	Linear Range (μM)	Ref.
GC-SWNT/EDC-NHS	2.4	10	0.5-8.5	50
GC-CLEC/GA	25.95	314	0.5-2.0	34
GC-MWNT/Na - FI	25	150	0.25-4	51
FI-Au-Ny/GA	2.29	100	1-10	60
MWNT-DNA/PEI	74	77	-	61
C-Ny/GA-Si	12	20	0.02-18	28
GC-MC-CB/Na	198	120	0.2-8	25
C/Na	1.45	400	4.6-46	62
GC-MC/Na	129	9	0.5-25	52
IML-PGE/GA	270	12	0.1-1	This Work
PtNP-IML-PGE/GA	370	3	0.1-1	This Work

GC – Glassy Carbon; SWNT – Single-walled Carbon Nanotubes; CLEC – Cross-linked Enzyme Crystals; GA – Glutaraldehyde; MWNT – Multi-walled Carbon Nanotubes; Na – Nafion; FI – Flow Injection; PEI – Polyethyleneimine; C – Carbon; Ny – Nylon; Si – Silicon Oil; MC – Mesoporous Carbon; CB – Carbon Black; PtNP – Platinum Nanoparticles; IML – Inkjet Maskless Lithography; PGE – Patterned Graphene Electrodes

3.2.2 Stability and Reusability

The PTE biofunctionalized PtNP-IML-PGE also demonstrated a high degree of stability, reusability, and selectivity. For example, the biosensor retains a steady (90%) anodic current over 1000 sec after 1 μM paraoxon concentration additions, demonstrating little surface polymerization and good operational stability (Figure 7a). Such resistance to surface fouling may be due to the hydrophobic nature of the laser annealed IML-PGE, as previously mentioned. Long-term biosensor stability was evaluated by testing the biosensors each week for 8 weeks (Note the biosensors were stored at 4°C when testing was not occurring.). The biosensor retained nearly 70% and 50% of initial sensitivity to paraoxon for PtNP-IML-PGE and IML-PGE, respectively (Figure 7b). This retainment in enzyme activity could be attributed to the biocompatibility of the graphene as well as the strong crosslinking of glutaraldehyde, all of

which may prevent enzyme denaturation. The biosensor also demonstrated a strong degree of reusability and retained 95% sensitivity to paraoxon even after 12 repeated uses (average of 0.3% decrease per time sensed, Figure 7c). Hence the original amperometric current response was nearly retained after each of the 12 sensing experiments.

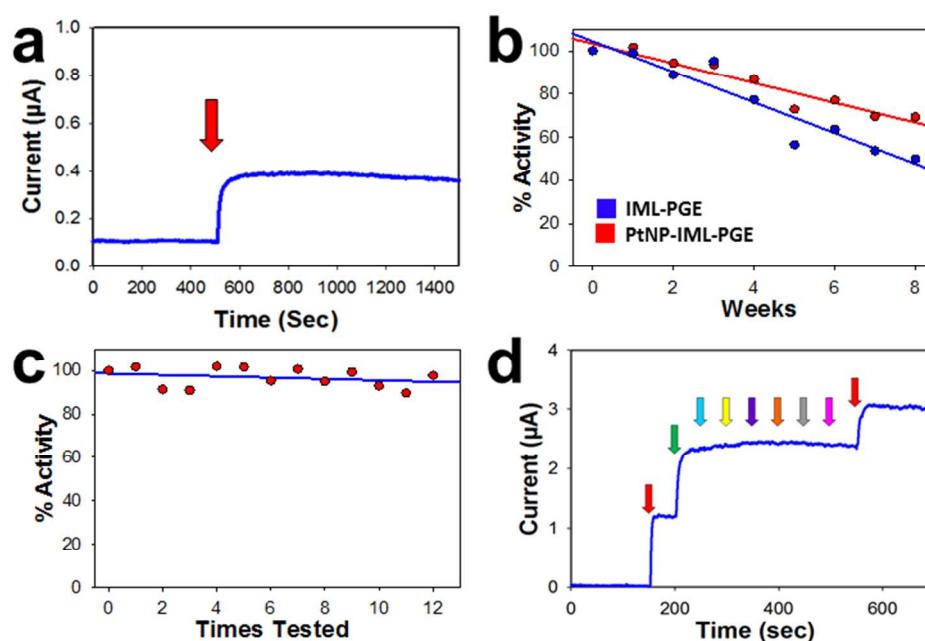


Figure 7. PtNP-IML-PGE biosensor characterization. **(a)** Stability test: steady oxidation current of 1 μM paraoxon addition over 1000 sec. **(b)** Longevity test: sensitivity of biosensors tested over 1-week intervals. **(c)** Reusability test: sensitivity of a single biosensor with repeated test runs. **(d)** Selectivity test: 5 μM spikes of paraoxon (red), *p*-nitrophenol (green), chlorpyrifos methyl (blue), Parathion (yellow), dichlorfenthion (purple), fenitrothion (orange), phoxim (grey), and dimethoate (pink).

Next, the selectivity of the designed biosensor was evaluated against potentially interfering nerve agents and within actual soil slurries. It should be noted here that OP sensors that rely on PTE are selective as the enzyme specifically targets triple O-linked phosphonate centers such as found in paraoxon, parathion, chlorpyrifos and chemical warfare agents such as Sarin and Soman. The selectivity of the biosensor was analyzed during amperometry by adding OP concentrations (5 μM additions) into buffer solution along with various pesticides. The biosensor exhibited a large current increase for paraoxon and *p*-nitrophenol, but an undetectable

amperometric increases for methyl parathion and chlorpyrifos (Figure 7d). The biosensors inability to detect these ubiquitous phosphates is consistent with the reported class of PTE that catalyzes these pesticides at a much slower rate.^{51, 54, 62} Additional pesticides that do not contain phenolic leaving groups or are not catalyzed by PTE (dichlofenthion, fenitrothion, phoxim, and dimethoate) were also tested and do not show any substantial increase in oxidation current. Paraoxon was then added again to the solution and a similar step height was observed demonstrating that none of the pesticide competitively inhibited PTE. The biosensor was next tested in a variety of biological solutions (tap water, river water, and a soil slurry) to evaluate its selectivity within actual biological matrices. All solutions were filtered with a 0.45 μm syringe filter, pH adjusted to 8.0 with NaOH, and ionic strength increased to 0.01 M PBS. The biosensor was able to detect low levels (5 μM) of paraoxon in a variety of real world solution mediums (Table 2). All biosensor test results were within 10% of pure buffer solutions (based on second order polynomial calibration plot, Figure 6a) demonstrating the biosensor is amendable to in-field or point-of-service testing in water and soil samples.

Table 2: Performance of the designed biosensor in a variety of mediums

Solution	Addition Spiked (μM)	Concentration Detected (μM)	Accuracy (%)
Tap Water	5	5.35	107
River Water	5	5.10	102
Soil Slurry	5	4.75	95

4. CONCLUSIONS

In conclusion, an amperometric biosensor for the detection of OPs (paraoxon) has been developed based on crosslinked PTE onto printed graphene electrodes that has been nano/microstructured *via* laser annealing and PtNP electrodeposition. Graphene provides an effective transduction material for rapidly monitoring the oxidation of *p*-nitrophenol due to high

conductivity, heterogenous charge transport, and biocompatibility. The transduction layer was further enhanced through laser annealing which fused graphene flakes together, increased surface area, and provided stable attachment locations through oxygen functional groups. The high surface area creates a hydrophobic biosensor that resists surface fouling by repelling non-specific species from adsorbing on the electrode surface. PtNP were utilized to increase sensitivity and improve biosensor performance (increased surface area and improved biosensor stability). The resulting biosensor exhibited the lowest detection limit (3 nM) and highest sensitivity (370 nA/ μ M) of any electrochemical PTE biosensor. The designed biosensor displayed a stable response to paraoxon (retained 90% anodic current over 1000 sec), long-term stability (70% over 8 weeks), reusability (90% after 12 repeated scans), and high selectivity to paraoxon. Finally, the biosensors were tested in real samples (tap water, river water, and a soil slurry) to demonstrate in-field biological matrices.

Inkjet Maskless Lithography (IML) provides a rapid and low-cost process to manufacture highly defined graphene electrodes for electrochemical sensing. PtNP-IML-PGE also can be implemented into a high-volume manufacturing (*e.g.*, roll-to-roll processing) as it does not require high cost photolithography steps and is patterned on a low-cost, disposable substrate. The designed biosensor utilizes PTE that is selective to triple O-linked phosphonate centers; therefore, it is advantageous over cholinesterase biosensors which require additional substrates, incubation periods, and are not selective to only organophosphates. In-field application of this biosensor could present farmers with a rapid, point-of-application sensor to monitor pesticide levels, which allows for a more accurate application of OPs, decreasing negative environmental impacts. The biosensor could be employed for drinking water testing⁶³⁻⁶⁴ or defense threat monitoring,^{20, 65} *via* a Boolean enzyme cascade for example, to provide high fidelity warnings for

proactive measures to be taken to protect human life.⁶⁶ Additionally, since the printing, laser annealing, and functionalization protocols can all be performed on thermally and chemically sensitive materials (e.g., polymers and paper), the developed graphene-based OP biosensor could be incorporated into wearable ring-based, glove-based, or textile-based sensor platforms for rapid in-field analysis and defense threat awareness of nerve agents.⁶⁷ Finally, the PtNP-IML-PGE fabrication protocol could be used for the scalable manufacturing of printed graphene-based electrodes for other applications in addition to biosensors including high-performance supercapacitors,⁶⁸ biofuel cells,⁶⁹ as well as dye-sensitized solar cells.⁷⁰

ASSOCIATED CONTENT

Supporting Information

The Supporting Information is available free of charge on the ACS Publications website at DOI:

SEMs of laser annealed graphene with various carving times, SEMs of platinum NPs with various number of cycles, Biosensor's sensitivity and detection limit depending on pH, Biosensor's sensitivity and detection limit based on applied potential, Sheet resistance of IML-PGE based on carving time, Cyclic voltammograms of SPCE, IML-PGE, and PtNP-IML-PGE with various scan rates in ferro/ferricyanide, Cyclic voltammograms of SPCE, IML-PGE, and PtNP-IML-PGE in buffer and 1 mM *p*-nitrophenol, Amperometric and sensitivity graphs for various concentrations of glutaraldehyde, Movie of IML graphene electrode fabrication.

AUTHOR INFORMATION

Corresponding Author

*(J.C.C.) Email jcclauss@iastate.edu

ORCID

John A. Hondred: [0000-0001-9913-7223](https://orcid.org/0000-0001-9913-7223)

Jonathan C. Claussen: [0000-0001-7065-1077](https://orcid.org/0000-0001-7065-1077)

Notes

The authors declare no competing financial interest.

ACKNOWLEDGEMENTS

J. C. C. gratefully acknowledges funding support for this work by the National Institute of Food and Agriculture, U.S. Department of Agriculture, under award number 2016-67021-25038, the National Science Foundation under award number CBET-1706994 as well as by the Iowa State University College of Engineering and Department of Mechanical Engineering.

REFERENCES

- (1) Martin Enserink, P. J. H., Sacha N. Vignieri, Nicholas S. Wigginton, and Jake S. Yeston. The Pesticide Paradox. *Science* **2013**, *341*, 730-731, DOI: 10.1126/science.341.6147.730.
- (2) Fenner, K.; Canonica, S.; Wackett, L. P.; Elsner, M. Evaluating pesticide degradation in the environment: blind spots and emerging opportunities. *Science* **2013**, *341*, 752-758.
- (3) Brown, M. A.; Brix, K. A. Review of health consequences from high-, intermediate-and low-level exposure to organophosphorus nerve agents. *J. Appl. Toxicol.* **1998**, *18*, 393-408.
- (4) Munro, N. B.; Talmage, S. S.; Griffin, G. D.; Waters, L. C.; Watson, A. P.; King, J. F.; Hauschild, V. The sources, fate, and toxicity of chemical warfare agent degradation products. *Environ. Health Perspect.* **1999**, *107*, 933.
- (5) Kim, K.; Tsay, O. G.; Atwood, D. A.; Churchill, D. G. Destruction and detection of chemical warfare agents. *Chem. Rev.* **2011**, *111*, 5345-5403.
- (6) Yanagisawa, N.; Morita, H.; Nakajima, T.; Okudera, H.; Shimizu, M.; Hirabayashi, H.; Nohara, M.; Midorikawa, Y.; Mimura, S. Sarin poisoning in Matsumoto, Japan. *Lancet* **1995**, *346*, 290-293.
- (7) Okumura, T.; Takasu, N.; Ishimatsu, S.; Miyanoki, S.; Mitsuhashi, A.; Kumada, K.; Tanaka, K.; Hinohara, S. Report on 640 victims of the Tokyo subway sarin attack. *Ann. Emerg. Med.* **1996**, *28*, 129-135.
- (8) Muñoz-Quezada, M. T.; Lucero, B. A.; Iglesias, V. P.; Muñoz, M. P.; Cornejo, C. A.; Achu, E.; Baumert, B.; Hanchey, A.; Concha, C.; Brito, A. M. Chronic exposure to organophosphate (OP) pesticides and neuropsychological functioning in farm workers: a review. *Int. J. Occup. Environ. Health* **2016**, *22*, 68-79.

- (9) Rothlein, J.; Rohlman, D.; Lasarev, M.; Phillips, J.; Muniz, J.; McCauley, L. Organophosphate pesticide exposure and neurobehavioral performance in agricultural and nonagricultural Hispanic workers. *Environ. Health Perspect.* **2006**, *114*, 691.
- (10) Zhang, X.; Wu, M.; Yao, H.; Yang, Y.; Cui, M.; Tu, Z.; Stallones, L.; Xiang, H. Pesticide poisoning and neurobehavioral function among farm workers in Jiangsu, People's Republic of China. *Cortex* **2016**, *74*, 396-404.
- (11) Raanan, R.; Balmes, J. R.; Harley, K. G.; Gunier, R. B.; Magzamen, S.; Bradman, A.; Eskenazi, B. Decreased lung function in 7-year-old children with early-life organophosphate exposure. *Thorax* **2016**, *71*, 148-153.
- (12) Jaipieam, S.; Visuthismajarn, P.; Sutheravut, P.; Siri Wong, W.; Thoumsang, S.; Borjan, M.; Robson, M. Organophosphate pesticide residues in drinking water from artesian wells and health risk assessment of agricultural communities, Thailand. *Hum. Ecol. Risk Assess.* **2009**, *15*, 1304-1316.
- (13) Fries, E.; Püttmann, W. Monitoring of the three organophosphate esters TBP, TCEP and TBEP in river water and ground water (Oder, Germany). *J. Environ. Monit.* **2003**, *5*, 346-352.
- (14) USDA-PDA, Pesticide Data Program Annual Summary, Calendar Year 2008. Available at: <http://www.ams.usda.gov/pdp>, 2008.
- (15) USDA, USDA Pesticide Data Program Analytical Methods. Available at: <http://www.ams.usda.gov/AMSV1.0/getfile?dDocName=STELPRDC5049940>, 2010.
- (16) Fenske, R. A.; Black, K. G.; Elkner, K. P.; Lee, C.-L.; Methner, M. M.; Soto, R. Potential exposure and health risks of infants following indoor residential pesticide applications. *Am. J. Public. Health Res.* **1990**, *80*, 689-693.
- (17) Mulchandani, A.; Mulchandani, P.; Chen, W.; Wang, J.; Chen, L. Amperometric thick-film strip electrodes for monitoring organophosphate nerve agents based on immobilized organophosphorus hydrolase. *Anal. Chem.* **1999**, *71*, 2246-2249.
- (18) Vo-Dinh, T.; Cullum, B. Biosensors and biochips: advances in biological and medical diagnostics. *Fresenius J. Anal. Chem.* **2000**, *366*, 540-551.
- (19) Kirsch, J.; Siltanen, C.; Zhou, Q.; Revzin, A.; Simonian, A. Biosensor technology: recent advances in threat agent detection and medicine. *Chem. Soc. Rev.* **2013**, *42*, 8733-8768.
- (20) Verma, N.; Bhardwaj, A. Biosensor technology for pesticides—a review. *Appl. Biochem. Biotechnol.* **2015**, *175*, 3093-3119.
- (21) Arduini, F.; Forchielli, M.; Amine, A.; Neagu, D.; Cacciotti, I.; Nanni, F.; Moscone, D.; Palleschi, G. Screen-printed biosensor modified with carbon black nanoparticles for the determination of paraoxon based on the inhibition of butyrylcholinesterase. *Microchim. Acta.* **2015**, *182*, 643-651.
- (22) Kesik, M.; Kanik, F. E.; Turan, J.; Kolb, M.; Timur, S.; Bahadir, M.; Toppare, L. An acetylcholinesterase biosensor based on a conducting polymer using multiwalled carbon nanotubes for amperometric detection of organophosphorous pesticides. *Sens. Actuators, B* **2014**, *205*, 39-49.
- (23) Guilhermino, L.; Barros, P.; Silva, M. C.; Soares, A. M. V. M. SHORT COMMUNICATION Should the use of inhibition of cholinesterases as a specific biomarker for organophosphate and carbamate pesticides be questioned. *Biomarkers* **1998**, *3*, 157-163.
- (24) Bigley, A. N.; Raushel, F. M. Catalytic mechanisms for phosphotriesterases. *Biochim. Biophys. Acta, Biophys.* **2013**, *1834*, 443-453.
- (25) Alizadeh, T.; Ganjali, M. R.; Norouzi, P.; Zare, M.; Zeraatkar, A. A novel high selective and sensitive para-nitrophenol voltammetric sensor, based on a molecularly imprinted polymer-carbon paste electrode. *Talanta* **2009**, *79*, 1197-1203.
- (26) Hu, Y.-f.; Zhang, Z.-h.; Zhang, H.-b.; Luo, L.-j.; Yao, S.-z. Sensitive and selective imprinted electrochemical sensor for p-nitrophenol based on ZnO nanoparticles/carbon nanotubes doped chitosan film. *Thin Solid Films* **2012**, *520*, 5314-5321.

- (27) Arvinte, A.; Mahosenaho, M.; Pinteala, M.; Sesay, A.-M.; Virtanen, V. Electrochemical oxidation of p-nitrophenol using graphene-modified electrodes, and a comparison to the performance of MWNT-based electrodes. *Microchim. Acta* **2011**, *174*, 337-343.
- (28) Chough, S. H.; Mulchandani, A.; Mulchandani, P.; Chen, W.; Wang, J.; Rogers, K. R. Organophosphorus hydrolase-based amperometric sensor: modulation of sensitivity and substrate selectivity. *Electroanalysis* **2002**, *14*, 273.
- (29) Li, J.; Kuang, D.; Feng, Y.; Zhang, F.; Xu, Z.; Liu, M. A graphene oxide-based electrochemical sensor for sensitive determination of 4-nitrophenol. *J. Hazard. Mater.* **2012**, *201*, 250-259.
- (30) Mulchandani, P.; Hangarter, C. M.; Lei, Y.; Chen, W.; Mulchandani, A. Amperometric microbial biosensor for p-nitrophenol using *Moraxella* sp.-modified carbon paste electrode. *Biosens. Bioelectron.* **2005**, *21*, 523-527.
- (31) Van Dyk, J. S.; Pletschke, B. Review on the use of enzymes for the detection of organochlorine, organophosphate and carbamate pesticides in the environment. *Chemosphere* **2011**, *82*, 291-307, DOI: <http://dx.doi.org/10.1016/j.chemosphere.2010.10.033>.
- (32) Hondred, J. A.; Stromberg, L. R.; Mosher, C. L.; Claussen, J. C. High Resolution Graphene Films for Electrochemical Sensing via Inkjet Maskless Lithography. *ACS Nano* **2017**, *11*, 9836-9845, DOI: 10.1021/acsnano.7b03554.
- (33) Breger, J. C.; Ancona, M. G.; Walper, S. A.; Oh, E.; Susumu, K.; Stewart, M. H.; Deschamps, J. R.; Medintz, I. L. Understanding how nanoparticle attachment enhances phosphotriesterase kinetic efficiency. *ACS Nano* **2015**, *9*, 8491-8503.
- (34) Laothanachareon, T.; Champreda, V.; Sritongkham, P.; Somasundrum, M.; Surareungchai, W. Cross-linked enzyme crystals of organophosphate hydrolase for electrochemical detection of organophosphorus compounds. *World J. Microbiol. Biotechnol.* **2008**, *24*, 3049-3055.
- (35) Sahin, A.; Dooley, K.; Cropek, D. M.; West, A. C.; Banta, S. A dual enzyme electrochemical assay for the detection of organophosphorus compounds using organophosphorus hydrolase and horseradish peroxidase. *Sens. Actuators, B* **2011**, *158*, 353-360.
- (36) Miller, G. C.; Crosby, D. G. Pesticide photoproducts: generation and significance. *J. Toxicol. Clin. Toxicol.* **1982**, *19*, 707-735.
- (37) Zhang, Y. I.; Zhang, L.; Zhou, C. Review of chemical vapor deposition of graphene and related applications. *Acc. Chem. Res.* **2013**, *46*, 2329-2339.
- (38) Claussen, J. C.; Artiles, M. S.; McLamore, E. S.; Mohanty, S.; Shi, J.; Rickus, J. L.; Fisher, T. S.; Porterfield, D. M. Electrochemical glutamate biosensing with nanocube and nanosphere augmented single-walled carbon nanotube networks: a comparative study. *Journal of Materials Chemistry* **2011**, *21*, 11224-11231.
- (39) Salinas-Torres, D.; Huerta, F.; Montilla, F.; Morallón, E. Study on electroactive and electrocatalytic surfaces of single walled carbon nanotube-modified electrodes. *Electrochimica Acta* **2011**, *56*, 2464-2470.
- (40) Das, S. R.; Nian, Q.; Cargill, A. A.; Hondred, J. A.; Ding, S.; Saei, M.; Cheng, G. J.; Claussen, J. C. 3D nanostructured inkjet printed graphene via UV-pulsed laser irradiation enables paper-based electronics and electrochemical devices. *Nanoscale* **2016**, *8*, 15870-15879.
- (41) Das, S. R.; Srinivasan, S.; Stromberg, L. R.; He, Q.; Garland, N.; Straszheim, W. E.; Ajayan, P. M.; Balasubramanian, G.; Claussen, J. C. Superhydrophobic inkjet printed flexible graphene circuits via direct-pulsed laser writing. *Nanoscale* **2017**, *9*, 19058-19065.
- (42) Hondred, J. A.; Stromberg, L. R.; Mosher, C. L.; Claussen, J. C. High Resolution Graphene Films for Electrochemical Sensing via Inkjet Maskless Lithography. *ACS nano* **2017**.
- (43) Claussen, J. C.; Kumar, A.; Jaroch, D. B.; Khawaja, M. H.; Hibbard, A. B.; Porterfield, D. M.; Fisher, T. S. Nanostructuring platinum nanoparticles on multilayered graphene petal nanosheets for electrochemical biosensing. *Adv. Funct. Mater.* **2012**, *22*, 3399-3405.

- (44) Dutta, N.; Biswas, S.; Saha, M. K. Biophysical characterization and activity analysis of nano-magnesium supplemented cellulase obtained from a psychrobacterium following graphene oxide immobilization. *Chem. Rev.* **2016**, *95*, 248-258.
- (45) Takmakov, P.; Zachek, M. K.; Keithley, R. B.; Walsh, P. L.; Donley, C.; McCarty, G. S.; Wightman, R. M. Carbon microelectrodes with a renewable surface. *Anal. Chem.* **2010**, *82*, 2020-2028.
- (46) Chandra, S.; Miller, A. D.; Bendavid, A.; Martin, P. J.; Wong, D. K. Y. Minimizing fouling at hydrogenated conical-tip carbon electrodes during dopamine detection in vivo. *Anal. Chem.* **2014**, *86*, 2443-2450.
- (47) Pérez-López, B.; Sola, J.; Alegret, S.; Merkoçi, A. A carbon nanotube PVC based matrix modified with glutaraldehyde suitable for biosensor applications. *Electroanalysis* **2008**, *20*, 603-610.
- (48) Zhang, H.; Lamb, R.; Lewis, J. Engineering nanoscale roughness on hydrophobic surface—preliminary assessment of fouling behaviour. *Sci. Technol. Adv. Mater.* **2005**, *6*, 236-239.
- (49) Claussen, J. C.; Kim, S. S.; Haque, A.; Artilles, M. S.; Porterfield, D. M.; Fisher, T. S. Electrochemical glucose biosensor of platinum nanospheres connected by carbon nanotubes. *J. Diabetes Sci. Technol.* **2010**, *4*, 312-319.
- (50) Pedrosa, V. A.; Paliwal, S.; Balasubramanian, S.; Nepal, D.; Davis, V.; Wild, J.; Ramanculov, E.; Simonian, A. Enhanced stability of enzyme organophosphate hydrolase interfaced on the carbon nanotubes. *Colloids Surf., B* **2010**, *77*, 69-74.
- (51) Deo, R. P.; Wang, J.; Block, I.; Mulchandani, A.; Joshi, K. A.; Trojanowicz, M.; Scholz, F.; Chen, W.; Lin, Y. Determination of organophosphate pesticides at a carbon nanotube/organophosphorus hydrolase electrochemical biosensor. *Anal. Chim. Acta.* **2005**, *530*, 185-189.
- (52) Tang, X.; Zhang, T.; Liang, B.; Han, D.; Zeng, L.; Zheng, C.; Li, T.; Wei, M.; Liu, A. Sensitive electrochemical microbial biosensor for p-nitrophenylorganophosphates based on electrode modified with cell surface-displayed organophosphorus hydrolase and ordered mesopore carbons. *Biosens. Bioelectron.* **2014**, *60*, 137-142.
- (53) Chen, Z.; Wang, J.; Chao, D.; Baikie, T.; Bai, L.; Chen, S.; Zhao, Y.; Sum, T. C.; Lin, J.; Shen, Z. Hierarchical porous LiNi_{1/3}Co_{1/3}Mn_{1/3}O₂ nano-/micro spherical cathode material: minimized cation mixing and improved Li⁺ mobility for enhanced electrochemical performance. *Sci. Rep.* **2016**, *6*, 25771.
- (54) Zhang, X.; Wu, R.; Song, L.; Lin, Y.; Lin, M.; Cao, Z.; Wu, W.; Mo, Y. Molecular dynamics simulations of the detoxification of paraoxon catalyzed by phosphotriesterase. *J. Comput. Chem.* **2009**, *30*, 2388-2401.
- (55) Hondred, J. A.; Breger, J. C.; Garland, N. T.; Oh, E.; Susumu, K.; Walper, S. A.; Medintz, I. L.; Claussen, J. C. Enhanced enzymatic activity from phosphotriesterase trimer gold nanoparticle bioconjugates for pesticide detection. *Analyst* **2017**, *142*, 3261-3271.
- (56) Breger, J. C.; Buckhout-White, S.; Walper, S. A.; Oh, E.; Susumu, K.; Ancona, M. G.; Medintz, I. L. Assembling high activity phosphotriesterase composites using hybrid nanoparticle peptide-DNA scaffolded architectures. *Nano Futures* **2017**, *1*, 011002.
- (57) Su, R.; Shi, P.; Zhu, M.; Hong, F.; Li, D. Studies on the properties of graphene oxide–alkaline protease bio-composites. *Bioresource technology* **2012**, *115*, 136-140.
- (58) Pavlidis, I. V.; Vorhaben, T.; Tsoufis, T.; Rudolf, P.; Bornscheuer, U. T.; Gournis, D.; Stamatis, H. Development of effective nanobiocatalytic systems through the immobilization of hydrolases on functionalized carbon-based nanomaterials. *Bioresource technology* **2012**, *115*, 164-171.
- (59) Kishore, D.; Talat, M.; Srivastava, O. N.; Kayastha, A. M. Immobilization of β -galactosidase onto functionalized graphene nano-sheets using response surface methodology and its analytical applications. *PLoS One* **2012**, *7*, e40708.
- (60) Wang, J.; Krause, R.; Block, K.; Musameh, M.; Mulchandani, A.; Schöning, M. J. Flow injection amperometric detection of OP nerve agents based on an organophosphorus–hydrolase biosensor detector. *Biosens. Bioelectron.* **2003**, *18*, 255-260.

- (61) Kirsch, J.; Davis, V. A.; Simonian, A. L. In *Direct and discriminative detection of organophosphate neurotoxins for food and agriculture products*, 2012; IEEE: pp 1-4.
- (62) Wang, J.; Chen, L.; Mulchandani, A.; Mulchandani, P.; Chen, W. Remote biosensor for in-situ monitoring of organophosphate nerve agents. *Electroanalysis* **1999**, *11*, 866-869.
- (63) Istamboulie, G.; Fournier, D.; Marty, J.-L.; Noguer, T. Phosphotriesterase: a complementary tool for the selective detection of two organophosphate insecticides: chlorpyrifos and chlorfenvinfos. *Talanta* **2009**, *77*, 1627-1631.
- (64) Karpuzcu, M. E.; Sedlak, D. L.; Stringfellow, W. T. Biotransformation of chlorpyrifos in riparian wetlands in agricultural watersheds: Implications for wetland management. *Journal of hazardous materials* **2013**, *244*, 111-120.
- (65) Mulchandani, A.; Chen, W.; Mulchandani, P.; Wang, J.; Rogers, K. R. Biosensors for direct determination of organophosphate pesticides. *Biosensors and bioelectronics* **2001**, *16*, 225-230.
- (66) Chuang, M.-C.; Windmiller, J. R.; Santhosh, P.; Ramírez, G. V.; Katz, E.; Wang, J. High-fidelity determination of security threats via a Boolean biocatalytic cascade. *Chem. Commun.* **2011**, *47*, 3087-3089.
- (67) Mishra, R. K.; Hubble, L. J.; Martín, A.; Kumar, R.; Barfidokht, A.; Kim, J.; Musameh, M. M.; Kyratzis, I. L.; Wang, J. Wearable flexible and stretchable glove biosensor for on-site detection of organophosphorus chemical threats. *ACS Sensors* **2017**, *2*, 553-561.
- (68) Kang, S.; Lim, K.; Park, H.; Park, J. B.; Park, S. C.; Cho, S.-P.; Kang, K.; Hong, B. H. Roll-to-roll laser-printed graphene-graphitic carbon electrodes for high-performance supercapacitors. *ACS Appl. Mater. Interfaces* **2017**.
- (69) Mano, N.; de Poulpique, A. O₂ Reduction in Enzymatic Biofuel Cells. *Chem. Rev.* **2017**.
- (70) Liu, H.-W.; Liang, S.-p.; Wu, T.-J.; Chang, H.; Kao, P.-K.; Hsu, C.-C.; Chen, J.-Z.; Chou, P.-T.; Cheng, I. C. Rapid atmospheric pressure plasma jet processed reduced graphene oxide counter electrodes for dye-sensitized solar cells. *ACS applied materials & interfaces* **2014**, *6*, 15105-15112.

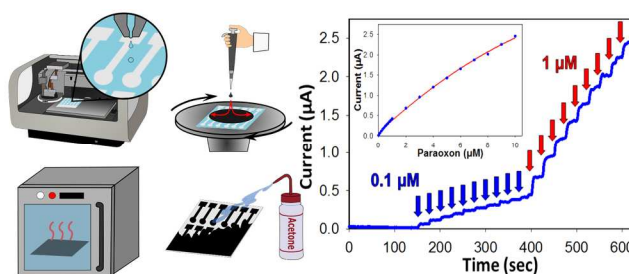


Table of Content (TOC) graphic