


Analyst

Accepted Manuscript



This article can be cited before page numbers have been issued, to do this please use: X. Zou, H. Xiaowei and M. Povey, *Analyst*, 2016, DOI: 10.1039/C5AN02152A.

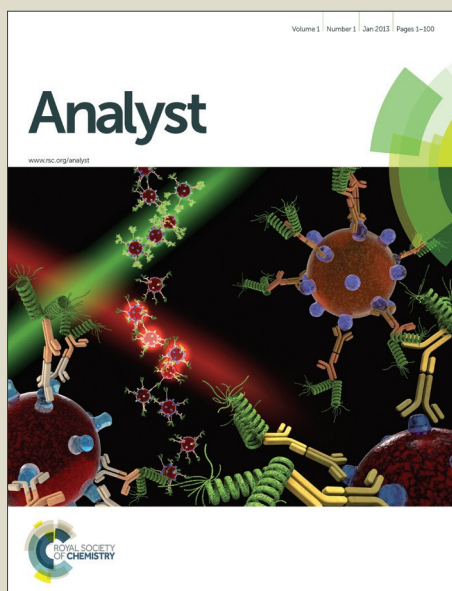

This is an *Accepted Manuscript*, which has been through the Royal Society of Chemistry peer review process and has been accepted for publication.

Accepted Manuscripts are published online shortly after acceptance, before technical editing, formatting and proof reading. Using this free service, authors can make their results available to the community, in citable form, before we publish the edited article. We will replace this *Accepted Manuscript* with the edited and formatted *Advance Article* as soon as it is available.

You can find more information about *Accepted Manuscripts* in the [Information for Authors](#).

Please note that technical editing may introduce minor changes to the text and/or graphics, which may alter content. The journal's standard [Terms & Conditions](#) and the [Ethical guidelines](#) still apply. In no event shall the Royal Society of Chemistry be held responsible for any errors or omissions in this *Accepted Manuscript* or any consequences arising from the use of any information it contains.

Non-invasive sensing for food reassurance

Zou Xiaobo^{*1,3}, Huang Xiaowei^{1,3}, Malcolm Povey^{*2,3}

¹ Agricultural Product Processing and Storage Lab, School of Food and Biological Engineering, Key Laboratory of Modern Agriculture Equipment and Technology, Jiangsu University, Zhenjiang, Jiangsu 212013, China

² School of Food Science and Nutrition, the University of Leeds, Leeds LS2 9JT, United Kingdom

³ contributed equally to the work

^{*} Corresponding author. Tel.: +86 511 88780174; fax: +86 511 88780201. Email: zou_xiaobo@ujs.edu.cn

^{*} Corresponding author. Tel.: +44 1132332963; fax: +44 1132332982. Email: m.j.w.povey@leeds.ac.uk

Abstract: Consumers and governments are increasingly interested in the safety, authenticity and quality of food commodities. This has driven attention towards non-invasive sensing techniques used for rapid analyzing these commodities. This paper provides an overview of the state of the art in, and available alternatives for, food assurance based on non-invasive sensing techniques. The main food quality traits of interest using non-invasive sensing techniques are sensory characteristics, chemical composition, physicochemical properties, health-protecting properties, nutritional characteristics and safety. A wide range of non-invasive sensing techniques, from optical, acoustical, electrical, to nuclear magnetic, x-ray, biosensor, microwave and terahertz, are organized according to physical principle. Some of these techniques are now in a period of transition between experimental and applied utilization and several sensors and instruments are reviewed. With continued innovation and attention to key challenges, such non-invasive sensors and biosensors are expected to open up new exciting avenues in the field of portable and wearable wireless sensing devices and connecting with mobile networks, thus finding considerable use in a wide range of food assurance applications. The need for an appropriate regulatory framework is emphasized which acts to exclude unwanted components in foods and includes needed components, with sensors as part of a reassurance framework supporting regulation and food chain management. The integration of these sensor modalities into a single technological and commercial platform offers an opportunity for a paradigm shift in food reassurance.

Keywords: Non-invasive sensing; food, machine vision; Vis/NIR spectroscopy; UV-Vis fluorescence; hyperspectral imaging, ultrasound; electronic nose; electronic tongue; conductivity; NMR; X-ray; Microwave; Terahertz; quality; reassurance

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Introduction

In recent years, consumers and governments are increasingly demanding information and reassurance on the content as well as on the origin of their food ¹⁻³. Food industry (suppliers, manufactures and supermarkets) are required to provide and confirm the authenticity and point of origin of food products and their components, in order to protect consumer rights and prevent fraudulent or deceptive practices such as food adulteration. Therefore, food reassurance is crucial to food production and security of food supply ⁴⁻⁶.

Food reassurance

The concept of reassurance relies on the fact that it is desirable to ensure that the food adheres to its implied or commonly understood description. For example, free from inanimate objects such as glass, plastic, metal that can enter through the manufacturing processes; free from unacceptable levels of animate material such as viruses, bacteria, prions and spores that could lead to infection that can enter through poor hygiene; free from unacceptable levels of biological inanimate contamination such as peanut, almonds, contaminated vegetable oil, etc.; corresponds to the packaging claims, including type of food and origin (e.g. British beef). Given that it is best to exclude food contaminants from the food chain, sensors are best deployed in a regulatory context within which the sensing techniques form part of a compliance framework, reassuring that regulation is effective. A strategy for food reassurance might be summarized as Prevent, Reassure, and Detect.

Prevention is the best defense. Detection provides reassurance

Prevention implies a threat to food supply and includes adulteration. Examples of adulteration ⁷ include horsemeat added to other meats ⁸, the addition of waste oil to vegetable oils ⁹, the addition of ethylene glycol in Austrian wine ¹⁰ and the addition of melamine to milk in order to increase the apparent protein level ¹¹. There is also an expectation that a product claiming to be meat does not contain unreasonable levels of fat and gristle.

The best approach to food security is pro-active - anticipate the threat and then prevent it; especially in the manufacturing part of the supply chain with the potential for foreign body contamination from the process line. However, assured prevention requires detection. The rise in food contamination incidents in the UK highlight the need for better detection methods that are

fast, reliable and economic.

Food incidents need reassurance

The number of food incidents is increasing (See Fig. 1) and the evidence is that this is massively under-reported as food manufacturers have an interest in disguising food recalls which will cost millions of pounds per recall.

Fig. 1.

(1) Foreign bodies: Pieces of metal in food, very often originating from process machinery are a common cause of complaint. Pieces of glass, plastic, bone and nut shell are other common contaminants. Other common foreign body contamination is insects (dead or alive - in which case this can be regarded as infestation), 'natural' plant materials, hair and fiber.

(2) Chemical contamination: Herbicide and insecticide contamination, particularly from organophosphates continues to be a threat to human health. Other examples include mercury pollution of the sea around Japan ¹² giving rise to unacceptably high mercury intakes for some populations relying on a fish diet. The Fukushima accident has also increased the threat of radioactive contamination of food ¹³ and in the UK, arising from the 1986 Chernobyl reactor explosion and up to 2012 sheep from a number of farms in North Wales, Southern Lake District and near nuclear facilities in Scotland were banned from human consumption ¹⁴.

(3) Infestation: A large proportion of food spoilage arises due to insect and other forms of infestation such as rodents.

(4) Food deterioration: Food may deteriorate as a result of poor storage and/or transport. For example, chocolate may bloom if stored at too high a temperature, a fatty spread may separate into water and oil. Fruit and vegetables may ripen to the point of unacceptability and may also become bruised or damaged in some other way.

(5) Counterfeiting of food: High value foods such as Iberian Ham are subject to extensive counterfeiting ¹⁵.

(6) Food borne disease: Food borne disease is one of the biggest causes of ill health and time off work ¹⁶.

Globalization of food supply need reassurance

This is contradictory because the globalization of food supply has led to a diversification and

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

in some ways an increase in food security, at least in some countries such as the UK. Arguably globalization of food supply is also a cause of food poverty in the less industrialized countries. The threat addressed here is that it is much more difficult to provide reassurance of food origin, authenticity and safety in a global food chain. Large multinationals can mitigate the risk through control of every stage in the process from the seed, through planting, fertilizer and herbicide/insecticide, harvesting, distribution even as far as controlling the produce on the supermarket shelf. The Bernard Matthews Turkey scandal illustrates the potential for public health impacts arising from the globalization of food supply. Waste meat imported from Matthew’s plant in Poland was contaminated with Bird Flu and was intended for feeding to Turkey’s in the UK ¹⁷. Bovine Spongiform Encephalopathy (BSE) was also likely caused by the feeding of contaminated beef to cows ¹⁸.

Non-invasive sensing shows promise for food reassurance

Common food reassurance methods, such as immunological and enzymatic techniques, DNA and protein based assays and triacylglycerol analysis as applied in laboratories ¹⁹⁻²¹ are usually capable of detecting low levels of adulteration, but they are expensive, invasive, sophisticated, laborious, and technically demanding ^{22, 23}.

Recently, non-invasive (NIV) rapid sensing techniques combined with multivariate data analysis show promise for food reassurance. Because NIV techniques do not permanently alter the food being inspected, they are highly valuable techniques that can save both money and time in reassurance. In comparison with these reported common methods ¹⁹ which are time-consuming, expensive, use harmful reagents, need expert laboratory staff and are strongly dependent on rigorously following a standardized protocol to obtain accuracy, non-invasive rapid sensing techniques are non-destructive, require only basic training in a user-friendly software, a few minutes for detecting and processing and no cost at all excluding initial instrument and software purchase. This is the major stimulant for continuous ongoing developments in the field of NIV. There have been continuously increasing research efforts in the last two decades according to the increasing number of publications in NIV

Although there are many complete reviews of non-invasive techniques, the great volume of recent research results in this field requires a constant update. In this article, we review non-

Analyst Accepted Manuscript

invasive techniques and normal chemometrics for food assurance. The techniques are organized according to physical principle rather than quality attribute, because some measurement techniques can be used to measure widely different quality attributes. The advantages, limitations, and future trends of the techniques will be reviewed.

Techniques employed for non-invasive food assurance

There are many non-invasive sensing techniques in food as shown in Fig. 2. Among the techniques used, NIV techniques are mainly based on physical methods of analysis except biosensors. Some NIV techniques such as machine vision can provide external information such as color, shape, size, and the absence of surface defects of food products²⁴, and some NIV techniques such as ultrasound can provide internal quality such as firmness and crispiness, taste, aroma, and absence of internal defects^{25, 26}. NIV techniques such as the electronic nose²⁷ and hyperspectral imaging²⁸⁻³¹ can give quality attributes such as freshness, safety, nutritional value and health-promoting properties, chemical residues. Looking at the enormous number of literature produced during the last fifteen years, two groups of methods: optical methods, (visible/near/mid-infrared spectroscopy and imaging) and acoustic methods, (ultrasound spectroscopy, imaging and passive acoustics), may be considered the most researched non-invasive techniques for the assurance of food.

Fig. 2.

Optical techniques

Physical methods often rely on electromagnetic waves (Fig. 3). A complex interplay between absorption and scattering of the electromagnetic waves (light) guides the light - food interaction. There are three basically different ways of obtaining signal from a sample by measurement of diffuse reflection (I_{fd}), Transmission (I_t), and Emission (I_e). I_{fd} , I_t , and I_e contain information about absorption and scattering of light in food. Therefore, they may give information regarding the structure and chemical component related information in food. For example, IR/NIR/MIR scattering are related to the microstructure of the cells and intra/extracellular environments and the C-H, O-H, and N-H bonds of the main compounds (water, carbohydrates, fats/oils and proteins) are responsible for the absorption.

Fig. 3.

Photons are most strongly scattered by structures with the same size as the photon

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

wavelength, and can be absorbed only if they have the right energy to excite the vibrational states of the molecule in food. Most food is opaque to radiation in ultra-violet (UV), visible (Vis), near-infrared (NIR) and infrared (IR) regions of the electromagnetic spectrum. In this region, the main optical techniques are Vis/NIR spectroscopy, UV-Vis fluorescence, machine vision, hyperspectral imaging, and Raman spectroscopy. Published applications of these techniques to food are too numerous to record comprehensively here, particularly covering the last thirty years.

Machine Vision

When consumers buy food, food perception is limited to visual perception. The external appearance of food is a very important quality for both consumer and producer. Machine vision (MV), or computer vision, that can give the visual sensation of food, is therefore an important food assurance technique. It consists essentially of a digital camera that is connected to a computer and software for image analysis. MVs in visible light regions could recognize size³², shape³³, color^{34, 35}, and texture³⁶ of food. Some machine vision systems are also able to inspect these objects in parts of the electromagnetic spectrum invisible to humans, such as X-ray³⁷, ultraviolet (UV)³⁸, near-infrared (NIR)³⁹, and infrared (IR)⁴⁰. It is growing at a fast pace due to recent advances in hardware and software⁴¹⁻⁴³. There are extensive reviews about machine vision applications to food⁴⁴⁻⁴⁷. The potential of machine vision in the food industry has long been recognized and the food industry is now ranked among the top 10 industries using this technology^{47, 48}.

Vis/NIR spectroscopy

The light in Vis/NIR region can penetrate quite deeply (up to a few centimeters, depending on the wavelength) into biological tissue, as the absorption by water is relatively low in the Vis/NIR range compared to the mid-infrared (MIR) ranges⁴⁹ and the scattering of the light in this region is significantly larger than in MIR, this enables light to diffuse in the sample volume and to be reemitted at the tissue boundaries⁵⁰⁻⁵². Therefore, Vis/NIR spectroscopy can produce fingerprint spectra for food assurance. Usually, advanced chemometric techniques are needed to extract information from these spectra. Vis/NIR spectroscopy has been used successfully to authenticate many foods such as fruit^{53, 54}, vegetable^{55, 56}, meat^{57, 58}, fish⁵⁹, vine⁶⁰, milk⁶¹, starch^{62, 63}, oil⁶⁴⁻⁶⁶, cereal⁶⁷, transgenic food⁶⁸, and others. It also successfully gives physical-

chemical parameters of food, such as freshness^{69, 70}, water content^{71, 72}, soluble solids contents^{73, 74}, acidity⁷⁵⁻⁷⁷, firmness⁷⁷⁻⁷⁹, texture⁸⁰⁻⁸², and others, that relate to quality and safety of foods. There are many reviews of this area in recent years^{66, 68, 83-92}.

UV-visible fluorescence spectroscopy

Fluorescence spectroscopy is able to determine several properties (functional, composition, nutritional) without the use of chemical reagents. UV light excites the electrons in the molecules of certain compounds in food and causes them to emit lower energy light. As molecules of compounds in food can drop down into any of several vibrational levels in the ground state, the photons emitted will have different energies and thus frequencies. Therefore, analyzing the different frequencies of light emitted in fluorescent spectroscopy, along with their relative intensities, makes it possible to ensure food contains particular fluorescent compounds e.g., tryptophan, heterocyclic aromatic amines in meat^{93, 94}.

Front face fluorescence is always used for food samples, as they are opaque. As the species excited depend on the excitation wavelength, it is worthwhile noting that fluorescence is a selective method. There are some important wavelengths for intrinsic fluorescence spectra of compounds in food, such as aromatic-amino-acids, nucleic-acids (excitation: 250 nm, emission: 280-480 nm), tryptophan residues (excitation: 290 nm, emission: 305-400 nm) of proteins and NADH (excitation: 336 nm, emission: 360-600 nm). These intrinsic fluorescence spectra can be considered as fingerprints of food⁹⁴. Karoui and Blecker (2011) provided an overview of fluorescence spectroscopy measurement for the quality assessment of food systems⁹³. The application of fluorescence spectra has been successfully investigated for the quality of animal (i.e., dairy^{95, 96}, meat^{94, 97}, fish^{48, 98, 99}, and egg¹⁰⁰) and vegetable (oils¹⁰¹, cereal¹⁰², sugar¹⁰³, fruit and vegetable^{96, 104-106}) products as well as the identification of bacteria^{95, 107, 108} of agro-alimentary interest.

However, foods are complex products containing numerous fluorescent compounds. In such cases the signals of the different chromophores may overlap, and it becomes more complicated for food assurance.

Hyperspectral imaging and multispectral imaging

Spectral imaging (i.e., hyperspectral and multispectral) has the capability to rapidly and non-

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

invasively monitor both physical and morphological characteristics and intrinsic chemical and molecular information of a food product for the purpose of assurance. During the last decade, spectral imaging has developed rapidly as a better tool for safety and quality inspection of various foods as it integrates conventional imaging and spectroscopy to attain both spatial and spectral information from an object^{109, 110}. Hyperspectral images are usually used as fundamental datasets from which to determine optimal wavebands that can be used by a multispectral imaging solution for a particular application¹¹¹. Systems within 400-1000 nm were mainly used for fruit and vegetables, because they are generally cheaper than those within 900-1700 nm and are less influenced by water^{112, 113}.

Combining different image acquisition methods (e.g., reflectance/transmittance and reflectance/fluorescence) can give hyperspectral/ multispectral imaging systems more inspection capabilities than systems that use only a single imaging mode¹¹⁴. Such image acquisition combinations along with data fusion techniques are likely to expand in the future for building multitask food inspection systems. There are many recent published reviews dealing with the application of Vis/NIR hyperspectral/ multispectral imaging for classification and grading^{115, 116}, defect¹¹⁷⁻¹¹⁹ and disease¹²⁰ detection, distribution visualization of chemical attributes^{121, 122}, and for inspection of meat^{123, 124}, fruit^{110, 125, 126} and vegetable^{110, 127, 128}, fish^{129, 130} and et al.

Raman spectroscopy

Raman spectroscopy can obtain detailed chemical information on a sample without the need for labeling and almost insensitive to water. It is also a non-invasive technique that yields reliable results for solid and liquid multicomponent food samples¹³¹. In a typical Raman analysis of food, the fingerprint of Raman spectra information can be used to identify a molecule of interest in complex food matrix as the assignment of Raman-scattering bands to corresponding vibrational modes of molecules is integral^{132, 133}. In addition, the changes in chemical composition or molecular structure of food can be monitored by intensity of frequency shifts of specific vibrational modes. Raman spectroscopy has a high potential in food assurance.

Raman spectroscopy has good application prospects in food quality for its spectra are not extremely sensitive to polar materials such as water^{131 134}. Raman spectroscopy for the study of molecular vibrations and structure of the chemical composition of heterogeneous foods and food

Analyst Accepted Manuscript

ingredients may be combined with FT-IR ¹³⁵. Raman spectroscopy has been successfully applied for characterizing olives ¹³⁶, juices ¹³⁷, fruits ¹³⁸, and analyzing wax ¹³⁹, fatty acid ¹⁴⁰, protein ¹⁴¹ et al in food, and investigating structural and texture ¹⁴² information of food. Raman spectroscopy is an advanced technique that enhances the vibrational spectrum of molecules adsorbed on or in the vicinity of metal particles and/or surfaces.

Summary of optical techniques

Optical techniques are applied over a wide range of length scales, from planetary to microscopic and are of many types. Optical radiations propagate well in the air, optical spectroscopy can be used without contact. The interaction between the optical radiation and the sample under test can be assessed by measuring either the reflected, transmitted, scattered or diffused light, or several of these parameters. Optical instrumentation may be quite inexpensive and easy to miniaturize allowing the development of portable devices suitable for industrial applications. Optical spectroscopy is rapid, ease to use, versatile and inexpensive; it is one of the most powerful analytical techniques among the non-destructive measuring techniques. For these reasons optical techniques have become the most widespread non-destructive measuring techniques for food reassurance, such as meat, vegetable, fruit and food productions. The typical detection results of optical techniques are shown in Fig. 4 taking meat as an example (adapted from the literature ¹⁴³⁻¹⁴⁷).

Fig. 4. ¹⁴³⁻¹⁴⁷

Acoustical techniques

Quality and acceptability of food products are often assessed based on the sounds produced during crushing or biting of the food ¹⁴⁸. At present instrumental acoustic methods (especially low power ultrasound) are becoming more and more popular for the investigation of food product properties because they are relatively cheap, simple and energy saving. Sound is transmitted through a food product to obtain the acoustic characteristics of the product used for food assurance. Some crisp food may be considered unacceptable and of poor quality for example when little sound is produced during breakage ¹⁴⁹. Acoustic Envelope Detector for crispness assessment of biscuits ¹⁵⁰. Crispness assessment of roasted almonds by an integrated approach to texture

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

description: texture, acoustics, sensory and structure ¹⁵¹. It is also used for monitoring the composition and physicochemical properties of food components and products during processing and storage, which is crucial for controlling the food properties and improving its quality.

From Fig. 5, by selecting the appropriate frequency range, sound can be utilized in many industrial applications including food ¹⁵². Sound propagates through food materials as mechanical waves causing alternating compressions and decompressions ¹⁵³. These sound waves have characteristic wavelength, velocity, frequency, pressure and period. The interaction of sound waves with matter alters both the velocity and attenuation of the sound waves via absorption and/or scattering mechanisms ¹⁵⁴.

Fig. 5.

For acoustic techniques, there are main four measurements instruments, microphone measurement technique, pulse-echo ultrasound technique, pitch and catch technique, and resonance techniques as shown in Fig. 6.

Fig. 6.

Acoustical techniques have been utilized for non-invasive analysis and monitoring of fresh vegetables and fruits in both pre- and postharvest, cheese during processing, commercial cooking oils, bread and cereal products, bulk and emulsified fat based food products, raw and fermented meat products, fish and poultry, food gels, aerated and frozen foods. Other applications include the detection of honey adulteration and assessment of the aggregation state, size and type of protein ¹⁵⁵.

Scanning acoustic microscopy and ultrasound imaging are the two main acoustic imaging techniques to form images of detection objects. In a scanning acoustic microscope a focused ultrasound beam is coupled into the sample and the returning back scattered signal analyzed in a variety of ways, including simple pulse echo ^{156, 157}. Ultrasonic imaging (ultrasonography) is a medical technology that has long been used as a diagnostic technique. The same probe that transmits the pulse listens for scattered waves to produce echo signals that are processed to form images. This technique has found several applications in food technology, such as the pulse-echo ultrasound has been used to detect defects in food packaging seals using ¹⁵⁶. Recently an airborne ultrasound technique has been used in food quality detection.

Electrical techniques

The interest in electrical characteristics of food materials has been associated with non-destructive measuring techniques for many years¹⁵⁸. As simple, rapid and non-destructive measuring techniques, dielectric properties used in the detection of processing condition or the quality of food. This technique is especially useful for detecting moisture content in foods as permittivity and moisture can be closely correlated when water content is high. In microwave thawing, it is very sensitive to the rates and uniformity of heating in partially frozen food material¹⁵⁹. The measurement is rapid and it does not destroy the substance; it is therefore suitable for on-line assurance of food quality^{94, 160}.

By using two electrodes to induce a current flow (I) and a voltage (V) between these two electrodes, it possible to deduce an electrical impedance by applying Ohm's law, $V = ZI$. This is the most elementary and commonly used method and apparatus for detect food quality. The impedance (Z) is a complex function of alternating current frequency f , e.g. $Z = Z_{\text{real}} + iZ_{\text{imag}}$, where Z_{real} is the real part (resistive), Z_{imag} the imaginary part (capacitive) and $i = (-1)^{1/2}$ ⁹⁴.

As most of food tissue is biomass, when an electric current passes through food tissue, it passes through the extracellular fluid (ECF) or through both the ECF and intracellular fluid (ICF) compartments¹⁶¹. The current pathway is generally represented as two parallel branches: one through the ECF and the other through the capacitive membrane and the ICF compartment. The extracellular pathway is considered to be purely resistive, whereas the intracellular pathway including the capacitive effect of the cell membrane is an impedance (i.e. complex), with a resistive part (real) and a capacitive part (imaginary), resulting in the magnitude of the intracellular impedance being frequency dependent¹⁶².

Conductivity plays a fundamental role in food assurance measurements¹⁶³⁻¹⁶⁷. The conductivity of a food is generally measured by passing a known current at constant voltage through a known volume of the material and by determining resistance. The electrical conductivity of foods has been found to increase linearly with temperature, and water/ionic content.

Electrical permittivity is another parameter which can be used to characterize the dielectric property of food. It depends on dielectric constant ϵ' , which is related to capacitance of a substance and its ability to store electrical energy, and the dielectric loss factor ϵ'' , related to

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

energy losses when the food is subjected to an alternating electrical field i.e., dielectric relaxation and ionic conduction ¹⁶⁸. The permittivity can be related to chemical composition, physical structure, frequency, and temperature, with moisture content being the dominant factor ¹⁶⁹. The ratio of dielectric loss factor to dielectric constant (ϵ''/ϵ') is called the loss tangent ($\tan\delta$) or dissipation factor, a descriptive dielectric parameter ¹⁶⁹.

Various factors influence the dielectric properties of food materials such as frequency of the applied alternating electric field, moisture content, bulk density, temperature ^{94, 159}. At constant temperatures, dielectric constant (ϵ') and loss factor (ϵ'') of food materials increase with decreasing frequency. The penetration depth (PD) decreased with increasing frequency, temperature and moisture content ^{159, 169}. At higher microwave frequencies only salty foods show an increase in ϵ'' with temperature but at lower microwave frequencies there is a general increase in ϵ'' ¹⁶⁹. Both ϵ' & ϵ'' of various foods increased with increasing moisture content. For fruits and vegetables ^{170, 171}, ϵ' increases with temperature, whereas ϵ'' increased with increasing temperature and ϵ' increased with temperature at lower frequencies, but decreased with temperature at the higher frequencies. For beef or meat ¹⁷², both ϵ' & ϵ'' increases with decreasing frequency at constant temperature; however, ϵ' decreases and ϵ'' increases with increasing temperature at constant frequency. For fish, a sharp increase in dielectric properties was observed around the freezing point ¹⁷³. Both ϵ' & ϵ'' increased with increased water content at constant temperature; ϵ' & ϵ'' of lean tuna were larger than those of fatty tuna. ϵ' of marinated catfish and shrimp, generally decreased with increasing temperature whereas ϵ'' increased with temperature. Both ϵ' & ϵ'' of fish meal increased non-linearly with moisture content and also increased with temperature in a relatively linear manner ¹⁷⁴⁻¹⁷⁶.

The interest in dielectric and electric properties of food materials has historically been associated with the design of electrical equipment. As shown in Fig. 7 (a), the simple detection devices only need a low frequency generator, a couple of electrodes and a view meter. It is a convenient method for evaluating food quality, especially for detecting moisture content in foods. However, in this bipolar system, electrode polarization can produce a systematic error in the voltage measured between the two electrodes caused by parasitic capacitive impedances occurring at the interface of the two electrode-sample ohmic contacts ¹⁶⁸. To eliminate this electrode-sample

contact effect, a tetrapolar measurement method can be deployed using two injection electrodes in which voltage is measured via two separate measurement electrodes. Another way is to use several aligned, regularly spaced electrodes and take bipolar measurements between each pair of electrodes. To avoid dispersion in measurement caused by influencing factors (such as temperature), normalized methods, such as ratio of impedances at two frequencies (1 kHz/100 kHz), index of anisotropy, et al, are frequently used. Fig. 7 (b) shows a circular multi-electrode sensors based on anisotropy index methods which was successfully used in meat aging detection¹⁶⁴. S. N. Jha et al¹⁵⁹ has given a detail review which covers theoretical aspects of different electrical properties, their measurement techniques, applications of dielectric properties in agriculture/food processing sector for quality and safety assessment in food processing. Electrical and dielectric apparatus has been applied for determination of various characteristics of food such as frost sensitivity, chilling and freezing tolerance, moisture content, seed germination, mechanical stress, pasteurization and other properties of grains, seeds, meat, sugar, milk, wood, soil, fruit and vegetable, infected food (moisture content, maturity of fruit, freshness of eggs, potential insect control in seeds, radio frequency heating)^{94, 161, 162, 165, 166, 176-182}.

Fig. 7.

X-ray techniques

As shown in Fig.8, the wavelengths of X-radiation (composed of X-rays) are shorter than those of UV rays and longer than those of gamma rays. X-rays have a wavelength in the range of 0.01 to 10 nanometers, corresponding to frequencies in the range 30 petahertz to 30 exahertz and energies in the range 100 eV to 100 keV. X-rays with photon energies above 5-10 keV (below 0.2-0.1 nm wavelength) are called hard X-rays, while those with lower energy are called soft X-rays^{183, 184}.

Fig. 8.¹⁸⁶

Since Röntgen discovered them in 1895, X-rays are widely used to image the inside of objects by using their penetrating ability¹⁸⁵. FDA (US Food and Drug Administration) recommend that the maximum dose permitted for irradiation of spice is 30 kGy. Different applications use different parts of the X-ray spectrum are shown in Fig.8. Food applications mainly use soft X-rays.

X-rays that are elastically or inelastically scattered from a sample provide valuable

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

information about the internal characteristics of a sample such as the molecular structure, density and atomic number ^{187, 188}. There are four techniques for quality and safety control of food based on X-rays. Firstly, the transmission imaging measurement, such as 2-dimensional radiography well-known from medicine or the line scan method producing images when the product passes through a vertical plane of X-rays used for foreign bodies detection in food ^{183, 189-191}. Secondly, X-ray microtomography for microstructural measurement ¹⁹²⁻¹⁹⁴; Thirdly, X-ray fluorescence spectroscopy measurement, such as X-ray fluorescence spectra for determination of trace elements in food ¹⁹⁵⁻¹⁹⁸; and fourthly, small angle measurement for the structure analysis of food component, such as the structure of proteins, allergens, starches, and et al ¹⁹⁹⁻²⁰³. Among these four techniques, X-ray transmission imaging measurement techniques are widely used in the food industry.

Conventional X-ray transmission imaging measurement technique as shown in Fig. 9 (a) has long been used for online detection of foreign bodies in food products relying on the absorption contrast between the foreign body and food product. As X-rays penetrates a food product, it loses some of its energy. A dense area, such as contaminant, will reduce the energy even further. As the X-rays exits the product, it then reaches a sensor. The sensor then converts the energy signal into an image of the interior of the food product ²⁰⁴. Foreign matter appears as a darker shade of grey that helps to identify foreign contaminants. The X-rays transmission inspection system, as shown in Fig. 9 (b), (c), mainly comprises a computer-controlled X-ray generator (i.e. X-ray source tube), a line-scanning sensor for X-ray detection, conveying belt, stepping motor, image-acquisition card and computer.

Fig. 9. ¹⁸⁵.

Foreign bodies are a major reason for consumer complaints in the food industry. The application of good manufacturing practice and hazard analysis throughout the whole food supply chain is the most effective way to prevent and reduce contamination and thereby protect consumers. X-rays have strong penetration ability, so the image can directly reflect internal defects of food and agriculture products, and structural organization changes in quality. X-ray transmission imaging measurement techniques have great potential in detecting the internal quality of animal products, and has been widely used in the food industry for the inspection of food quality and safety.

For the meat industry, the principle of operation of X-ray measurement systems is that various components of muscle-lean meat, fat, and bone have different properties when exposed to physical energy from X-rays. The relative density is the critical property, as lean tissue has a consistent density of 1.07 to 1.08, whereas fat varies depending on the temperature. Skin has a similar density to lean meat, which means that collagen measurement is hardly possible. As materials attenuate X-rays depending on their energy, use can be made of the selective attenuation of one, two, or more energy levels; that is, mono, dual (DEXA), or multiple energy X-ray absorptiometry (MEXA) ²⁰⁵⁻²⁰⁷. Some internal disorders with negative effects on quality that should be detectable by X-ray techniques include cork spot, bitter pit, water core, and brown core for apple, blossom and decline, membranous stain, black rot, seed germination, and freeze damage for citrus, and hollow heart, bruises, and perhaps black heart for potato ^{56, 191, 208, 209}, where the aim is to analyze internal elements that are undetectable to the naked eye. Because the method is primarily dependent on the density of the tissue, not the chemical composition, the selectivity is limited. X-rays have not yet been used to their fullest potential in a range of application areas, especially the agricultural and food industries. Zwiggelaar, Reyer, et al. ¹⁸³ applied X-rays imaging to detection of perspex, a soft plastic, and cellulose in a water environment as a simulation approach in food and agricultural products. They also indicated possible applications of these techniques within the agricultural and food industries, such as foreign-body detection, quality control and food processing ¹⁸³. McFarlane, N. J. B., et al examined constraints on foreign body detection in food by using Compton scattered X-rays. The detection of a 4 mm glass fragment in water, instant coffee and muesli using Compton scatter was demonstrated by experiment ²¹⁰. Mery, Domingo, et al developed an X-ray machine vision approach to automatically detect fish bones in fish fillets (Fig. 9 (d)) ¹⁸⁵. Nielsen, Mikkel Schou, et al ¹⁸⁹ present a novel approach for detection of organic foreign bodies such as paper and insects in two food products using X-ray dark-field imaging with a grating interferometer.

Nuclear magnetic resonance (NMR) and magnetic resonance imaging (MRI)

Nuclear magnetic resonance (NMR)

NMR is based on the emission and absorption of energy in the radiofrequency range of the electromagnetic spectrum ²¹¹. All nuclei that contain odd numbers of protons or neutrons can be

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

observed with NMR. Nuclear magnetic resonance techniques have been used for examining agricultural products from the biological and physiological points of view since the mid-1950s; however small sample sizes and slow data processing have limited the usefulness of these studies in terms of in-line sorting. With the development of large magnets for medical applications, a variety of new types of magnets and radio frequency coils have become available for use in engineering applications of NMR ²¹². The most commonly measured nuclei are ¹H and ¹³C, although nuclei from the isotopes of many other elements can be observed (²³Na, ³¹P, etc.). NMR is sensitive to the existence of mobile water, oil, and sugar, which are major components of agricultural materials. Therefore, owing to its non-invasive nature, NMR has a high potential for use in internal-quality evaluation of agricultural products whenever a component of the product contains an NMR sensitive nuclei that is correlated with quality. NMR spectra can also be considered as a type of a fingerprint for a product that carries qualitative and quantitative information on the composition ²¹¹.

(1) ¹H NMR is a better spectroscopic method for assessing water holding capacity (WHC), intra muscular fat (IMF) and total water content in porcine muscles than visual, fluorescent and near infrared (NIR) reflectance spectrophotometry. As water protons are easily visible with ¹H NMR, this technique is obviously especially useful for studying water in food products. The parameters linked to vegetable, fruit, meat and fish products are numerous: water content, WHC, water distribution (i.e. water state) ²¹³, water mobility, etc. In additional, ¹H NMR can identify variations in water-protein interactions and then in protein states, so it is a potential tool for studying structure. It has been shown that NMR parameters are highly sensitive to differences in the muscle structure of farmed and wild cod and to the effect of brine injection, brining, and rigor tension on the muscle.

(2) ³¹P NMR is mainly applied to post mortem evaluation in meat and fish muscle. ³¹P NMR is used in the prediction of fish freshness, of WHC in rabbit muscle, in association with ¹H MAS and NMR ²¹⁴.

(3) ¹³C NMR spectroscopy has been successfully used for detection of sugars and acids and that ¹³C resonances of amino acids can be used as fingerprint for the monitoring of wines. Proton and ¹³C NMR data have been used for the differentiation of white wines coming from three

German regions^{211, 214, 215}.

(4) ²³Na NMR is performed to quantify salt content in meat and fish products. For instance, in association with ²³Na MRI, it is a rapid and reliable alternative for optimizing and understanding industrial salting processes in the fish industry²¹⁶.

Magnetic resonance imaging (MRI)

Similarity to the NMR, MRI is also a nondestructive, nonintrusive spectroscopic technique based on the interaction of electromagnetic radiation in the radiofrequency range with matter. MRI is particularly suitable for biological materials (given that protons are abundant therein), mainly in water, but also in fat, oil, or salt, and it allows one to distinguish these components²¹⁷. Furthermore, MRI is sensitive to several quality parameters affecting the produce, particularly those that affect the water concentration or mobility (e.g., internal browning).

MRI has been used successfully in the past to measure several quality parameters of fresh fruit and vegetables, including the presence of internal defects, such as chilling injury in microtom tomato²¹⁸, watercore development in apples²¹⁹, postharvest ripening of tomato²²⁰, microporosity in fruit²¹¹. MRI has also been used to measure physical properties, such as size, shape and volume, and has been correlated with firmness, soluble solids, or acid content²²¹⁻²²³. MRI has been also used successfully to measure several quality parameters of meat and meat products. An original experimental approach has been developed based on the quantitative, local, dynamic and in situ analysis deformation and water content of chicken during cooking²²⁴. MRI has been used to detect the water distribution²²⁵, viscoelastic properties²²⁶ and muscle structure²²⁷ in meat.

Compared to other techniques such as X-ray imaging, MRI image acquisition speed is relatively low, and is strongly determined by the required image quality and whether 1D or 2D imaging is performed²¹². In Fig. 10 CT and MRI images of a healthy apple and one with severe water core symptoms—a disorder characterized by water-soaked regions in the fruit—are compared. The affected regions are clearly visible in both images, although the imaging principle is very different: In CT, the contrast between healthy and affected tissue is due to the increased density in the latter due to the water soaking; in MRI, the affected area lights up because the water mobility is very different from that of healthy tissue. MRI shows large potential for online grading,

sorting, or quality evaluation of fresh produce²¹².

Fig. 10.²¹⁷.

Microwaves and terahertz waves

Microwaves

In North America, only four microwave and three radio frequencies are permitted by the Federal Communications Commission (FCC) for dielectric heating applications (Decareau, 1985). The allotted microwave frequencies are 915, 2450, 5800MHz and the radio frequencies are 13.56, 27.12, and 40.68MHz²²⁸. The interest in the dielectric properties of food has been principally for predicting heating rates describing the behaviour of materials. The relevant quality attributes that can be assessed with the structure, composition (particularly water content), water state and water distribution in the product, and particularly water content profiles²²⁹. In the high frequency range the dielectric properties of food are closely correlated with water state and water content. Dielectric relaxation spectroscopy determines the response of the molecular motion of polar molecules in the sample to a weak external alternating electric field²³⁰. As the frequency of the electric field is increased, it reaches a frequency called the relaxation frequency when the polar molecule can no longer rotate with the electric field. Dielectric properties change significantly around this relaxation frequency²³¹.

The rare industrial applications currently using microwave are based either on cavity, antenna or probe measurements. A specific method using transmission-reflection measurements should be highlighted. The basic configuration of this method uses two antennas, one transmitting and one receiving, the meat streaming on a conveyor belt between the two non-contacting antennas²³². Applications of microwave sensors in other sectors of the food industry could be adapted for the meat industry, particularly for measuring water content. Work has been carried out over the last two decades by the US Department of Agriculture on water content, water state and density of grain and seed²³³, and meat²³¹.

Terahertz

Terahertz (THz) radiation, or THz wave, is an electromagnetic wave whose frequency lies between mid-infrared and microwave radiation. Unlike X-rays, terahertz waves are not harmful, so there are no exposure worries for practitioners or patients. Moreover, THz waves have the

properties of penetration for various materials, low photon energy, and sub-millimeter spatial resolution. Therefore THz spectroscopy has received considerable attention as a nondestructive inspection method. In particular, this low photon energy method is suitable for food inspection with active substances^{234, 235}. Due to the high absorbance of THz radiation by water, the most widespread application of THz spectroscopy would seem to be for quantification of total moisture content in foods.²³⁶ At the same time, THz radiation interacts only very weakly with materials composed of non-polar molecules, such as plastics and ceramics and is reflected by most metals^{236, 237}. This indicates the THz technology has the potential for detection of some foreign material in food²³⁸. A transmission continuous-wave (CW) THz imaging system using reflecting mirrors is illustrated schematically in Fig. 11²³⁹.

Fig. 11.²³⁹

One demonstration of THz imaging for foreign body detection in foods has been reported, for the detection of contaminants in chocolate. Due to its high fat and low moisture content, chocolate is relatively transparent to THz energy. When foreign objects, such as glass or plastic, are placed in chocolate, they alter the scattering profile of a transmitted THz wave and are thus detectable. Foreign bodies (glass, stone and metal) were concealed within the interior of a bar of chocolate and THz images of the contaminated sample were obtained using a raster scanning Thz-TDS system operating in transmission mode. It was possible to identify foreign bodies in the chocolate sample, both in the presence and absence of its plastic foil packaging²³⁶. THz-TDS in transmission mode was used for the characterization of the dielectric properties of oil-water complexes with water content ranging from 0.43 to 3.28%. This enabled determination of the absorption coefficient and refractive index of the samples, and thus determination of the amount and structure of water in these complexes. The results indicated the formation of a hydrogen bonded oil--water complex, rather than dissolved water clusters in the oil-water complexes. The developed system was employed for simultaneous determination of the sugar and alcohol content of commercial alcoholic beverages independent of other properties such as colour, organic matter content, carbonation and flavor²⁴⁰. Common packaging materials made from cardboard and polymers are transparent to THz radiation. This makes THz spectroscopy and imaging attractive tools for quality validation of packaged products²⁴¹. THz spectroscopy may also be used to detect

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

pesticide in food powders (sticky rice, sweet potato, and lotus root)²⁴², antibiotic in milk²⁴² and egg powder²⁴³, the characteristic optical properties in vegetable oil (sunflower, peanut, soybean and rapeseed oil)²⁴⁴,

Although THz waves are useful for food inspection, a few researchers have reported many drawbacks²⁴⁵. One of the limitations of THz spectroscopy for moisture content detection is that it is not suitable for high moisture products of thickness greater than 1 mm. This is due to the high absorption of THz radiation by water. Another challenge facing practitioners of THz spectroscopy is the effect of physical variations in a sample (e.g. particle size) on the refractive index of a material. This is particularly pertinent in the case of quality monitoring of fresh produce which shows high variability in this respect. Scattering effects may adversely affect measurements of THz absorption in certain materials. When the grain size of solids is comparable to the THz wavelength, extinction spectra are severely influenced by scattering losses.

Biosensors techniques

Electronic nose and electronic tongues

The electronic nose (e-nose) was developed in order to mimic human olfaction that functions as a non-separative mechanism: i.e. an odor (Fig. 12). An odor stimulus generates a characteristic fingerprint (or smell-print) from the sensor array. The sensor array consists of broadly tuned (non-specific) sensors made of a variety of odor-sensitive biological or chemical materials. The patterns or fingerprints are used to construct a database and train a pattern recognition system so that unknown odors can subsequently be classified and identified. The detection system of e-noses usually consists of an array of chemical gas sensors or biosensors (i.e., sensors that incorporate a biological sensing element). For chemical gas sensors, a variety of different sensor types have been developed, in which three types of materials are commonly used: metal oxides semiconductors (MOS)²⁴⁶, conducting polymers composites and intrinsically conducting polymers. Recently, new technologies such as optical sensors²⁴⁷, gas sensitive field effect transistors²⁴⁸ and quartz microbalance (QMB) sensors²⁴⁹ and ion mobility spectrometry (IMS)²⁵⁰ have entered this field.

Fig. 12.⁴¹

Similarly to an e-nose, electronic tongues (e-tongues) can be also considered as analytical

instruments which simulate the human senses. The e-tongue devices are composed of a sensor array coupled to chemometric processing used to characterize complex liquid samples. Although the e-tongues works in liquid media, such as the biological tongue, the sensitivity of the artificial system can be much higher, and its capabilities much wider; this makes the performance of the e-tongues closer to that of the olfactory system. In fact, the e-tongues can be thought of as an analogue to both olfaction and taste senses and can recognize the flavour of liquid or liquefied products. The e-tongue can also be used for quantitative detection of a variety of dissolved compounds, including volatile substances that are responsible for odours but originate from either the liquid or solid phases.

E-nose and e-tongue are composed of three elements: (i) sampler component, (ii) array of chemical sensors with different selectivity, and (iii) software with the appropriate algorithm to process the signal and get the results ²⁵¹. Another common feature of all e-nose and e-tongues systems is, therefore, the utilization of an array of nonspecific sensors together with data processing by pattern recognition methods. Once the data from the individual sensors from the array is collected, the e-nose systems require a suitable post processing procedure to analyze and classify the data. Pre-processing of multivariate signals in sensor arrays represents an essential part of the measuring system. Again, similar to biology, one of the most often used data-processing methods is an artificial neural network (ANN) the algorithms of which are based on modelling of learning and recognition processes in the human brain ²⁵². Other data processing techniques such as principal component analysis (PCA), linear discriminate analysis (LDA), partial least squares (PLS), functional discriminate analysis (FDA), cluster analysis (CA), fuzzy logic are also widely used for processing of the data from multi-sensor systems. Among these techniques, PCA, PLS, LDA, FDA and CA are based on a linear approach while fuzzy logic, ANN and PNN are regarded as nonlinear methods ^{251, 253}.

The strengths of both the electronic nose and tongue include high sensitivity and the fact that they are easy to build, cost-effective and provide a short analysis time. Therefore, these devices are becoming more and more popular as objective automated non-destructive techniques to classify and recognize of a large variety of foods, such as meats ^{254, 255}, vegetable ²⁵⁶, fishes ^{257, 258}, juice ^{259, 260}, beverages ²⁶¹, oil ²⁶² and wines ²⁶³.

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Colorimetric sensor array

E-nose systems have a distinct advantage over most other gas detection technologies as it allows non-destructive method to detect odour. However, it also has a number of disadvantages, including poor detection sensitivity at low compound concentration relative to their vapor pressure and poor discrimination between compounds; the latter proves especially problematic in interference from the large environmental changes in humidity and acidity. Recently, a new artificial olfaction technology based on a colorimetric sensor array is used for odours and volatile organic compounds (VOCs). This colorimetric sensor array comprises thin films of chemically responsive dyes on porous membranes. The array of multiple dyes, whose colors change according to the full range of intermolecular interactions, provides enormous discriminatory power among odorants in a simple device that can be easily digitally imaged. The chemically responsive dyes are usually Porphyrins, metallo-porphyrins, phthalocyanine and pH indicator.

Normal electronic nose systems generally allow for distinction between analytes of different chemical functionality, the discrimination of compounds within similar chemical compounds remains a challenging goal. Previous array technologies for such electronic noses generally rely on multiple, cross-reactive sensors based primarily on changes in properties (e.g., mass, volume, conductivity) of some set of polymers or on electrochemical oxidations at a set of heated metal oxides. Specific examples include conductive polymers and polymer composites, polymers impregnated with a solvatochromic dye or fluorophore, mixed metal oxide sensors, and polymer-coated surface acoustic wave devices. For the colorimetric sensor array, it relies on bond formation, acid-base interactions, hydrogen-bonding, dipolar and multipolar interactions, p-p molecular complexation, van der Waals and physical adsorption interactions between sensor and analyte. This is believed to be a fundamental flaw in the development of chemical sensors with both high sensitivity and high selectivity^{264, 265}.

A colorimetric sensor array system is depicted in Fig. 13. Gas streams (N₂) containing the vapors of interests were generated by flowing nitrogen through the sample chamber in a thermostated, glass-fritted bubbler. Digital mass-flow controllers were utilized to control nitrogen flow speed. The ‘before’ image was first acquired on the flatbed scanner; an array was then exposed to a flowing stream of N₂ containing the analytes of interest, and the array was then scanned again

after equilibration. Experiments were run until full equilibration was demonstrated by comparison of repeated scans. The response of the array is mass transport limited; interaction times (ligation, proton transfer, etc.) are much faster than the typically observed array response. Under proper conditions of rapid gas flow, equilibration of the array occurs within 2 min, even at ppmv analyte concentrations; under static diffusion conditions, equilibration (especially with low volatility analytes) can take 1 hour more, depending of course on the specific cell configuration. Color-difference maps were obtained from the scanned RGB images by digitally subtracting the image before exposure to analytes from the image after exposure, using a 314-pixel average from the center of each pigment spot (thus avoiding subtraction artifacts at the periphery of the spots) as follows (Fig.13)²⁶⁶.

$$\Delta R = |R_a - R_b| \quad (1)$$

$$\Delta G = |G_a - G_b| \quad (2)$$

$$\Delta B = |B_a - B_b| \quad (3)$$

Here, *a* represent after, *b* represent before. ΔR , ΔG , ΔB are the color-difference.

Fig. 13.

This colorimetric sensor array is not sensitive to humidity and temperature due to the hydrophobicity of the sensor materials and sensors plate^{264, 267}. It is superior to traditional MOX gas sensor techniques in the analysis of solid and liquid samples aroma. Therefore, the colorimetric sensor array can act as a fingerprint for food assurance. Usually, advanced chemometric techniques are needed to extract information from these color-difference maps. The colorimetric sensor array has been used successfully to detect many foods such as evaluation of meat^{268, 269} and fish freshness^{257, 270, 271}, discrimination of wine^{272, 273}, vinegar²⁷⁴⁻²⁷⁶, coffee²⁷⁷, sugar²⁷⁸ and tea^{279, 280}.

The previous sections have described sensing odours using an artificial olfaction but this is a significant technical challenge. In recent years, instead of attempting to reproduce human odor impression, most commercially available instruments have other application areas. Table 1 gives an overview of electronic noses on the market according to the criteria above, listing their manufacturers and technology basis²⁸¹.

Table 1. Commercially Available Electronic Noses (adapt from Röck, Barsan, and Weimar²⁸¹)

manufacturer	no. of systems sold	model	technology
Agilent, http://www.chem.agilent.com/		4440A	quadrupole fingerprint mass spectrometry
AIRSENSE Analytics, http://www.airsense.com/	180	i-PEN	gas sensor array
		PEN3	gas sensor array
Alpha MOS, http://www.alpha-mos.com/	500	GDA 2	IMS, PID, EC, 2 MOX sensors
		FOX 2000	6 MOX sensors (or QMB/CP)
		FOX 3000	12 MOX sensors (or QMB/CP)
		FOX 4000	18 MOX sensors (or QMB/CP)
		Gemini	gas sensor array
		Kronos	quadrupole fingerprint mass spectrometry
		Heracles	2 capillary columns (1-3 m) and 2 FIDs
		RQ Box	EC, PID, MOX sensors
AltraSens, http://www.altrasens.de/	>100 000	Prometheus	MS and 18 MOX sensors
AppliedSensor, http://www.appliedsensor.com/		OdourVector	6 sensors
Chemsensing, http://www.chemsensing.com/		Air Quality Module	2 MOX sensors
CSIRO, http://www.csiro.au/			colorimetric array
Dr. Foedisch AG, http://www.foedisch.de/		Cybernose	receptor-based array
		OMD 98	2×6 sensors
		OMD 1.10	2×5 MOX sensors
Draeger, http://www.draeger-safety.com/		Multi-IMS	ion mobility spectrometry
		MSI150 Pro2i	ECs
Electronic Sensor Technology, http://www.estcal.com/		ZNose 4200	GC and SAW
		ZNose 4300	GC and SAW
		ZNose 7100	GC and SAW
EnviroNics, http://www.environics.fi/	9000	M90-D1-C	ion mobility spectrometry
Forschungszentrum Karlsruhe, http://www.fzk.de/		ChemPro100	ion mobility spectrometry
Gerstel GmbH & Co. KG, http://www.gerstel.com/		SAGAS	8 SAW sensors
GSG Mess- und Analysengeräte, http://www.gsg-analytical.com/		QCS	3 MOX sensors
Illumina, http://www.illumina.com/		MOSES II	modular gas sensor array
Microsensor Systems Inc., http://microsensorsystems.com/		oNose	fluorescence sensorssbead array
		Hazmatcad	SAW
		Hazmatcad Plus	SAW array and EC
		Fuel Sniffer	SAW
		CW Sentry 3G	SAW and electrochemical sensor array
		SAW MiniCAD mk II	2 SAW array
		VaporLab	GC and EC
Owlstone Nanotech, Inc., http://www.owlstonenanotech.com/		Tourist	field asymmetric ion mass spectrometry
		Lonestar	field asymmetric ion mass spectrometry
Proengin, http://www.proengin.com/		AP2C	flame spectrophotometer
		TIMs detector	flame spectrophotometer
		ChemRAE	ion mobility spectrometry
RaeSystemes, http://www.raesystems.com/		UltraRAE	separation tube and PID

		Eagel monitor AreaRAE monitor	GC and EC PID, 2 ECs, 1 catalytic bead sensor, O ₂ sensor
		IAQRAE	PID, NIRD CO ₂ , EC, polymer-capacitated humidity sensor, thermistor, humidity-temperature sensor
RST-Rostock, http://www.rst-rostock.de/		FF2 GFD1	6 MOX, <i>T</i> , humidity
Sacmi, http://www.sacmi.eu/		EOS 835	6 MOX, <i>T</i> , humidity
Scensive Technologies Ltd., http://www.scensive.com/	<100	EOS Ambiente	gas sensor array
ScenTrak, http://www.cogniscentinc.com/		Bloodhound ST214	gas sensor array
SMart Nose, http://smartnose.com/	250		14 conducting polymers
Smith Group, http://www.smithsdetection.com/		SMart Nose 2000	fluorescent dye quadrupole fingerprint mass spectrometry
		Cyranose 320	gas sensor array
		IONSCAN SENTINEL II CENTURION	ion mobility spectrometry
		GID-2A	ion mobility spectrometry
		GID-3	ion mobility spectrometry
		SABRE 4000	ion mobility spectrometry
		ADP 2000	ion mobility spectrometry
		CAM	ion mobility spectrometry
Sysca AG, http://www.sysca-ag.de/		Artinose	38 MOX sensors
Technobiochip, http://www.technobiochip.com/		LibraNOSE 2.1	8 QCM sensors

Abbreviations: MOX: Metal oxide sensors, CP: conducting polymers sensors, GC: gas chromatography sensors, QCM: quartz crystal microbalance sensors, SAW: surface acoustic wave sensors, PID: Photo ionization detectors, EC: electrochemical conductivity sensors

Integrating non-invasive sensors

Integrating non-invasive sensors from farm to table

There are many factors that influence the quality of food from the farm to table, such as agro-processing, time, handling procedure, environmental conditions and the processes which they undergo. In each of these steps, the quality of food needs to be monitored and controlled. Non-invasive sensors can illuminate these steps and address the important issue of “traceability” in global trade. Sensors may be deployed on satellites, on drones, on robots, on towers and close to the production line as shown in Fig. 14.

Fig. 14.

From space, satellite remote sensing, such as hyperspectral imaging and microwave imaging, can provide key information in near-real time over large areas, such as monitoring climate change impacts on agriculture, monitoring global crop and natural vegetation conditions, guiding the pesticide and irrigation on crops, et al ^{282, 283}. From the air, drone aircrafts with spectrometers, airborne sound sensors, microwave sensors, et al, can used in precision farming in land or

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

greenhouse, that is to adapt the application of input factors (e.g. nitrogen or pesticides) to the current demand of the plant, and adapt management based on the given growing conditions (for example seeding based on soil moisture) ^{284, 285}. For a robot worked in greenhouse and factory or at line, non-invasive sensors are viewed as the “eyes”. The sensors guide the actions of robots. For example, for an unattended function automatic milking systems (AMS) require extensive sensor systems. These are necessary for identifying and monitoring cows, for monitoring technical equipment and for teat location, as well as for assessing the udder and the product quality ²⁸⁶⁻²⁹¹.

A vision of the future

Advances in laboratory instrumentation have made it possible to integrate a variety of sensors for insuring food quality and safety. However, the transfer of the promising, and in many cases proven techniques to industry is taking place at a slow pace. Hence, there are great opportunities for non-invasive sensing to be commercialized. For example an integrating sensor on robots in a greenhouse could be used with:

- Passive acoustic sensors to detect small mammal and insect activity,
- With aid of sensor integration and data processing reposition sensors to accurately locate and correctly identify activity,
- If the activity is a threat, robots ‘herd’ the targets using power ultrasound,
- Once confined to a small area, the targets are then removed. This could remove the need for spraying an entire store or field and provide a faster and economic response to infestation.
- Microwave sensors on towers map mobile water in fields and greenhouses.
- Combining data from many sensors creates “New ways of seeing”.

Conclusions and future trends

This review article covers different non-invasive sensing techniques such as Machine vision, NIR spectroscopy, hyperspectral imaging, Raman spectroscopy, electronic nose, ultrasound, magnetic resonance imaging technique, X-ray, and Terahertz, with their basic concepts & principles and their applications. Table 2 shows the main features of nondestructive techniques for food assurance. The advantages and limitations are also outlined. Non-destructive evaluation techniques provide information on product properties such as discontinuities and separations;

structure; dimensions and metrology; physical and mechanical properties; composition and chemical analysis; stress and dynamic response; signature analysis and et al. As computers become ever more powerful non-invasive sensing techniques in assessment and evaluation of food samples is becoming more popular. All these techniques are complementary, meeting the needs of ever growing consumer expectations and can be considered the tools for a future food industry and market. They can make direct measurements on samples and provide multi-parametric information suitable to be treated online to improve the decision-making of customer.

Table 2.

Understanding the best way to evaluate food samples is of vital importance to the food scientist²⁸². For external attributes such as color, size, and absence of external defects, techniques such as machine visions, spectral imaging, are now widely used on commercial sorting lines. For internal quality attributes, there are also several techniques available, such as spectroscopy, ultrasound, X-ray, and nuclear magnetic resonance. These techniques measure a complex signal that needs to be related to the quality attribute of interest via chemometric techniques. Some techniques such as NIR spectroscopy require frequent recalibration. For flavor of food, the emerging technology of electronic nose and electronic tongue based on the biosensors are also available commercially. The success of techniques for food assurance often depends critically on how their measurement principle mimics the way humans assess a particular property. Future sensor designs would, therefore, preferably be based on biomimetic principles.

From the sensing research viewpoint, the key challenges in the development of non-invasive sensing for food reassurance devices are the improvement of signal-to-noise ratio (SNR) and sensitivity, development of wearable continuous non-invasive systems, evaluation of analytical performance, development of procedures for highly precise food reassurance determination, and reducing the time taken for food reassurance measurement. The signal-to-noise ratio (SNR) and the sensitivity of non-invasive sensing for food reassurance devices can be improved by employing next-generation of transducers and methods that can do the parallel monitoring of multiple parameters. Although all the results presented in this review seem to be very promising, in our opinion these devices are still in an early stage of development, especially biosensors techniques, and much more research has to be carried out in order to implement them in the

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

process production. Major concerns include the lack of intermediate precision studies (i.e. using different operators or instruments) and long term studies, more validation studies and higher number of analyzed samples being required in some cases to extract more reliable conclusions. Scientists are now trying to use sensor technology in every aspect of life so that considerable efforts are given to improve the performance of the non-invasive sensing and reduce the cost of production. Other practical issues such as sensor surface contamination, drift of responses and calibration stability have also to be addressed. It is also very important to develop portable and wearable instruments, and that involves great reduction in energy requirements and power consumption and makes it desirable to miniaturize equipment.

From the food industry and market viewpoint, firstly, for methods to be useful to the industry, they should be rapid, easy to operate, widely accepted, so that different companies use the same methods and therefore know what the other side in the buyer-seller relationship has been measuring; comparable to and even better than current evaluation methods. All the techniques used in this review are essentially non-invasive. Whether they will become widely accepted by the food industry remains to be seen. The costs of labour and training of assessors are likely to increase and the cost of instrumentation such as the image analysis is set to decrease dramatically. Consumer and governmental pressures for better description of quality and traceability of food products will also increase. Secondly, portable and wearable non-invasive will bring many exciting opportunities for food assurance applications. With the entry of big multinational companies, including food industry (such as Nestle), supermarkets (Tesco), internet companies (Google), and several smaller sensing companies, the nascent field of wearable and portable, non-invasive sensing is expected to grow rapidly, with new innovative devices entering the consumer market in the coming years.

From the technique viewpoint, firstly, for each non-invasive technique, there are still lots of challenges. For example developing time- and space-resolved spectroscopy for more accurate measurements of quality attributes of food than NIR spectroscopy, improving hardware and software so that real-time X-ray tomography and MRI become available for reasonable costs, reducing drift and improving reproducibility of electronic noses with improved sensor designs for aroma measurements, et al. Secondly, a multi-sensor device food assurance with a combination of

instrumental techniques (electronic noses, spectroscopic methods, texture-meters, image analysers, colour meters and devices measuring electrical properties) is a challenging but potentially rewarding problem. This will enable and facilitate comparison and evaluation of the techniques, by minimizing the problem of biological variation and the effect of different handling of the food. The combination (fusion) of outputs of different instrumental techniques has emerged as a means for increasing the reliability of classification or prediction of foodstuff specifications as compared to using a single analytical technique²⁸³.

Finally, integration of radiofrequency identification or Bluetooth devices with non-invasive sensors will enable users to wirelessly transmit data to their cellphone/computer in a more user-friendly fashion. Such real-time monitoring devices will enable a more comprehensive assessment of the food quality. A wide variety of new non-invasive sensing devices are thus expected to be introduced for the food industry and market in the near future.

Table 2 the main features of non-destructive techniques for food assurance.

Class	Technique	Analyte	Speed	Penetration depth*	Cost	Application modes	Disadvantages
Optical techniques	MV	Color, size, shape; surface defects	fast	Surface	Cheap to moderate	Lab, portable, commercial	Low chemical information
	IR/NIR spectroscopy	Component, active ingredients physical attributes	fast	Several mm	moderate	Lab, portable, commercial	Susceptible to moisture, single point, requires training
	UV/UVF	Chemical components, defects, spoilage	fast	Several mm	moderate	Lab, portable, commercial	Influence by lighting and other chemical, , requires training
	Raman	Component, active ingredients, physical attributes	fast	Several mm	high	Lab, portable	Insensitive to polar materials, expensive, requires training
Acoustical techniques	MSI/HSI	Chemical components and distribution, physical attributes	fast	Several mm	Moderate to high	Lab, portable	Large dataset, requires training
	Sound	Internal physical attributes	fast	several cm	Cheap	Lab, portable	
	Ultrasound	Internal physical attributes chemical composition	fast	several cm	moderate	Lab, portable	Limited to acoustics impedance
Nuclear magnetic	NMR/MRI	Internal chemical composition, distributes	slow	several cm.	high	Lab	Expensive equipment
Radiation	Soft X-ray	Internal disorders	Fast	several cm	Moderate	Lab, commercial	
	Dual X-ray	Density, thickness, chemical composition	Fast	several cm	high	Lab	Hazardous, not applicable to bulk flowing products
Electrical techniques	Conductivity	Physical attributes, moisture	Fast	several cm	Cheap	Lab, portable	
	Dielectric properties	Physical structure, chemical composition	Fast	several cm	cheap	Lab, portable	Requires training
	Micro waves	structure, composition (particularly water content)	Fast	Several cm	Cheap	Lab, portable, commercial	
Biosensor	Terahertz	Component, active ingredients physical attributes	Fast	several cm	high	Lab	Susceptible to moisture
	E-nose	Odor composition	Fast	-	moderate	Lab, portable	
	E-tongue	Taste composition	Fast	-	moderate	Lab, portable	Require training
	Colorimetric sensor array	Odor composition	Fast	-	cheap	Lab, portable	Require data base

* : Penetration depth of the techniques for meat

Abbreviations: MV, machine vision; IR/NIR, infrared/near infrared; UV/UVF, ultraviolet and ultraviolet fluorescence; MSI/HIS: multispectral and hyperspectral imaging; NMR/MRI, Nuclear magnetic resonance and Magnetic resonance imaging; E-nose/E-tongue, electronic nose and electronic tongue.

Glossary

ANN: artificial neural network; CA: cluster analysis; CP: conducting polymers sensors; EC: electrochemical conductivity sensors; E-nose/E-tongue: electronic nose and electronic tongue; FDA: functional discriminate analysis; GC: gas chromatography sensors; IR/NIR/MIR: infrared/near infrared; LDA: linear discriminate analysis; MOX: Metal oxide sensors; MSI/HIS: multispectral and hyperspectral imaging; MV: machine vision; NMR/MRI: Nuclear magnetic resonance and magnetic resonance imaging; PCA: principal component analysis; PID: Photo ionization detectors; PLS: partial least squares; QCM: quartz crystal microbalance sensors; SAW: surface acoustic wave sensors; SERS: Surface enhanced Raman Spectroscopy; UV/UVF: ultraviolet and ultraviolet fluorescence; NIV: non-invasive; THz: Terahertz.

Acknowledgements

The authors gratefully acknowledge the financial support provided by the national science and technology support program (2015BAD17B04, 2015BAD19B03), the national natural science foundation of China (Grant No.61301239), the natural science foundation of Jiangsu province (BK20130505).

References

1. I. Castanheira, M. Roe, S. Westenbrink, J. Ireland, A. Møller, S. Salvini, H. Beernaert, M. Oseredczuk and M. A. Calhau, *Food Chemistry*, 2009, 113, 776-780.
2. L. Bai, C. Ma, S. Gong and Y. Yang, *Food Control*, 2007, 18, 480-484.
3. C. Morris and C. Young, *Journal of Rural Studies*, 2000, 16, 103-115.
4. P. Karipidis, K. Athanassiadis, S. Aggelopoulos and E. Giompliakis, *Food Control*, 2009, 20, 93-98.
5. M. Farrell-Evans and W. Warren, in *Encyclopedia of Food Safety*, ed. Y. Motarjemi, Academic Press, Waltham, 2014, pp. 293-300.
6. J. Trienekens and P. Zuurbier, *International Journal of Production Economics*, 2008, 113, 107-122.
7. H. Deelstra, D. T. Burns and M. J. Walker, *European Food Research and Technology*, 2014, 239, 725-744.
8. J. Meikle and H. McDonald, *The Guardian (London)*, 2013-1-16.

9. J. Butler, in *Olive Oil Times*, 2013-10-4.

10. Scandal over poisoned wine embitters village in Austria, <http://www.nytimes.com/1985/08/02/world/scandal-over-poisoned-wine-embitters-village-inaustria.html>, (accessed September 1990).

11. J. Macartney, in *The Times (London)*, 2008-9-22.

12. J. Hightower, *Diagnosis Mercury: Money, Politics and Poison*, Island Press, 2008.

13. T. Bawden, in *The Independent*, 2015-4-14.

14. The Food Standards Agency, Post-Chernobyl monitoring and controls survey reports - See more at: <http://www.food.gov.uk/science/research/radiologicalresearch/radiosurv/chernobyl>, 2015.

15. C. Dalvit, M. De Marchi and M. Cassandro, *Meat Science*, 2007, 77, 437–449.

16. J. Kadariya, T. C. Smith and D. Thapaliya, *BioMed Research International*, 2014, 1-9.

17. Wikipedia, 2007 Bernard Matthews H5N1 outbreak, https://en.wikipedia.org/wiki/2007_Bernard_Matthews_H5N1_outbreak, (accessed September 2015).

18. The BSE Inquiry, Animal Health, <http://webarchive.nationalarchives.gov.uk/20060715141954/bseinquiry.gov.uk/>, (accessed August 2015) .

19. N. Z. Ballin, *Meat Science*, 2010, 86, 577-587.

20. N. Z. Ballin and R. Lametsch, *Meat Science*, 2008, 80, 151-158.

21. R. Rodríguez-Ramírez, A. F. González-Córdova and B. Vallejo-Cordoba, *Analytica Chimica Acta*, 2011, 685, 120-126.

22. S. Esslinger, J. Riedl and C. Fauhl-Hassek, *Food Research International*, 2014, 60, 189-204.

23. V. A. Huck-Pezzei, I. Seitz, R. Karer, M. Schmutzler, L. De Benedictis, B. Wild and C. W. Huck, *Food Research International*, 2014, 62, 984-990.

24. M. Aghbashlo, S. Hosseinpour and M. Ghasemi-Varnamkhasti, *Trends in Food Science & Technology*, 2014, 39, 76-84.

25. J. Chandrapala, C. Oliver, S. Kentish and M. Ashokkumar, *Trends in Food Science & Technology*, 2012, 26, 88-98.

26. P. Oliveri, V. Di Egidio, T. Woodcock and G. Downey, *Food Chemistry*, 2011, 125, 1450-1456.
27. O. Canhoto, F. Pinzari, C. Fanelli and N. Magan, *International Biodeterioration & Biodegradation*, 2004, 54, 303-309.
28. J.-H. Cheng and D.-W. Sun, *Trends in Food Science & Technology*, 2014, 37, 78-91.
29. J.-H. Cheng and D.-W. Sun, *LWT - Food Science and Technology*, 2015, 62, 1060-1068.
30. G. J. Edelman, E. Gaston, T. G. van Leeuwen, P. J. Cullen and M. C. G. Aalders, *Forensic Science International*, 2012, 223, 28-39.
31. M. Á. Fernández de la Ossa, J. M. Amigo and C. García-Ruiz, *Forensic Science International*, 2014, 242, 228-235.
32. M. Atas, Y. Yardimci and A. Temizel, *Computers and Electronics in Agriculture*, 2012, 87, 129-141.
33. C. Igathinathane, L. O. Pordesimo and W. D. Batchelor, *Food Research International*, 2009, 42, 76-84.
34. M. Dowlati, S. S. Mohtasebi, M. Omid, S. H. Razavi, M. Jamzad and M. de la Guardia, *Journal of Food Engineering*, 2013, 119, 277-287.
35. Y. Yagiz, M. O. Balaban, H. G. Kristinsson, B. A. Welt and M. R. Marshall, *Journal of the Science of Food and Agriculture*, 2009, 89, 728-730.
36. I. Kerr, F. Shi, N. Brown, M. Jackson and R. Parkin, *Proceedings of the Institution of Mechanical Engineers Part B-Journal of Engineering Manufacture*, 2004, 218, 1591-1599.
37. C. Nansen, T. Herrman and R. Swanson, *Applied Spectroscopy*, 2010, 64, 637-643.
38. C. C. Yang, K. Chao, M. S. Kim, D. E. Chan, H. L. Early and M. Bell, *Poultry Science*, 2010, 89, 1252-1264.
39. D.-J. Lee, R. Schoenberger, J. Archibald and S. McCollum, *Journal of Food Engineering*, 2008, 86, 388-398.
40. M. Teena, A. Manickavasagan, A. Mothershaw, S. El Hadi and D. S. Jayas, *Food and Bioprocess Technology*, 2013, 6, 1621-1634.
41. M. S. M. Alfatni, A. R. M. Shariff, M. Z. Abdullah, M. H. B. Marhaban and O. M. B. Saeed, *Journal of Food Engineering*, 2013, 116, 703-725.

42. Y. Ying, W. Zhang, Y. Jiang and Y. Zhao, *Nongye Jixie Xuebao/Transactions of the Chinese Society of Agricultural Machinery*, 2000, 31, 112-115.

43. T. Brosnan and D. W. Sun, *Computers and Electronics in Agriculture*, 2002, 36, 193-213.

44. Y. R. Chen, K. L. Chao and M. S. Kim, *Computers and Electronics in Agriculture*, 2002, 36, 173-191.

45. E. R. Davies, *Imaging Science Journal*, 2009, 57, 197-217.

46. B. Gumus, M. O. Balaban and M. Unlusayin, *Turkish Journal of Fisheries and Aquatic Sciences*, 2011, 11, 167-176.

47. S. Janardhana, J. Jaya, K. J. Sabareesaan, J. George and Ieee, *2013 International Conference on Current Trends in Engineering and Technology (Icctet)*, 2013, 29-33.

48. M. Ottavian, L. Fasolato, P. Facco and M. Barolo, *Journal of Food Engineering*, 2013, 119, 765-775.

49. E. M. Dianov, M. J. F. Digonnet, S. Jiang, J. W. Glesener and J. C. Dries, in *Optical Components and Materials V*, eds. 2008, pp, 8900-8900.

50. E. Hemmer, N. Venkatachalam, H. Hyodo, A. Hattori, Y. Ebina, H. Kishimoto and K. Soga, *Nanoscale*, 2013, 5, 11339-11361.

51. S. Luo, E. Zhang, Y. Su, T. Cheng and C. Shi, *Biomaterials*, 2011, 32, 7127-7138.

52. M. Peng, G. Dong, L. Wondraczek, L. Zhang, N. Zhang and J. Qiu, *Journal of Non-Crystalline Solids*, 2011, 357, 2241-2245.

53. B. M. Nicolai, K. Beullens, E. Bobelyn, A. Peirs, W. Saeys, K. I. Theron and J. Lammertyn, *Postharvest Biology and Technology*, 2007, 46, 99-118.

54. L. S. Magwaza, U. L. Opara, H. Nieuwoudt, P. J. R. Cronje, W. Saeys and B. Nicolai, *Food and Bioprocess Technology*, 2012, 5, 425-444.

55. B. M. Nicolaie, K. Beullens, E. Bobelyn, A. Peirs, W. Saeys, K. I. Theron and J. Lammertyn, *Postharvest Biology and Technology*, 2007, 46, 99-118.

56. P. Butz, C. Hofmann and B. Tauscher, *Journal of Food Science*, 2005, 70, R131-R141.

57. J. Mlcek, O. Rop, K. Sustova, J. Simeonovova and R. Gal, *Chemické Listy*, 2010, 104, 855-860.

58. M. Prevolnik, M. Candek-Potokar and D. Skorjanc, *Czech Journal of Animal Science*, 2004,

- 49, 500-510.
59. D. Liu, X.-A. Zeng and D.-W. Sun, *Applied Spectroscopy Reviews*, 2013, 48, 609-628.
60. B. Sethuramasamyraja, S. Sachidhanantham, M. Yen and R. Wample, Minneapolis, MN, United States, 2007.
61. J. Ruzickova and K. Sustova, *Czech Journal of Food Sciences*, 2006, 24, 255-260.
62. V. A. McGlone, C. J. Clark and R. B. Jordan, *Postharvest Biology and Technology*, 2007, 46, 1-9.
63. N. Dai, M. A. German, T. Matsevit, R. Hanael, D. Swartzberg, Y. Yeselson, M. Petreikov, A. A. Schaffer and D. Granot, *Plant Science*, 2002, 162, 423-430.
64. H. Schulz, M. Baranska, R. Quilitzsch, W. Schutze and G. Losing, *Journal of Agricultural and Food Chemistry*, 2005, 53, 3358-3363.
65. G. B. C. Borges, J. J. R. Rohwedder and E. C. Bortoni, *Aasri Conference on Power and Energy Systems*, 2012, 2, 56-61.
66. C. A. Nunes, *Food Research International*, 2014, 60, 255-261.
67. Z. Qiu, L. Feng, W. Li and Y. He, *International Society for Optical Engineering, Bellingham WA, WA 98227-0010*, 2005, 60452.
68. A. Alishahi, H. Farahmand, N. Prieto and D. Cozzolino, *Spectrochimica Acta Part a-Molecular and Biomolecular Spectroscopy*, 2010, 75, 1-7.
69. Y. M. Bae, S. I. Cho, Y. Y. Kim, T. S. Park and K. Y. Hwang, *Transactions of the ASABE*, 2006, 49, 557-561.
70. Y.-R. Chen, R. W. Huffman and B. Park, *Journal of Food Process Engineering*, 1996, 19, 121-134.
71. V. Kestens, J. Charoud-Got, A. Bau, A. Bernreuther and H. Emteborg, *Food Chemistry*, 2008, 106, 1359-1365.
72. K. Thorvaldsson and C. Skjoldebrand, *Method and instrument for measuring local water content inside food*, Report 0346-718X, Chalmers Tekniska Hogskola, Goteborg, Sweden, 1998, 11.
73. M. C. Alamar, E. Bobelyn, J. Lammertyn, B. M. Nicolai and E. Molto, *Postharvest Biology and Technology*, 2007, 45, 38-45.

74. H. Y. Cen, Y. He and M. Huang, *Journal of Agricultural and Food Chemistry*, 2006, 54, 7437-7443.

75. Y. Shao, Y. He and S. Feng, *Food Research International*, 2007, 40, 835-841.

76. R. Karoui, L. Pillonel, E. Schaller, J. O. Bosset and J. De Baerdemaeker, *Food Chemistry*, 2007, 101, 1121-1129.

77. A. H. Gomez, Y. He and A. G. Pereira, *Journal of Food Engineering*, 2006, 77, 313-319.

78. Y. N. Shao, Y. He, A. H. Gomez, A. G. Pereir, Z. J. Qiu and Y. Zhang, *Journal of Food Engineering*, 2007, 81, 672-678.

79. G. Ma, Y. Ying, X. Fu, H. Lu, H. Yu and Y. Liu, *International Society for Optical Engineering, Bellingham WA, WA 98227-0010*, 2005, 59960-59961.

80. W. Srisawas, V. K. Jindal and W. Thanapase, *Journal of near Infrared Spectroscopy*, 2007, 15, 333-340.

81. S. W. Bruun, I. Sondergaard and S. Jacobsen, *Journal of Agricultural and Food Chemistry*, 2007, 55, 7244-7251.

82. R. M. Garcia-Rey, J. Garcia-Olmo, E. De Pedro, R. Quiles-Zafra and M. D. L. de Castro, *Meat Science*, 2005, 70, 357-363.

83. S. Schmitt, S. Garrigues and M. de la Guardia, *Critical Reviews in Analytical Chemistry*, 2014, 44, 186-197.

84. K. Usha and B. Singh, *Scientia Horticulturae*, 2013, 153, 71-83.

85. C. A. Teixeira dos Santos, M. Lopo, R. N. M. J. Pascoa and J. A. Lopes, *Applied Spectroscopy*, 2013, 67, 1215-1233.

86. A. Lopez, S. Arazuri, I. Garcia, J. Mangado and C. Jaren, *Journal of Agricultural and Food Chemistry*, 2013, 61, 5413-5424.

87. T. M. P. Cattaneo and S. E. Holroyd, *Journal of near Infrared Spectroscopy*, 2013, 21, 341-349.

88. X. Shao, Y. Ning, F. Liu, J. Li and W. Cai, *Acta Chimica Sinica*, 2012, 70, 2109-2114.

89. J. Weeranantanaphan, G. Downey, P. Allen and D.-W. Sun, *Journal of near Infrared Spectroscopy*, 2011, 19, 61-104.

90. L. E. Rodriguez-Saona and M. E. Allendorf, in *Annual Review of Food Science and*

- Technology*, Vol 2, eds. M. P. Doyle and T. R. Klaenhammer, 2011, 2, pp. 467-483.
91. V. Kehlenbeck, *11th International Congress on Engineering and Food (Icef11)*, 2011, 1, 2015-2022.
92. J. Wang, J.-q. Wang, D.-p. Bu, W.-j. Guo, J.-s. Shen, H.-y. Wei, L.-y. Zhou and K.-l. Liu, *Spectroscopy and Spectral Analysis*, 2009, 29, 1281-1285.
93. R. Karoui and C. Blecker, *Food Bioprocess Technol*, 2011, 4, 364-386.
94. J.-L. Damez and S. Clerjon, *Meat Science*, 2013, 95, 879-896.
95. X. Chen, X. Wu, M. Gan, F. Xu, L. He, D. Yang, H. Xu, N. P. Shah and H. Wei, *Journal of Dairy Science*, 2015, 98, 1563-1570.
96. A. M. Lefcourt, M. S. Kim and Y. R. Chen, *Computers and Electronics in Agriculture*, 2005, 48, 63-74.
97. G. Jordan, R. Thomasius, H. Schröder, J. S. Wulf, O. Schlüter, B. Sumpf, M. Maiwald, H. Schmidt, H. D. Kronfeldt, R. Scheuer, F. Schwägele and K.-D. Lang, *J. Verbr. Lebensm.*, 2009, 4, 7-14.
98. A. Hassoun and R. Karoui, *Food Control*, 2015, 54, 240-249.
99. R. Karoui, E. Thomas and E. Dufour, *Food Research International*, 2006, 39, 349-355.
100. J. P. Abels and R. D. Ludescher, *Journal of Agricultural and Food Chemistry*, 2003, 51, 544-549.
101. Z. Bai, B. Wang, H. Chen and M. Wang, *Sensors and Actuators B: Chemical*, 2015, 215, 330-336.
102. Z.-Y. Liu, T. Zhu, E.-d. Gu, Y. Liu and C.-y. Song, *Spectroscopy and Spectral Analysis*, 2008, 28, 2409-2412.
103. B. Švecová, M. Bordovská, D. Kalvachová and T. Hájek, *Journal of Food Composition and Analysis*, 2015, 38, 80-88.
104. S.-J. Huang, C.-P. Lin and S.-Y. Tsai, *Journal of Food Composition and Analysis*, 2015, 42, 38-45.
105. S. Pao, C. L. Davis, L. M. Friedrich and M. E. Parish, *Journal of Food Protection*, 2002, 65, 1943-1948.
106. T. Pérez-Ruiz, C. Martínez-Lozano, V. Tomás and J. Martín, *Talanta*, 2001, 54, 989-995.

107. P. Chaumpluk and P. Chaiprasart, *Ix International Mango Symposium*, 2013, 992, 551-560.

108. N. Thepwiwatjit, A. Thattiyaphong, P. Limsuwan, K. Tuitemwong and P. Tuitemwong, *Journal of Nanomaterials*, 2014.

109. K.-S. Lee, W. B. Cohen, R. E. Kennedy, T. K. Maierasperger and S. T. Gower, *Remote Sensing of Environment*, 2004, 91, 508-520.

110. B. M. Nicolaï, K. Beullens, E. Bobelyn, A. Peirs, W. Saeys, K. I. Theron and J. Lammertyn, *Postharvest Biology and Technology*, 2007, 46, 99-118.

111. J. Qin, K. Chao, M. S. Kim, R. Lu and T. F. Burks, *Journal of Food Engineering*, 2013, 118, 157-171.

112. D. Wu and D.-W. Sun, *Innovative Food Science & Emerging Technologies*, 2013, 19, 1-14.

113. D. Wu and D.-W. Sun, *Innovative Food Science & Emerging Technologies*, 2013, 19, 15-28.

114. D. P. Ariana and R. Lu, *Sensing and Instrumentation for Food Quality and Safety*, 2008, 2.

115. J. Jin, L. Tang, Z. Hruska and H. Yao, *Computers and Electronics in Agriculture*, 2009, 69, 158-164.

116. L. Jiang, B. Zhu, Y. Tao and S. Professor Da-Wen, in *Hyperspectral Imaging for Food Quality Analysis and Control*, Academic Press, San Diego, 2010, pp. 79-98.

117. B.-K. Cho, M. S. Kim, I.-S. Baek, D.-Y. Kim, W.-H. Lee, J. Kim, H. Bae and Y.-S. Kim, *Postharvest Biology and Technology*, 2013, 76, 40-49.

118. P. M. Mehl, Y.-R. Chen, M. S. Kim and D. E. Chan, *Journal of Food Engineering*, 2004, 61, 67-81.

119. D. P. Ariana and R. Lu, *Journal of Food Engineering*, 2010, 96, 583-590.

120. M. Zhang, Z. Qin, X. Liu and S. L. Ustin, *International Journal of Applied Earth Observation and Geoinformation*, 2003, 4, 295-310.

121. X. Zou, J. Shi, L. Hao, J. Zhao, H. Mao, Z. Chen, Y. Li and M. Holmes, *Analytica Chimica Acta*, 2011, 706, 105-112.

122. B. A. Schaeffer, J. M. Morrison, D. Kamykowski, G. C. Feldman, L. Xie, Y. Liu, W. Sweet, A. McCulloch and S. Banks, *Remote Sensing of Environment*, 2008, 112, 3044-3054.

123. G. ElMasry and D.-W. Sun, in *Hyperspectral Imaging for Food Quality Analysis and Control*, ed. S. Professor Da-Wen, Academic Press, San Diego, 2010, pp. 175-240.

-
124. R. Díaz, L. Cervera, S. Fenollosa, C. Ávila and J. Belenguer, *Procedia Engineering*, 2011, 25, 313-316.
125. X. Ye, K. Sakai, A. Sasao and S.-i. Asada, *Chemometrics and Intelligent Laboratory Systems*, 2008, 90, 132-144.
126. R. Lu and S. Da-Wen, in *Computer Vision Technology for Food Quality Evaluation*, Academic Press, Amsterdam, 2008, pp. 319-348.
127. M. Huang, X. Wan, M. Zhang and Q. Zhu, *Journal of Food Engineering*, 2013, 116, 45-49.
128. J. Qin and R. Lu, *Postharvest Biology and Technology*, 2008, 49, 355-365.
129. P. B. Garcia-Allende, O. M. Conde, J. Mirapeix, A. Cobo and J. M. Lopez-Higuera, *Sensors and Actuators B: Chemical*, 2008, 129, 977-984.
130. A. H. Sivertsen, C.-K. Chu, L.-C. Wang, F. Godtliebsen, K. Heia and H. Nilsen, *Journal of Food Engineering*, 2009, 90, 317-324.
131. B. Schrader, H. Schulz, G. N. Andreev, H. H. Klump and J. Sawatzki, *Talanta*, 2000, 53, 35-45.
132. J. Qin, K. Chao and M. S. Kim, *Journal of Food Engineering*, 2011, 107, 277-288.
133. A. Daarre, R. Jaffiol, A. Richard and P. Tchtio, *Chemical Physics Letters*, 2002, 366, 274-278.
134. A. Celedon and J. M. Aguilera, *Food Science and Technology International*, 2002, 8, 101-108.
135. L. G. Thygesen, M. M. Lokke, E. Micklander and S. B. Engelsens, *Trends in Food Science & Technology*, 2003, 14, 50-57.
136. B. Muik, B. Lendl, A. Molina-Diaz, D. Ortega-Calderon and M. J. Ayora-Canada, *Journal of Agricultural and Food Chemistry*, 2004, 52, 6055-6060.
137. C. Camerlingo, F. Zenone, I. Delfino, N. Diano, D. G. Mita and M. Lepore, *Sensors*, 2007, 7, 2049-2061.
138. K. Seidler-Lozykowska, M. Baranska, R. Baranski and D. Krol, *Journal of Agricultural and Food Chemistry*, 2010, 58, 5271-5275.
139. L. C. Prinsloo, W. du Plooy and C. van der Merwe, *Journal of Raman Spectroscopy*, 2004, 35, 561-567.

140. N. K. Afseth, V. H. Segtnan, B. J. Marquardt and J. P. Wold, *Applied Spectroscopy*, 2005, 59, 1324-1332.

141. Y. Zhao, C. Y. Ma, S. N. Yuen and D. L. Phillips, *Journal of Food Science*, 2004, 69, 206-213.

142. A. M. Herrero, *Critical Reviews in Food Science and Nutrition*, 2008, 48, 512-523.

143. K. Chen, X. Sun, C. Qin and X. Tang, *Computers and Electronics in Agriculture*, 2010, 70, 27-32.

144. L. Huang, J. Zhao, Q. Chen and Y. Zhang, *Food Chemistry*, 2014, 145, 228-236.

145. M. Estévez, P. Kylli, E. Puolanne, R. Kivikari and M. Heinonen, *Meat Science*, 2008, 80, 1290-1296.

146. A. M. Herrero, M. I. Cambero, J. A. Ordóñez, L. de la Hoz and P. Carmona, *Food Chemistry*, 2008, 109, 25-32.

147. Q. Chen, Y. Zhang, J. Zhao and Z. Hui, *Analytical Methods*, 2013, 5, 6382-6388.

148. M. L. Demattè, N. Pojer, I. Endrizzi, M. L. Corollaro, E. Betta, E. Aprea, M. Charles, F. Biasioli, M. Zampini and F. Gasperi, *Food Quality and Preference*, 2014, 38, 58-64.

149. J. Chen, C. Karlsson and M. Povey, *Journal Of Texture Studies*, 2005, 36, 139-156.

150. E. M. Castro-Prada, H. Luyten, W. Lichtendonk, R. J. Hamer and T. Van Vliet, *Journal Of Texture Studies*, 2007, 38, 698-724.

151. P. Varela, J. Chen, S. Fiszman and M. J. W. Povey, *Journal Of Chemometrics*, 2006, 20, 311-320.

152. V. Mohammadi, M. Ghasemi-Varnamkhasti, R. Ebrahimi and M. Abbasvali, *Measurement*, 2014, 58, 93-102.

153. M. J. W. Povey, *Academic Press, New York*, 1997.

154. M. J. W. Povey, in *Understanding and Controlling the Microstructure of Complex Foods*, ed. D. J. McClements, Woodhead Publishing, 2007, pp. 311-333.

155. T. S. Awad, H. A. Moharram, O. E. Shaltout, D. Asker and M. M. Youssef, *Food Research International*, 2012, 48, 410-427.

156. M. J. W. Povey, N. Watson and N. G. Parker, in *Food Microstructures*, ed. V. J. M. Groves, Woodhead Publishing, 2013, pp. 192-222.

-
157. M. J. W. Povey, *Food Hydrocolloids*, 2014, 42, Part 1, 118-129.
158. N. SO, *Trans ASAE*, 1973, 16, 384-400.
159. S. N. Jha, K. Narsaiah, A. L. Basediya, R. Sharma, P. Jaiswal, R. Kumar and R. Bhardwaj, *Journal of Food Science and Technology-Mysore*, 2011, 48, 387-411.
160. B. Picard, B. Lebret, I. Cassar-Malek, L. Liaubet, C. Berri, E. Le Bihan-Duval, J. F. Hocquette and G. Renand, *Meat Science*, 2015, 109, 18-26.
161. R. Zywnica, G. Pierzynowska-Korniak and J. Wojcik, *Journal of Food Engineering*, 2005, 67, 413-418.
162. J. L. Damez and S. Clerjon, *53rd International Congress of Meat Science and Technology*, 2007, 1, 215-216.
163. S. Krauss, W. H. Schnitzler, J. Grassmann and M. Witke, *Journal of Agricultural and Food Chemistry*, 2006, 54, 441-448.
164. E. Garcia-Breijo, J. M. Barat, O. L. Torres, R. Grau, L. Gil, J. Ibanez, M. Alcaniz, R. Masot and R. Fraile, *Sensors and Actuators a-Physical*, 2008, 148, 63-67.
165. H. Bozkurt and F. Icier, *Journal of Food Engineering*, 2010, 96, 86-92.
166. Y. Yang, Q. Li, X. Yu, X. Chen and Y. Wang, *Food Control*, 2014, 39, 198-203.
167. S. Zhu, Y. Luo, L. Feng and Y. Bao, *Journal of Food Processing and Preservation*, 2015, 39, 167-174.
168. J.-L. Damez, S. Clerjon, S. Abouelkaram and J. Lepetit, *Meat Science*, 2007, 77, 512-519.
169. S. Rynänen, *Journal of Food Engineering*, 1995, 26, 409-429.
170. M. E. Sosa-Morales, G. Tiwari, S. Wang, J. Tang, H. S. Garcia and A. Lopez-Malo, *Biosystems Engineering*, 2009, 103, 287-296.
171. M. E. Sosa-Morales, G. Tiwari, S. Wang, J. Tang, H. S. Garcia and A. Lopez-Malo, *Biosystems Engineering*, 2009, 103, 297-303.
172. T. VN and S. SS, *Journal of Microwave Power*, 1987, 22, 29-33.
173. L. C and S. N, *journal of the japanese society for food science and technology*, 1999, 20, 42-45.
174. Ø. G. Martinsen, S. Grimnes and P. Mirtaheri, *Journal of Food Engineering*, 2000, 43, 189-192.

175. P. Basaran, N. Basaran-Akgul and B. A. Rasco, *Food Chemistry*, 2010, 120, 361-370.

176. M. E. Sosa-Morales, L. Valerio-Junco, A. López-Malo and H. S. García, *LWT - Food Science and Technology*, 2010, 43, 1169-1179.

177. D. L. Corwin and R. E. Plant, *Computers and Electronics in Agriculture*, 2005, 46, 1-10.

178. A. Legrand, J. C. Leuliet, S. Duquesne, R. Kesteloot, P. Winterton and L. Fillaudeau, *Journal of Food Engineering*, 2007, 81, 447-458.

179. J.-L. Damez, S. Clerjon, S. Abouelkaram and J. Lepetit, *Food Control*, 2008, 19, 931-939.

180. X. Zhao, J. Yin, J. Chen, G. Song, L. Wang, H. Zhu, D. Brining and J. D. Z. Chen, *American Journal of Physiology-Regulatory Integrative and Comparative Physiology*, 2009, 296, R36-R42.

181. Y. Jin, N. Yang, X. Duan, F. Wu, Q. Tong and X. Xu, *Biosystems Engineering*, 2015, 129, 70-77.

182. R. Zywnica and J. K. Banach, *Journal of Food Engineering*, 2015, 158, 8-12.

183. R. Zwiggelaar, C. R. Bull and M. J. Mooney, *Journal of Agricultural Engineering Research*, 1996, 63, 161-170.

184. A. Warning, P. Verboven, B. Nicolai, G. van Dalen and A. K. Datta, *Innovative Food Science & Emerging Technologies*, 2014, 24, 14-27.

185. D. Mery, I. Lillo, H. Loebel, V. Rizzo, A. Soto, A. Cipriano and J. M. Aguilera, *Journal of Food Engineering*, 2011, 105, 485-492.

186. Wikipedia, X-ray, <https://en.wikipedia.org/wiki/X-ray>, Accessed 2015-9-2.

187. H. Leboutet and J. Aucouturier, *Radiation Physics and Chemistry (1977)*, 1985, 25, 233-242.

188. C. R. Bull, R. Zwiggelaar and R. D. Speller, *Journal of Food Engineering*, 1997, 33, 167-179.

189. M. S. Nielsen, T. Lauridsen, L. B. Christensen and R. Feidenhans'l, *Food Control*, 2013, 30, 531-535.

190. E. Sjögren, B. Abrahamsson, P. Augustijns, D. Becker, M. B. Bolger, M. Brewster, J. Brouwers, T. Flanagan, M. Harwood, C. Heinen, R. Holm, H.-P. Juretschke, M. Kubbinga, A. Lindahl, V. Lukacova, U. Münster, S. Neuhoff, M. A. Nguyen, A. v. Peer, C. Reppas, A. R. Hodgeman, C. Tannergren, W. Weitschies, C. Wilson, P. Zane, H. Lennernäs and P. Langguth,

- European Journal of Pharmaceutical Sciences*, 2014, 57, 99-151.
191. N. Toyofuku and R. P. Haff, in *Computer Vision Technology in the Food and Beverage Industries*, ed. D.-W. Sun, Woodhead Publishing, 2012, pp. 181-205.
192. E. Herremans, P. Verboven, T. Defraeye, S. Rogge, Q. T. Ho, M. L. A. T. M. Hertog, B. E. Verlinden, E. Bongaers, M. Wevers and B. M. Nicolai, *Nuclear Instruments and Methods in Physics Research Section B: Beam Interactions with Materials and Atoms*, 2014, 324, 88-94.
193. J. Laverse, M. Mastromatteo, P. Frisullo and M. A. Del Nobile, *Journal of Dairy Science*, 2011, 94, 43-50.
194. K. S. Lim and M. Barigou, *Food Research International*, 2004, 37, 1001-1012.
195. K. K. Nielson, A. W. Mahoney, L. S. Williams and V. C. Rogers, *Journal of Food Composition and Analysis*, 1991, 4, 39-51.
196. A. Jastrzębska, B. Brudka, T. Szymański and E. Szłyk, *Food Chemistry*, 2003, 83, 463-467.
197. L. Perring, D. Andrey, M. Basic-Dvorzak and D. Hammer, *Journal of Food Composition and Analysis*, 2005, 18, 655-663.
198. A. Otaka, A. Hokura and I. Nakai, *Food Chemistry*, 2014, 147, 318-326.
199. N. J. B. McFarlane, C. R. Bull, R. D. Tillett, R. D. Speller, G. J. Royle and K. R. A. Johnson, *Journal of Agricultural Engineering Research*, 2000, 75, 265-274.
200. A. P. G. Almeida, D. Braz, R. C. Barroso and R. T. Lopes, *Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment*, 2007, 580, 764-767.
201. J. Blazek and E. P. Gilbert, *Carbohydrate Polymers*, 2011, 85, 281-293.
202. M. V. Petoukhov and D. I. Svergun, *The International Journal of Biochemistry & Cell Biology*, 2013, 45, 429-437.
203. M. Khandelwal and A. H. Windle, *International Journal of Biological Macromolecules*, 2014, 68, 215-217.
204. Q. Chen, C. Zhang, J. Zhao and Q. Ouyang, *TrAC Trends in Analytical Chemistry*, 2013, 52, 261-274.
205. Y. Xia, D. L. Ergun, W. K. Wacker, X. Wang, C. E. Davis and S. Kaul, *Journal of Clinical Densitometry*, 2014, 17, 78-83.

206. O. Grégoire, M. R. Cleland, J. Mittendorfer, S. Dababneh, D. A. E. Ehlermann, X. Fan, F. Käppeler, J. Logar, J. Meissner, B. Mullier, F. Stichelbaut and D. W. Thayer, *Radiation Physics and Chemistry*, 2003, 67, 169-183.

207. R. B. Solanki, M. Prasad, A. U. Sonawane and S. K. Gupta, *Annals of Nuclear Energy*, 2012, 43, 123-130.

208. G. Demareux and L. Sallé, in *Food Safety Management*, ed. Y. M. Lelieveld, Academic Press, San Diego, 2014, pp. 511-533.

209. M. Edwards, in *Hygiene in Food Processing (Second edition)*, eds. H. L. M. Lelieveld, J. T. Holah and D. Napper, Woodhead Publishing, 2014, pp. 441-464.

210. N. J. B. McFarlane, C. R. Bull, R. D. Tillett, R. D. Speller and G. J. Royle, *Journal of Agricultural Engineering Research*, 2001, 79, 407-418.

211. M. Musse, F. De Guio, S. Quellec, M. Cambert, S. Challos and A. Davenel, *Magnetic Resonance Imaging*, 2010, 28, 1525-1534.

212. S.-M. Kim, P. Chen, M. J. McCarthy and B. Zion, *Journal of Agricultural Engineering Research*, 1999, 74, 293-301.

213. H. C. Bertram, A. Kohler, U. Bocker, R. Ofstad and H. J. Andersen, *Journal Of Agricultural And Food Chemistry*, 2006, 54, 1740-1746.

214. H. C. Bertram, H. Jian Zhi, D. N. Rommereim, R. A. Wind and H. J. Andersen, *Journal of Agricultural and Food Chemistry*, 2004, 52, 2681-2688.

215. M. A. Brescia, V. Caldarola, A. De Giglio, D. Benedetti, F. P. Fanizzi and A. Sacco, *Analytica Chimica Acta*, 2002, 458, 177-186.

216. H. C. Bertram, S. J. Holdsworth, A. K. Whittaker and H. J. Andersen, *Journal of Agricultural and Food Chemistry*, 2013, 53, 7814-7818.

217. B. M. N. I, T. Defraeye, B. De Ketelaere, E. Herremans, M. L. A. T. Hertog, W. Saeys, A. Torricelli, T. Vandendriessche and P. Verboven, *The Annual Review of Food Science and Technology*, 2014, 5, 285-312.

218. F. Tao, L. Zhang, M. J. McCarthy, D. M. Beckles and M. Saltveit, *Postharvest Biology and Technology*, 2014, 97, 62-67.

219. A. Melado-Herreros, M.-A. Muñoz-García, A. Blanco, J. Val, M. E. Fernández-Valle and P.

- Barreiro, *Postharvest Biology and Technology*, 2013, 86, 125-133.
220. M. Musse, S. Quellec, M. Cambert, M.-F. Devaux, M. Lahaye and F. Mariette, *Postharvest Biology and Technology*, 2009, 53, 22-35.
221. J. A. Abbott, R. Lu, B. Upchurch and R. Stroshine, *Horticultural Reviews*, 1997, 20, 1-120.
222. C. J. Clark, P. D. Hockings, D. C. Joyce and R. A. Mazucco, *Postharvest Biology and Technology*, 1997, 11, 1-21.
223. L. E. J, J. A. D, S. A. L and H. A. M, *LWT - Food Science and Technology*, 2003, 36, 19-27.
224. I. Campos, R. Masot, M. Alcañiz, L. Gil, J. Soto, J. L. Vivancos, E. García-Breijo, R. H. Labrador, J. M. Barat and R. Martínez-Mañez, *Sensors and Actuators B: Chemical*, 2010, 149, 71-78.
225. H. C. Bertram, R. H. Andersen and H. J. Andersen, *Meat Science*, 2014, 75, 128-133.
226. M. L. H. Gruwel, P. Latta, B. Matwiy, B. Tomanek, *Food Research International*, 2010, 43, 2087-2092.
227. F. Badii and N. K. Howell, *Food Hydrocolloids*, 2006, 20, 630-640.
228. M. S. Venkatesh and G. S. V. Raghavan, *Biosystems Engineering*, 2004, 88, 1-18.
229. J.-L. Damez and S. Clerjon, *Meat Science*, 2013, 95, 879-896.
230. S. Clerjon and J.-L. Damez, *Journal of Food Engineering*, 2009, 94, 379-389.
231. S. Clerjon, J.-D. Daudin and J.-L. Damez, *Food Chemistry*, 2003, 82, 87-97.
232. E. Nyfors, *Subsurface Sensing Technologies*, 2000, 1, 23-43.
233. S. O. Nelson and S. Trabelsi, *Transactions of the ASABE*, 2008, 51, 1829-1834.
234. P. Parasoglou, E. P. J. Parrott, J. A. Zeitler, J. Rasburn, H. Powell, L. F. Gladden and M. L. Johns, *Terahertz Science and Technology*, 2010, 3, 172-182.
235. G.-J. Kim, J.-I. Kim, S.-G. Jeon, J. Kim, K.-K. Park and C.-H. Oh, *Journal of Infrared, Millimeter, and Terahertz Waves*, 2012, 33, 125-129.
236. A. A. Gowen, C. O'Sullivan and C. P. O'Donnell, *Trends in Food Science & Technology*, 2012, 25, 40-46.
237. G. Ok, H. J. Kim, H. S. Chun and S.-W. Choi, *Food Control*, 2014, 42, 284-289.
238. J. Qin, L. Xie and Y. Ying, *Food Chemistry*, 2015, 170, 415-422.
239. G.-J. Kim, J.-I. Kim, S.-G. Jeon, J. Kim, K.-K. Park and C.-H. Oh, *Journal of Infrared*,

Millimeter, and Terahertz Waves, 2012, 33, 657–664.

240. P. U. Jepsen, U. Møller and H. Merbold, *Optics Express*, 2007, 15, 14717–14737.

241. C. Jordens and M. Koch, *Optical Engineering*, 2008, 47.

242. Y. F. Hua and H. J. Zhang, *IEEE Transactions on Microwave Theory and Techniques*, 2012, 58, 2064–2070.

243. A. Redo-Sanchez and X. C. Zhang, *Analyst*, 2011, 136, 1733–1738.

244. J. S. Li, *Applied Spectroscopy*, 2010, 64, 231–234.

245. D. Banerjee, W. v. Spiegel, M. D. Thomson, S. Schabel and H. G. Roskos, *Optics Express*, 2008, 16, 9060–9066.

246. X. Tian, J. Wang and S. Cui, *Journal of Food Engineering*, 2013, 119, 744–749.

247. M. K. Morsy, K. Zór, N. Kostasheva, T. S. Alstrøm, A. Heiskanen, H. El-Tanahi, A. Sharoba, D. Papkovsky, J. Larsen, H. Khalaf, M. H. Jakobsen and J. Emnéus, *Food Control*, 2016, 60, 346–352.

248. G.-S. Ryu, K. H. Park, W.-T. Park, Y.-H. Kim and Y.-Y. Noh, *Org. Electron.*, 2015, 23, 76–81.

249. Q. Kang, X. Zhu, X. Ma, L. Kong, W. Xu and D. Shen, *Sensors and Actuators B: Chemical*, 2015, 220, 472–480.

250. S. Oller-Moreno, G. Singla-Buxarraiz, J. M. Jiménez-Soto, A. Pardo, R. Garrido-Delgado, L. Arce and S. Marco, *Sensors and Actuators B: Chemical*, 2015, 217, 13–21.

251. M. Peris and L. Escuder-Gilabert, *Analytica Chimica Acta*, 2013, 804, 29–36.

252. Y. Vlasov, A. Legin and A. Rudnitskaya, *Analytical and Bioanalytical Chemistry*, 2002, 36–146.

253. N. Prieto, P. Oliveri, R. Leardi, M. Gay, C. Apetrei, M. L. Rodríguez-Méndez and J. A. de Saja, *Sensors and Actuators B: Chemical*, 2013, 183, 52–57.

254. D. Wang, X. Wang, T. Liu and Y. Liu, *Meat Science*, 2012, 90, 373–377.

255. R. H. Labrador, R. Masot, M. Alcañiz, D. Baigts, J. Soto, R. Martínez-Mañez, E. García-Breijo, L. Gil and J. M. Barat, *Food Chemistry*, 2010, 122, 864–870.

256. C. Phat, B. Moon and C. Lee, *Food Chemistry*, 2016, 192, 1068–1077.

257. A. Alimelli, G. Pennazza, M. Santonico and R. Paolesse, *Analytica Chimica Acta*, 2007, 582, 320–328.

258. J.-H. Cheng, D.-W. Sun, H. Pu and Z. Zhu, *Food Chemistry*, 2015, 185, 245-253.
259. E. O. Baldeón, M. Alcañiz, R. Masot, E. M. Fuentes, J. M. Barat and R. Grau, *Food Control*, 2015, 54, 181-187.
260. S. Qiu, J. Wang and L. Gao, *LWT - Food Science and Technology*, 2015, 60, 115-123.
261. L. G. Dias, C. Sequeira, A. C. A. Veloso, M. E. B. C. Sousa and A. M. Peres, *Analytica Chimica Acta*, 2014, 848, 32-42.
262. A. C. A. Veloso, L. G. Dias, N. Rodrigues, J. A. Pereira and A. M. Peres, *Talanta*, 2016, 146, 585-593.
263. A. M. Simoes Costa, M. M. Costa Sobral, I. Delgadillo, A. Cerdeira and A. Rudnitskaya, *Sensors and Actuators B: Chemical*, 2015, 207, Part B, 1095-1103.
264. N. Rakow and K. Suslick, *Nature*, 2000, 406, 710-713.
265. K. S. Suslick, N. A. Rakow and A. Sen, *Tetrahedron*, 2004, 60, 11133-11138.
266. X. Huang, X. Zou, J. Zhao, J. Shi, X. Zhang, Z. Li and L. Shen, *Meat Science*, 2014, 98, 203-210.
267. T. Soga, Y. Jimbo, K. Suzuki and D. Citterio, *Analytical Chemistry*, 2013, 85, 8973-8978.
268. Q. Chen, H. Li, Q. Ouyang and J. Zhao, *Sensors and Actuators B: Chemical*, 2014, 205, 1-8.
269. X. Huang, F. Zhou and F. Jiang, *Nongye Jixie Xuebao/Transactions of the Chinese Society of Agricultural Machinery*, 2011, 42, 142-145+124.
270. P. Zaragoza, A. Fuentes, M. Ruiz-Rico, J.-L. Vivancos, I. Fernández-Segovia, J. V. Ros-Lis, J. M. Barat and R. Martínez-Máñez, *Food Chemistry*, 2015, 175, 315-321.
271. X. Huang, J. Xin and J. Zhao, *Journal of Food Engineering*, 2011, 105, 632-637.
272. C. Zhang, D. P. Bailey and K. S. Suslick, *Journal of Agricultural and Food Chemistry*, 2006, 54, 4925-4931.
273. H. Qin, D. Huo, L. Zhang, L. Yang, S. Zhang, M. Yang, C. Shen and C. Hou, *Food Research International*, 2012, 45, 45-51.
274. Q. Chen, A. Liu, J. Zhao, Q. Ouyang, Z. Sun and L. Huang, *Sensors and Actuators B: Chemical*, 2013, 183, 608-616.
275. Z. Xiaobo, Z. Jian and Z. Jiewen, *Transactions of the Chinese Society Agricultural Engineering*, 2008, 24, 165-168.

276. Z. Xiaobo, Z. Jiewen and W. Shouyi, *Transactions of the Chinese Society Agricultural Engineering*, 2002, 18, 226-230.

277. B. Suslick, L. Feng and K. Suslick, *Analytical Chemistry*, 2010, 82, 2067-2073.

278. C. J. Musto and K. S. Suslick, *Current Opinion in Chemical BiologyModel Systems/Biomolecular Synthesis and Modification*, 2010, 14, 758-766.

279. D. Huo, Y. Wu, M. Yang, H. Fa, X. Luo and C. Hou, *Food Chemistry*, 2014, 145, 639-645.

280. Q. Chen, A. Liu, J. Zhao and Q. Ouyang, *Journal of Pharmaceutical and Biomedical Analysis*, 2013, 84, 77-83.

281. F. Röck, N. Barsan and U. Weimar, *Chemical Reviews*, 2008, 108, 705-725.

282 Y.-C. Liu, H.-M. Gao, *Applied Computing in Medicine and Health, Morgan Kaufmann, Boston*, 2016, pp. 244-268.

283 J. Link, D. Senner, W. Claupein, *Computers and Electronics in Agriculture*, 2013,94, 20-28.

284 F. Garcia-Ruiz, S. Sankaran, J.M. Maja, W.S. Lee, J. Rasmussen, R. Ehsani, *Computers and Electronics in Agriculture*, 2013, 91, 106-115.

285 R. Artmann, Sensor systems for milking robots, *Computers and Electronics in Agriculture*, 1997, 17, 9-40.

286 J.E. Hillerton, *Computers and Electronics in Agriculture*, 1997, 17, 41-51.

287 T. Torii, *Computers and Electronics in Agriculture*, 2000, 25, 133-153.

288 A.R. Frost, A.P. French, R.D. Tillett, T.P. Pridmore, S.K. Welch, *Computers and Electronics in Agriculture*, 2004, 44, 93-106.

289 K. Tanigaki, T. Fujiura, A. Akase, J. Imagawa, *Computers and Electronics in Agriculture*, 2008, 63, 65-72.

290 S.A. Hiremath, G.W.A.M. van der Heijden, F.K. van Evert, A. Stein, C.J.F. ter Braak, *Computers and Electronics in Agriculture*, 2014, 100, 41-50.

291 C. Blanes, C. Ortiz, M. Mellado, P. Beltrán, *Computers and Electronics in Agriculture*, 2015, 113, 44-50.

Figure captions:

Fig. 1. Incident by category 2006 and 2012 UK, Adapted from ESP KTN “Sensing in Food” workshop report 25th February 2014.

Fig. 2. Non-invasive sensing techniques in food assurance.

Fig. 3. The light–food interaction and the electromagnetic spectrum (adapted from Google image).

Fig. 4. Typical detection results from optical techniques used in meat detection. (Abbreviations: MV: machine vision, NIR: near infrared; UV: ultraviolet and ultraviolet fluorescence; HIS: multispectral and hyperspectral imaging.)¹⁴³⁻¹⁴⁷

Fig. 5. Approximate frequency ranges corresponding to sound, with rough guide of some applications.

Fig. 6. Acoustic techniques, (a) microphone, (b) pulse-echo, (c) pitch and catch, (d) resonance techniques.

Fig. 7. A handled device for impedance measurement with two electrodes (a) and a multidirectional sensor (b).

Fig. 8. Different applications use different parts of the X-ray spectrum (adapted from Wikipedia²⁰⁰, we added some soft X-ray applications).

Fig. 9. Principle of X-rays transmission radiography (a) and soft X-ray inspection system (b) picture, (c) schematic diagram, (d) X-ray image of fish fillets in which the fish bones are detectable¹⁹⁹.

Fig. 10. X-ray CT (*left*) and MRI (*right*) images of Ascara apples without (*a,b*) and with (*c,d*) water core. Both techniques are capable of detecting the water core region inside the fruit; however, the contrast in the MRI images is better due to the particular pulse sequence used. Figure reprinted from Herremans et al. (2014) with permission from Elsevier. Abbreviations: CT, computed tomography; MRI, magnetic resonance imaging²³⁰.

Fig. 11. Transmission CW THz imaging system based on the parabolic mirrors operating at 0.2 THz using a pyramidal horn antenna located in front of the sample (adapt from Kim, G., et al.)²³⁹.

Fig. 12. Schematic representation of the components of an electronic nose⁴¹.

Fig. 13. The diagram of colorimetric measurement. A, B, C: three-way valve, During the

measurement, three different phases could be distinguished: concentration, measurement and cleaning. The electro-valves, controlled by a computer program, guided the N₂ through different circuits depending on the measurement phase.

Fig. 14. Sensors, sensor deployment and length scales.

Analyst Accepted Manuscript

Fig. 1.

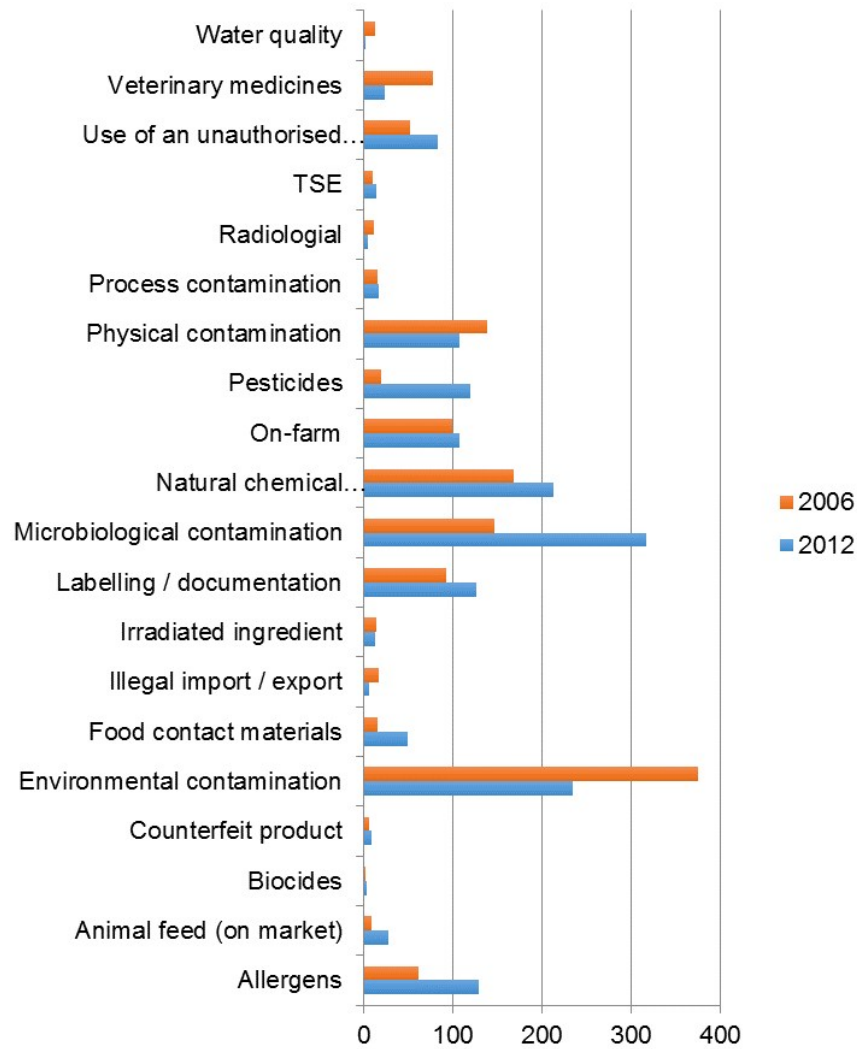


Fig. 2.

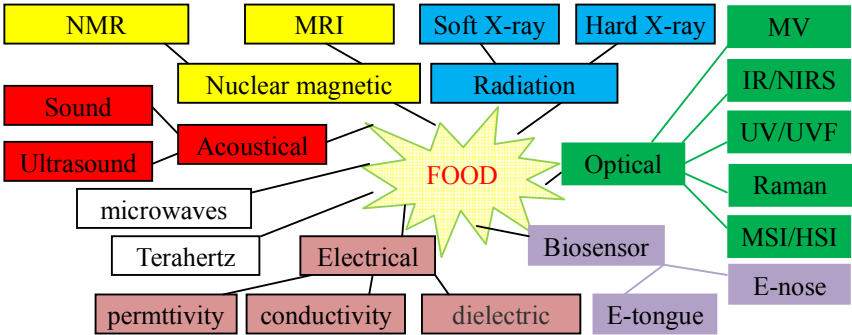


Fig. 3.

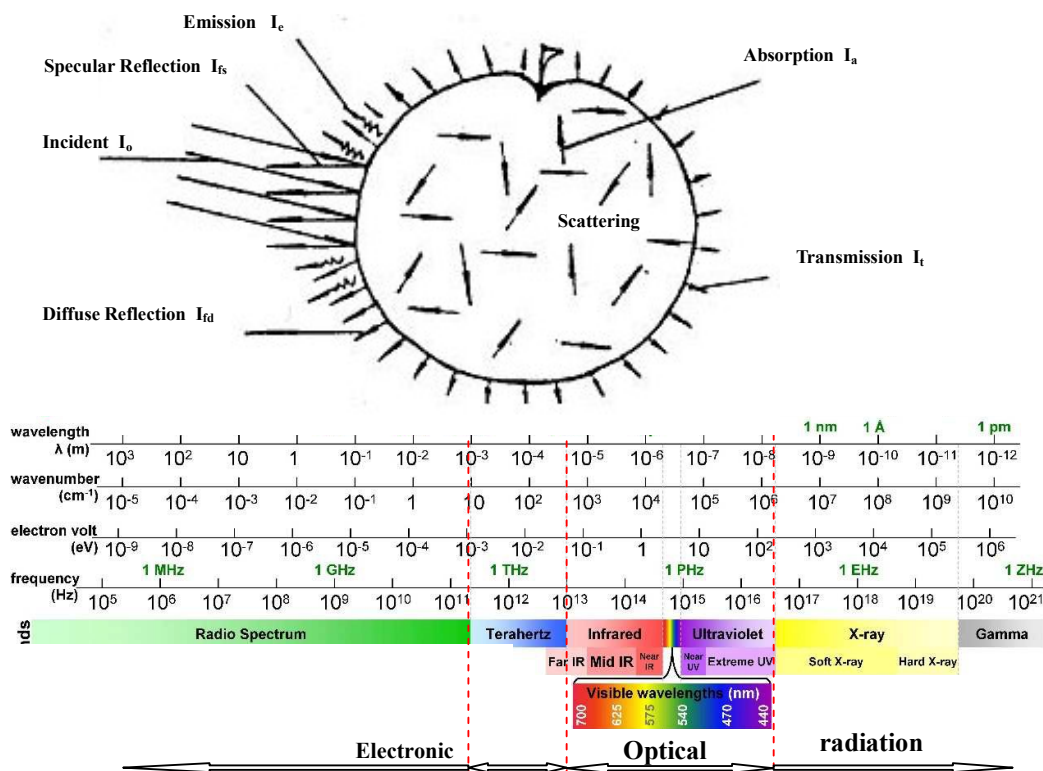


Fig. 4.

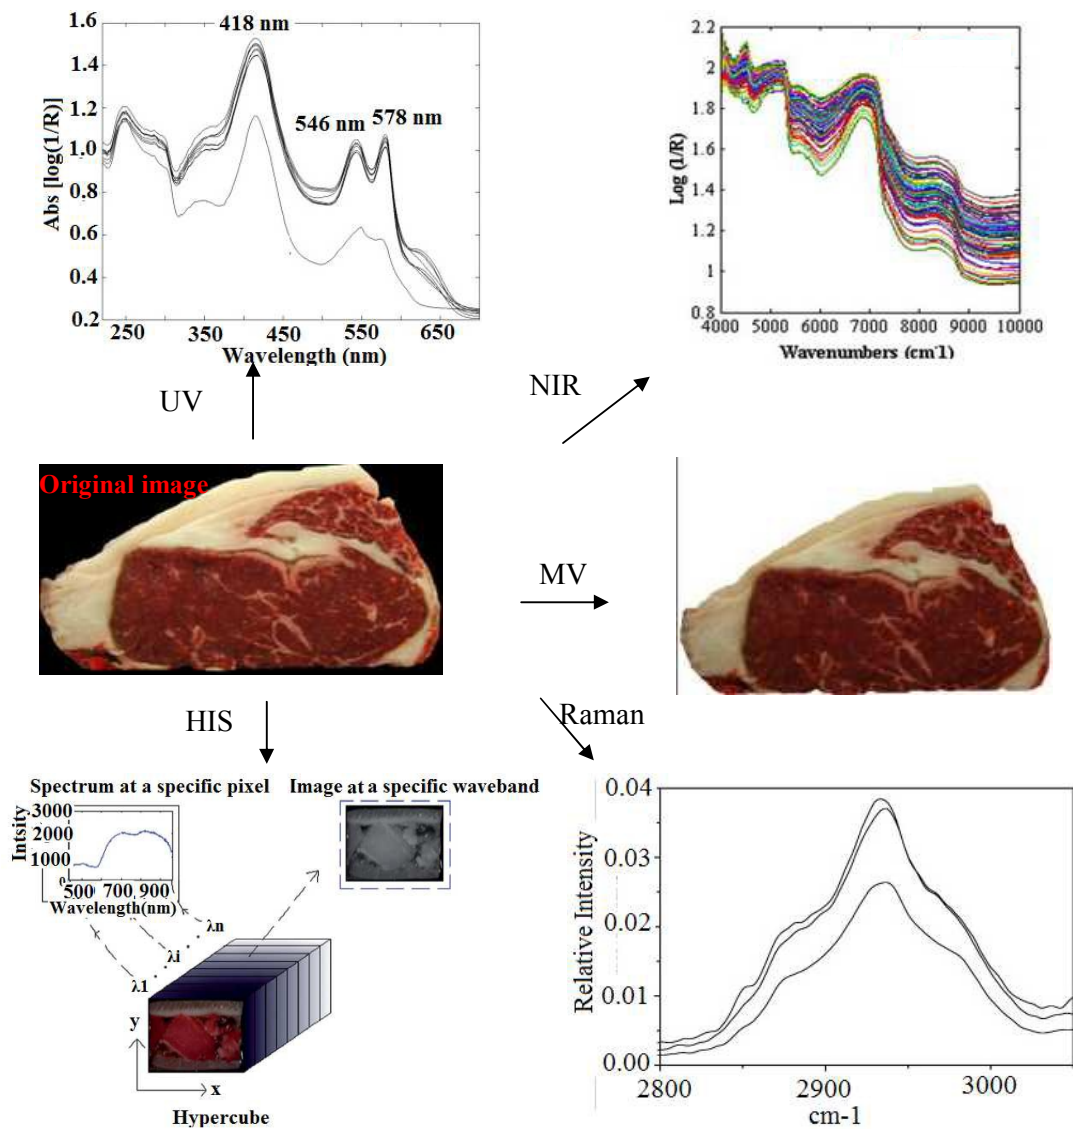


Fig. 5.

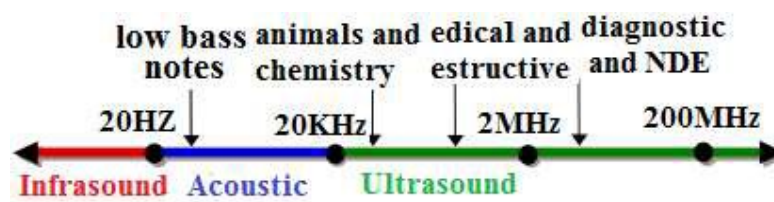


Fig. 6.

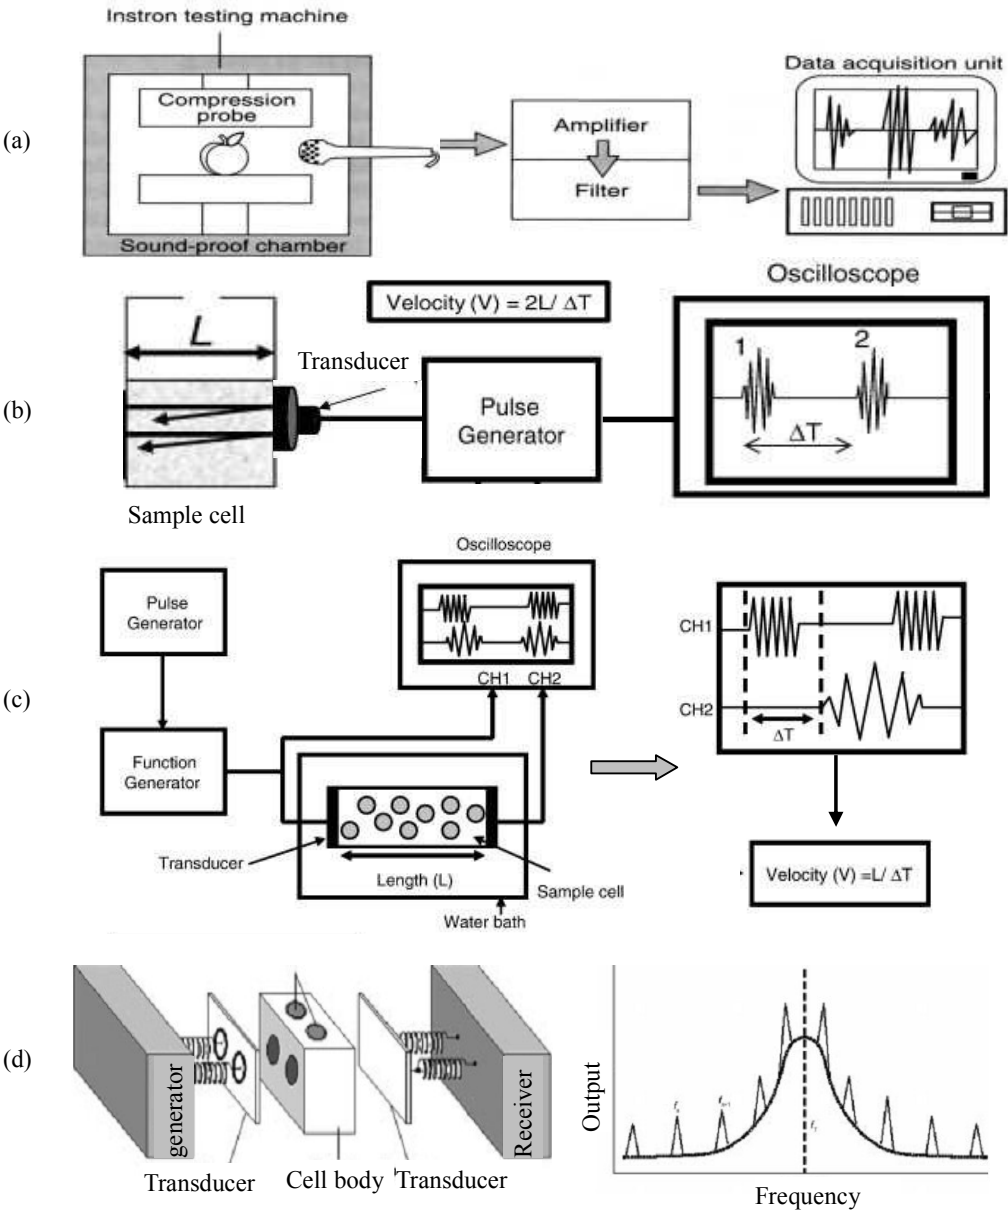


Fig. 7.



(a)



(b)

Fig. 8.

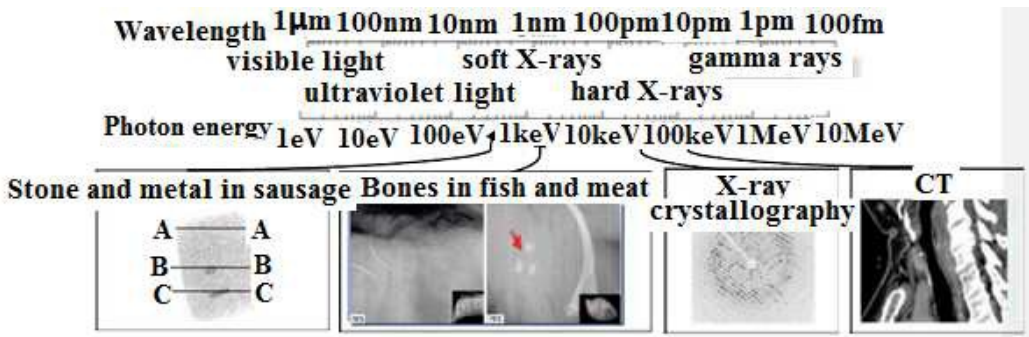


Fig. 9.

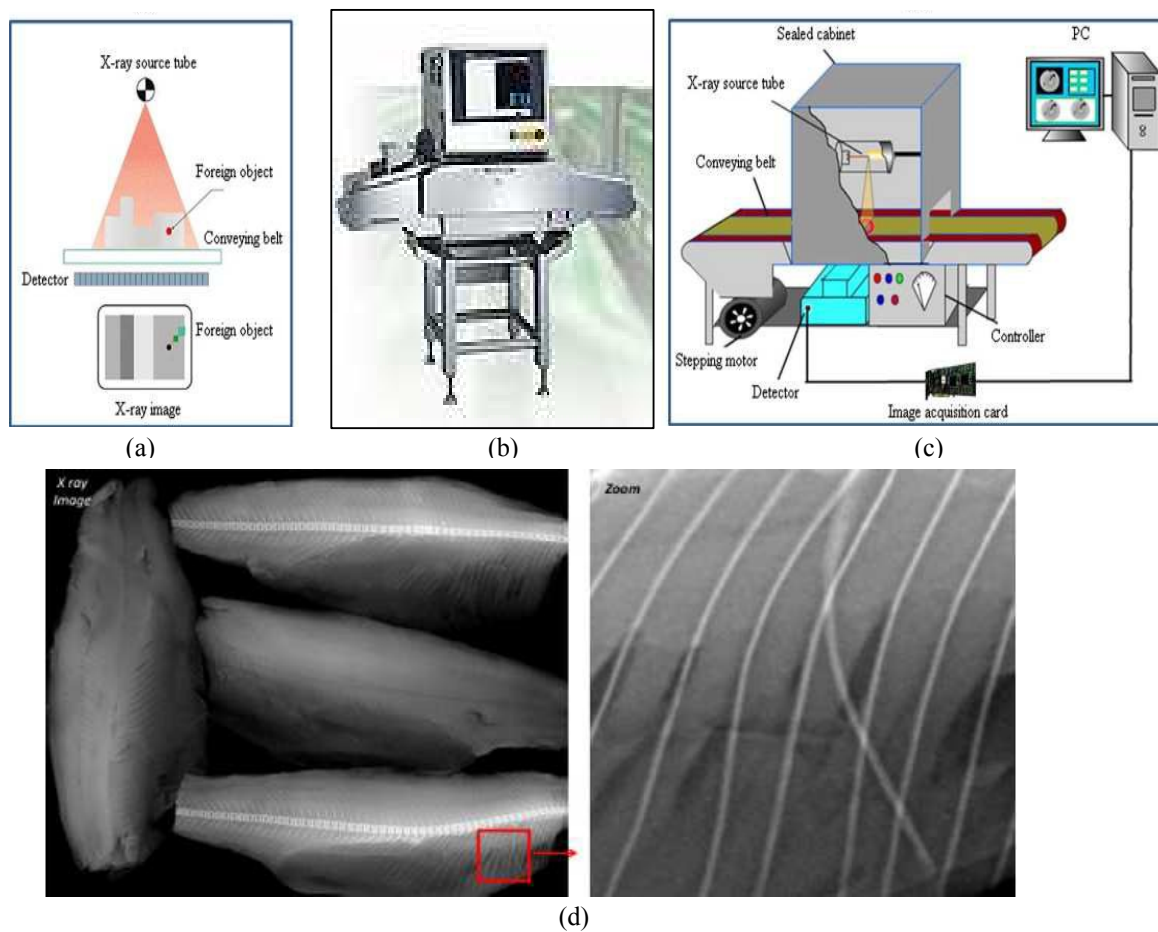


Fig. 10.

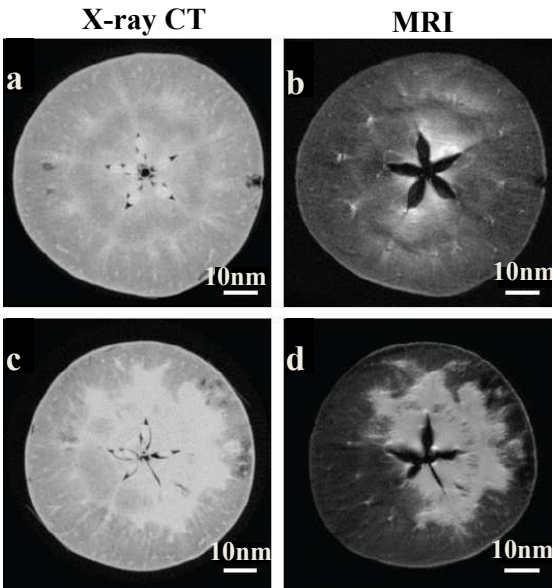


Fig. 11.

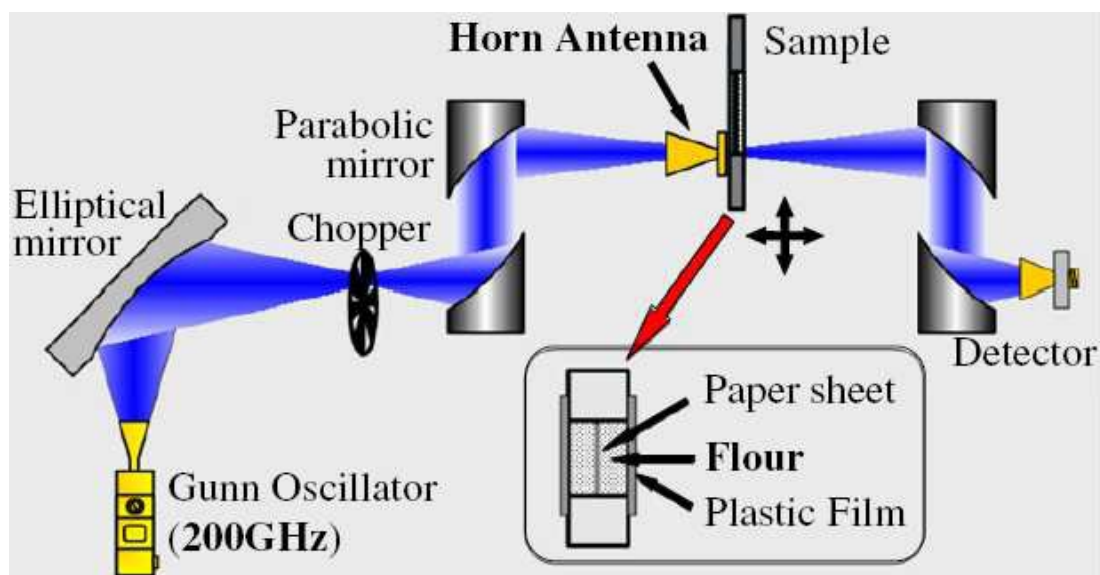


Fig. 12.

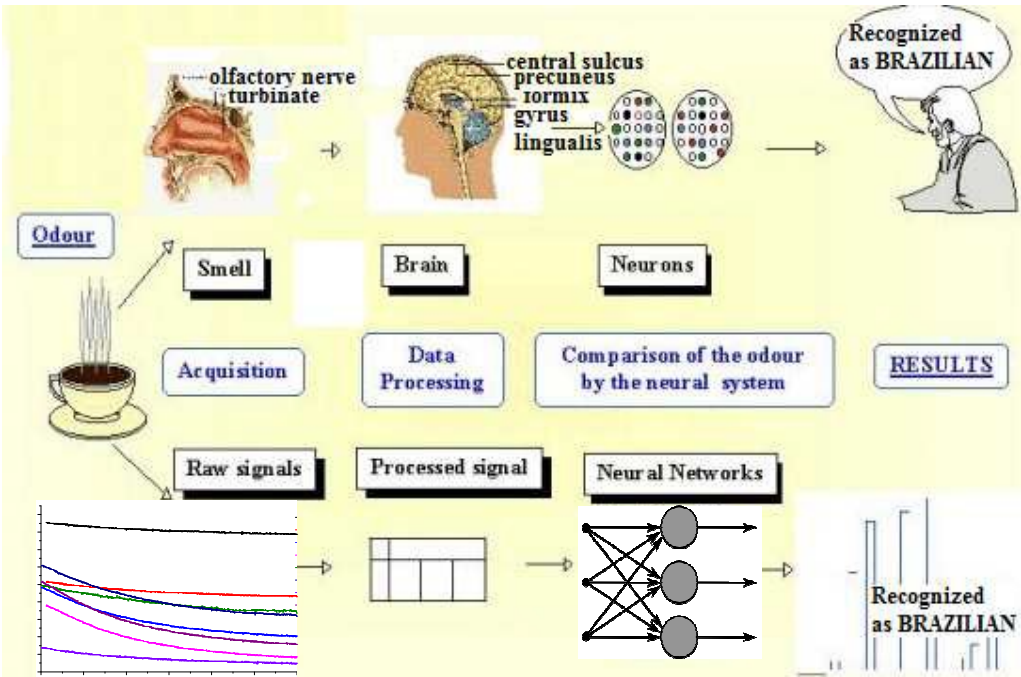


Fig. 13.

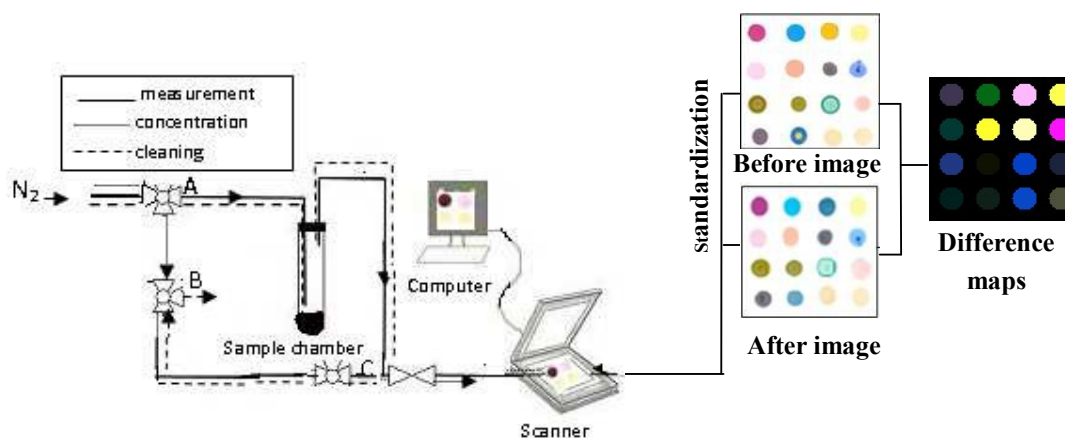


Fig. 14.

