

# Monitoring biofilm growth and dispersal in real-time with impedance biosensors

Matthew McGlennen <sup>1,2</sup>, Markus Dieser <sup>1,3</sup>, Christine M. Foreman <sup>1,3</sup>, Stephan Warnat <sup>1,2</sup>

<sup>1</sup>Center for Biofilm Engineering, Montana State University, Bozeman, MT 59717, USA

<sup>2</sup>Mechanical and Industrial Engineering, Montana State University, Bozeman, MT 59717, USA

<sup>3</sup>Chemical and Biological Engineering, Montana State University, Bozeman, MT 59717, USA


Correspondence should be addressed to: Stephan Warnat, Montana State University, Roberts Hall 304, Bozeman, MT 59717, USA. Phone: +(406) 994-6284; Fax: (406) 994-6292; E-mail: [stephan.warnat@montana.edu](mailto:stephan.warnat@montana.edu)

**Abstract:** Microbial biofilm contamination is a widespread problem that requires precise and prompt detection techniques to effectively control its growth. Microfabricated electrochemical impedance spectroscopy (EIS) biosensors offer promise as a tool for early biofilm detection and monitoring of elimination. This study utilized a custom flow cell system with integrated sensors to make real-time impedance measurements of biofilm growth under flow conditions, which were correlated with confocal laser scanning microscopy (CLSM) imaging. Biofilm growth on EIS biosensors in basic aqueous growth media (tryptic soy broth, TSB) and an oil–water emulsion (metalworking fluid, MWF) attenuated in a sigmoidal decay pattern, which lead to an ~22–25% decrease in impedance after 24 Hrs. Subsequent treatment of established biofilms increased the impedance by ~14% and ~41% in TSB and MWF, respectively. In the presence of furanone C-30, a quorum-sensing inhibitor (QSI), impedance remained unchanged from the initial time point for 18 Hrs in TSB and 72 Hrs in MWF. Biofilm changes enumerated from CLSM imaging corroborated impedance measurements, with treatment significantly reducing biofilm. Overall, these results support the application of microfabricated EIS biosensors for evaluating the growth and dispersal of biofilm *in situ* and demonstrate potential for use in industrial settings.

**One-Sentence Summary:** This study demonstrates the use of microfabricated electrochemical impedance spectroscopy (EIS) biosensors for real-time monitoring and treatment evaluation of biofilm growth, offering valuable insights for biofilm control in industrial settings.

**Keywords:** Biofilm, Quorum-sensing inhibition, Biocide, Electrochemical impedance spectroscopy, Biosensor, Metalworking fluid

## Graphical abstract

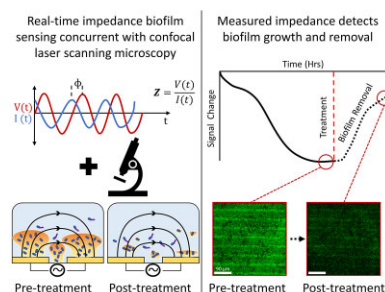

The accurate real-time detection of biofilm growth and removal is effectively demonstrated through the combination of impedance biosensors and high-resolution confocal laser scanning microscopy.

## Introduction

Biofilms are complex, structured microbial communities encased in a self-produced extracellular polymeric substance (EPS) adhered to surfaces. The formation of biofilms is the most common mode of growth for microorganisms on Earth (Costerton et al., 1999) and provides protection from chemical, mechanical, and physical stressors, improves evasion of host defense mechanisms, and increases virulence factors (Lappin-Scott & Costerton, 1989; Azeredo et al., 2017). Globally, microbial biofilm contamination

is a problem in natural, industrial, and medical settings, costing roughly \$4 trillion annually (Cámara et al., 2022).

Current standard techniques to assess/identify biofilm growth vary in analysis time, sensitivity, cost, and complexity. Standard wet lab techniques include plate counts, dip slides, polymerase chain reactions (PCR), enzyme-linked immunosorbent assays (ELISA), fluorescent *in-situ* hybridization (FISH), and spectroscopic methods such as infrared, ultraviolet, and visible light spectroscopy (Saha & Donofrio, 2012; Saha et al., 2012; Assenhaimer et al., 2017; Kiefer et al., 2018; Passman & Küenzi, 2020).

Received: May 19, 2023. Accepted: August 22, 2023.

© The Author(s) 2023. Published by Oxford University Press on behalf of Society of Industrial Microbiology and Biotechnology. This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<https://creativecommons.org/licenses/by/4.0/>), which permits unrestricted reuse, distribution, and reproduction in any medium, provided the original work is properly cited.

Microsensors have been designed to detect biofilm by changes in oxygen, pH, and temperature (Funari & Shen, 2022; Saccomano et al., 2021) to name a few. Each technique shows both strengths and weaknesses based on its application, highlighting the lack of a one-size fits all approach. Moreover, many of these techniques are destructive endpoint diagnostic tools and cannot be easily deployed to assess in real-time the onset of biofilm formation up to maturation and treatment response.

Over the last decade, microfabricated electrochemical impedance spectroscopy (EIS) biosensors have expanded to the field of microbiology. Compared to standard microbiology techniques, EIS biosensors can obtain information about microbes both in planktonic (Mallén-Alberdi et al., 2016; Brosel-Oliu et al., 2018; McGlennen et al., 2020; Sidhu et al., 2020) and biofilm stages (Chabowski et al., 2017; Huiszoon et al., 2021; Liu et al., 2018). In general, EIS is a technique used to characterize electrochemical properties of solids, liquids, and gases, and is achieved by supplying a sinusoidal electrical perturbation to an electrochemical system and measuring the time-varying response. The measurement is carried out across a frequency sweep (typically  $\sim 1$  MHz–1 mHz) (Magar et al., 2021). When applied to biosensors, changes to EIS spectra over time can indicate the presence of microbes at or near the sensor surface. Furthermore, impedance measurements can be carried out at single frequencies, which reduce data acquisition time, simplify analysis, and improve efficiency. Most recently, McGlennen et al. showed that microfabricated EIS sensors using optimized single-frequency impedance measurements could differentiate stages of biofilm growth, starting with the initial attachment of cells through the maturation of biofilm (McGlennen et al., 2023). Based on sensor characteristics and affinity, the analytical detection limit of microfabricated EIS sensor measurements can be less than 10 colony-forming units (CFUs)  $\text{mL}^{-1}$  (Abdelrasoul et al., 2020). Moreover, EIS sensors are noninvasive and label free, making them desirable for industrial applications and could be expanded into the analysis of formulated liquids.

Biofilm formation is a complex biological process, beginning with initial attachment of cells, proliferation, maturation, and subsequent detachment. Biofilm management has been approached by targeting both the formation process of biofilms and their eradication. Focus has been placed on various additives that interfere with bacterial signaling pathways [i.e., quorum sensing (QS)] or disrupt extracellular DNA, proteins, lipopolysaccharides, and exopolysaccharides during early stages of biofilm formation (Lu et al., 2019; Ozcan et al., 2019). Alternative strategies have also been explored, including the development of antiadhesion coatings, material modifications (Lisoñ et al., 2022; Rather et al., 2021), or incorporation of mechanical removal procedures (Sadekuzzaman et al., 2015). Nonetheless, the use of antimicrobials largely remains the standard approach to prevent and remove biofilm (Bott, 2009; Di Pippo et al., 2018). Despite extensive efforts to remove biofilms, microbial contaminants persist, leading to rapid recolonization (Davies, 2003; Stoodley et al., 2004; Stewart et al., 2019; Trafny, 2013). Mature biofilms consist of cells securely attached to the substrate, encased by protective EPS making them resistant to chemical and mechanical forces (Lebeaux et al., 2014; Peterson et al., 2015). Compared to mature biofilms, early-stage biofilms are less securely established, less resistant to antimicrobials, and more susceptible to other chemical treatments (Fu et al., 2021; Høiby et al., 2001). Thus, it is postulated that early detection and treatment could be a highly effective strategy for combating biofilm.

The potential of EIS biosensors to detect early-stage biofilm formation makes them a particularly attractive tool for combatting biofilms. Herein, EIS biosensors were deployed to monitor treatment responses using commercially available anti-biofilm compounds that target a range of different control strategies [e.g., chlorine, biocide, and quorum-sensing inhibitor (QSI)]. Furthermore, the EIS biosensors were tested against biofilms grown in metalworking fluid (MWF), a mixture of oils, emulsifiers, and other additives, to extend their utility beyond simple aqueous environments, as biofilm contamination poses a significant problem in industrial settings (Passman & Küenzi, 2020).

## Material and Methods

### System Overview


A three-dimensional (3D) printed flow cell system with integrated interdigitated electrode ( $\mu$ IDE) sensors was designed to monitor the growth and treatment of biofilm in a controlled manner, as previously described (McGlennen et al., 2023). The overarching methodology for using the system is depicted graphically (Fig. 1). Briefly, biofilm growth occurs within flow chambers composed of a microfabricated sensor as the bottom substrate, and a glass microscope slide serving as the top substrate viewing chamber (Fig. 1b). Single-frequency impedance analysis indicates the initial attachment of cells to the sensor substrate, early-stage irreversible biofilm proliferation, mature biofilm establishment, and changes due to detachment and regrowth of biofilm (Fig. 1c). Abiotic baseline impedance starts at 0% and decreases correspondingly to increasing biofilm biomass. Impedance changes tend to reach a maximum and stabilize upon uniform biofilm substrate coverage. At this stage, biofilm treatment is introduced, reducing biofilm biomass, and the impedance response correspondingly increases.

### Sensor Design

$\mu$ IDEs were selected for this application as they have proven to be easily fabricated, are highly sensitive, and do not require the use of a reference electrode (Dorledo de Faria et al., 2019; Furst & Francis, 2019; Park et al., 2018). EIS sensors were microfabricated as previously described (McGlennen et al., 2023). Briefly, the sensor design consisted of interdigitated electrodes 15  $\mu\text{m}$  in width with a spacing of 10  $\mu\text{m}$  for a total of 50 electrode pairs. Sensor surfaces were modified with poly (4-styrenesulfonic acid) doped with pyrrole, termed PPy:PSS, to enhance electrochemical stability and increase sensitivity. One side of each of the  $\mu$ IDEs was coated with 450  $\mu\text{C}$  PPy:PSS before experimentation (McGlennen et al., 2023).

### Flow Cell Operation

Biofilm cultivation was carried out in 3D-printed flow cell systems (McGlennen et al., 2023). Briefly, the flow cell was filled with sterile media (i.e., 1:10X TSB or 5% MWF), and an initial EIS measurement was collected. Subsequently, 1 mL of cell culture enrichments were injected into the flow chambers and left to adhere to the sensor surface for 2 Hrs. Following the 2 Hrs of incubation, a continuous flow of sterile media was initiated into the flow chambers at a rate of 1  $\mu\text{L min}^{-1}$  (Genie Touch Syringe Pump, Kent Scientific, USA). Abiotic (no biofilm) control trials were used to determine the effect of treatment amendments on impedance following the same procedure.

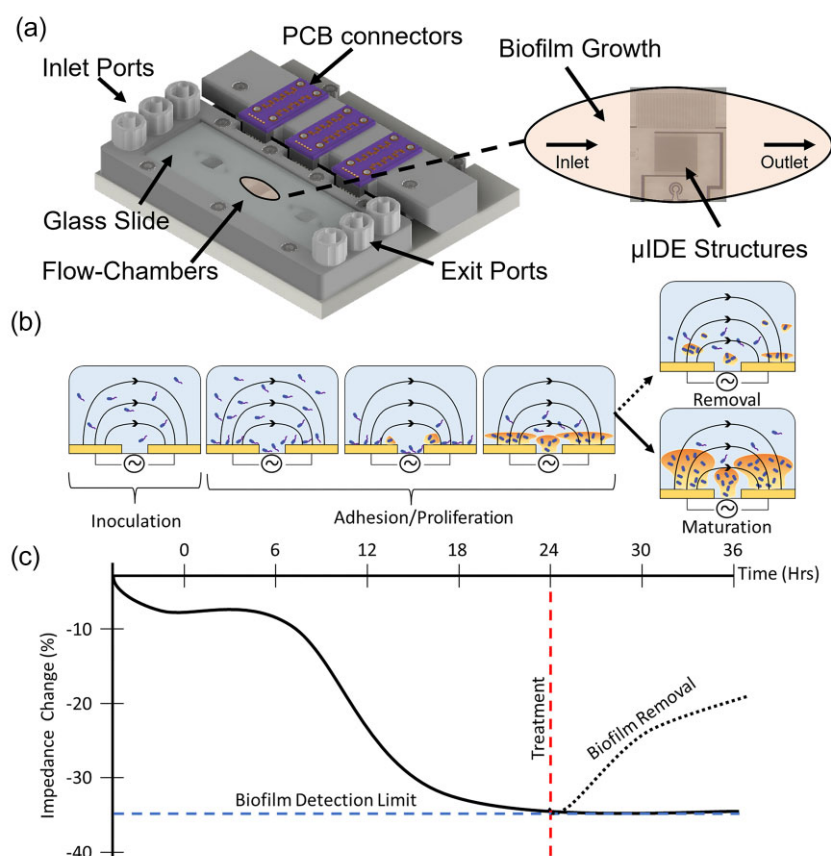

**Fig. 1.** Graphical representation of platform design and experimental setup for analyzing biofilm: (a) 3D printed flow cell system CAD rendering with detailed top view of flow chamber with integrated EIS biosensor for biofilm growth and analysis, (b) cross-section schematic of biofilm development stages on EIS biosensor electrodes within flow chambers, and (c) anticipated impedance changes in response to biofilm growth and removal.

## Bacterial Strain Selection and Culturing Conditions

The model biofilm-forming bacterial strain *Pseudomonas aeruginosa* PA01 expressing green fluorescent protein (GFP) was used (Nivens et al., 2001). Freezer stocks were transferred to tryptic soy agar (TSA; Fischer Scientific, USA) plates and incubated at 37°C for 24 Hrs. All cell cultures were grown in the presence of 50  $\mu\text{g ml}^{-1}$  of carbenicillin (Fisher Scientific, USA). Enrichments were made from single colonies grown in 1X tryptic soy broth (TSB; Fisher Scientific, USA) at 37°C while shaking at 150 RPM for 18 Hrs.

Following 18 Hrs of incubation, enrichments were harvested by centrifugation at 10 000  $\times g$  for 5 min. The resulting cell pellets were either resuspended in 1:10X TSB or an industrial oil-water emulsion (i.e., SC-506 CF metalworking fluid (MWF), Hangsterfer's, USA). Cells, which were resuspended in 1:10X TSB, were incubated at 22°C while shaking at 150 RPM for 6 Hrs to allow cells to adjust to ambient conditions selected for biofilm growth in the flow cell. Enrichments were harvested at an optical density at a wavelength of 600 nm of  $\text{OD}_{600} = 0.2$ , resulting in a cell concentration of  $\sim 1 \times 10^8$  CFUs  $\text{mL}^{-1}$ . For assays in MWF, cells were washed twice in autoclaved municipal tap water before resuspending cell pellets in autoclaved municipal tap water mixed with MWF (final concentration 5% v/v). The cell concentration of the final mixture was  $\sim 1 \times 10^8$  CFUs  $\text{mL}^{-1}$ . All enrichments were transferred to 10 mL sterile luer lock syringes (Becton Dickinson, USA), equipped with 20  $\frac{1}{2}$  ga. needles (Fisher Scientific), prior to injection into flow chambers.

## Biofilm Treatment

The effects of three different biofilm treatments were investigated. After 24 Hrs of growth in the flow cell, established biofilms were treated with either chlorine (Sodium hypochlorite solution; 20% w/v, Sigma-Aldrich, USA) or a biocide (Proxel GXL; Lonza Inc., USA). Treatment concentrations were 1.41 mM chlorine and 0.1% biocide (v/v) in 1:10X TSB and 1.0% biocide (v/v) in 5% MWF. The chlorine concentration was chosen as it has been shown to disperse biofilm in a flow-cell-based system with only partial destruction of biomass (Davison et al., 2010). Proxel GXL was applied at concentrations of 4X and 40X above the recommended minimum inhibitory concentration for planktonically growing *P. aeruginosa*, respectively (Lonza Inc., USA). Chlorine solutions were manually injected as a one-time treatment into each of the three flow chambers (Fig. 1b) at a rate of 1  $\text{mL min}^{-1}$  for 1 min. Sterile media flow was paused during chlorine injection and resumed thereafter at a flowrate of 1  $\mu\text{L min}^{-1}$  for 12 Hrs. Biofilm was in contact with chlorine for  $\sim 1.5$  Hrs. Conversely, the biocide Proxel GXL was applied as a continuous treatment, in accordance with the manufacturer's recommendations. Sterile media were exchanged with media containing biocide and applied at a flowrate of 1  $\mu\text{L min}^{-1}$  for 12 Hrs.

As a third treatment, biofilm formation was suppressed by targeting QS, a communication process between bacterial cells that regulates the growth and behavior of the microbial population (Miller & Bassler, 2001). Biofilm formation was investigated both in the presence and absence of the quorum-sensing

inhibition (QSI) reagent (Z-)-4-Bromo-5-(bromomethylene)-2(5H)-furanone (Furanone C-30; Sigma-Aldrich, USA). Cells, either resuspended in 1:10X TSB or MWF as described above, were supplemented with 75  $\mu\text{M}$  Furanone C-30, as this concentration showed high efficiency at reducing biofilm formation (Ozcan et al., 2019). Enrichments were incubated for 60 min at 22°C while shaking at 150 RPM to allow time for the QSI inhibitor to block cell communication prior to flow chamber injection. After inoculating the flow chambers, 75  $\mu\text{M}$  Furanone C-30 mixed with 1:10X TSB or 5% MWF was continuously supplied at a flowrate of 1  $\mu\text{L min}^{-1}$  for either 36 Hrs for 1:10X TSB or 72 Hrs for 5% MWF.

## Electrochemical Impedance Spectroscopy Measurement

EIS measurements were carried out with a Hioki IM3533 LCR (inductance (L), capacitance (C), and resistance (R)) meter connected to a Keysight 970A data acquisition system (DAQ) with a DAQ905A RF 2 GHz Dual 1:4 RF Multiplexer, 50 ohm switching module. The instruments were controlled by a custom-built virtual interface (VI; LabView 2017), providing multiplexed four-channel EIS measurements. During EIS data collection, PPY:PSS-coated sensors were connected to the LCR meter such that the coated side of the  $\mu\text{IDEs}$  served as both the counter electrode (CE) and reference electrode (RE). Impedance spectra were collected every 30 min across a frequency range of 200 kHz–100 Hz and 25 logarithmically spaced data points with a signal source that was a sine wave with an amplitude of 10 mV RMS and no DC bias for both 1:10X TSB and 5% MWF. A previous study showed that biofilm detection was most sensitive using 1.26 kHz as the source frequency for impedance measurements in 1:10X TSB (McGlennen et al., 2023). The single frequency that best captured biofilm growth in 5% MWF was 200 kHz (see Supplemental Material). In both cases, time-dependent changes to impedance were reported as given by Equation (1):

$$\text{Impedance Change (\%)} = \frac{|Z_{(f,t)}| - |Z_{(f,t_0)}|}{|Z_{(f,t_0)}|} * 100\%, \quad (1)$$

where  $|Z_{(f,t_0)}|$  is the impedance measurement at the selected frequency of interest ( $f$ ), measured at the initial timepoint ( $t_0$ ), and  $|Z_{(f,t)}|$  is every subsequent impedance measurement.


## Biofilm Assessment with Confocal Laser Scanning Microscopy and Image Analysis

Biofilm experiments and EIS data collection were performed while the flow cell was mounted on a confocal laser scanning microscope (CLSM; SP5 upright confocal, Leica, USA). GFP-expressing *P. aeruginosa* PAO1 was used for all biofilm-related experiments, allowing visualization under the microscope without the need of staining (Nivens et al., 2001). Total biovolume from each CLSM image stack was calculated using Imaris 9.8 surfaces analysis with a custom fluorescence intensity filter and by eliminating particle sizes smaller than 2  $\mu\text{m}$ . The resulting calculation represents the total biovolume present in each confocal stack. The data presented here were normalized to the field of view by using Equation (2), similarly to Lim et al. (2016), creating a biofilm index.

$$\text{Biofilm Index} = \frac{\sum \text{Total Biovolume } (\mu\text{m}^3)}{\text{Field of View } (\mu\text{m}^2)}. \quad (2)$$

## Statistical Analyses

Data were processed with Matlab 2021a. Significant impedance changes and biofilm index differences were analyzed using an

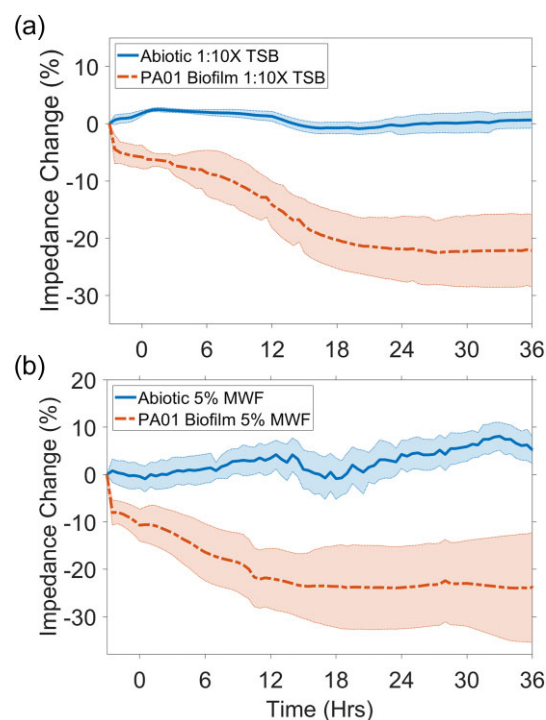

**Fig. 2.** Impedance changes for abiotic controls and biofilm growth in (a) 1:10X TSB and (b) 5% MWF. Shaded regions represent standard deviation.

unpaired t-test. Student's t-test determined statistical differences between EIS data.

## Results

### Real-time Impedance Measurements of Biofilm Growth

The flow cell allowed for nondestructive, real-time visualization of biofilm growth and removal without disruption in flow and EIS measurements (Fig. 1). To establish a baseline understanding of the effect of media and the absence/presence of microbial cells, impedance was measured at 1.26 and 200 kHz in 1:10X TSB and 5% MWF, respectively, every 30 min for 36 Hrs (Fig. 2).


Under continuous flow of abiotic 1:10X TSB, impedance remained stable (Fig. 2a,  $\leq 4\%$  variation) and displayed no statistical difference between 0 and 36 Hrs (t-Test,  $p$ -value  $\geq 0.079$ ). Injection of planktonic cells into the flow chambers resulted in an instantaneous decrease of  $\sim 5\%$  in impedance. When flow was initiated after 2 Hrs of seeding (i.e., 0 Hr) impedance decreased in a sigmoidal decay pattern until reaching a plateau at  $\sim -22\%$  by 24 Hrs of growth (24–36 Hrs, t-Test,  $p$ -value = 0.956). Visual confirmation of the different biofilm stages from seeding to monolayer establishment in relation to EIS can be found in McGlennen et al. (2023).

Similar to impedance changes in 1:10X TSB, impedance displayed no statistical difference between 0 and 36 Hrs of continuous flow under abiotic conditions in 5% MWF (t-Test,  $p$ -value  $\geq 0.051$ ). In the presence of cells, impedance attenuated in a sigmoidal decay pattern, reaching a plateau of  $\sim -25\%$  by 24 Hrs of growth (24–36 Hrs, t-Test,  $p$ -value = 0.996).

### Real-time Impedance Measurements of Biofilm Treatment

To investigate biofilm removal using EIS biosensors, 24-Hr biofilms were treated with either 1.41 mM chlorine or 0.1% biocide. The



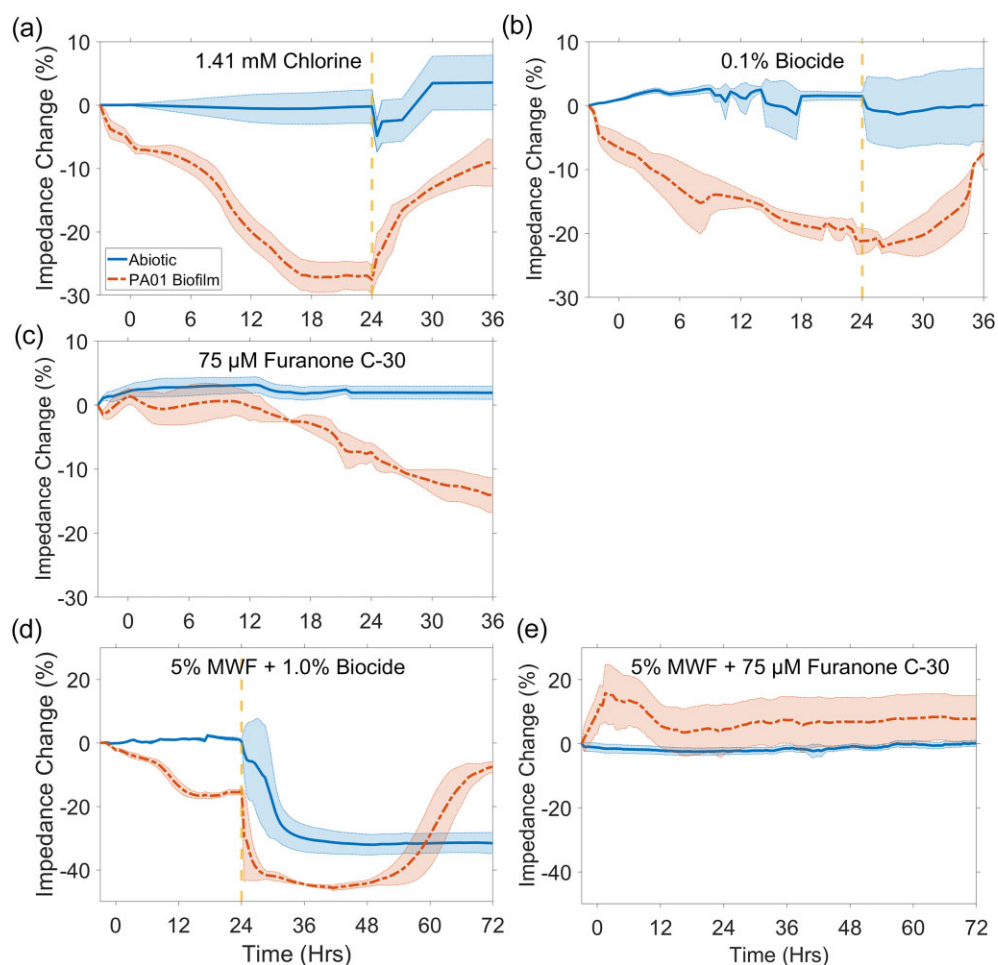

**Fig. 3.** Impedance changes at 1.26 kHz over time for abiotic controls and biofilm grown in 1:10X TSB: (a) treated at 24 Hrs with 1.41 mM chlorine, (b) treated at 24 Hrs with 0.1% biocide, (c) exposed to 75 µM furanone C-30 for 36 Hrs. Impedance changes at 200 kHz over time for abiotic controls and biofilm grown in 5% MWF, (d) treated at 72 Hrs 1.0% biocide, and (e) exposed to 75 µM furanone C-30 for 72 Hrs. Shaded regions represent standard deviation. Dashed line indicates time of treatment implementation.


addition of these agents altered the electrochemical properties of 1:10X TSB and 5% MWF, and hence, the impedance baseline. Effects on impedance were noisier in the abiotic media compared to biosensors overgrown with biofilm, which increased impedance variability by 10 and 7% on average in abiotic 1:10X TSB and 5% MWF, respectively (Fig. 3a,b). The addition of chlorine decreased impedance sharply by ~5% in abiotic 1:10X TSB and plateaued 6 Hrs after treatment with an overall impedance increase of ~5% (Fig. 3a). Impedance changes caused by the addition of chlorine and biocide to 1:10X TSB were, however, not statistically significant (t-test,  $p$ -value  $\geq 0.414$ ; Fig. 4). In 5% MWF, the addition of the biocide triggered a large drop in impedance of ~30% before stabilizing 12 Hrs later for both abiotic sensors and sensors exposed to biofilm (Fig. 3d). Impedance remained stable between 36 and 72 Hrs in abiotic 5% MWF (t-Test,  $p$ -value = 0.339; Fig. 4); thus, the impedance at 36 Hrs was selected as the new baseline for treatment effect calculations.

All biosensors covered with biofilm reflected a treatment response upon contact with chlorine and biocide, with impedance changes nearing abiotic baselines (Fig. 3). Differences were evident with respect to response time. Impedance changes for biosensors treated with a one-time injection of chlorine were instant and followed a saturation curve pattern (Fig. 3a). During continuous treatment of biofilm in both 1:10X TSB and 5% MWF with a bio-

cide, impedance changes followed a sigmoidal pattern with a pronounced lag phase (Fig. 3b,d). Overall, impedance increased by  $13 \pm 3\%$  and  $14 \pm 3\%$  for chlorine and biocide-treated biofilms in 1:10X TSB, respectively, and by  $41 \pm 3\%$  for biocide-treated biofilms in 5% MWF. Importantly, changes in impedance were statistically significantly different between key timepoints of pre-treatment (24 Hrs) and post-treatment (36 Hrs) for EIS biosensors treated with chlorine (t-Test,  $p$ -value = 0.003) and biocide (t-Test,  $p$ -value = 0.002) in 1:10X TSB (Fig. 4). Likewise, in response to biofilm treated with biocide in MWF, the impedance change was statistically different between pre-treatment (36 Hrs) and post-treatment (72 Hrs) (t-Test,  $p$ -value < 0.001).

### Real-time Impedance Measurements of Delayed Biofilm Development

To investigate whether EIS biosensors could monitor the effects of QSI on biofilm formation, cell enrichments were grown in the presence of 75 µM of the QSI compound furanone C-30 for 36 and 72 Hrs in 1:10X TSB and 5% MWF, respectively. Electrochemically, the addition of furanone C-30 had negligible effects on impedance (Fig. 3c,e). Compared to 0 Hr, impedance remained stable in abiotic 1:10X TSB (t-test,  $p$ -value = 0.811) and abiotic MWF (t-test,  $p$ -value = 0.246) for 36 and 72 Hrs, respectively. Impedance

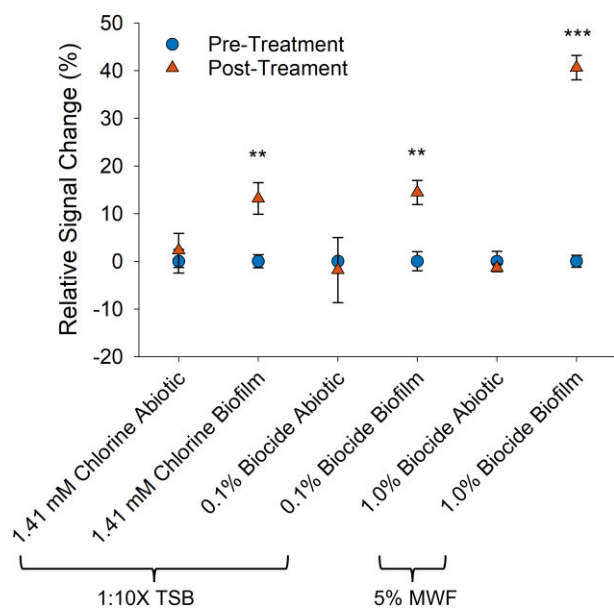

**Fig. 4.** Magnitude of impedance change between pre-treated and post-treated biofilm grown in 1:10X TSB and 5% MWF. Error bars indicate standard deviation. Differences that met significant levels are shown as \* $\leq 0.05$ , \*\* $\leq 0.01$ , \*\*\* $\leq 0.001$ .

indicated that biofilm proliferation was suppressed in 1:10X TSB and 5% MWF for 18 and 72 Hrs, respectively (t-test,  $p$ -value  $\geq 0.329$ ; Fig. 3c and e). In 1:10X TSB, changes in impedance became statistically different from 0 Hr after 18 Hrs (t-test,  $p$ -value = 0.016). A gradual decrease in impedance, reaching  $\sim 17\%$  by 36 Hrs, suggested that cells eventually overcame the inhibitory effects of furanone C-30 and biofilm began to develop.

### Validation of Biofilm Removal and Delay By CLSM Imaging

CLSM imaging was used to confirm biofilm development and treatment in 1:10X TSB media but was not possible in 5% MWF as the fluid is opaque. CLSM images at key timepoints of pre-treatment (24 Hrs) and post-treatment (36 Hrs) were evaluated (Fig. 5). Consistently, biofilm monolayers attached to biosensor substrata had formed after 24 Hrs (Fig. 5a-1, b-1, and c-1) and continued to proliferate without treatment (Figs. 5a-2). Conversely, exposure to either chlorine or biocide removed biofilm (Figs. 5b-2 and c-2). Biofilm removal was quantified using Imaris 9.8 by calculating changes in biofilm index (B.I.; Equation 2) between pre-treatment and post-treatment. Chlorine and biocide treatment resulted in an average B.I. reduction of  $1.87 \pm 0.75 \mu\text{m}^3 \mu\text{m}^{-2}$  and  $2.13 \pm 0.89 \mu\text{m}^3 \mu\text{m}^{-2}$  between pre-treatment and post-treatment, respectively. Both treatments resulted in a significant reduction of biofilm when compared to biofilm without treatment (t-Test,  $p$ -value  $\leq 0.024$ ). Cells treated with  $75 \mu\text{M}$  furanone C-30 developed thinner biofilms, exhibiting  $\sim 40\%$  reduction in overall thickness compared to untreated biofilms (Fig. 6).

### Discussion


The developed platform consisted of EIS biosensors integrated into a microfluidic flow environment, allowing for impedance measurements that reflect naturally proliferating biofilm conditions. Live-cell imaging from CLSM supplemented impedance data as a nondestructive visual confirmation of adherent biofilm. The marriage of these characteristics makes the current report

unique in that biofilm growth under flow conditions and the expansion of the sensors into alternative fluids and QSI is explored. Extending findings by McGlennen et al. (2023) on linking biofilm growth to EIS measurements, this study assessed the applicability of impedance to monitor biofilm treatment and the application of QSI in real-time. The behavior of microfabricated sensors used to evaluate biofilm growth is highly dependent on the experimental setup, such as the type of media, flow characteristics (e.g., static vs. continuous flow), organism selection, electrode geometry (e.g., 2- vs. 3-dimensional), and selected frequency range (Furst & Francis, 2019; Subramanian et al., 2020; Funari & Shen, 2022). All of these factors complicate direct comparisons between reports.

In the present study, a flow-based system using  $\mu$ IDEs coated with an electrically conductive polymer (i.e., PPy:PSS), measured at an optimized single frequency (i.e., 1.26 and 200 kHz) was deployed. Impedance decreased in the presence of proliferating biofilm following sigmoidal decay curves (Figs. 2 and 3). Others have found a similar relationship between biofilm growth and impedance (Paredes et al., 2012, 2013, 2014; Subramanian et al., 2017; Huiszoon et al., 2019). These studies reported impedance changes ranging from  $\sim 10$  to  $\sim 40\%$ , and plateaus were reached between 10 and 48 Hrs, bracketing our findings of 20–25% before leveling off at  $\sim 24$  Hrs. Likewise, impedance in the low-frequency ranges (i.e., 10 Hz–10 kHz) was most representative of signals from the electrode/electrolyte interface and provided the highest sensitivity toward biofilm growth (McGlennen et al., 2023; Paredes et al., 2014). While the frequency range in 1:10X TSB growth medium was optimized at 1.26 kHz, this frequency was not suitable for MWFs. Industrial oil–water emulsions can form rigid dielectric barriers that hinder the mobility of charge carriers at the interface of the electrode (Perini et al., 2012), suggesting that higher frequencies may be more effective in measuring biofilm. We found that the most appropriate frequency range for measuring biofilm in 5% MWF was  $\geq 100$  kHz, as detailed in the supplemental information. However, it should be noted that the degree of hindrance to charge carriers can vary depending on the amount of water in the emulsion, and optimal sensor signal responses may need to be tailored to individual systems. MWF was chosen as a representative medium to test EIS biosensors since MWF is prone to *P. aeruginosa* biofilm contamination (Di Maiuta et al., 2017; Passman & Kuenzi, 2020). Importantly, EIS detected biofilm growth in MWF with the same degree of sensitivity as in 1:10X TSB (Figs. 2 and 3).

While the exact mechanisms behind the impedance decrease in response to biofilm are not fully understood, we hypothesize that biofilm metabolic processes modify ionic concentrations at the capacitive double-layer of the sensor electrodes. This leads to a decreased Debye length, and thus, an elevated capacitive double-layer that results in a decline in impedance (Huiszoon et al., 2019, 2021; McGlennen et al., 2023). Additionally, upon the production of EPS, electrochemically active metabolites such as phenazine, pyocyanin (PYO), or *Pseudomonas* quinolone signal (PQS) may become entrapped within the EPS matrix, leading to the accumulation of electrochemically active sites (Becerro et al., 2016; Bosire et al., 2016). Cells may also act as small capacitors, decreasing impedance (i.e., capacitance increase; Turick et al., 2019). Conversely, biofilm treatment causes damage to cells and/or disruption of the EPS matrix, and decreases metabolic processes, resulting in the release and subsequent decrease in the concentration of electroactive redox compounds. These compounds are then carried away by the flow, and thus, the impedance increases. With regards to these mechanisms, chlorine causes the detachment of biofilm clusters and the breakdown of metabolites



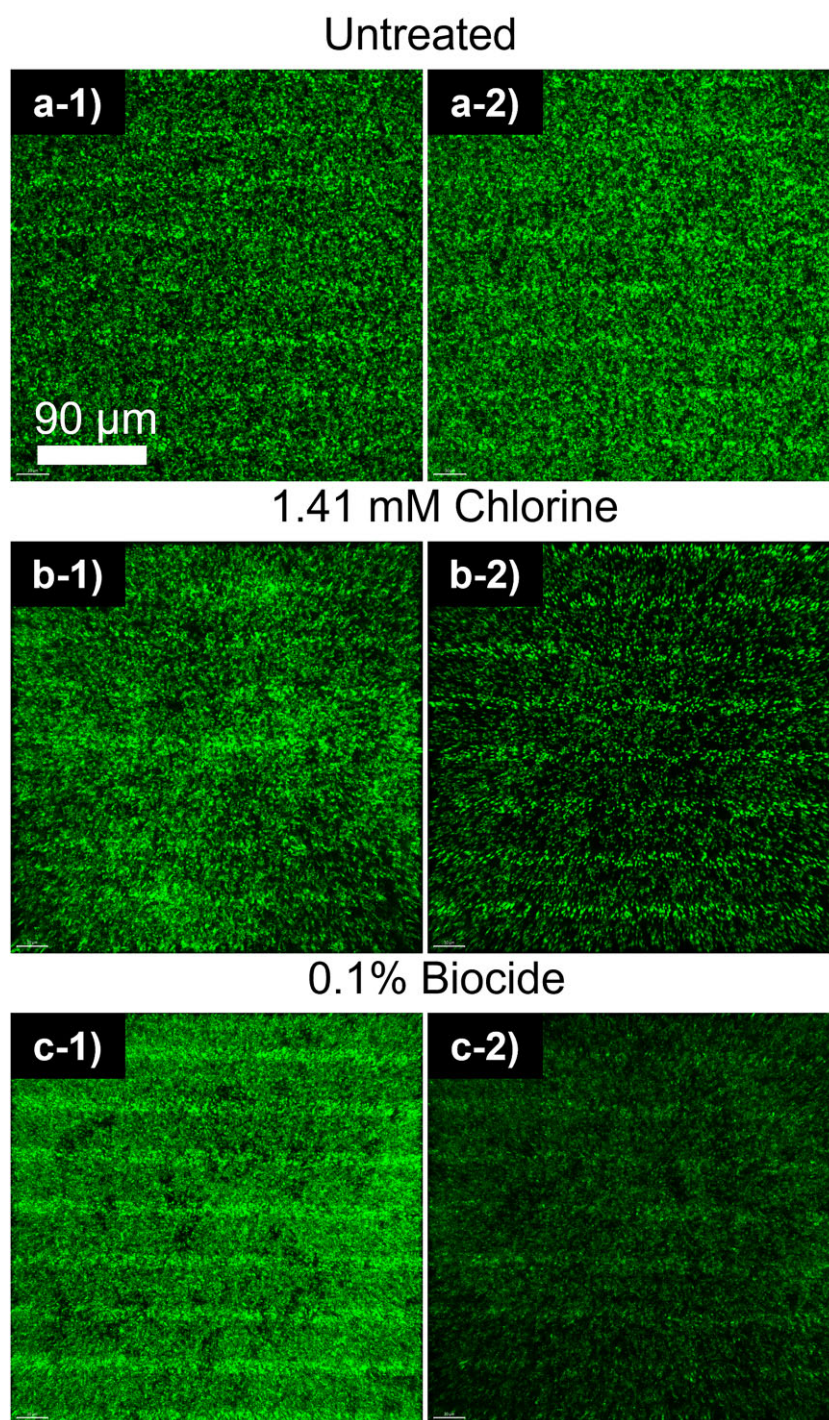


**Fig. 5.** CLSM images of (left panel: –1) pre-treatment (24 Hrs) and (right panel: –2) post-treatment (36 Hrs) biofilm. (a) Untreated, (b) chlorine treatment, and (c) biocide treatment. Scalebar represents 90  $\mu\text{m}$ .

by oxidation of organic materials (Davison et al., 2010), whereas 1,2-benzisothiazolinon-3-one (i.e., biocide) is believed to inhibit bacterial growth and metabolic activity (Green et al., 2018; Silva et al., 2020). Both chlorine and biocide treatments resulted in impedance increases (Figs. 3b and c). While indicative of biofilm reduction, impedance did not fully rise to abiotic levels. Further, the reduced slope of the impedance curves not only implied incomplete removal of biofilm but also that biofilm became less susceptible to the treatment. Incomplete biofilm removal was confirmed by CLSM (Fig. 5). The measured ~14% impedance in-

crease corresponded to an ~68% decrease in biomass. However, it is important to note that this study aimed to detect changes in impedance in response to biofilm treatment rather than optimizing biofilm treatment doses.

Furanone C-30 is a QSI compound and has been demonstrated to delay biofilm formation and maturation (Wu et al., 2004; He et al., 2012; Zhao et al., 2018). QS is a type of bacterial communication to sense and respond to cell population density, mediated by chemical signaling molecules (Mukherjee & Bassler, 2019). Briefly, the abundance of signaling molecules is low or absent

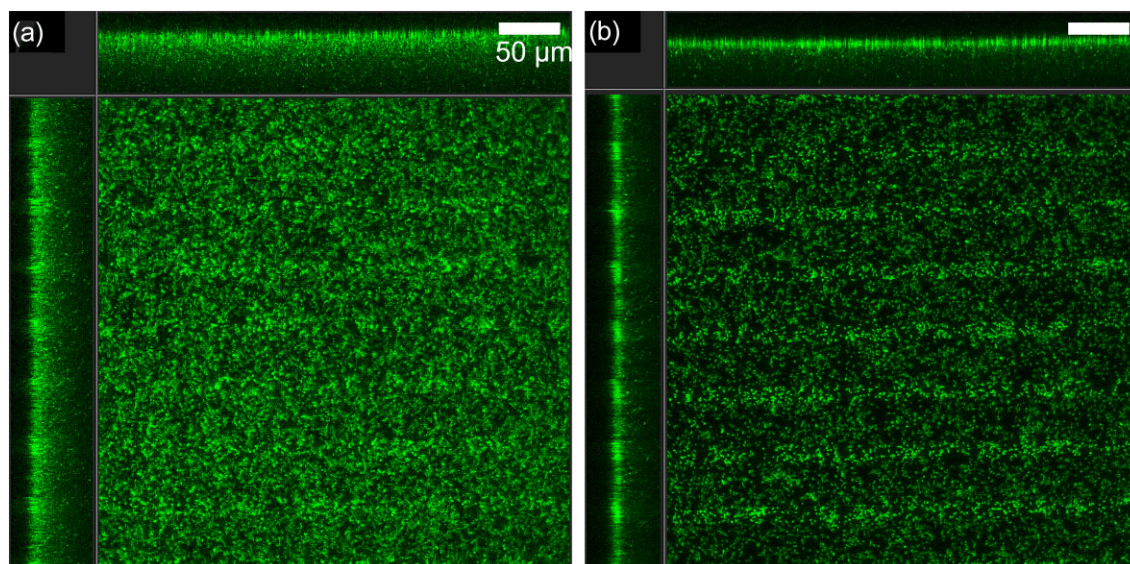

**Fig. 6.** CLSM images of (a) untreated biofilm at 36 Hrs, and (b) biofilm exposed for 36 Hrs to 75  $\mu\text{M}$  of the QSI compound Furanone C-30. Scalebar represents 50  $\mu\text{m}$ . Top and side panels show side-view profiles of biofilm z-stacks.

at low cell densities. The production, release, and extracellular concentration of signaling molecules increase as a function of growing cell density, ultimately triggering a synchronized cell population-wide response such as biofilm formation and architecture (Davey et al., 2003). As such, QS systems are autoregulated and depend on a threshold concentration of signaling molecules (Miller & Bassler, 2001). By destabilizing QS regulatory proteins, furanone C-30 decreases the synthesis of signaling molecules [i.e., acyl-homoserine lactones (AHLs) and PQS] (Markus et al., 2021; Skindersoe et al., 2008), which further downregulates the production of other redox mediators such as phenazine and PYO (Davies et al., 1998; Hentzer et al., 2003; Proctor et al., 2020). When biofilm was grown in the presence of furanone C-30, impedance remained unchanged for 72 Hrs in 5% MWF (Fig. 3e). In 1:10X TSB, impedance remained stable for 18 Hrs (Fig. 3c), and the subsequent decrease in impedance indicated that QSI was overcome. Ozcan et al. tested *P. aeruginosa* PAO1 biofilm growing in both TSB and MWF in the presence of furanone C-30, and reported lower concentrations of signaling molecules (PQS and AHLs) critical to biofilm development (Ozcan et al., 2019), affirming the potential role of these mediators in affecting impedance.

The use of  $\mu\text{IDEs}$  in combination with PPy:PSS electrode coatings results in highly sensitive biofilm detection and enhanced measurement integrity/repeatability (this study; McGlennen et al., 2023). Recent reviews have identified four criteria relevant for developing robust biofilm detection tools: Analytical techniques need to be (i) noninvasive (i.e., cannot perturb or damage biofilm), (ii) provide real-time analysis with high temporal and spatial resolution, (iii) be applicable to diverse analytes and settings, and (iv) be cheap, require low maintenance, and operate continuously for a long time (Funari & Shen 2022; Saccomano et al. 2021). The EIS biosensors developed herein hold promise to fulfill these criteria as they have the advantages of being able to be manufactured at low cost and can be configured for automated data collection and interpretation, all of which results in a higher efficiency and real-time evaluation of biofilm. To take advantage of the capabilities of EIS, further research is needed to better understand the mechanisms that drive changes in impedance. For instance, this study investigated the model

organism, *P. aeruginosa* PAO1, but other organisms likely have different electrochemical compositions. It will be necessary to assess the performance of these sensors in diverse biofilm compositions (e.g., mixed species and/or inter-kingdom), different types of supporting fluids (e.g., opaque, liquid formulations), and under varying environmental conditions (e.g., fluctuations in temperature, conductivity, or pH). If further validated, impedance sensors would be a significant advancement where biofilm contamination is prevalent and the reliance on current monitoring techniques are inadequate.

## Conclusion

In this study, microfabricated EIS biosensors were effective at assessing the growth and removal of *P. aeruginosa* biofilm in 1:10X TSB and 5% MWF. Additionally, EIS biosensors detected delayed effects of biofilm growth from targeting bacterial QS inhibition. The use of EIS biosensors holds great potential for the early detection and continuous monitoring of biofilms. Expanding our understanding of the sensors' uses and limitation beyond laboratory-based testing is vital to ensure future technological expansion into industrial, medical, and natural environments.

## Acknowledgments

Green fluorescent protein (GFP) expressing *Pseudomonas aeruginosa* PAO1 was kindly provided by Dr. Mike Franklin.

## Supplementary Material

Supplementary material is available online at JIMB ([www.academic.oup.com/jimb](http://www.academic.oup.com/jimb)).

## Author Contributions

Conceptualization: M.M., M.D., C.M.F., and S.W.; experimental design: M.M., M.D., C.M.F., and S.W.; methodology: M.M.; data analysis and curation M.M., M.D., and S.W.; and writing, review, and editing: M.M., M.D., C.M.F., and S.W.



## Funding

This work was performed in part at the Montana Nanotechnology Facility, a member of the National Nanotechnology Coordinated Infrastructure (NNCI), which is supported by the National Science Foundation (Grant# ECCS1542210) and the Center for Biofilm Engineering, Montana State University. The work was supported by NSF (Grant #1760616) to C. M. Foreman, Montana State University start-up package to S. Warnat, and USDA (Grant # AM22ACERMT1020) to S. Warnat.

Imaging was made possible by the Center for Biofilm Engineering Imaging Facility at Montana State University, which is supported by funding from the National Science Foundation MRI Program (2 018 562), the M. J. Murdock Charitable Trust (202 016 116), and the US Department of Defense (77369LSRIP).

## Conflicts of Interest

The authors declare no conflicts of interest.

## References

- Abdelrasoul, G. N., Anwar, A., MacKay, S., Tamura, M., Shah, M. A., Khasa, D. P., Montgomery, R. R., Ko, A. I., & Chen, J. (2020). DNA aptamer-based non-faradaic impedance biosensor for detecting *E. coli*. *Analytica Chimica Acta*, 1107, 135–144. <https://doi.org/10.1016/j.aca.2020.02.004>
- Assenhaimer, C., Domingos, A. S., Glasse, B., Fritsching, U., & Guardani, R. (2017). Long-term monitoring of metalworking fluid emulsion aging using a spectroscopic sensor. *Canadian Journal of Chemical Engineering*, 95(12), 2341–2349. <https://doi.org/10.1002/cjce.22931>
- Azeredo, J., Azevedo, N. F., Briandet, R., Cerca, N., Coenye, T., Costa, A. R., Desvaux, M., Di Bonaventura, G., Hébraud, M., Jaglic, Z., Kačániová, M., Knöchel, S., Lourenço, A., Mergulhão, F., Meyer, R. L., Nychas, G., Simões, M., Tresse, O., & Sternberg, C. (2017). Critical review on biofilm methods. *Critical Reviews in Microbiology*, 43(3), 313–351. <https://doi.org/10.1080/1040841X.2016.1208146>
- Becerro, S., Paredes, J., Mujika, M., Perez Lorenzo, E., & Arana, S. (2016). Electrochemical real-time analysis of bacterial biofilm adhesion and development by means of thin-film biosensors. *IEEE Sensors Journal*, 16(7), 1856–1864. <https://doi.org/10.1109/JSEN.2015.2504495>
- Bosire, E. M., Blank, L. M., & Rosenbaum, M. A. (2016). Strain- and substrate-dependent redox mediator and electricity production by *Pseudomonas aeruginosa*. *Applied and Environmental Microbiology*, 82(16), 5026–5038. <https://doi.org/10.1128/AEM.01342-16>
- Bott, T. R. (2009). Biofouling control in cooling water. *International Journal of Chemical Engineering*, 2009, 1–4. <https://doi.org/10.1155/2009/619873>
- Brosel-Oliu, S., Ferreira, R., Uriá, N., Abramova, N., Gargallo, R., Muñoz-Pascual, F. X., & Bratov, A. (2018). Novel impedimetric aptasensor for label-free detection of *Escherichia coli* O157:H7. *Sensors and Actuators, B: Chemical*, 255, 2988–2995. <https://doi.org/10.1016/j.snb.2017.09.121>
- Cámara, M., Green, W., MacPhee, C. E., Rakowska, P. D., Raval, R., Richardson, M. C., Slater-Jefferies, J., Steventon, K., & Webb, J. S. (2022). Economic significance of biofilms: a multidisciplinary and cross-sectoral challenge. *NPJ Biofilms and Microbiomes*, 8(1), 42–42. <https://doi.org/10.1038/s41522-022-00306-y>
- Chabowski, K., Junka, A. F., Piasecki, T., Nowak, D., Nitsch, K., Smutnicka, D., Bartoszewicz, M., Moczala, M., & Szymczyk, P. (2017). Impedance sensors made in PCB and LTCC technologies for monitoring growth and degradation of pseudomonal biofilm. *Metrology and Measurement Systems*, 24(2), 369–380. <https://doi.org/10.1515/mms-2017-0032>
- Costerton, J. W., Stewart, P. S., & Greenberg, E. P. (1999). Bacterial biofilms: a common cause of persistent infections. *Science (American Association for the Advancement of Science)*, 284(5418), 1318–1322. <https://doi.org/10.1126/science.284.5418.1318>
- Davey, M. E., Caiazza, N. C., & O'Toole, G. A. (2003). Rhamnolipid surfactant production affects biofilm architecture in *Pseudomonas aeruginosa* PAO1. *Journal of Bacteriology*, 185(3), 1027–1036. <https://doi.org/10.1128/JB.185.3.1027-1036.2003>
- Davies, D. (2003). Understanding biofilm resistance to antibacterial agents. *Nature Reviews Drug Discovery*, 2(2), 114–122. <https://doi.org/10.1038/nrd1008>
- Davies, D. G., Parsek, M. R., Pearson, J. P., Iglewski, B. H., Costerton, J. W., & Greenberg, E. P. (1998). The involvement of cell-to-cell signals in the development of a bacterial biofilm. *Science (American Association for the Advancement of Science)*, 280(5361), 295–298. <https://doi.org/10.1126/science.280.5361.295>
- Davison, W. M., Pitts, B., & Stewart, P. S. (2010). Spatial and temporal patterns of biocide action against *Staphylococcus epidermidis* biofilms. *Antimicrobial Agents and Chemotherapy*, 54(7), 2920–2927. <https://doi.org/10.1128/AAC.01734-09>
- Di Maiuta, N., Rüfenacht, A., & Küenzi, P. (2017). Assessment of bacteria and archaea in metalworking fluids using massive parallel 16S rRNA gene tag sequencing. *Letters in Applied Microbiology*, 65(4), 266–273. <https://doi.org/10.1111/lam.12782>
- Di Pippo, F., Di Gregorio, L., Congestri, R., Tandoi, V., & Rossetti, S. (2018). Biofilm growth and control in cooling water industrial systems. *FEMS Microbiology Ecology*, 94(5), 1–13. <https://doi.org/10.1093/femsec/fiy044>
- Dorledo de Faria, R. A., Dias Heneine, L. G., Matencio, T., & Messaddeq, Y. (2019). Faradaic and non-faradaic electrochemical impedance spectroscopy as transduction techniques for sensing applications. *International Journal of Biosensors & Bioelectronics*, 5(1):29–31. <https://doi.org/10.15406/ijbsbe.2019.05.00148>
- Fu, J., Zhang, Y., Lin, S., Zhang, W., Shu, G., Lin, J., Li, H., Xu, F., Tang, H., Peng, G., Zhao, L., Chen, S., & Fu, H. (2021). Strategies for interfering with bacterial early stage biofilms. *Frontiers in Microbiology*, 12, 675843. <https://doi.org/10.3389/fmicb.2021.675843>
- Funari, R., & Shen, A. Q. (2022). Detection and characterization of bacterial biofilms and biofilm-based sensors. *ACS Sensors*, 7(2), 347–357. <https://doi.org/10.1021/acssensors.1c02722>
- Furst, A. L., & Francis, M. B. (2019). Impedance-based detection of bacteria. *Chemical Reviews*, 119(1), 700–726. <https://doi.org/10.1021/acs.chemrev.8b00381>
- Green, A. E., Amézquita, A., Le Marc, Y., Bull, M. J., Connor, T. R., & Mahenthiralingam, E. (2018). The consistent differential expression of genetic pathways following exposure of an industrial *Pseudomonas aeruginosa* strain to preservatives and a laundry detergent formulation. *FEMS Microbiology Letters*, 365(9), 1–8. <https://doi.org/10.1093/femsle/fny062>
- He, Z., Wang, Q., Hu, Y., Liang, J., Jiang, Y., Ma, R., Tang, Z., & Huang, Z. (2012). Use of the quorum sensing inhibitor furanone C-30 to interfere with biofilm formation by *Streptococcus mutans* and its luxS mutant strain. *International Journal of Antimicrobial Agents*, 40(1), 30–35. <https://doi.org/10.1016/j.ijantimicag.2012.03.016>
- Hentzer, M., Wu, H., Andersen, J. B., Riedel, K., Rasmussen, T. B., Bagge, N., Kumar, N., Schembri, M. A., Song, Z., Kristoffersen, P., Mane-field, M., Costerton, J. W., Molin, S., Eberl, L., Steinberg, P., Kjelleberg, S., Høiby, N., & Givskov, M. (2003). Attenuation of *Pseudomonas aeruginosa* virulence by quorum sensing inhibitors. *The EMBO Journal*, 22(15), 3803–3815. <https://doi.org/10.1093/emboj/cdg366>

- Høiby, N., Johansen, H. K., Moser, C., Song, Z., Ciofu, O., & Kharazmi, A. (2001). *Pseudomonas aeruginosa* and the in vitro and in vivo biofilm mode of growth. *Microbes and Infection*, 3(1), 23–35. [https://doi.org/10.1016/S1286-4579\(00\)01349-6](https://doi.org/10.1016/S1286-4579(00)01349-6)
- Huiszoon, R. C., Han, J. J., Chu, S., Stine, J. M., Beardslee, L. A., & Ghodssi, R. (2021). Integrated system for bacterial detection and biofilm treatment on indwelling urinary catheters. *IEEE Transactions on Biomedical Engineering*, 68, 3241–3249.
- Huiszoon, R. C., Subramanian, S., Ramiah Rajasekaran, P., Beardslee, L. A., Bentley, W. E., & Ghodssi, R. (2019). Flexible platform for In situ impedimetric detection and bioelectric effect treatment of *Escherichia coli* biofilms. *IEEE Transactions on Biomedical Engineering*, 66(5), 1337–1345. <https://doi.org/10.1109/TBME.2018.2872896>
- Kiefer, J., Seidel, B., & Meyer, D. (2018). Optical spectroscopy for analysis and monitoring of metalworking fluids. *Applied Spectroscopy*, 72(12), 1790–1797. <https://doi.org/10.1177/0003702818789700>
- Lappin-Scott, H. M., & Costerton, J. W. (1989). Bacterial biofilms and surface fouling. *Biofouling (Chur, Switzerland)*, 1(4), 323–342. <https://doi.org/10.1080/08927018909378120>
- Lebeaux, D., Ghigo, J.-M., & Beloin, C. (2014). Biofilm-related infections: Bridging the gap between clinical management and fundamental aspects of recalcitrance toward antibiotics. *Microbiology and Molecular Biology Reviews*, 78(3), 510–543. <https://doi.org/10.1128/MMBR.00013-14>
- Lim, C. P., Mai, P. N. Q., Roizman Sade, D., Lam, Y. C., & Cohen, Y. (2016). Biofilm development of an opportunistic model bacterium analysed at high spatiotemporal resolution in the framework of a precise flow cell. *NPJ Biofilms and Microbiomes*, 2(1), 16023–16023. <https://doi.org/10.1038/npjbiofilms.2016.23>
- Lisoń, J., Taratuta, A., Paszenda, Z., Szindler, M., & Basiaga, M. (2022). Perspectives in prevention of biofilm for medical applications. *Coatings (Basel)*, 12(2), 197. <https://doi.org/10.3390/coatings12020197>
- Liu, L., Xu, Y., Cui, F., Xia, Y., Chen, L., Mou, X., & Lv, J. (2018). Monitoring of bacteria biofilms forming process by in-situ impedimetric biosensor chip. *Biosensors & Bioelectronics*, 112, 86–92. <https://doi.org/10.1016/j.bios.2018.04.019>
- Lu, L., Hu, W., Tian, Z. R., Yuan, D. D., Yi, G. J., Zhou, Y. Y., Cheng, Q., Zhu, J., & Li, M. X. (2019). Developing natural products as potential anti-biofilm agents. *Chinese Medicine*, 14(1), 11. <https://doi.org/10.1186/s13020-019-0232-2>
- Magar, H. S., Hassan, R. Y. A., & Mulchandani, A. (2021). Electrochemical impedance spectroscopy (EIS): principles, construction, and biosensing applications. *Sensors (Basel, Switzerland)*, 21(19), 6578. <https://doi.org/10.3390/s21196578>
- Mallén-Alberdi, M., Vigués, N., Mas, J., Fernández-Sánchez, C., & Baldi, A. (2016). Impedance spectral fingerprint of *E. coli* cells on interdigitated electrodes: a new approach for label free and selective detection. *Sensing and Bio-Sensing Research*, 7, 100–106. <https://doi.org/10.1016/j.sbsr.2016.02.001>
- Markus, V., Golberg, K., Terali, K., Ozer, N., Kramarsky-Winter, E., Marks, R. S., & Kushmaro, A. (2021). Assessing the molecular targets and mode of action of Furanone C-30 on *Pseudomonas aeruginosa* quorum sensing. *Molecules (Basel, Switzerland)*, 26(6), 1620. <https://doi.org/10.3390/molecules26061620>
- McGlennen, M., Dieser, M., Foreman, C. M., & Warnat, S. (2023). Using electrochemical impedance spectroscopy to study biofilm growth in a 3D-printed flow cell system. *Biosensors and Bioelectronics*, X, 14, 100326. <https://doi.org/10.1016/j.biosx.2023.100326>
- McGlennen, M., Neubauer, M., Driesler, M., Dieser, M., Foreman, C. M., & Warnat, S. (2020). Microsensors in icy environments to detect microbial activities. *Journal of Microelectromechanical Systems*, 29(5), 853–859. <https://doi.org/10.1109/JMEMS.2020.3012420>
- Miller, M. B., & Bassler, B. L. (2001). Quorum sensing in bacteria. *Annual Review of Microbiology*, 55(1), 165–199. <https://doi.org/10.1146/annurev.micro.55.1.165>
- Mukherjee, S., & Bassler, B. L. (2019). Bacterial quorum sensing in complex and dynamically changing environments. *Nature Reviews. Microbiology*, 17(6), 371–382. <https://doi.org/10.1038/s41579-019-0186-5>
- Nivens, D. E., Ohman, D. E., Williams, J., & Franklin, M. J. (2001). Role of Alginate and its O acetylation in formation of *Pseudomonas aeruginosa* microcolonies and biofilms. *Journal of Bacteriology*, 183(3), 1047–1057. <https://doi.org/10.1128/JB.183.3.1047-1057.2001>
- Özcan, S. S., Dieser, M., Parker, A. E., Balasubramanian, N., & Foreman, C. M. (2019). Quorum sensing inhibition as a promising method to control biofilm growth in metalworking fluids. *Journal of Industrial Microbiology & Biotechnology*, 46(8), 1103–1111. <https://doi.org/10.1007/s10295-019-02181-7>
- Paredes, J., Becerro, S., & Arana, S. (2014). Label-free interdigitated microelectrode based biosensors for bacterial biofilm growth monitoring using petri dishes. *Journal of Microbiological Methods*, 100, 77–83. <https://doi.org/10.1016/j.mimet.2014.02.022>
- Paredes, J., Becerro, S., & Arana, S. (2014). Comparison of real time impedance monitoring of bacterial biofilm cultures in different experimental setups mimicking real field environments. *Sensors and Actuators B: Chemical*, 195, 667–676.
- Paredes, J., Becerro, S., Arizti, F., Aguinaga, A., Del Pozo, J. L., & Arana, S. (2012). Real time monitoring of the impedance characteristics of staphylococcal bacterial biofilm cultures with a modified CDC reactor system. *Biosensors & Bioelectronics*, 38(1), 226–232. <https://doi.org/10.1016/j.bios.2012.05.027>
- Paredes, J., Becerro, S., Arizti, F., Aguinaga, A., Del Pozo, J. L., & Arana, S. (2013). Interdigitated microelectrode biosensor for bacterial biofilm growth monitoring by impedance spectroscopy technique in 96-well microtiter plates. *Sensors and Actuators B: Chemical*, 178, 663–670. <https://doi.org/10.1016/j.snb.2013.01.027>
- Park, J. S., Kim, H. J., Lee, J.-H., Park, J. H., Kim, J., Hwang, K. S., & Lee, B. C. (2018). Amyloid beta detection by faradaic electrochemical impedance spectroscopy using interdigitated microelectrodes. *Sensors (Basel, Switzerland)*, 18(2), 426. <https://doi.org/10.3390/s18020426>
- Passman, F. J., & Küenzi, P. (2020). Microbiology in water-miscible metalworking fluids. *Tribology Transactions*, 63(6), 1147–1171. <https://doi.org/10.1080/10402004.2020.1764684>
- Perini, N., Prado, A. R., Sad, C. M. S., Castro, E. V. R., & Freitas, M. B. J. G. (2012). Electrochemical impedance spectroscopy for in situ petroleum analysis and water-in-oil emulsion characterization. *Fuel (Guildford)*, 91(1), 224–228. <https://doi.org/10.1016/j.fuel.2011.06.057>
- Peterson, B. W., He, Y., Ren, Y., Zerdoum, A., Libera, M. R., Sharma, P. K., van Winkelhoff, A.-J., Neut, D., Stoodley, P., van der Mei, H. C., & Busscher, H. J. (2015). Viscoelasticity of biofilms and their recalcitrance to mechanical and chemical challenges. *FEMS Microbiology Reviews*, 39(2), 234–245. <https://doi.org/10.1093/femsre/fuu008>
- Proctor, C. R., McCarron, P. A., & Ternan, N. G. (2020). Furanone quorum-sensing inhibitors with potential as novel therapeutics against *Pseudomonas aeruginosa*. *Journal of Medical Microbiology*, 69(2), 195–206. <https://doi.org/10.1099/jmm.0.001144>
- Rather, M. A., Gupta, K., & Mandal, M. (2021). Microbial biofilm: Formation, architecture, antibiotic resistance, and control strategies. *Brazilian Journal of Microbiology*, 52(4), 1701–1718. <https://doi.org/10.1007/s42770-021-00624-x>
- Saccomano, S. C., Jewell, M. P., & Cash, K. J. (2021). A review of chemosensors and biosensors for monitoring biofilm dynamics.

- Sensors and Actuators Reports, 3, 100043. <https://doi.org/10.1016/j.snr.2021.100043>
- Sadekuzzaman, M., Yang, S., Mizan, M. F. R., & Ha, S. D. (2015). Current and recent advanced strategies for combating biofilms. *Comprehensive Reviews in Food Science and Food Safety*, 14(4), 491–509. <https://doi.org/10.1111/1541-4337.12144>
- Saha, R. & Donofrio, R. S. (2012). The microbiology of metalworking fluids. *Applied Microbiology and Biotechnology*, 94(5), 1119–1130. <https://doi.org/10.1007/s00253-012-4055-7>
- Saha, R., Donofrio, R. S., Goeres, D. M., & Bagley, S. T. (2012). Rapid detection of rRNA group I pseudomonads in contaminated metalworking fluids and biofilm formation by fluorescent in situ hybridization. *Applied Microbiology and Biotechnology*, 94(3), 799–808. <https://doi.org/10.1007/s00253-011-3647-y>
- Sidhu, R. K., Cavallaro, N. D., Pola, C. C., Danyluk, M. D., McLamore, E. S., & Gomes, C. L. (2020). Planar interdigitated aptasensor for flow-through detection of *Listeria* spp. in Hydroponic Lettuce Growth Media. *Sensors (Basel, Switzerland)*, 20(20), 5773. <https://doi.org/10.3390/s20205773>
- Silva, V., Silva, C., Soares, P., Garrido, E. M., Borges, F., & Garrido, J. (2020). Isothiazolinone biocides: chemistry, biological, and toxicity profiles. *Molecules (Basel, Switzerland)*, 25(4), 991. <https://doi.org/10.3390/molecules25040991>
- Skindersoe, M. E., Alhede, M., Phipps, R., Yang, L., Jensen, P. O., Rasmussen, T. B., Bjarnsholt, T., Tolker-Nielsen, T., Hoiby, N., & Givskov, M. (2008). Effects of antibiotics on quorum sensing in *Pseudomonas aeruginosa*. *Antimicrobial Agents and Chemotherapy*, 52(10), 3648–3663. <https://doi.org/10.1128/AAC.01230-07>
- Stewart, P. S., White, B., Boegli, L., Hamerly, T., Williamson, K. S., Franklin, M. J., Bothner, B., James, G. A., Fisher, S., Vital-Lopez, F. G., & Wallqvist, A. (2019). Conceptual model of biofilm antibiotic tolerance that integrates phenomena of diffusion, metabolism, gene expression, and physiology. *Journal of Bacteriology*, 201(22), e00307-19. <https://doi.org/10.1128/JB.00307-19>
- Stoodley, P., Hall-Stoodley, L., & Costerton, J. W. (2004). Bacterial biofilms: From the natural environment to infectious diseases. *Nature Reviews. Microbiology*, 2(2), 95–108. <https://doi.org/10.1038/nrmicro821>
- Subramanian, S., Huiszoon, R. C., Chu, S., Bentley, W. E., & Ghodssi, R. (2020). Microsystems for biofilm characterization and sensing – A review. *Biofilm*, 2, 100015. <https://doi.org/10.1016/j.biofilm.2019.100015>
- Subramanian, S., Tolstaya, E. I., Winkler, T. E., Bentley, W. E., & Ghodssi, R. (2017). An integrated microsystem for real-time detection and threshold-activated treatment of bacterial biofilms. *ACS Applied Materials & Interfaces*, 9(37), 31362–31371. <https://doi.org/10.1021/acsami.7b04828>
- Trafny, E. A. (2013). Microorganisms in metalworking fluids: current issues in research and management. *International Journal of Occupational Medicine and Environmental Health*, 26(1), 4–15. <https://doi.org/10.2478/S13382-013-0075-5>
- Turick, C. E., Shimpalee, S., Satjaritanun, P., Weidner, J., & Greenway, S. (2019). Convenient non-invasive electrochemical techniques to monitor microbial processes: Current state and perspectives. *Applied Microbiology and Biotechnology*, 103(20), 8327–8338. <https://doi.org/10.1007/s00253-019-10091-y>
- Wu, H., Song, Z., Hentzer, M., Andersen, J. B., Molin, S., Givskov, M., & Høiby, N. (2004). Synthetic furanones inhibit quorum-sensing and enhance bacterial clearance in *Pseudomonas aeruginosa* lung infection in mice. *Journal of Antimicrobial Chemotherapy*, 53(6), 1054–1061. <https://doi.org/10.1093/jac/dkh223>
- Zhao, J., Cheng, W., He, X., Liu, Y., Li, J., Sun, J., Li, J., Wang, F., & Gao, Y. (2018). Association of furanone C-30 with biofilm formation & antibiotic resistance in *Pseudomonas aeruginosa*. *Indian Journal of Medical Research (New Delhi, India : 1994)*, 147(4), 400–406. [https://doi.org/10.4103/ijmr.IJMR\\_2010\\_16](https://doi.org/10.4103/ijmr.IJMR_2010_16)